

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052825\
 Data File : VX046381.D
 Acq On : 28 May 2025 13:29
 Operator : JC/MD
 Sample : Q2130-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-3

Quant Time: May 29 03:35:46 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 06 07:12:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	60688	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	122066	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	119742	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	51343	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	61667	54.504	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 109.000%	
35) Dibromofluoromethane	5.379	113	44866	51.042	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.080%	
50) Toluene-d8	8.647	98	157008	51.607	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 103.220%	
62) 4-Bromofluorobenzene	11.079	95	61270	52.502	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 105.000%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.307	50	46	0.051	ug/l #	43
5) Bromomethane	1.612	94	55	0.141	ug/l #	4
6) Chloroethane	1.618	64	47	0.105	ug/l #	44
16) Acetone	2.380	43	57337	126.391	ug/l	100
17) Carbon Disulfide	2.508	76	173	0.101	ug/l #	76
18) Methyl Acetate	2.703	43	2270	2.156	ug/l #	89
20) Methylene Chloride	2.788	84	6738	7.751	ug/l	93
23) Vinyl Acetate	3.751	43	19	0.008	ug/l #	74
25) 2-Butanone	4.581	43	4600	6.985	ug/l #	82
37) Ethyl Acetate	4.788	43	183	0.125	ug/l #	70
41) Methacrylonitrile	5.044	41	133	0.174	ug/l #	34
42) 1,2-Dichloroethane	6.111	62	19	0.013	ug/l #	78
43) Isopropyl Acetate	6.348	43	11335	5.092	ug/l	96
52) Toluene	8.720	92	24	0.011	ug/l #	21
53) t-1,3-Dichloropropene	8.946	75	212	0.178	ug/l #	43
56) Ethyl methacrylate	9.244	69	198	0.149	ug/l #	1
67) Ethyl Benzene	10.311	91	226	0.049	ug/l #	81
68) m/p-Xylenes	10.305	106	106	0.063	ug/l	99
70) Styrene	10.665	104	50	0.019	ug/l #	23
73) Isopropylbenzene	11.079	105	97	0.024	ug/l #	49
78) n-propylbenzene	11.305	91	24	0.005	ug/l #	54
79) 2-Chlorotoluene	11.305	91	24	0.008	ug/l #	44
80) 1,3,5-Trimethylbenzene	11.457	105	59	0.018	ug/l #	30
82) 4-Chlorotoluene	11.305	91	24	0.007	ug/l #	48
84) 1,2,4-Trimethylbenzene	11.762	105	67	0.020	ug/l #	33
85) sec-Butylbenzene	12.012	105	52	0.013	ug/l #	33
86) p-Isopropyltoluene	12.006	119	49	0.014	ug/l #	1
87) 1,3-Dichlorobenzene	12.037	146	26	0.015	ug/l #	1
88) 1,4-Dichlorobenzene	12.037	146	26	0.015	ug/l #	1
95) Naphthalene	13.792	128	254	0.071	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052825\
Data File : VX046381.D
Acq On : 28 May 2025 13:29
Operator : JC/MD
Sample : Q2130-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-3

Quant Time: May 29 03:35:46 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260
QLast Update : Tue May 06 07:12:22 2025
Response via : Initial Calibration




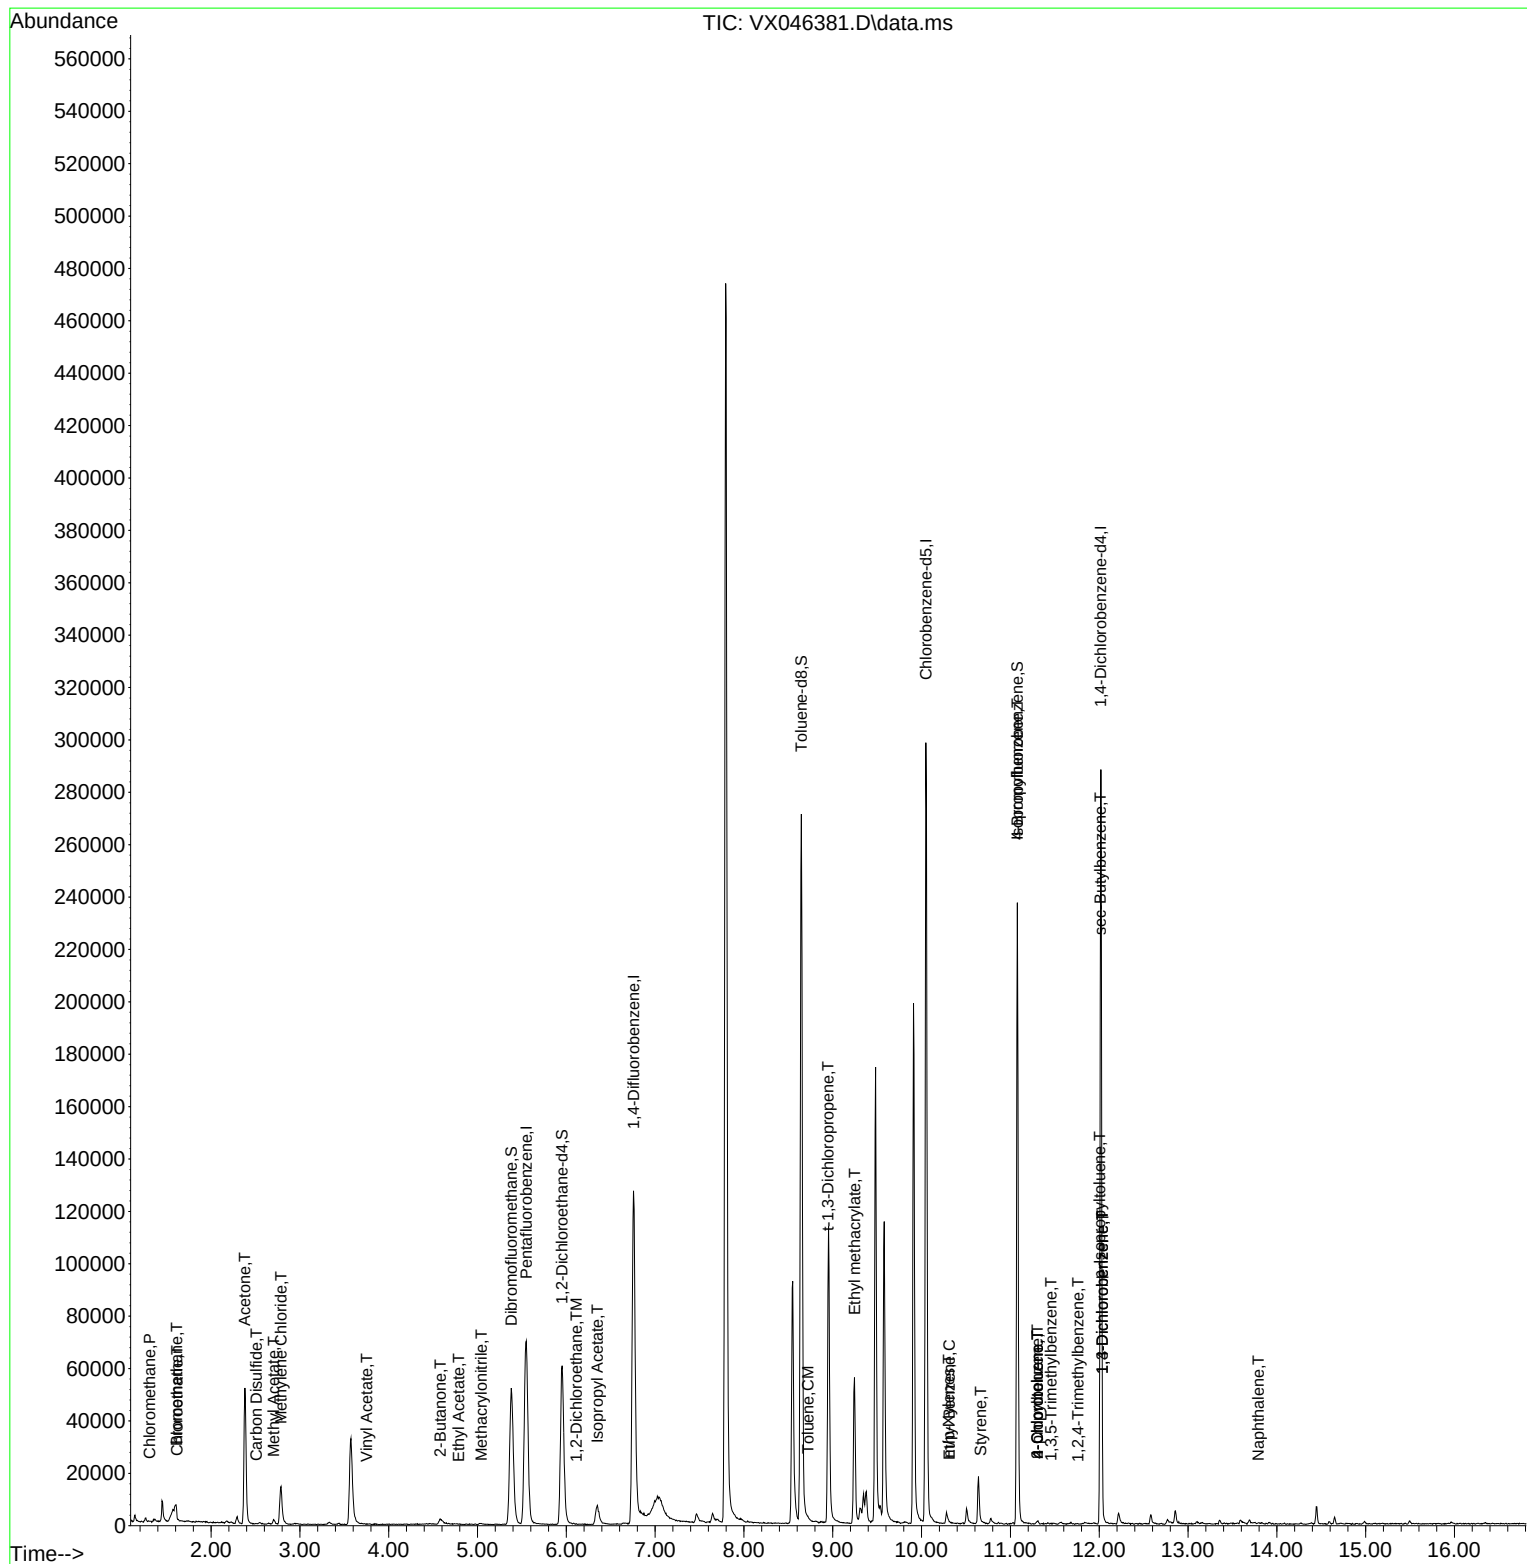




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29




Instrument :
MSVOA_X
ClientSampleId :
TP-3


Tgt Ion:168 Resp: 60688
Ion Ratio Lower Upper
168 100
99 70.7 54.9 82.3



#3
Chloromethane
Concen: 0.051 ug/l
RT: 1.307 min Scan# 36
Delta R.T. 0.000 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29

Tgt Ion: 50 Resp: 46
Ion Ratio Lower Upper
50 100
52 0.0 25.4 38.2#


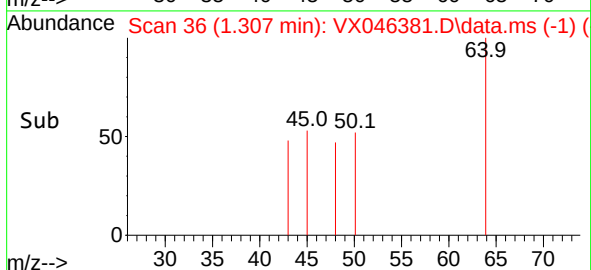




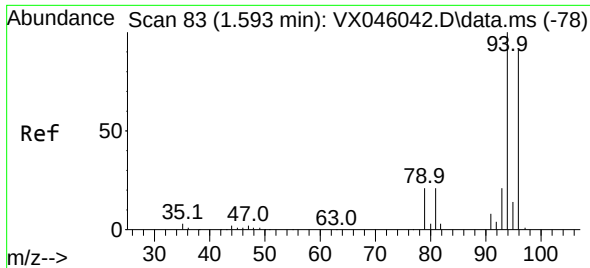

#5
Bromomethane
Concen: 0.141 ug/l
RT: 1.612 min Scan# 80
Delta R.T. 0.018 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29




Instrument :
MSVOA_X
ClientSampleId :
TP-3


Tgt Ion: 94 Resp: 55
Ion Ratio Lower Upper
94 100
96 0.0 72.8 109.2#

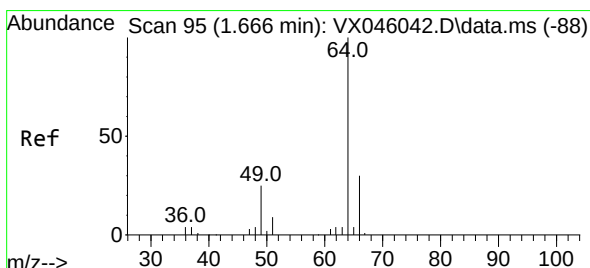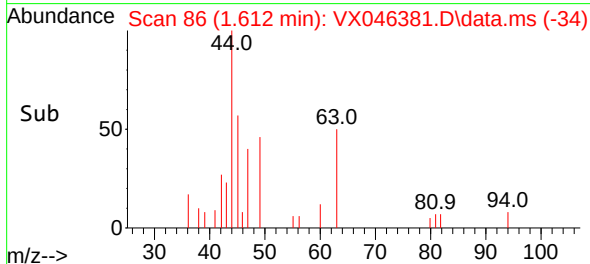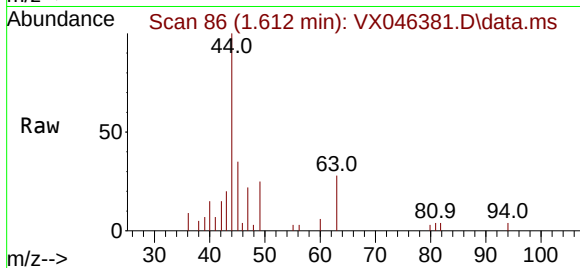

#6
Chloroethane
Concen: 0.105 ug/l
RT: 1.618 min Scan# 87
Delta R.T. -0.049 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29

Tgt Ion: 64 Resp: 47
Ion Ratio Lower Upper
64 100
66 0.0 24.3 36.5#


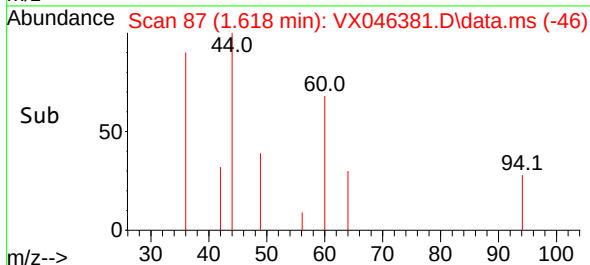

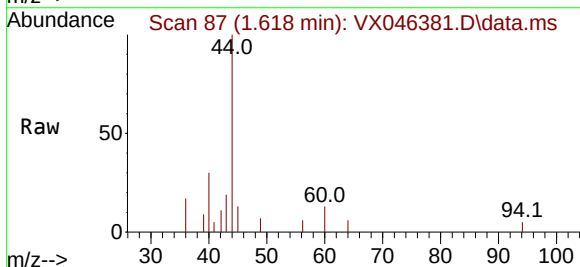




#16
Acetone
Concen: 126.391 ug/l
RT: 2.380 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29




Instrument :
MSVOA_X
ClientSampleId :
TP-3


Tgt Ion: 43 Resp: 57337
Ion Ratio Lower Upper
43 100
58 26.3 21.2 31.8



#17
Carbon Disulfide
Concen: 0.101 ug/l
RT: 2.508 min Scan# 233
Delta R.T. 0.006 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29

Tgt Ion: 76 Resp: 173
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.4#


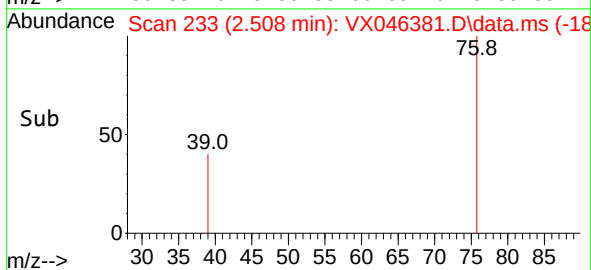






#18
Methyl Acetate
Concen: 2.156 ug/l
RT: 2.703 min Scan# 218
Delta R.T. 0.000 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29




Instrument :
MSVOA_X
ClientSampleId :
TP-3


Tgt Ion: 43 Resp: 2270
Ion Ratio Lower Upper
43 100
74 15.8 16.7 25.1#

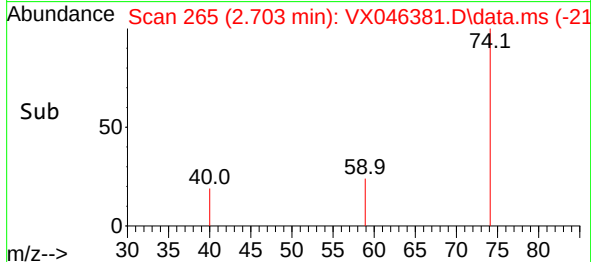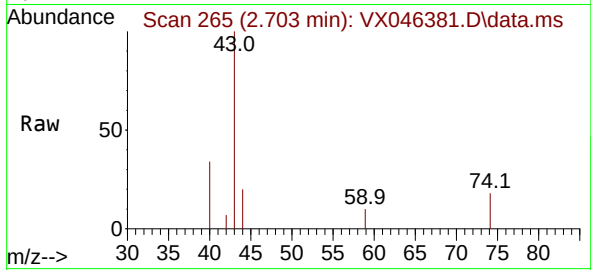

#20
Methylene Chloride
Concen: 7.751 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.006 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29

Tgt Ion: 84 Resp: 6738
Ion Ratio Lower Upper
84 100
49 131.6 113.9 170.9
51 42.2 33.5 50.3
86 60.7 53.8 80.8


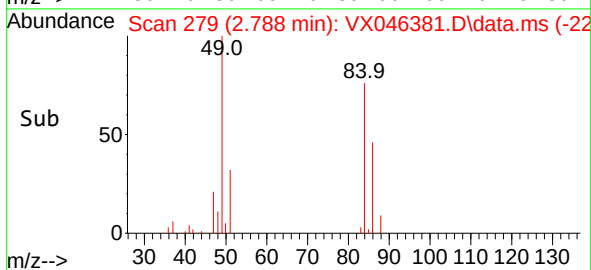






#23
 Vinyl Acetate
 Concen: 0.008 ug/l
 RT: 3.751 min Scan# 41
 Delta R.T. 0.031 min
 Lab File: VX046381.D
 Acq: 28 May 2025 13:29




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-3


Tgt Ion: 43 Resp: 19
 Ion Ratio Lower Upper
 43 100
 86 0.0 7.5 11.3#

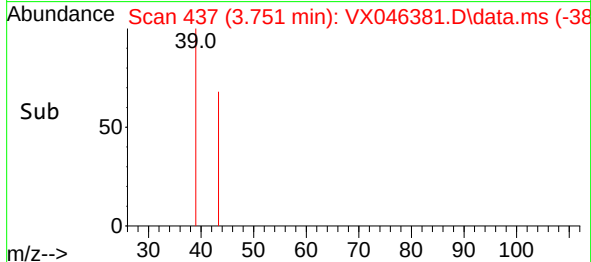

#25
 2-Butanone
 Concen: 6.985 ug/l
 RT: 4.581 min Scan# 573
 Delta R.T. 0.024 min
 Lab File: VX046381.D
 Acq: 28 May 2025 13:29

Tgt Ion: 43 Resp: 4600
 Ion Ratio Lower Upper
 43 100
 72 14.4 18.4 27.6#




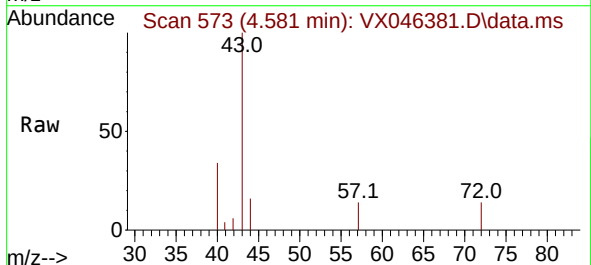




#33
 1,2-Dichloroethane-d4
 Concen: 54.504 ug/l
 RT: 5.952 min Scan# 798
 Delta R.T. 0.000 min
 Lab File: VX046381.D
 Acq: 28 May 2025 13:29




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-3


Tgt Ion: 65 Resp: 61667
 Ion Ratio Lower Upper
 65 100
 67 49.4 0.0 99.0

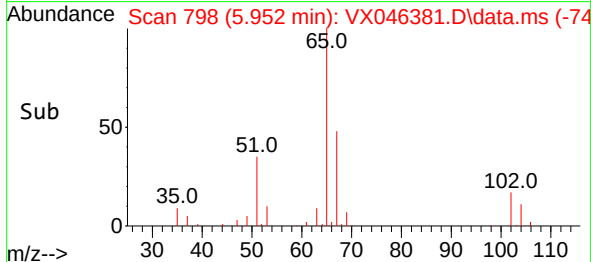

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 930
 Delta R.T. 0.000 min
 Lab File: VX046381.D
 Acq: 28 May 2025 13:29

Tgt Ion: 114 Resp: 122066
 Ion Ratio Lower Upper
 114 100
 63 23.8 0.0 49.2
 88 18.3 0.0 33.6


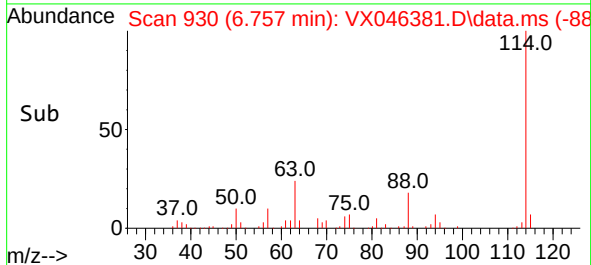






#35
Dibromofluoromethane
Concen: 51.042 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.000 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29




Instrument :
MSVOA_X
ClientSampleId :
TP-3


Tgt Ion:113 Resp: 44866
Ion Ratio Lower Upper
113 100
111 103.0 83.1 124.7
192 16.5 13.3 19.9

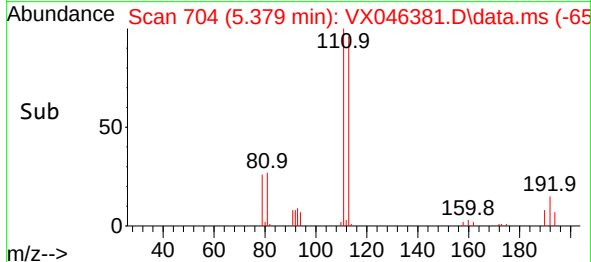

#37
Ethyl Acetate
Concen: 0.125 ug/l
RT: 4.788 min Scan# 607
Delta R.T. 0.073 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29

Tgt Ion: 43 Resp: 183
Ion Ratio Lower Upper
43 100
61 0.0 10.3 15.5#
70 0.0 7.9 11.9#


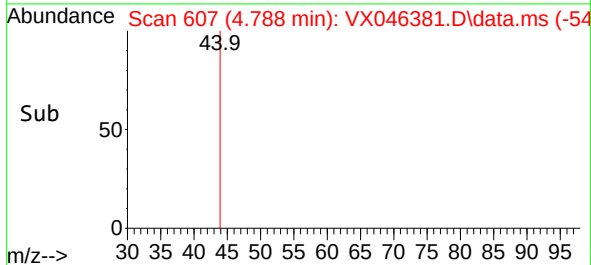






#41
Methacrylonitrile
Concen: 0.174 ug/l
RT: 5.044 min Scan# 649
Delta R.T. 0.128 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29




Instrument :
MSVOA_X
ClientSampleId :
TP-3


Tgt Ion:	41	Resp:	133
Ion	Ratio	Lower	Upper
41	100		
39	100.8	47.2	70.8#
67	0.0	50.7	76.1#
52	0.0	24.6	37.0#

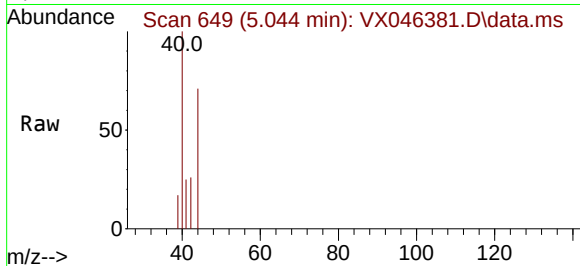

#42
1,2-Dichloroethane
Concen: 0.013 ug/l
RT: 6.111 min Scan# 824
Delta R.T. 0.031 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29

Tgt Ion:	62	Resp:	19
Ion	Ratio	Lower	Upper
62	100		
98	0.0	0.0	15.2


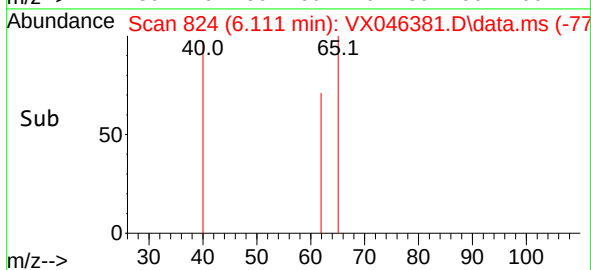

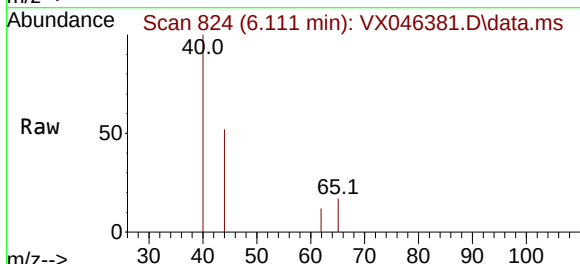




#43
Isopropyl Acetate
Concen: 5.092 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.012 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29




Instrument :
MSVOA_X
ClientSampleId :
TP-3


Tgt Ion: 43 Resp: 11335
Ion Ratio Lower Upper
43 100
61 16.2 14.3 21.5
87 10.4 9.5 14.3



#50
Toluene-d8
Concen: 51.607 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29

Tgt Ion: 98 Resp: 157008
Ion Ratio Lower Upper
98 100
100 65.3 53.5 80.3

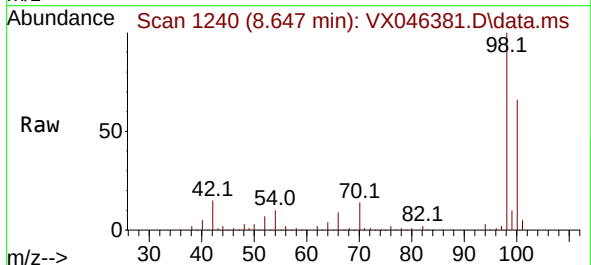

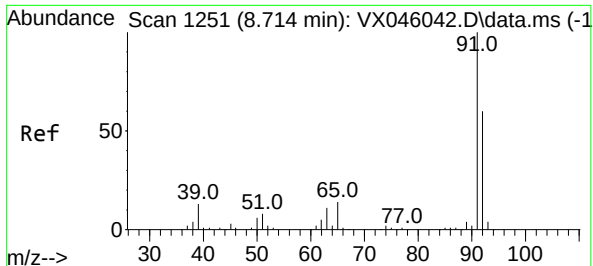

#52

Toluene

Concen: 0.011 ug/l

RT: 8.720 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX046381.D

Acq: 28 May 2025 13:29

Instrument :

MSVOA_X

ClientSampleId :





TP-3

Tgt Ion: 92 Resp: 24

Ion Ratio Lower Upper

92 100

91 279.2 136.6 205.0#

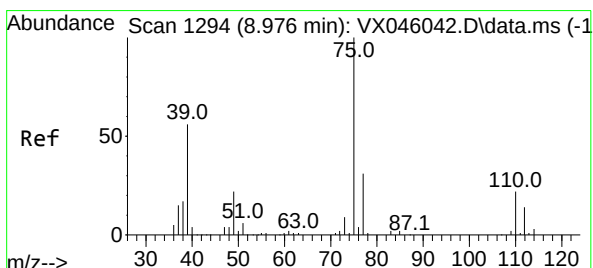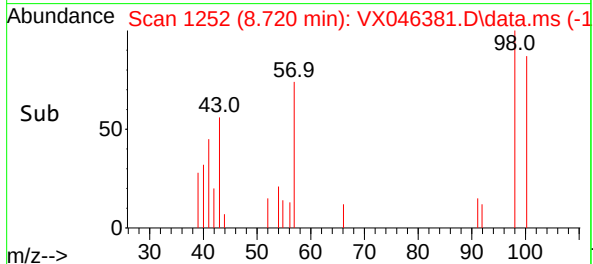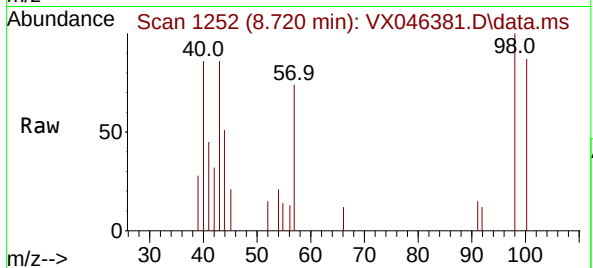

#53

t-1,3-Dichloropropene

Concen: 0.178 ug/l

RT: 8.946 min Scan# 1289

Delta R.T. -0.030 min

Lab File: VX046381.D




Acq: 28 May 2025 13:29


Tgt Ion: 75 Resp: 212

Ion Ratio Lower Upper

75 100

77 0.0 25.0 37.6#

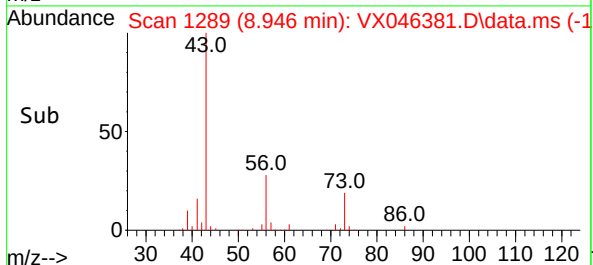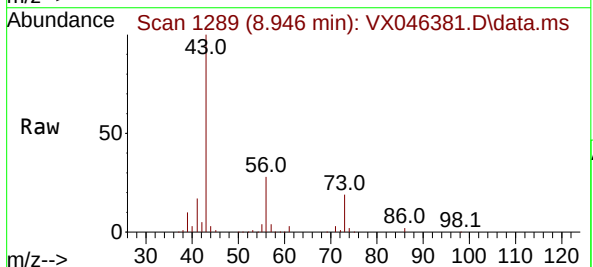



#56

Ethyl methacrylate

Concen: 0.149 ug/l

RT: 9.244 min Scan# 1

Delta R.T. 0.128 min

Lab File: VX046381.D

Acq: 28 May 2025 13:29

Instrument :

MSVOA_X

ClientSampleId :

TP-3





Tgt Ion: 69 Resp: 198

Ion Ratio Lower Upper

69 100

41 5250.5 60.8 91.2#

39 2503.5 39.0 58.6#

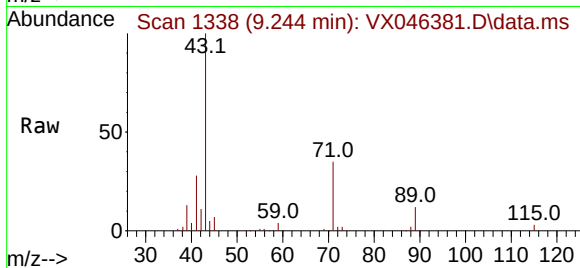

#62

4-Bromofluorobenzene

Concen: 52.502 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX046381.D

Acq: 28 May 2025 13:29




Tgt Ion: 95 Resp: 61270


Ion Ratio Lower Upper

95 100

174 66.5 0.0 135.8

176 64.0 0.0 131.4


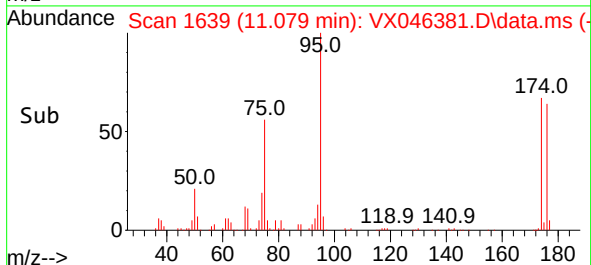

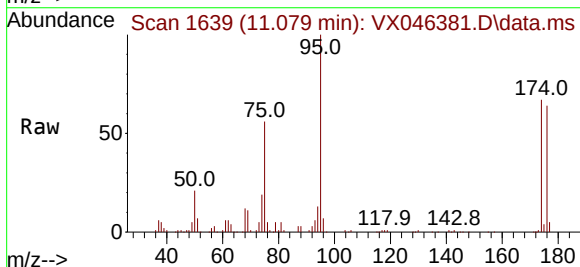




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29




Instrument :
MSVOA_X
ClientSampleId :
TP-3


Tgt Ion:117 Resp: 119742
Ion Ratio Lower Upper
117 100
82 61.6 50.6 76.0
119 31.8 25.8 38.6

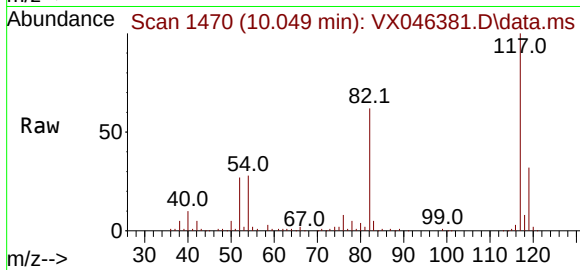

#67
Ethyl Benzene
Concen: 0.049 ug/l
RT: 10.311 min Scan# 1513
Delta R.T. 0.122 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29

Tgt Ion: 91 Resp: 226
Ion Ratio Lower Upper
91 100
106 39.7 23.4 35.2#




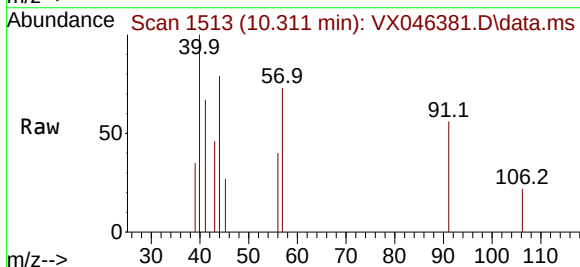




#68
m/p-Xylenes
Concen: 0.063 ug/l
RT: 10.305 min Scan# 1511
Delta R.T. 0.006 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29




Instrument :
MSVOA_X
ClientSampleId :
TP-3


Tgt Ion:106 Resp: 106
Ion Ratio Lower Upper
106 100
91 213.2 171.2 256.8

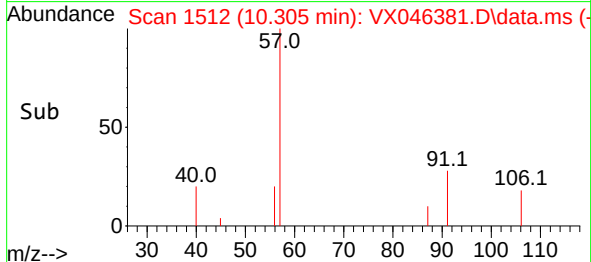

#70
Styrene
Concen: 0.019 ug/l
RT: 10.665 min Scan# 1571
Delta R.T. 0.012 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29

Tgt Ion:104 Resp: 50
Ion Ratio Lower Upper
104 100
78 0.0 45.7 68.5#
103 0.0 43.7 65.5#




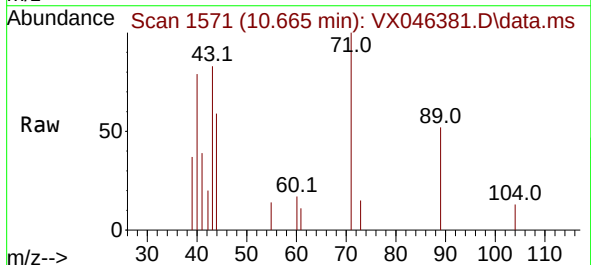




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29




Instrument :
MSVOA_X
ClientSampleId :
TP-3


Tgt Ion:152 Resp: 51343
Ion Ratio Lower Upper
152 100
115 65.7 46.9 140.7
150 156.8 0.0 351.0

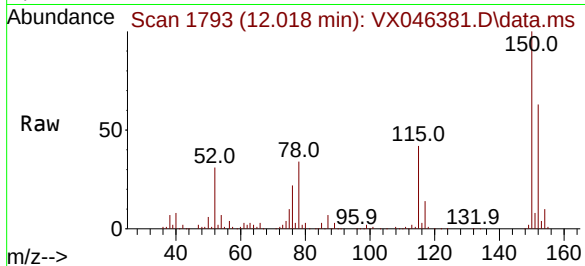

#73
Isopropylbenzene
Concen: 0.024 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.122 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29

Tgt Ion:105 Resp: 97
Ion Ratio Lower Upper
105 100
120 0.0 12.8 38.4#

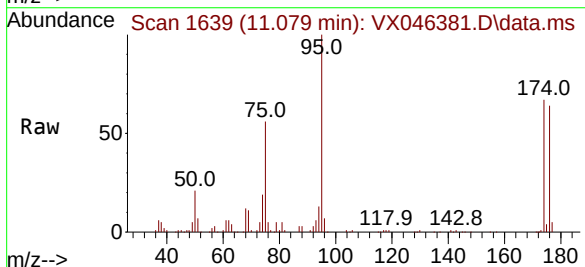

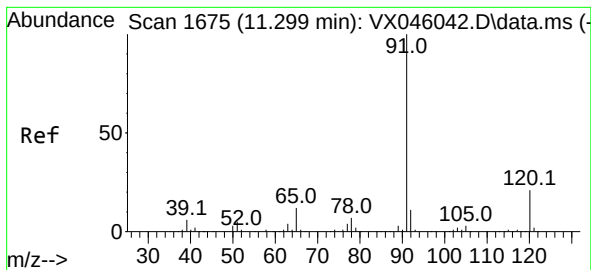

#78

n-propylbenzene

Concen: 0.005 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.006 min

Lab File: VX046381.D

Acq: 28 May 2025 13:29

Instrument :

MSVOA_X

ClientSampleId :





TP-3

Tgt Ion: 91 Resp: 24

Ion Ratio Lower Upper

91 100

120 0.0 10.8 32.4#

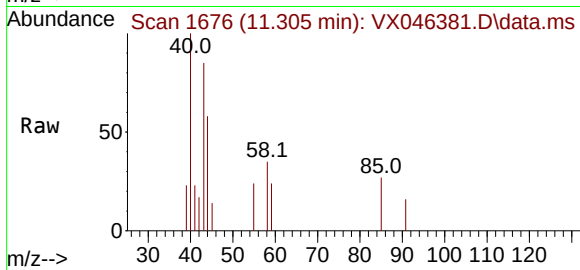

#79

2-Chlorotoluene

Concen: 0.008 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.055 min

Lab File: VX046381.D




Acq: 28 May 2025 13:29


Tgt Ion: 91 Resp: 24

Ion Ratio Lower Upper

91 100

126 0.0 15.6 46.7#




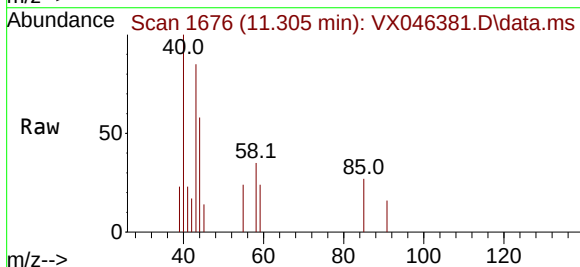




#80
1,3,5-Trimethylbenzene
Concen: 0.018 ug/l
RT: 11.457 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29




Instrument :
MSVOA_X
ClientSampleId :
TP-3


Tgt Ion:105 Resp: 59
Ion Ratio Lower Upper
105 100
120 0.0 23.1 69.2#

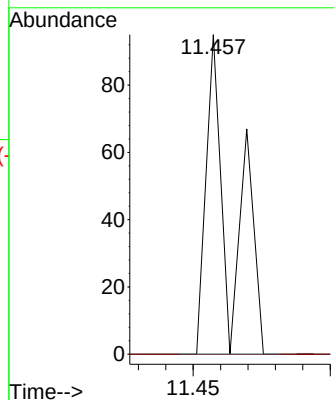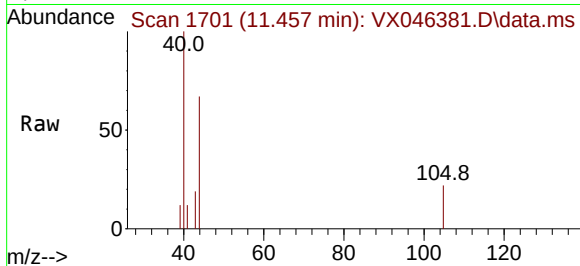

#82
4-Chlorotoluene
Concen: 0.007 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.146 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29

Tgt Ion: 91 Resp: 24
Ion Ratio Lower Upper
91 100
126 0.0 13.3 39.8#



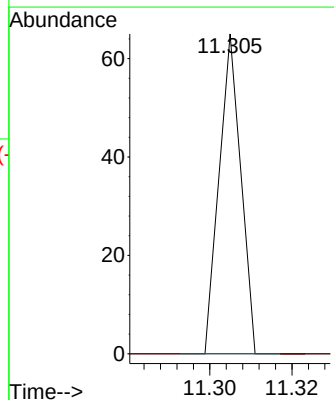
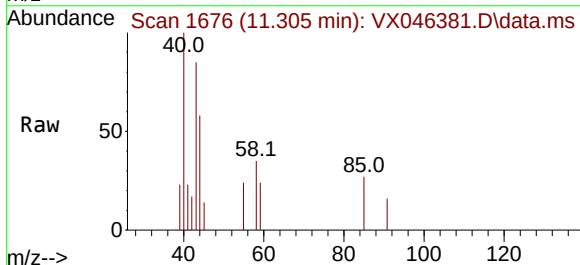




#84
1,2,4-Trimethylbenzene
Concen: 0.020 ug/l
RT: 11.762 min Scan# 11
Delta R.T. 0.012 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29




Instrument :
MSVOA_X
ClientSampleId :
TP-3


Tgt Ion:105 Resp: 67
Ion Ratio Lower Upper
105 100
120 0.0 21.2 63.6#

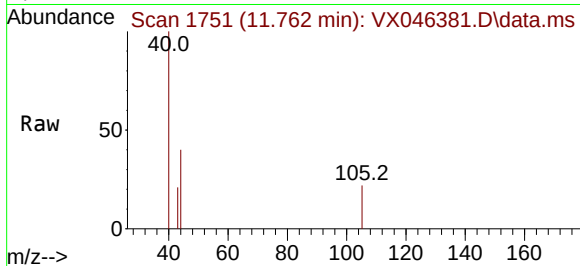

#85
sec-Butylbenzene
Concen: 0.013 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. 0.122 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29

Tgt Ion:105 Resp: 52
Ion Ratio Lower Upper
105 100
134 50.0 9.7 29.1#









#86
 p-Isopropyltoluene
 Concen: 0.014 ug/l
 RT: 12.006 min Scan# 1791
 Delta R.T. 0.000 min
 Lab File: VX046381.D
 Acq: 28 May 2025 13:29




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-3


Tgt Ion:119 Resp: 49
 Ion Ratio Lower Upper
 119 100
 134 53.1 12.5 37.5#
 91 551.0 13.8 41.4#

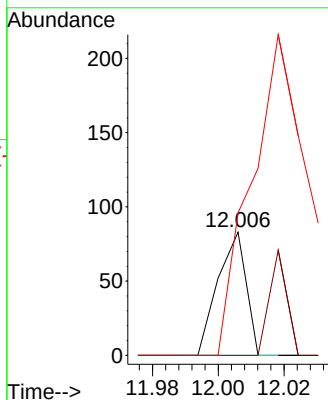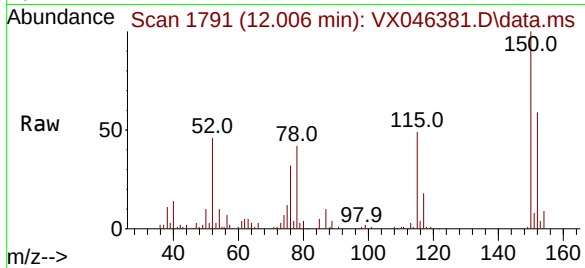

#87
 1,3-Dichlorobenzene
 Concen: 0.015 ug/l
 RT: 12.037 min Scan# 1796
 Delta R.T. 0.067 min
 Lab File: VX046381.D
 Acq: 28 May 2025 13:29

Tgt Ion:146 Resp: 26
 Ion Ratio Lower Upper
 146 100
 111 3361.5 22.1 66.3#
 148 850.0 32.1 96.5#


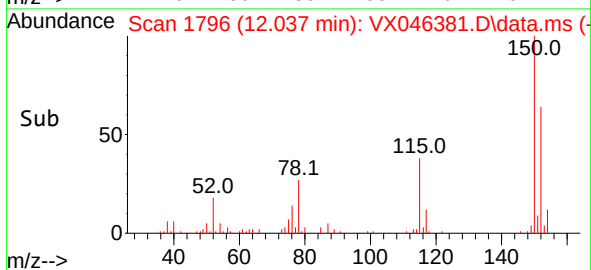
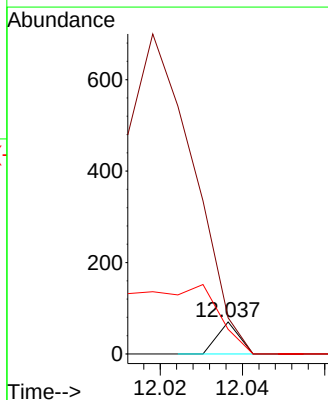
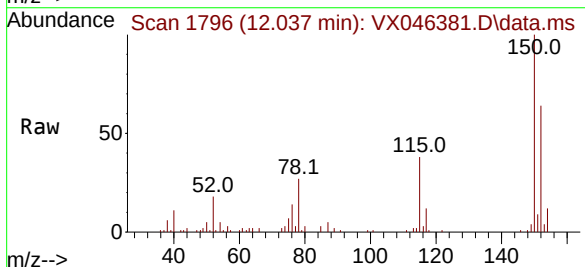




#88
1,4-Dichlorobenzene
Concen: 0.015 ug/l
RT: 12.037 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29

Instrument :
MSVOA_X
ClientSampleId :
TP-3

Tgt Ion:146 Resp: 26
Ion Ratio Lower Upper
146 100
111 3361.5 21.3 63.9#
148 850.0 31.9 95.5#



#95
Naphthalene
Concen: 0.071 ug/l
RT: 13.792 min Scan# 2084
Delta R.T. 0.018 min
Lab File: VX046381.D
Acq: 28 May 2025 13:29

Tgt Ion:128 Resp: 254
Ion Ratio Lower Upper
128 100
127 0.0 10.4 15.6#
129 0.0 8.6 13.0#

