

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX052918\
 Data File : VX002098.D
 Acq On : 29 May 2018 17:33
 Operator : JC/MD
 Sample : J3164-11
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB-01-052418

Quant Time: May 30 13:09:15 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 24 13:09:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	298339	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	416665	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	369960	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	197754	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	195484	36.66	ug/l	0.00
Spiked Amount	50.000		Recovery	=	73.32%	
35) Dibromofluoromethane	5.51	113	149874	35.97	ug/l	0.00
Spiked Amount	50.000		Recovery	=	71.94%	
50) Toluene-d8	8.72	98	593747	39.36	ug/l	0.00
Spiked Amount	50.000		Recovery	=	78.72%	
62) 4-Bromofluorobenzene	11.14	95	207844	35.22	ug/l	0.00
Spiked Amount	50.000		Recovery	=	70.44%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX052918\
Data File : VX002098.D
Acq On : 29 May 2018 17:33
Operator : JC/MD
Sample : J3164-11
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-01-052418

Quant Time: May 30 13:09:15 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Quant Title : SW846 8260
QLast Update : Thu May 24 13:09:03 2018
Response via : Initial Calibration

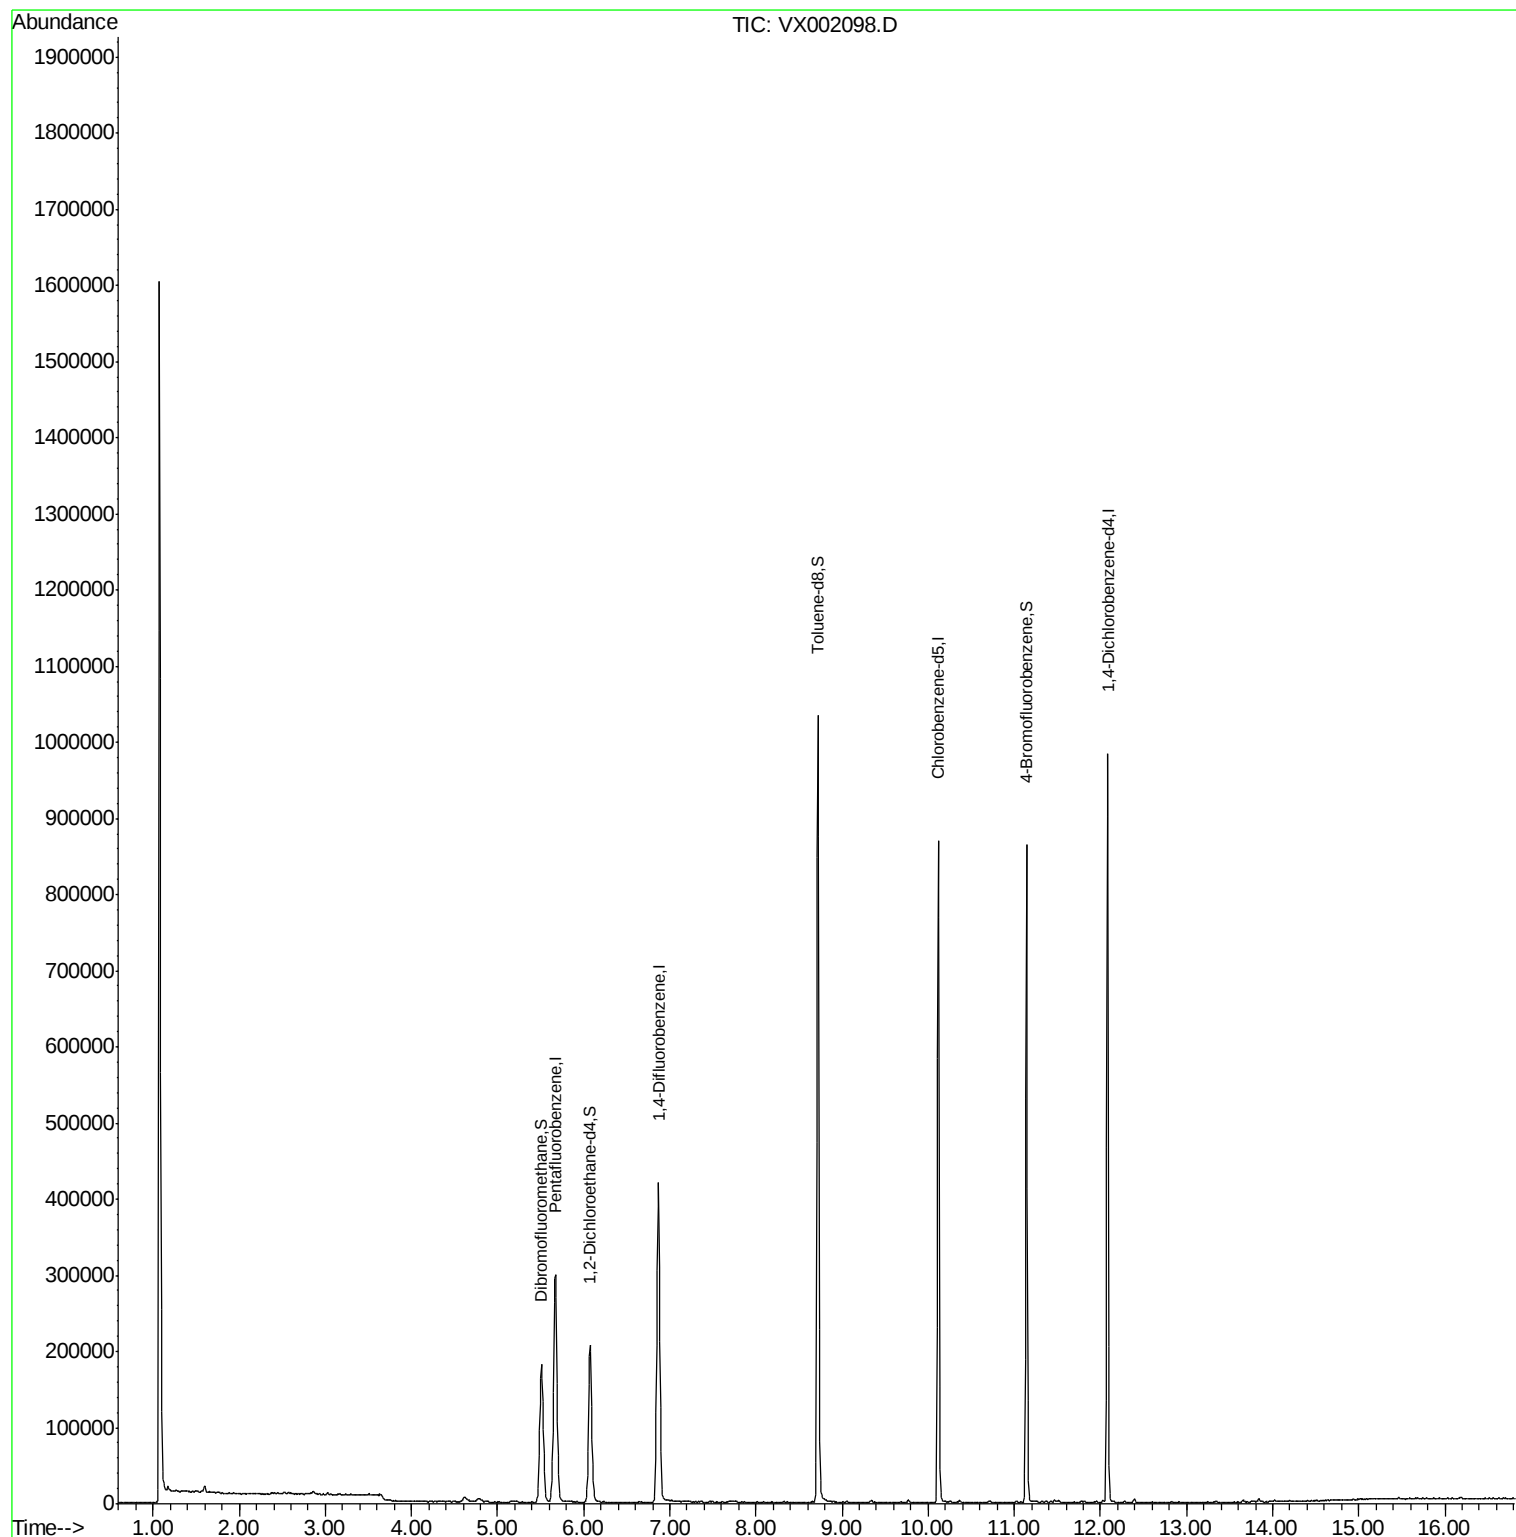



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.00 min

Lab File: VX002098.D

Acq: 29 May 2018 17:33

Instrument :

MSVOA_X

ClientSampleId :


FB-01-052418

Tot Ion:168 Resp: 298339

Ion Ratio Lower Upper

168 100

99 51.7 41.0 61.4

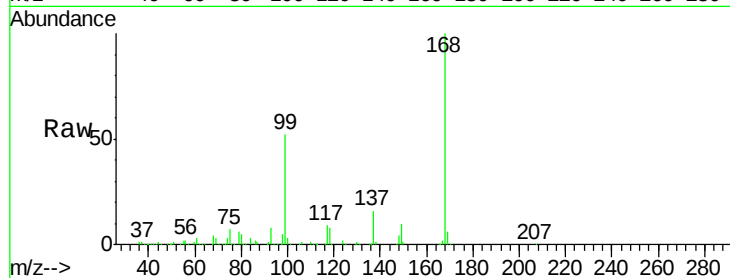

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

120000

100000

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

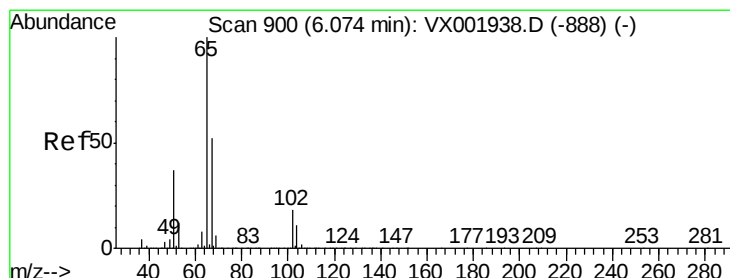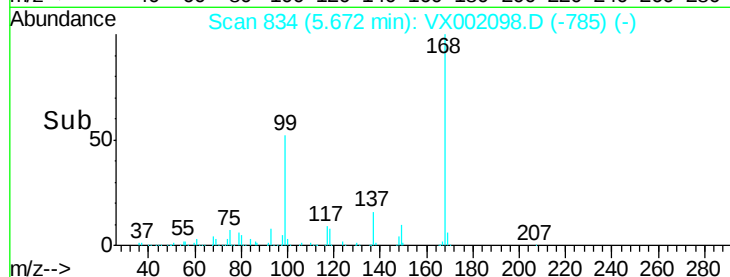

#33

1,2-Dichloroethane-d4

Concen: 36.66 ug/l

RT: 6.07 min Scan# 900

Delta R.T. -0.00 min

Lab File: VX002098.D


Acq: 29 May 2018 17:33

Tgt Ion: 65 Resp: 195484

Ion Ratio Lower Upper

65 100

67 52.0 0.0 104.0

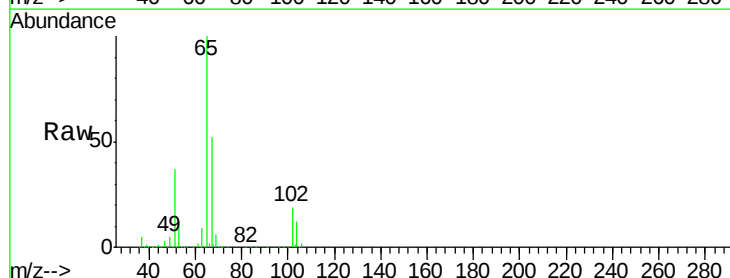

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

80000


60000


40000

20000

0

Time--> 6.00 6.10 6.20

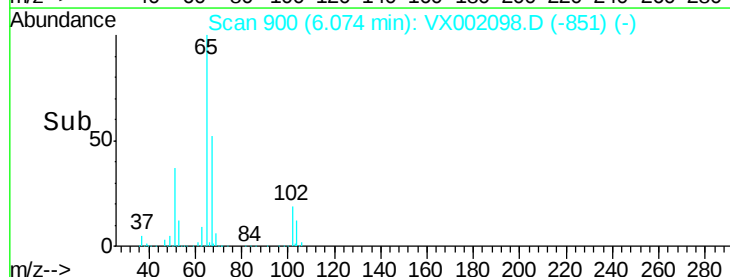

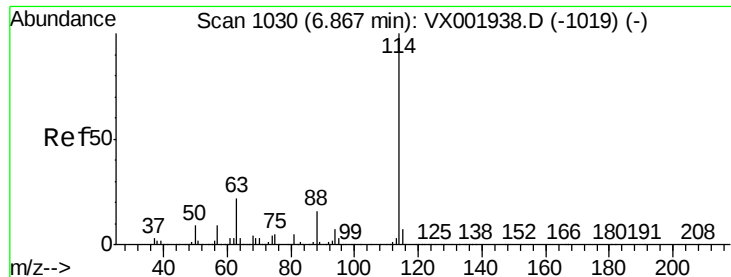

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VX002098.D

Acq: 29 May 2018 17:33

Instrument :

MSVOA_X

ClientSampleId :

FB-01-052418


Tot Ion:114 Resp: 416665

Ion Ratio Lower Upper

114 100

63 22.3 0.0 43.2




88 16.1 0.0 31.6

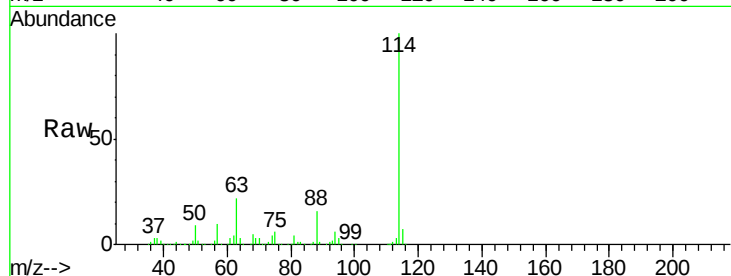

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

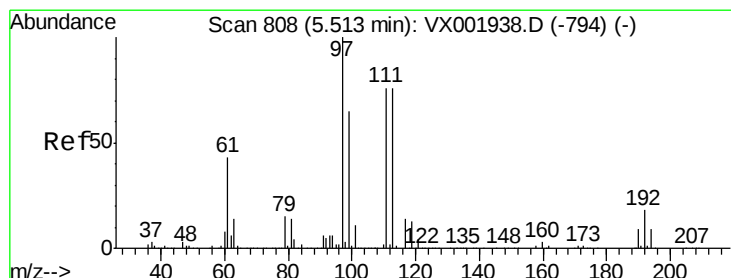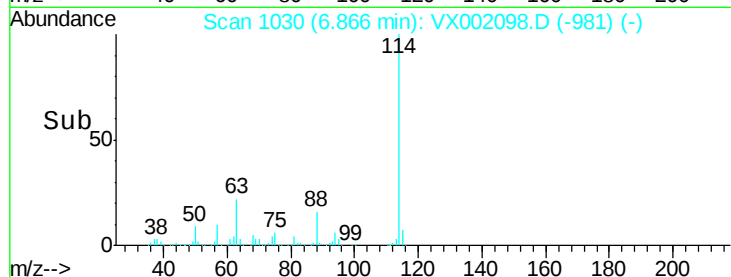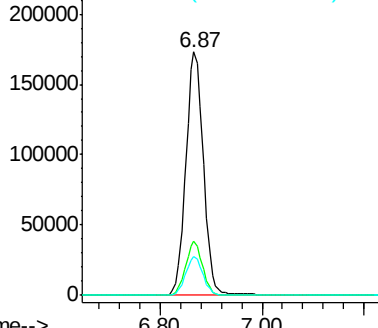

#35

Dibromofluoromethane

Concen: 35.97 ug/l

RT: 5.51 min Scan# 807

Delta R.T. -0.01 min

Lab File: VX002098.D

Acq: 29 May 2018 17:33


Tgt Ion:113 Resp: 149874

Ion Ratio Lower Upper

113 100

111 102.1 82.0 123.0



192 22.9 18.9 28.3

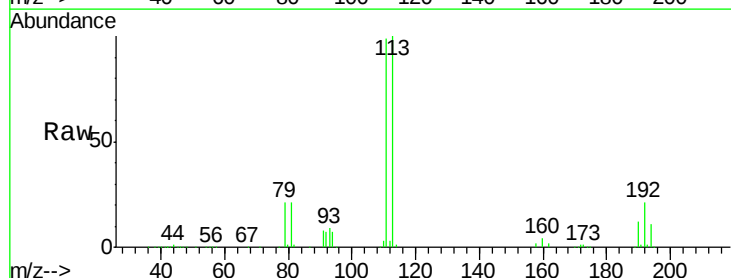


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

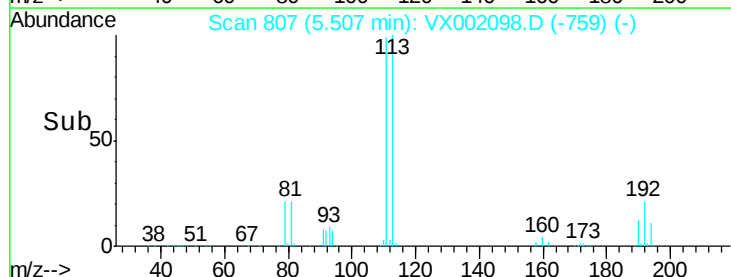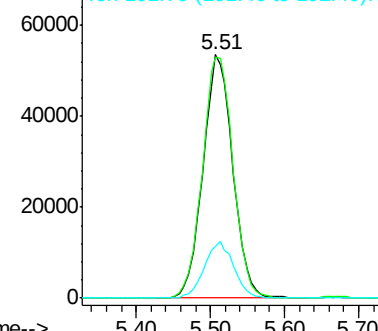

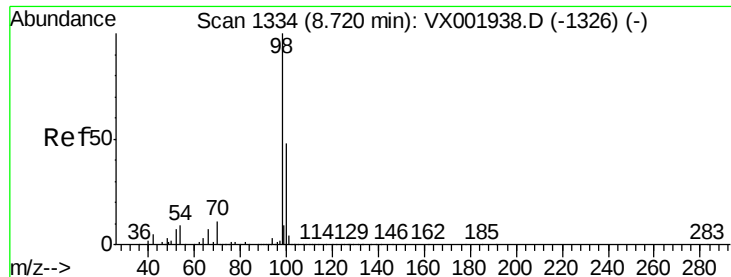

#50

Toluene-d8

Concen: 39.36 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX002098.D

Acq: 29 May 2018 17:33

Instrument :

MSVOA_X

ClientSampleId :


FB-01-052418

Tot Ion: 98 Resp: 593747

Ion Ratio Lower Upper




98 100

100 63.3 51.5 77.3

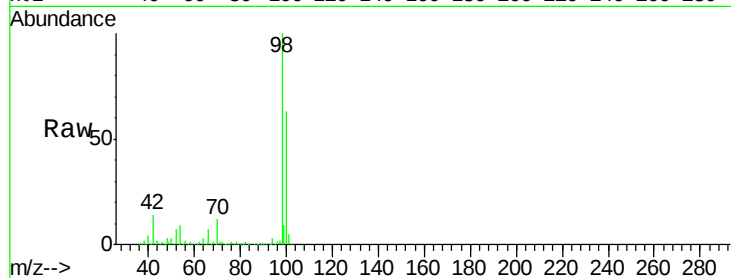

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

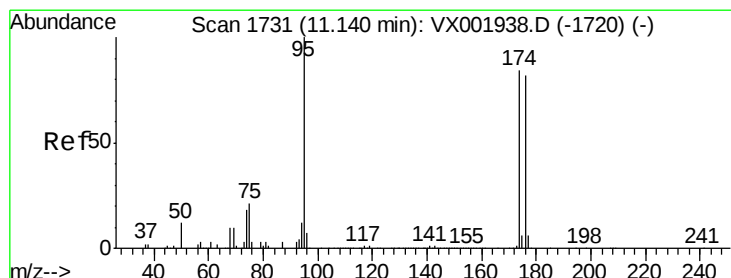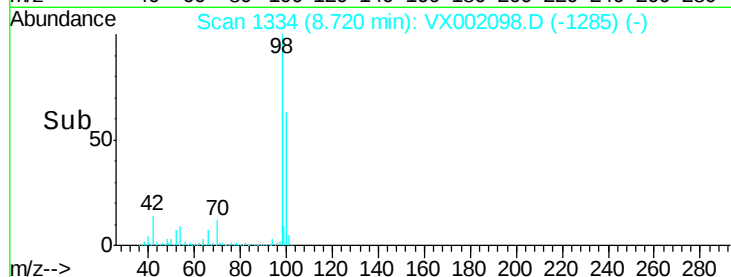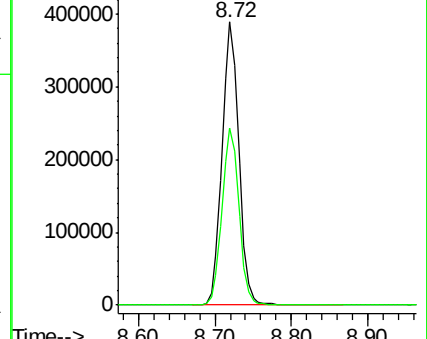

#62

4-Bromofluorobenzene

Concen: 35.22 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.00 min

Lab File: VX002098.D

Acq: 29 May 2018 17:33


Tgt Ion: 95 Resp: 207844

Ion Ratio Lower Upper

95 100

174 90.9 0.0 178.8



176 88.3 0.0 175.6

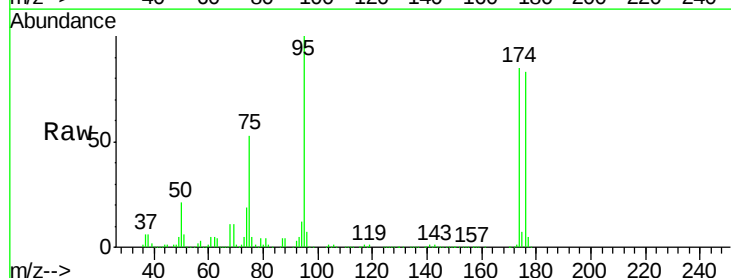


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

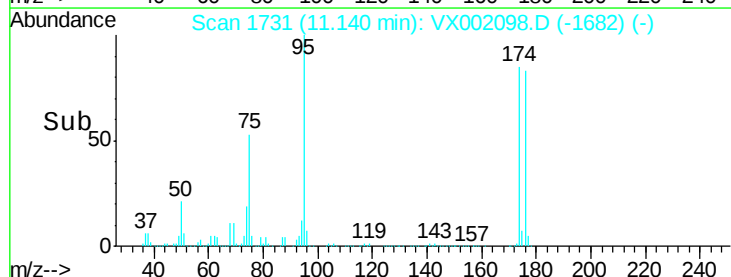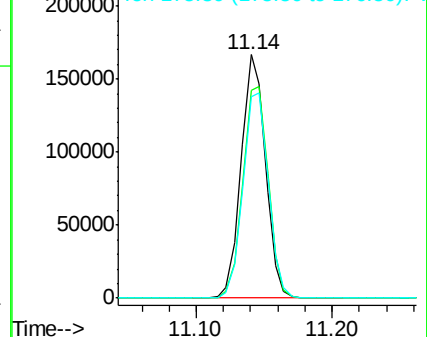

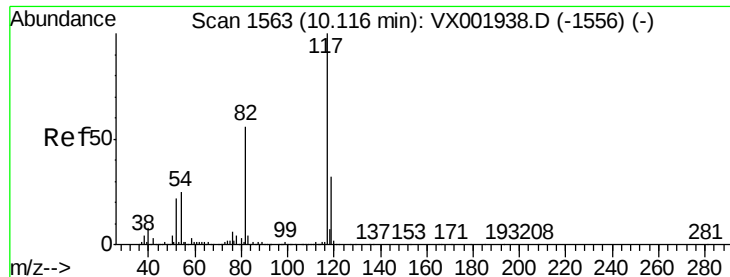

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 10.12 min Scan# 1563

Delta R.T. -0.00 min

Lab File: VX002098.D

Acq: 29 May 2018 17:33

Instrument :

MSVOA_X

ClientSampleId :

FB-01-052418


Tot Ion:117 Resp: 369960

Ion Ratio Lower Upper

117 100

82 55.9 44.8 67.2




119 32.0 25.5 38.3

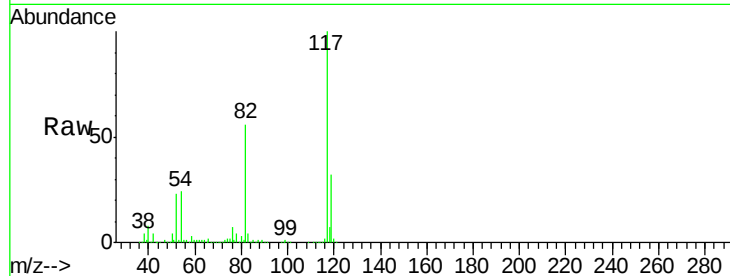

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

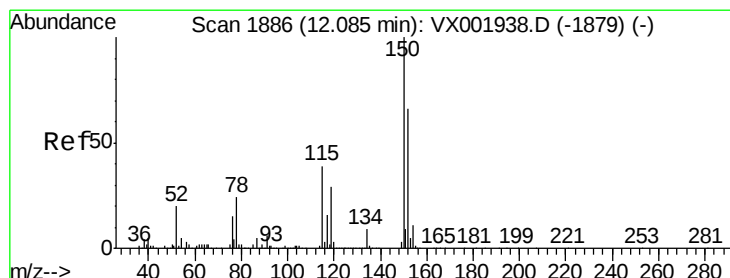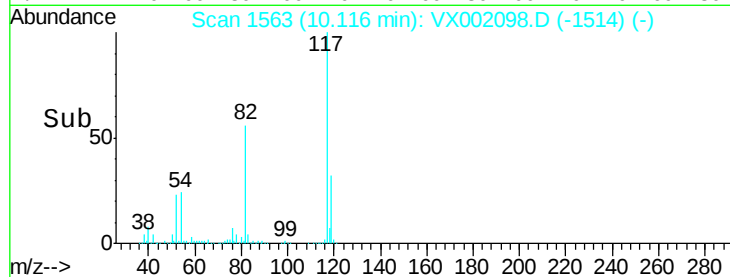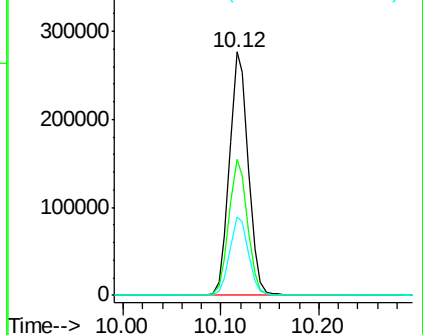

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.09 min Scan# 1886

Delta R.T. -0.00 min

Lab File: VX002098.D

Acq: 29 May 2018 17:33


Tgt Ion:152 Resp: 197754

Ion Ratio Lower Upper

152 100

115 56.2 42.3 126.8

150 157.5 0.0 351.0

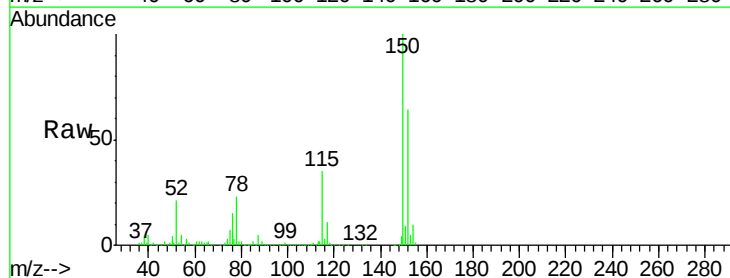

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

