


Data Path : W:\HPCHEM1\MSVOA X\Data\VX052918\
Data File : VX002108.D
Acq On : 29 May 2018 22:26
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Title : SW846 8260
Last Update : Thu May 24 13:09:03 2018

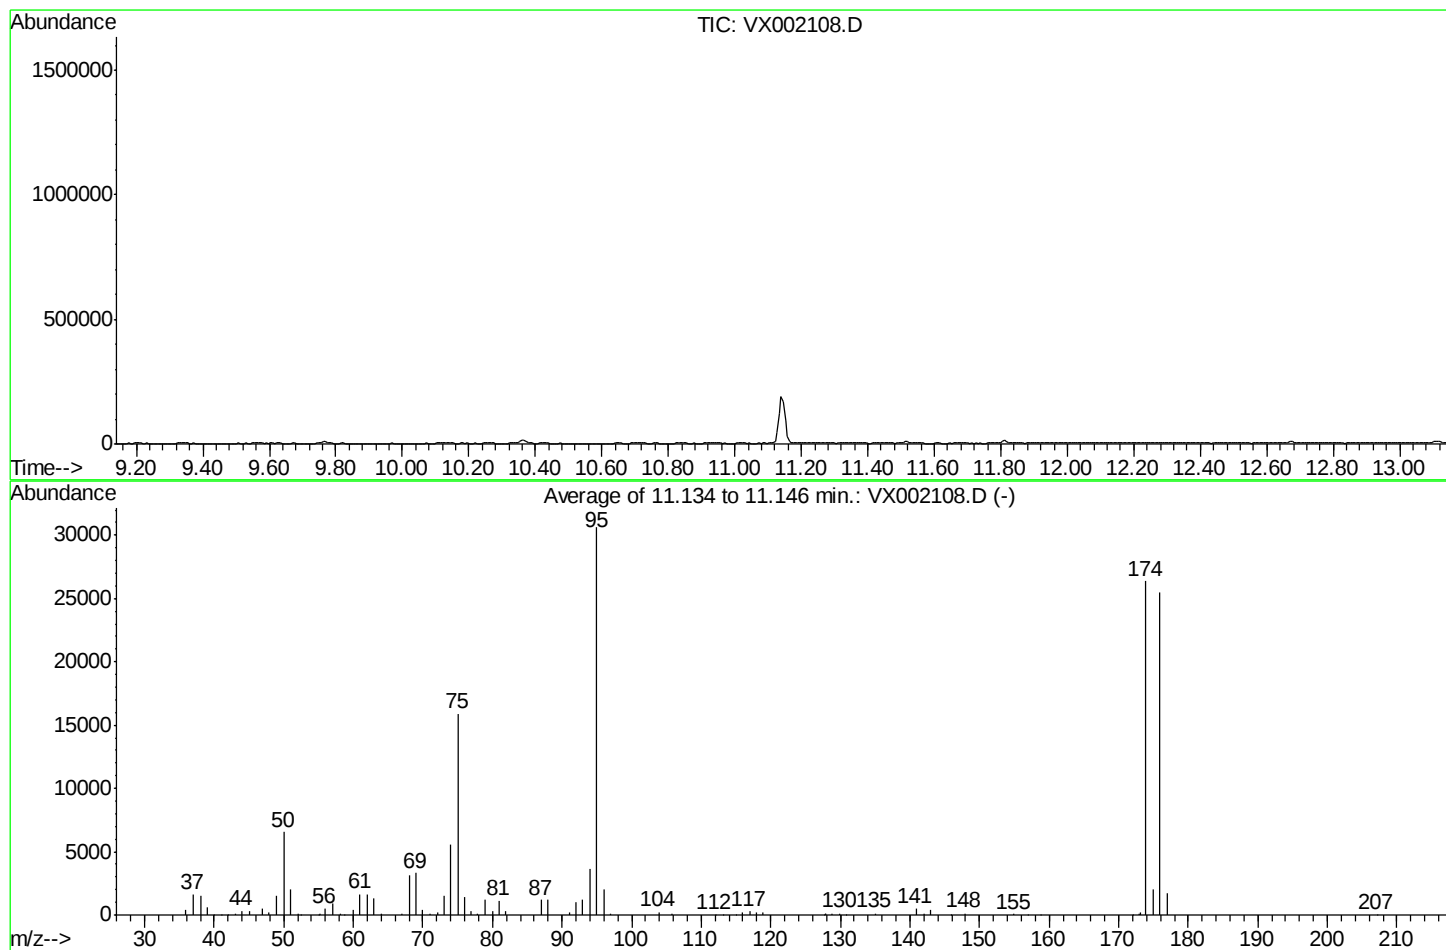

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	6527	PASS
75	95	30	60	51.9	15894	PASS
95	95	100	100	100.0	30626	PASS
96	95	5	9	6.6	2012	PASS
173	174	0.00	2	0.9	238	PASS
174	95	50	100	86.1	26360	PASS
175	174	5	9	7.6	2000	PASS
176	174	95	101	96.5	25448	PASS
177	176	5	9	6.6	1677	PASS