

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX053018\
 Data File : VX002135.D
 Acq On : 30 May 2018 12:26
 Operator : JC/MD
 Sample : VX0530WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0530WBL01

Quant Time: May 31 05:17:31 2018
 Quant Method : W:\HPCHEM1\MSVOA X\METHOD\624X052518W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri May 25 02:17:15 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.02	128	52546	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	6.87	114	307125	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.12	117	268891	30.00	ug/l	0.00

System Monitoring Compounds

27) 1,2-Dichloroethane-d4	6.07	65	129097	31.22	ug/l	-0.01
Spiked Amount	30.000	Range	50 - 169	Recovery	=	104.07%
60) 4-Bromofluorobenzene	11.14	95	126546	27.49	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	91.63%
63) Toluene-d8	8.72	98	366592	30.59	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	101.97%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX053018\
Data File : VX002135.D
Acq On : 30 May 2018 12:26
Operator : JC/MD
Sample : VX0530WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0530WBL01

Quant Time: May 31 05:17:31 2018
Quant Method : W:\HPCHEM1\MSVOA X\METHOD\624X052518W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri May 25 02:17:15 2018
Response via : Initial Calibration

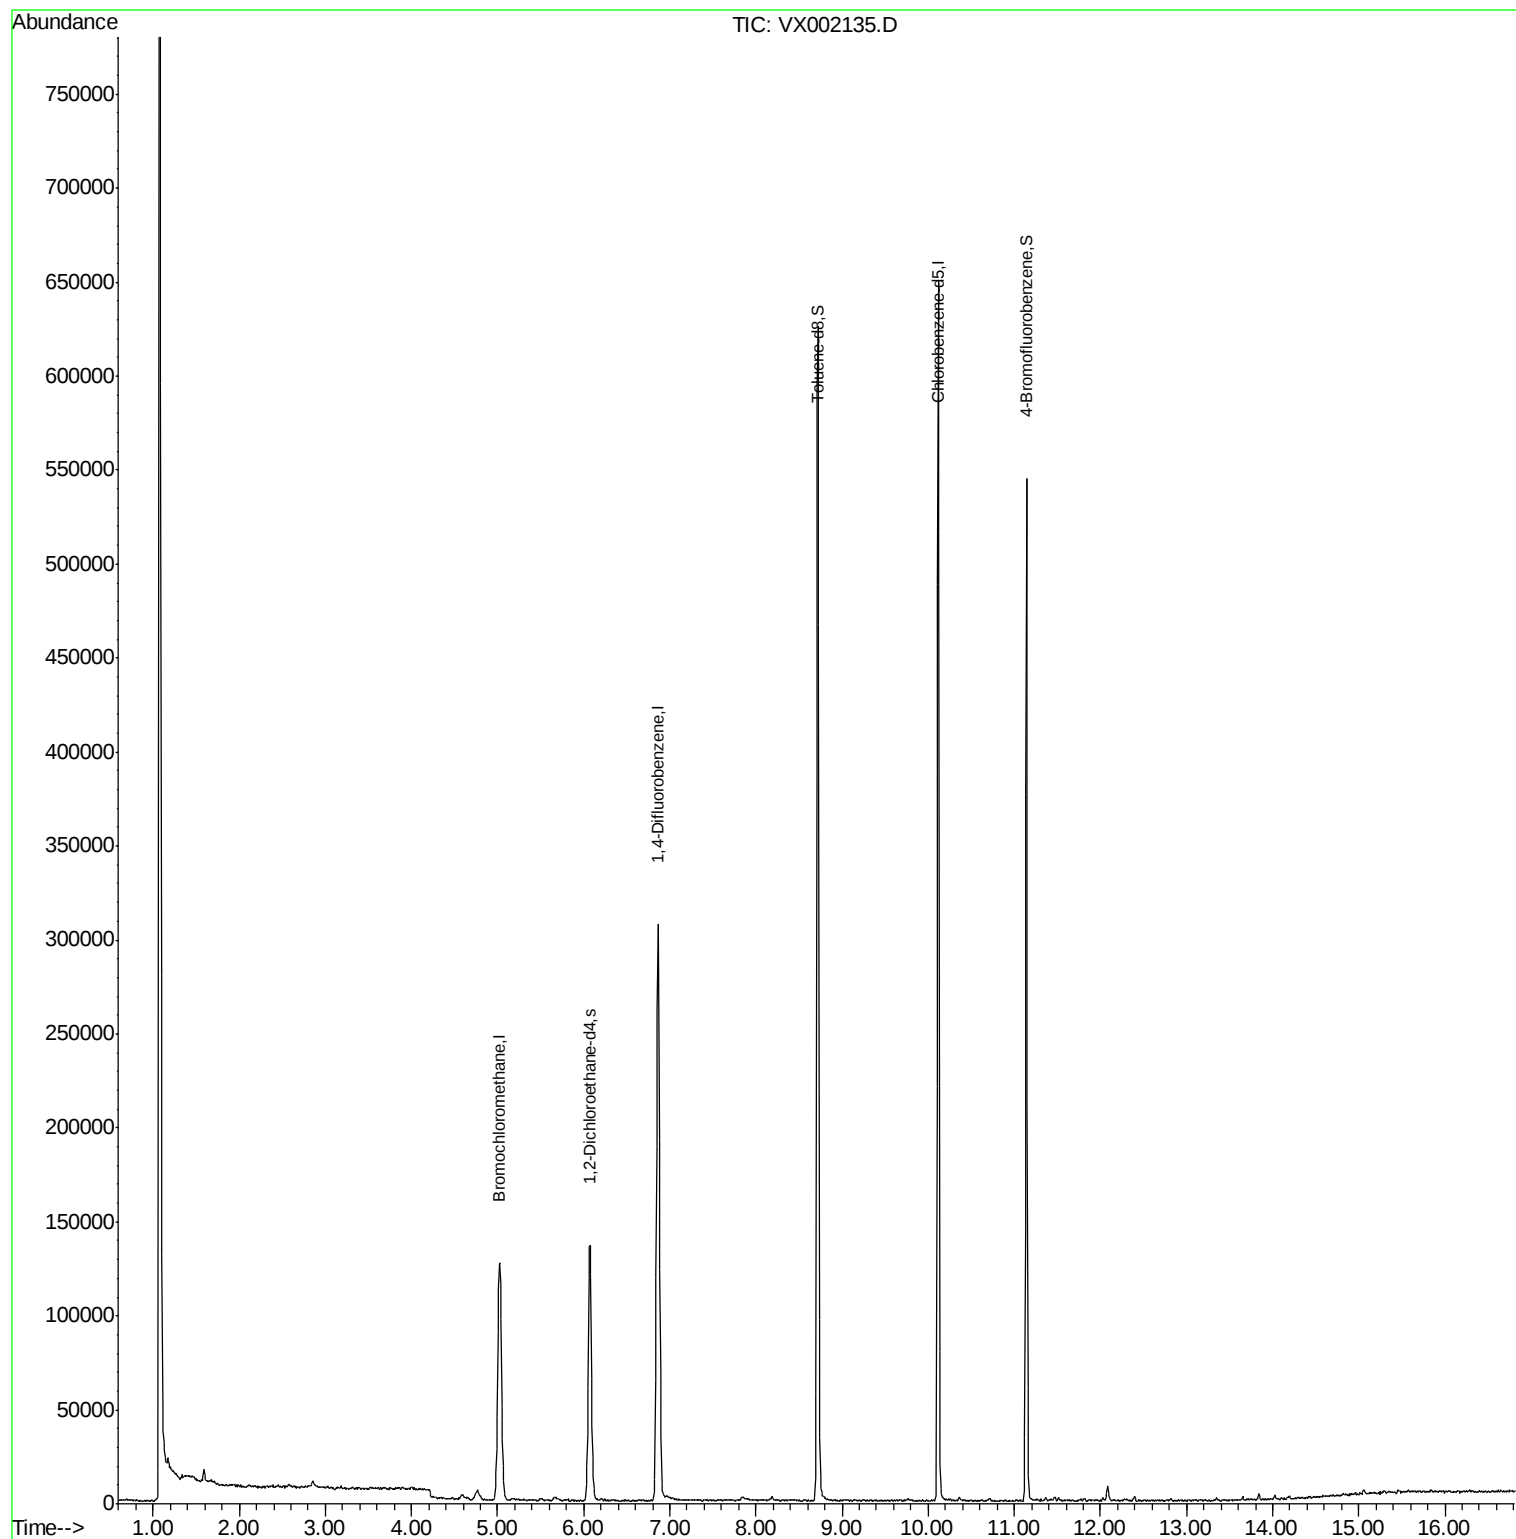

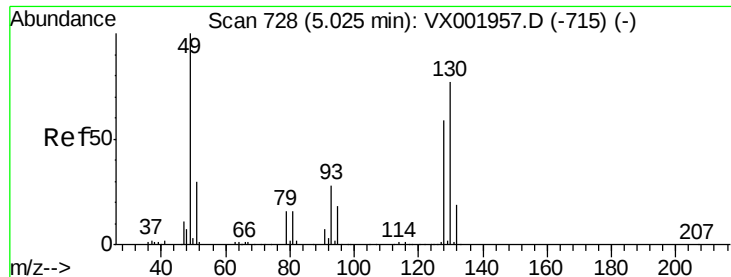

#1

Bromochloromethane

Concen: 30.00 ug/l

RT: 5.02 min Scan# 727

Delta R.T. -0.01 min

Lab File: VX002135.D

Acq: 30 May 2018 12:26

Instrument :

MSVOA_X

ClientSampleId :

VX0530WBL01


Tot Ion:128 Resp: 52546

Ion Ratio Lower Upper

128 100

49 170.7 0.0 423.0




130 128.6 0.0 324.3

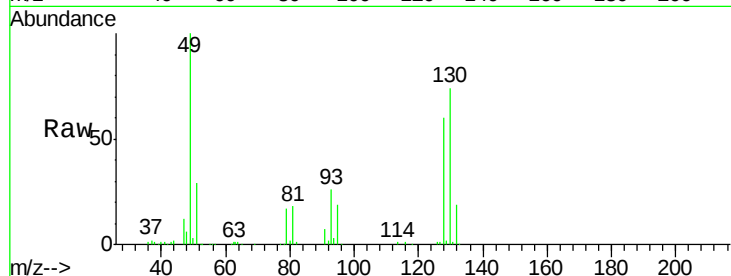

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VX0

Ion 130.00 (129.70 to 130.70): V

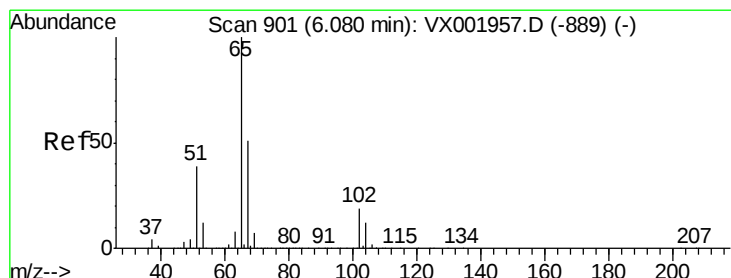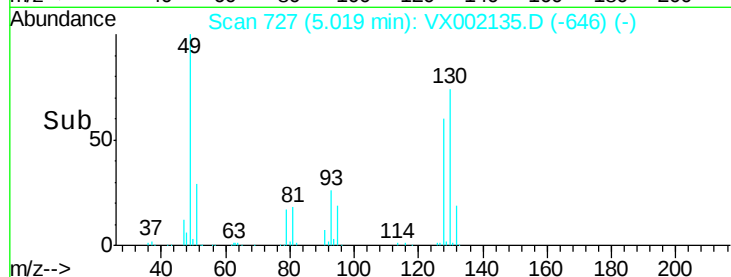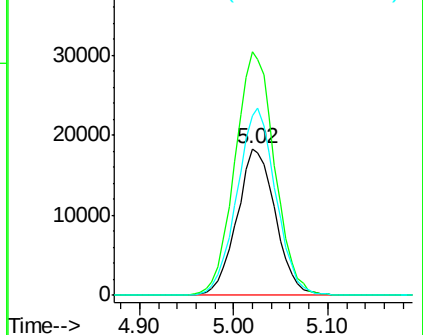

#27

1,2-Dichloroethane-d4

Concen: 31.22 ug/l

RT: 6.07 min Scan# 899

Delta R.T. -0.01 min

Lab File: VX002135.D


Acq: 30 May 2018 12:26

Tgt Ion: 65 Resp: 129097

Ion Ratio Lower Upper



65 100


67 52.2 40.9 61.3

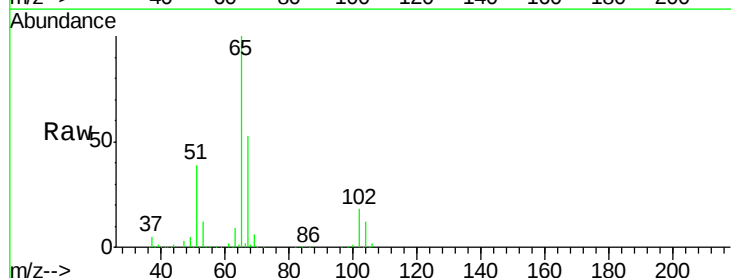

Abundance Ion 65.00 (64.70 to 65.70): VX0

Ion 67.00 (66.70 to 67.70): VX0



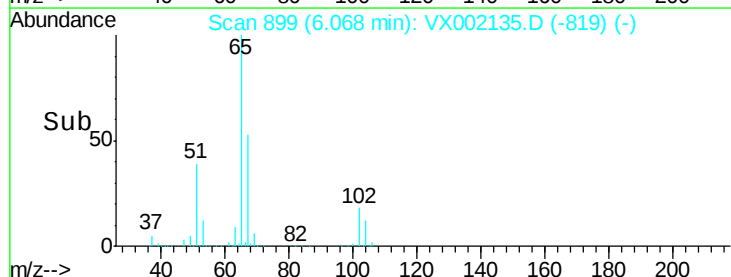
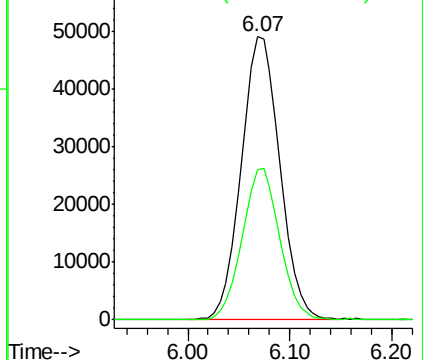


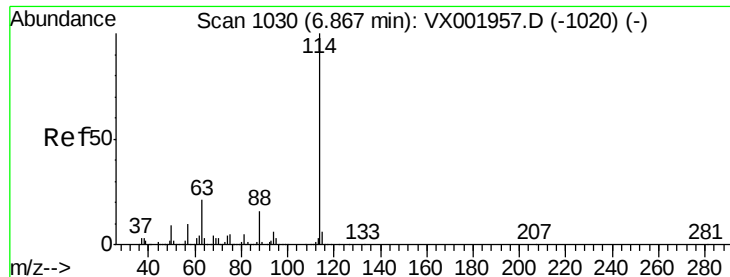

#28
 1,4-Difluorobenzene
 Concen: 30.00 ug/l
 RT: 6.87 min Scan# 1030
 Delta R.T. 0.00 min
 Lab File: VX002135.D
 Acq: 30 May 2018 12:26




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0530WBL01


Tot Ion	Ratio	Lower	Upper
114	100		
63	21.5	17.1	25.7
88	15.4	12.6	19.0

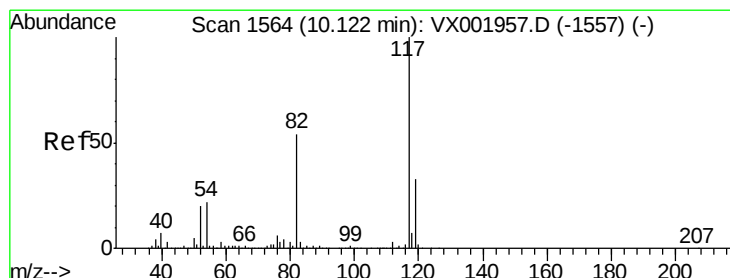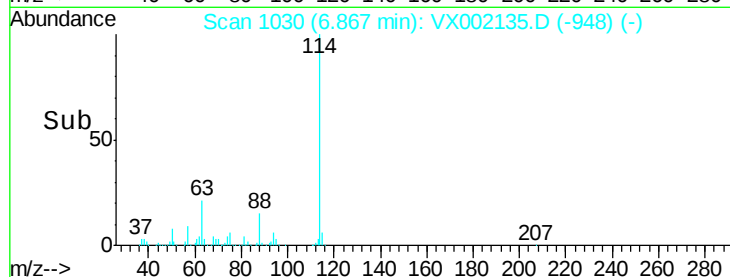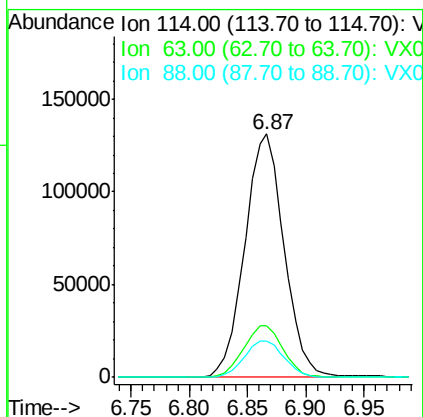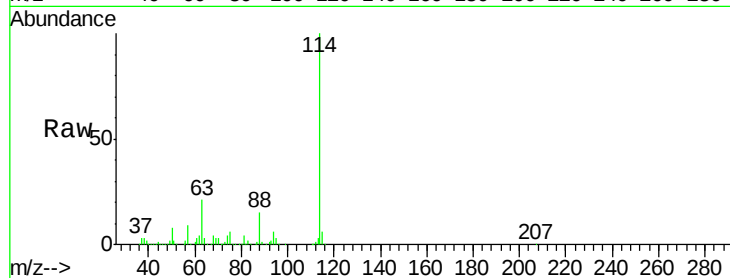

#57
 Chlorobenzene-d5
 Concen: 30.00 ug/l
 RT: 10.12 min Scan# 1563
 Delta R.T. -0.01 min
 Lab File: VX002135.D
 Acq: 30 May 2018 12:26

Tgt Ion	Ratio	Lower	Upper
117	100		
82	55.3	44.3	66.5
119	32.7	25.7	38.5


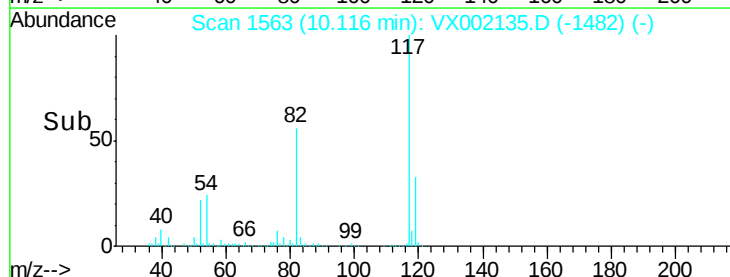
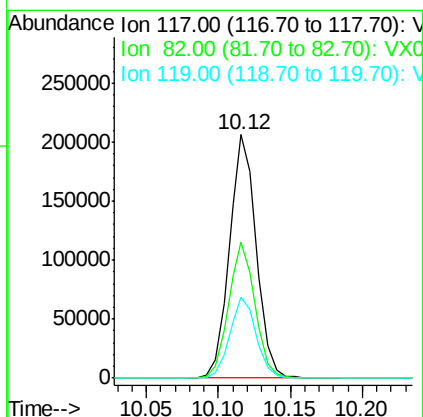
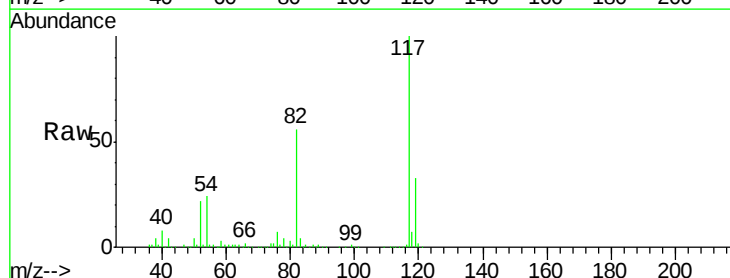


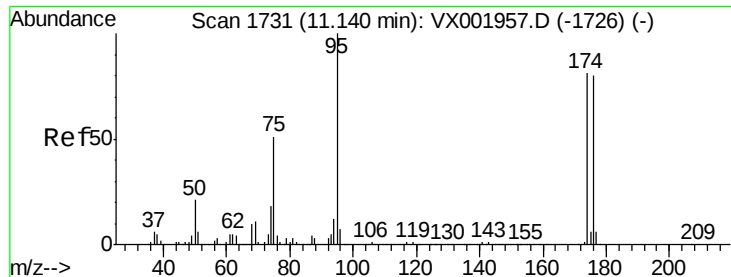

#60
4-Bromofluorobenzene
Concen: 27.49 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. 0.00 min
Lab File: VX002135.D
Acq: 30 May 2018 12:26

Instrument :
MSVOA_X
ClientSampled :
VX0530WBL01

Tot Ion: 95 Resp: 126546
Ion Ratio Lower Upper
95 100
174 91.6 71.8 107.6
176 89.5 70.1 105.1

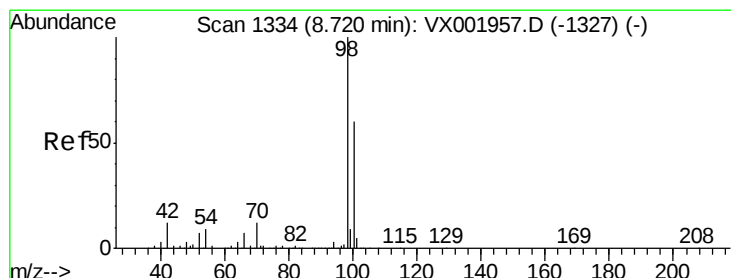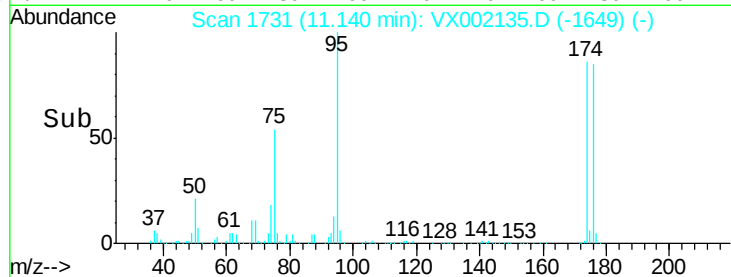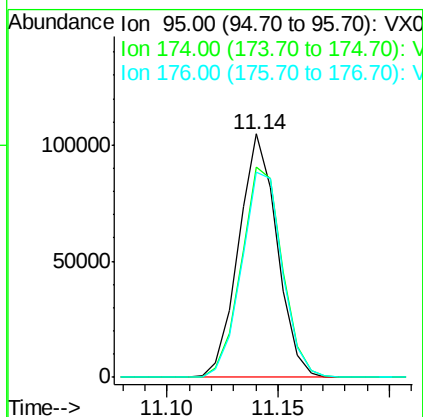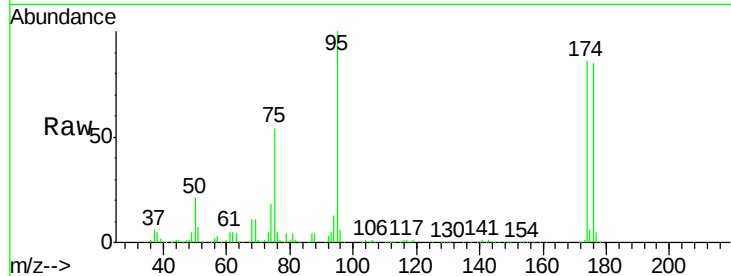

#63
Toluene-d8
Concen: 30.59 ug/l
RT: 8.72 min Scan# 1334
Delta R.T. 0.00 min
Lab File: VX002135.D
Acq: 30 May 2018 12:26

Tgt Ion: 98 Resp: 366592
Ion Ratio Lower Upper
98 100
100 63.8 50.8 76.2

