

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX053018\
 Data File : VX002143.D
 Acq On : 30 May 2018 17:23
 Operator : JC/MD
 Sample : VX0530WBL02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0530WBL02

Quant Time: May 31 04:01:07 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 24 13:09:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	292898	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	421028	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	376856	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	209749	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	257028	49.09	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.18%	
35) Dibromofluoromethane	5.51	113	194431	46.18	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.36%	
50) Toluene-d8	8.72	98	763842	50.11	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.22%	
62) 4-Bromofluorobenzene	11.14	95	275960	46.27	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.54%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX053018\
Data File : VX002143.D
Acq On : 30 May 2018 17:23
Operator : JC/MD
Sample : VX0530WBL02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0530WBL02

Quant Time: May 31 04:01:07 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Quant Title : SW846 8260
QLast Update : Thu May 24 13:09:03 2018
Response via : Initial Calibration

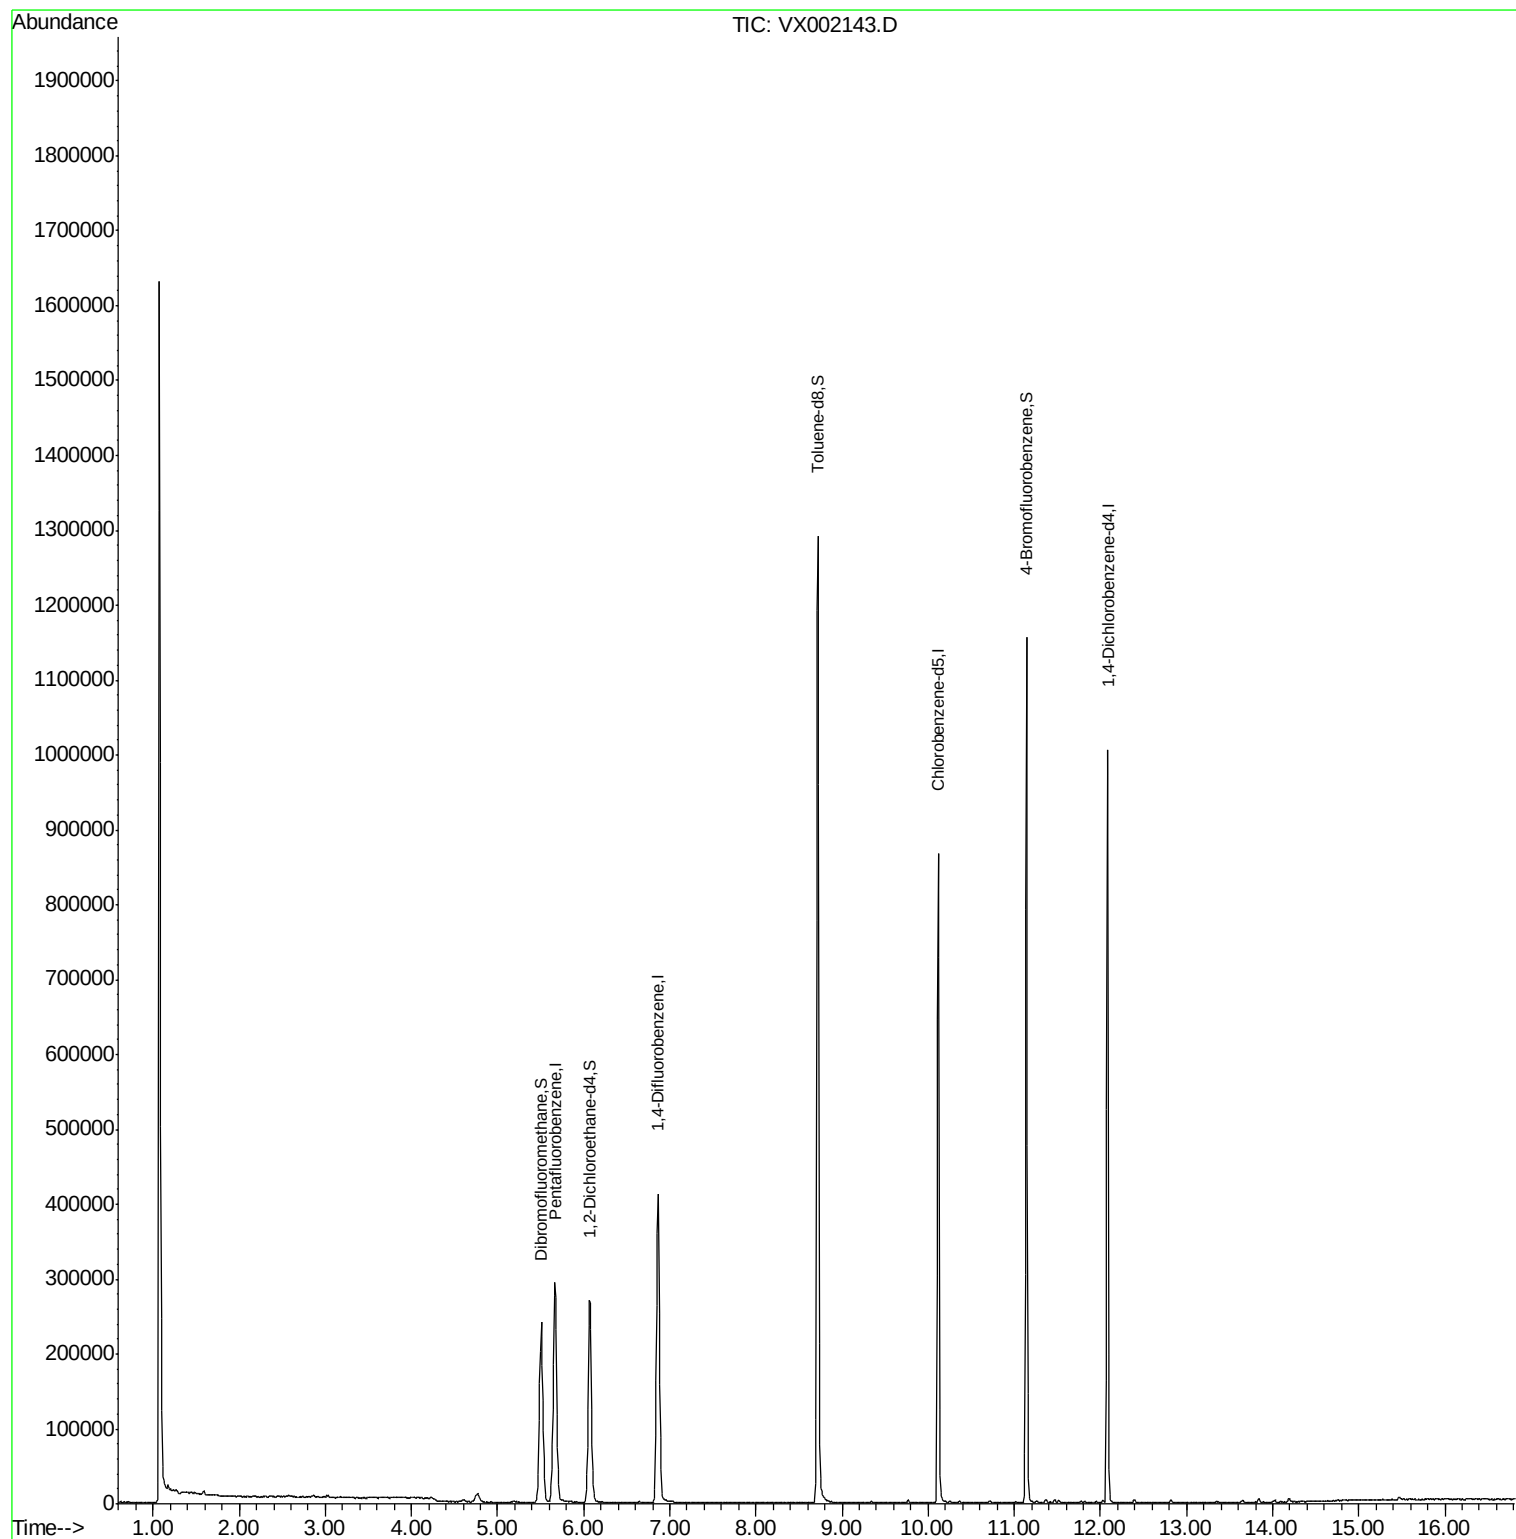

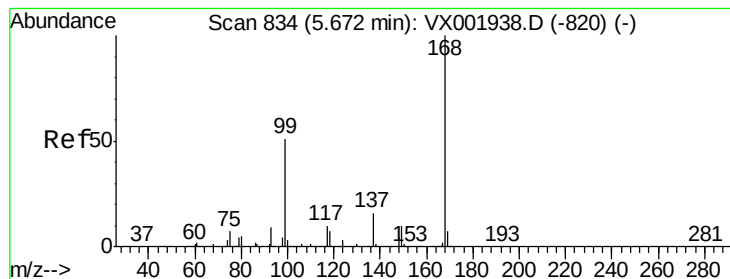

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.01 min

Lab File: VX002143.D

Acq: 30 May 2018 17:23

Instrument :

MSVOA_X

ClientSampleId :


VX0530WBL02

Tot Ion:168 Resp: 292898

Ion Ratio Lower Upper

168 100

99 52.4 41.0 61.4

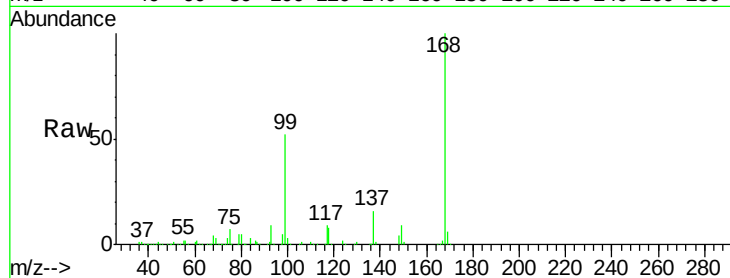

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

120000

100000

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

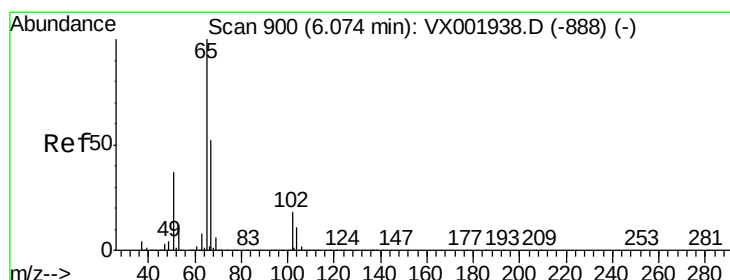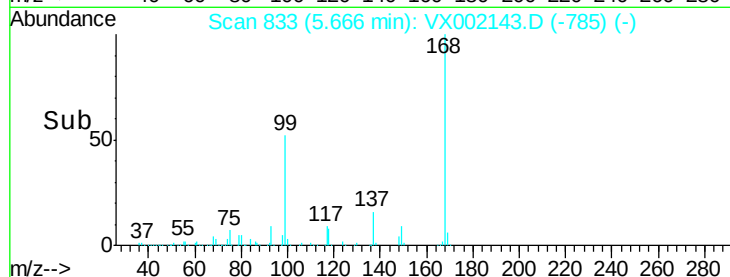

#33

1,2-Dichloroethane-d4

Concen: 49.09 ug/l

RT: 6.07 min Scan# 899

Delta R.T. -0.01 min

Lab File: VX002143.D


Acq: 30 May 2018 17:23

Tgt Ion: 65 Resp: 257028

Ion Ratio Lower Upper

65 100

67 52.1 0.0 104.0

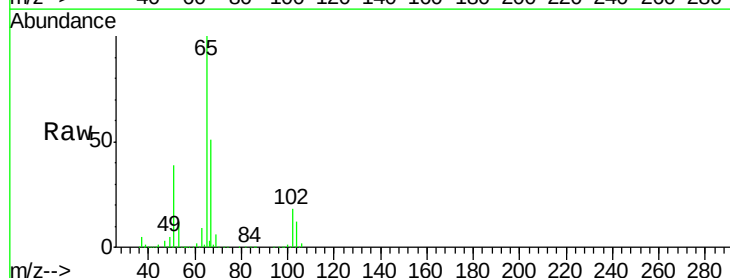

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

100000

80000


60000


40000

20000

0

Time--> 5.90 6.00 6.10 6.20 6.30

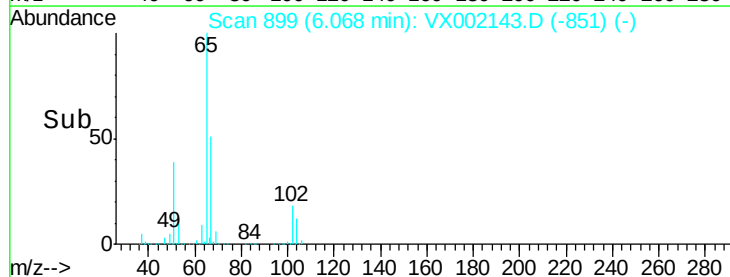

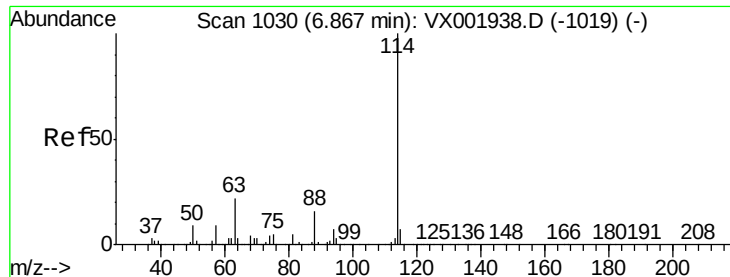

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.86 min Scan# 1029

Delta R.T. -0.01 min

Lab File: VX002143.D

Acq: 30 May 2018 17:23

Instrument :

MSVOA_X

ClientSampleId :

VX0530WBL02


Tot Ion:114 Resp: 421028

Ion Ratio Lower Upper

114 100

63 21.2 0.0 43.2




88 15.1 0.0 31.6

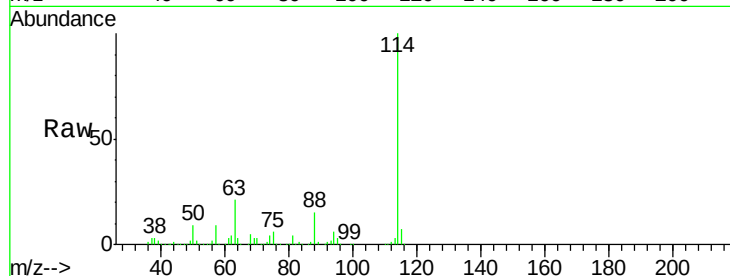

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

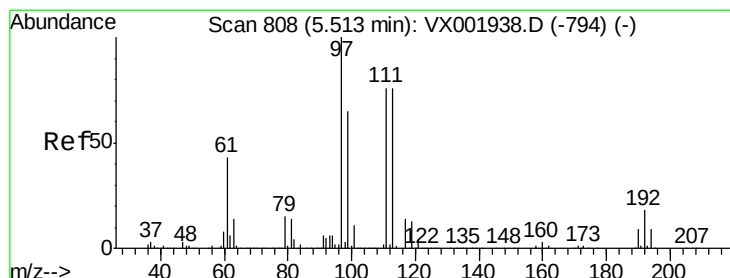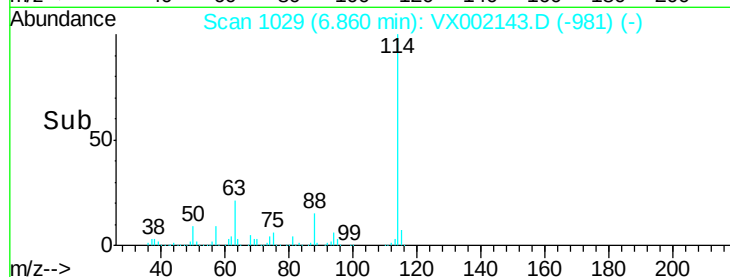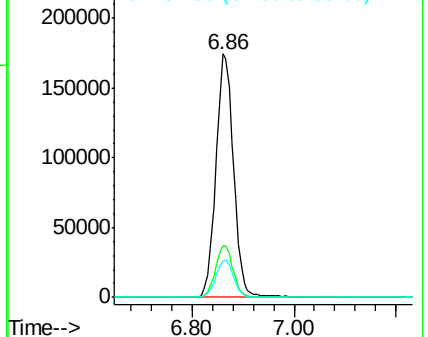

#35

Dibromofluoromethane

Concen: 46.18 ug/l

RT: 5.51 min Scan# 807

Delta R.T. -0.01 min

Lab File: VX002143.D

Acq: 30 May 2018 17:23


Tgt Ion:113 Resp: 194431

Ion Ratio Lower Upper

113 100

111 103.0 82.0 123.0



192 23.2 18.9 28.3

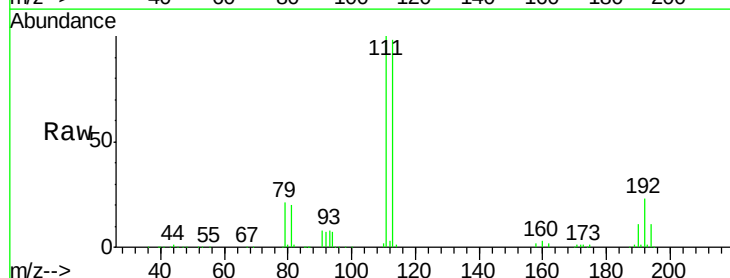


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

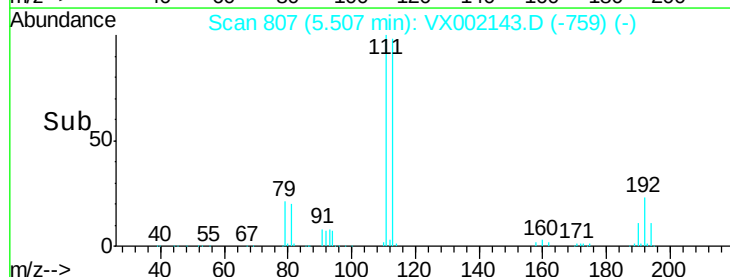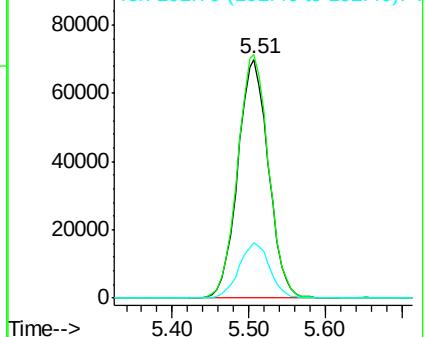

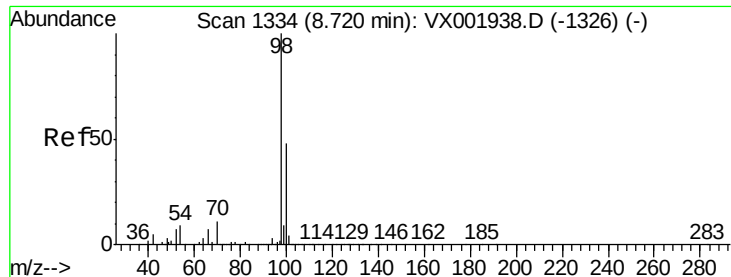

#50

Toluene-d8

Concen: 50.11 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX002143.D

Acq: 30 May 2018 17:23

Instrument :

MSVOA_X

ClientSampleId :





VX0530WBL02

Tot Ion: 98 Resp: 763842

Ion Ratio Lower Upper

98 100

100 63.5 51.5 77.3

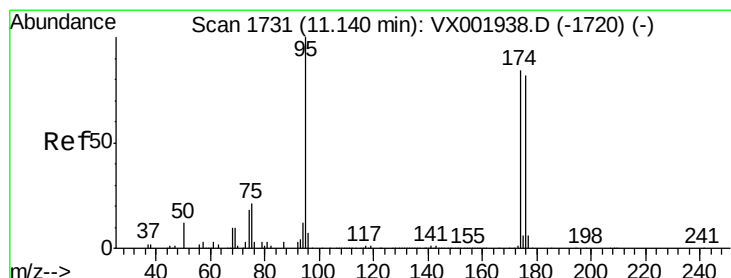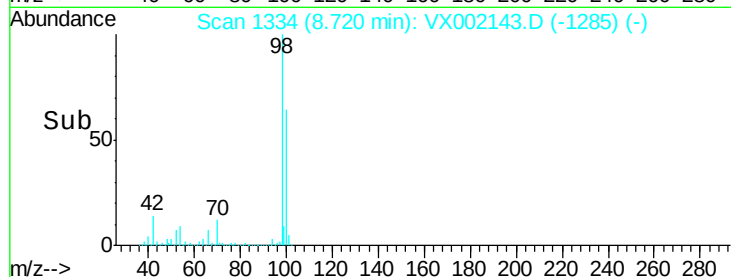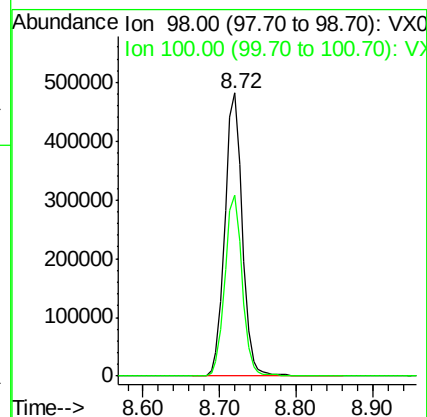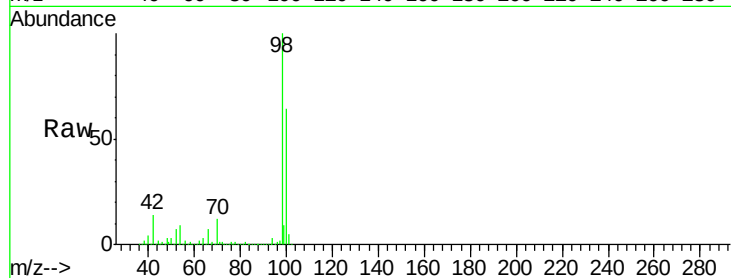

#62

4-Bromofluorobenzene

Concen: 46.27 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.00 min

Lab File: VX002143.D

Acq: 30 May 2018 17:23




Tgt Ion: 95 Resp: 275960


Ion Ratio Lower Upper

95 100

174 91.4 0.0 178.8

176 89.0 0.0 175.6


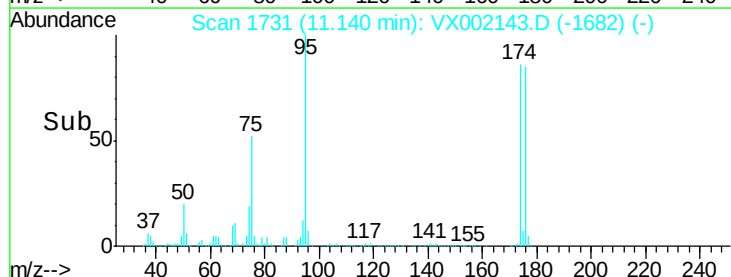
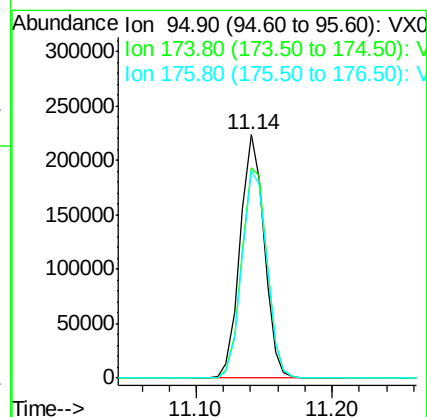
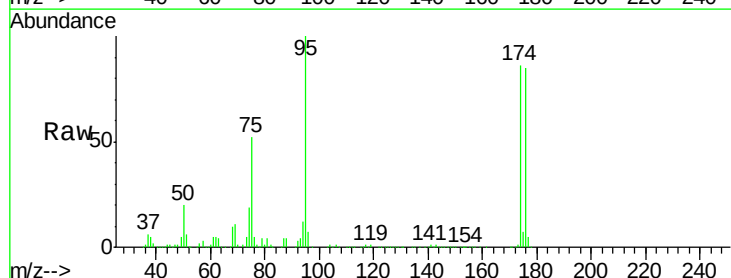


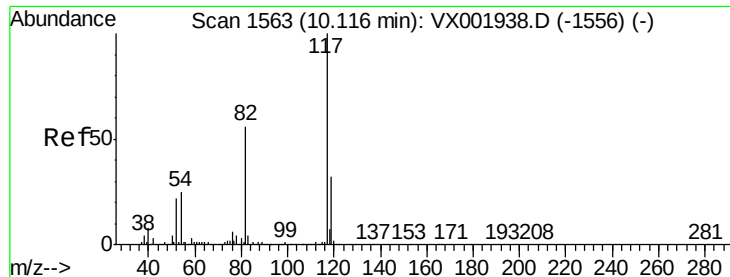

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. -0.00 min
Lab File: VX002143.D
Acq: 30 May 2018 17:23

Instrument :
MSVOA_X
ClientSampleId :
VX0530WBL02

Tot Ion	Ratio	Lower	Upper
117	100		
82	56.0	44.8	67.2
119	32.0	25.5	38.3

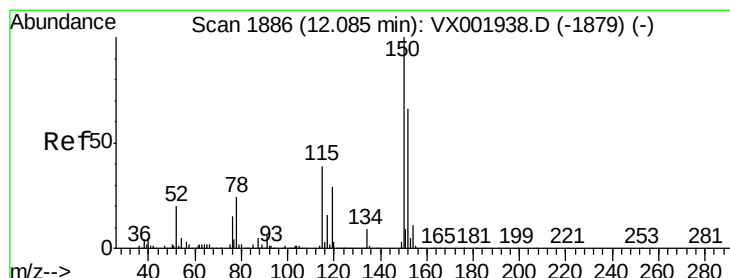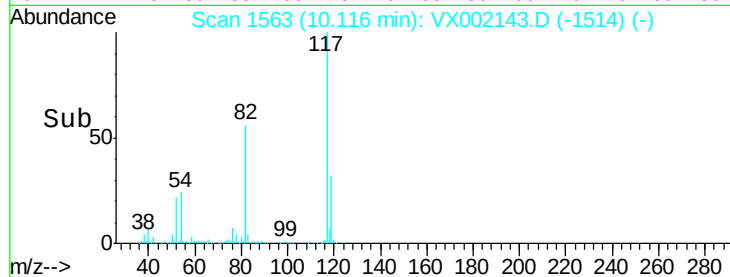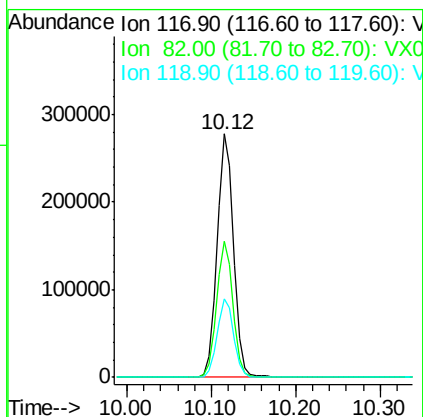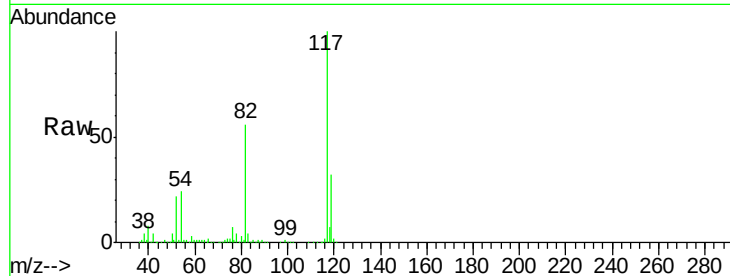

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.09 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX002143.D
Acq: 30 May 2018 17:23

Tgt Ion	Ratio	Lower	Upper
152	100		
115	55.6	42.3	126.8
150	157.4	0.0	351.0

