

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX053018\
 Data File : VX002149.D
 Acq On : 30 May 2018 20:52
 Operator : JC/MD
 Sample : J3093-02 5X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 14B-2

Quant Time: May 31 05:34:35 2018
 Quant Method : W:\HPCHEM1\MSVOA X\METHOD\624X052518W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri May 25 02:17:15 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.03	128	50087	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	6.87	114	289138	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.12	117	252765	30.00	ug/l	0.00

System Monitoring Compounds

27) 1,2-Dichloroethane-d4	6.07	65	124145	31.50	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	105.00%
60) 4-Bromofluorobenzene	11.14	95	115506	26.69	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	88.97%
63) Toluene-d8	8.72	98	344483	30.58	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	101.93%

Target Compounds


					Ovalue
25) Chloroform	5.22	83	336079	61.15	ug/l 99
41) Bromodichloromethane	7.90	83	54064	11.76	ug/l 99
53) Dibromochloromethane	9.59	129	4534	1.17	ug/l 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX053018\
Data File : VX002149.D
Acq On : 30 May 2018 20:52
Operator : JC/MD
Sample : J3093-02 5X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
14B-2

Quant Time: May 31 05:34:35 2018
Quant Method : W:\HPCHEM1\MSVOA X\METHOD\624X052518W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri May 25 02:17:15 2018
Response via : Initial Calibration

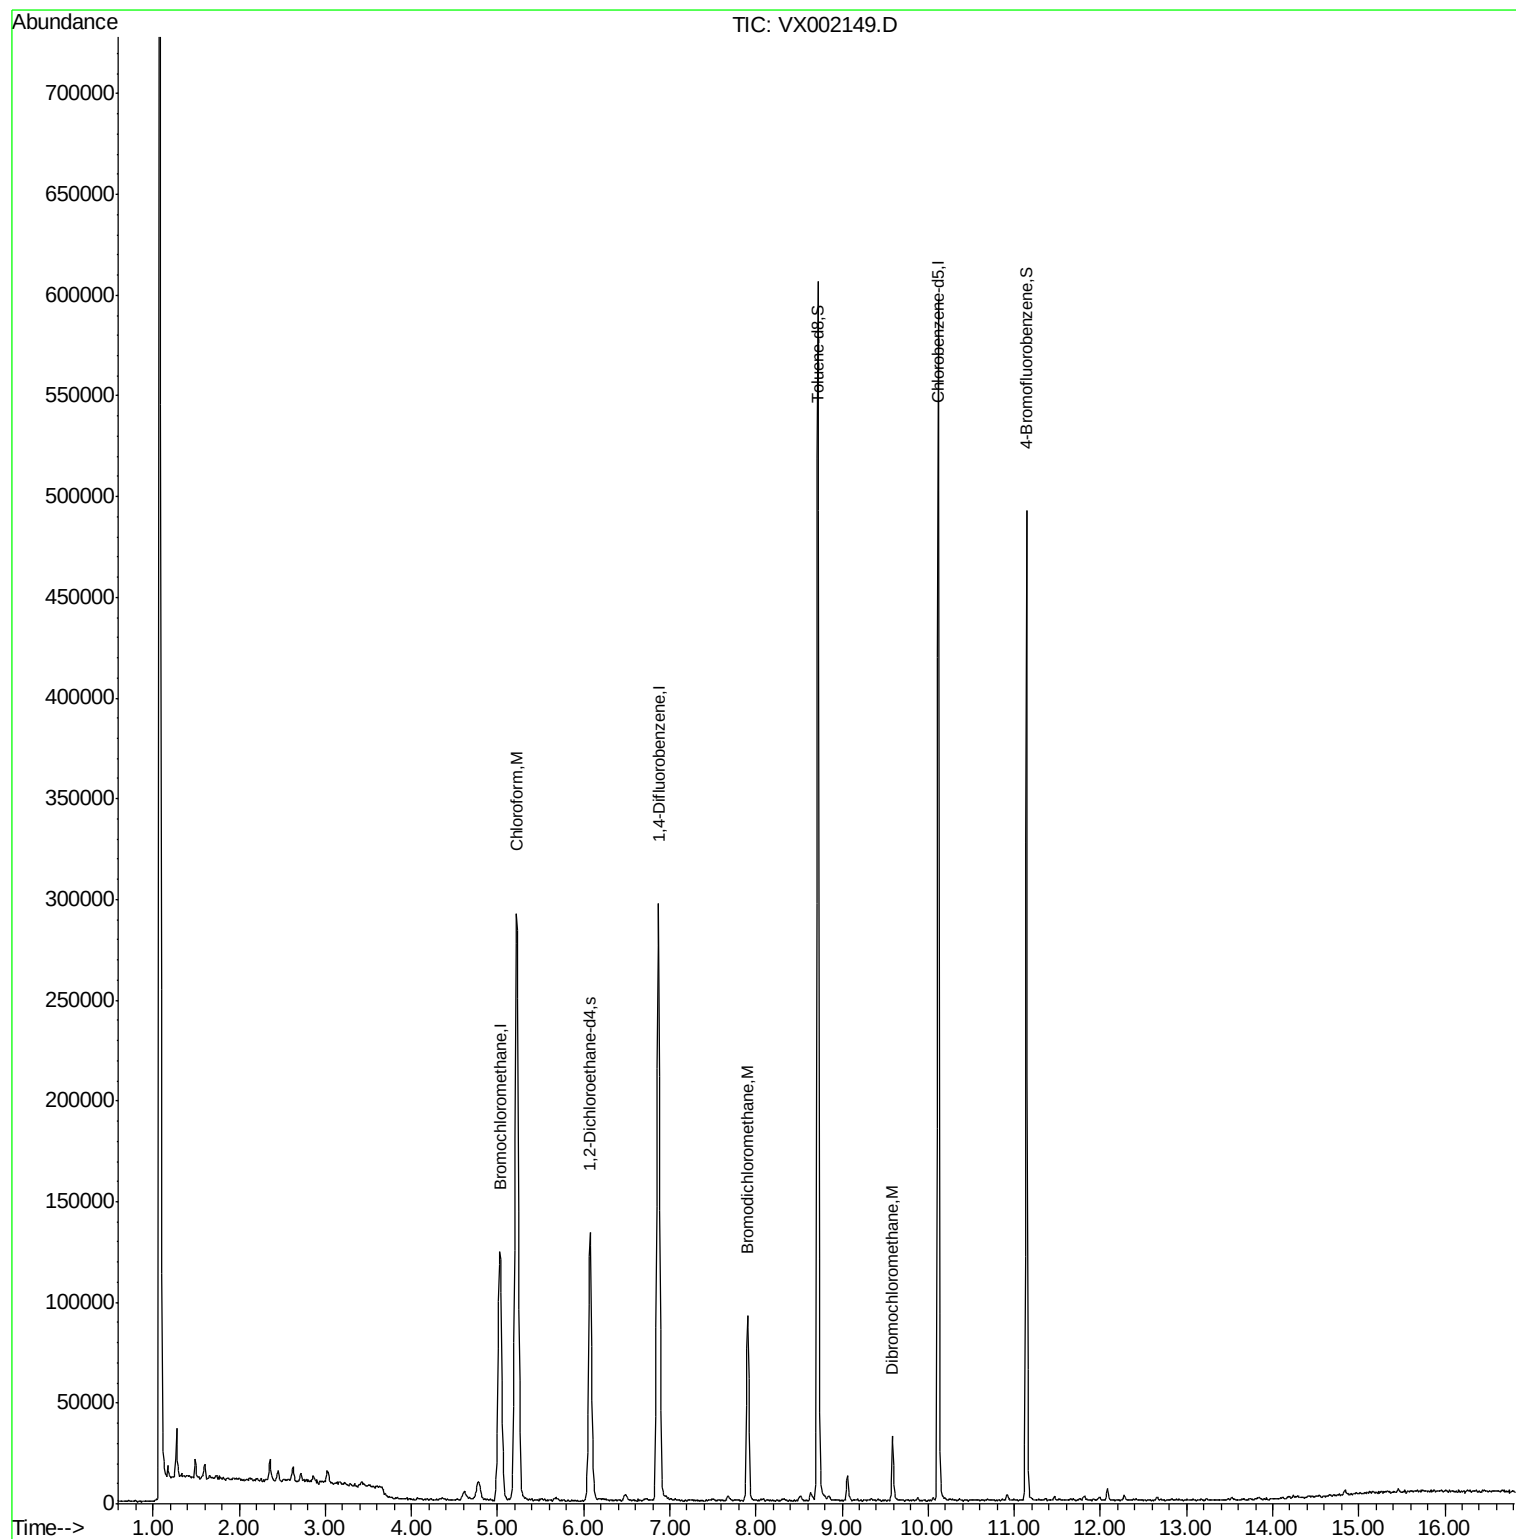

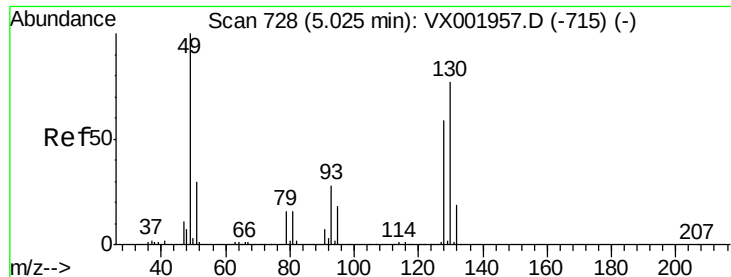

#1

Bromochloromethane

Concen: 30.00 ug/l

RT: 5.03 min Scan# 728

Delta R.T. -0.00 min

Lab File: VX002149.D

Acq: 30 May 2018 20:52

Instrument :

MSVOA_X

ClientSampleId :

14B-2


Tot Ion:128 Resp: 50087

Ion Ratio Lower Upper

128 100

49 173.9 0.0 423.0




130 130.0 0.0 324.3

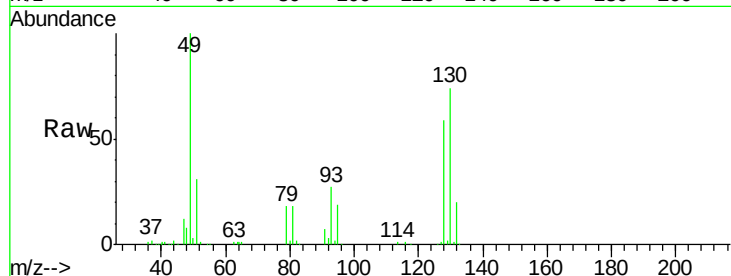

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VX0

Ion 130.00 (129.70 to 130.70): V

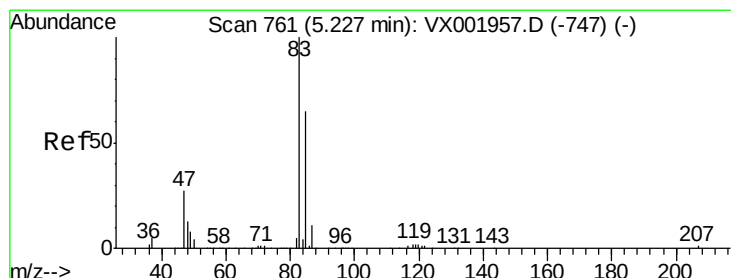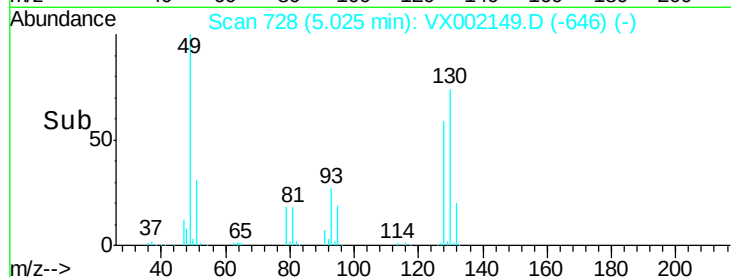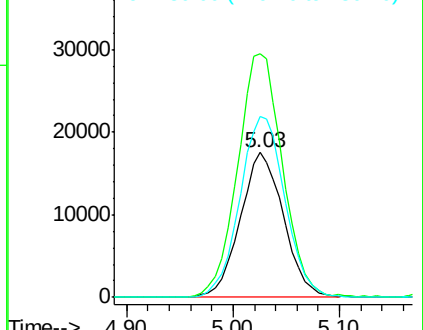

#25

Chloroform

Concen: 61.15 ug/l

RT: 5.22 min Scan# 760

Delta R.T. -0.01 min

Lab File: VX002149.D


Acq: 30 May 2018 20:52

Tgt Ion: 83 Resp: 336079

Ion Ratio Lower Upper



83 100


85 64.0 51.9 77.9

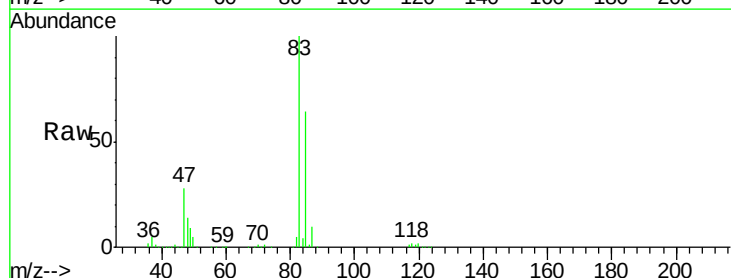

Abundance Ion 83.00 (82.70 to 83.70): VX0

Ion 85.00 (84.70 to 85.70): VX0



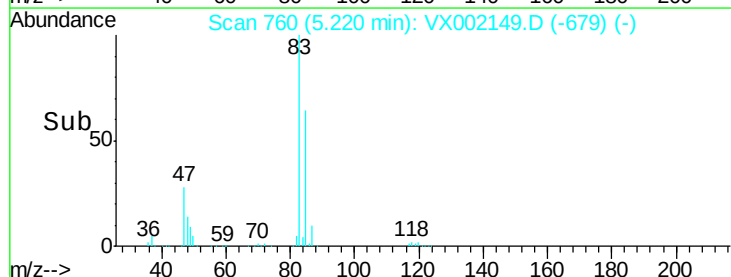
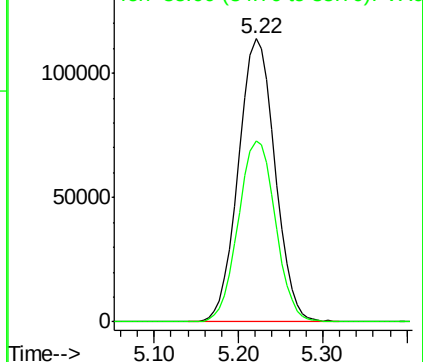


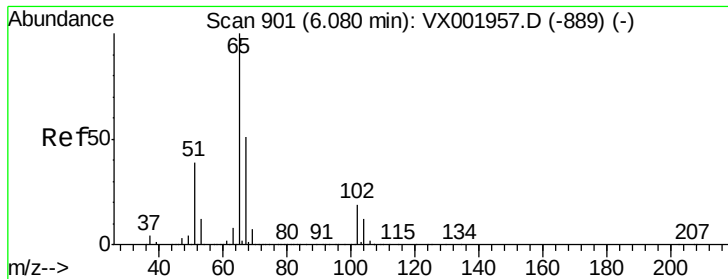

#27
 1,2-Dichloroethane-d4
 Concen: 31.50 ug/l
 RT: 6.07 min Scan# 900
 Delta R.T. -0.01 min
 Lab File: VX002149.D
 Acq: 30 May 2018 20:52




Instrument :
 MSVOA_X
 ClientSampled :
 14B-2


Tot Ion: 65 Resp: 124145
 Ion Ratio Lower Upper
 65 100
 67 51.4 40.9 61.3

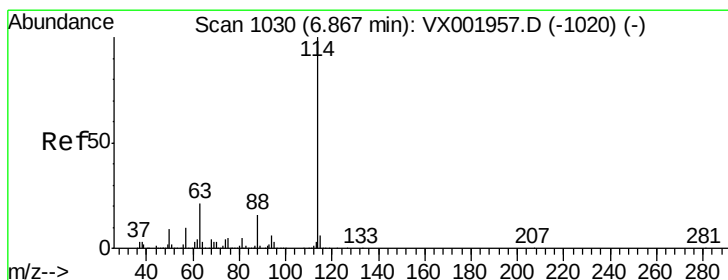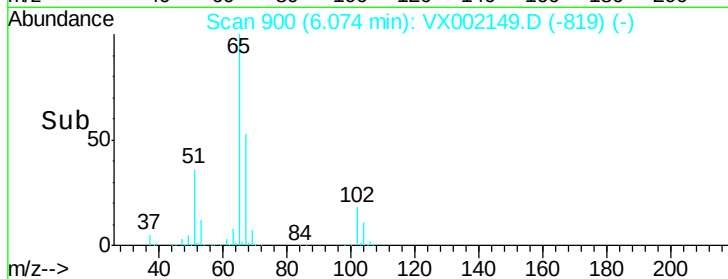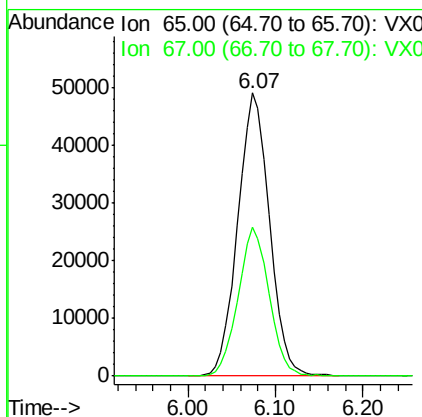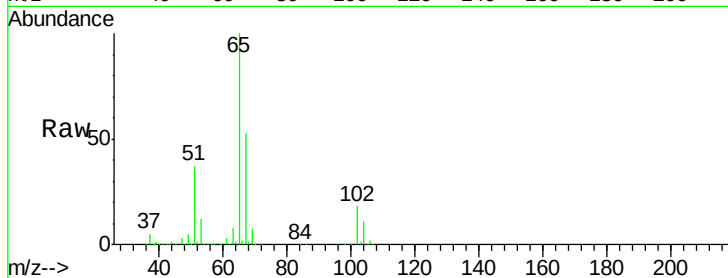

#28
 1,4-Difluorobenzene
 Concen: 30.00 ug/l
 RT: 6.87 min Scan# 1030
 Delta R.T. -0.00 min
 Lab File: VX002149.D
 Acq: 30 May 2018 20:52

Tgt Ion: 114 Resp: 289138
 Ion Ratio Lower Upper
 114 100
 63 21.5 17.1 25.7
 88 15.5 12.6 19.0

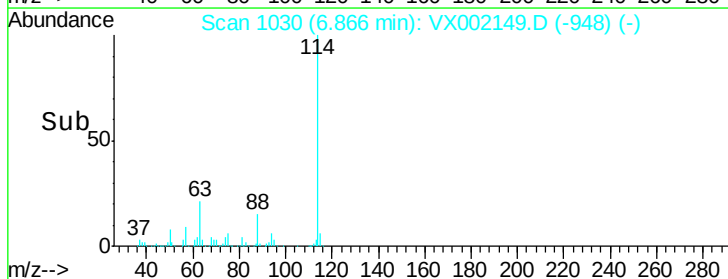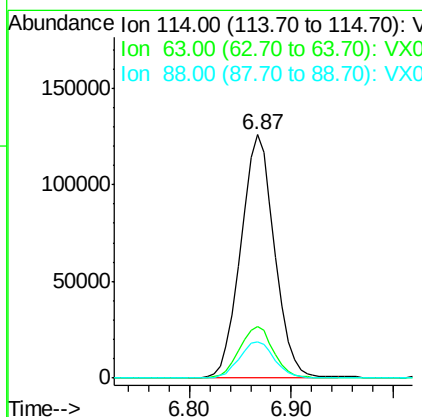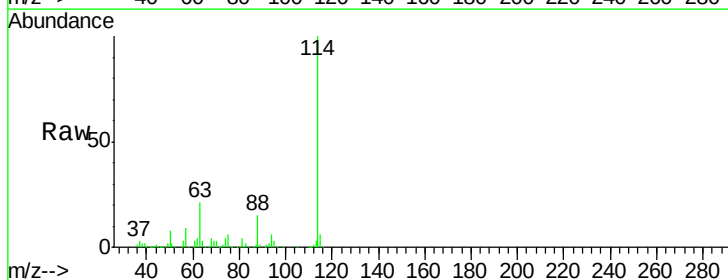

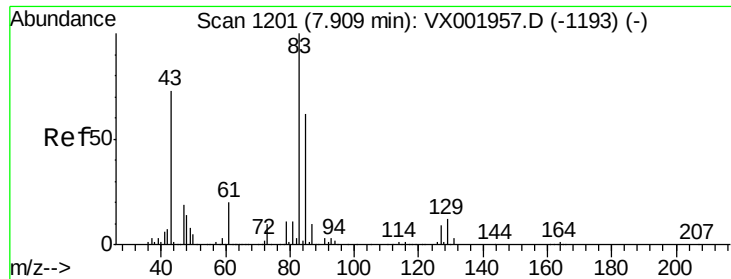

#41

Bromodichloromethane

Concen: 11.76 ug/l

RT: 7.90 min Scan# 1200

Delta R.T. -0.01 min

Lab File: VX002149.D

Acq: 30 May 2018 20:52

Instrument :

MSVOA_X

ClientSampled :

14B-2


Tot Ion: 83 Resp: 54064

Ion Ratio Lower Upper

83 100

85 63.3 49.8 74.8




127 9.3 7.3 10.9

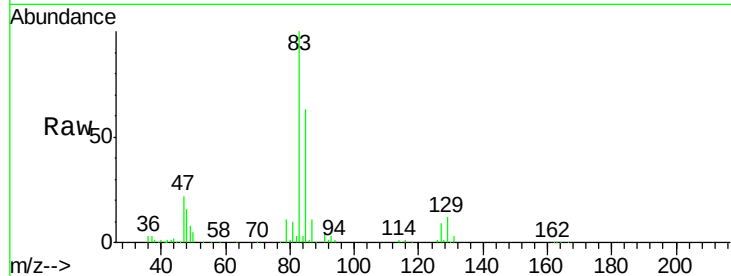

Abundance Ion 83.00 (82.70 to 83.70): VX001957.D (-1193) (-)

Ion 85.00 (84.70 to 85.70): VX001957.D (-1193) (-)

Ion 127.00 (126.70 to 127.70): VX001957.D (-1193) (-)

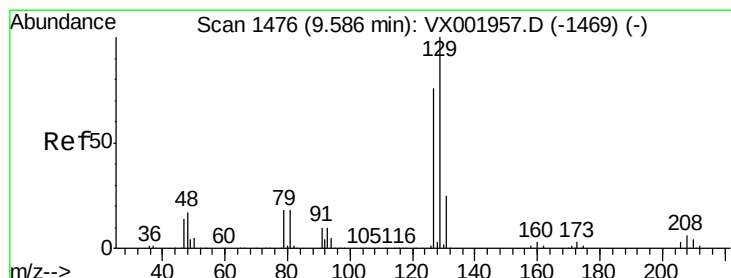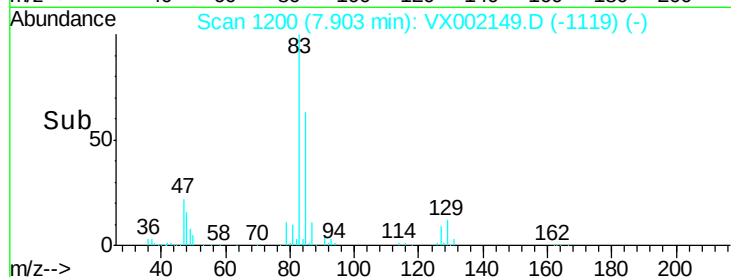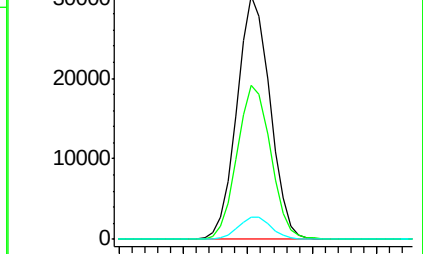

#53

Dibromochloromethane

Concen: 1.17 ug/l

RT: 9.59 min Scan# 1476

Delta R.T. -0.00 min

Lab File: VX002149.D


Acq: 30 May 2018 20:52

Tgt Ion: 129 Resp: 4534

Ion Ratio Lower Upper



129 100


127 79.8 38.5 115.3

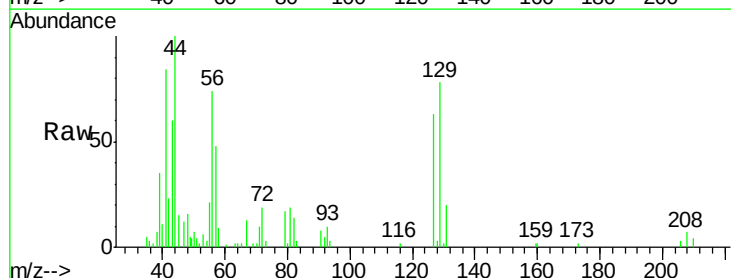

Abundance Ion 129.00 (128.70 to 129.70): VX001957.D (-1469) (-)

Ion 127.00 (126.70 to 127.70): VX001957.D (-1469) (-)



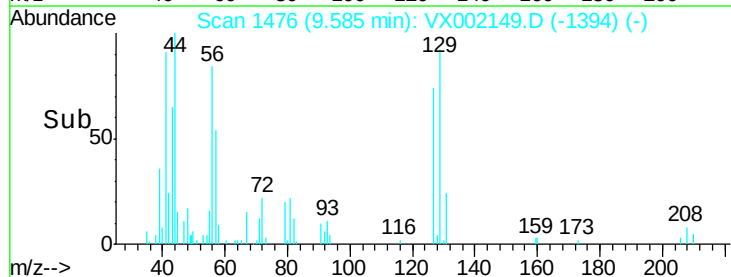
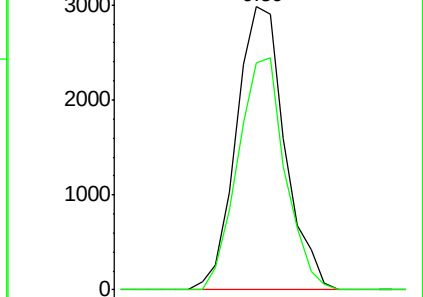


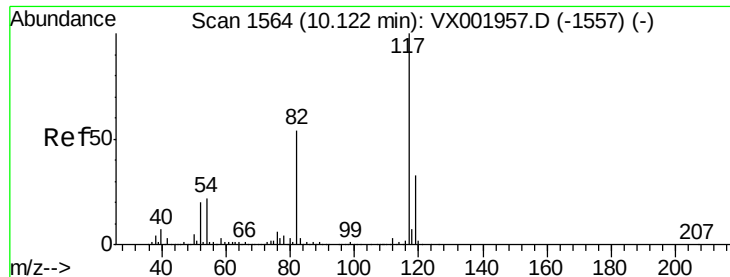

#57
Chlorobenzene-d5
Concen: 30.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. -0.01 min
Lab File: VX002149.D
Acq: 30 May 2018 20:52




Instrument :
MSVOA_X
ClientSampled :
14B-2


Tot Ion	Ratio	Lower	Upper
117	100		
82	54.8	44.3	66.5
119	32.2	25.7	38.5

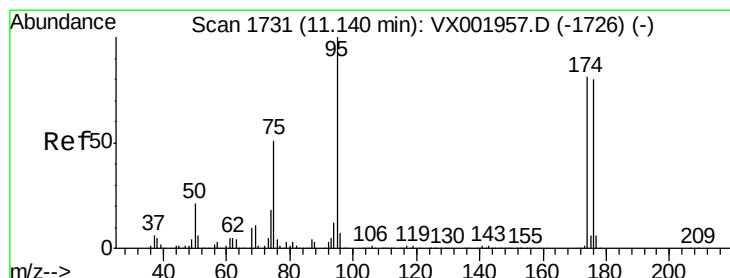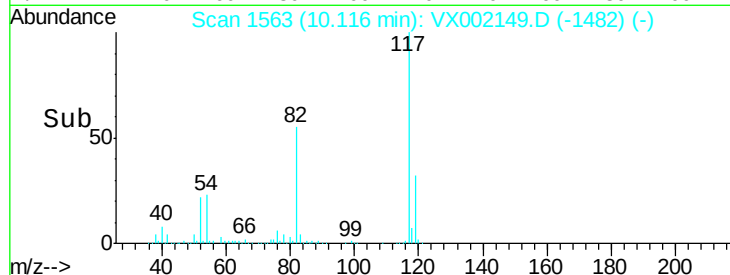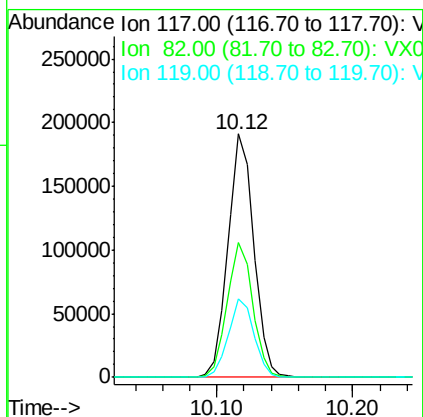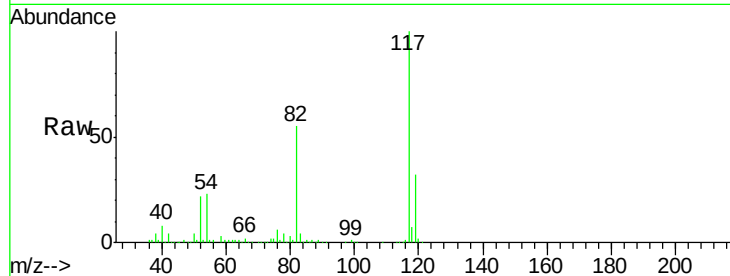

#60
4-Bromofluorobenzene
Concen: 26.69 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. -0.00 min
Lab File: VX002149.D
Acq: 30 May 2018 20:52

Tgt Ion	Ratio	Lower	Upper
95	100		
174	91.6	71.8	107.6
176	89.7	70.1	105.1

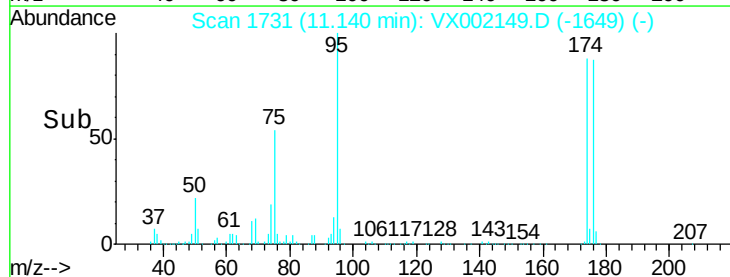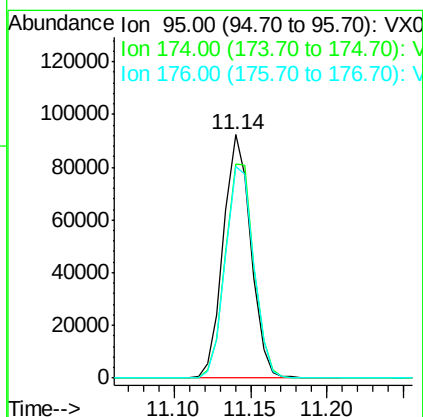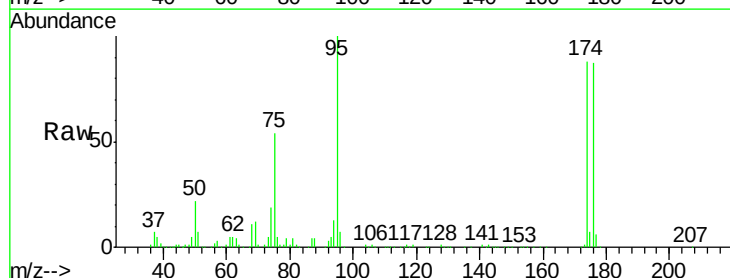

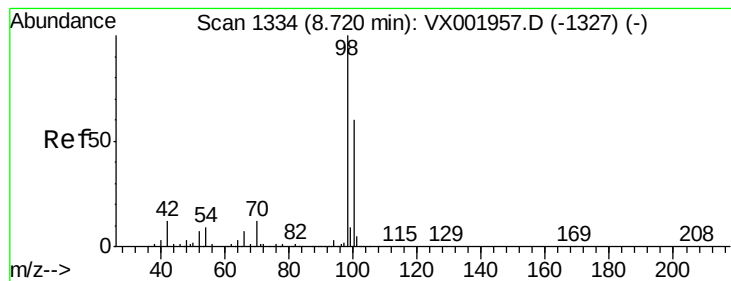

#63

Toluene-d8

Concen: 30.58 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. -0.00 min

Lab File: VX002149.D

Acq: 30 May 2018 20:52

Instrument :

MSVOA_X

ClientSampleId :

14B-2

Tot Ion: 98 Resp: 344483

Ion Ratio Lower Upper

98 100

100 63.8 50.8 76.2

