


Data Path : W:\HPCHEM1\MSVOA X\Data\VX053018\
Data File : VX002133.D
Acq On : 30 May 2018 10:13
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\624X052518W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri May 25 02:17:15 2018

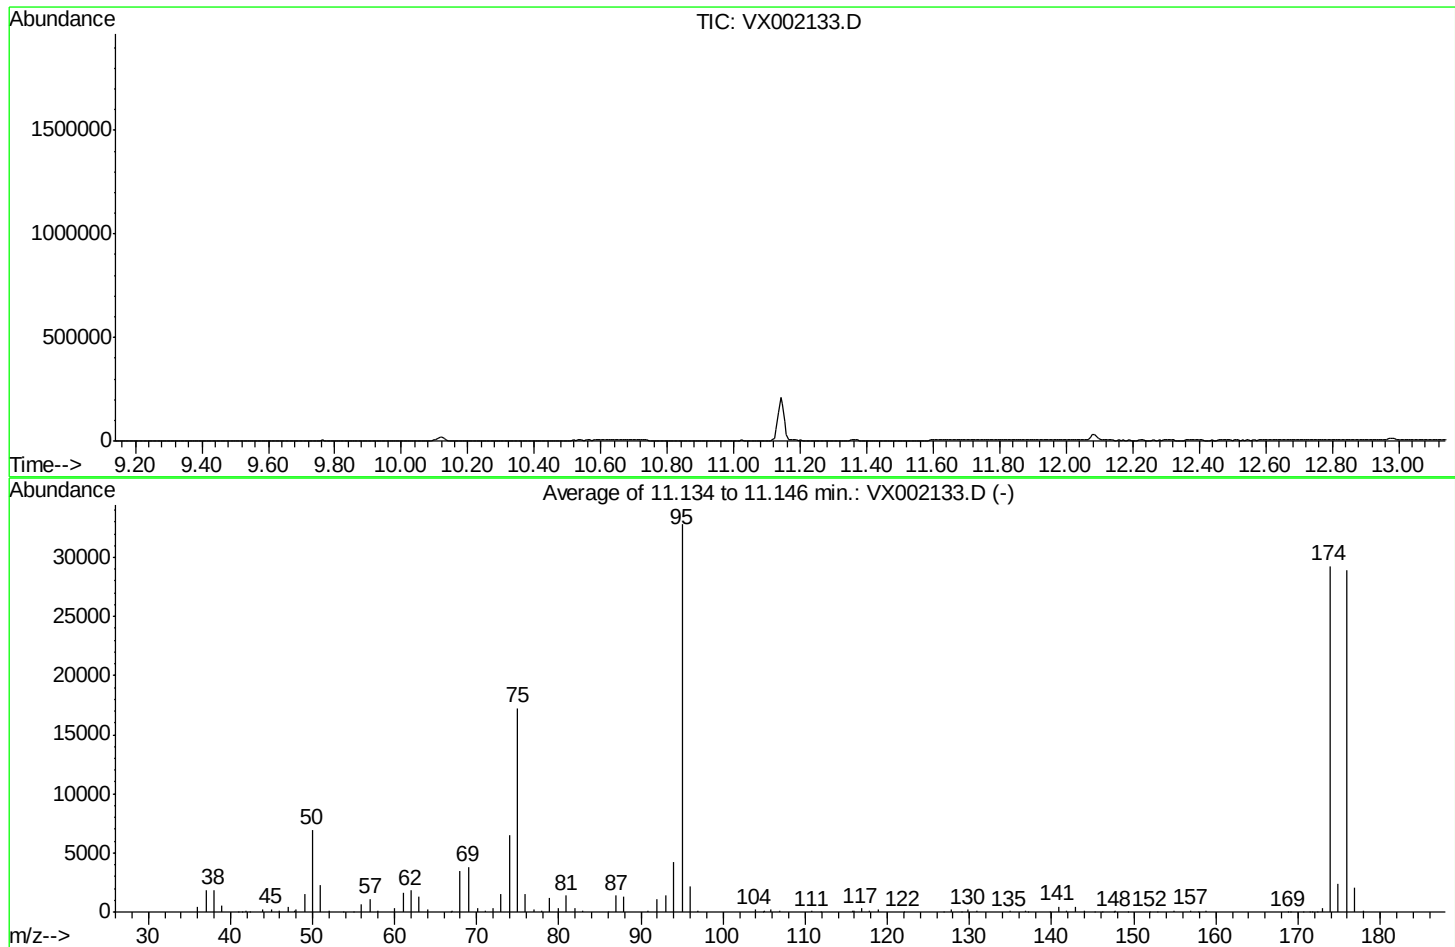

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	6962	PASS
75	95	30	60	52.5	17232	PASS
95	95	100	100	100.0	32794	PASS
96	95	5	9	6.7	2194	PASS
173	174	0.00	2	1.2	351	PASS
174	95	50	100	89.3	29280	PASS
175	174	5	9	8.0	2337	PASS
176	174	95	101	98.7	28904	PASS
177	176	5	9	7.1	2038	PASS