


Data Path : W:\HPCHEM1\MSVOA X\Data\VX053018\  
 Data File : VX002157.D  
 Acq On : 31 May 2018 00:24  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 25 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT3.P

Method : W:\HPCHEM1\MSVOA\_X\METHOD\624X052518W.M  
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
 Last Update : Fri May 25 02:17:15 2018

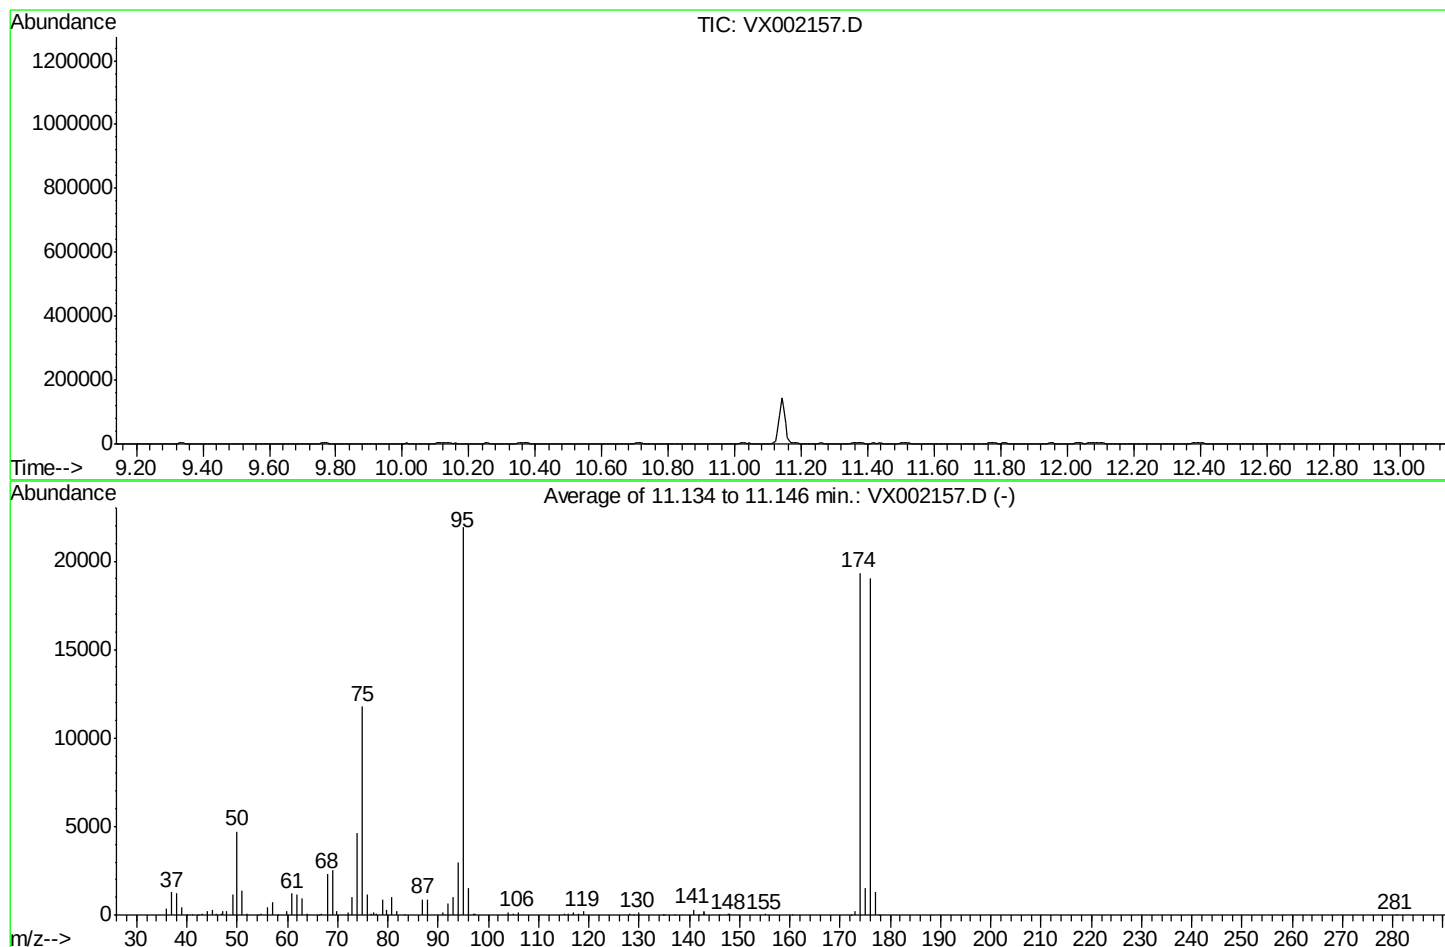

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 21.5      | 4713    | PASS             |
| 75          | 95           | 30           | 60           | 53.7      | 11757   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 21906   | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 1499    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.0       | 200     | PASS             |
| 174         | 95           | 50           | 100          | 88.3      | 19349   | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 1550    | PASS             |
| 176         | 174          | 95           | 101          | 98.3      | 19016   | PASS             |
| 177         | 176          | 5            | 9            | 6.8       | 1297    | PASS             |