


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX053118\
Data File : VX002171.D
Acq On : 31 May 2018 10:21
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Title : SW846 8260
Last Update : Thu May 24 13:09:03 2018

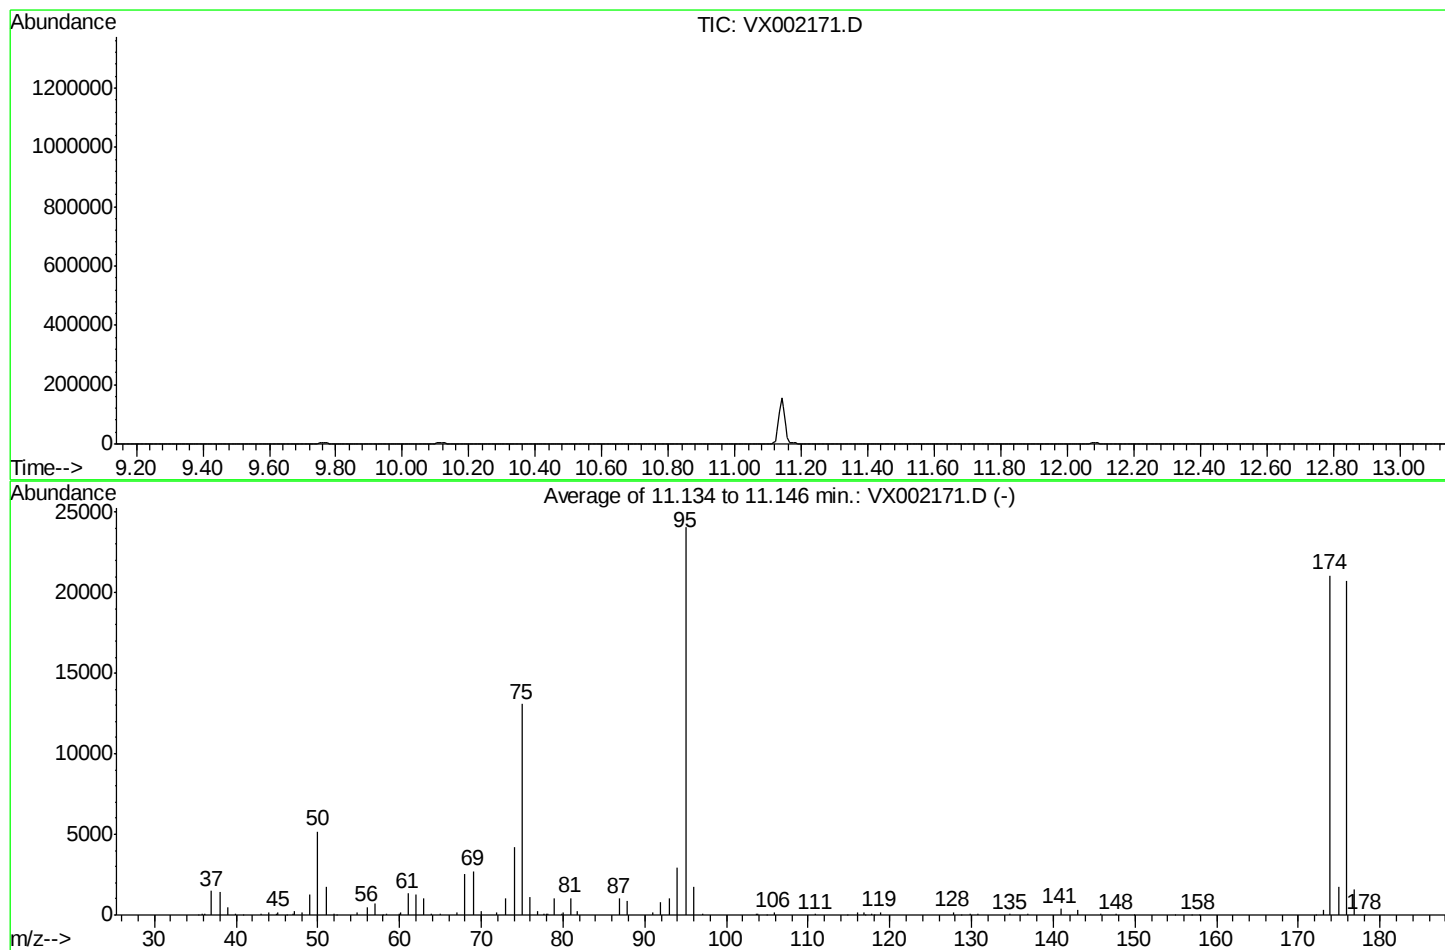

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	5202	PASS
75	95	30	60	54.4	13087	PASS
95	95	100	100	100.0	24048	PASS
96	95	5	9	7.2	1733	PASS
173	174	0.00	2	1.4	299	PASS
174	95	50	100	87.5	21042	PASS
175	174	5	9	8.2	1733	PASS
176	174	95	101	98.7	20758	PASS
177	176	5	9	7.7	1607	PASS