


Data Path : W:\HPCHEM1\MSVOA_X\Data\VX060118\
Data File : VX002214.D
Acq On : 01 Jun 2018 13:24
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Title : SW846 8260
Last Update : Thu May 24 13:09:03 2018

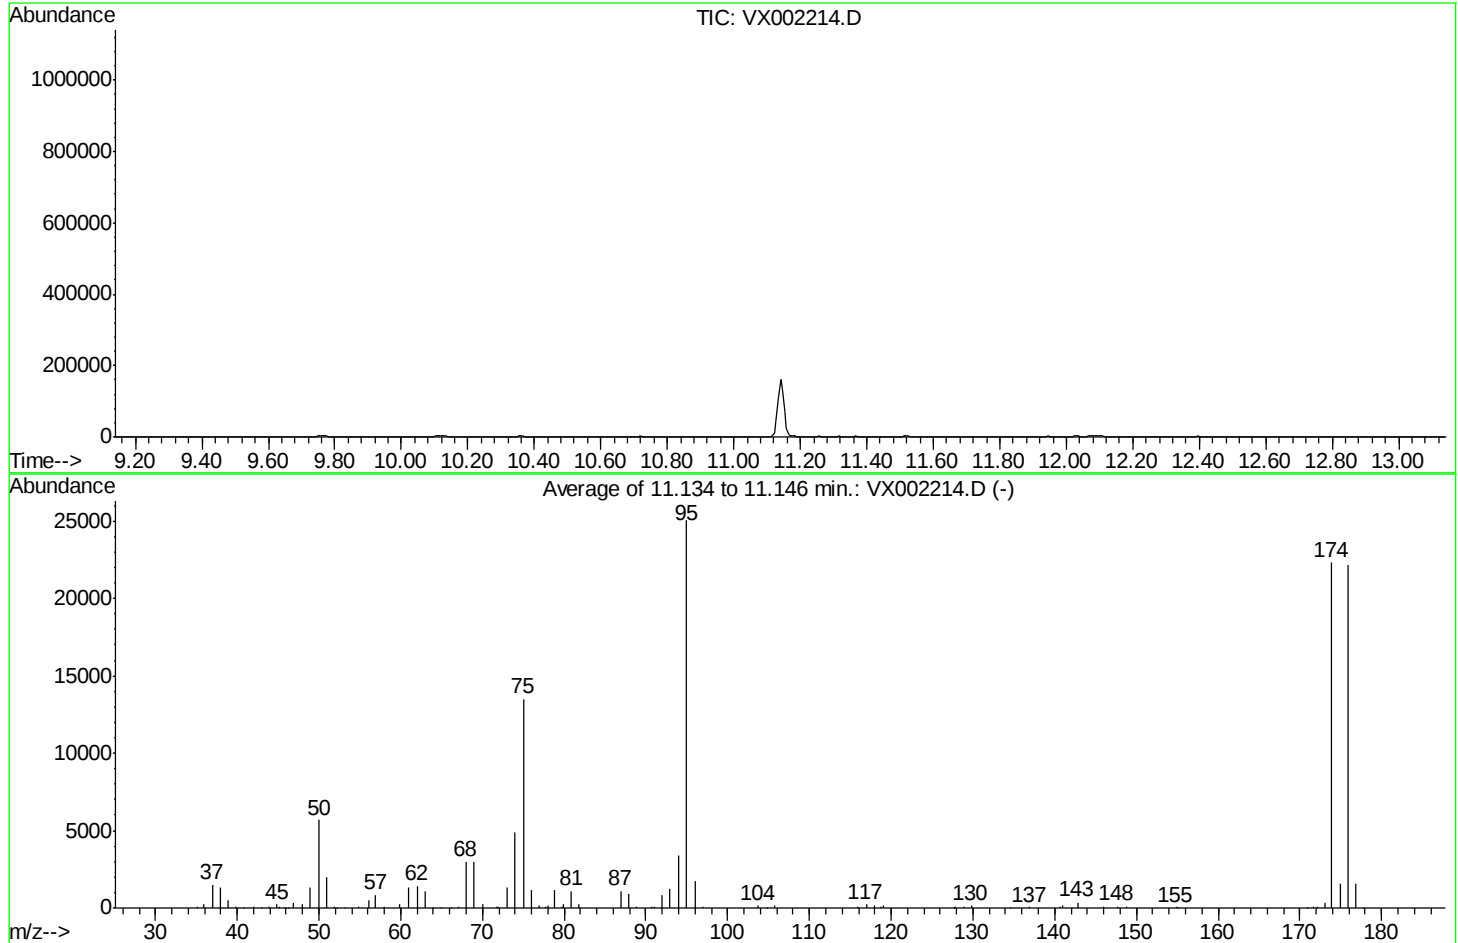

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	5703	PASS
75	95	30	60	53.8	13484	PASS
95	95	100	100	100.0	25048	PASS
96	95	5	9	6.9	1722	PASS
173	174	0.00	2	1.3	300	PASS
174	95	50	100	89.1	22309	PASS
175	174	5	9	7.1	1579	PASS
176	174	95	101	99.3	22143	PASS
177	176	5	9	7.1	1577	PASS