

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX060218\
 Data File : VX002239.D
 Acq On : 02 Jun 2018 15:10
 Operator : JC/MD
 Sample : J3151-08
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jun 04 05:06:15 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 24 13:09:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	261027	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	367649	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	334241	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	190306	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	233117	49.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.92%	
35) Dibromofluoromethane	5.51	113	171337	46.60	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.20%	
50) Toluene-d8	8.72	98	669343	50.29	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.58%	
62) 4-Bromofluorobenzene	11.14	95	236126	45.34	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.68%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.20	85	209	Below Cal	#	41
3) Chloromethane	1.33	50	1058	0.26	ug/l	91
10) Methyl Iodide	2.51	142	3887	0.88	ug/l	# 91
11) Tert butyl alcohol	3.09	59	322	0.35	ug/l	# 35
12) 1,1-Dichloroethene	2.37	96	1135	0.37	ug/l	97
13) Acrolein	2.30	56	388	0.98	ug/l	# 46
15) Acrylonitrile	3.15	53	725	0.38	ug/l	# 67
16) Acetone	2.45	43	2135	1.19	ug/l	95
17) Carbon Disulfide	2.57	76	1807	0.21	ug/l	96
18) Methyl Acetate	2.78	43	876	Below Cal	#	84
20) Methylene Chloride	2.86	84	1009	Below Cal	#	72
21) trans-1,2-Dichloroethene	3.17	96	755	Below Cal		89
25) 2-Butanone	4.71	43	1101	0.33	ug/l	# 53
27) cis-1,2-Dichloroethene	4.60	96	25072	6.32	ug/l	95
28) Bromochloromethane	5.01	49	105	Below Cal	#	14
29) Tetrahydrofuran	5.18	42	877	0.41	ug/l	# 85
38) Carbon Tetrachloride	5.67	117	24585	4.12	ug/l	# 14
41) Methacrylonitrile	5.07	41	379	Below Cal	#	45
74) N-amyl acetate	6.48	43	418	Below Cal	#	81
75) 1,1,2,2-Tetrachloroethane	11.27	83	293	Below Cal	#	59
76) 1,2,3-Trichloropropane	11.14	75	125508	27.46	ug/l	# 33
79) 2-Chlorotoluene	11.43	91	1357	Below Cal		95
81) trans-1,4-Dichloro-2-buten	11.14	75	125508	65.99	ug/l	# 10
93) 1,2,4-Trichlorobenzene	13.65	180	1975	0.35	ug/l	98
95) Naphthalene	13.84	128	3502	0.20	ug/l	97
96) 1,2,3-Trichlorobenzene	14.03	180	1512	0.26	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX060218\
Data File : VX002239.D
Acq On : 02 Jun 2018 15:10
Operator : JC/MD
Sample : J3151-08
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jun 04 05:06:15 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Quant Title : SW846 8260
QLast Update : Thu May 24 13:09:03 2018
Response via : Initial Calibration

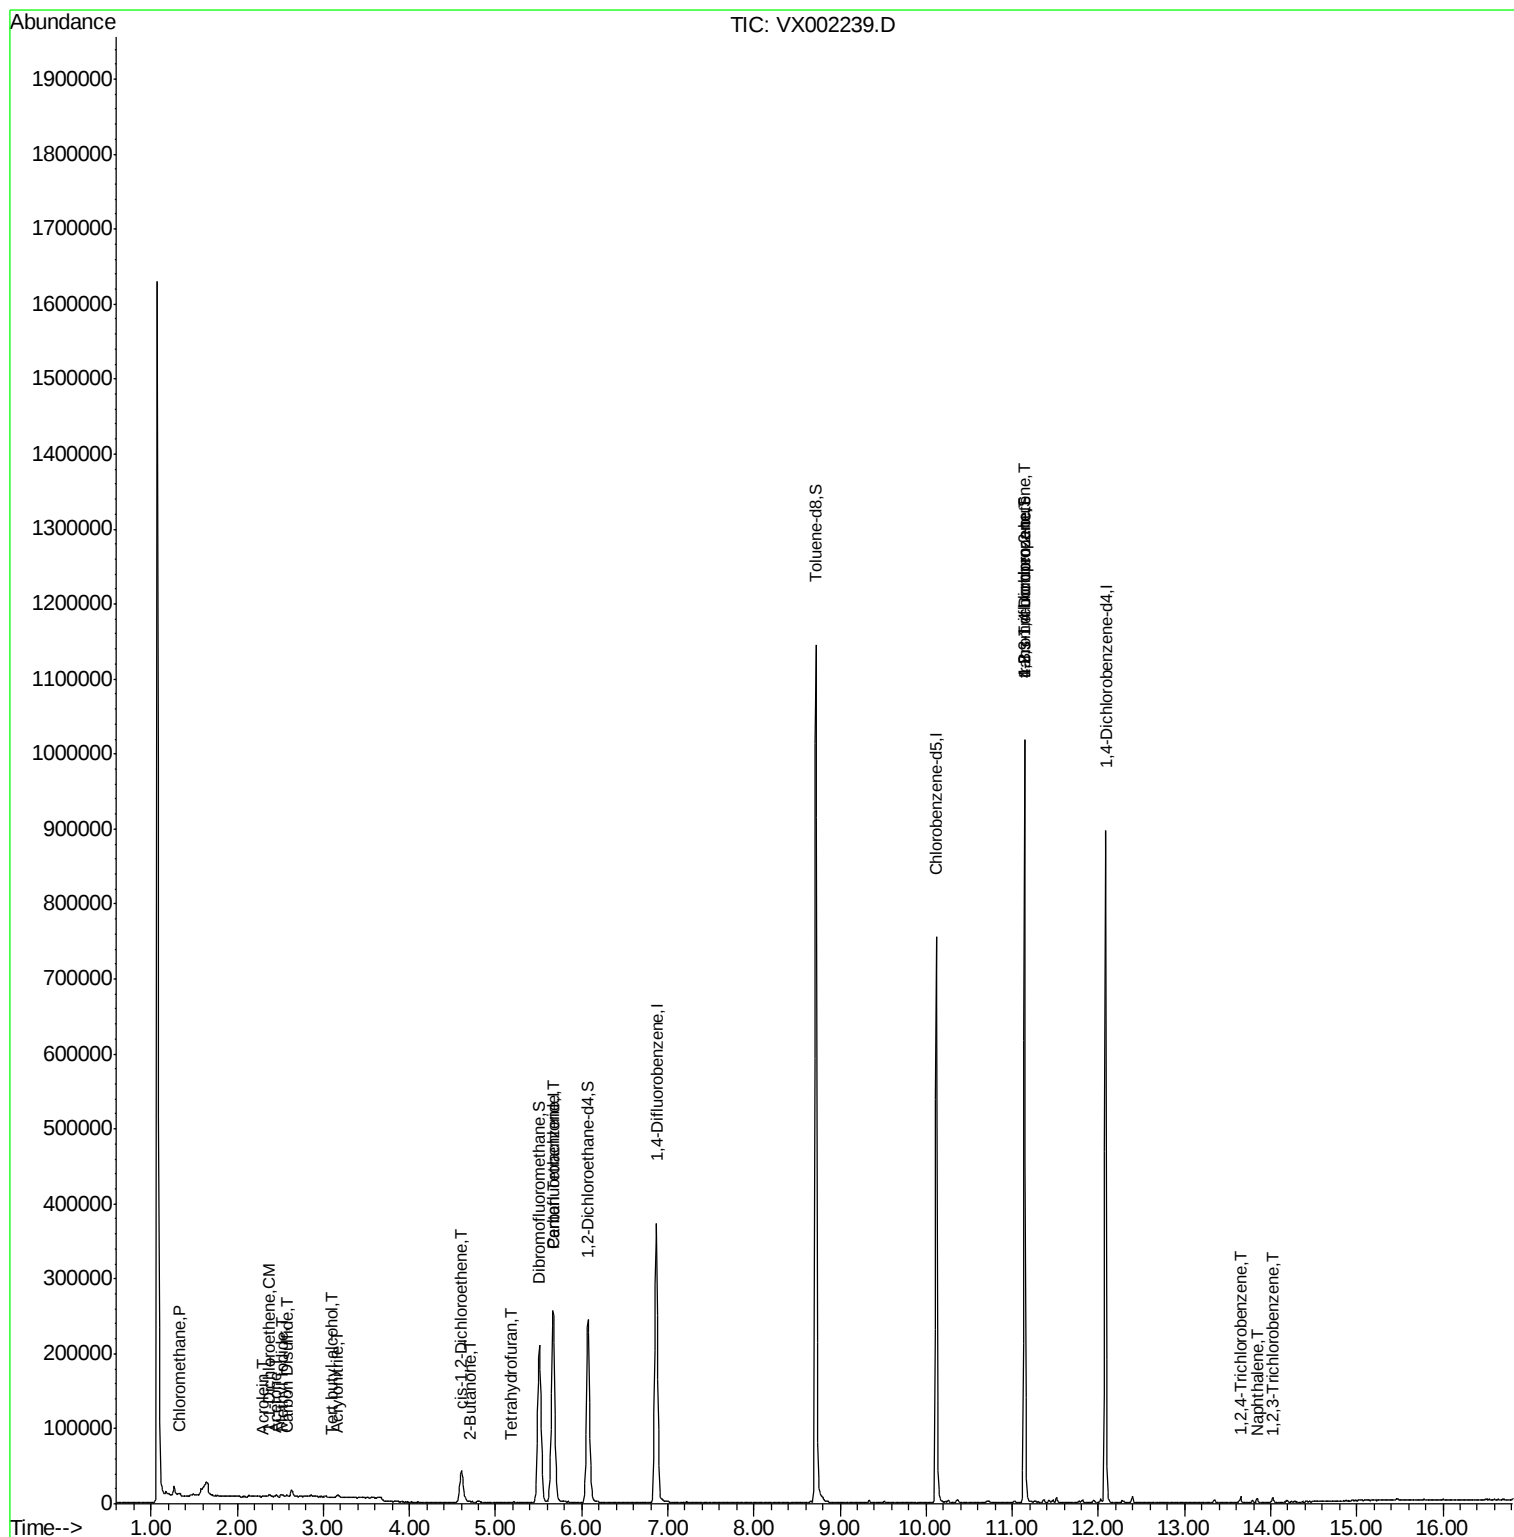







#1

Pentafluorobenzene
 Concen: 50.00 ug/l
 RT: 5.67 min Scan# 833
 Delta R.T. -0.01 min
 Lab File: VX002239.D
 Acq: 02 Jun 2018 15:10

Instrument :
 MSVOA_X
 ClientSampleId :




Tot Ion:168 Resp: 261027
 Ion Ratio Lower Upper
 168 100
 99 51.4 41.0 61.4

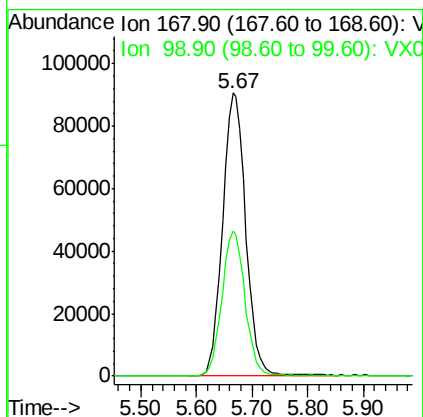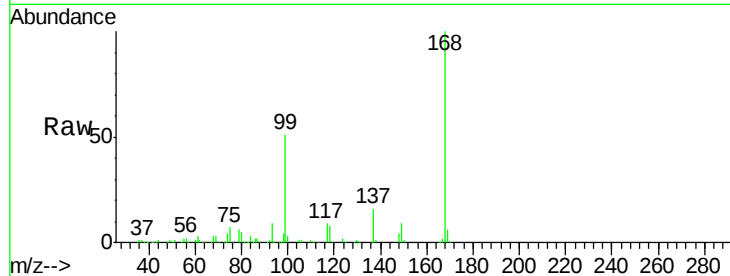


#2

Dichlorodifluoromethane
 Concen: Below Cal
 RT: 1.20 min Scan# 101
 Delta R.T. 0.01 min
 Lab File: VX002239.D
 Acq: 02 Jun 2018 15:10

Tgt Ion: 85 Resp: 209
 Ion Ratio Lower Upper
 85 100
 87 0.0 16.7 50.0#

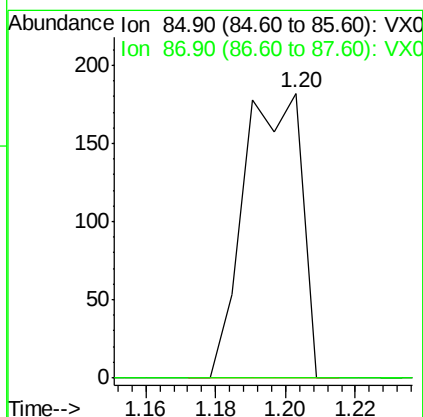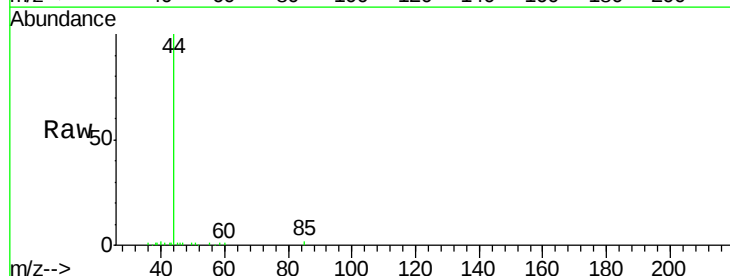



#3

Chloromethane

Concen: 0.26 ug/l

RT: 1.33 min Scan# 122

Delta R.T. 0.01 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 50 Resp: 1058

Ion Ratio Lower Upper

50 100

52 37.6 26.0 39.0



Abundance Ion 49.90 (49.60 to 50.60): VX001938.D (-115) (-)

Ion 51.90 (51.60 to 52.60): VX001938.D (-115) (-)

1.33

600



400

200

0

1.30 1.35 1.40

Time-->



#10

Methyl Iodide

Concen: 0.88 ug/l

RT: 2.51 min Scan# 316

Delta R.T. 0.01 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10


Tgt Ion: 142 Resp: 3887

Ion Ratio Lower Upper

142 100

127 49.1 35.5 53.3

141 19.4 11.3 16.9#



Abundance Ion 141.80 (141.50 to 142.50): VX001938.D (-307) (-)

Ion 126.80 (126.50 to 127.50): VX001938.D (-307) (-)

Ion 140.80 (140.50 to 141.50): VX001938.D (-307) (-)

2000

1500


1000


500

0

2.45 2.50 2.55 2.60

Time-->









#11

Tert butyl alcohol
Concen: 0.35 ug/l
RT: 3.09 min Scan# 411
Delta R.T. 0.01 min
Lab File: VX002239.D
Acq: 02 Jun 2018 15:10

Instrument :
MSVOA_X
ClientSampled :




Tot Ion: 59 Resp: 322
Ion Ratio Lower Upper
59 100
57 35.7 8.9 13.3#

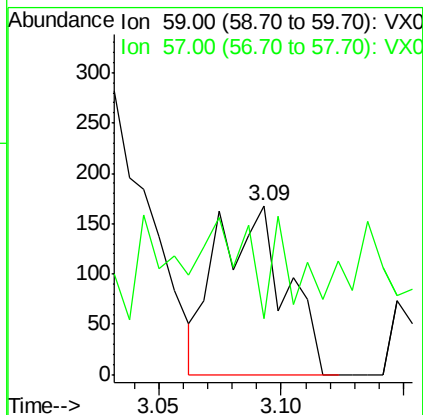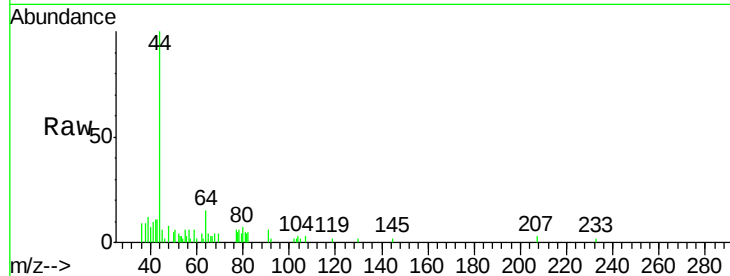


#12

1,1-Dichloroethene
Concen: 0.37 ug/l
RT: 2.37 min Scan# 292
Delta R.T. -0.01 min
Lab File: VX002239.D
Acq: 02 Jun 2018 15:10

Tgt Ion: 96 Resp: 1135
Ion Ratio Lower Upper
96 100
61 165.0 131.7 197.5
98 71.5 51.6 77.4

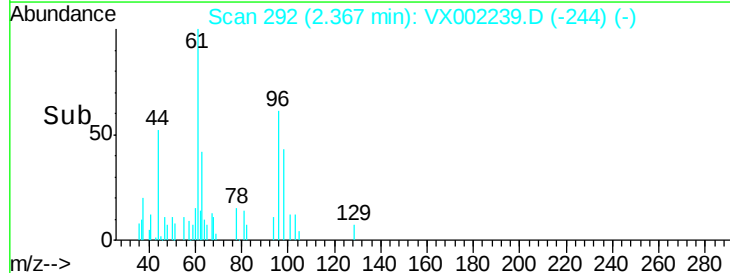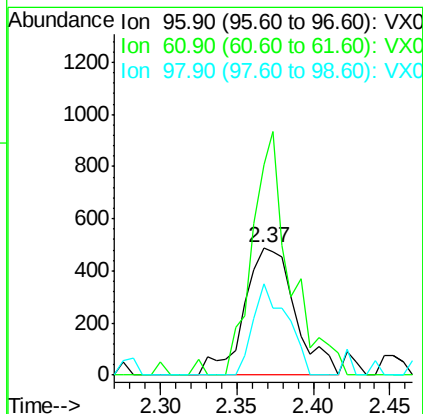



#13

Acrolein

Concen: 0.98 ug/l

RT: 2.30 min Scan# 281

Delta R.T. -0.00 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10

Instrument :

MSVOA_X





ClientSampled :

Tot Ion: 56 Resp: 388

Ion Ratio Lower Upper

56 100

55 26.5 56.8 85.2#

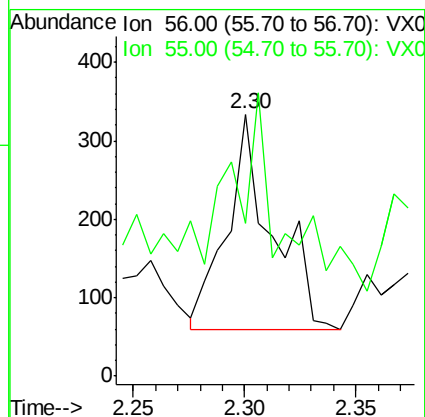

#15

Acrylonitrile

Concen: 0.38 ug/l

RT: 3.15 min Scan# 421

Delta R.T. -0.00 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10




Tgt Ion: 53 Resp: 725


Ion Ratio Lower Upper

53 100

52 94.9 66.4 99.6

51 82.5 29.3 43.9#

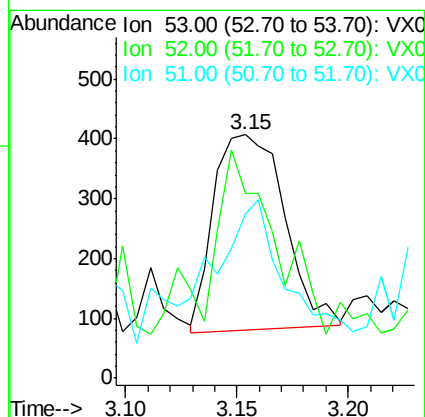

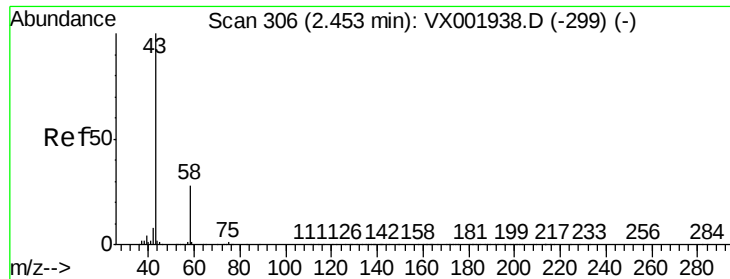

#16

Acetone

Concen: 1.19 ug/l

RT: 2.45 min Scan# 306

Delta R.T. -0.00 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 43 Resp: 2135

Ion Ratio Lower Upper




43 100

58 30.4 22.3 33.5



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

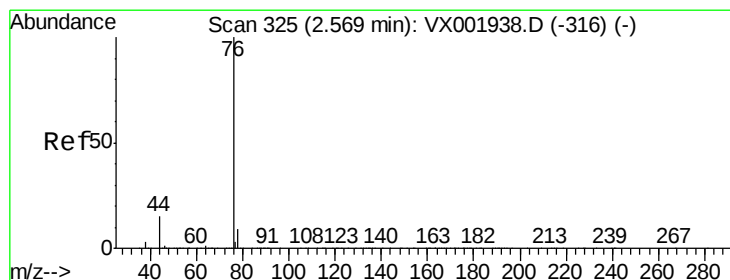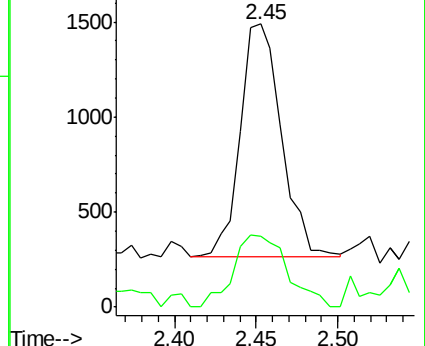

#17

Carbon Disulfide

Concen: 0.21 ug/l

RT: 2.57 min Scan# 325

Delta R.T. -0.00 min

Lab File: VX002239.D


Acq: 02 Jun 2018 15:10

Tgt Ion: 76 Resp: 1807

Ion Ratio Lower Upper



76 100


78 10.9 7.4 11.2

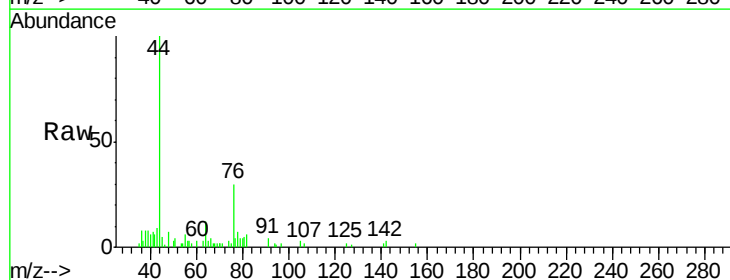

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0



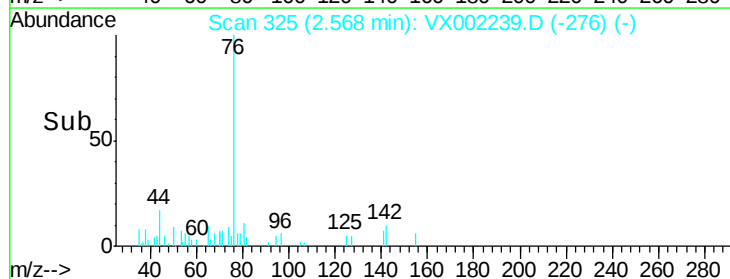
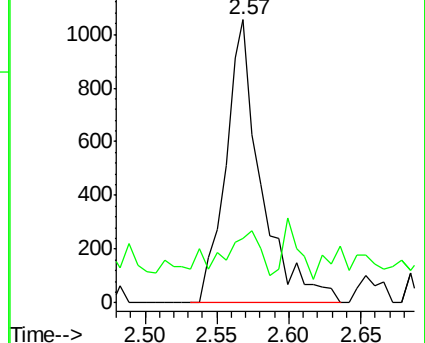


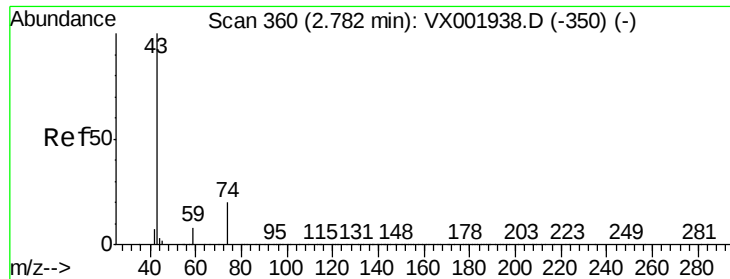

#18
Methyl Acetate
Concen: Below Cal
RT: 2.78 min Scan# 360
Delta R.T. 0.00 min
Lab File: VX002239.D
Acq: 02 Jun 2018 15:10




Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 43 Resp: 876
Ion Ratio Lower Upper
43 100
74 13.6 16.8 25.2#

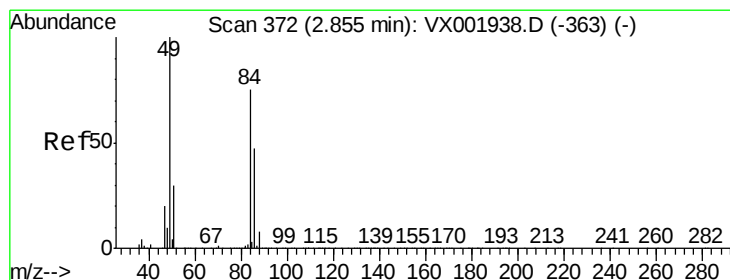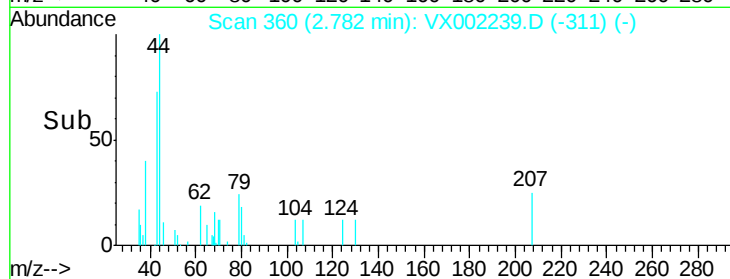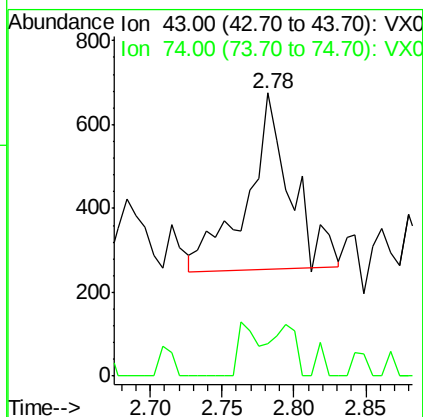

#20
Methylene Chloride
Concen: Below Cal
RT: 2.86 min Scan# 373
Delta R.T. 0.01 min
Lab File: VX002239.D
Acq: 02 Jun 2018 15:10

Tgt Ion: 84 Resp: 1009
Ion Ratio Lower Upper
84 100
49 93.9 107.2 160.8#
51 43.8 32.4 48.6
86 40.0 50.4 75.6#


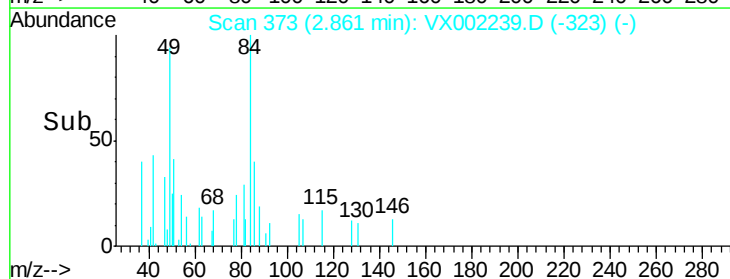
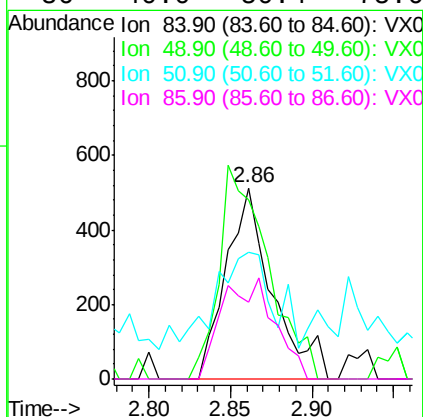
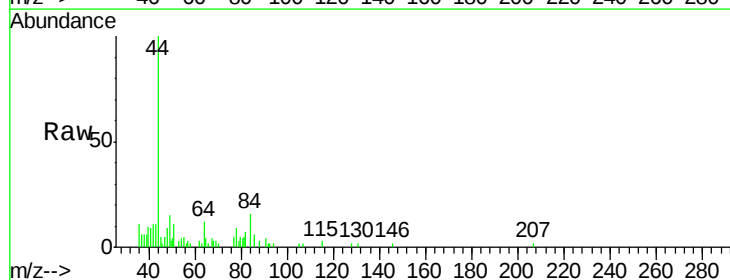


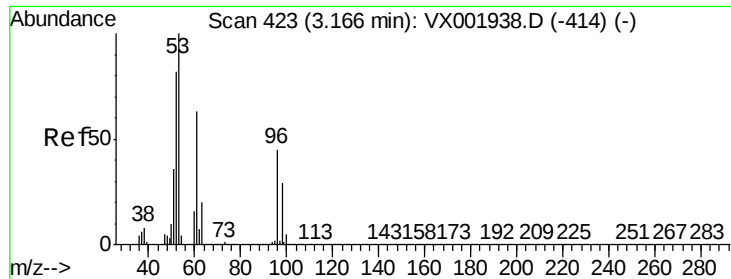

#21
trans-1,2-Dichloroethene
Concen: Below Cal
RT: 3.17 min Scan# 423
Delta R.T. -0.00 min
Lab File: VX002239.D
Acq: 02 Jun 2018 15:10




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 96 Resp: 755
Ion Ratio Lower Upper
96 100
61 125.5 113.3 169.9
98 70.4 51.7 77.5

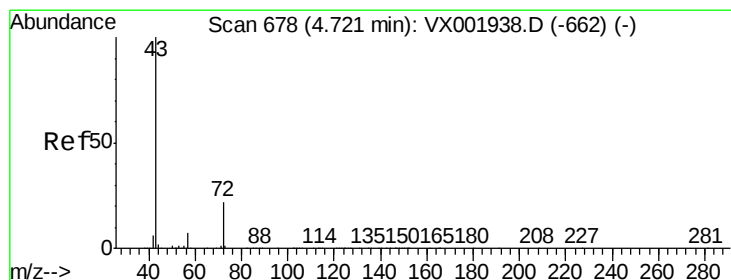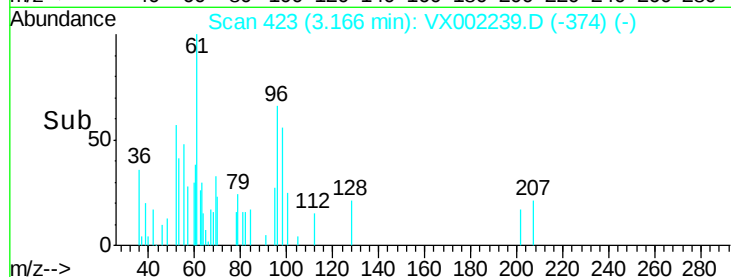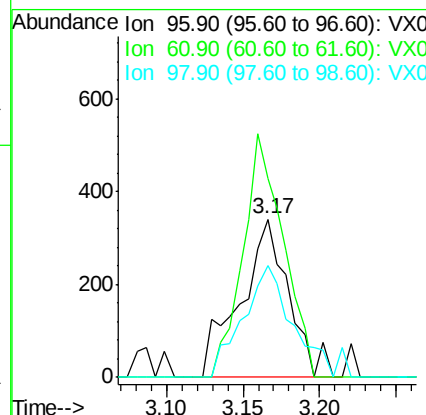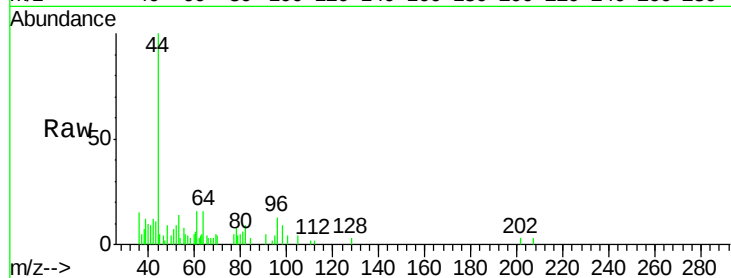

#25
2-Butanone
Concen: 0.33 ug/l
RT: 4.71 min Scan# 676
Delta R.T. -0.01 min
Lab File: VX002239.D
Acq: 02 Jun 2018 15:10

Tgt Ion: 43 Resp: 1101
Ion Ratio Lower Upper
43 100
72 0.0 17.9 26.9#

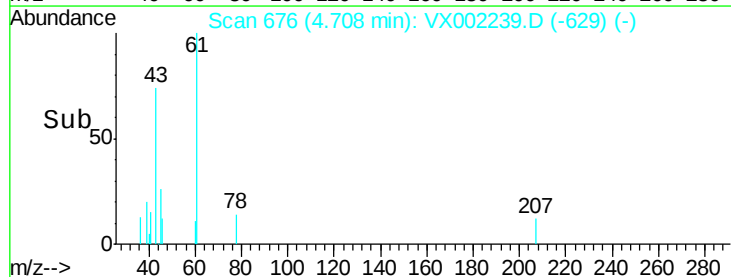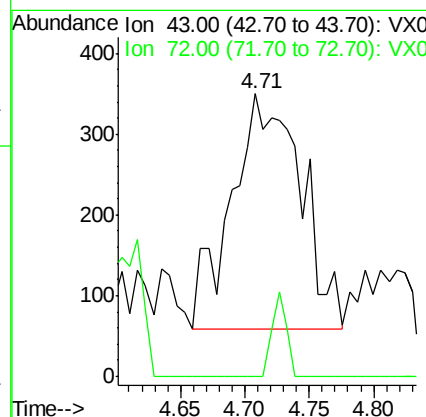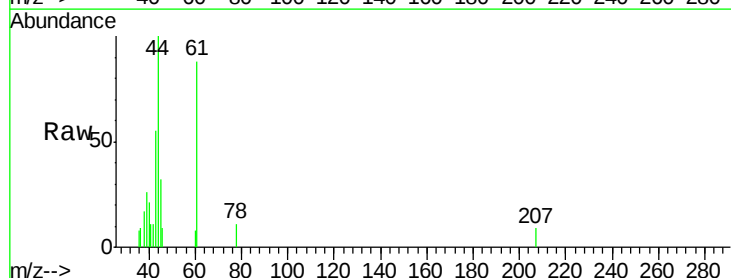

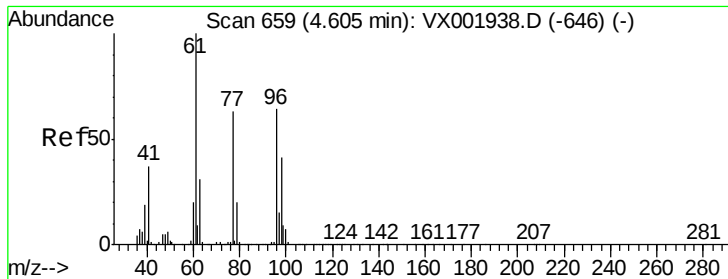

#27

cis-1,2-Dichloroethene

Concen: 6.32 ug/l

RT: 4.60 min Scan# 659

Delta R.T. -0.00 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion: 96 Resp: 25072

Ion Ratio Lower Upper

96 100

61 183.8 0.0 348.4




98 63.5 0.0 128.6

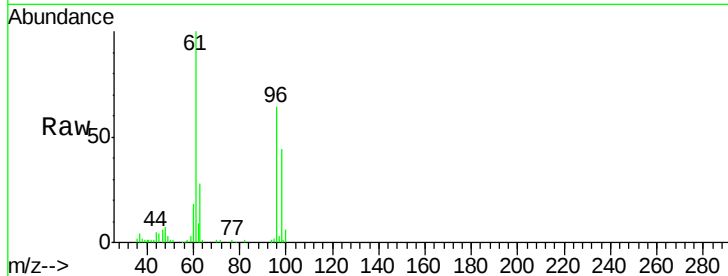

Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

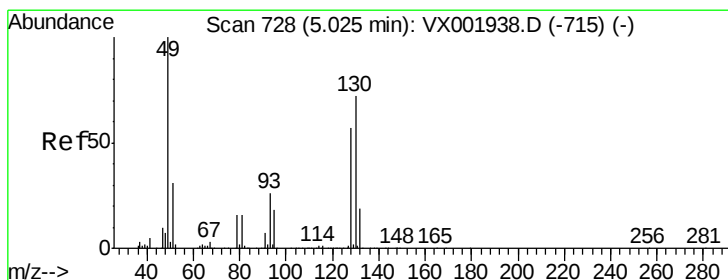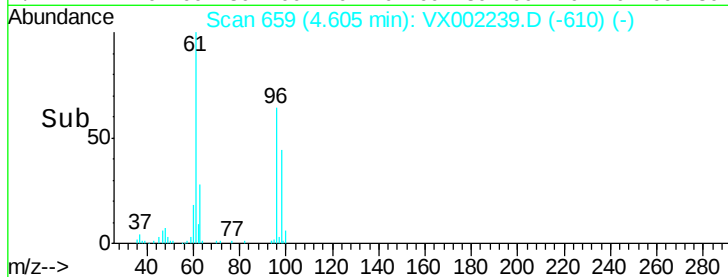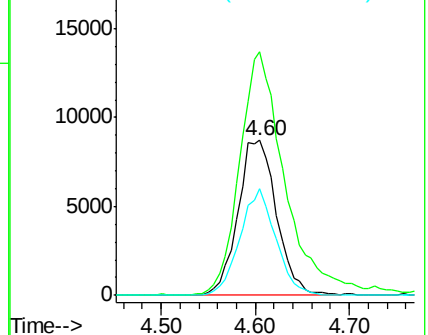

#28

Bromochloromethane

Concen: Below Cal

RT: 5.01 min Scan# 725

Delta R.T. -0.02 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10


Tgt Ion: 49 Resp: 105

Ion Ratio Lower Upper

49 100

129 0.0 0.0 3.8



130 0.0 59.4 89.2#

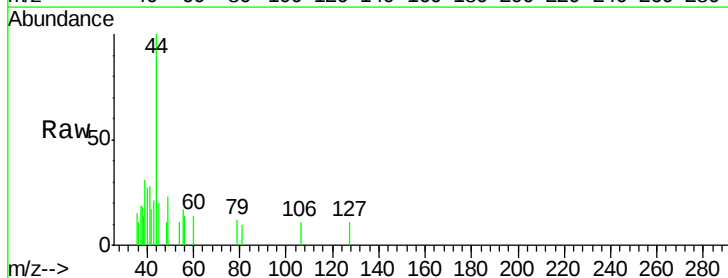


Abundance Ion 48.90 (48.60 to 49.60): VX0

Ion 128.80 (128.50 to 129.50): V

Ion 129.80 (129.50 to 130.50): V



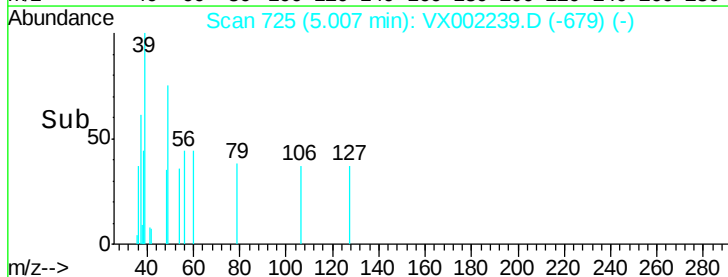
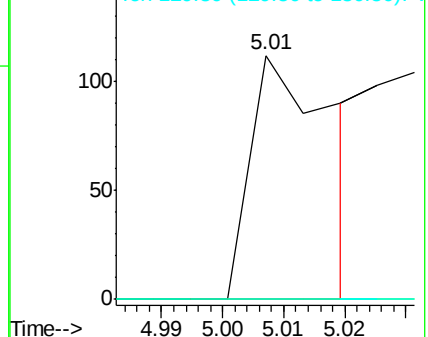




#29
Tetrahydrofuran
Concen: 0.41 ug/l
RT: 5.18 min Scan# 753
Delta R.T. -0.00 min
Lab File: VX002239.D
Acq: 02 Jun 2018 15:10




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 42 Resp: 877
Ion Ratio Lower Upper
42 100
72 27.7 31.4 47.0#
71 30.8 29.5 44.3

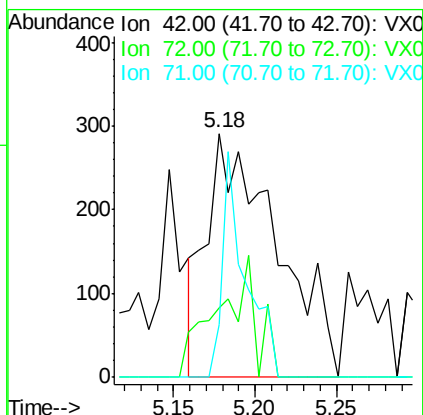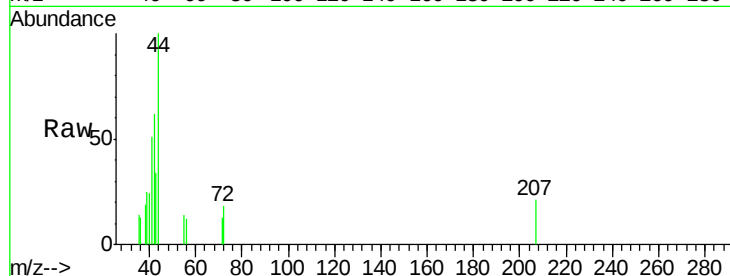

#33
1,2-Dichloroethane-d4
Concen: 49.96 ug/l
RT: 6.07 min Scan# 900
Delta R.T. -0.00 min
Lab File: VX002239.D
Acq: 02 Jun 2018 15:10

Tgt Ion: 65 Resp: 233117
Ion Ratio Lower Upper
65 100
67 51.2 0.0 104.0

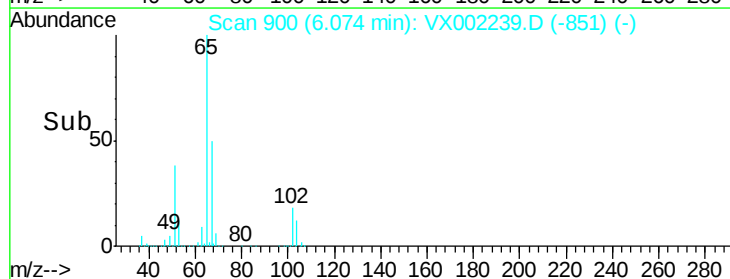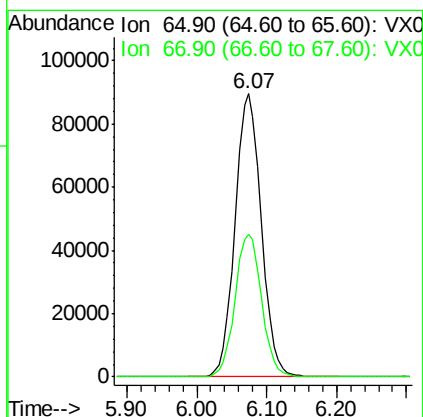

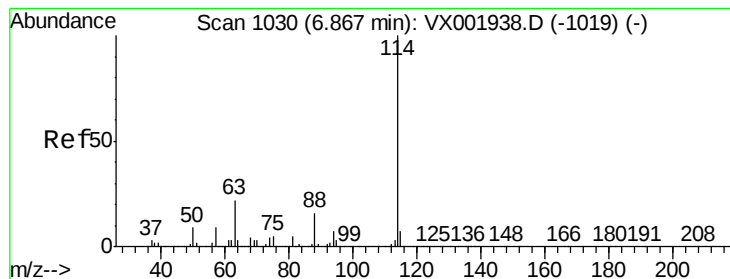

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:114 Resp: 367649

Ion Ratio Lower Upper

114 100

63 20.7 0.0 43.2




88 15.5 0.0 31.6



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

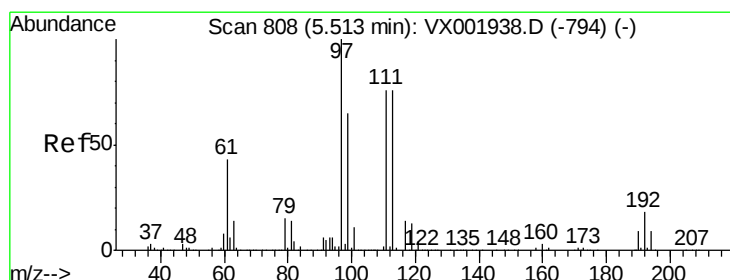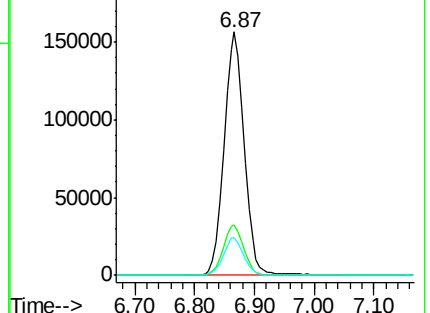

#35

Dibromofluoromethane

Concen: 46.60 ug/l

RT: 5.51 min Scan# 808

Delta R.T. -0.00 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10


Tgt Ion:113 Resp: 171337

Ion Ratio Lower Upper

113 100

111 102.7 82.0 123.0



192 23.0 18.9 28.3




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

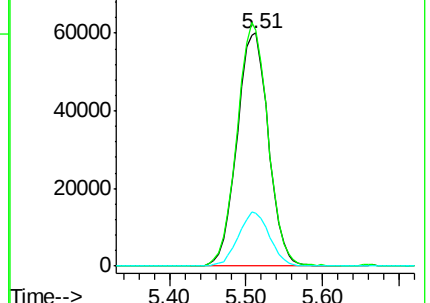

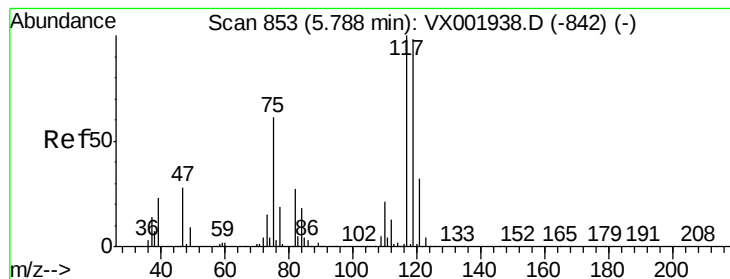

#38

Carbon Tetrachloride

Concen: 4.12 ua/l

RT: 5.67 min Scan# 834

Delta R.T. -0.12 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10

Instrument :
MSVOA_X
ClientSampleId :


Tot Ion:117 Resp: 24585

Ion Ratio Lower Upper




117 100

119 4.4 78.5 117.7#

121 0.0 25.5 38.3#



Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V

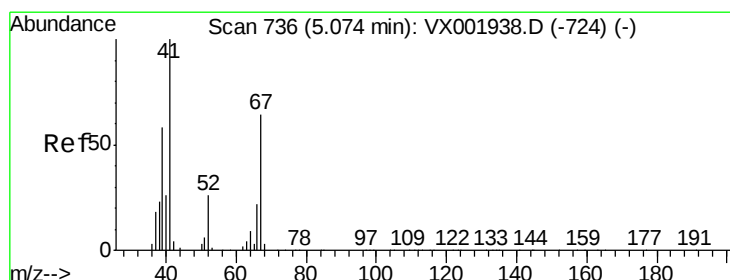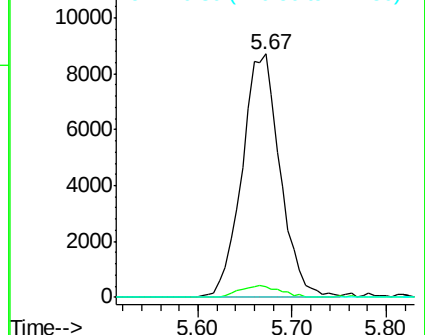

#41

Methacrylonitrile

Concen: Below Cal

RT: 5.07 min Scan# 735

Delta R.T. -0.01 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10

Tgt Ion: 41 Resp: 379


Ion Ratio Lower Upper

41 100



39 0.0 46.0 69.0#


67 23.0 50.6 75.8#

52 18.5 21.9 32.9#



Abundance Ion 41.00 (40.70 to 41.70): VX0
Ion 39.00 (38.70 to 39.70): VX0
Ion 67.00 (66.70 to 67.70): VX0
Ion 52.00 (51.70 to 52.70): VX0

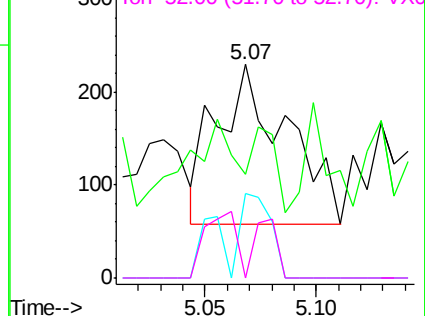

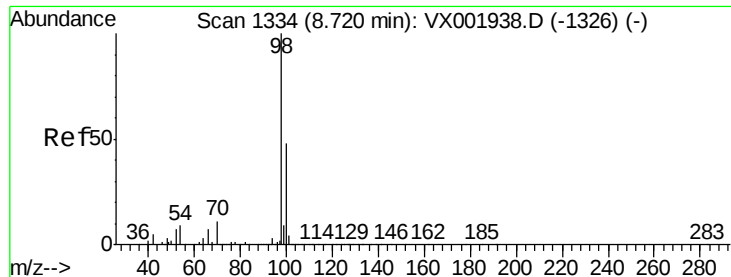

#50

Toluene-d8

Concen: 50.29 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 98 Resp: 669343

Ion Ratio Lower Upper

98 100

100 63.1 51.5 77.3

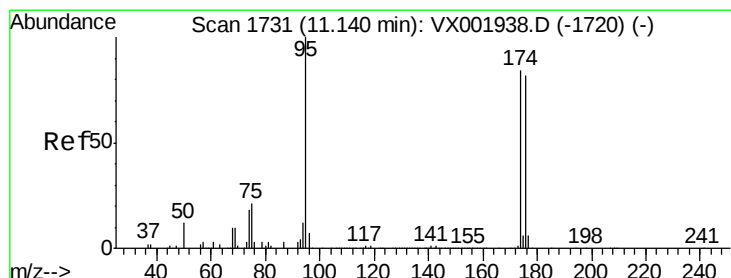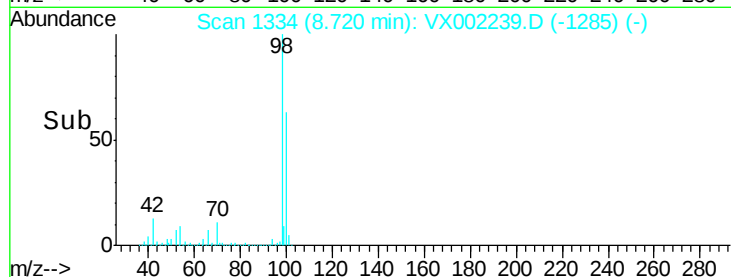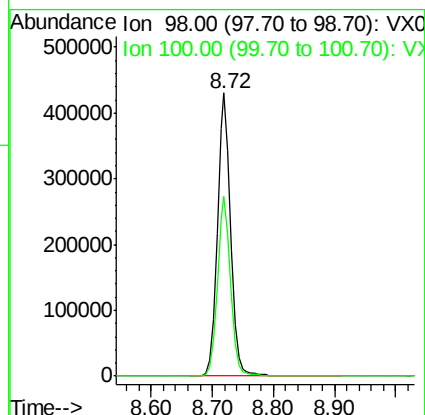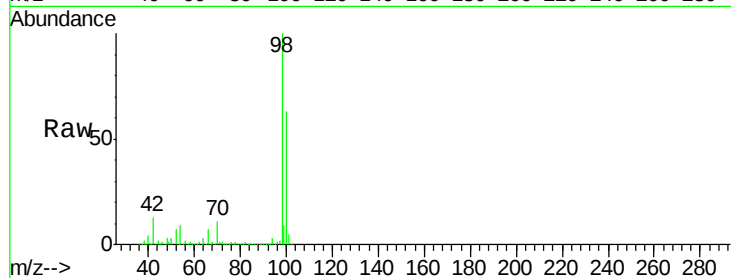

#62

4-Bromofluorobenzene

Concen: 45.34 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.00 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10




Tgt Ion: 95 Resp: 236126


Ion Ratio Lower Upper

95 100

174 92.4 0.0 178.8

176 90.5 0.0 175.6

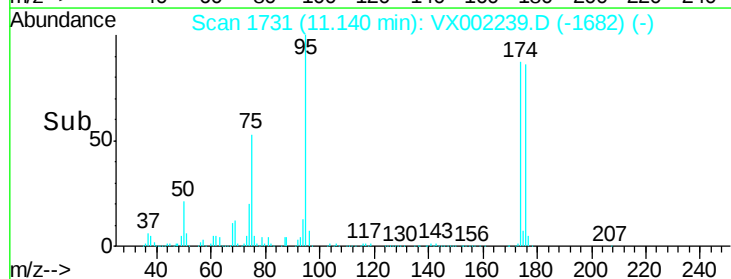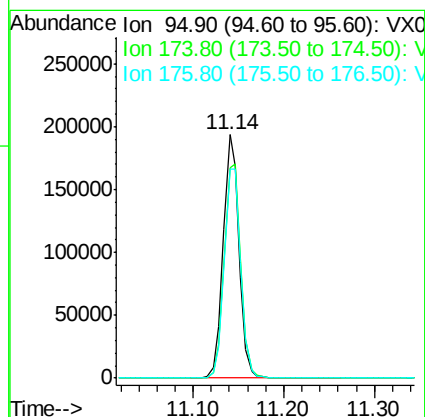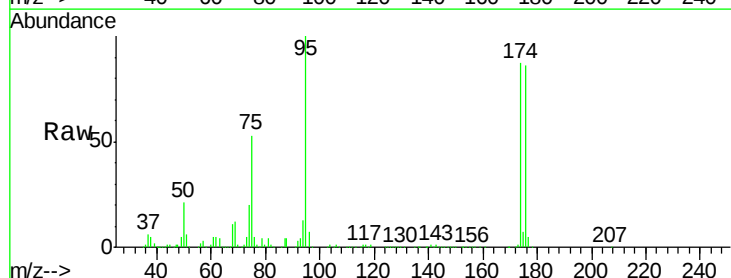



#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 10.12 min Scan# 1563

Delta R.T. -0.00 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:117 Resp: 334241

Ion Ratio Lower Upper

117 100

82 55.4 44.8 67.2




119 31.7 25.5 38.3



Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

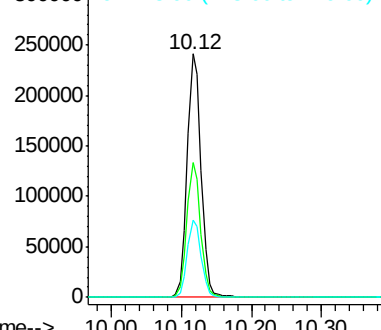

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.09 min Scan# 1886

Delta R.T. -0.00 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10


Tgt Ion:152 Resp: 190306

Ion Ratio Lower Upper

152 100

115 55.2 42.3 126.8



150 153.6 0.0 351.0




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

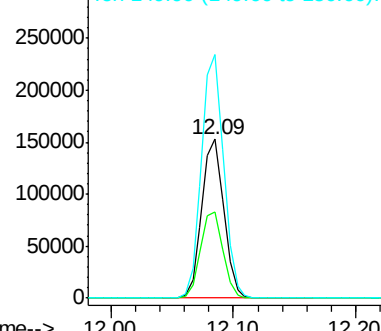



#74

N-amvl acetate

Concen: Below Cal

RT: 6.48 min Scan# 966





Delta R.T. 0.00 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion:	43	Resp:	418
Ion	Ratio	Lower	Upper
43	100		
70	0.0	0.1	0.1#
55	41.1	0.1	0.1#
61	9.8	14.5	21.7#

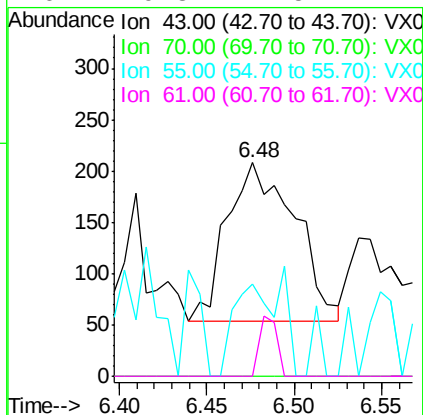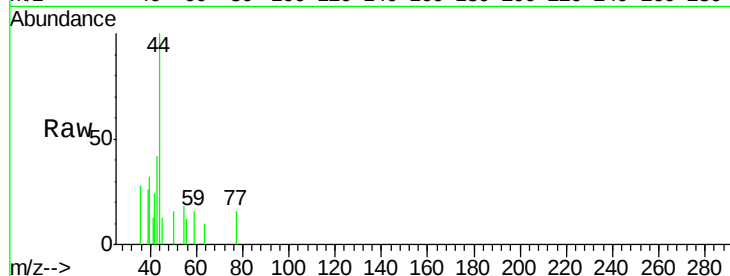

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal




RT: 11.27 min Scan# 1753


Delta R.T. 0.00 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10

Tgt Ion:	83	Resp:	293
Ion	Ratio	Lower	Upper
83	100		
131	0.0	5.7	17.0#
85	31.1	32.6	97.7#



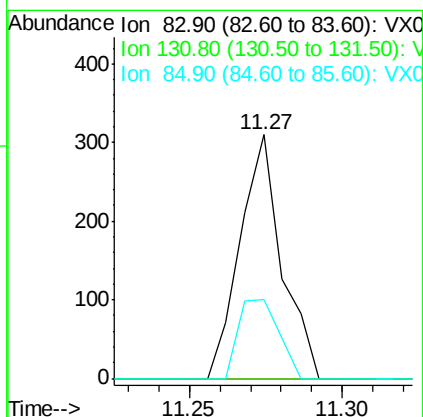



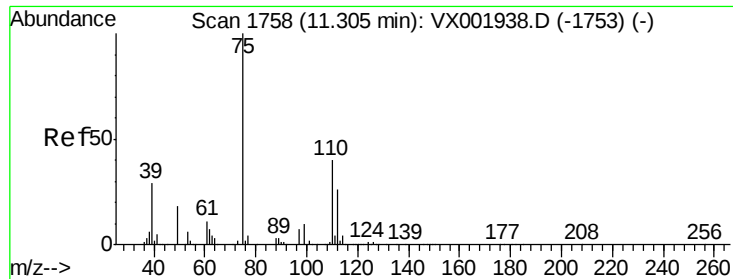

#76
 1,2,3-Trichloropropane
 Concen: 27.46 ug/l
 RT: 11.14 min Scan# 1731
 Delta R.T. -0.16 min
 Lab File: VX002239.D
 Acq: 02 Jun 2018 15:10




Instrument :
 MSVOA_X
 ClientSampleId :


Tot Ion: 75 Resp: 125508
 Ion Ratio Lower Upper
 75 100
 77 1.2 22.8 68.3#

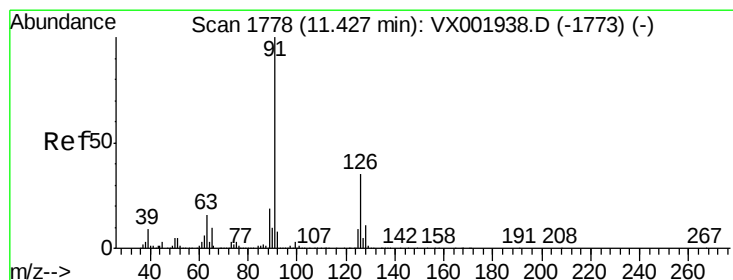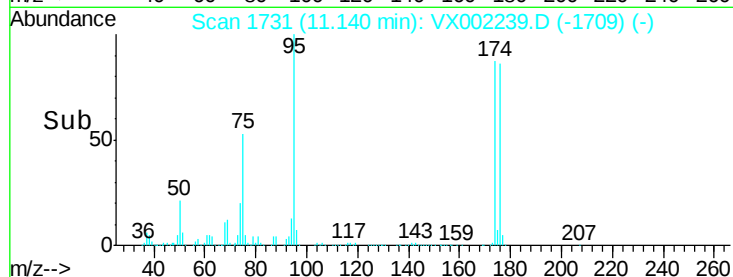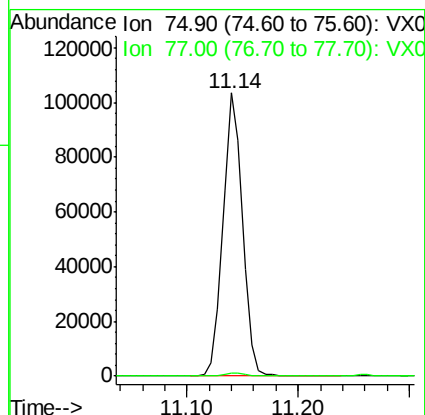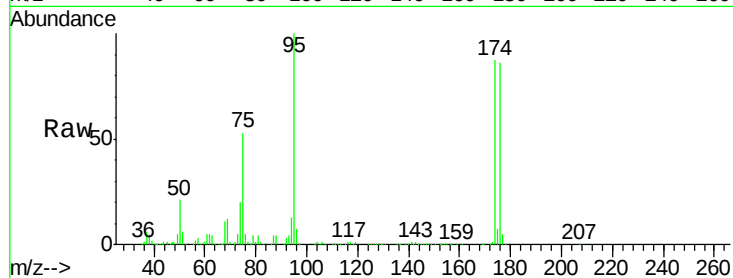

#79
 2-Chlorotoluene
 Concen: Below Cal
 RT: 11.43 min Scan# 1778
 Delta R.T. 0.00 min
 Lab File: VX002239.D
 Acq: 02 Jun 2018 15:10

Tgt Ion: 91 Resp: 1357
 Ion Ratio Lower Upper
 91 100
 126 31.9 17.4 52.2

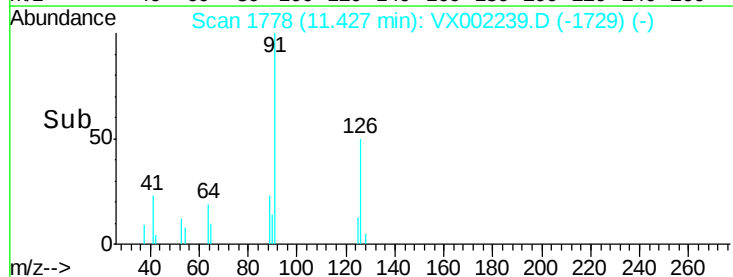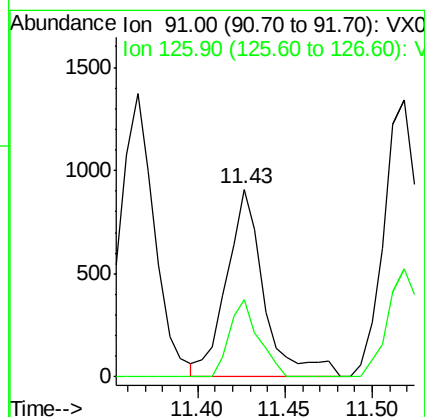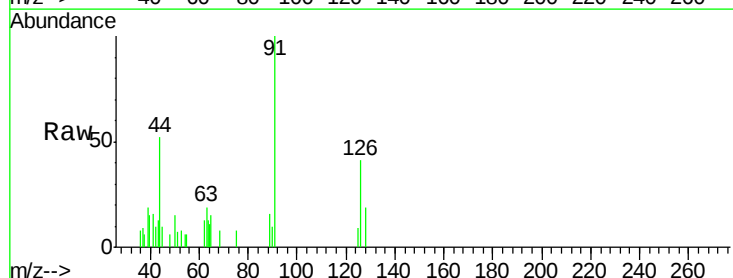



#81

trans-1,4-Dichloro-2-butene

Concen: 65.99 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.06 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion: 75 Resp: 125508

Ion Ratio Lower Upper

75 100

53 0.0 78.0 117.0#




89 0.0 39.4 59.2#

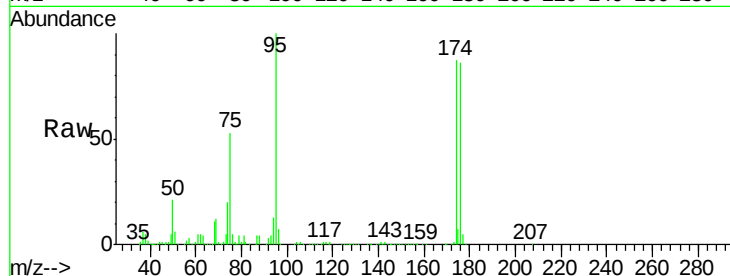

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

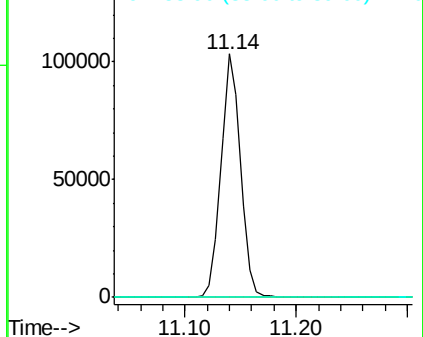

#93

1,2,4-Trichlorobenzene

Concen: 0.35 ug/l

RT: 13.65 min Scan# 2143

Delta R.T. -0.00 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10


Tgt Ion: 180 Resp: 1975

Ion Ratio Lower Upper

180 100

182 94.8 47.7 143.1



145 25.2 14.4 43.0




Abundance Ion 179.80 (179.50 to 180.50): V

Ion 181.80 (181.50 to 182.50): V

Ion 144.80 (144.50 to 145.50): V

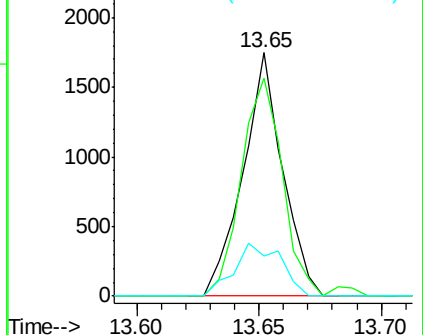



#95

Naphthalene

Concen: 0.20 ug/l

RT: 13.84 min Scan# 2174

Delta R.T. -0.00 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:128 Resp: 3502

Ion Ratio Lower Upper

128 100

127 14.0 10.4 15.6




129 10.0 8.8 13.2



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

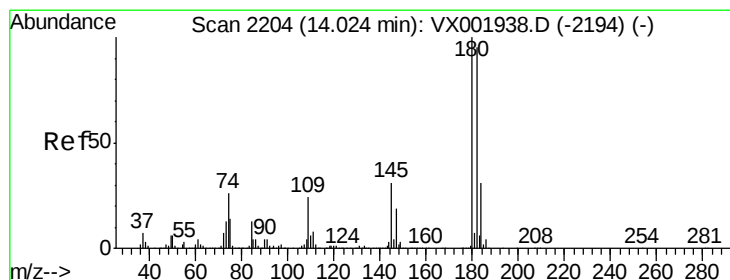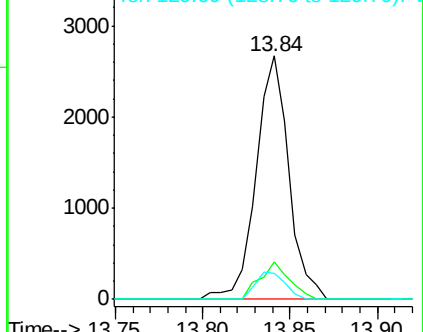

#96

1,2,3-Trichlorobenzene

Concen: 0.26 ug/l

RT: 14.03 min Scan# 2205

Delta R.T. 0.01 min

Lab File: VX002239.D

Acq: 02 Jun 2018 15:10


Tgt Ion:180 Resp: 1512

Ion Ratio Lower Upper

180 100

182 99.2 47.9 143.6

145 35.9 15.1 45.3



Abundance Ion 179.80 (179.50 to 180.50): V

Ion 181.80 (181.50 to 182.50): V

Ion 144.90 (144.60 to 145.60): V

