


Data Path : W:\HPCHEM1\MSVOA X\Data\VX060218\
Data File : VX002234.D
Acq On : 02 Jun 2018 09:11
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X052418W.M
Title : SW846 8260
Last Update : Thu May 24 13:09:03 2018

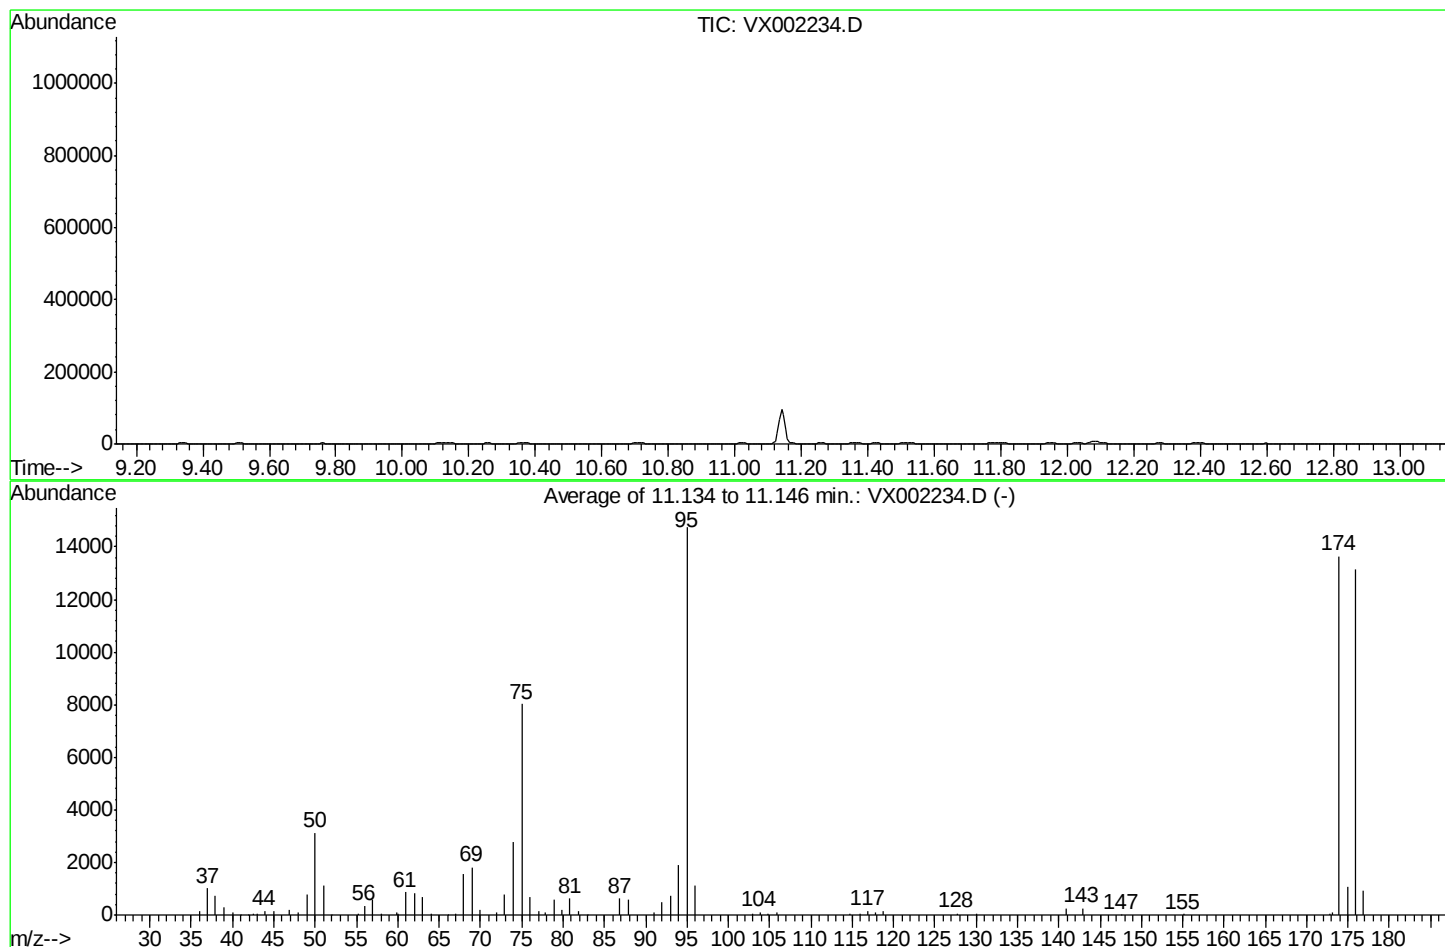

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	3123	PASS
75	95	30	60	54.3	8012	PASS
95	95	100	100	100.0	14746	PASS
96	95	5	9	7.5	1113	PASS
173	174	0.00	2	0.9	123	PASS
174	95	50	100	92.5	13637	PASS
175	174	5	9	7.7	1055	PASS
176	174	95	101	96.3	13139	PASS
177	176	5	9	6.9	908	PASS