

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060324\
 Data File : VX041709.D
 Acq On : 03 Jun 2024 17:04
 Operator : JC/MD
 Sample : P2660-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-13

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
 Title : SW846 8260

Signal : TIC: VX041709.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	34	rBV2	28240	41392	6.27%	1.071%
2	1.453	56	60	63	rBV	5256	6678	1.01%	0.173%
3	1.587	69	82	83	rBV6	10962	34608	5.24%	0.896%
4	2.391	208	214	223	rBV	14236	25184	3.81%	0.652%
5	2.940	298	304	311	rBV	3033	6897	1.04%	0.178%
6	5.385	695	705	722	rBV2	75735	227017	34.38%	5.874%
7	5.549	722	732	754	rVB	133283	379398	57.46%	9.817%
8	5.958	788	799	810	rBV	80421	214929	32.55%	5.561%
9	6.763	920	931	948	rBV	197210	480418	72.76%	12.431%
10	8.646	1234	1240	1263	rVB	424285	660303	100.00%	17.086%
11	9.530	1379	1385	1394	rBV4	3787	7857	1.19%	0.203%
12	10.055	1465	1471	1487	rBV	443820	607230	91.96%	15.713%
13	11.079	1634	1639	1657	rBV	377002	499970	75.72%	12.937%
14	12.024	1788	1794	1806	rBV	477261	598887	90.70%	15.497%
15	12.219	1822	1826	1838	rBV2	6964	11312	1.71%	0.293%
16	12.859	1926	1931	1938	rBV3	5148	7525	1.14%	0.195%
17	13.231	1983	1992	2000	rVB7	2118	7009	1.06%	0.181%
18	13.889	2086	2100	2114	rBV9	6706	28881	4.37%	0.747%
19	14.914	2264	2268	2272	rBV5	4465	7230	1.09%	0.187%
20	15.694	2388	2396	2403	rBV7	4960	11877	1.80%	0.307%




Sum of corrected areas: 3864602

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060324\
Data File : VX041709.D
Acq On : 03 Jun 2024 17:04
Operator : JC/MD
Sample : P2660-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

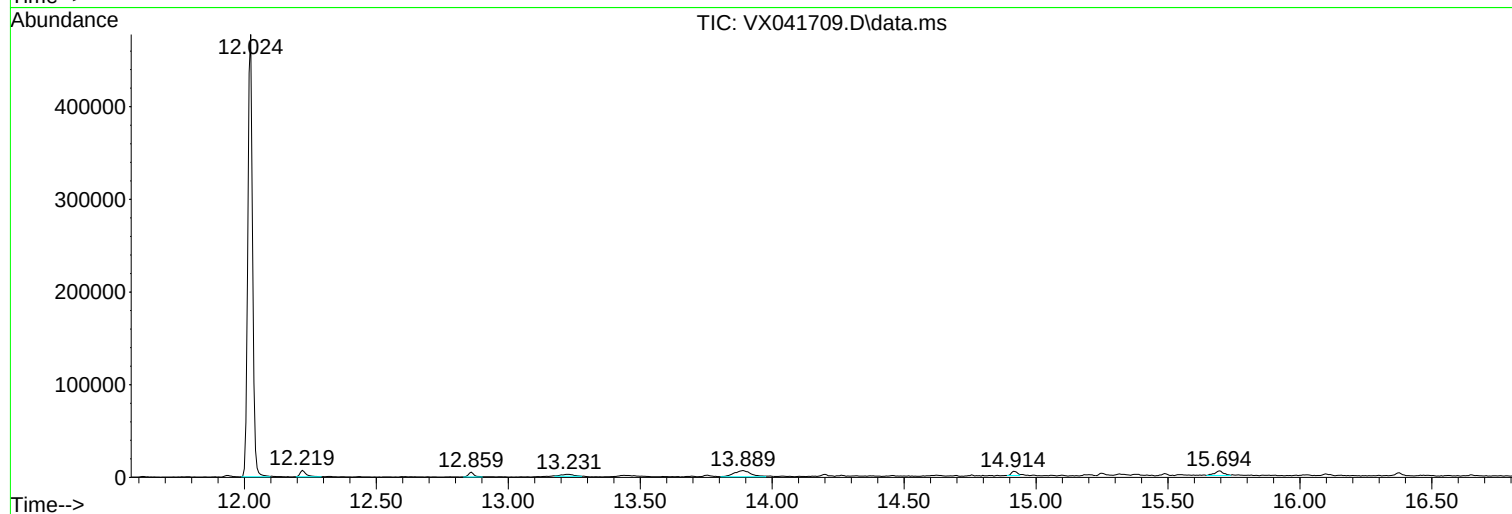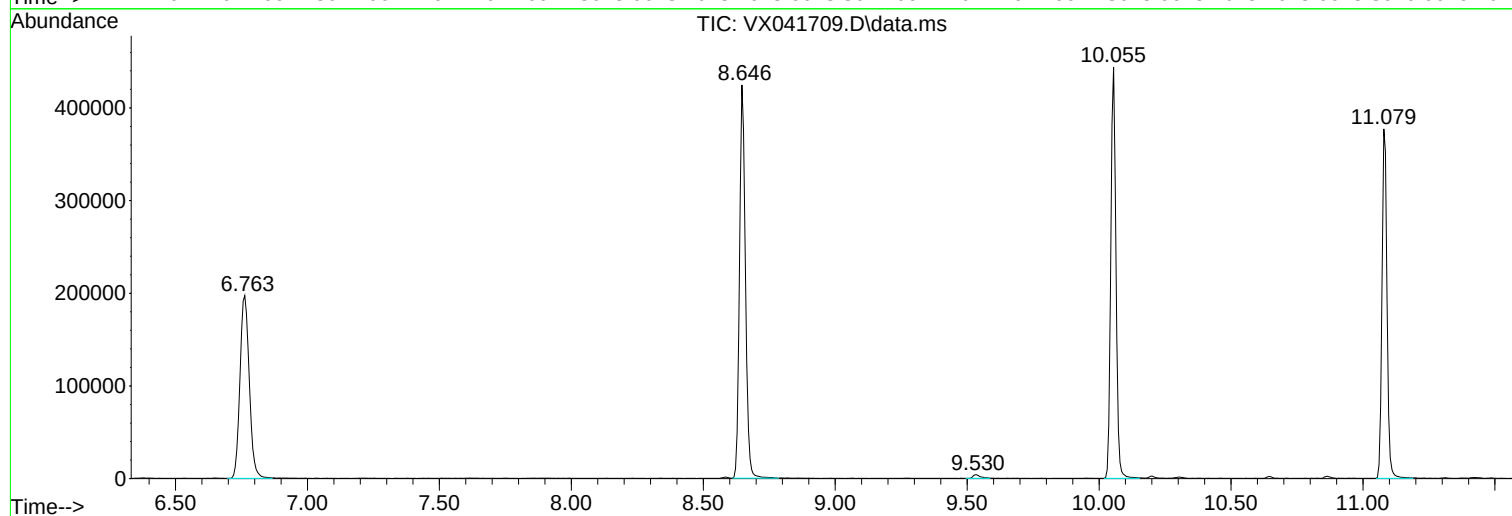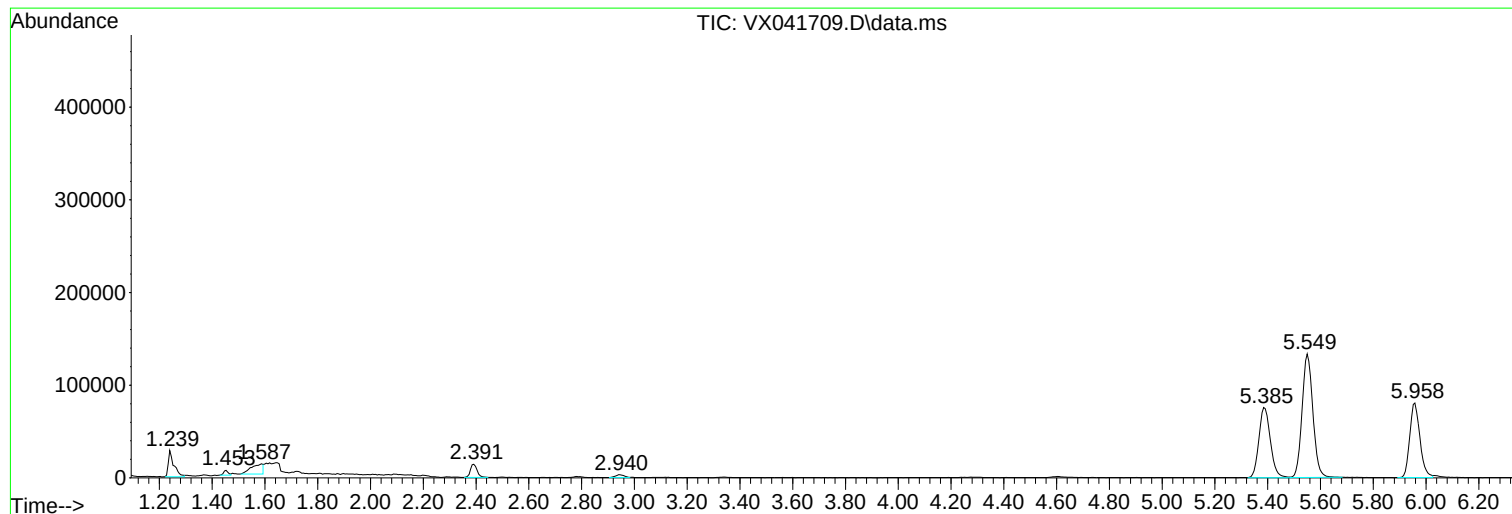

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060324\
Data File : VX041709.D
Acq On : 03 Jun 2024 17:04
Operator : JC/MD
Sample : P2660-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-13










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.239	5.45 ug/l	41392	Pentafluorobenzene	5.549

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	83
2			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
3			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	4

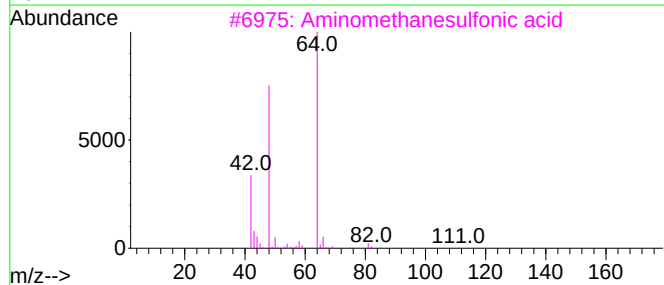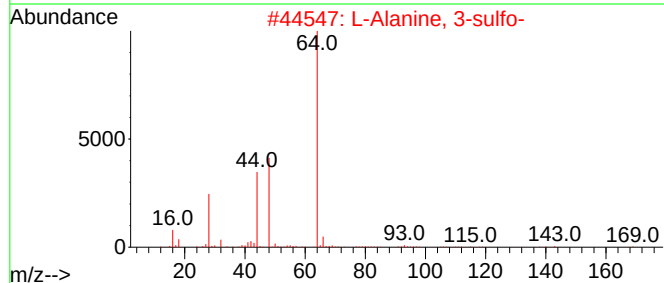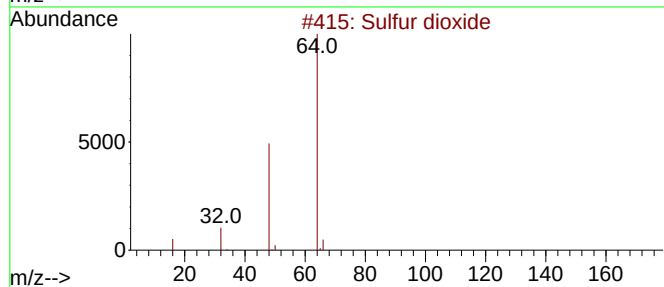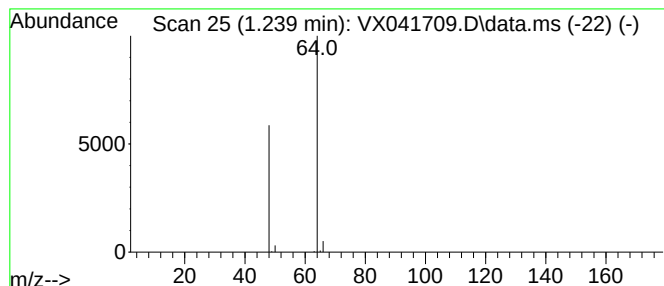

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060324\
Data File : VX041709.D
Acq On : 03 Jun 2024 17:04
Operator : JC/MD
Sample : P2660-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X052924W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.239	5.5	ug/l	41392	1	5.549	379398	50.0