



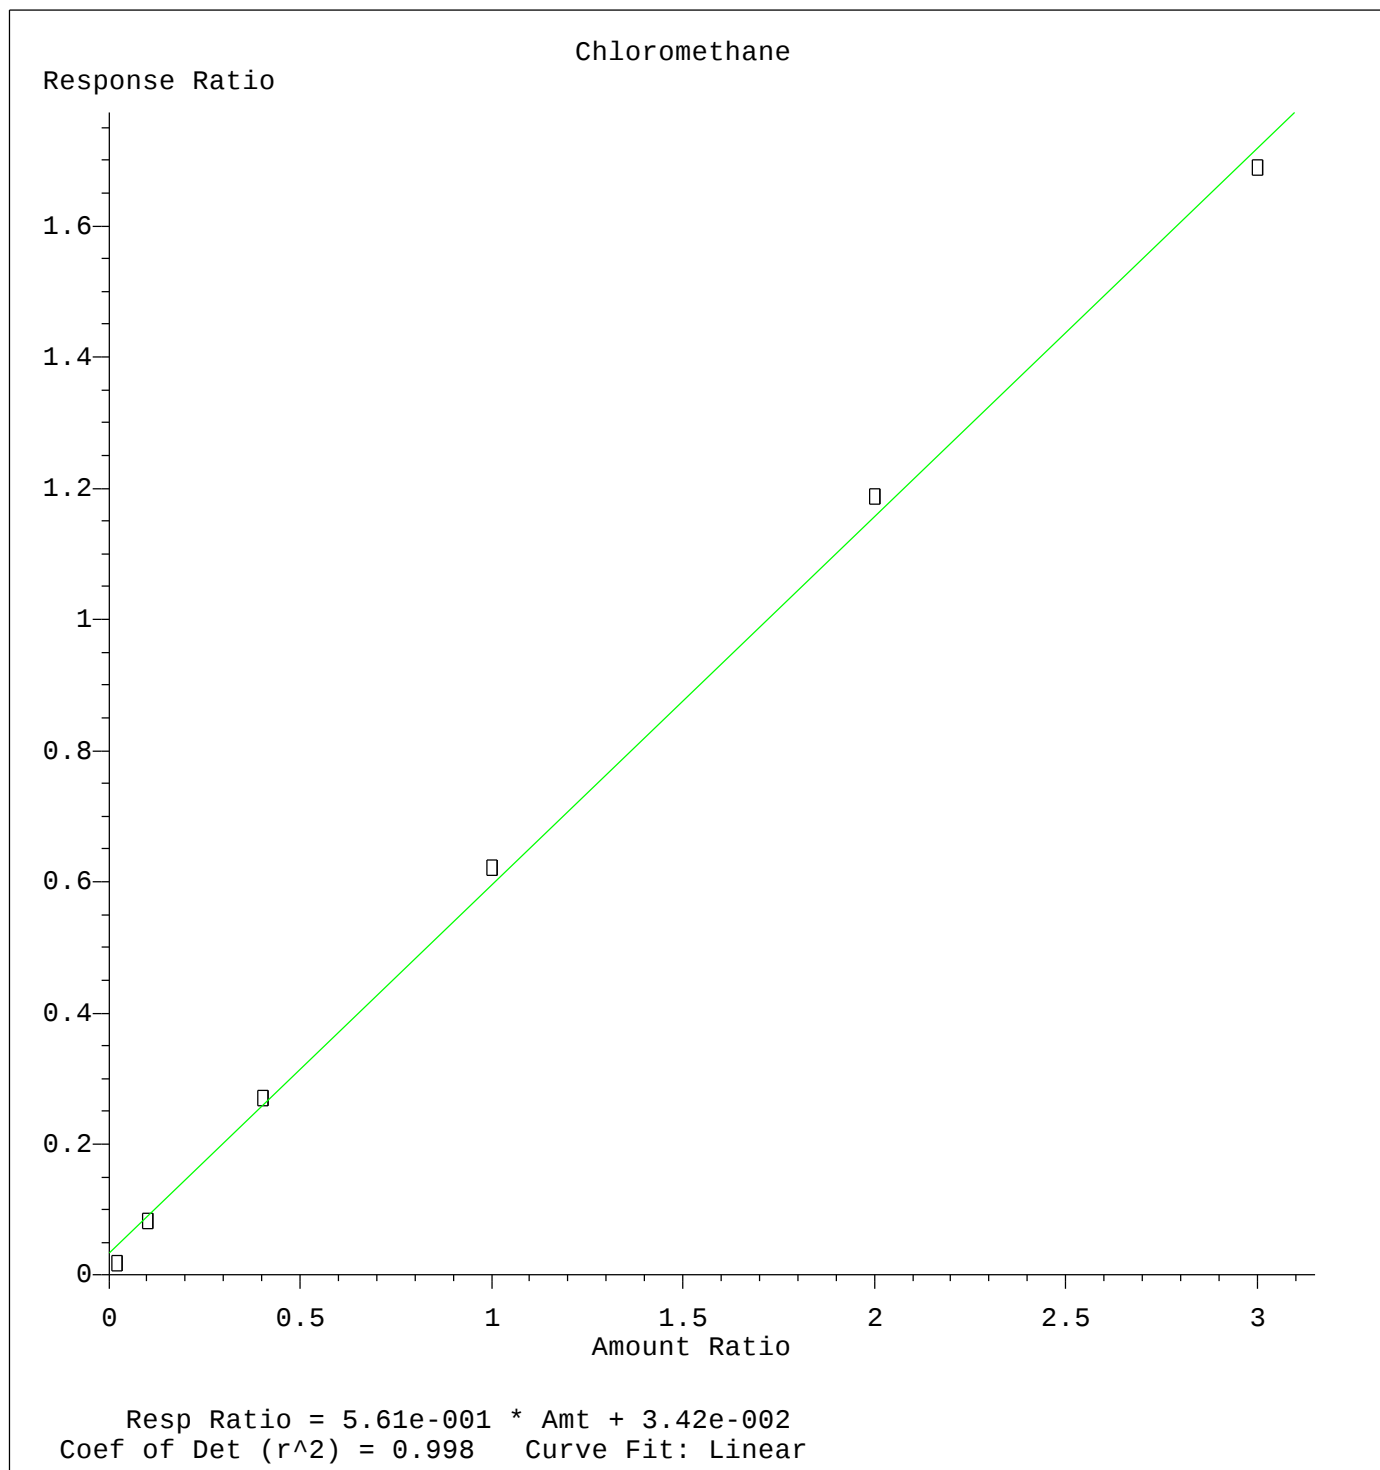


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018

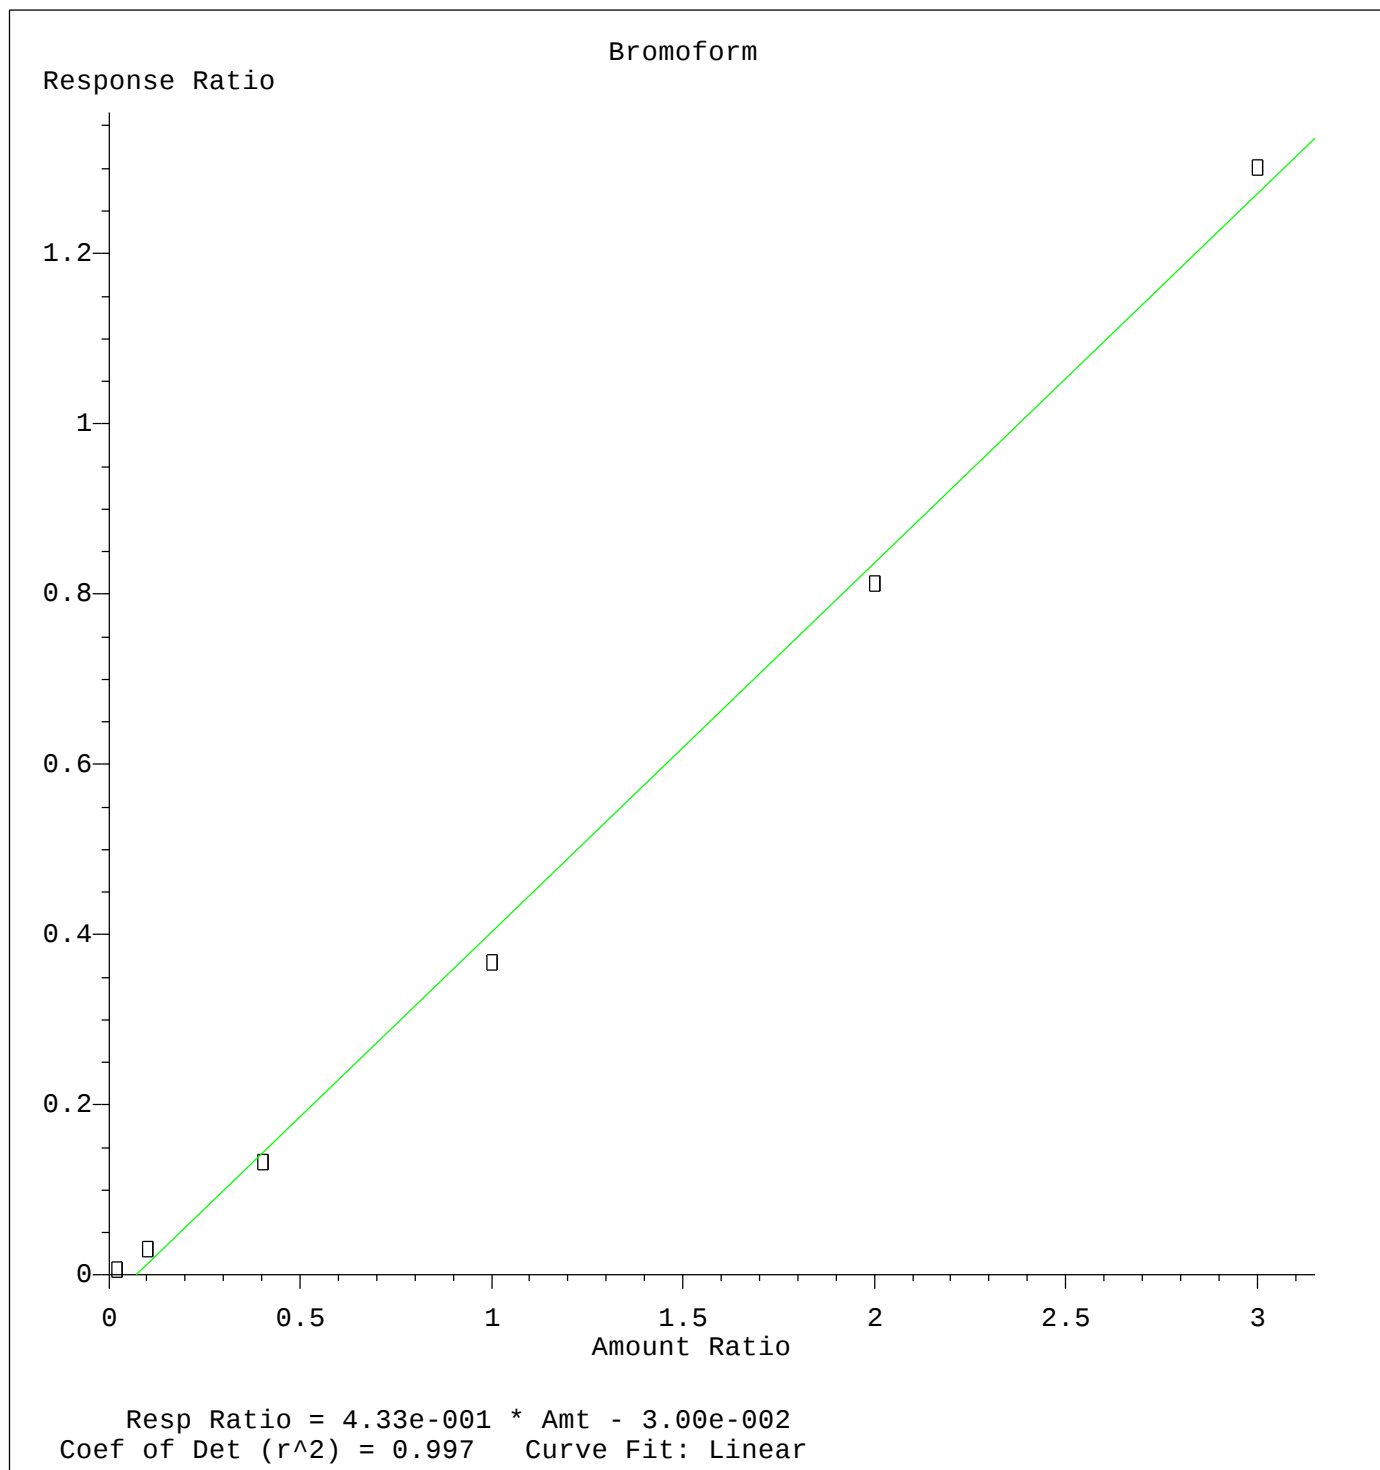

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018

Methylcyclohexane

Response Ratio

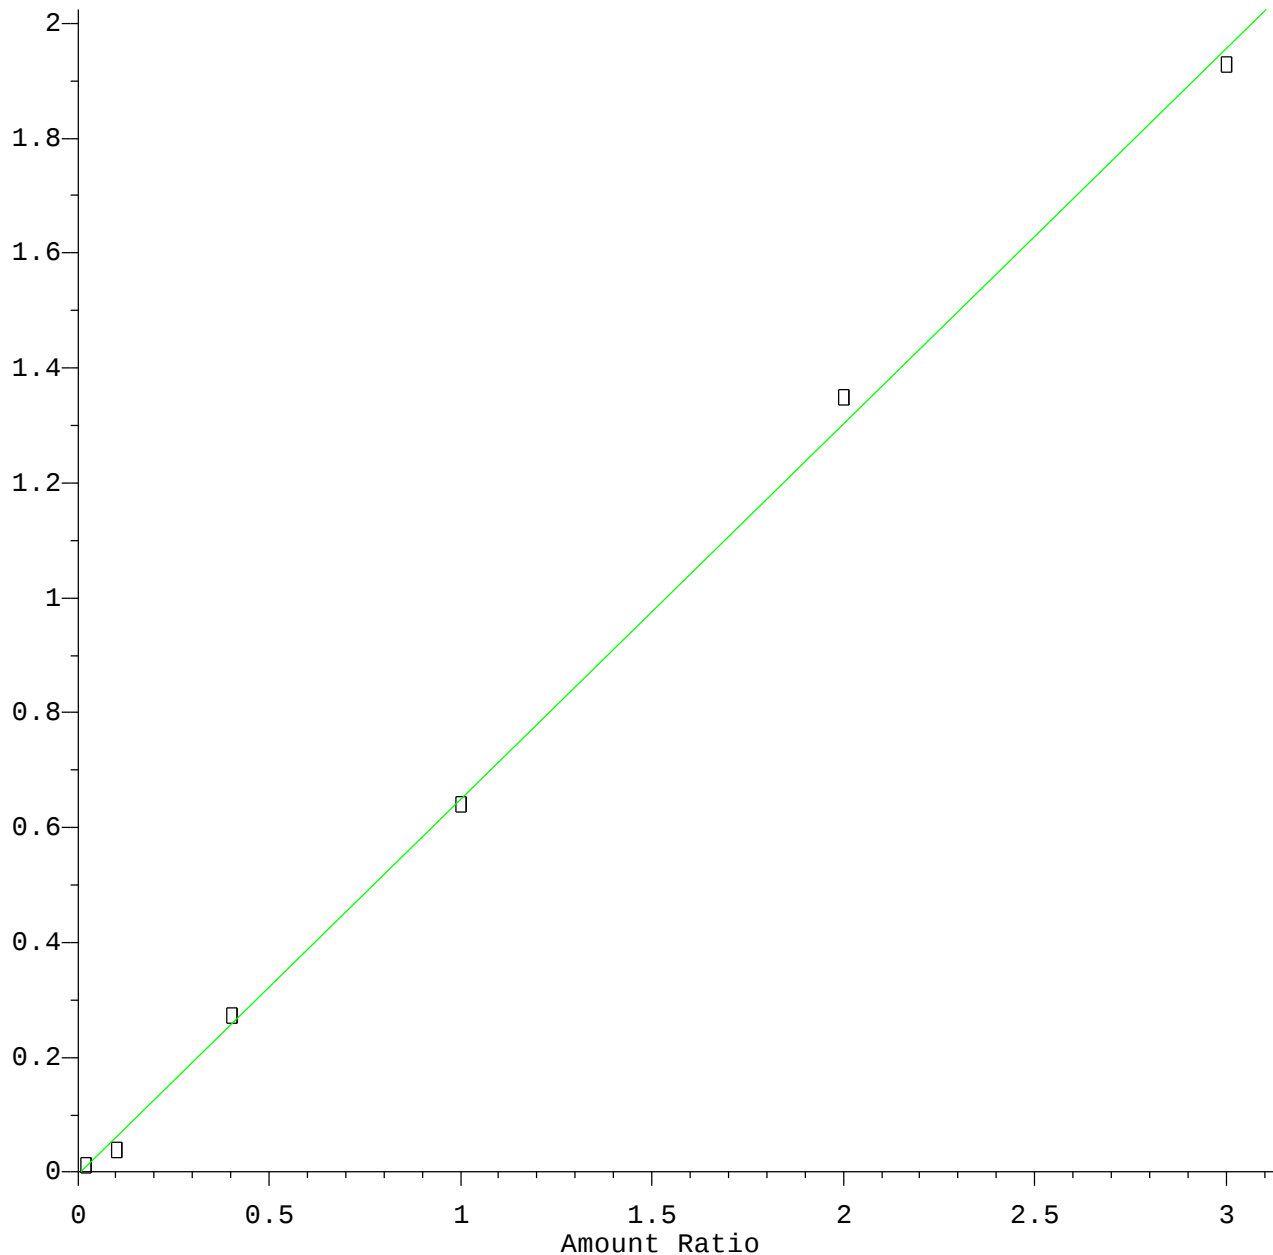


Resp Ratio = 6.53e-001 * Amt - 3.43e-003
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018

1,2-Dichloroethane-d4

Response Ratio

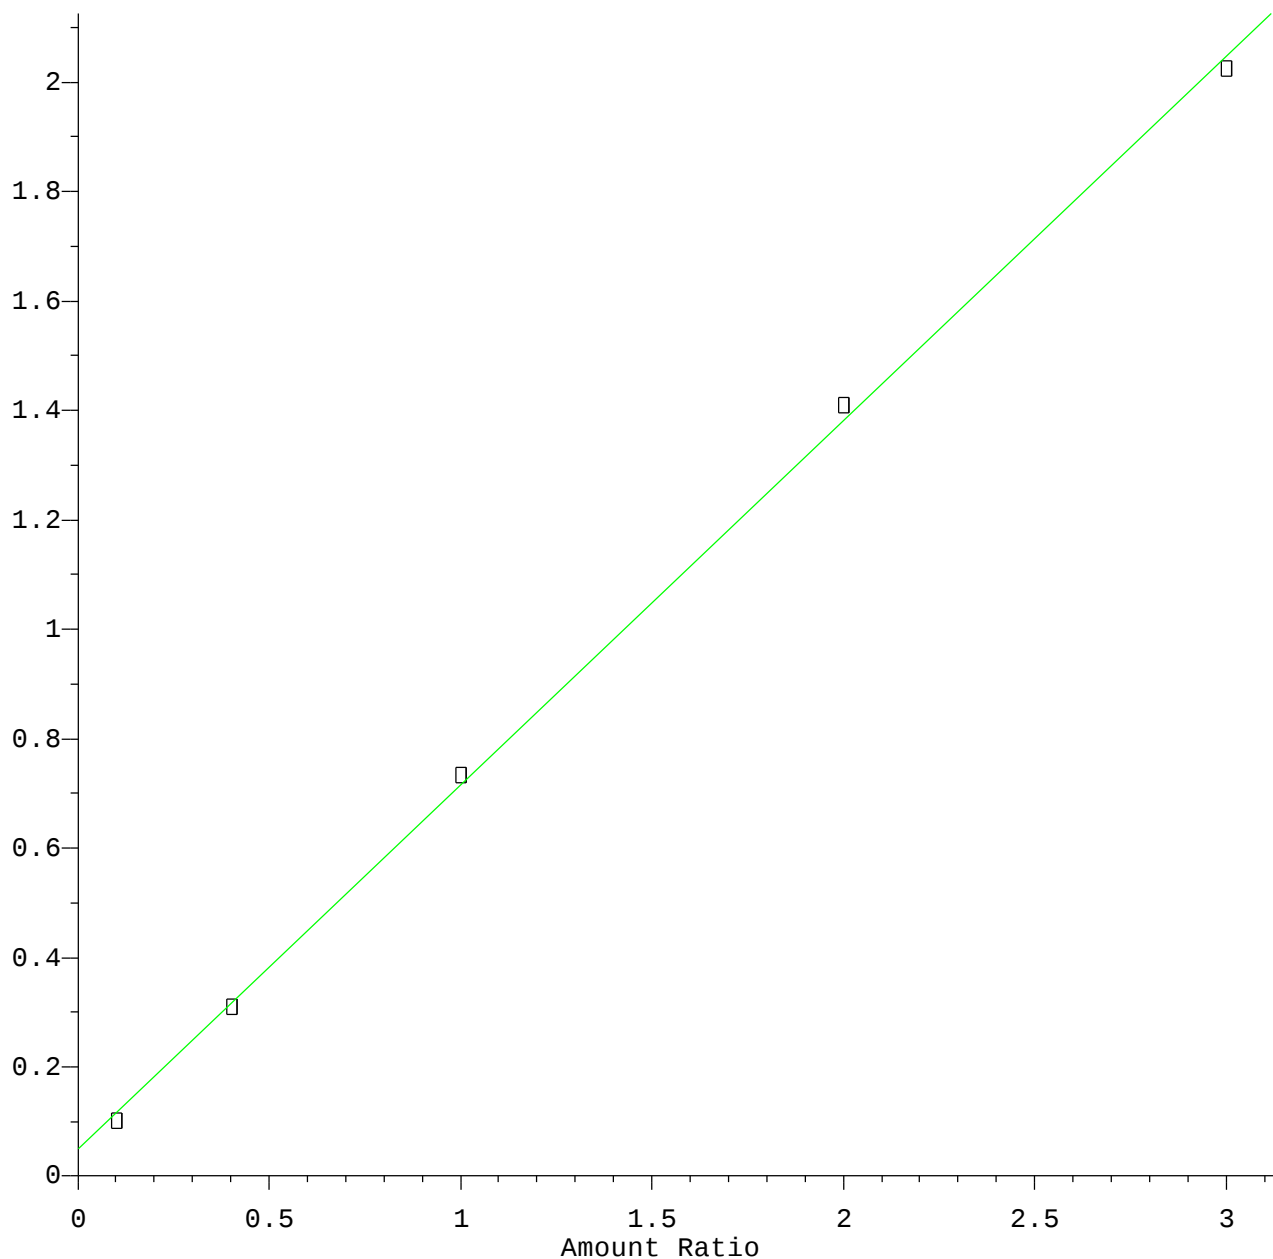


Resp Ratio = $6.66 \times 10^{-1} \times \text{Amt} + 4.95 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018

Bromochloromethane

Response Ratio

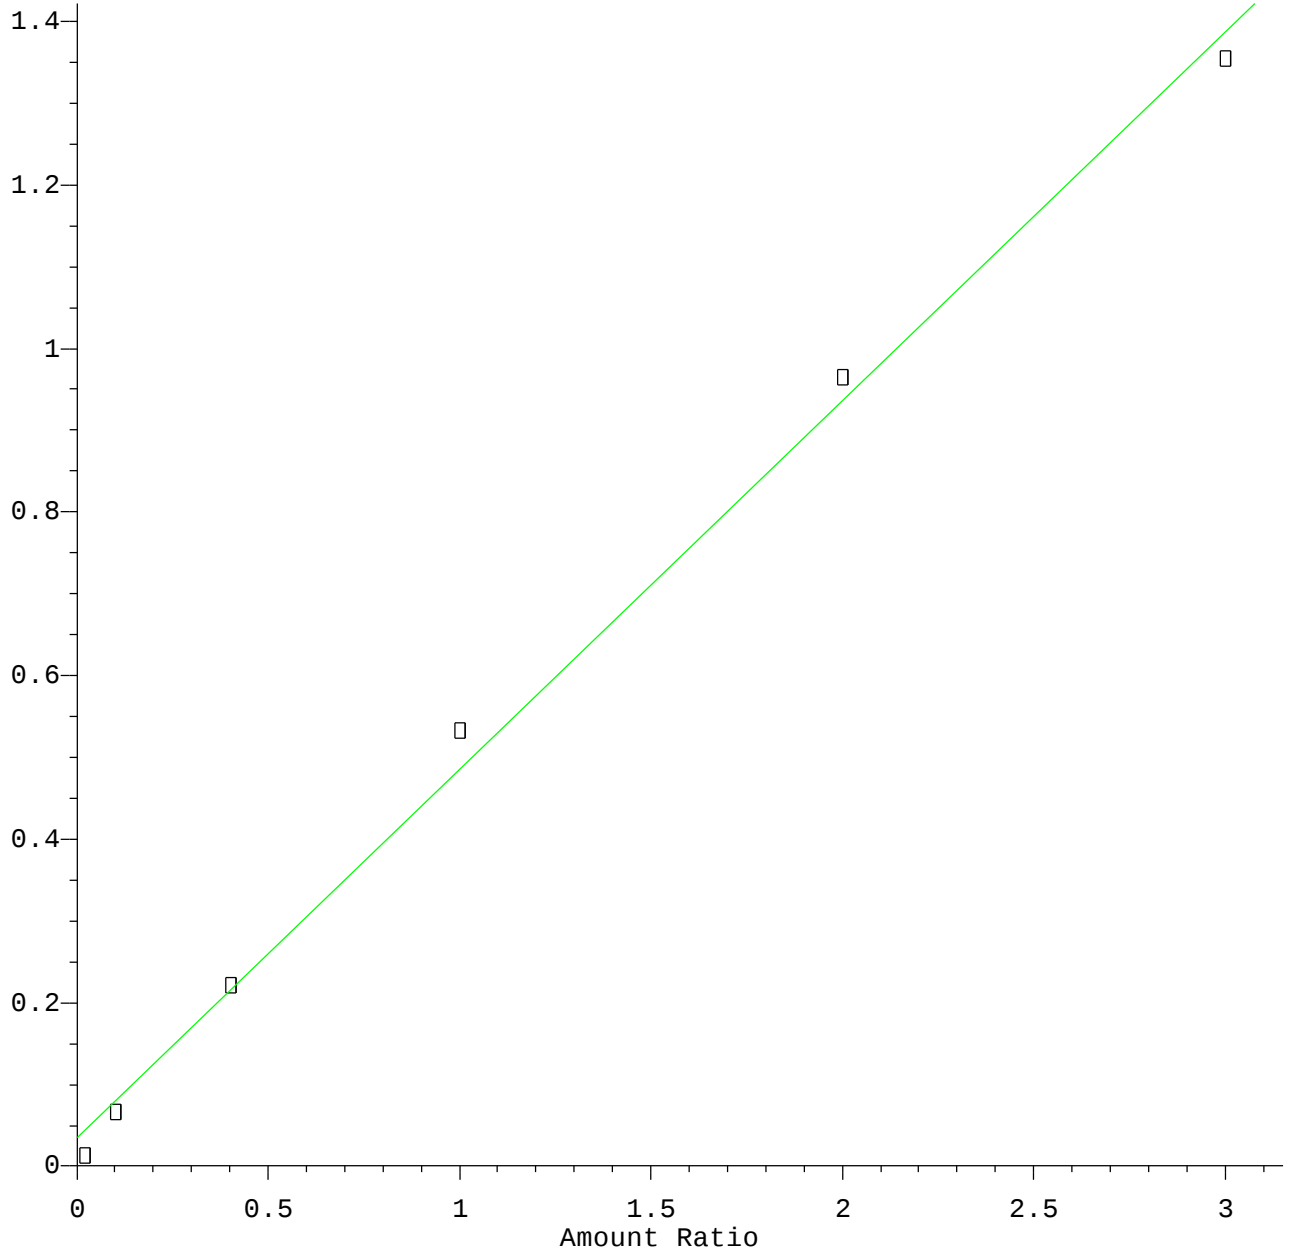


Resp Ratio = $4.51 \times 10^{-1} \times \text{Amt} + 3.46 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018

Diisopropyl ether

Response Ratio

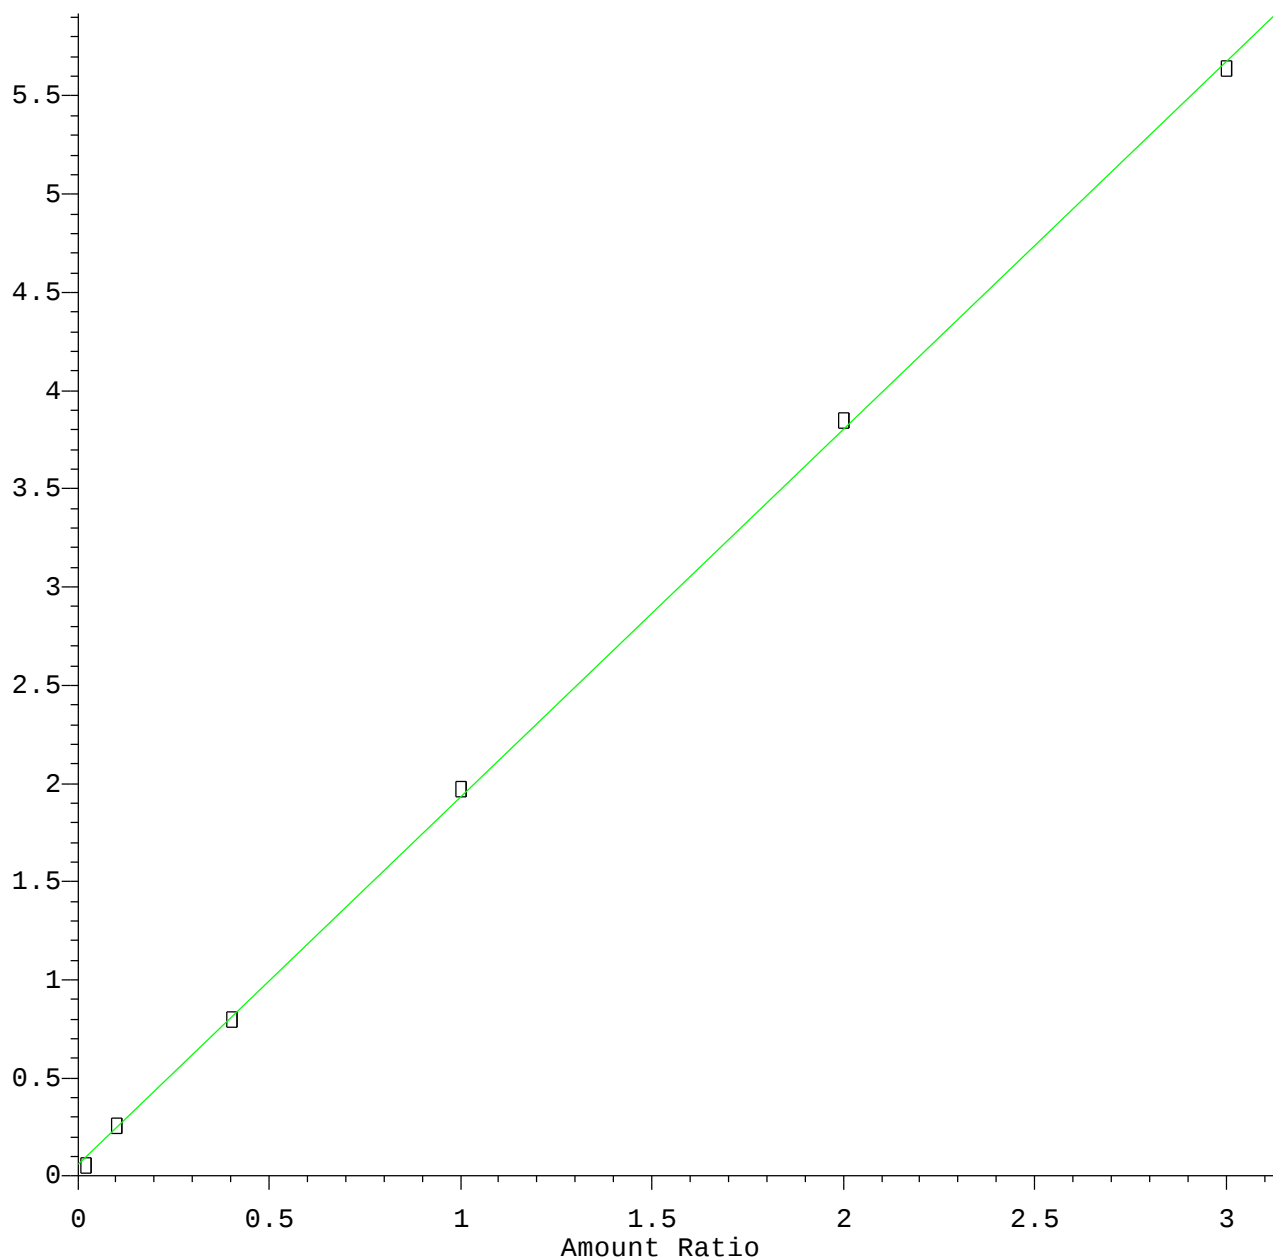


Resp Ratio = 1.87e+000 * Amt + 5.74e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018

Methylene Chloride

Response Ratio

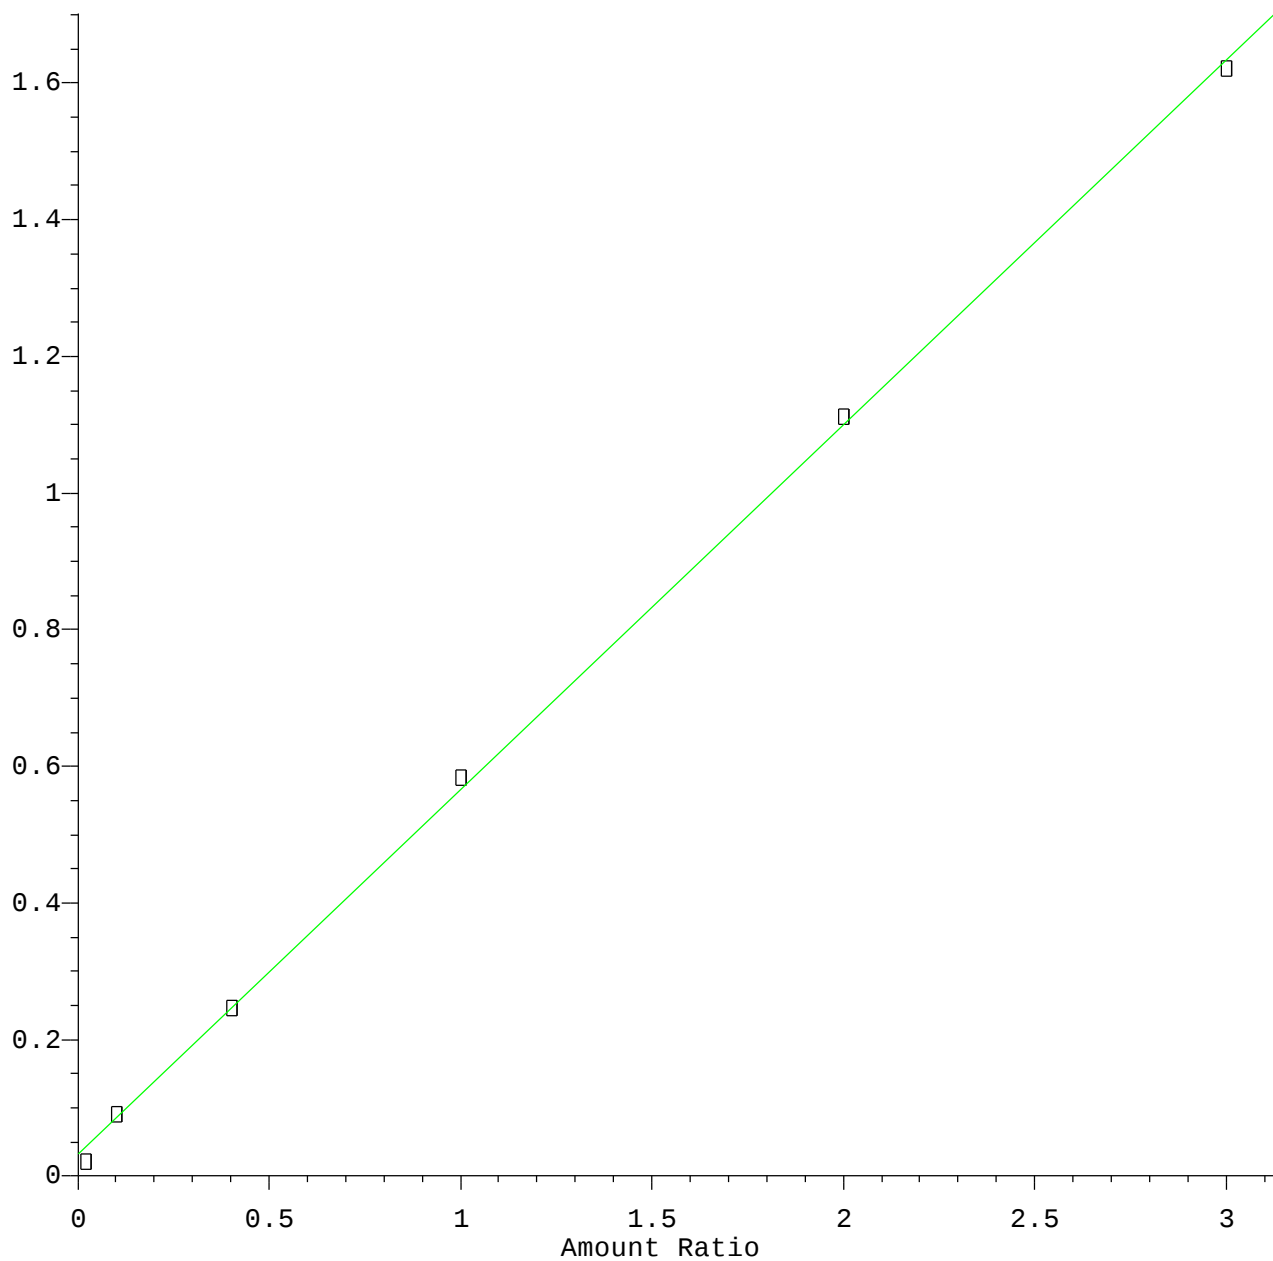


Resp Ratio = $5.34 \times 10^{-1} \times \text{Amt} + 3.12 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018


Methyl tert-butyl Ether

Response Ratio

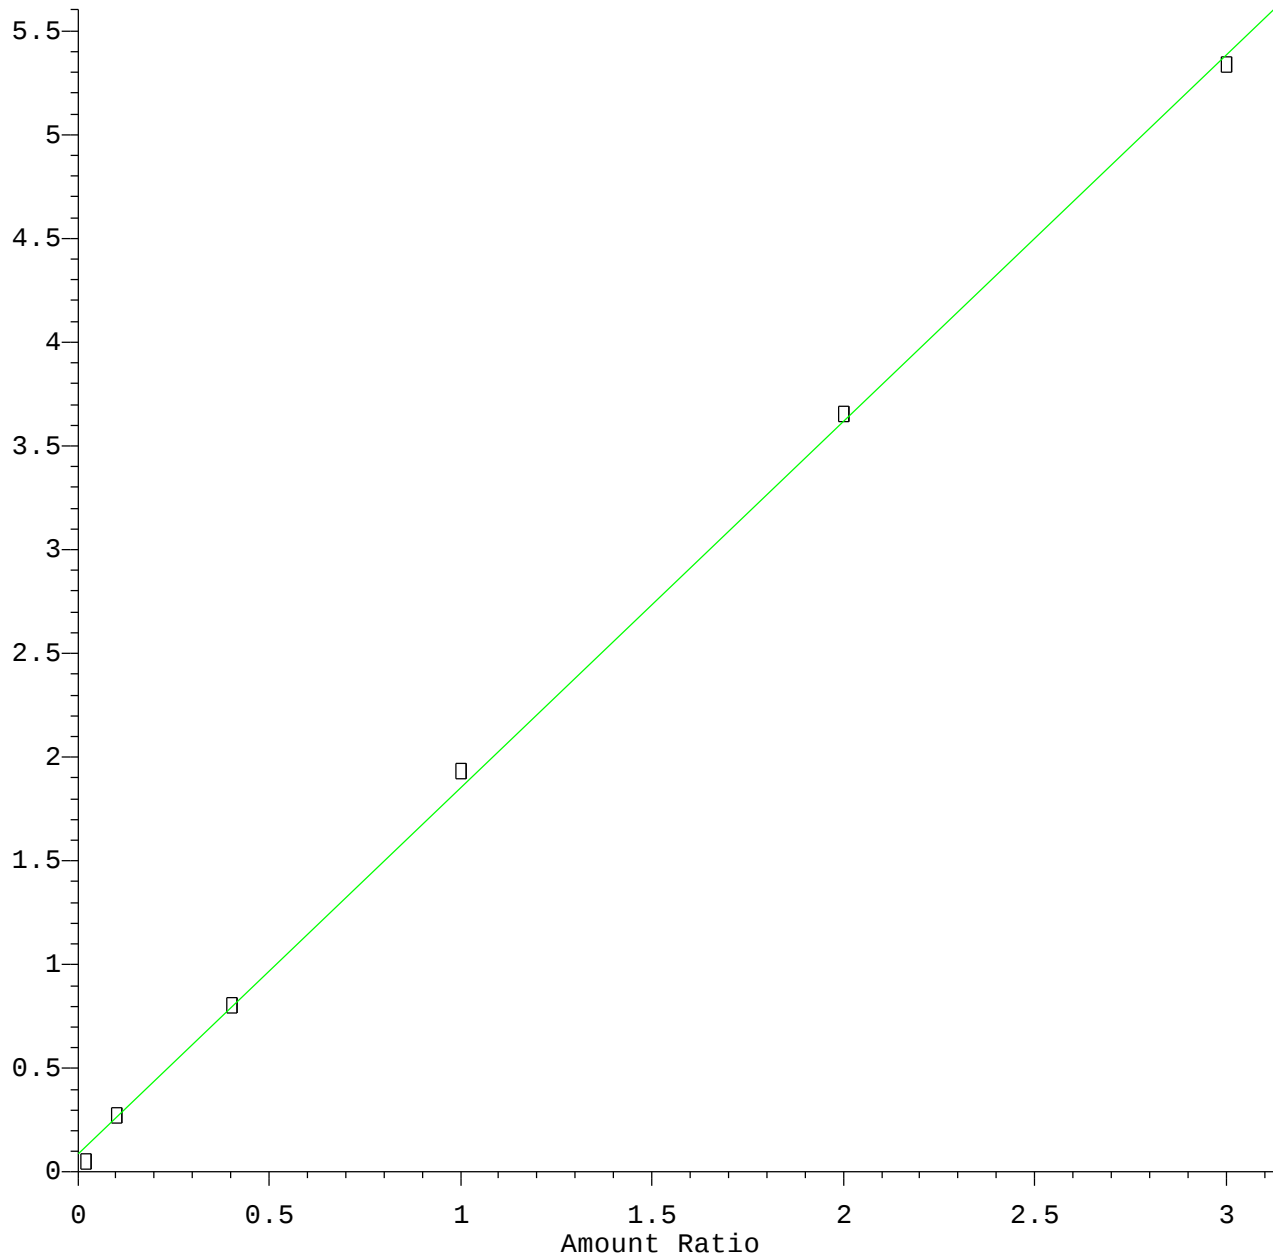


Resp Ratio = 1.76e+000 * Amt + 8.86e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018

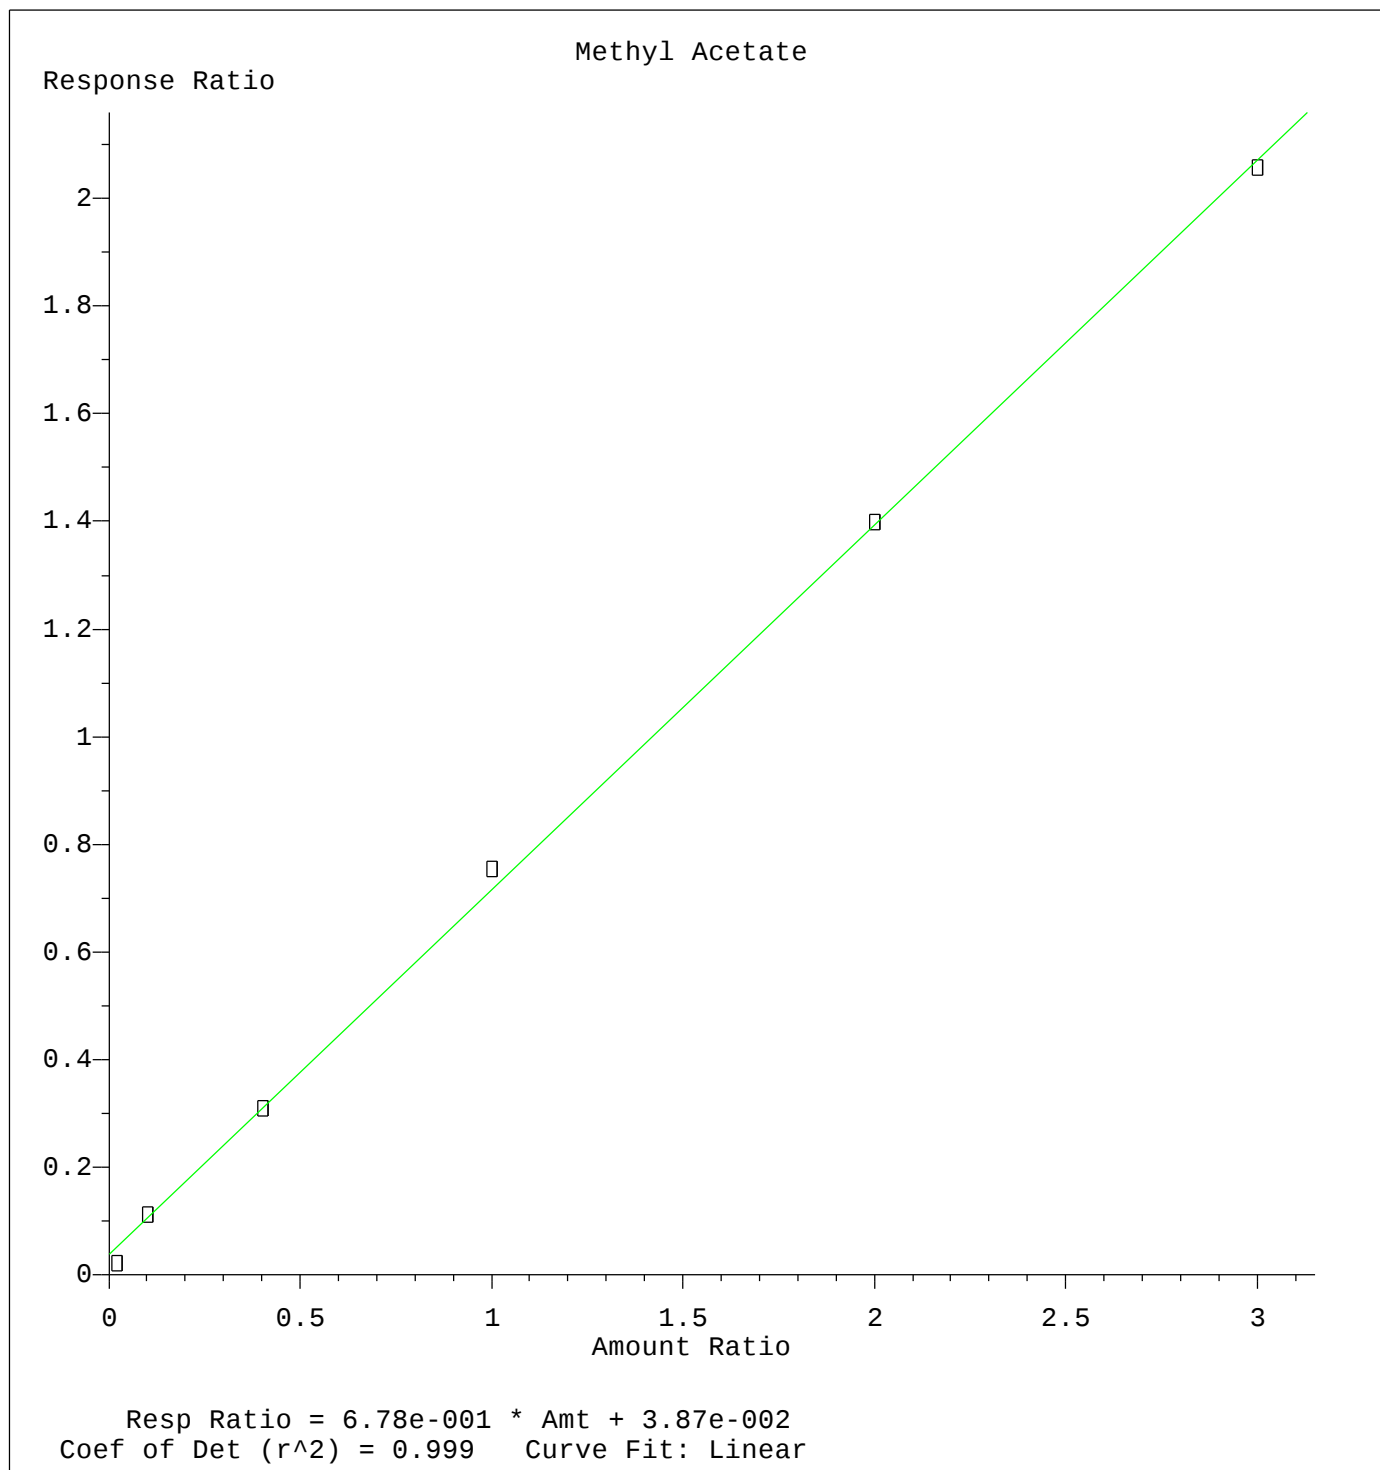

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018

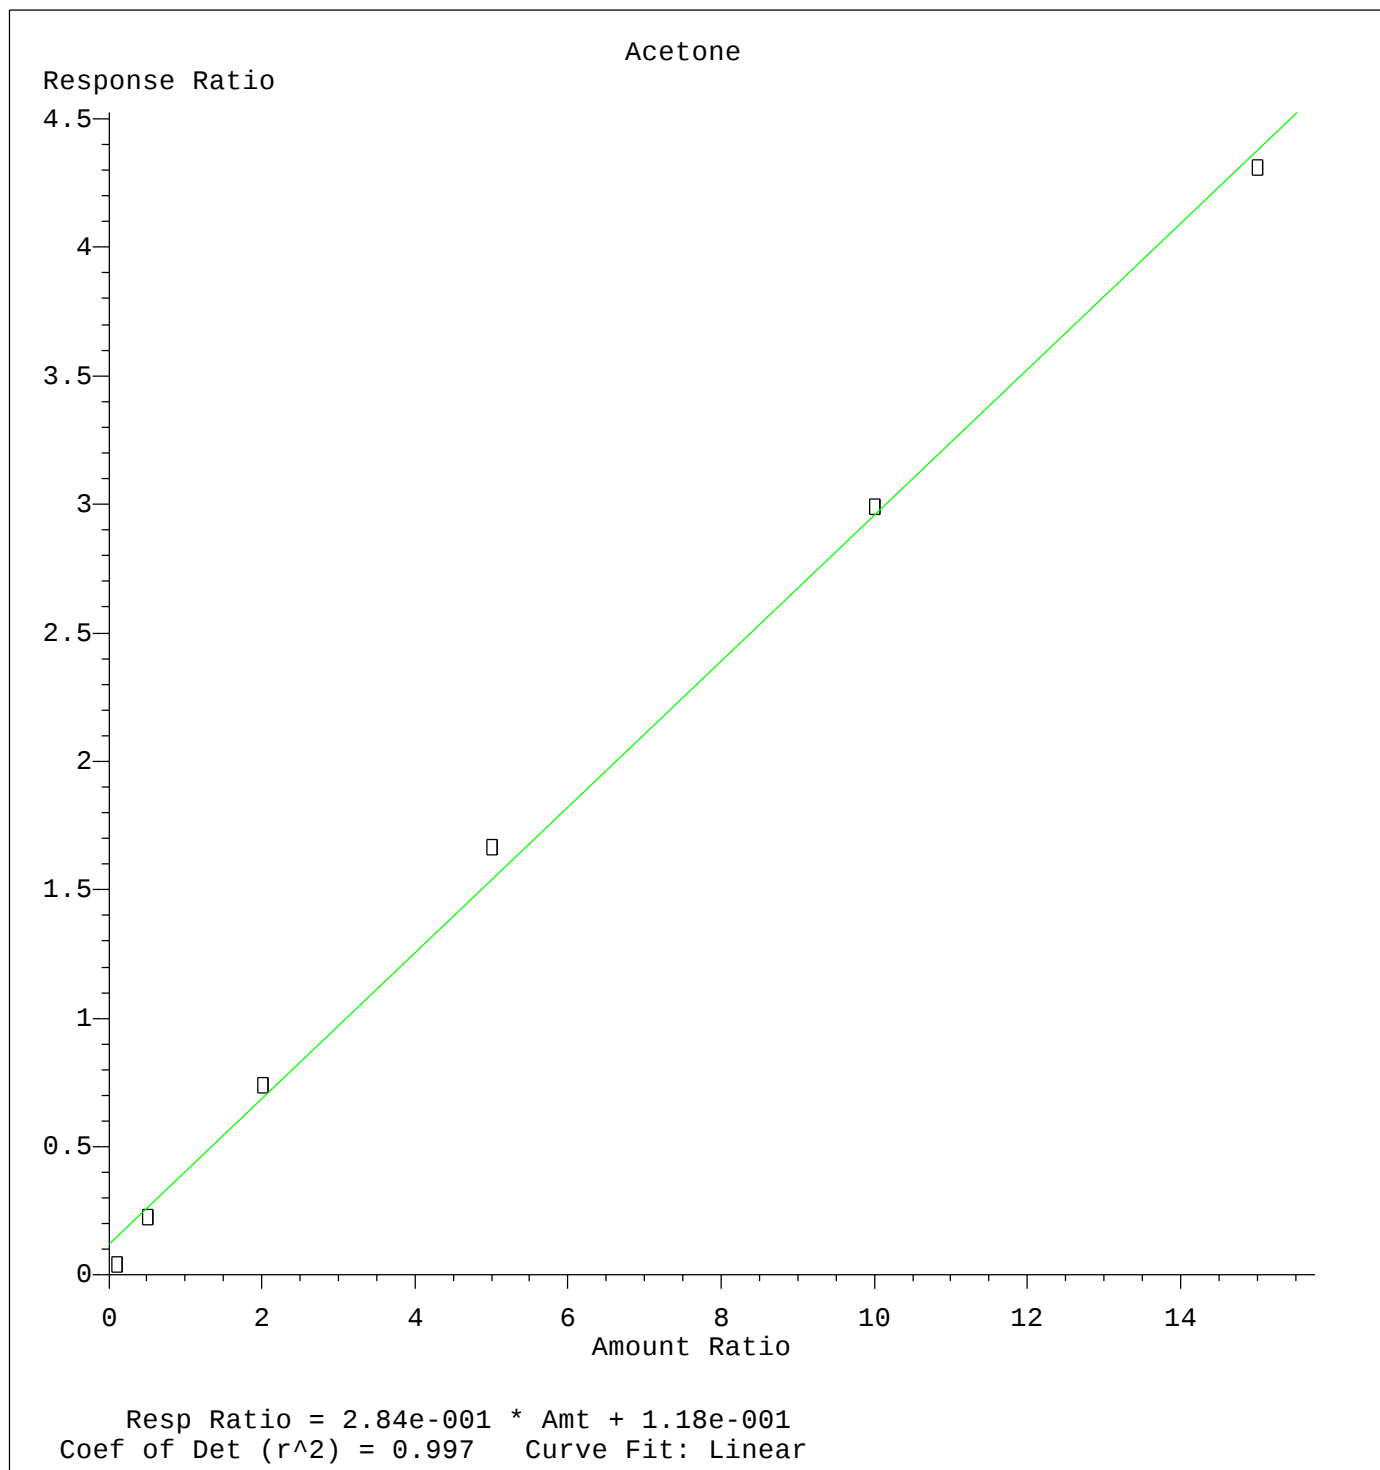


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018

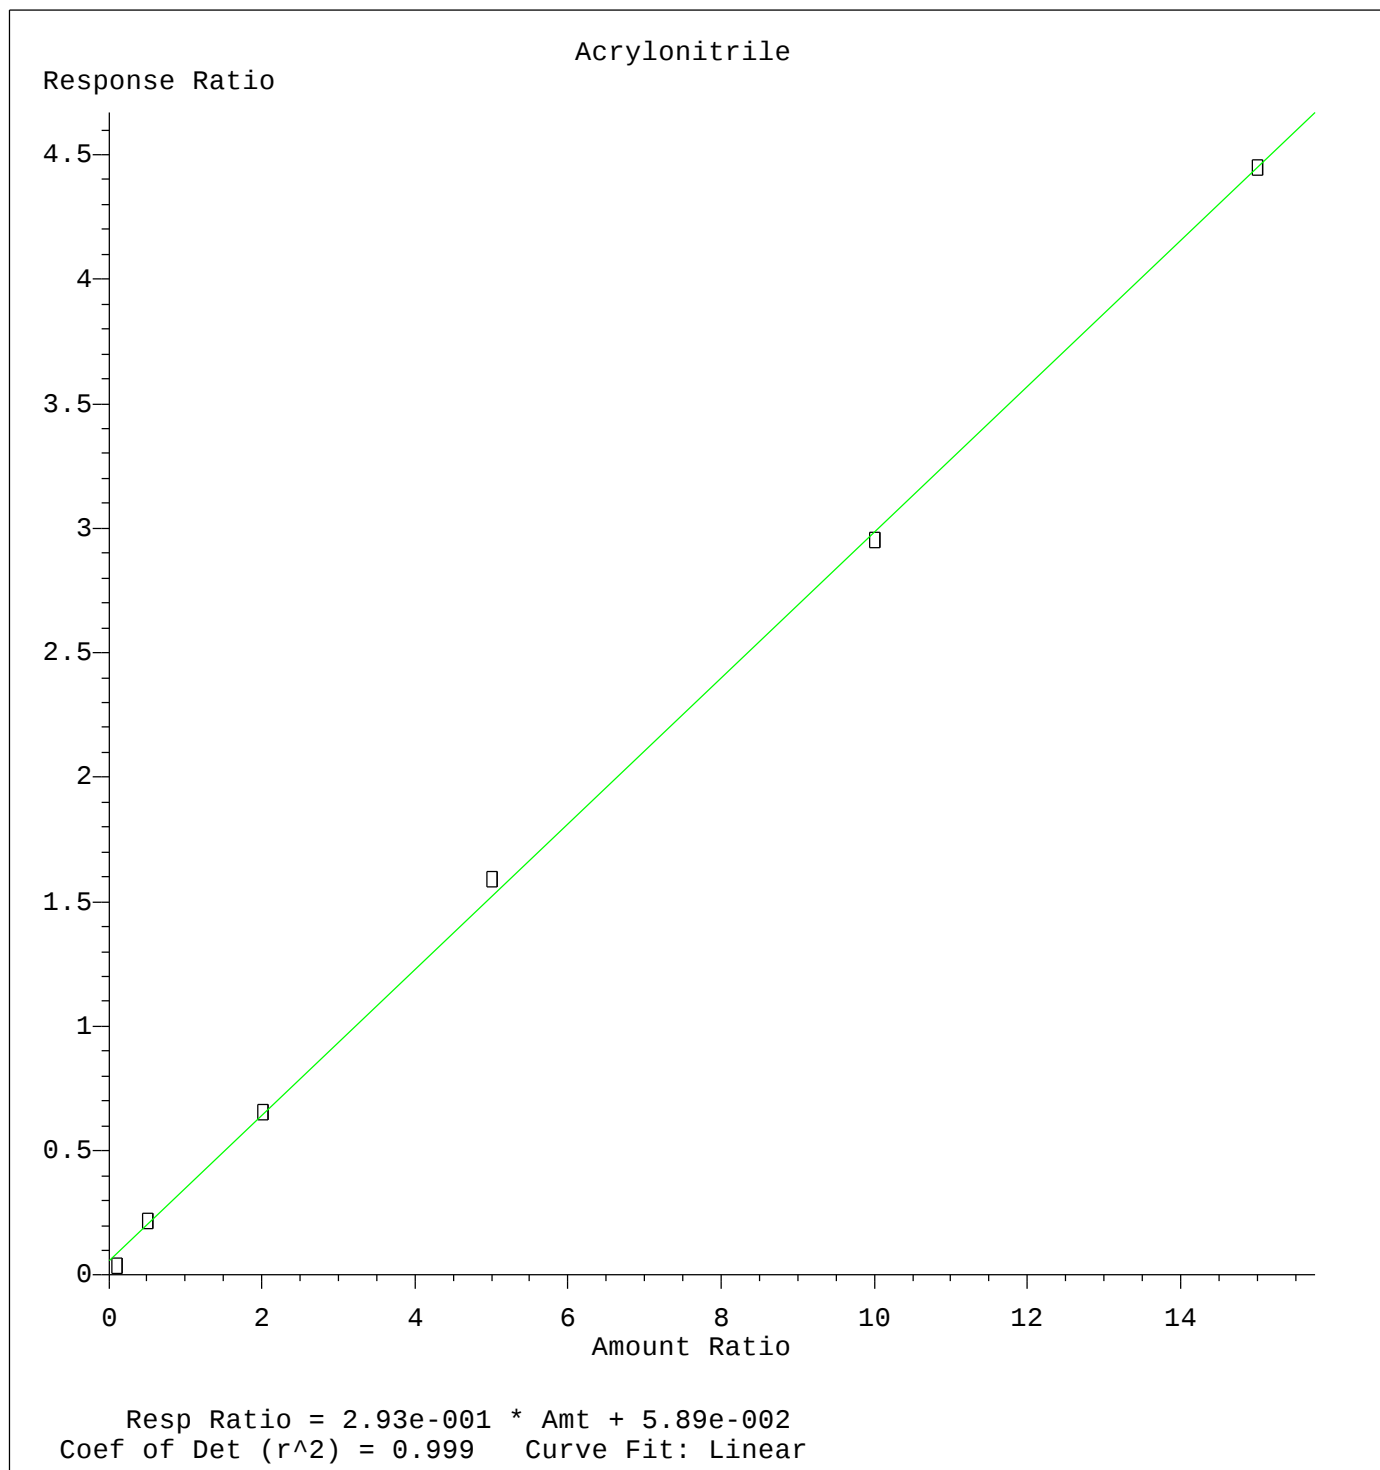

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018


Acrolein

Response Ratio

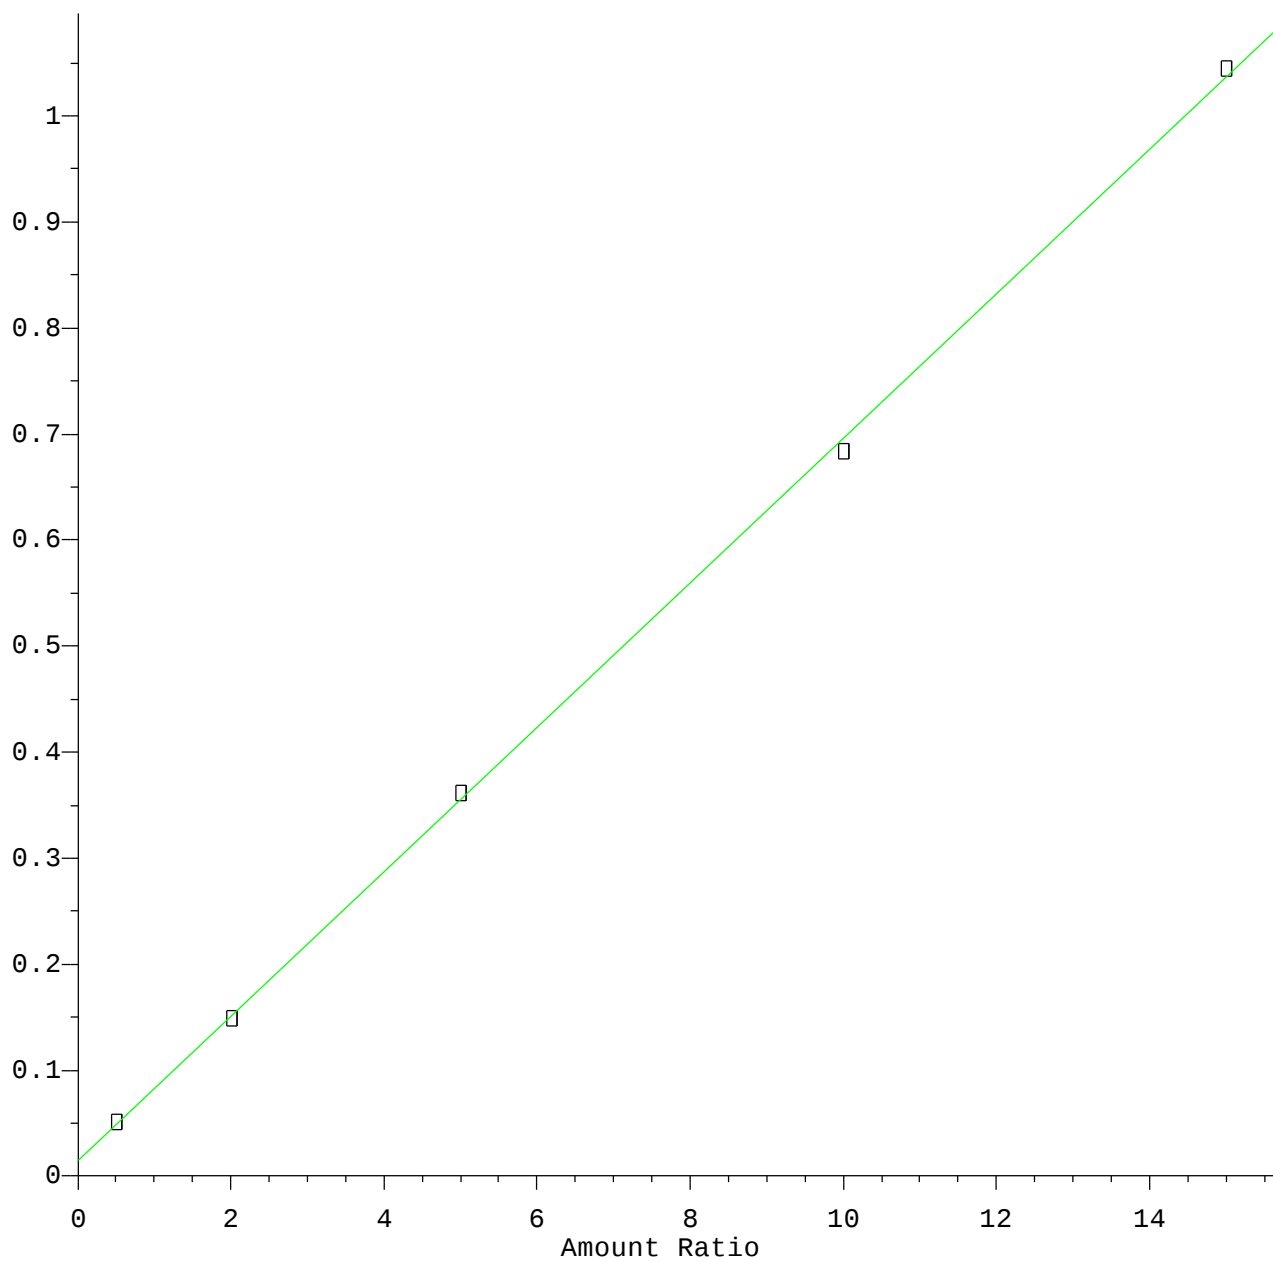


Resp Ratio = $6.82 \times 10^{-2} \times \text{Amt} + 1.39 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018

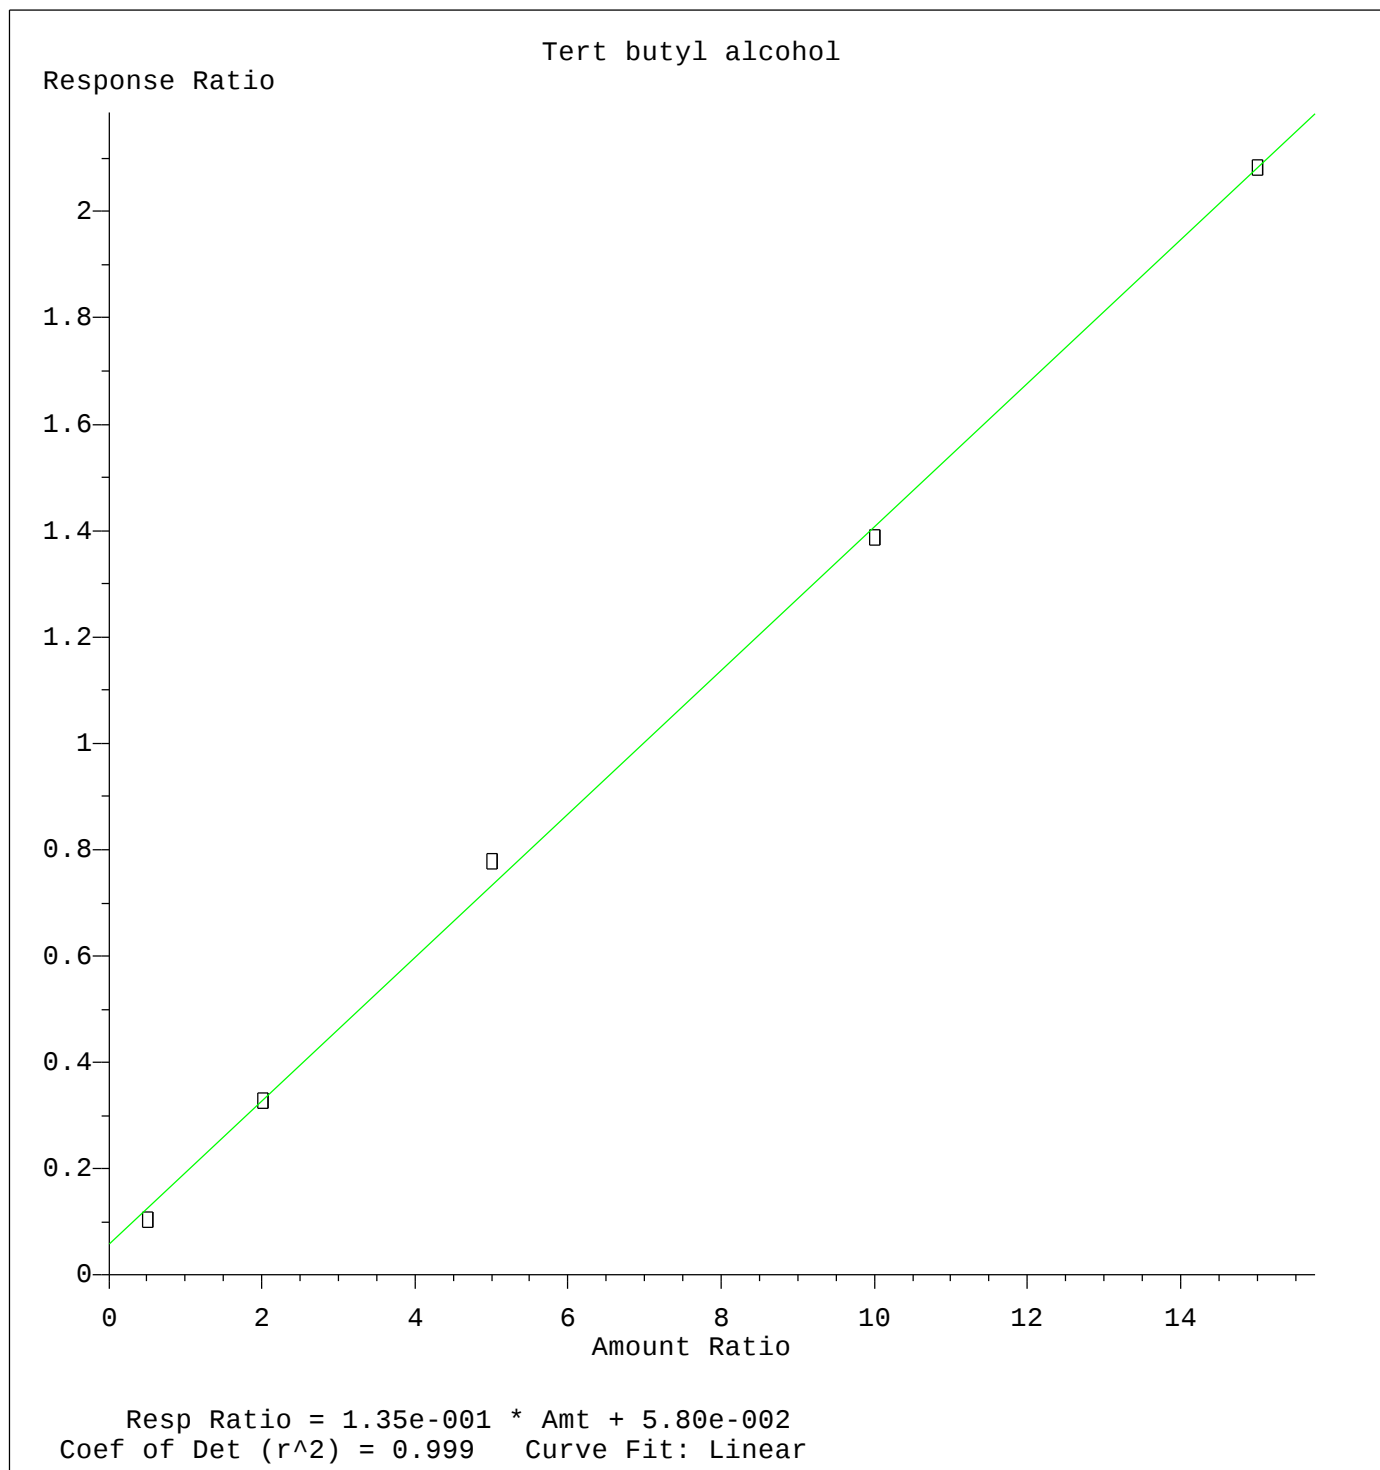

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018

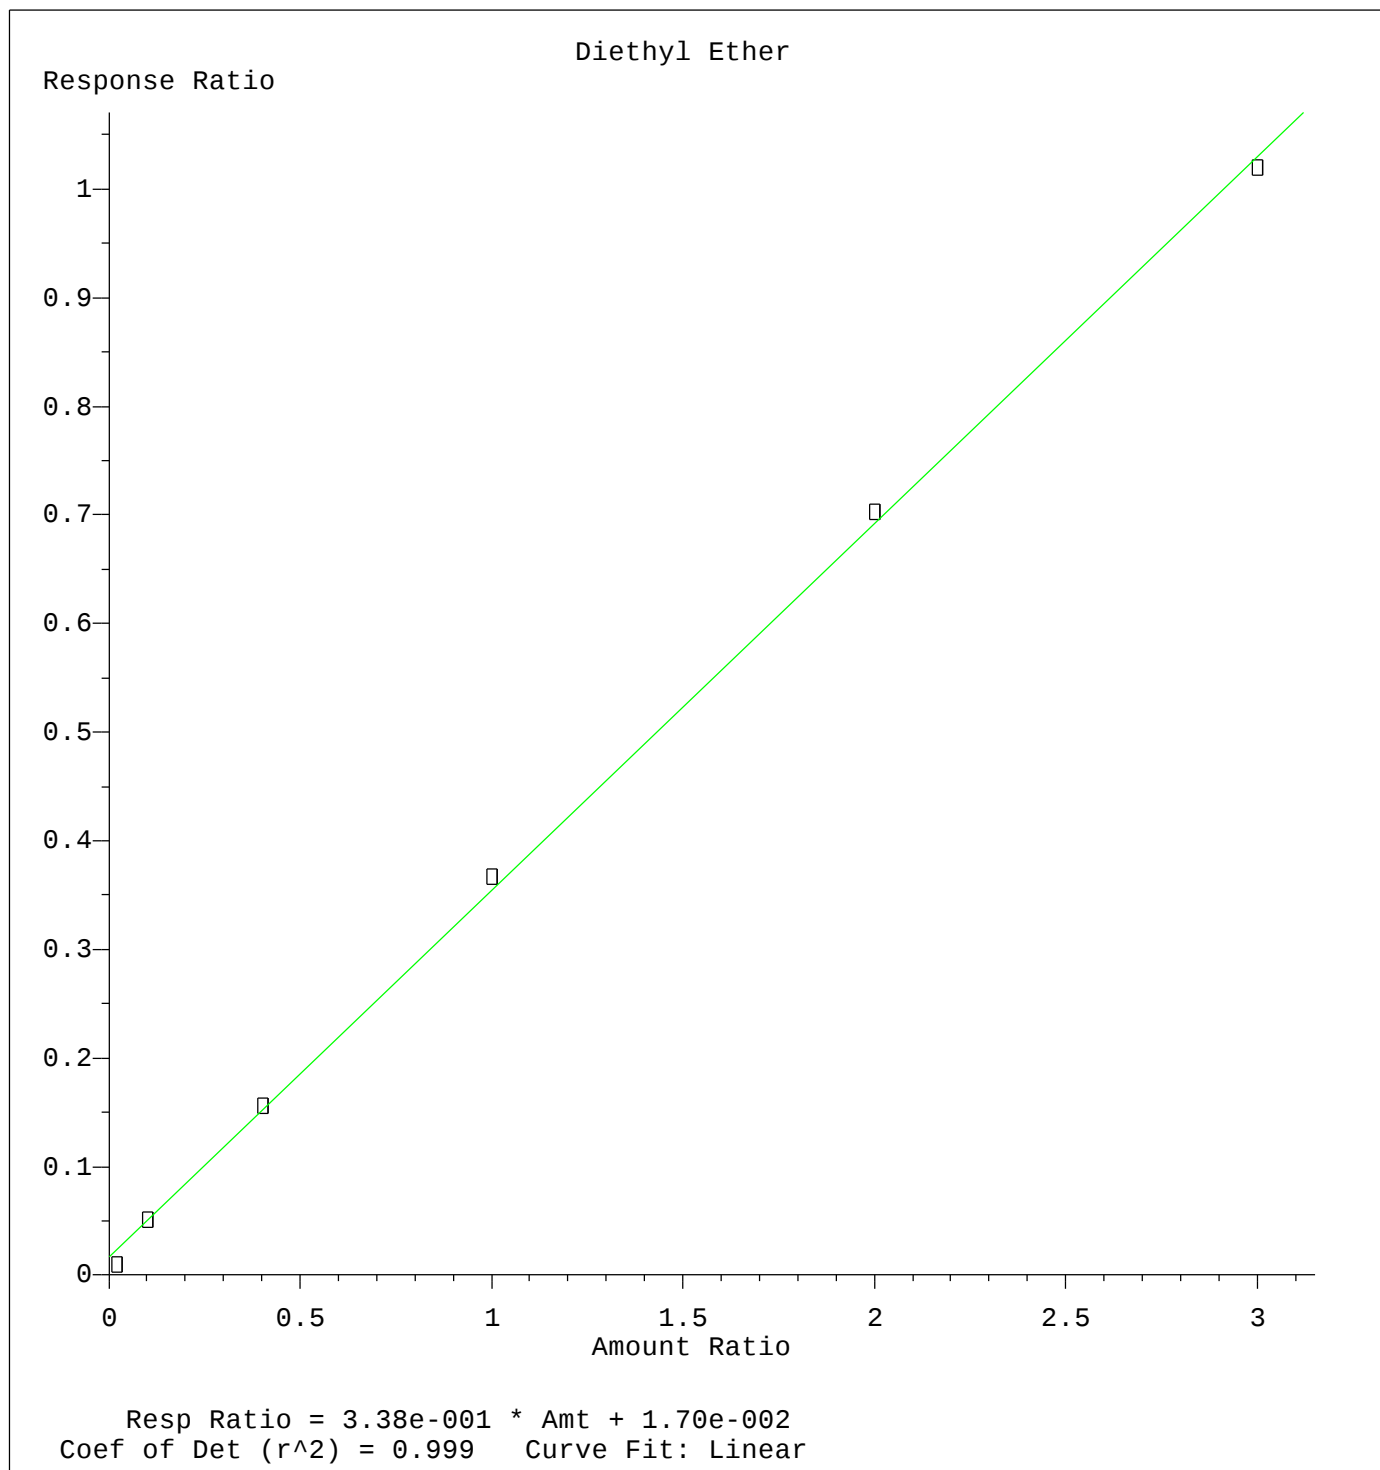

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018

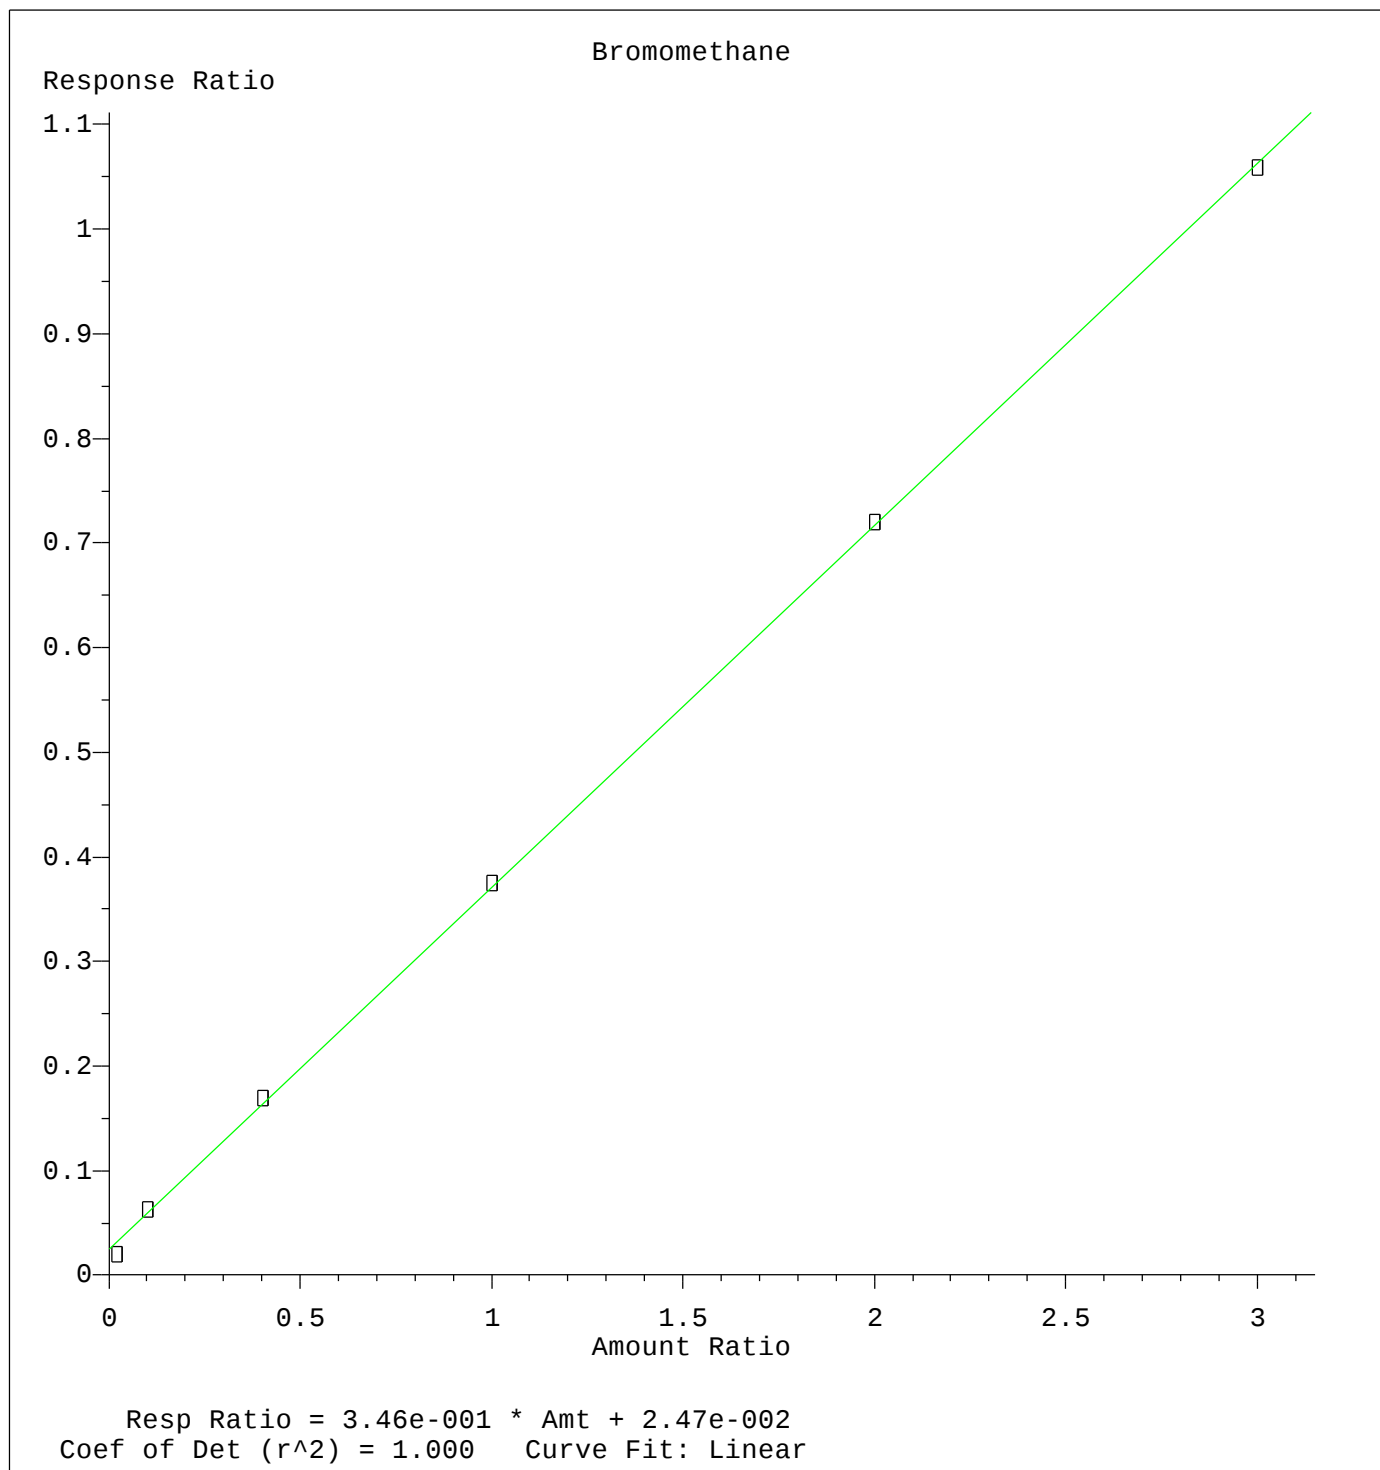

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Calibration Table Last Updated: Tue Jun 05 03:22:35 2018