

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060421\
 Data File : VX022418.D
 Acq On : 04 Jun 2021 17:24
 Operator : JC/MD
 Sample : M2583-01ME
 Misc : 5.05g/10mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jun 05 03:21:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	63093	50.000	ug/l	#-0.01
34) 1,4-Difluorobenzene	6.763	114	129485	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	114309	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	50382	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	50654	52.046	ug/l	0.00
Spiked Amount 50.000	Range 78	- 117	Recovery	=	104.100%	
35) Dibromofluoromethane	5.397	113	37492	45.659	ug/l	0.00
Spiked Amount 50.000	Range 75	- 124	Recovery	=	91.320%	
50) Toluene-d8	8.653	98	159426	50.402	ug/l	0.00
Spiked Amount 50.000	Range 92	- 112	Recovery	=	100.800%	
62) 4-Bromofluorobenzene	11.085	95	57489	49.172	ug/l	0.00
Spiked Amount 50.000	Range 83	- 123	Recovery	=	98.340%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.294	50	224	0.271	ug/l #	77
5) Bromomethane	1.599	94	497	0.974	ug/l #	78
6) Chloroethane	1.691	64	111	0.213	ug/l #	53
10) Methyl Iodide	2.428	142	888	1.105	ug/l #	94
11) Tert butyl alcohol	2.953	59	2171	9.753	ug/l #	73
13) Acrolein	2.252	56	76	0.515	ug/l #	26
16) Acetone	2.434	43	4898	11.558	ug/l	95
17) Carbon Disulfide	2.471	76	1819	0.960	ug/l #	94
18) Methyl Acetate	2.678	43	276	0.245	ug/l #	47
20) Methylene Chloride	2.770	84	852	0.905	ug/l #	72
25) 2-Butanone	4.617	43	294	0.429	ug/l #	45
29) Tetrahydrofuran	5.068	42	733	1.796	ug/l #	64
31) Cyclohexane	5.495	56	1072	0.877	ug/l #	20
36) 1,1-Dichloropropene	5.550	75	6019	5.027	ug/l #	47
38) Carbon Tetrachloride	5.544	117	7451	6.362	ug/l #	15
39) Methylcyclohexane	7.379	83	483	0.356	ug/l #	54
51) 4-Methyl-2-Pentanone	8.598	43	1487	1.034	ug/l #	54
52) Toluene	8.720	92	10003	4.288	ug/l	96
59) 2-Hexanone	9.439	43	422	0.390	ug/l	62
67) Ethyl Benzene	10.195	91	2833	0.647	ug/l	95
68) m/p-Xylenes	10.305	106	5007	3.027	ug/l	94
69) o-Xylene	10.646	106	2112	1.313	ug/l	71
70) Styrene	10.659	104	1170	0.444	ug/l #	72
73) Isopropylbenzene	10.970	105	1067	0.250	ug/l #	69
74) N-amyl acetate	10.860	43	522	0.258	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.220	83	343	0.243	ug/l #	26
76) 1,2,3-Trichloropropane	11.085	75	30362	24.428	ug/l #	39
78) n-propylbenzene	11.305	91	1181	0.236	ug/l	100
79) 2-Chlorotoluene	11.372	91	627	0.207	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.457	105	2663	0.754	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.085	75	30362	57.878	ug/l #	12
82) 4-Chlorotoluene	11.457	91	809	0.232	ug/l #	57
84) 1,2,4-Trimethylbenzene	11.756	105	5613	1.578	ug/l	97
85) sec-Butylbenzene	11.890	105	949	0.220	ug/l	82
86) p-Isopropyltoluene	12.012	119	3845	1.057	ug/l #	81
89) n-Butylbenzene	12.335	91	1428	0.424	ug/l #	62


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060421\
Data File : VX022418.D
Acq On : 04 Jun 2021 17:24
Operator : JC/MD
Sample : M2583-01ME
Misc : 5.05g/10mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jun 05 03:21:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260
QLast Update : Wed May 19 14:23:10 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
90) Hexachloroethane	12.530	117	547	0.910	ug/l #	9
93) 1,2,4-Trichlorobenzene	13.591	180	329	0.326	ug/l #	32
94) Hexachlorobutadiene	13.731	225	305	0.773	ug/l	65
95) Naphthalene	13.780	128	1933	0.491	ug/l #	72
96) 1,2,3-Trichlorobenzene	13.975	180	294	0.289	ug/l #	64

(#) = qualifier out of range (m) = manual integration (+) = signals summed






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.012 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Instrument :
MSVOA_X
ClientSampled :







Tgt Ion:168 Resp: 63093
Ion Ratio Lower Upper
168 100
99 70.9 45.8 68.6#

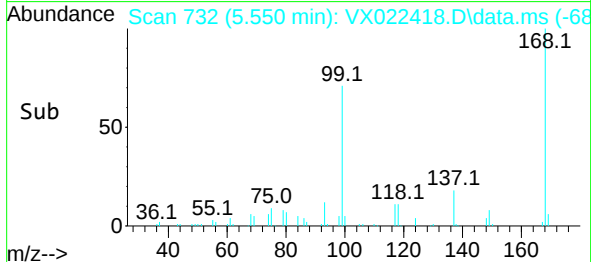

#3
Chloromethane
Concen: 0.271 ug/l
RT: 1.294 min Scan# 34
Delta R.T. -0.001 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion: 50 Resp: 224
Ion Ratio Lower Upper
50 100
52 20.1 26.4 39.6#


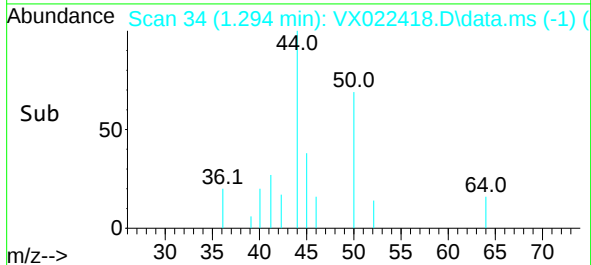

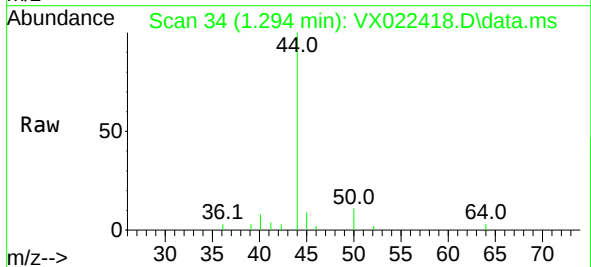


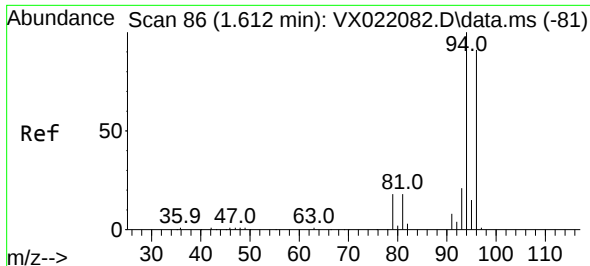

#5
Bromomethane
Concen: 0.974 ug/l
RT: 1.599 min Scan# 84
Delta R.T. -0.013 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 94 Resp: 497
Ion Ratio Lower Upper
94 100
96 74.5 76.4 114.6#

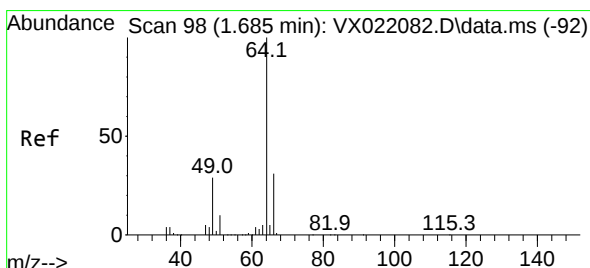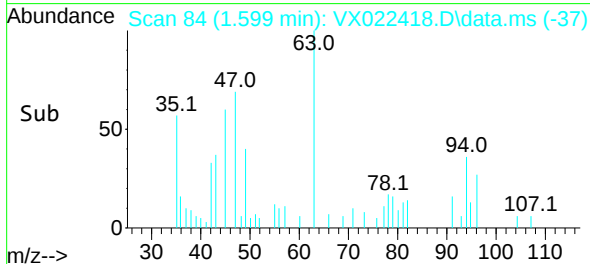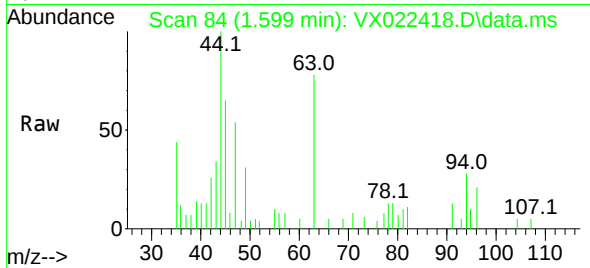

#6
Chloroethane
Concen: 0.213 ug/l
RT: 1.691 min Scan# 99
Delta R.T. 0.006 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion: 64 Resp: 111
Ion Ratio Lower Upper
64 100
66 5.5 25.4 38.0#


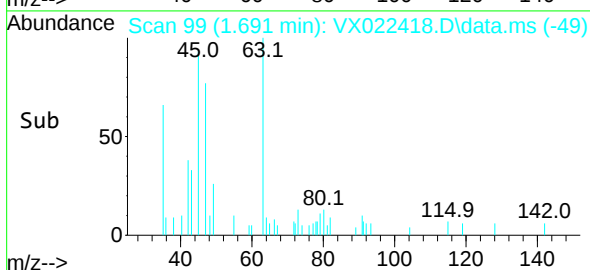

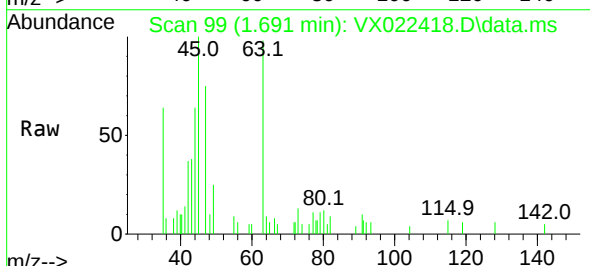




#10
Methyl Iodide
Concen: 1.105 ug/l
RT: 2.428 min Scan# 220
Delta R.T. -0.025 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:142 Resp: 888
Ion Ratio Lower Upper
142 100
127 41.7 33.3 49.9
141 5.1 11.4 17.0#

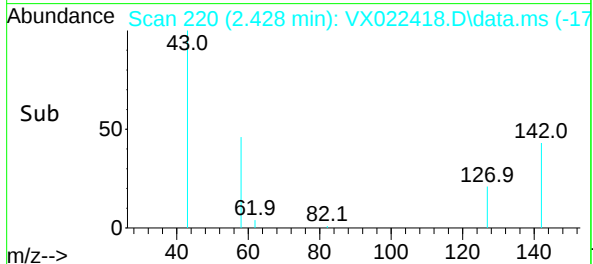

#11
Tert butyl alcohol
Concen: 9.753 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.036 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion: 59 Resp: 2171
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#




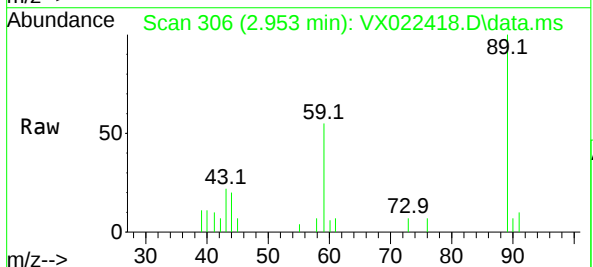




#13
Acrolein
Concen: 0.515 ug/l
RT: 2.252 min Scan# 191
Delta R.T. 0.012 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 56 Resp: 76
Ion Ratio Lower Upper
56 100
55 131.6 56.4 84.6#



#16
Acetone
Concen: 11.558 ug/l
RT: 2.434 min Scan# 221
Delta R.T. 0.042 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion: 43 Resp: 4898
Ion Ratio Lower Upper
43 100
58 32.0 27.8 41.8

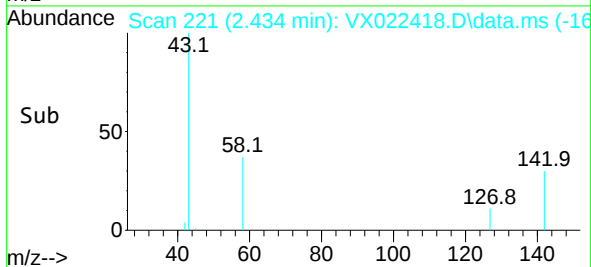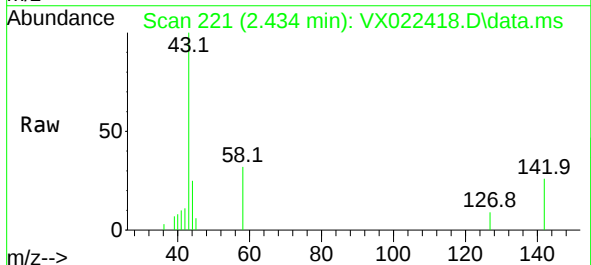

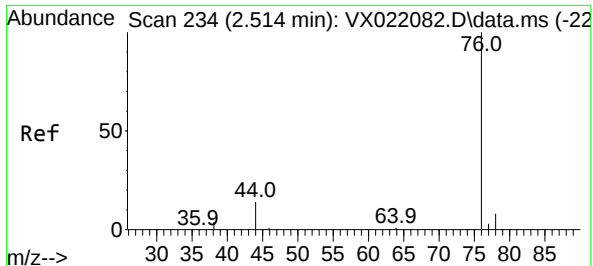

#17

Carbon Disulfide

Concen: 0.960 ug/l

RT: 2.471 min Scan# 227

Delta R.T. -0.043 min

Lab File: VX022418.D





Acq: 04 Jun 2021 17:24

Tgt Ion: 76 Resp: 1819

Ion Ratio Lower Upper

76 100

78 11.3 7.2 10.8#

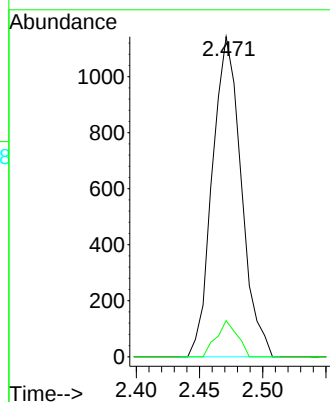

#18

Methyl Acetate

Concen: 0.245 ug/l

RT: 2.678 min Scan# 261

Delta R.T. -0.031 min

Lab File: VX022418.D




Acq: 04 Jun 2021 17:24


Tgt Ion: 43 Resp: 276

Ion Ratio Lower Upper

43 100

74 0.0 21.9 32.9#

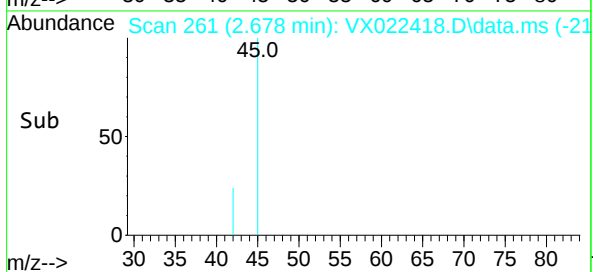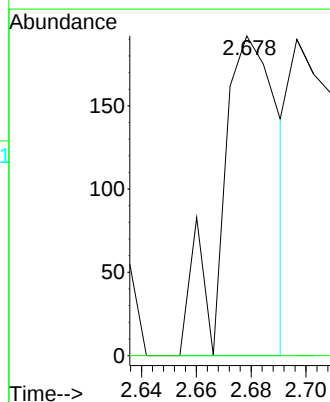



#20

Methylene Chloride

Concen: 0.905 ug/l

RT: 2.770 min Scan# 276

Delta R.T. -0.024 min

Lab File: VX022418.D

Acq: 04 Jun 2021 17:24

Tgt Ion: 84 Resp: 852





Ion Ratio Lower Upper

84 100

49 82.1 88.6 132.8#

51 46.4 27.0 40.6#

86 37.1 50.3 75.5#

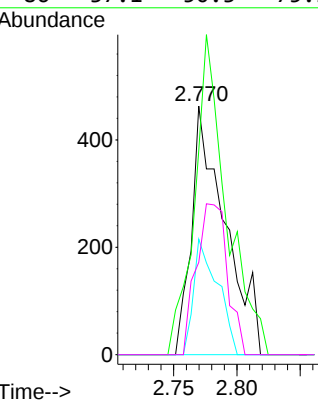

#25

2-Butanone

Concen: 0.429 ug/l

RT: 4.617 min Scan# 579

Delta R.T. 0.049 min

Lab File: VX022418.D




Acq: 04 Jun 2021 17:24


Tgt Ion: 43 Resp: 294

Ion Ratio Lower Upper

43 100

72 0.0 23.7 35.5#

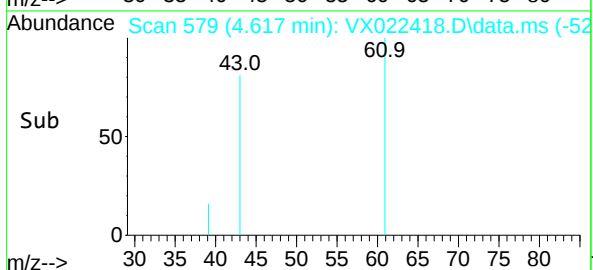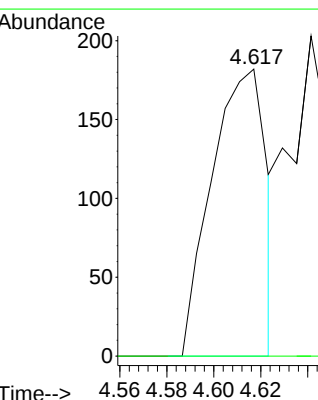



#29

Tetrahydrofuran

Concen: 1.796 ug/l

RT: 5.068 min Scan# 653





Delta R.T. 0.055 min

Lab File: VX022418.D

Acq: 04 Jun 2021 17:24

Tgt Ion:	42	Resp:	733
Ion	Ratio	Lower	Upper
42	100		
72	8.6	41.7	62.5#
71	42.6	38.4	57.6

Instrument :
MSVOA_X
ClientSampleId :



#31

Cyclohexane

Concen: 0.877 ug/l




RT: 5.495 min Scan# 723


Delta R.T. 0.012 min

Lab File: VX022418.D

Acq: 04 Jun 2021 17:24

Tgt Ion:	56	Resp:	1072
Ion	Ratio	Lower	Upper
56	100		
69	0.0	25.3	37.9#
84	6.2	71.4	107.0#

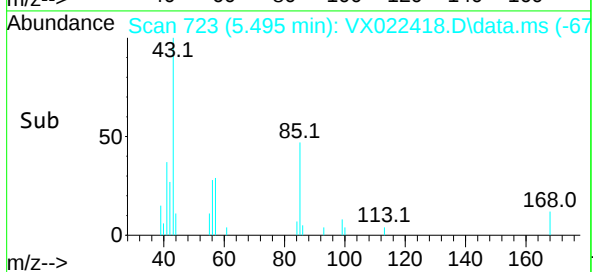







#33

1,2-Dichloroethane-d4
Concen: 52.046 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Instrument :
MSVOA_X
ClientSampled :




Tgt Ion: 65 Resp: 50654
Ion Ratio Lower Upper
65 100
67 52.7 0.0 105.4

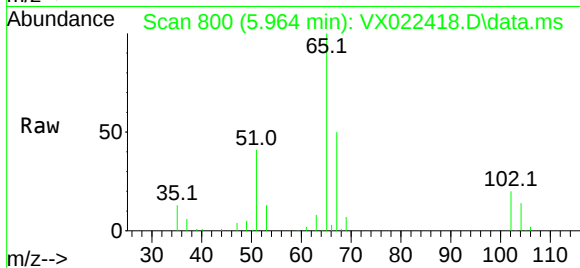


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. -0.006 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion: 114 Resp: 129485
Ion Ratio Lower Upper
114 100
63 22.4 0.0 40.8
88 16.3 0.0 32.8

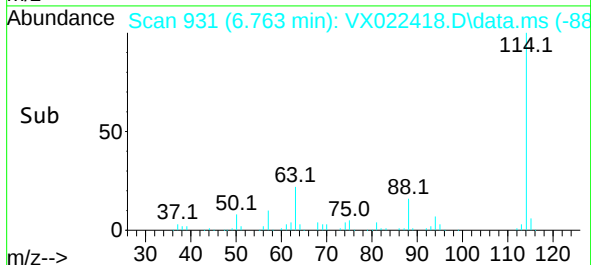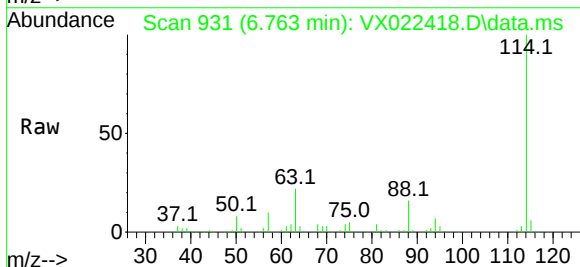



#35

Dibromofluoromethane

Concen: 45.659 ug/l

RT: 5.397 min Scan# 707

Delta R.T. 0.006 min

Lab File: VX022418.D

Acq: 04 Jun 2021 17:24





Tgt Ion:113 Resp: 37492

Ion Ratio Lower Upper

113 100

111 102.8 81.9 122.9

192 15.6 16.7 25.1#

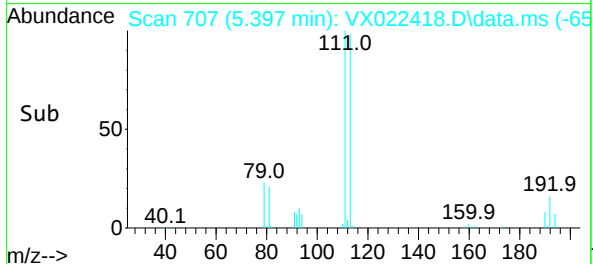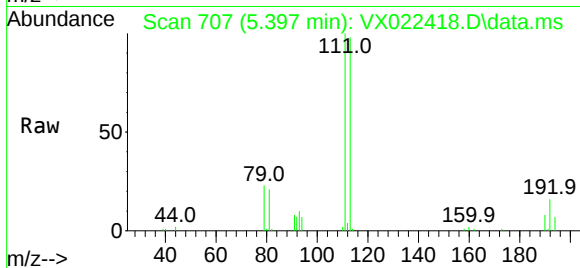

#36

1,1-Dichloropropene

Concen: 5.027 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.152 min

Lab File: VX022418.D

Acq: 04 Jun 2021 17:24




Tgt Ion: 75 Resp: 6019


Ion Ratio Lower Upper

75 100

110 6.7 18.1 54.4#


77 0.0 25.3 37.9#

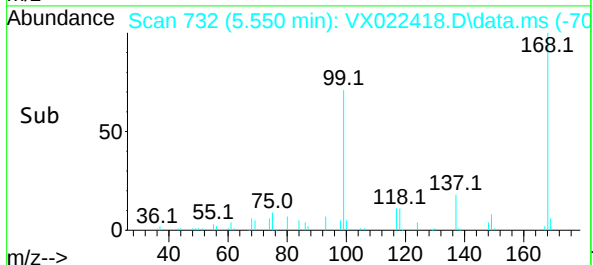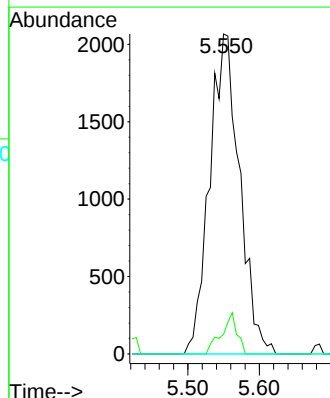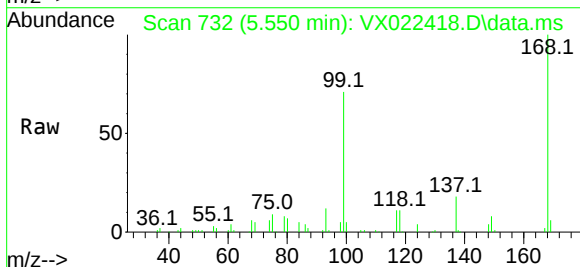






#38
Carbon Tetrachloride
Concen: 6.362 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.146 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Instrument :
MSVOA_X
ClientSampled :



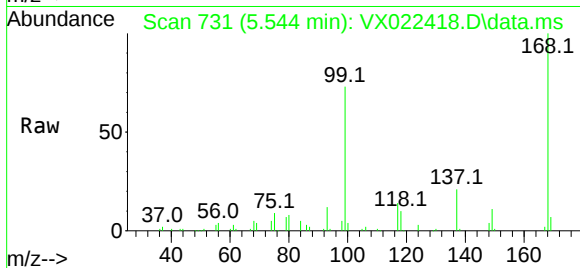



Tgt Ion:117 Resp: 7451
Ion Ratio Lower Upper
117 100
119 3.4 76.2 114.2#
121 0.0 24.8 37.2#



#39
Methylcyclohexane
Concen: 0.356 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion: 83 Resp: 483
Ion Ratio Lower Upper
83 100
55 122.2 58.9 88.3#
98 28.4 38.1 57.1#


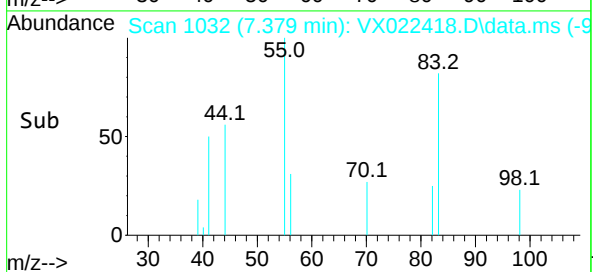

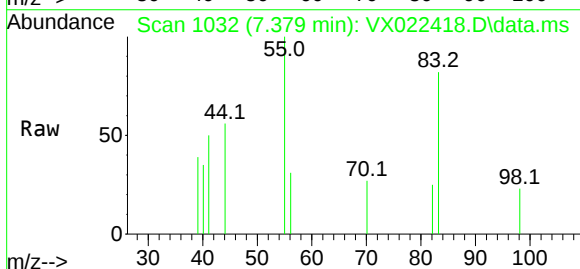




#50
Toluene-d8
Concen: 50.402 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 98 Resp: 159426
Ion Ratio Lower Upper
98 100
100 64.3 51.9 77.9



#51
4-Methyl-2-Pentanone
Concen: 1.034 ug/l
RT: 8.598 min Scan# 1232
Delta R.T. 0.018 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion: 43 Resp: 1487
Ion Ratio Lower Upper
43 100
58 14.1 35.4 53.0#


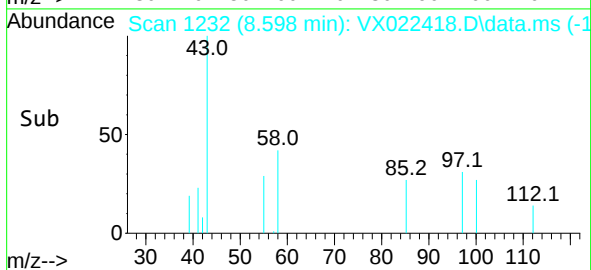

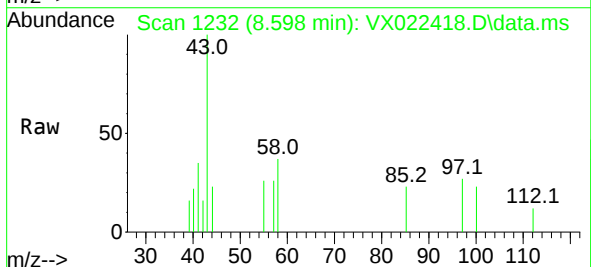




#52
Toluene
Concen: 4.288 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.006 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 92 Resp: 10003
Ion Ratio Lower Upper
92 100
91 166.0 137.1 205.7

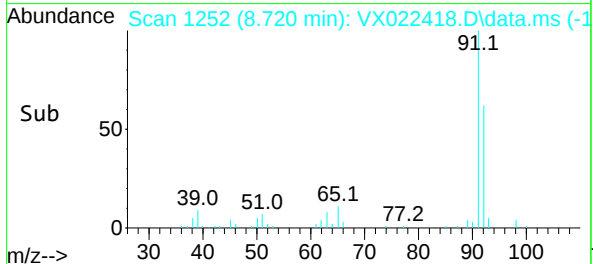

#59
2-Hexanone
Concen: 0.390 ug/l
RT: 9.439 min Scan# 1370
Delta R.T. 0.006 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion: 43 Resp: 422
Ion Ratio Lower Upper
43 100
58 32.7 30.9 92.8


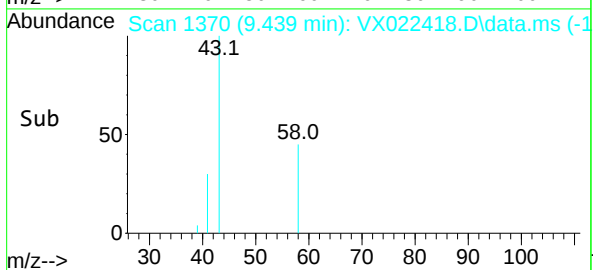

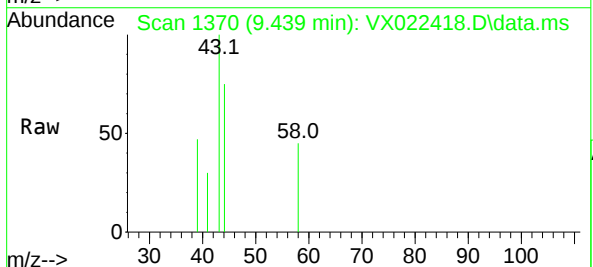




#62
4-Bromofluorobenzene
Concen: 49.172 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 57489
Ion Ratio Lower Upper
95 100
174 65.0 0.0 154.6
176 60.5 0.0 155.8

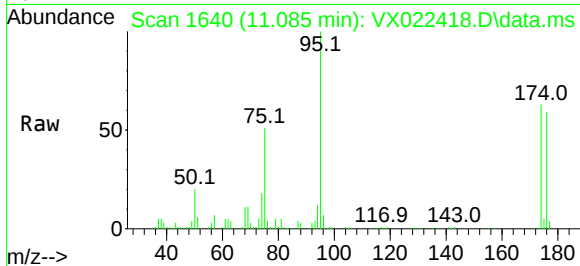

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion: 117 Resp: 114309
Ion Ratio Lower Upper
117 100
82 58.5 47.4 71.2
119 31.4 26.6 39.8


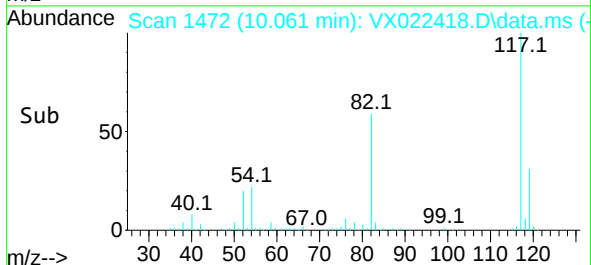

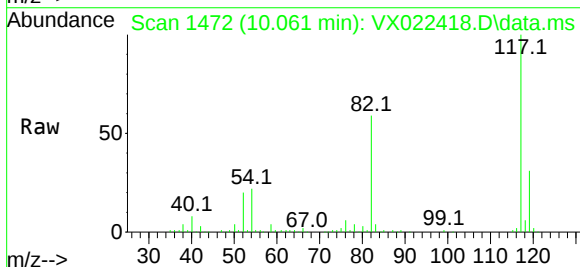




#67
Ethyl Benzene
Concen: 0.647 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 2833
Ion Ratio Lower Upper
91 100
106 28.1 24.6 37.0

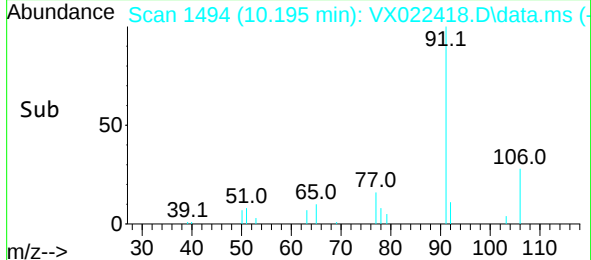

#68
m/p-Xylenes
Concen: 3.027 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion: 106 Resp: 5007
Ion Ratio Lower Upper
106 100
91 213.1 162.8 244.2


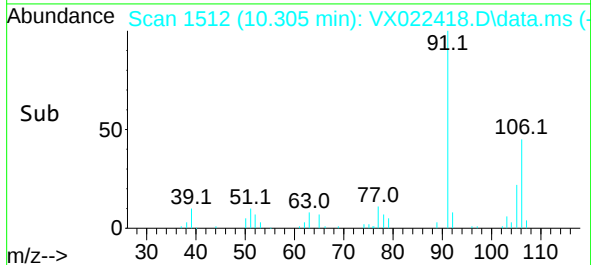

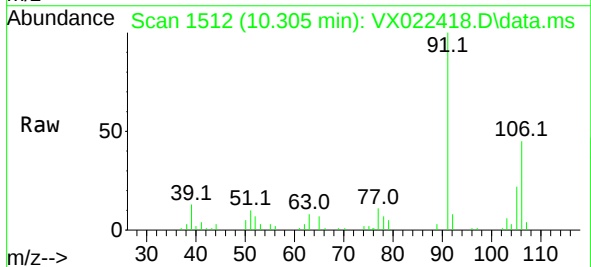




#69
o-Xylene
Concen: 1.313 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.001 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 2112
Ion Ratio Lower Upper
106 100
91 262.0 108.1 324.2

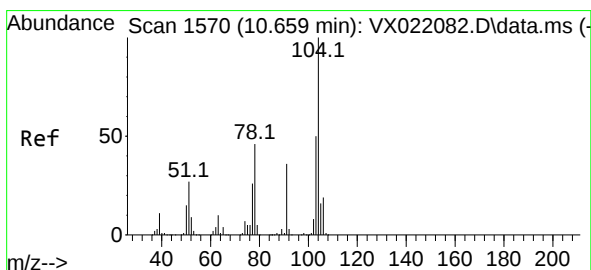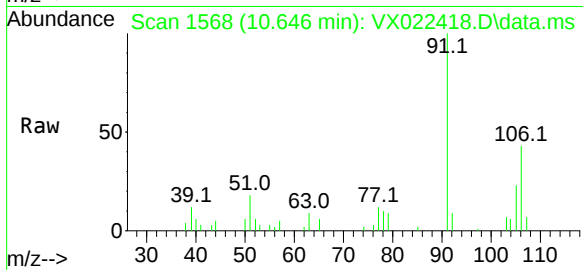

#70
Styrene
Concen: 0.444 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. -0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion:104 Resp: 1170
Ion Ratio Lower Upper
104 100
78 77.8 40.0 60.0#
103 66.5 43.4 65.0#


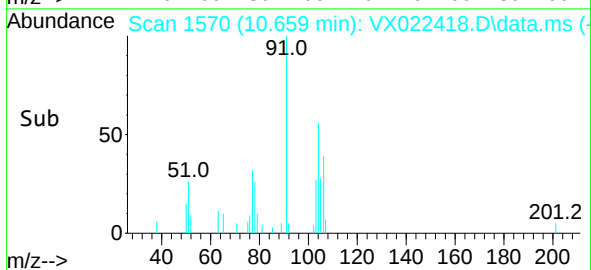

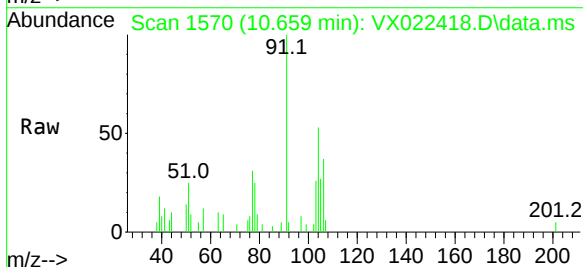




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:152 Resp: 50382
Ion Ratio Lower Upper
152 100
115 66.5 41.1 123.3
150 158.6 0.0 349.0

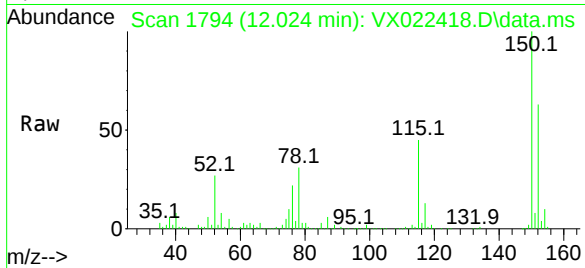

#73
Isopropylbenzene
Concen: 0.250 ug/l
RT: 10.970 min Scan# 1621
Delta R.T. 0.006 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24


Tgt Ion:105 Resp: 1067
Ion Ratio Lower Upper
105 100
120 10.4 13.2 39.6#

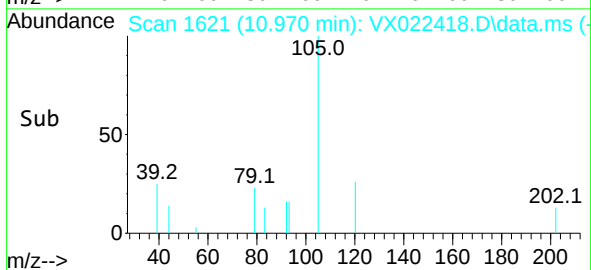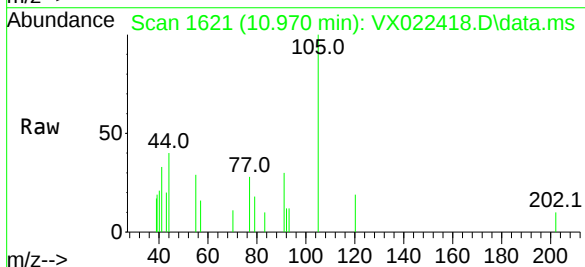






#74
N-amy1 acetate
Concen: 0.258 ug/l
RT: 10.860 min Scan# 1603
Delta R.T. 0.012 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Instrument :
MSVOA_X
ClientSampled :



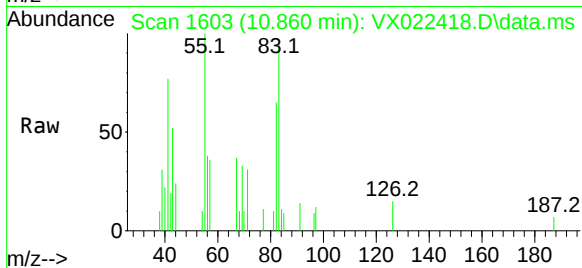



Tgt Ion: 43 Resp: 522
Ion Ratio Lower Upper
43 100
70 35.1 39.0 58.6#
55 265.1 21.5 32.3#
61 0.0 22.1 33.1#



#75
1,1,2,2-Tetrachloroethane
Concen: 0.243 ug/l
RT: 11.220 min Scan# 1662
Delta R.T. 0.005 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion: 83 Resp: 343
Ion Ratio Lower Upper
83 100
131 0.0 5.1 15.2#
85 0.0 31.8 95.4#




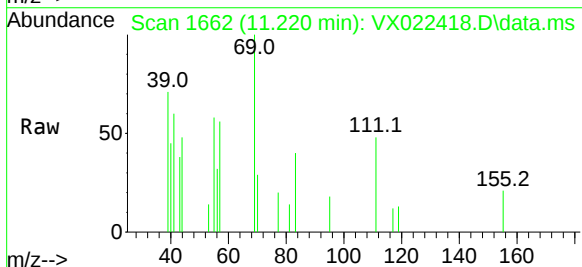




#76
1,2,3-Trichloropropane
Concen: 24.428 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 75 Resp: 30362
Ion Ratio Lower Upper
75 100
77 1.6 19.1 57.5#

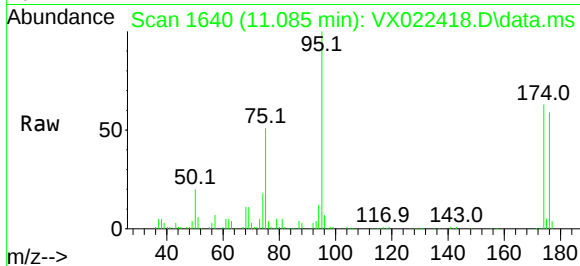

#78
n-propylbenzene
Concen: 0.236 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion: 91 Resp: 1181
Ion Ratio Lower Upper
91 100
120 23.1 11.5 34.5


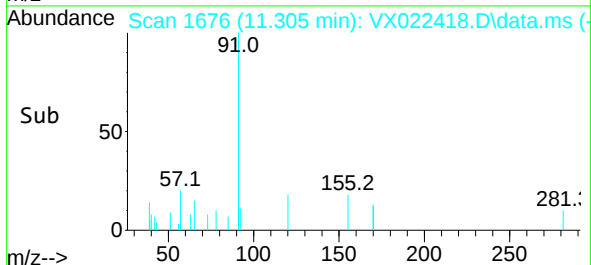

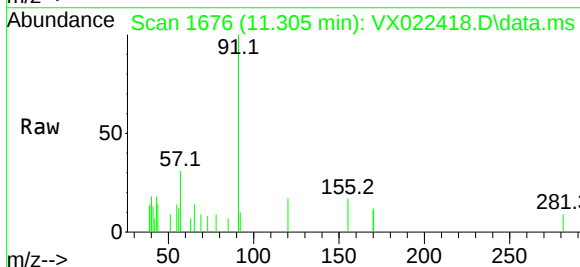




#79
2-Chlorotoluene
Concen: 0.207 ug/l
RT: 11.372 min Scan# 1687
Delta R.T. 0.006 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 627
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#

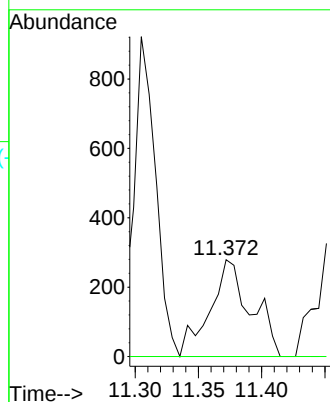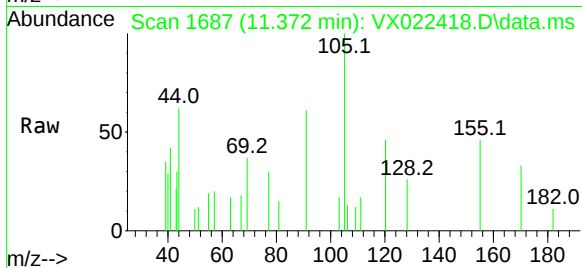

#80
1,3,5-Trimethylbenzene
Concen: 0.754 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion: 105 Resp: 2663
Ion Ratio Lower Upper
105 100
120 47.1 23.8 71.5


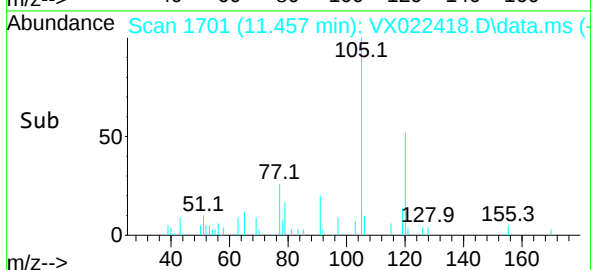

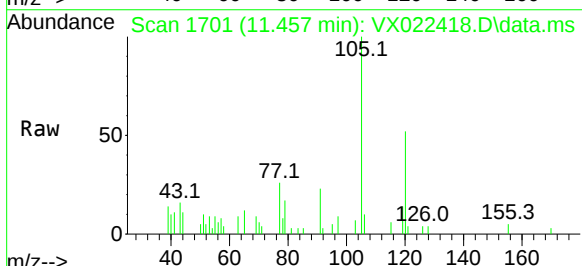




#81
trans-1,4-Dichloro-2-butene
Concen: 57.878 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.060 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 75 Resp: 30362
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.1 37.9 56.9#

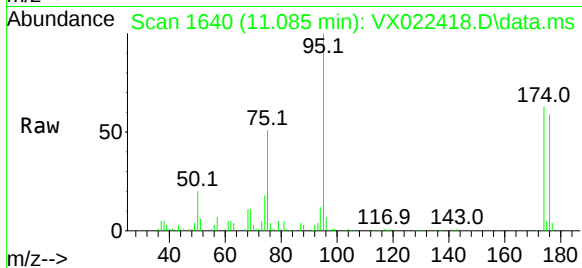

#82
4-Chlorotoluene
Concen: 0.232 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion: 91 Resp: 809
Ion Ratio Lower Upper
91 100
126 6.7 14.9 44.5#


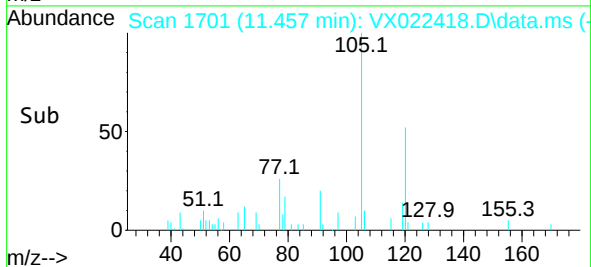

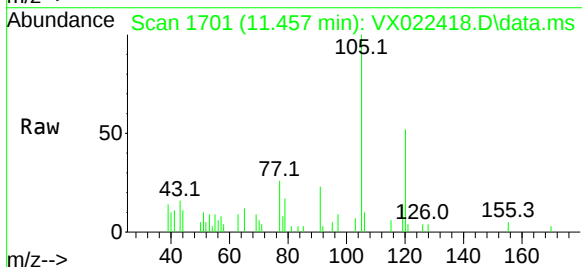




#84
1,2,4-Trimethylbenzene
Concen: 1.578 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:105 Resp: 5613
Ion Ratio Lower Upper
105 100
120 43.2 22.4 67.3

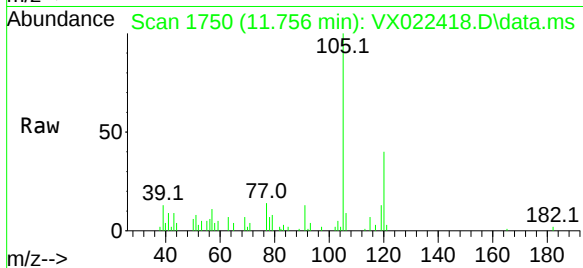

#85
sec-Butylbenzene
Concen: 0.220 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. -0.006 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion:105 Resp: 949
Ion Ratio Lower Upper
105 100
134 28.1 10.0 29.8


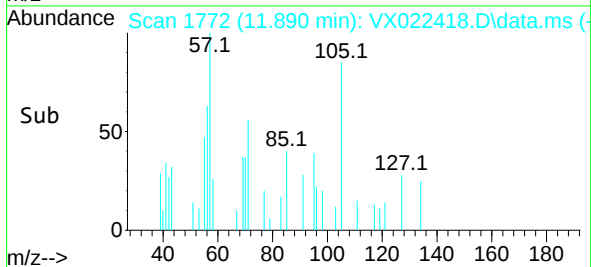

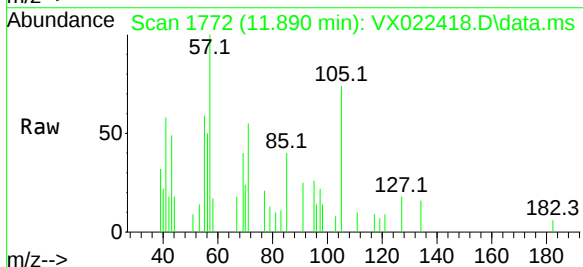




#86
p-Isopropyltoluene
Concen: 1.057 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. 0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:119 Resp: 3845
Ion Ratio Lower Upper
119 100
134 29.0 12.9 38.7
91 39.7 11.7 35.0#

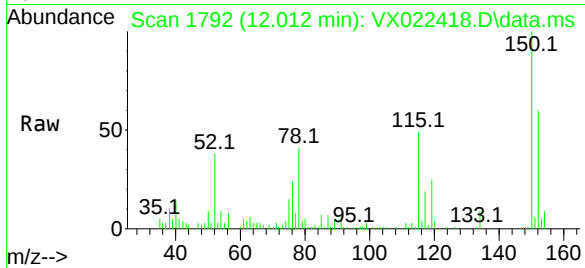

#89
n-Butylbenzene
Concen: 0.424 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24


Tgt Ion: 91 Resp: 1428
Ion Ratio Lower Upper
91 100
92 33.6 27.4 82.0
134 55.4 13.2 39.5#

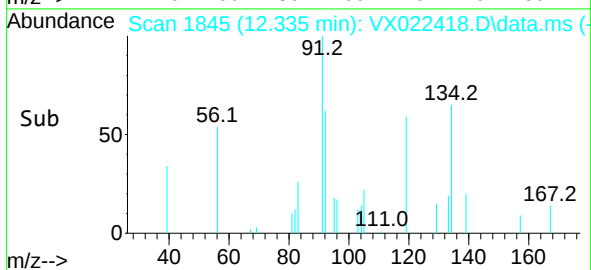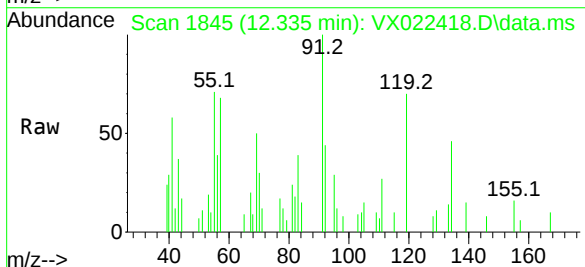






#90
Hexachloroethane
Concen: 0.910 ug/l
RT: 12.530 min Scan# 1877
Delta R.T. -0.013 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Instrument :
MSVOA_X
ClientSampleId :



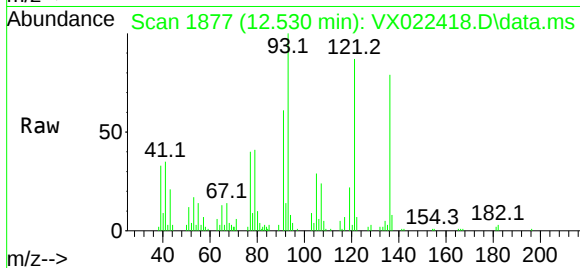



Tgt Ion:117 Resp: 547
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#



#93
1,2,4-Trichlorobenzene
Concen: 0.326 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24

Tgt Ion:180 Resp: 329
Ion Ratio Lower Upper
180 100
182 92.1 47.7 143.1
145 178.4 15.0 45.0#




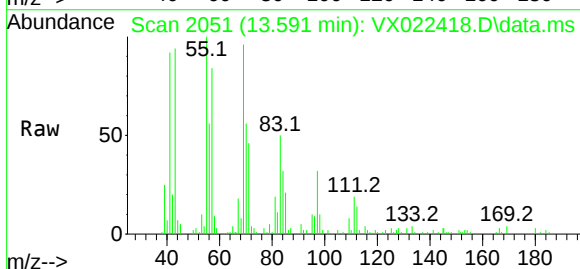




#94
Hexachlorobutadiene
Concen: 0.773 ug/l
RT: 13.731 min Scan# 2074
Delta R.T. 0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:	225	Resp:	305
Ion	Ratio	Lower	Upper
225	100		
223	34.8	31.1	93.2
227	36.7	31.6	95.0

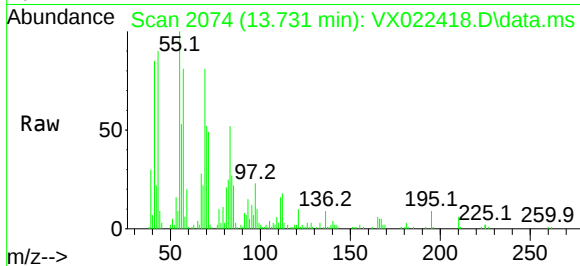

#95
Naphthalene
Concen: 0.491 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX022418.D
Acq: 04 Jun 2021 17:24


Tgt Ion:	128	Resp:	1933
Ion	Ratio	Lower	Upper
128	100		
127	13.6	10.3	15.5
129	33.7	8.8	13.2#

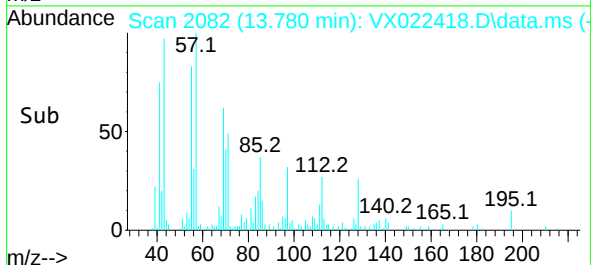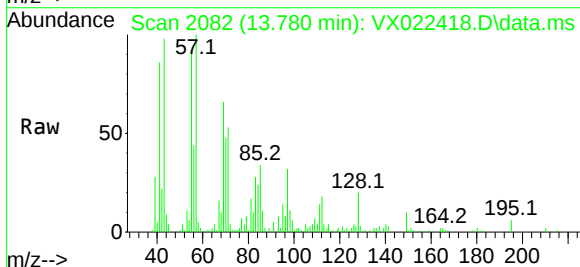

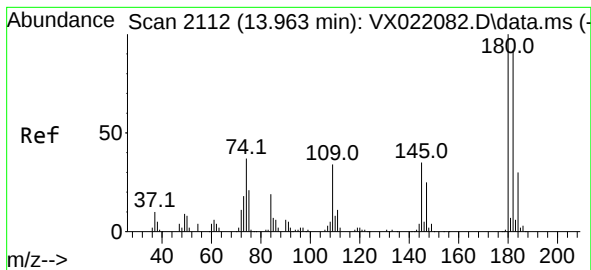

#96
 1,2,3-Trichlorobenzene
 Concen: 0.289 ug/l
 RT: 13.975 min Scan# 2114
 Delta R.T. 0.012 min
 Lab File: VX022418.D
 Acq: 04 Jun 2021 17:24

Instrument :
 MSVOA_X
 ClientSampleId :

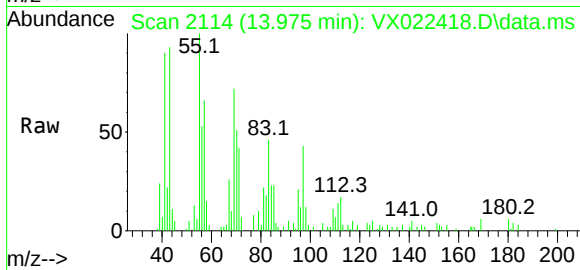

Tgt Ion:180 Resp: 294
 Ion Ratio Lower Upper
 180 100
 182 115.6 47.6 142.9
 145 76.2 16.1 48.3#

