

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060421\
 Data File : VX022425.D
 Acq On : 04 Jun 2021 20:09
 Operator : JC/MD
 Sample : M2580-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jun 05 03:23:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	68154	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	141677	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	126035	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	50339	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	56097	53.359	ug/l	0.00
Spiked Amount 50.000	Range	78 - 117	Recovery	=	106.720%	
35) Dibromofluoromethane	5.397	113	41134	45.783	ug/l	0.00
Spiked Amount 50.000	Range	75 - 124	Recovery	=	91.560%	
50) Toluene-d8	8.653	98	173084	50.011	ug/l	0.00
Spiked Amount 50.000	Range	92 - 112	Recovery	=	100.020%	
62) 4-Bromofluorobenzene	11.085	95	60579	47.356	ug/l	0.00
Spiked Amount 50.000	Range	83 - 123	Recovery	=	94.720%	
Target Compounds						
					Qvalue	
5) Bromomethane	1.630	94	162	0.294	ug/l #	44
11) Tert butyl alcohol	2.983	59	299	1.243	ug/l #	73
13) Acrolein	2.245	56	400	2.508	ug/l #	33
16) Acetone	2.386	43	20909	45.675	ug/l	89
17) Carbon Disulfide	2.514	76	2262	1.106	ug/l #	87
18) Methyl Acetate	2.715	43	709	0.582	ug/l #	72
20) Methylene Chloride	2.794	84	3418	3.363	ug/l #	69
25) 2-Butanone	4.574	43	5635	7.609	ug/l #	70
29) Tetrahydrofuran	5.037	42	311	0.706	ug/l #	39
31) Cyclohexane	5.556	56	1978	1.497	ug/l #	1
36) 1,1-Dichloropropene	5.568	75	6213	4.742	ug/l #	48
37) Ethyl Acetate	4.574	43	5635	3.509	ug/l #	64
38) Carbon Tetrachloride	5.562	117	7484	5.840	ug/l #	17
40) Benzene	6.043	78	1579	0.392	ug/l	100
43) Isopropyl Acetate	6.348	43	11704	4.456	ug/l #	91
48) Methyl methacrylate	7.604	41	3508	2.898	ug/l #	10
51) 4-Methyl-2-Pentanone	8.555	43	40109	25.490	ug/l #	46
52) Toluene	8.726	92	8107	3.176	ug/l	93
54) cis-1,3-Dichloropropene	8.555	75	18147	10.475	ug/l #	61
55) 1,1,2-Trichloroethane	9.104	97	257	0.248	ug/l #	15
57) 1,3-Dichloropropane	9.488	76	9520	5.381	ug/l #	42
59) 2-Hexanone	9.488	43	131354	110.994	ug/l #	44
67) Ethyl Benzene	10.195	91	27445	5.686	ug/l	98
68) m/p-Xylenes	10.305	106	30031	16.464	ug/l	98
69) o-Xylene	10.646	106	8569	4.830	ug/l	84
70) Styrene	10.646	104	684	0.235	ug/l #	1
73) Isopropylbenzene	10.963	105	3877	0.910	ug/l	94
74) N-amyl acetate	10.896	43	602	0.298	ug/l #	45
76) 1,2,3-Trichloropropane	11.085	75	31888	25.677	ug/l #	39
78) n-propylbenzene	11.305	91	2706	0.542	ug/l	99
79) 2-Chlorotoluene	11.384	91	1834	0.606	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.457	105	7344	2.080	ug/l	96
81) trans-1,4-Dichloro-2-b...	11.085	75	31888	60.839	ug/l #	12
82) 4-Chlorotoluene	11.457	91	1055	0.303	ug/l #	45
83) tert-Butylbenzene	11.975	119	1583	0.467	ug/l	81
84) 1,2,4-Trimethylbenzene	11.756	105	19699	5.542	ug/l	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060421\
 Data File : VX022425.D
 Acq On : 04 Jun 2021 20:09
 Operator : JC/MD
 Sample : M2580-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jun 05 03:23:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
86) p-Isopropyltoluene	12.012	119	4413	1.214	ug/l	87
88) 1,4-Dichlorobenzene	12.042	146	770	0.428	ug/l #	1
89) n-Butylbenzene	12.329	91	1121	0.333	ug/l #	31
90) Hexachloroethane	12.652	117	498	0.829	ug/l #	9
91) 1,2-Dichlorobenzene	12.335	146	625	0.374	ug/l	86
92) 1,2-Dibromo-3-Chloropr...	12.963	75	186	0.616	ug/l #	1
95) Naphthalene	13.780	128	838917	213.087	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060421\
 Data File : VX022425.D
 Acq On : 04 Jun 2021 20:09
 Operator : JC/MD
 Sample : M2580-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jun 05 03:23:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration




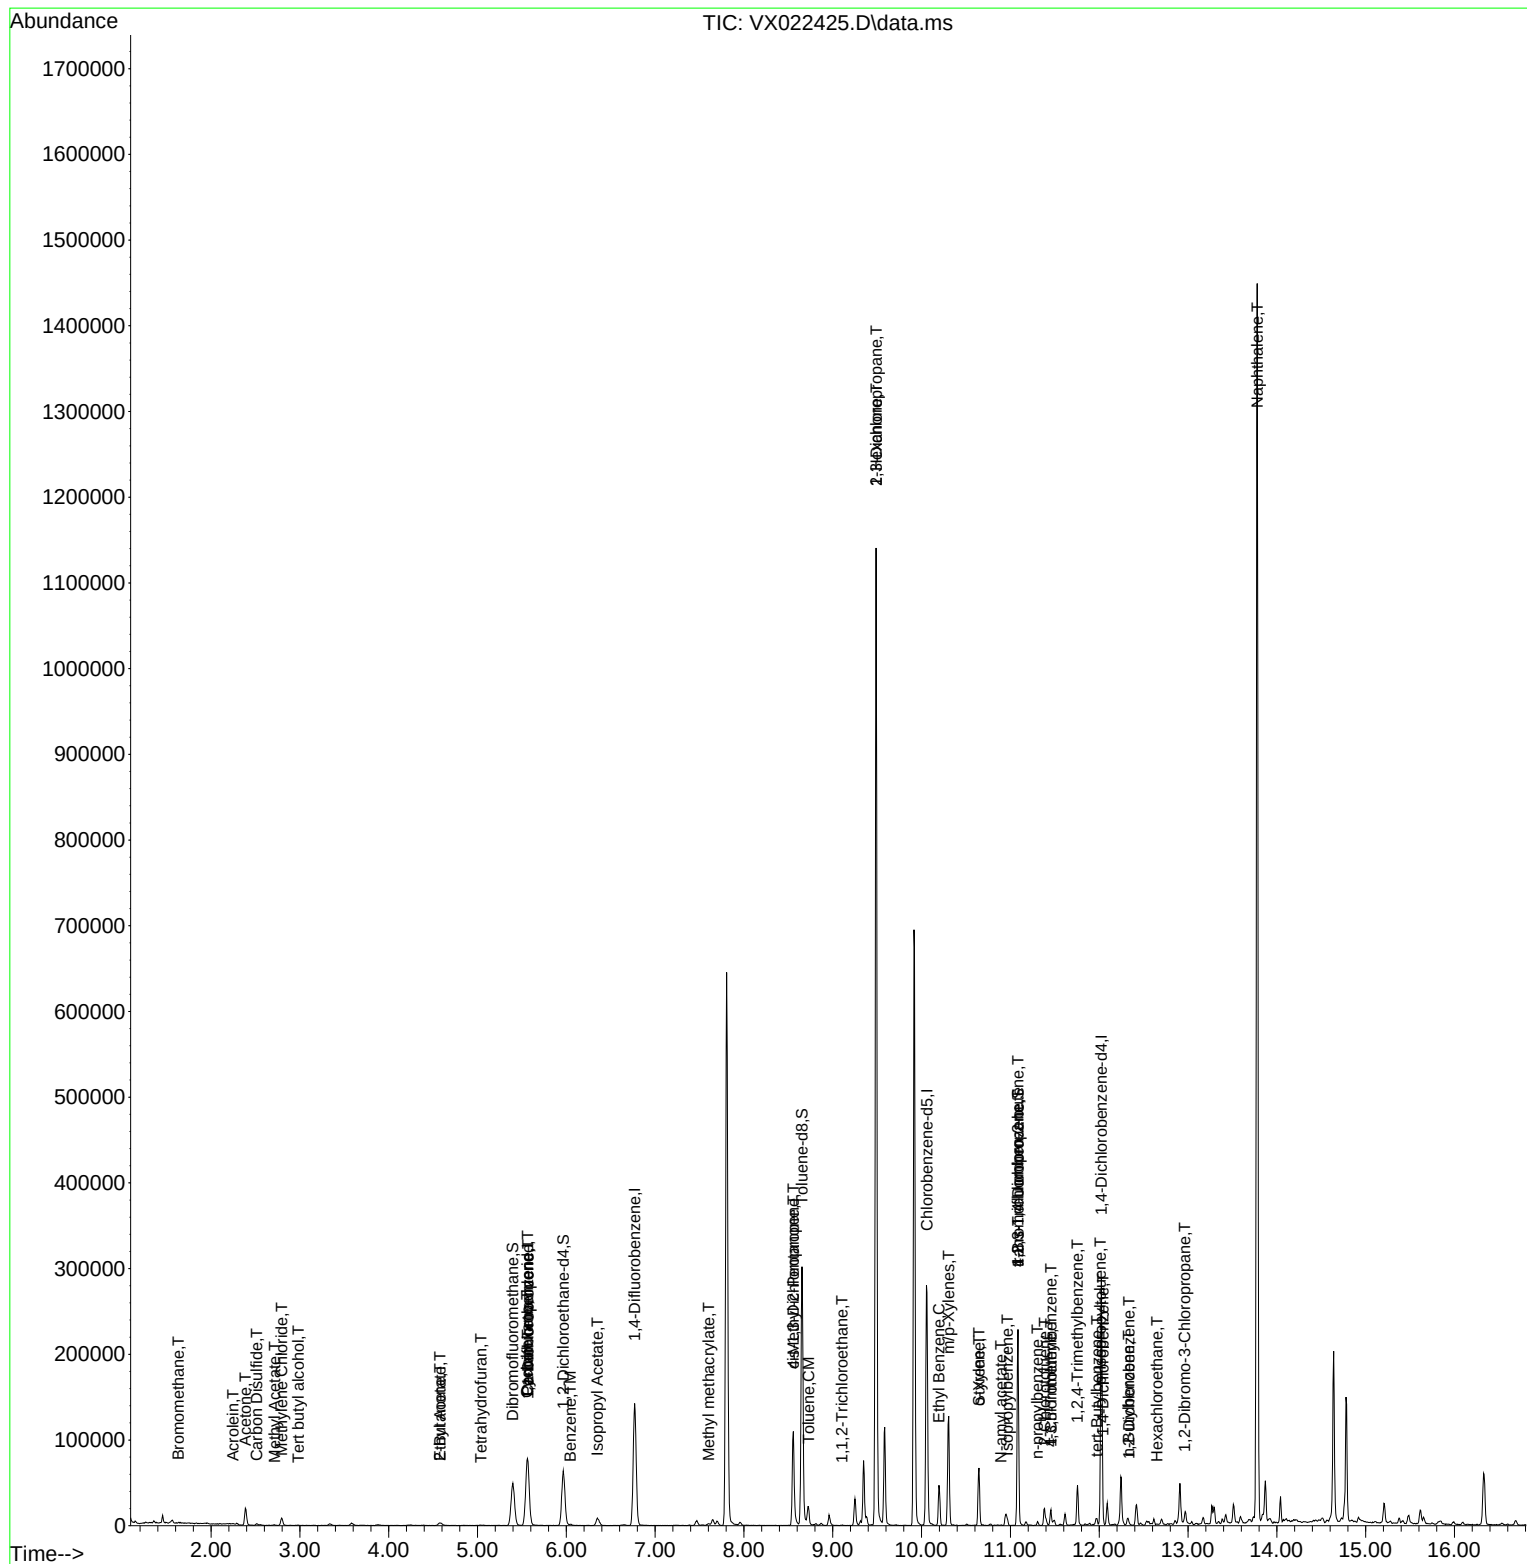




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 68154
Ion Ratio Lower Upper
168 100
99 66.2 45.8 68.6

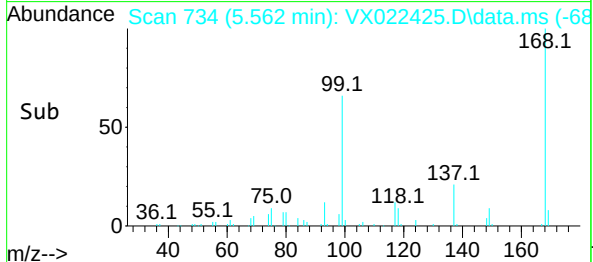

#5
Bromomethane
Concen: 0.294 ug/l
RT: 1.630 min Scan# 89
Delta R.T. 0.018 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion: 94 Resp: 162
Ion Ratio Lower Upper
94 100
96 40.9 76.4 114.6#

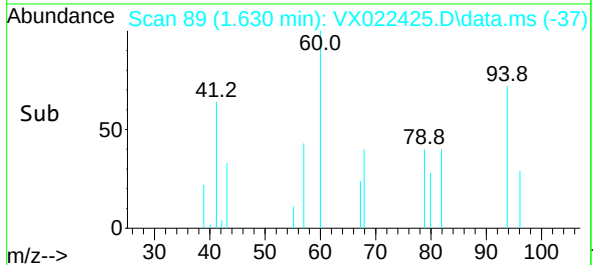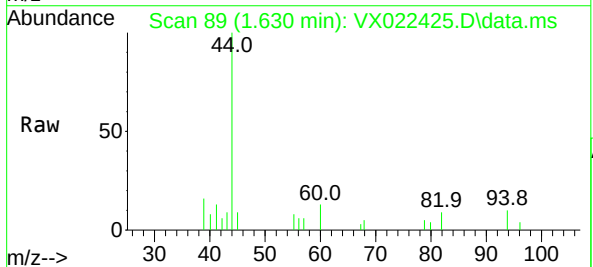







#11

Tert butyl alcohol
Concen: 1.243 ug/l
RT: 2.983 min Scan# 311
Delta R.T. -0.006 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Instrument :
MSVOA_X
ClientSampled :




Tgt Ion: 59 Resp: 299
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

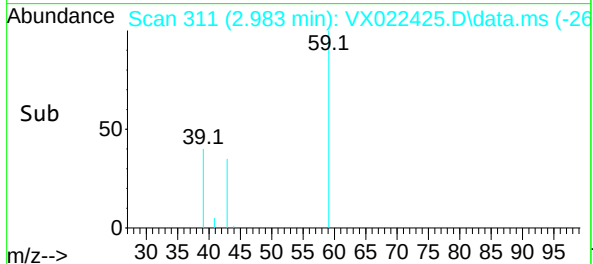


#13

Acrolein
Concen: 2.508 ug/l
RT: 2.245 min Scan# 190
Delta R.T. 0.005 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion: 56 Resp: 400
Ion Ratio Lower Upper
56 100
55 125.8 56.4 84.6#


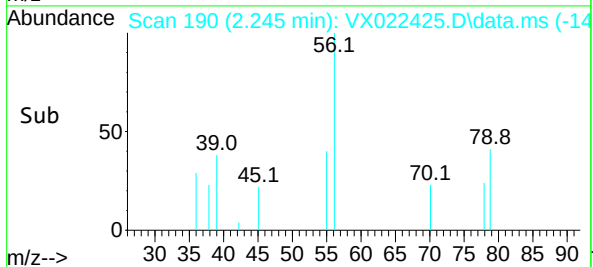

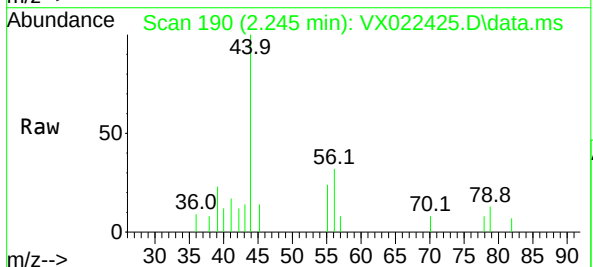




#16
Acetone
Concen: 45.675 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 20909
Ion Ratio Lower Upper
43 100
58 28.4 27.8 41.8

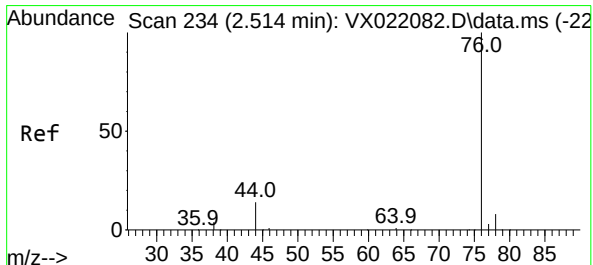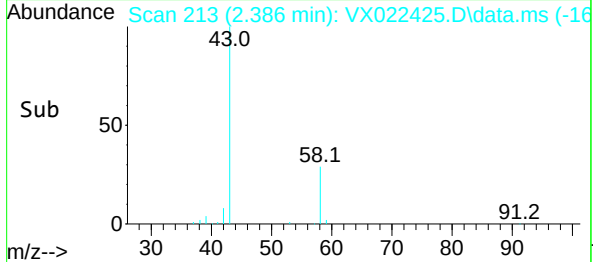

#17
Carbon Disulfide
Concen: 1.106 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion: 76 Resp: 2262
Ion Ratio Lower Upper
76 100
78 4.3 7.2 10.8#


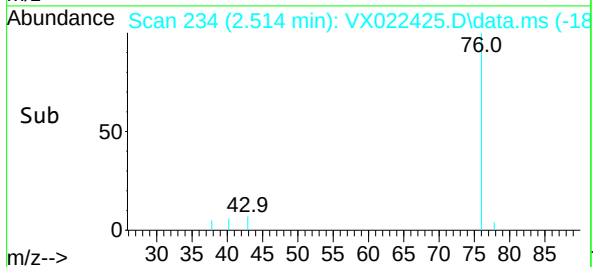

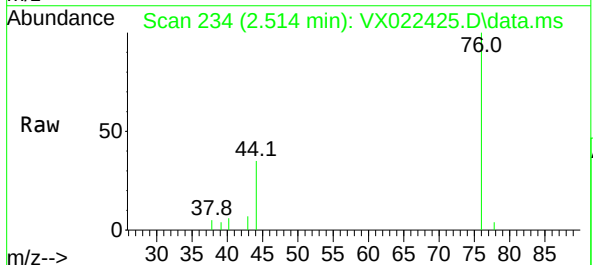




#18
Methyl Acetate
Concen: 0.582 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.006 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 709
Ion Ratio Lower Upper
43 100
74 12.6 21.9 32.9#

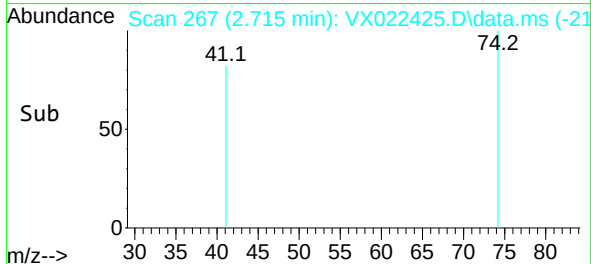

#20
Methylene Chloride
Concen: 3.363 ug/l
RT: 2.794 min Scan# 280
Delta R.T. -0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion: 84 Resp: 3418
Ion Ratio Lower Upper
84 100
49 153.3 88.6 132.8#
51 44.5 27.0 40.6#
86 80.2 50.3 75.5#




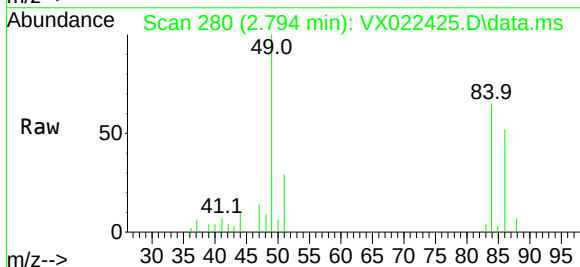




#25
2-Butanone
Concen: 7.609 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.006 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 5635
Ion Ratio Lower Upper
43 100
72 13.2 23.7 35.5#

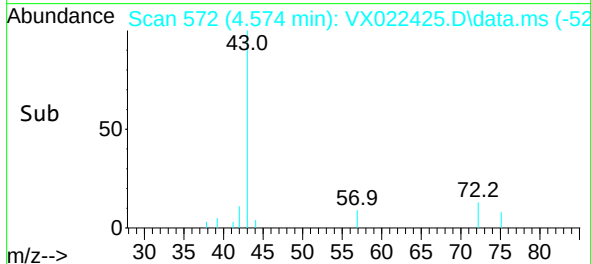

#29
Tetrahydrofuran
Concen: 0.706 ug/l
RT: 5.037 min Scan# 648
Delta R.T. 0.024 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09


Tgt Ion: 42 Resp: 311
Ion Ratio Lower Upper
42 100
72 0.0 41.7 62.5#
71 15.8 38.4 57.6#

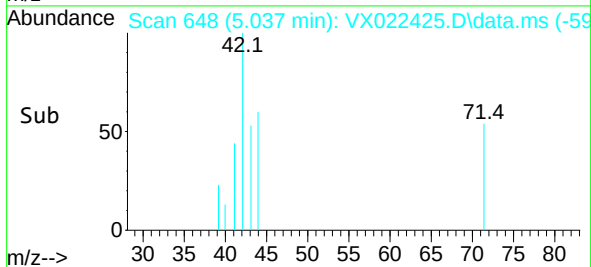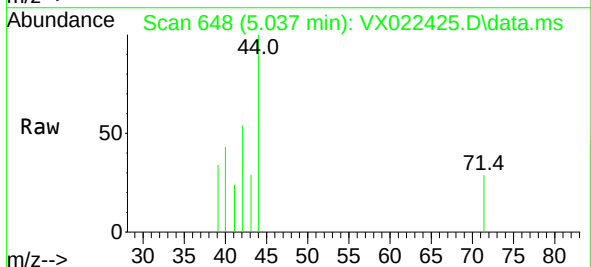






#31
Cyclohexane
Concen: 1.497 ug/l
RT: 5.556 min Scan# 733
Delta R.T. 0.073 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Instrument :
MSVOA_X
ClientSampled :







Tgt Ion: 56 Resp: 1978
Ion Ratio Lower Upper
56 100
69 190.1 25.3 37.9#
84 137.6 71.4 107.0#



#33
1,2-Dichloroethane-d4
Concen: 53.359 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion: 65 Resp: 56097
Ion Ratio Lower Upper
65 100
67 52.6 0.0 105.4


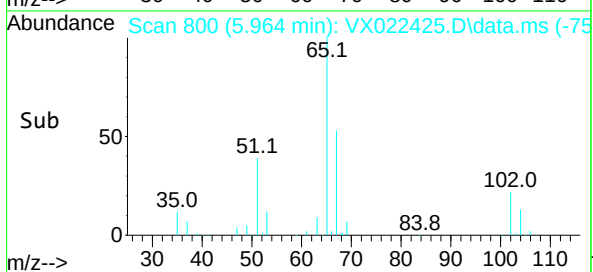






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:114 Resp: 141677
Ion Ratio Lower Upper
114 100
63 20.2 0.0 40.8
88 17.9 0.0 32.8

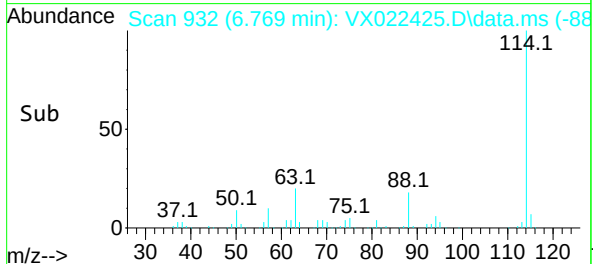

#35
Dibromofluoromethane
Concen: 45.783 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.006 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09


Tgt Ion:113 Resp: 41134
Ion Ratio Lower Upper
113 100
111 104.5 81.9 122.9
192 16.2 16.7 25.1#

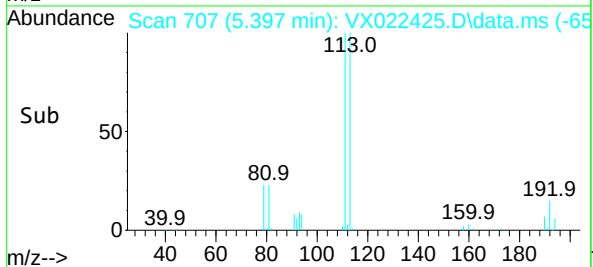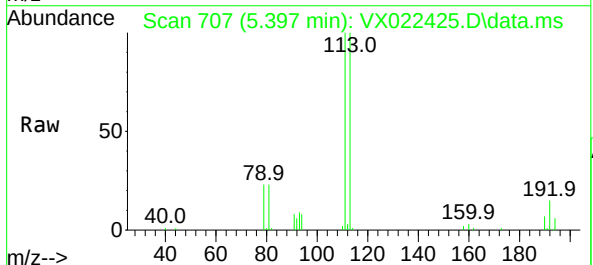






#36
1,1-Dichloropropene
Concen: 4.742 ug/l
RT: 5.568 min Scan# 735
Delta R.T. -0.134 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion: 75 Resp: 6213
Ion Ratio Lower Upper
75 100
110 8.2 18.1 54.4#
77 0.0 25.3 37.9#




#37
Ethyl Acetate
Concen: 3.509 ug/l
RT: 4.574 min Scan# 572
Delta R.T. -0.147 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

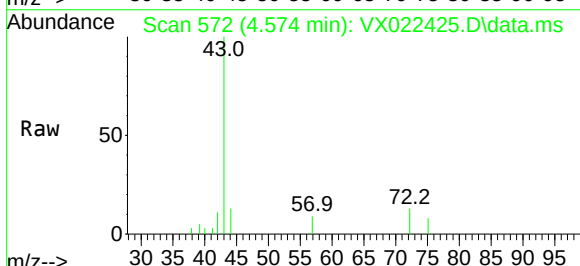


Tgt Ion: 43 Resp: 5635
Ion Ratio Lower Upper
43 100
61 0.0 12.8 19.2#
70 0.0 10.5 15.7#








#38
Carbon Tetrachloride
Concen: 5.840 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.128 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 7484
Ion Ratio Lower Upper
117 100
119 5.7 76.2 114.2#
121 0.0 24.8 37.2#



#40
Benzene
Concen: 0.392 ug/l
RT: 6.043 min Scan# 813
Delta R.T. -0.001 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion: 78 Resp: 1579
Ion Ratio Lower Upper
78 100
77 23.8 18.9 28.3




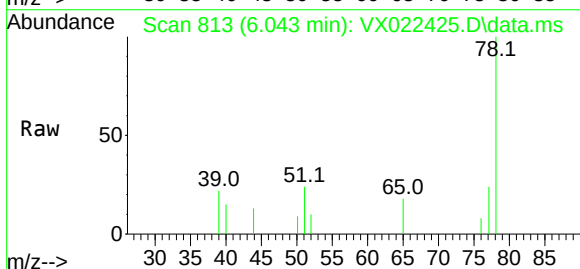




#43
Isopropyl Acetate
Concen: 4.456 ug/l
RT: 6.348 min Scan# 863
Delta R.T. -0.001 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 11704
Ion Ratio Lower Upper
43 100
61 19.5 18.2 27.4
87 10.7 12.5 18.7#

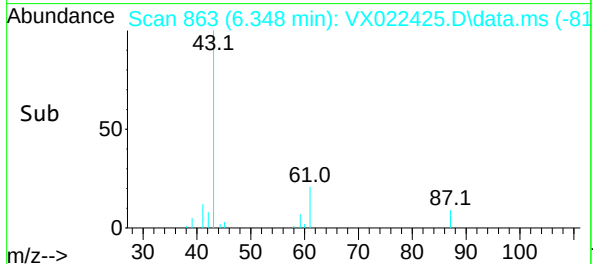

#48
Methyl methacrylate
Concen: 2.898 ug/l
RT: 7.604 min Scan# 1069
Delta R.T. -0.092 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion: 41 Resp: 3508
Ion Ratio Lower Upper
41 100
69 0.0 76.0 114.0#
39 0.0 44.6 67.0#


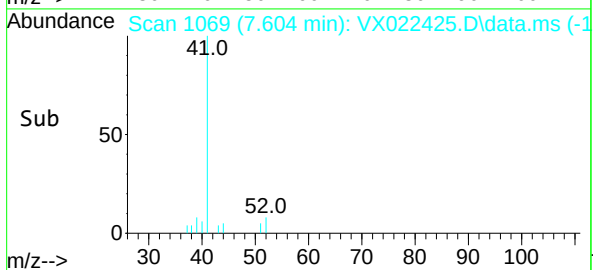

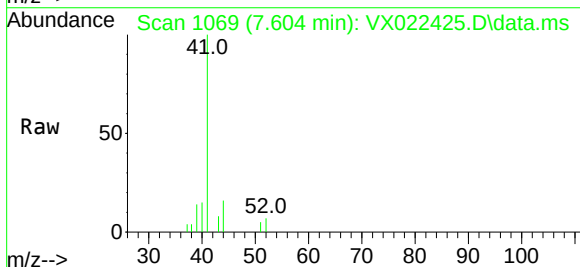




#50
Toluene-d8
Concen: 50.011 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 98 Resp: 173084
Ion Ratio Lower Upper
98 100
100 66.4 51.9 77.9

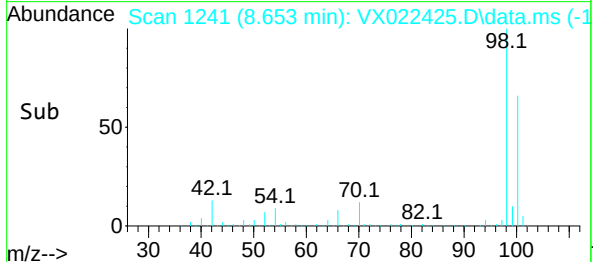

#51
4-Methyl-2-Pentanone
Concen: 25.490 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. -0.025 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion: 43 Resp: 40109
Ion Ratio Lower Upper
43 100
58 9.1 35.4 53.0#


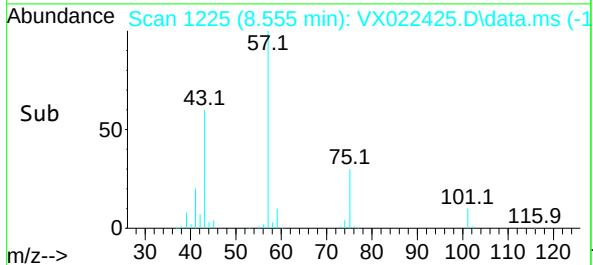

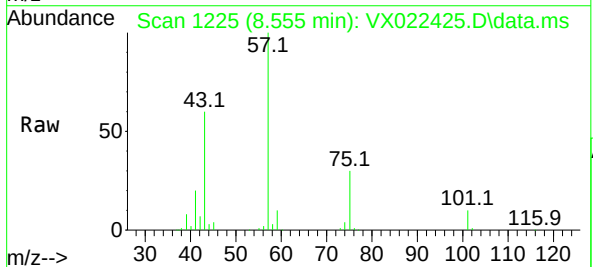




#52
Toluene
Concen: 3.176 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. -0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 92 Resp: 8107
Ion Ratio Lower Upper
92 100
91 162.1 137.1 205.7

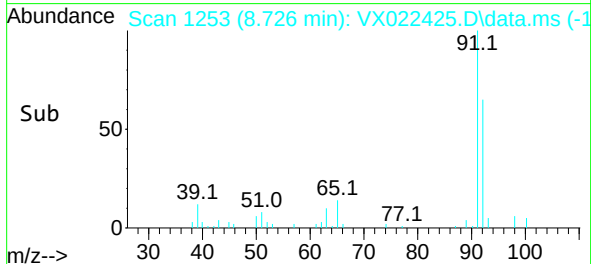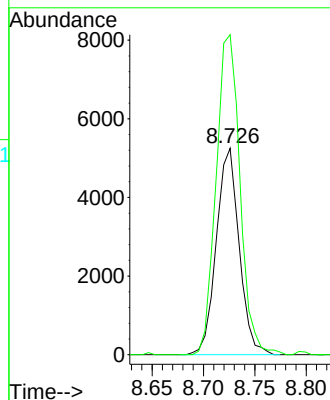

#54
cis-1,3-Dichloropropene
Concen: 10.475 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. 0.182 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09


Tgt Ion: 75 Resp: 18147
Ion Ratio Lower Upper
75 100
77 0.5 25.7 38.5#
39 26.9 35.1 52.7#

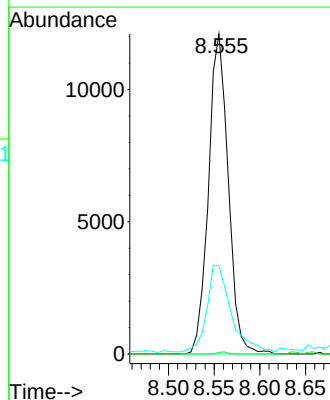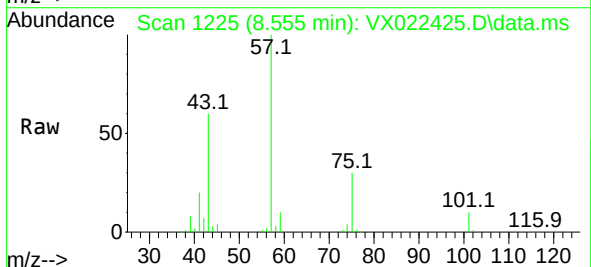






#55
1,1,2-Trichloroethane
Concen: 0.248 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.055 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Instrument :
MSVOA_X
ClientSampled :







Tgt Ion	Ratio	Lower	Upper
97	100		
83	0.0	69.3	103.9#
85	0.0	44.3	66.5#
99	0.0	50.3	75.5#

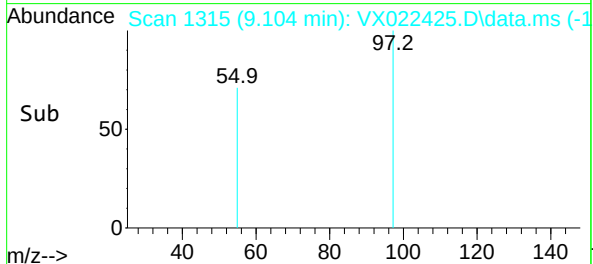

#57
1,3-Dichloropropane
Concen: 5.381 ug/l
RT: 9.488 min Scan# 1378
Delta R.T. 0.177 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion	Ratio	Lower	Upper
76	100		
78	0.0	26.2	39.2#


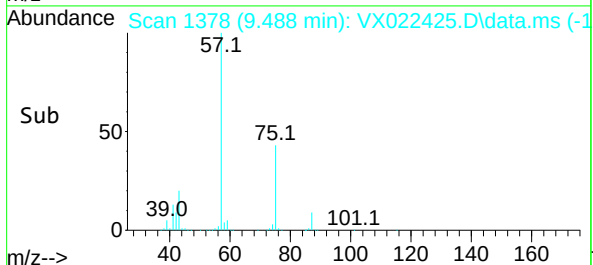

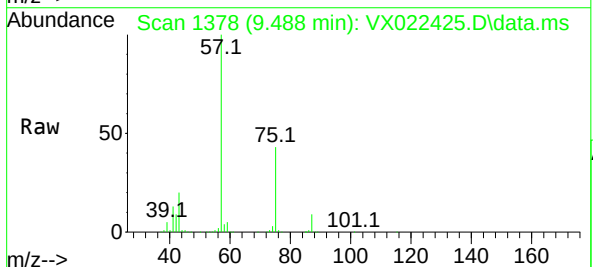




#59
2-Hexanone
Concen: 110.994 ug/l
RT: 9.488 min Scan# 1378
Delta R.T. 0.055 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 131354
Ion Ratio Lower Upper
43 100
58 19.0 30.9 92.8#

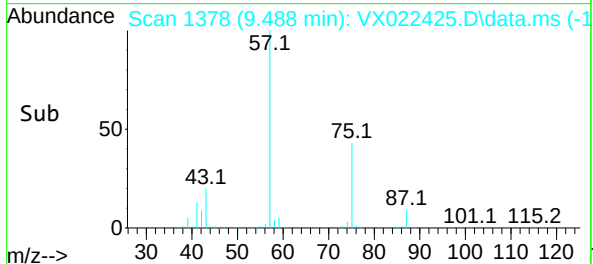

#62
4-Bromofluorobenzene
Concen: 47.356 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion: 95 Resp: 60579
Ion Ratio Lower Upper
95 100
174 64.1 0.0 154.6
176 59.6 0.0 155.8




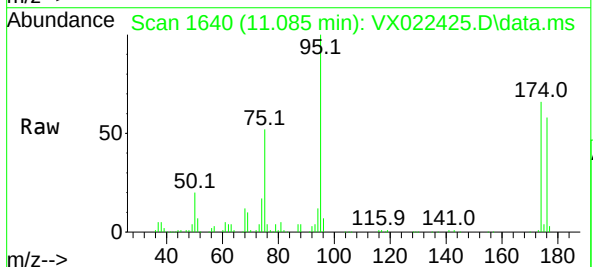




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. -0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:117 Resp: 126035
Ion Ratio Lower Upper
117 100
82 56.5 47.4 71.2
119 29.8 26.6 39.8



#67
Ethyl Benzene
Concen: 5.686 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion: 91 Resp: 27445
Ion Ratio Lower Upper
91 100
106 29.5 24.6 37.0




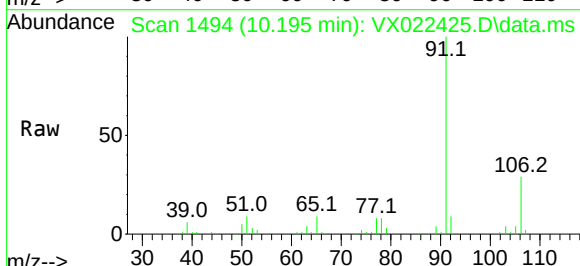




#68
m/p-Xylenes
Concen: 16.464 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:106 Resp: 30031
Ion Ratio Lower Upper
106 100
91 200.2 162.8 244.2

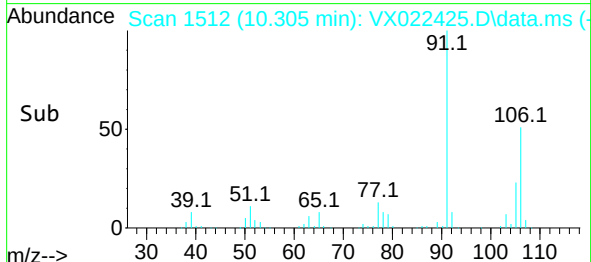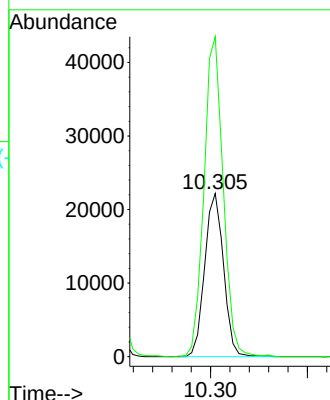

#69
o-Xylene
Concen: 4.830 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.001 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion:106 Resp: 8569
Ion Ratio Lower Upper
106 100
91 242.0 108.1 324.2



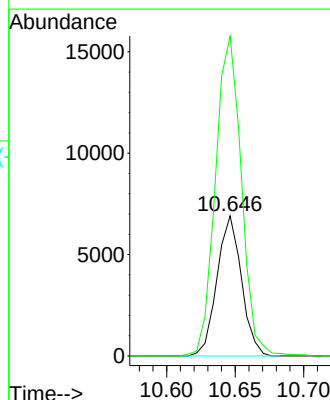
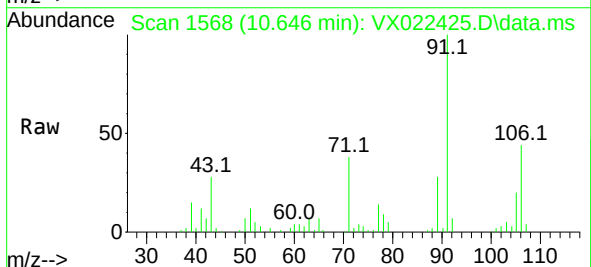




#70
Styrene
Concen: 0.235 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.013 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:104 Resp: 684
Ion Ratio Lower Upper
104 100
78 255.1 40.0 60.0#
103 170.8 43.4 65.0#

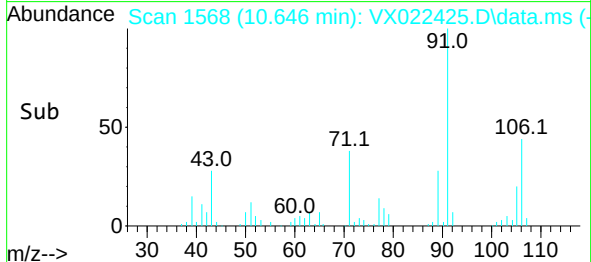

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion:152 Resp: 50339
Ion Ratio Lower Upper
152 100
115 67.6 41.1 123.3
150 156.1 0.0 349.0


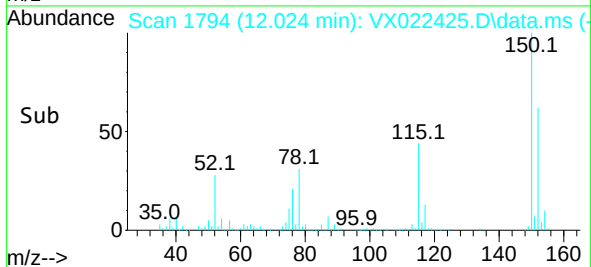

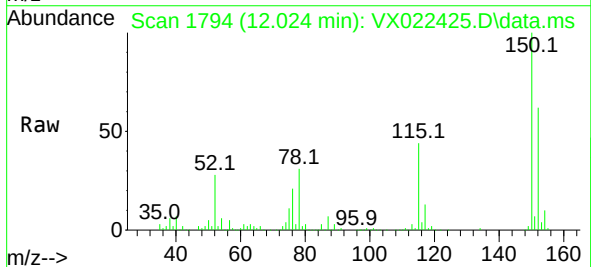




#73
Isopropylbenzene
Concen: 0.910 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.001 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:105 Resp: 3877
Ion Ratio Lower Upper
105 100
120 23.3 13.2 39.6

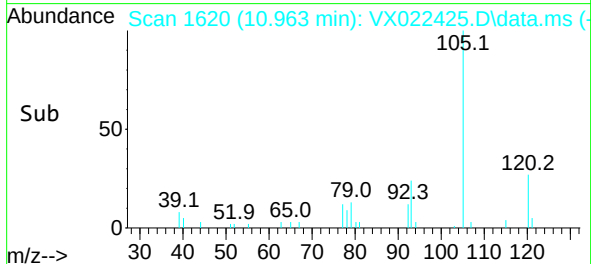

#74
N-ethyl acetate
Concen: 0.298 ug/l
RT: 10.896 min Scan# 1609
Delta R.T. 0.048 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion: 43 Resp: 602
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.6#
55 13.8 21.5 32.3#
61 0.0 22.1 33.1#




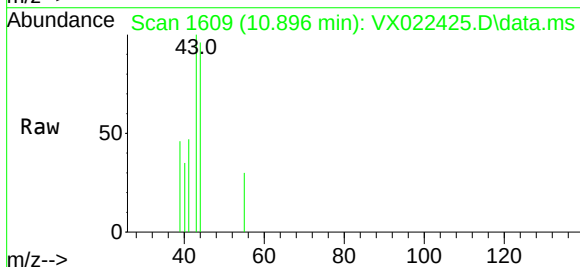




#76
1,2,3-Trichloropropane
Concen: 25.677 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 75 Resp: 31888
Ion Ratio Lower Upper
75 100
77 1.4 19.1 57.5#

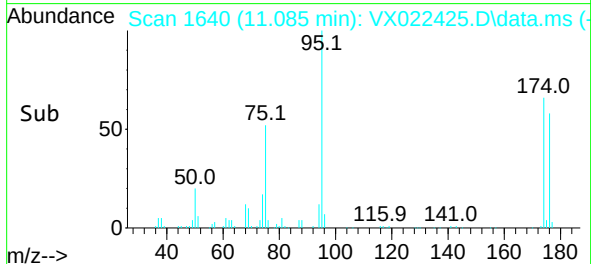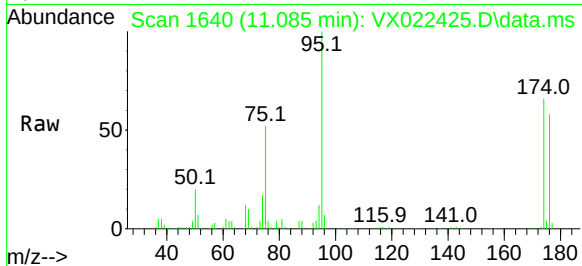

#78
n-propylbenzene
Concen: 0.542 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion: 91 Resp: 2706
Ion Ratio Lower Upper
91 100
120 23.6 11.5 34.5


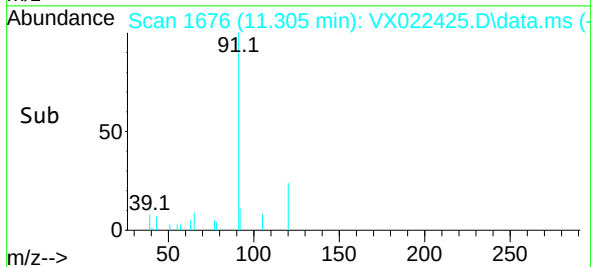

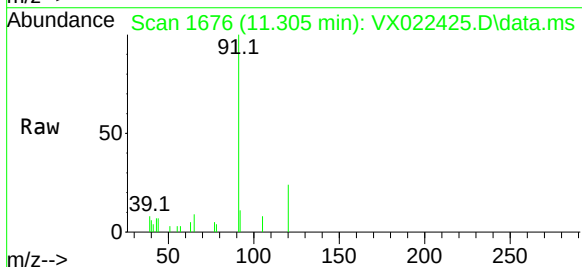




#79
2-Chlorotoluene
Concen: 0.606 ug/l
RT: 11.384 min Scan# 1689
Delta R.T. 0.018 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 1834
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#

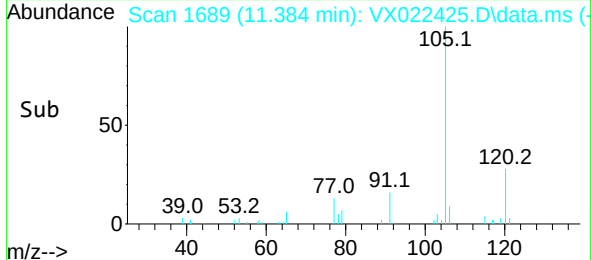

#80
1,3,5-Trimethylbenzene
Concen: 2.080 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion: 105 Resp: 7344
Ion Ratio Lower Upper
105 100
120 45.3 23.8 71.5


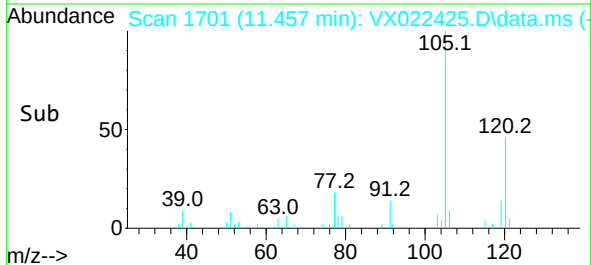

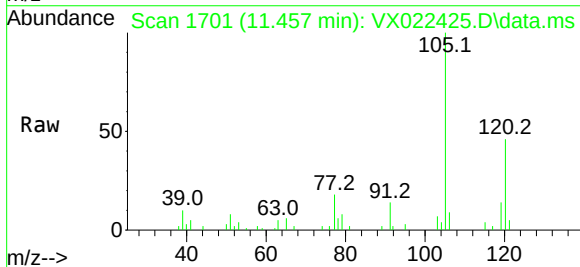




#81
trans-1,4-Dichloro-2-butene
Concen: 60.839 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.060 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 75 Resp: 31888
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

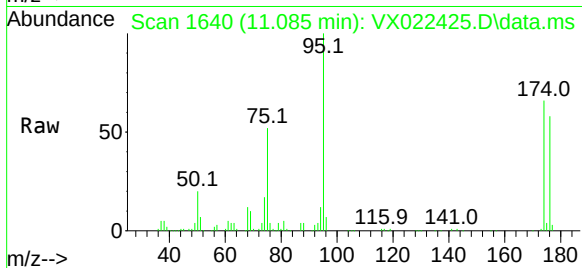

#82
4-Chlorotoluene
Concen: 0.303 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion: 91 Resp: 1055
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#




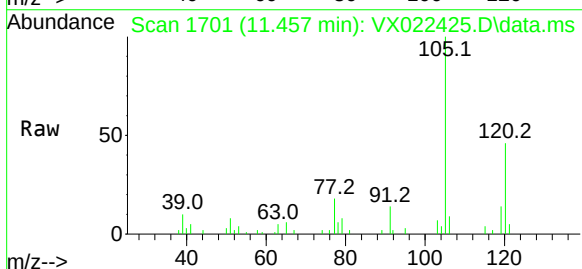




#83
tert-Butylbenzene
Concen: 0.467 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. 0.255 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:119 Resp: 1583
Ion Ratio Lower Upper
119 100
91 38.0 27.9 83.7
134 26.2 11.3 33.9

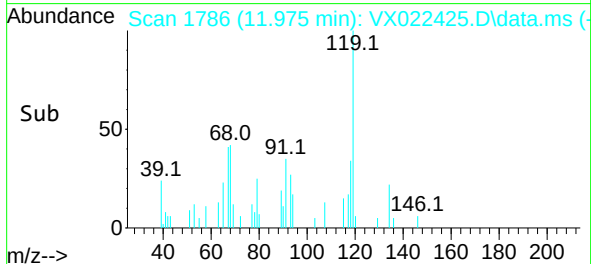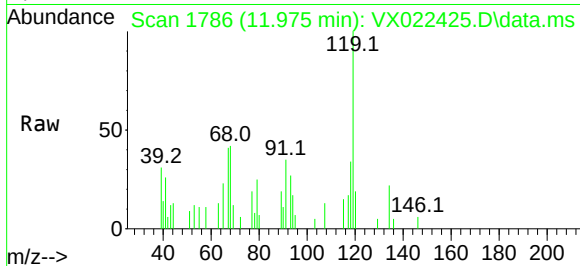

#84
1,2,4-Trimethylbenzene
Concen: 5.542 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Tgt Ion:105 Resp: 19699
Ion Ratio Lower Upper
105 100
120 43.3 22.4 67.3


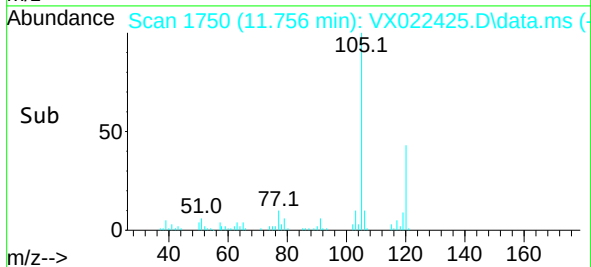

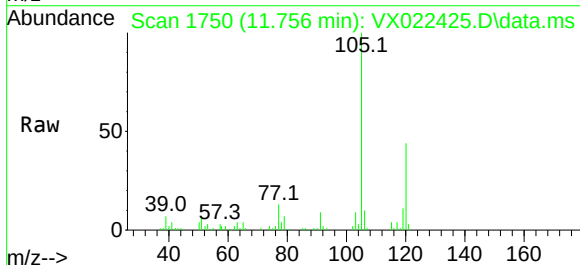




#86
 p-Isopropyltoluene
 Concen: 1.214 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. -0.000 min
 Lab File: VX022425.D
 Acq: 04 Jun 2021 20:09




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:119 Resp: 4413
 Ion Ratio Lower Upper
 119 100
 134 29.7 12.9 38.7
 91 32.9 11.7 35.0

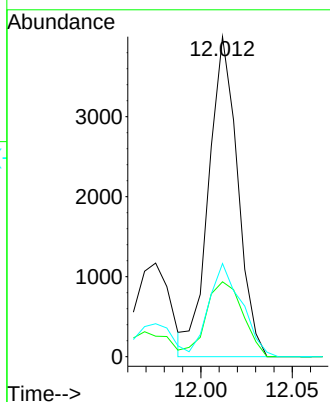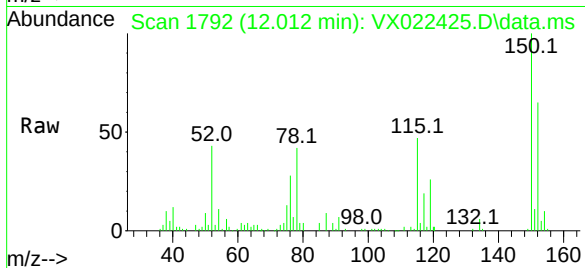

#88
 1,4-Dichlorobenzene
 Concen: 0.428 ug/l
 RT: 12.042 min Scan# 1797
 Delta R.T. -0.001 min
 Lab File: VX022425.D
 Acq: 04 Jun 2021 20:09

Tgt Ion:146 Resp: 770
 Ion Ratio Lower Upper
 146 100
 111 157.9 19.6 58.8#
 148 94.2 31.6 95.0

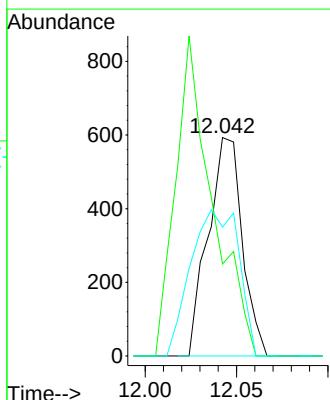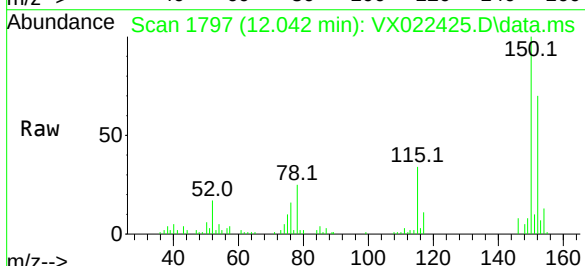



#89

n-Butylbenzene

Concen: 0.333 ug/l

RT: 12.329 min Scan# 1844





Delta R.T. -0.006 min

Lab File: VX022425.D

Acq: 04 Jun 2021 20:09

Tgt Ion: 91	Resp: 1121
Ion Ratio	Lower Upper
91	100
92	30.1 27.4 82.0
134	98.8 13.2 39.5#

Instrument :
MSVOA_X
ClientSampled :

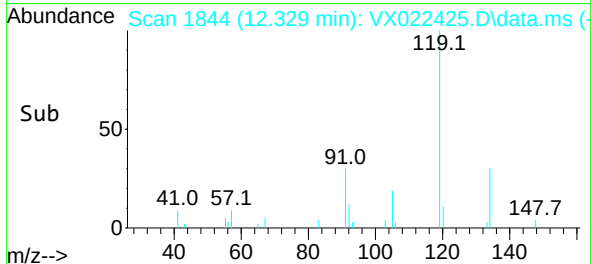

#90

Hexachloroethane

Concen: 0.829 ug/l




RT: 12.652 min Scan# 1897


Delta R.T. 0.109 min

Lab File: VX022425.D

Acq: 04 Jun 2021 20:09

Tgt Ion: 117	Resp: 498
Ion Ratio	Lower Upper
117	100
201	0.0 40.4 121.2#


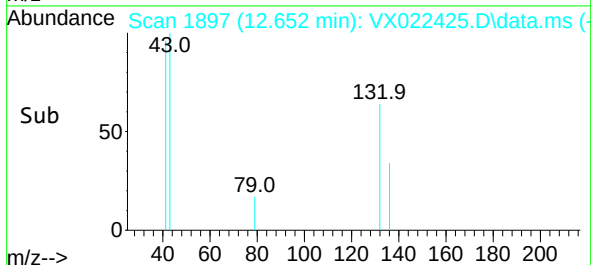

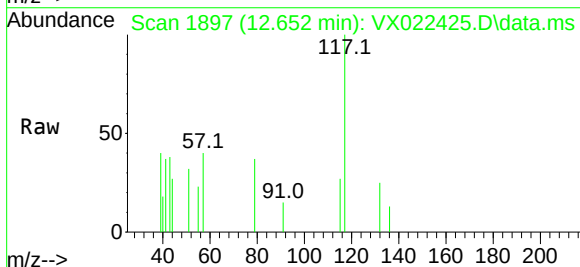




#91
1,2-Dichlorobenzene
Concen: 0.374 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. -0.006 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:146 Resp: 625
Ion Ratio Lower Upper
146 100
111 44.5 20.8 62.2
148 48.6 31.9 95.5

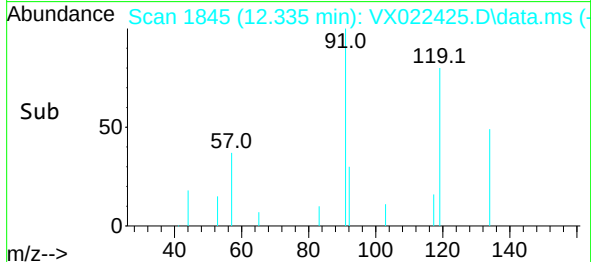

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.616 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.018 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09


Tgt Ion: 75 Resp: 186
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

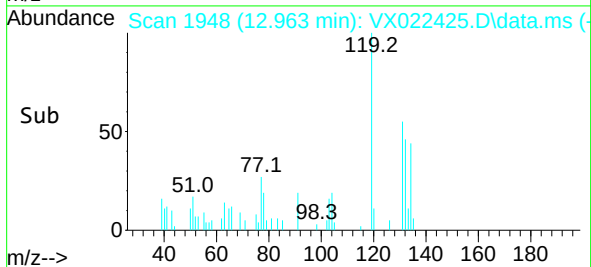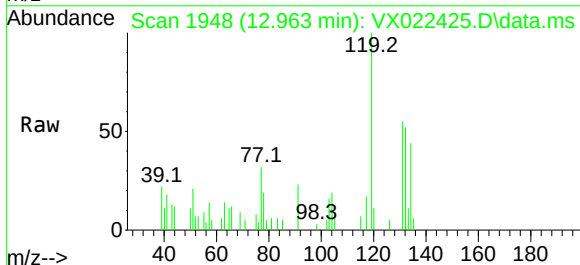



#95
Naphthalene
Concen: 213.087 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX022425.D
Acq: 04 Jun 2021 20:09

Instrument :
MSVOA_X
ClientSampleId :



Tgt Ion:128 Resp: 838917
Ion Ratio Lower Upper
128 100
127 12.8 10.3 15.5
129 11.2 8.8 13.2

