

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060421\
 Data File : VX022414.D
 Acq On : 04 Jun 2021 15:58
 Operator : JC/MD
 Sample : M2619-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PILOT-PLANT-PROCESS-BLEED

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.392	209	214	221	rVB	6611	10983	2.47%	0.490%
2	2.550	233	240	250	rVB2	2914	5594	1.26%	0.250%
3	5.099	651	658	669	rVB3	7811	23450	5.28%	1.046%
4	5.397	696	707	722	rBV2	45431	132828	29.89%	5.924%
5	5.562	722	734	751	rBV	74208	206838	46.54%	9.226%
6	5.964	789	800	811	rBV	59700	155554	35.00%	6.938%
7	6.769	921	932	945	rBV	132990	316983	71.32%	14.138%
8	8.653	1234	1241	1253	rBV	284605	444455	100.00%	19.824%
9	10.055	1465	1471	1480	rBV	273370	373090	83.94%	16.641%
10	11.085	1634	1640	1648	rBV	202250	259033	58.28%	11.554%
11	12.024	1789	1794	1800	rBV	258363	313208	70.47%	13.970%




Sum of corrected areas: 2242016

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060421\
Data File : VX022414.D
Acq On : 04 Jun 2021 15:58
Operator : JC/MD
Sample : M2619-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PILOT-PLANT-PROCESS-BLEED

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

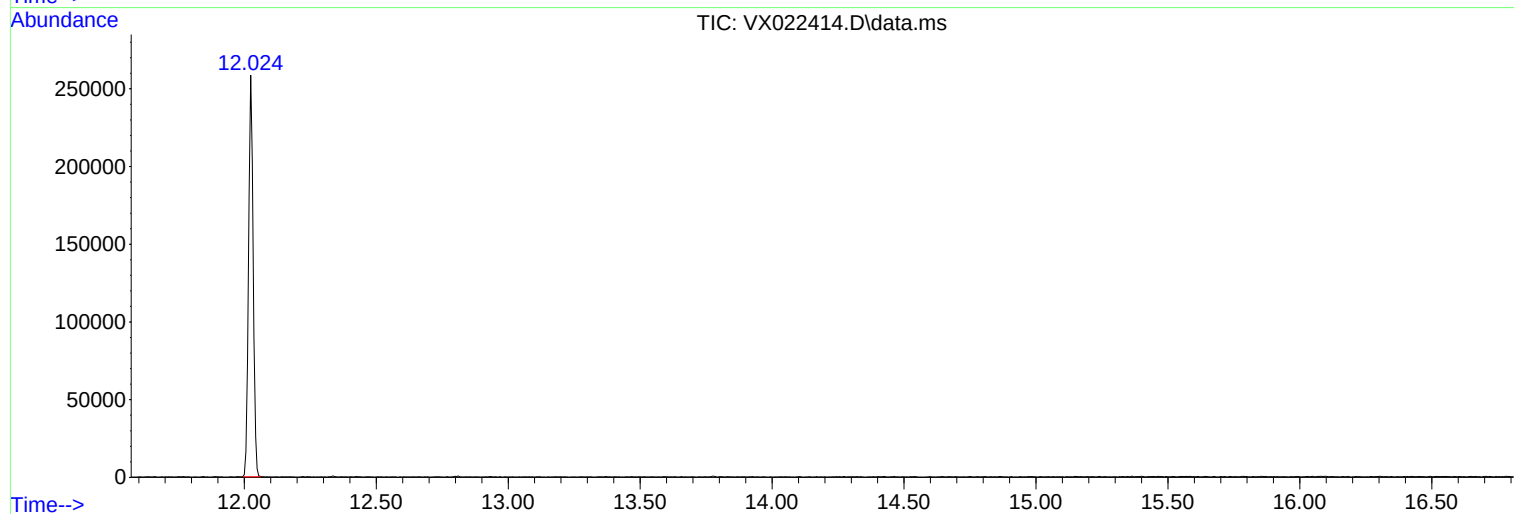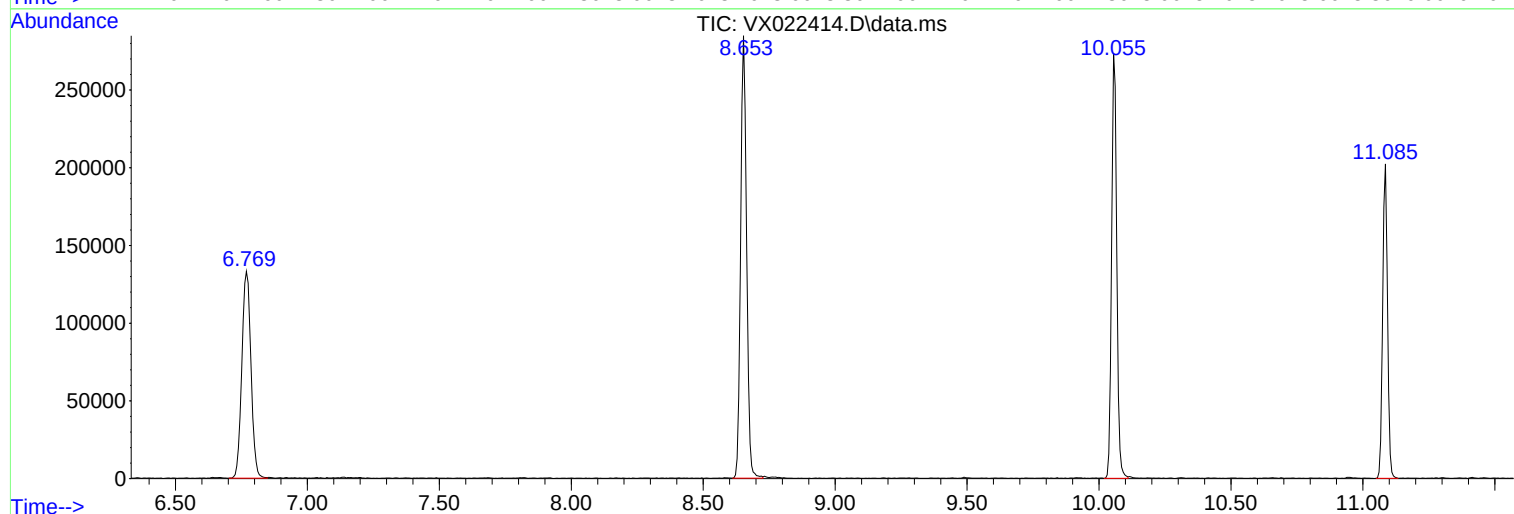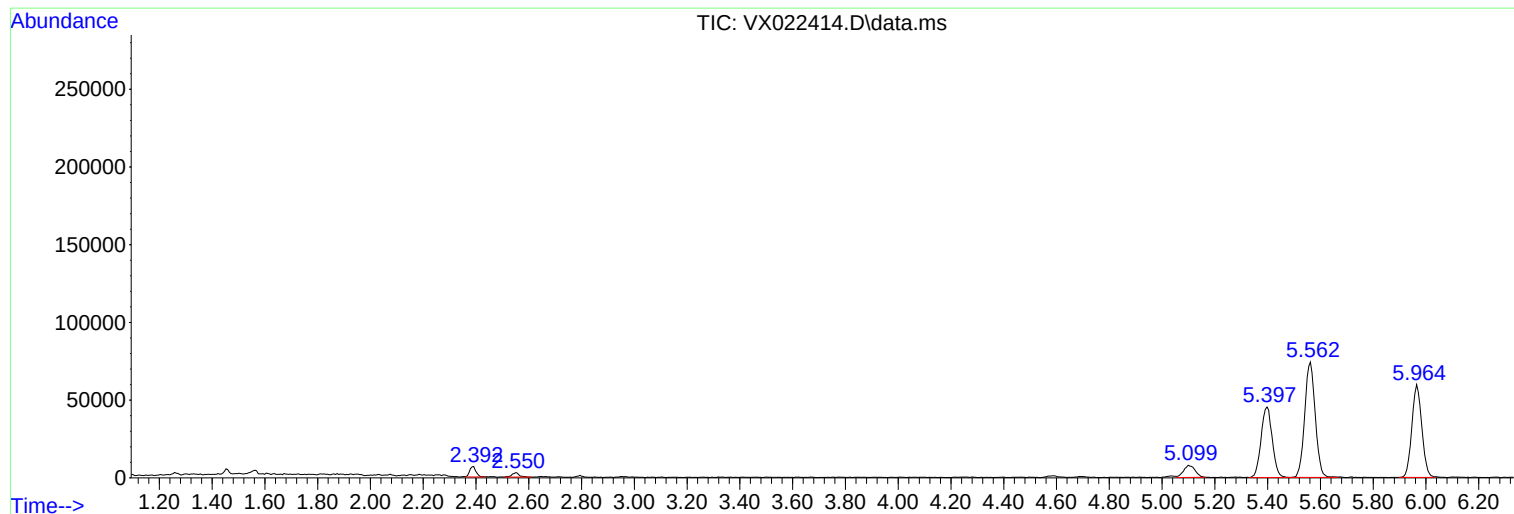

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060421\
Data File : VX022414.D
Acq On : 04 Jun 2021 15:58
Operator : JC/MD
Sample : M2619-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PILOT-PLANT-PROCESS-BLEED

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060421\
Data File : VX022414.D
Acq On : 04 Jun 2021 15:58
Operator : JC/MD
Sample : M2619-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PILOT-PLANT-PROCESS-BLEED

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
