
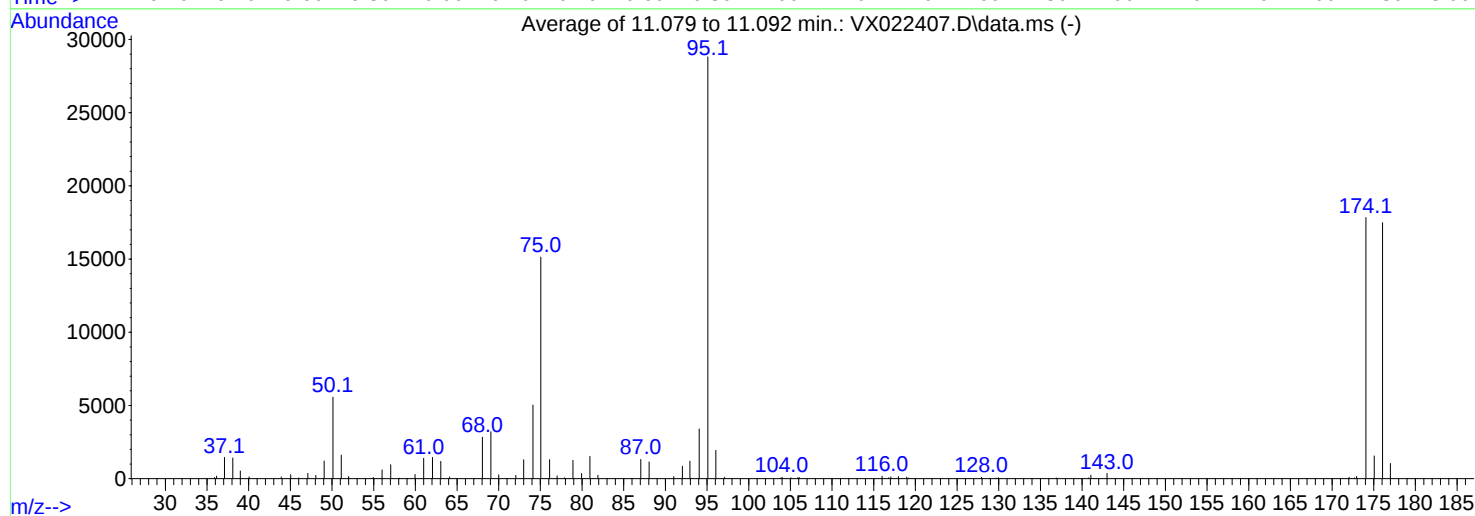


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060421\
 Data File : VX022407.D
 Acq On : 04 Jun 2021 08:57
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Title : SW846 8260
 Last Update : Wed May 19 14:23:10 2021

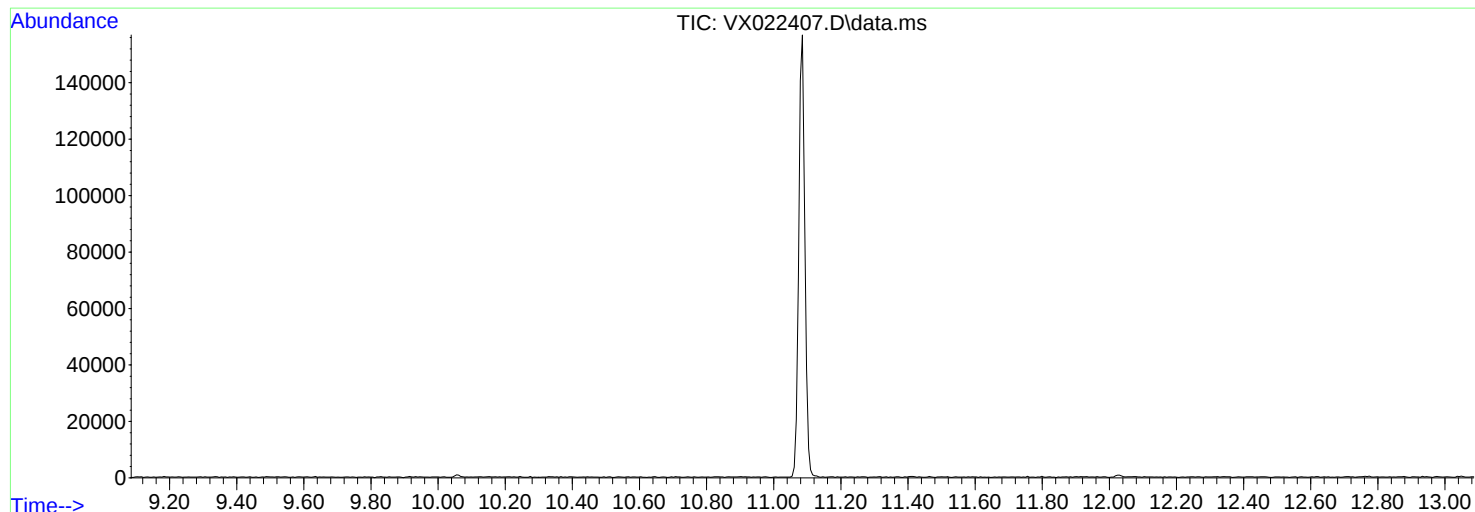

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	5565	PASS
75	95	30	60	52.5	15134	PASS
95	95	100	100	100.0	28813	PASS
96	95	5	9	6.7	1936	PASS
173	174	0.00	2	0.8	151	PASS
174	95	50	100	61.9	17834	PASS
175	174	5	9	8.7	1553	PASS
176	174	95	101	98.1	17488	PASS
177	176	5	9	5.9	1038	PASS