

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX060518\
 Data File : VX002307.D
 Acq On : 05 Jun 2018 15:57
 Operator : JC/MD
 Sample : J3270-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 LF6-0057

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	93	rBV	1346063	1679295	100.00%	16.380%
2	1.203	98	101	107	rVV	65559	75171	4.48%	0.733%
3	1.270	107	112	119	rVB2	13486	28087	1.67%	0.274%
4	1.392	128	132	139	rBV	67397	73524	4.38%	0.717%
5	1.642	170	173	177	rVB5	14713	24731	1.47%	0.241%
6	1.885	209	213	221	rVB	15454	23480	1.40%	0.229%
7	2.190	257	263	280	rVB	366142	537381	32.00%	5.242%
8	5.507	794	807	822	rBV	151796	440230	26.22%	4.294%
9	5.665	822	833	847	rVV	242176	684346	40.75%	6.675%
10	6.074	888	900	907	rBV	182681	477142	28.41%	4.654%
11	6.147	907	912	928	rVB	60191	154429	9.20%	1.506%
12	6.866	1017	1030	1046	rBV	362772	863502	51.42%	8.423%
13	8.720	1327	1334	1342	rBV	903669	1391635	82.87%	13.574%
14	8.787	1342	1345	1352	rVB2	10831	18057	1.08%	0.176%
15	10.116	1556	1563	1574	rBV2	766970	1225986	73.01%	11.959%
16	10.366	1599	1604	1611	rVB	81663	103362	6.16%	1.008%
17	11.024	1706	1712	1717	rBV	29178	39206	2.33%	0.382%
18	11.140	1725	1731	1739	rBV	787623	991803	59.06%	9.674%
19	11.365	1763	1768	1774	rVB3	20419	27775	1.65%	0.271%
20	11.810	1837	1841	1846	rVB	19818	24588	1.46%	0.240%
21	12.085	1880	1886	1893	rBV	925196	1218586	72.57%	11.886%
22	12.304	1916	1922	1928	rVV	39961	53761	3.20%	0.524%
23	12.396	1931	1937	1942	rVB	20942	28335	1.69%	0.276%
24	13.353	2087	2094	2099	rBV3	19845	30834	1.84%	0.301%
25	13.841	2168	2174	2181	rVB	27607	36651	2.18%	0.358%


Sum of corrected areas: 10251897

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX060518\
Data File : VX002307.D
Acq On : 05 Jun 2018 15:57
Operator : JC/MD
Sample : J3270-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LF6-0057

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

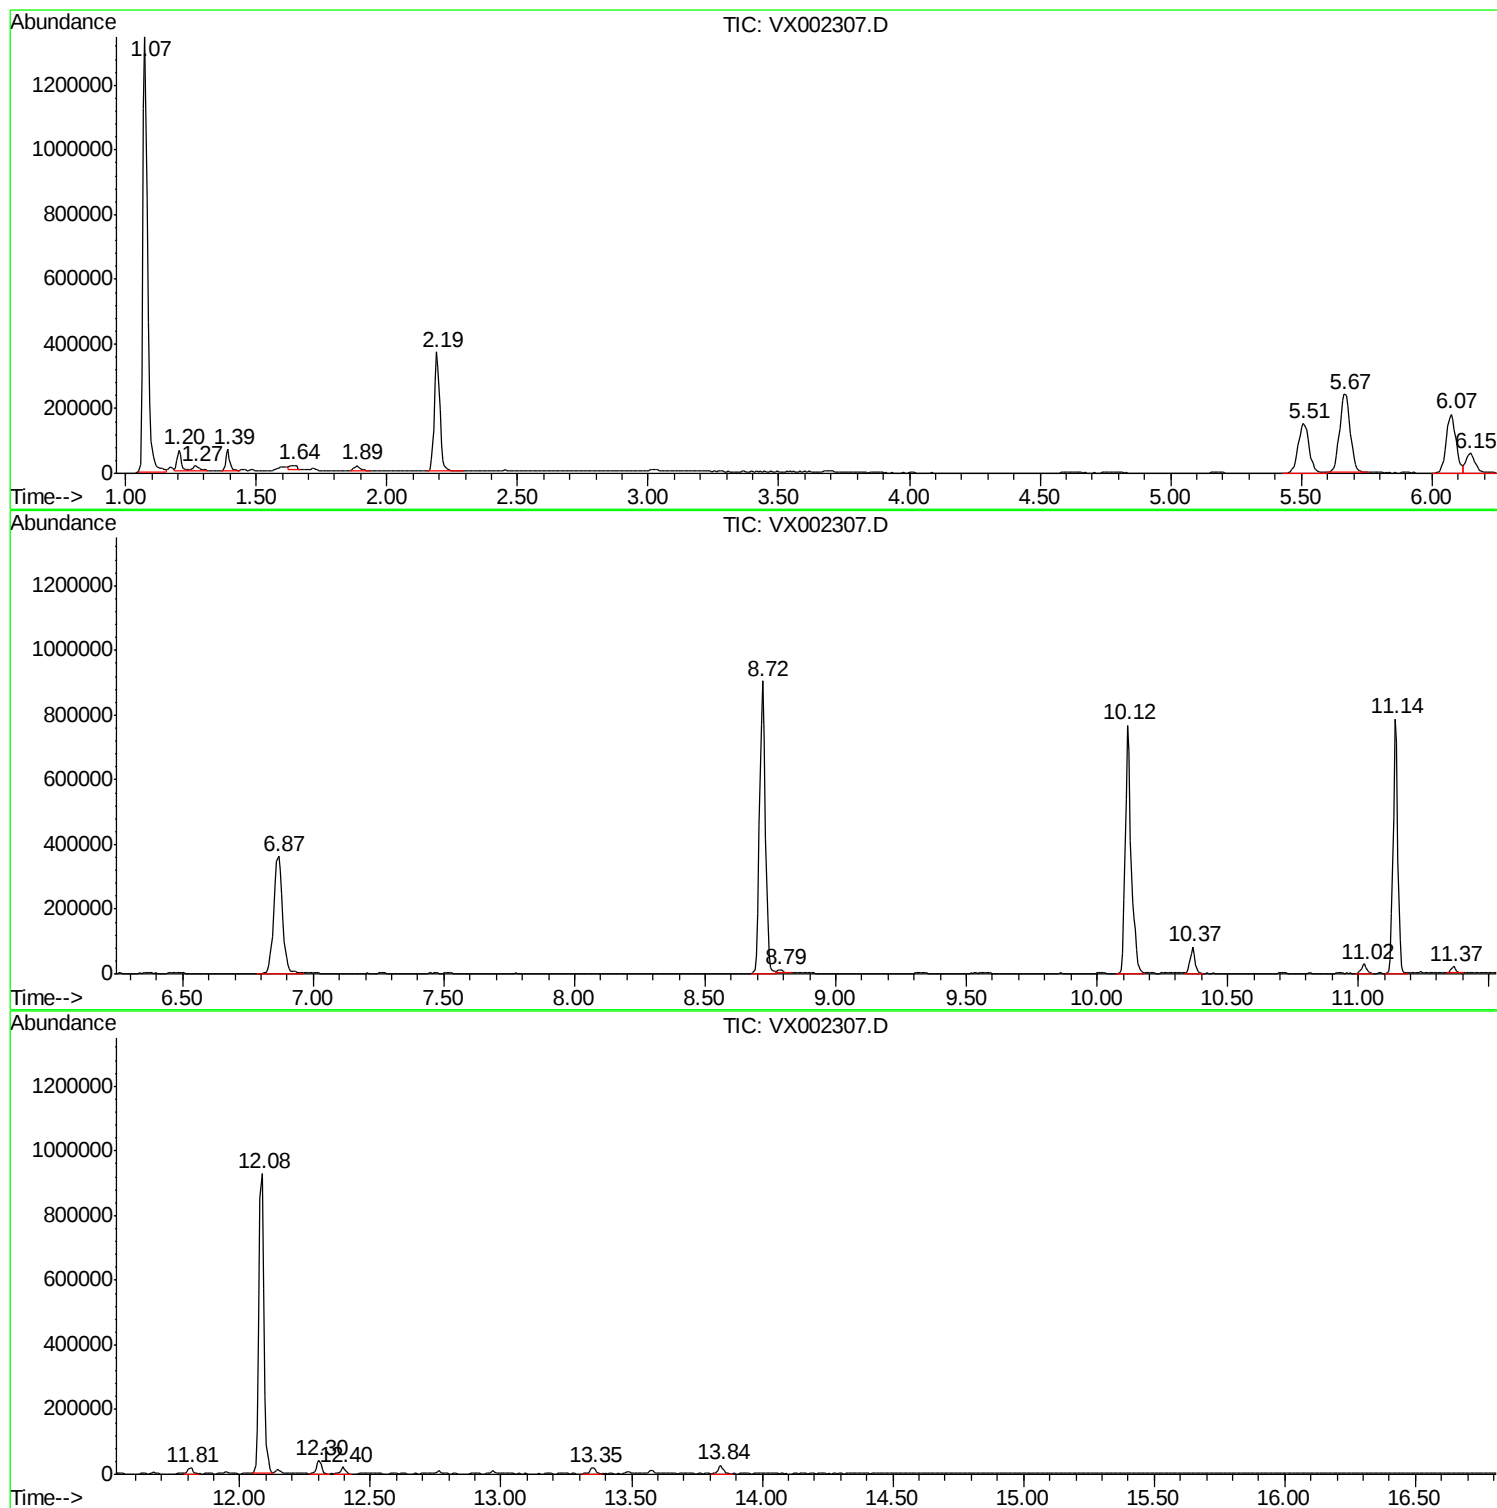

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX060518\
Data File : VX002307.D
Acq On : 05 Jun 2018 15:57
Operator : JC/MD
Sample : J3270-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LF6-0057

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Difluorochloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
1.20	5.49 ug/l	75171	Pentafluorobenzene	5.67	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Difluorochloromethane	86	CHClF2	000075-45-6	91
2	Ethane, 1,1-difluoro-	66	C2H4F2	000075-37-6	5
3	Propiolonitrile	51	C3HN	001070-71-9	4
4	1-Buten-3-yne, 1-chloro-, (Z)-	86	C4H3Cl	020374-90-7	2
5	2-p-Nitrobenzoyl-1,3,5-tribenzyl...	569	C33H31NO8	1000129-85-6	1

Peak Number 2 Methane, chlorofluoro- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.	
1.39	5.37 ug/l	73524	Pentafluorobenzene	5.67	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Methane, chlorofluoro-	68	CH2ClF	000593-70-4	91
2	Ethyl Chloride	64	C2H5Cl	000075-00-3	9
3	1,4-Pentadiene	68	C5H8	000591-93-5	4
4	2,3-Pentadiene	68	C5H8	000591-96-8	4
5	Furan	68	C4H4O	000110-00-9	3

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX060518\
Data File : VX002307.D
Acq On : 05 Jun 2018 15:57
Operator : JC/MD
Sample : J3270-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LF6-0057

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Difluorochloromet...	1.20	5.5	ug/l	75171	1	5.67	684346	50.0
Methane, chlorofl...	1.39	5.4	ug/l	73524	1	5.67	684346	50.0