


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX060518\
 Data File : VX002295.D
 Acq On : 05 Jun 2018 09:29
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
 Title : SW846 8260
 Last Update : Tue Jun 05 03:22:35 2018

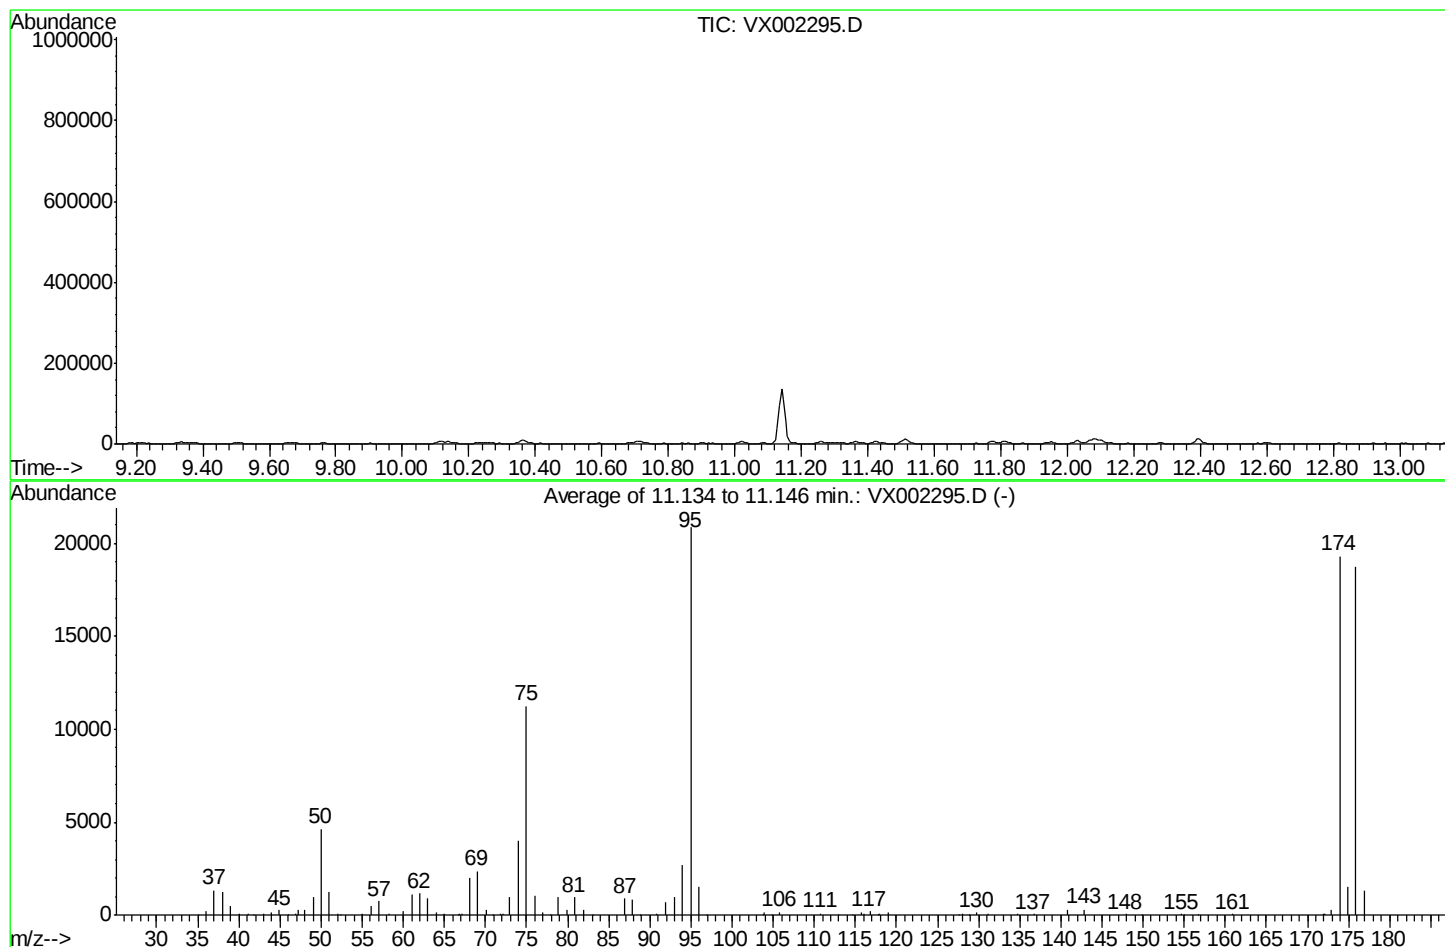

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	4648	PASS
75	95	30	60	54.0	11265	PASS
95	95	100	100	100.0	20880	PASS
96	95	5	9	7.3	1529	PASS
173	174	0.00	2	1.5	282	PASS
174	95	50	100	92.5	19314	PASS
175	174	5	9	7.7	1493	PASS
176	174	95	101	97.3	18784	PASS
177	176	5	9	7.1	1335	PASS