


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX060518\
Data File : VX002320.D
Acq On : 05 Jun 2018 22:11
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Title : SW846 8260
Last Update : Tue Jun 05 03:22:35 2018

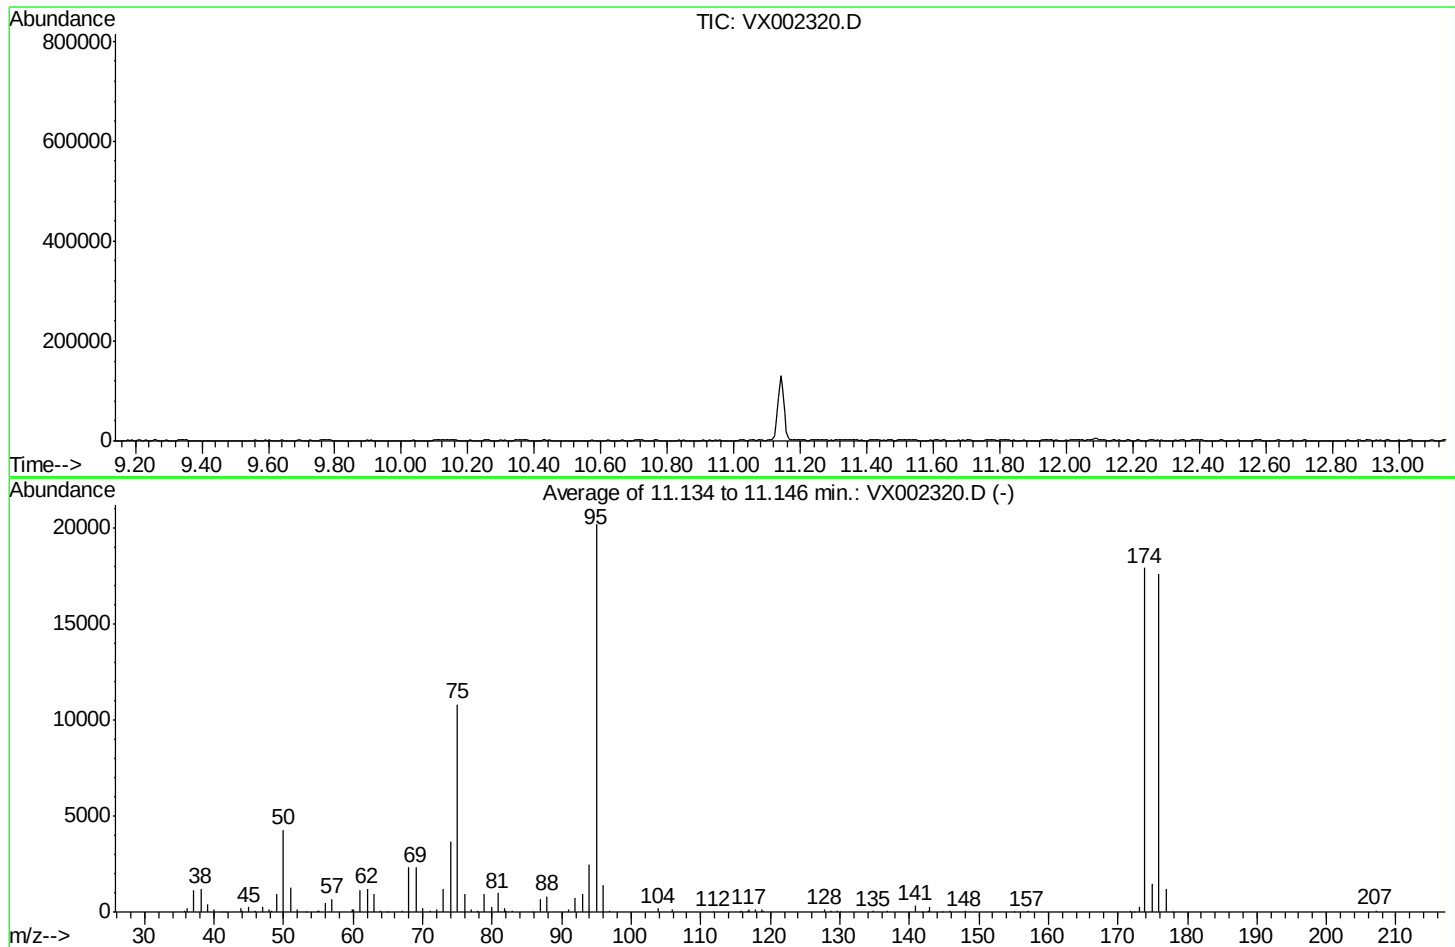

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	4295	PASS
75	95	30	60	53.7	10843	PASS
95	95	100	100	100.0	20208	PASS
96	95	5	9	6.9	1396	PASS
173	174	0.00	2	1.4	258	PASS
174	95	50	100	88.8	17937	PASS
175	174	5	9	8.1	1446	PASS
176	174	95	101	98.1	17589	PASS
177	176	5	9	6.7	1186	PASS