

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX060618\
 Data File : VX002365.D
 Acq On : 06 Jun 2018 20:49
 Operator : JC/MD
 Sample : J3312-09
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 W-25

Quant Time: Jun 07 03:27:13 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 05 03:22:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	230008	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	333791	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	302240	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	170222	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	157574	47.75	ug/l	0.00
Spiked Amount 50.000			Recovery =	95.50%		
35) Dibromofluoromethane	5.51	113	117827	44.89	ug/l	0.00
Spiked Amount 50.000			Recovery =	89.78%		
50) Toluene-d8	8.72	98	475690	47.28	ug/l	0.00
Spiked Amount 50.000			Recovery =	94.56%		
62) 4-Bromofluorobenzene	11.14	95	165835	42.74	ug/l	0.00
Spiked Amount 50.000			Recovery =	85.48%		


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.27	50	2024	Below Cal	#	43
5) Bromomethane	1.65	94	957	Below Cal		84
6) Chloroethane	1.62	64	6378	3.27	ug/l	56
8) Diethyl Ether	2.18	74	97	Below Cal	#	1
10) Methyl Iodide	2.51	142	970	0.28	ug/l	95
11) Tert butyl alcohol	3.07	59	1539	Below Cal	#	83
13) Acrolein	2.29	56	302	Below Cal	#	14
15) Acrylonitrile	3.16	53	157	Below Cal	#	61
16) Acetone	2.45	43	10352	Below Cal		92
18) Methyl Acetate	2.78	43	243	Below Cal	#	83
19) Methyl tert-butyl Ether	3.21	73	4321	Below Cal	#	85
20) Methylene Chloride	2.86	84	883	Below Cal		94
22) Diisopropyl ether	3.86	45	120	Below Cal	#	35
25) 2-Butanone	4.71	43	491	0.22	ug/l	78
28) Bromochloromethane	5.01	49	26	Below Cal	#	13
36) 1,1-Dichloropropene	5.67	75	16786	4.78	ug/l	51
38) Carbon Tetrachloride	5.67	117	21723	5.92	ug/l	16
39) Methylcyclohexane	7.48	83	49	0.27	ug/l	16
49) 1,4-Dioxane	7.64	88	20	0.30	ug/l	1
65) Chlorobenzene	10.14	112	1902	0.25	ug/l	92
76) 1,2,3-Trichloropropane	11.14	75	90124	24.13	ug/l	33
81) trans-1,4-Dichloro-2-buten	11.14	75	90124	84.58	ug/l	7
83) tert-Butylbenzene	11.77	119	3928	0.40	ug/l	87
85) sec-Butylbenzene	11.95	105	2891	0.25	ug/l	72
90) Hexachloroethane	12.66	117	464	0.28	ug/l	1
91) 1,2-Dichlorobenzene	12.40	146	1866	0.30	ug/l	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX060618\
Data File : VX002365.D
Acq On : 06 Jun 2018 20:49
Operator : JC/MD
Sample : J3312-09
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
W-25

Quant Time: Jun 07 03:27:13 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 05 03:22:35 2018
Response via : Initial Calibration

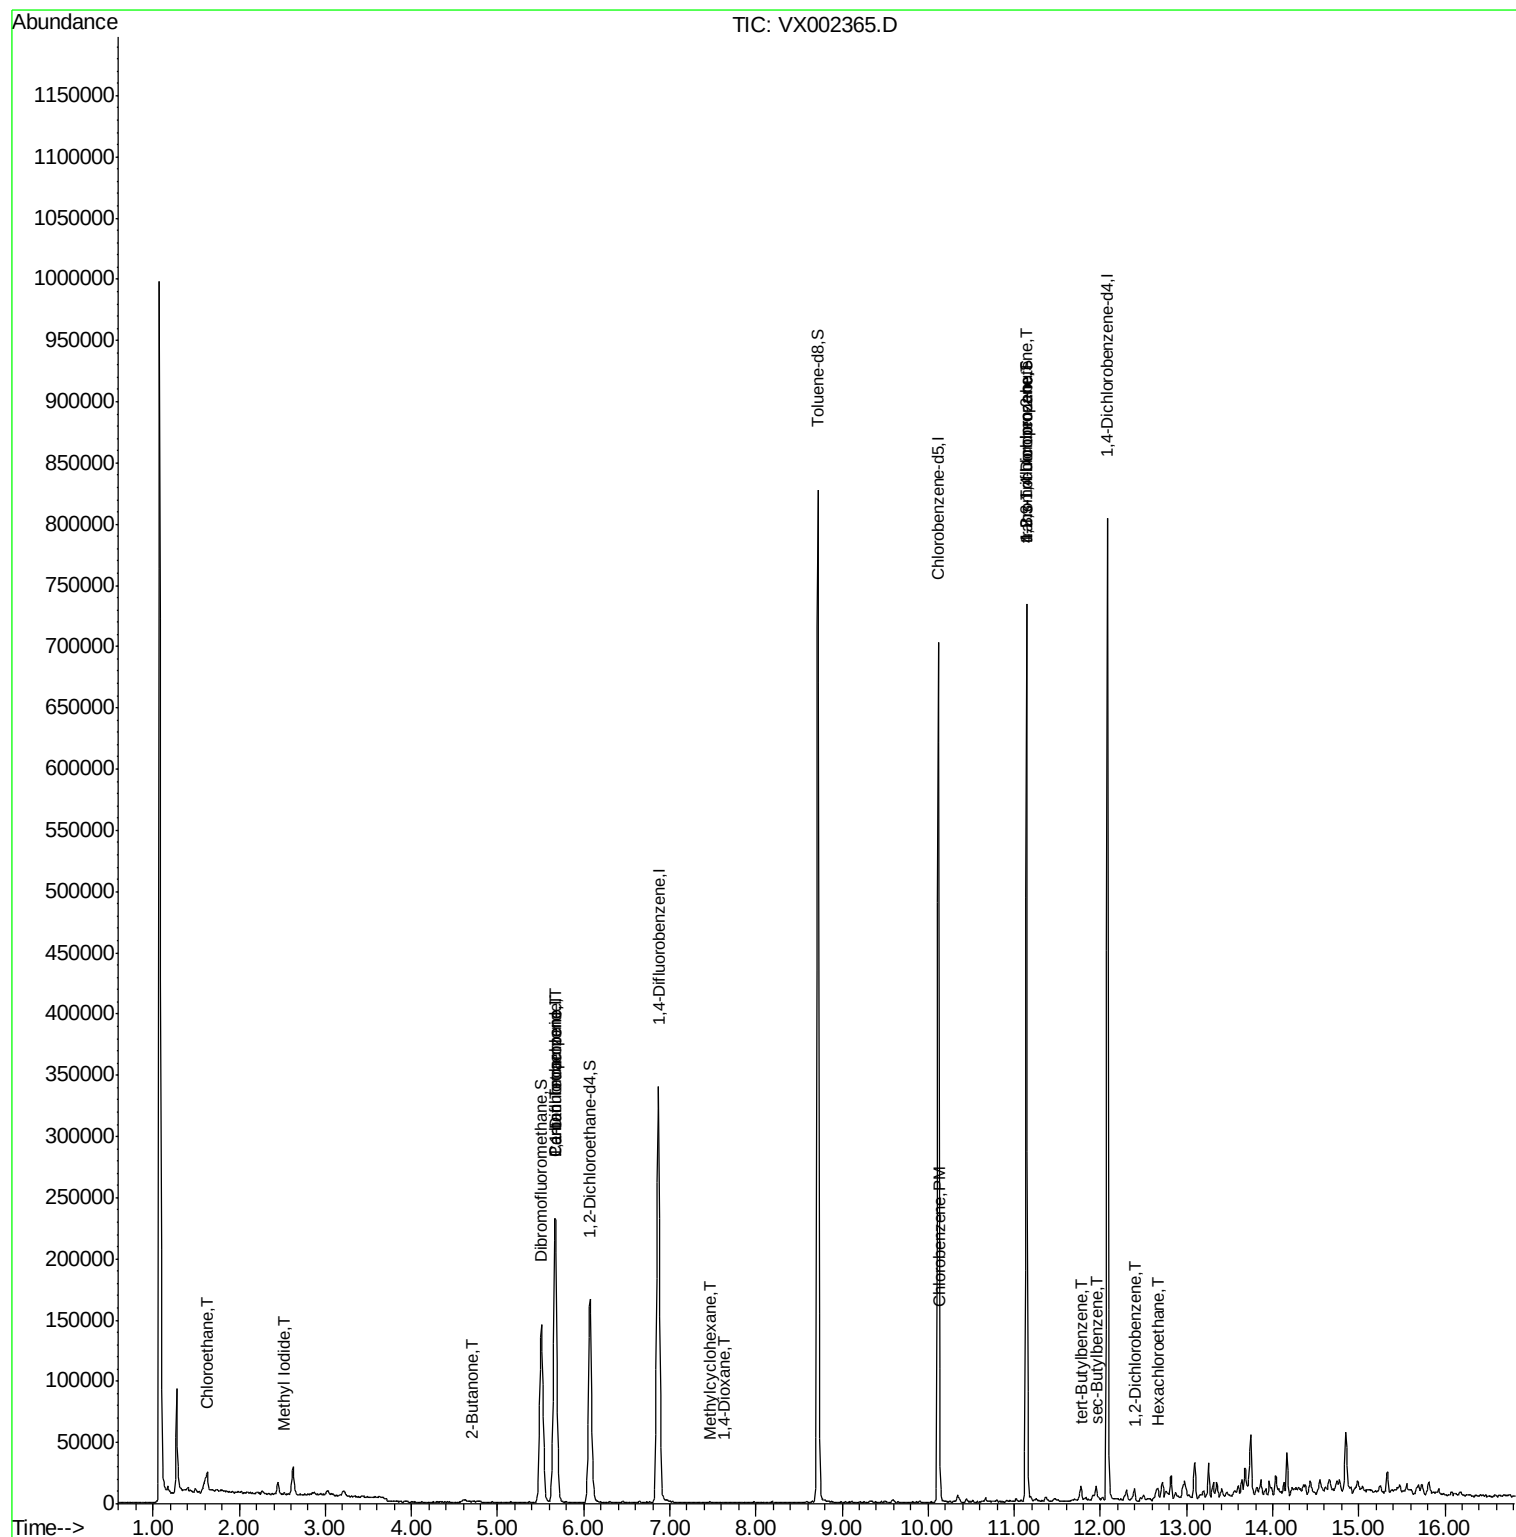



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.00 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49

Instrument :

MSVOA_X

ClientSampleId :


W-25

Tot Ion:168 Resp: 230008

Ion Ratio Lower Upper




168 100

99 51.5 39.3 58.9

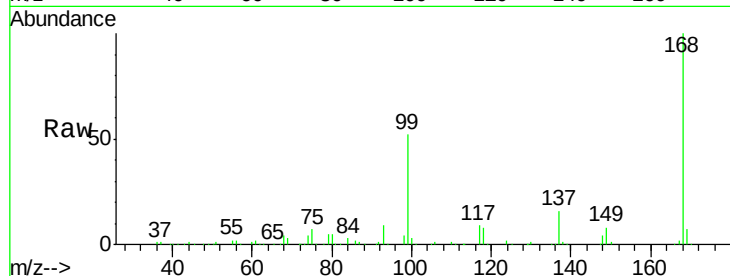

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

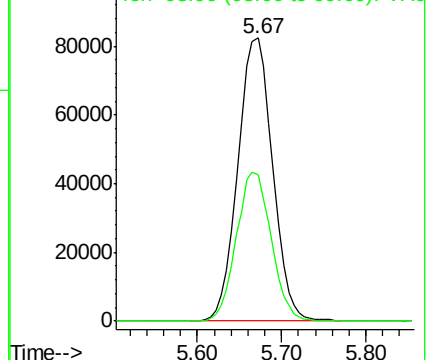

#3

Chloromethane

Concen: Below Cal

RT: 1.27 min Scan# 112

Delta R.T. -0.05 min

Lab File: VX002365.D


Acq: 06 Jun 2018 20:49

Tgt Ion: 50 Resp: 2024

Ion Ratio Lower Upper



50 100


52 0.0 25.7 38.5#



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

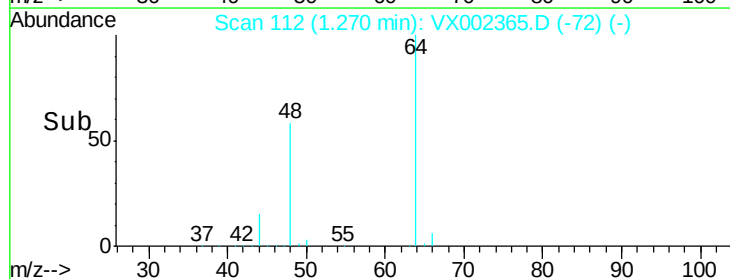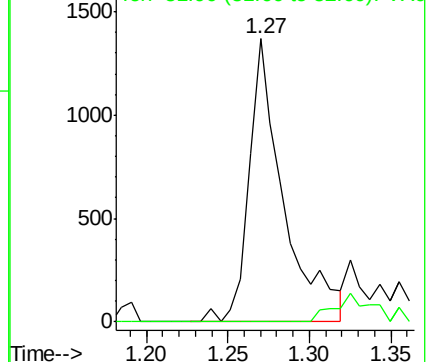

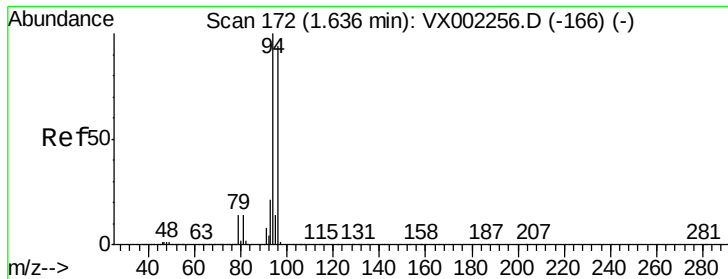

#5

Bromomethane

Concen: Below Cal

RT: 1.65 min Scan# 174

Delta R.T. 0.01 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49

Instrument :

MSVOA_X

ClientSampleId :





W-25

Tot Ion: 94 Resp: 957

Ion Ratio Lower Upper

94 100

96 78.0 74.9 112.3

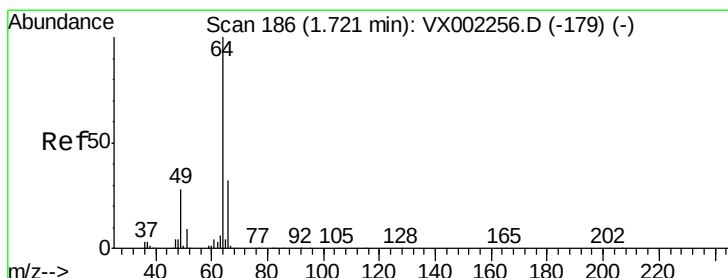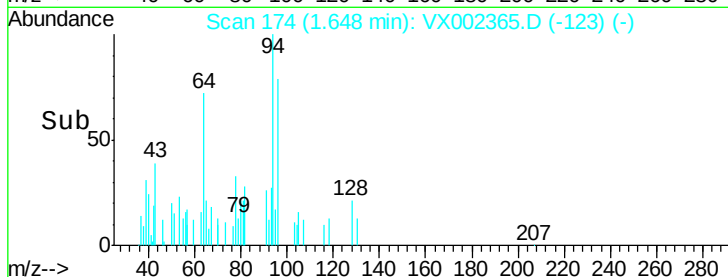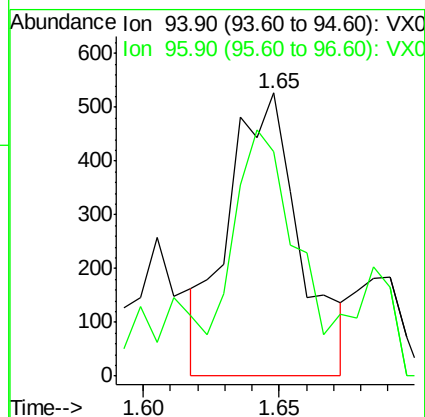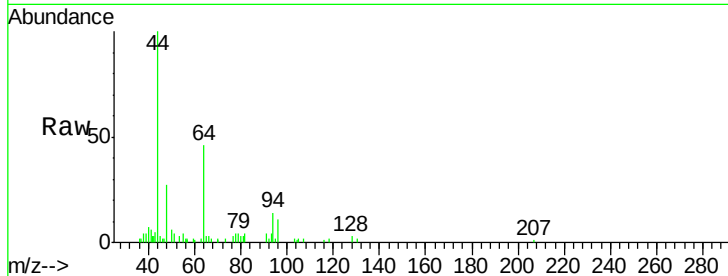

#6

Chloroethane

Concen: 3.27 ug/l

RT: 1.62 min Scan# 170

Delta R.T. -0.10 min

Lab File: VX002365.D




Acq: 06 Jun 2018 20:49


Tgt Ion: 64 Resp: 6378

Ion Ratio Lower Upper

64 100

66 7.2 25.5 38.3#

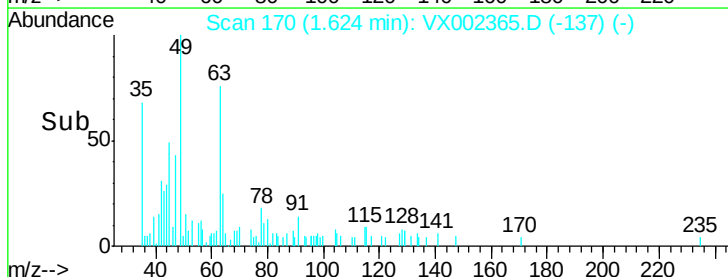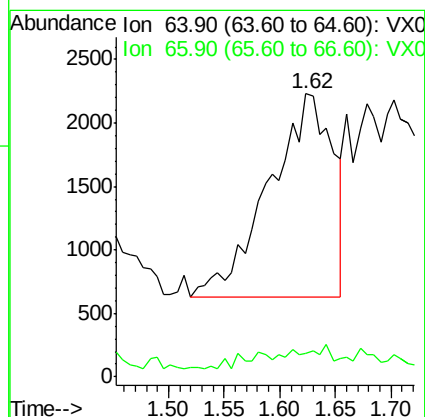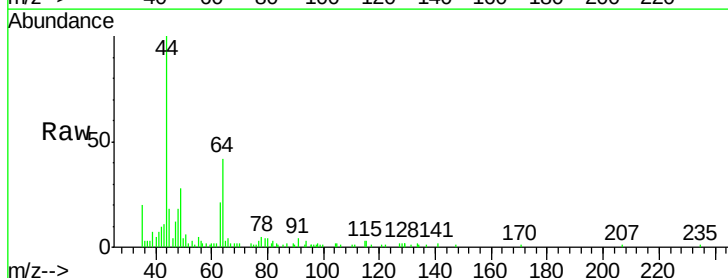

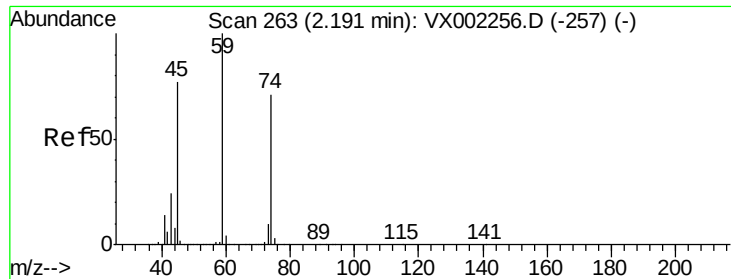

#8

Diethyl Ether

Concen: Below Cal

RT: 2.18 min Scan# 262

Delta R.T. -0.01 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49

Instrument :

MSVOA_X

ClientSampleId :


W-25

Tot Ion: 74 Resp: 97

Ion Ratio Lower Upper




74 100

45 0.0 53.1 159.4#

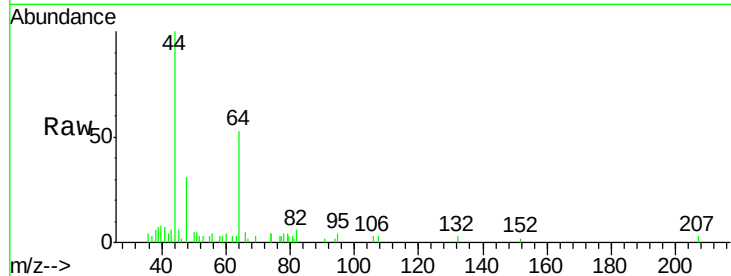

Abundance Ion 74.00 (73.70 to 74.70): VX0

Ion 45.00 (44.70 to 45.70): VX0

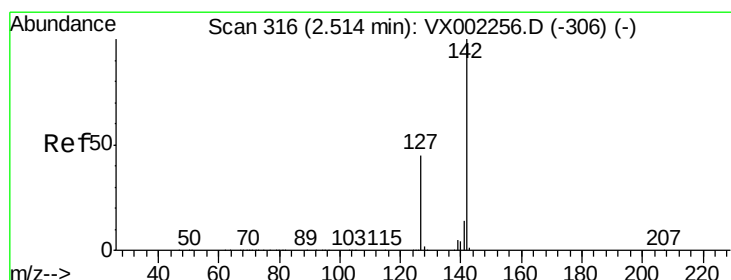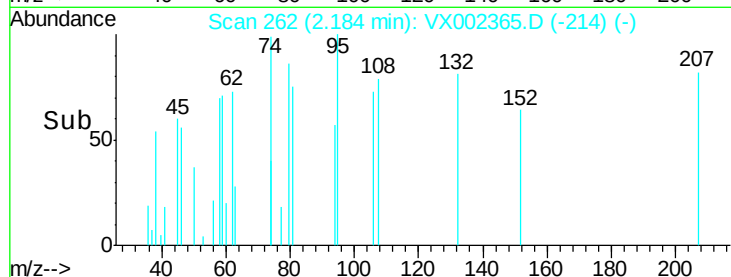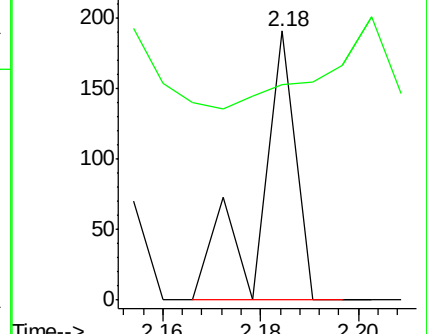

#10

Methyl Iodide

Concen: 0.28 ug/l

RT: 2.51 min Scan# 316

Delta R.T. -0.00 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49


Tgt Ion: 142 Resp: 970

Ion Ratio Lower Upper

142 100

127 45.2 36.6 55.0



141 22.0 11.3 16.9#

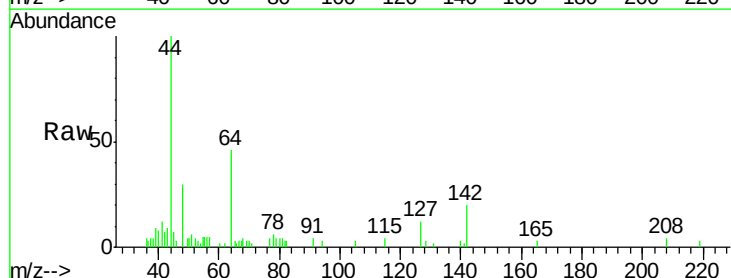


Abundance Ion 141.80 (141.50 to 142.50): V

Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V

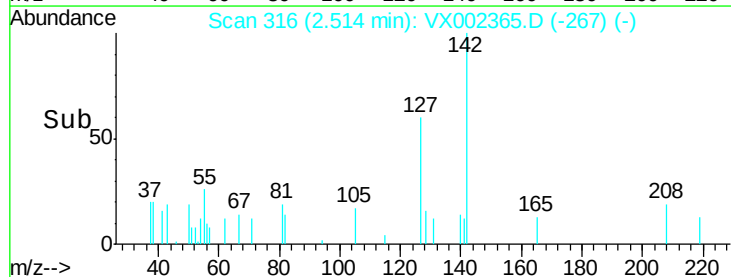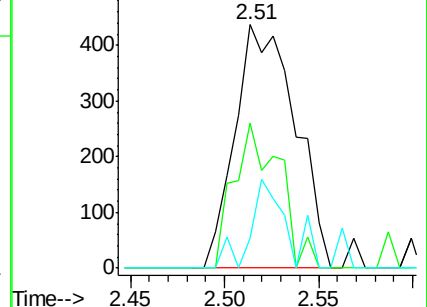




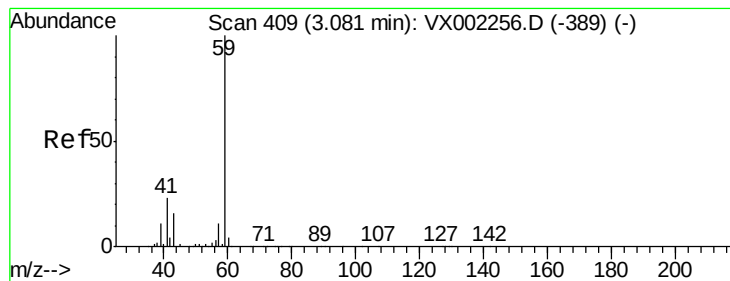


#11

Tert butyl alcohol
Concen: Below Cal
RT: 3.07 min Scan# 408
Delta R.T. -0.01 min
Lab File: VX002365.D
Acq: 06 Jun 2018 20:49

Instrument :
MSVOA_X
ClientSampled :
W-25




Tot Ion: 59 Resp: 1539
Ion Ratio Lower Upper
59 100
57 16.6 8.2 12.2#

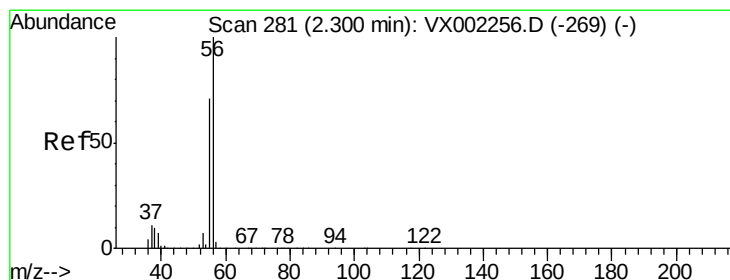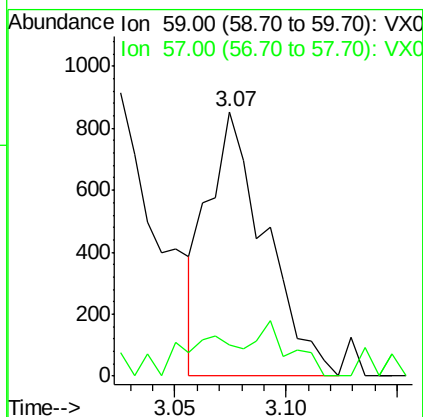


#13

Acrolein
Concen: Below Cal
RT: 2.29 min Scan# 280
Delta R.T. -0.01 min
Lab File: VX002365.D
Acq: 06 Jun 2018 20:49

Tgt Ion: 56 Resp: 302
Ion Ratio Lower Upper
56 100
55 0.0 57.0 85.4#

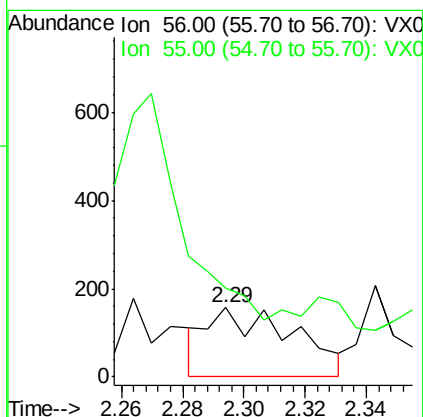

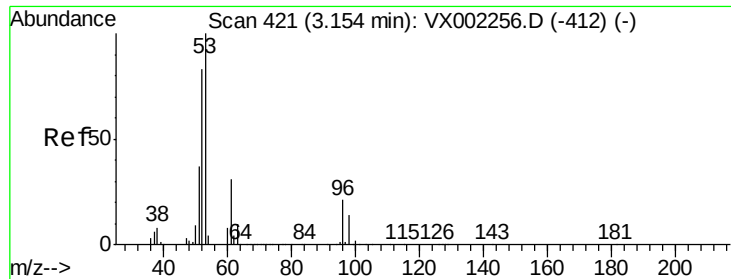

#15

Acrylonitrile

Concen: Below Cal

RT: 3.16 min Scan# 422

Delta R.T. 0.01 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49

Instrument :

MSVOA_X

ClientSampleId :

W-25





Tot Ion: 53 Resp: 157

Ion Ratio Lower Upper

53 100

52 108.9 66.7 100.1#

51 0.0 29.9 44.9#

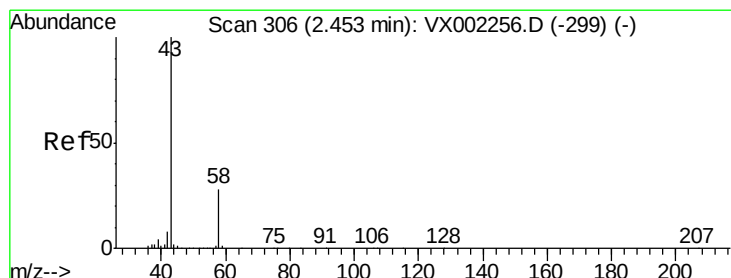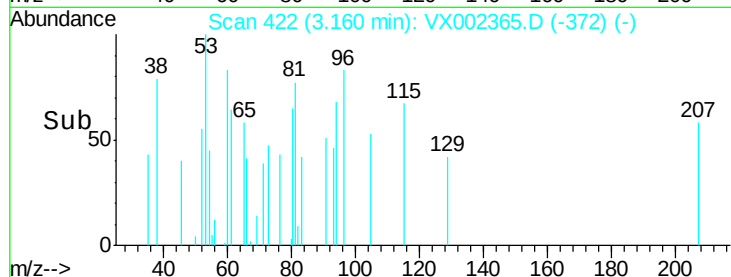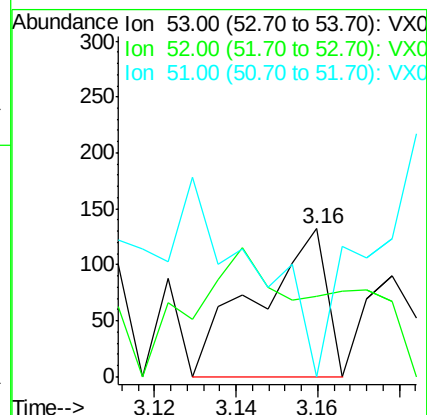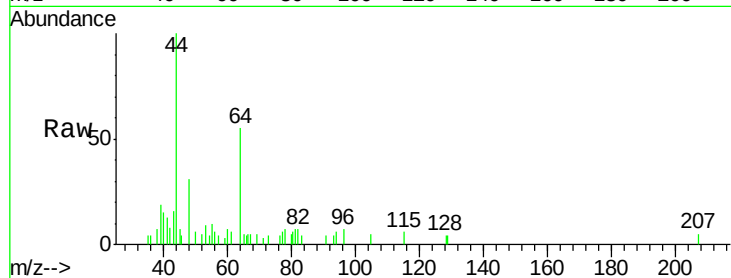

#16

Acetone

Concen: Below Cal

RT: 2.45 min Scan# 305

Delta R.T. -0.01 min

Lab File: VX002365.D




Acq: 06 Jun 2018 20:49


Tgt Ion: 43 Resp: 10352

Ion Ratio Lower Upper

43 100

58 23.6 22.1 33.1


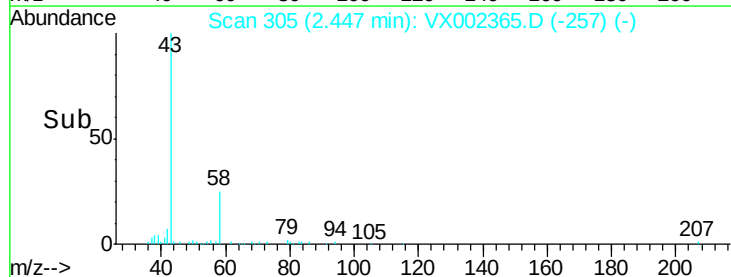
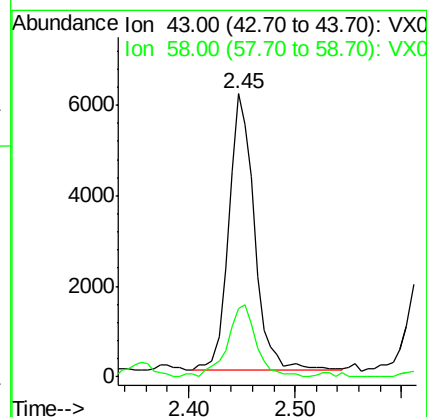
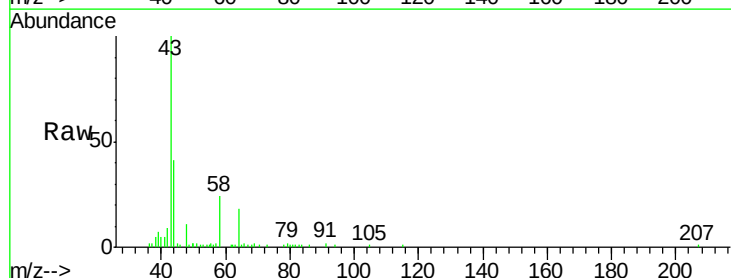


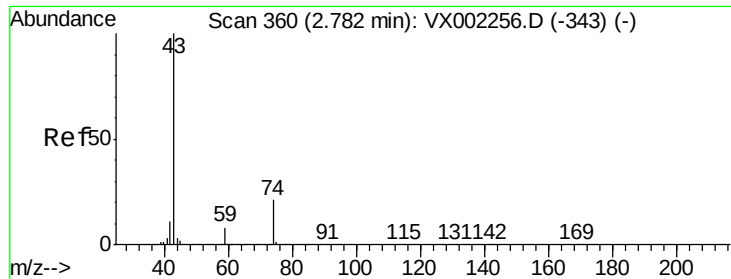

#18
Methyl Acetate
Concen: Below Cal
RT: 2.78 min Scan# 359
Delta R.T. -0.01 min
Lab File: VX002365.D
Acq: 06 Jun 2018 20:49




Instrument :
MSVOA_X
ClientSampled :
W-25


Tot Ion: 43 Resp: 243
Ion Ratio Lower Upper
43 100
74 28.8 16.7 25.1#

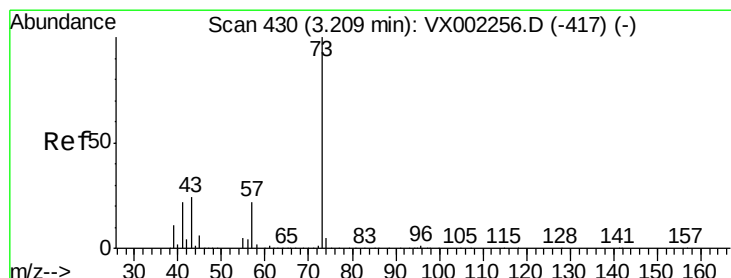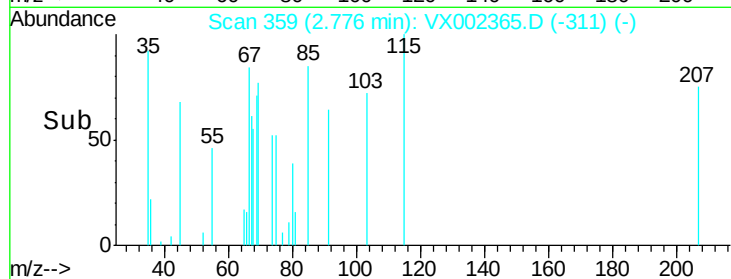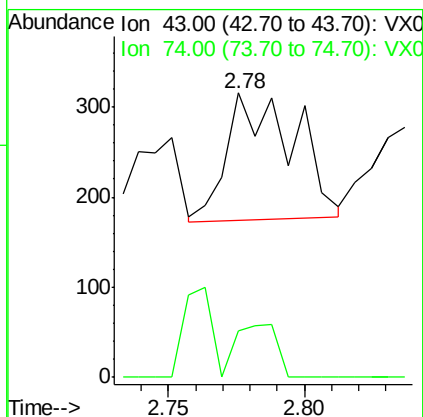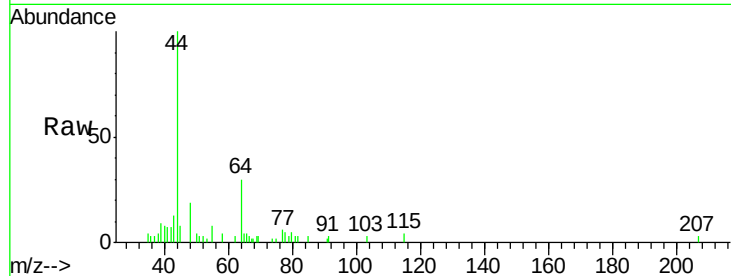

#19
Methyl tert-butyl Ether
Concen: Below Cal
RT: 3.21 min Scan# 430
Delta R.T. 0.00 min
Lab File: VX002365.D
Acq: 06 Jun 2018 20:49

Tgt Ion: 73 Resp: 4321
Ion Ratio Lower Upper
73 100
57 14.9 17.7 26.5#


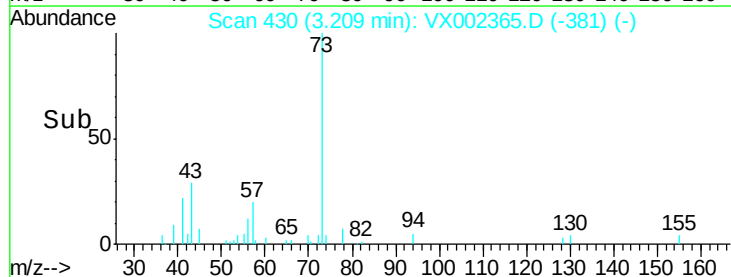
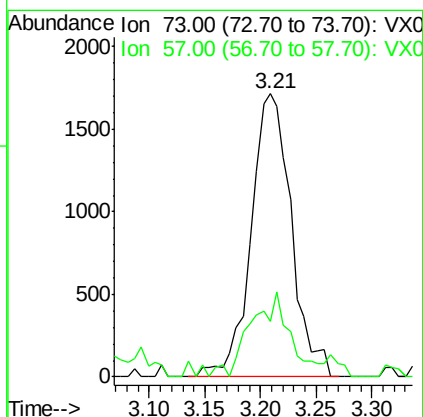
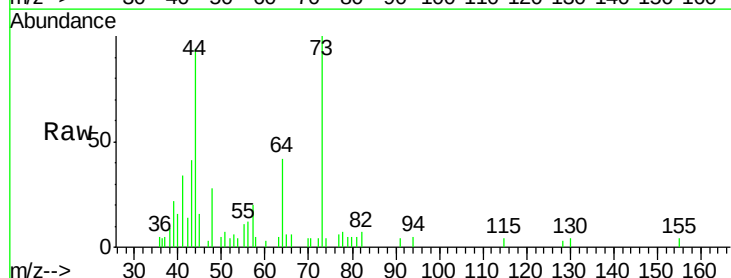


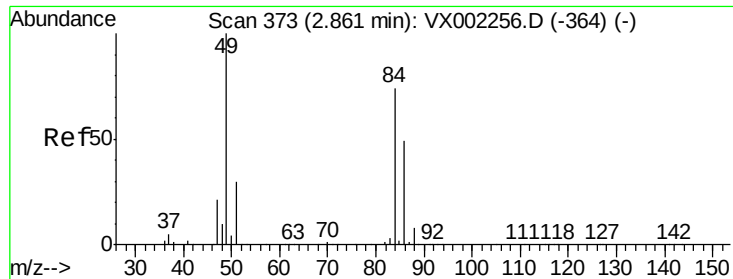

#20
Methvlene Chloride
Concen: Below Cal
RT: 2.86 min Scan# 372
Delta R.T. -0.01 min
Lab File: VX002365.D
Acq: 06 Jun 2018 20:49




Instrument :
MSVOA_X
ClientSampleId :
W-25


Tot Ion: 84 Resp: 883
Ion Ratio Lower Upper
84 100
49 133.3 107.8 161.6
51 36.5 32.8 49.2
86 78.0 52.5 78.7

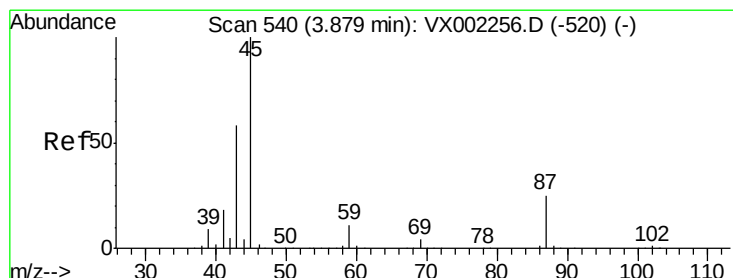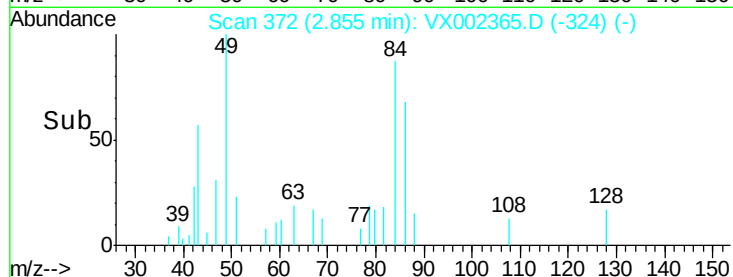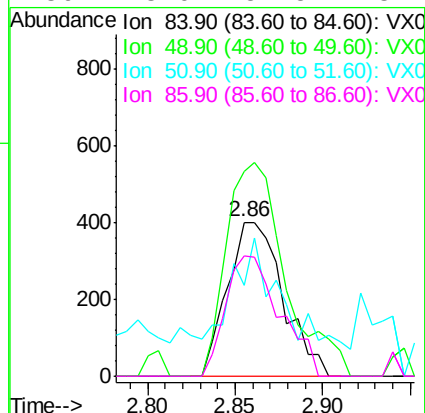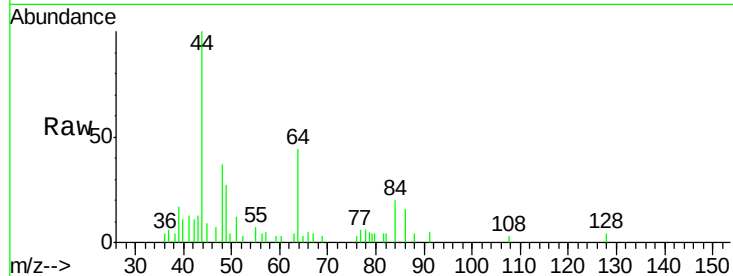

#22
Diisopropyl ether
Concen: Below Cal
RT: 3.86 min Scan# 537
Delta R.T. -0.02 min
Lab File: VX002365.D
Acq: 06 Jun 2018 20:49

Tgt Ion: 45 Resp: 120
Ion Ratio Lower Upper
45 100
43 0.0 46.8 70.2#
87 0.0 20.2 30.4#
59 0.0 8.7 13.1#

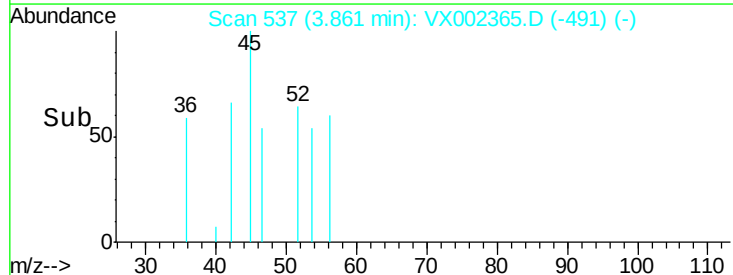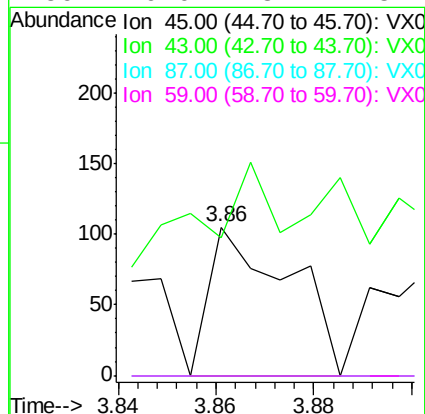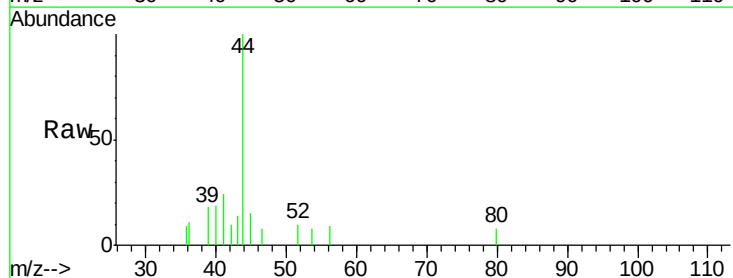

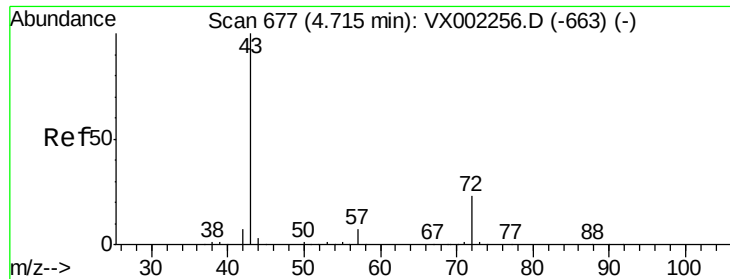

#25

2-Butanone

Concen: 0.22 ug/l

RT: 4.71 min Scan# 676

Delta R.T. -0.01 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49

Instrument :

MSVOA_X

ClientSampled :


W-25

Tot Ion: 43 Resp: 491

Ion Ratio Lower Upper




43 100

72 33.7 18.5 27.7#

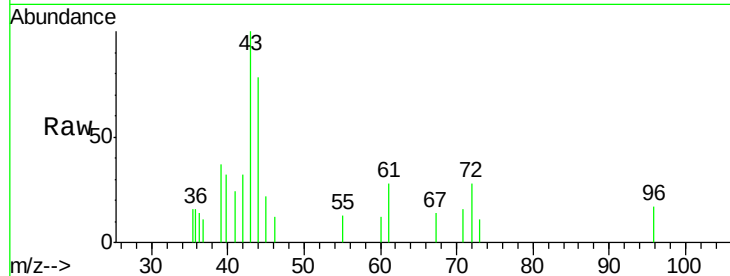

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

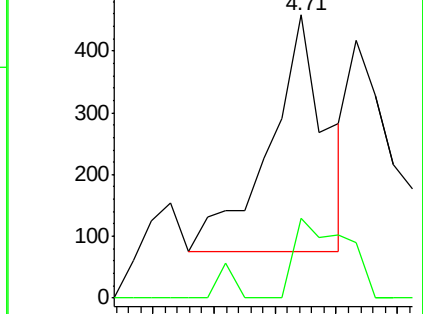

#28

Bromochloromethane

Concen: Below Cal

RT: 5.01 min Scan# 725

Delta R.T. -0.02 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49


Tgt Ion: 49 Resp: 26

Ion Ratio Lower Upper

49 100

129 0.0 0.0 4.2



130 0.0 61.2 91.8#




Abundance Ion 48.90 (48.60 to 49.60): VX0

Ion 128.80 (128.50 to 129.50): V

Ion 129.80 (129.50 to 130.50): V




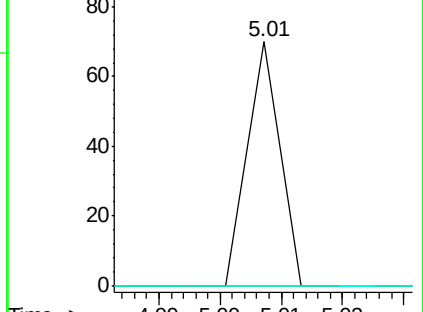


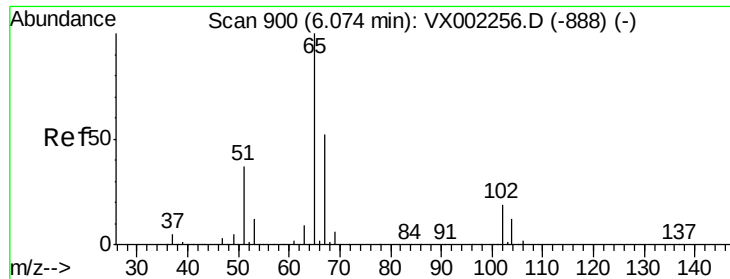

#33
 1,2-Dichloroethane-d4
 Concen: 47.75 ug/l
 RT: 6.07 min Scan# 900
 Delta R.T. -0.00 min
 Lab File: VX002365.D
 Acq: 06 Jun 2018 20:49




Instrument :
 MSVOA_X
 ClientSampleId :
 W-25


Tot Ion: 65 Resp: 157574
 Ion Ratio Lower Upper
 65 100
 67 51.9 0.0 102.6

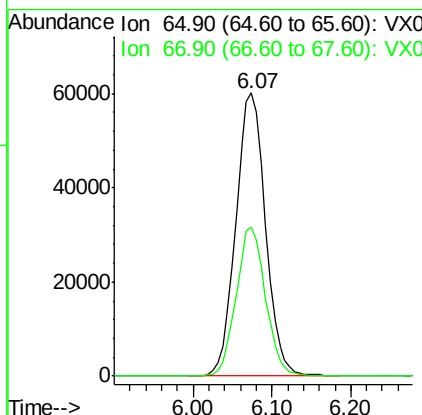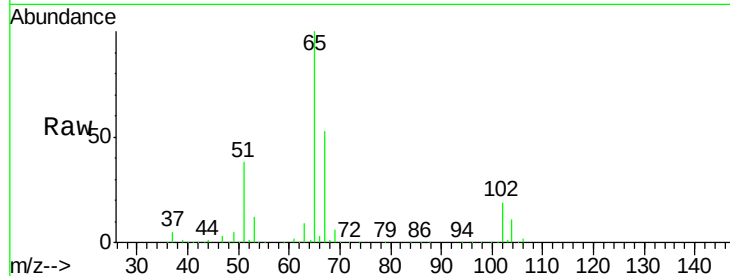

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.87 min Scan# 1030
 Delta R.T. -0.00 min
 Lab File: VX002365.D
 Acq: 06 Jun 2018 20:49

Tgt Ion: 114 Resp: 333791
 Ion Ratio Lower Upper
 114 100
 63 21.5 0.0 41.4
 88 15.2 0.0 30.0

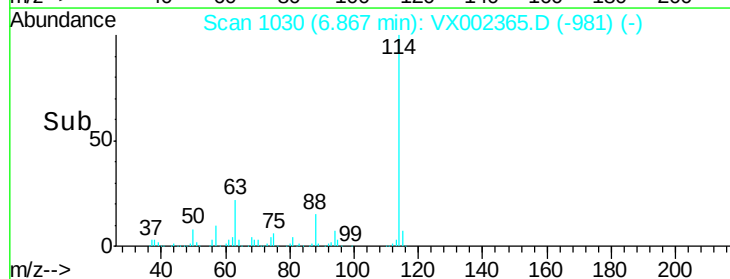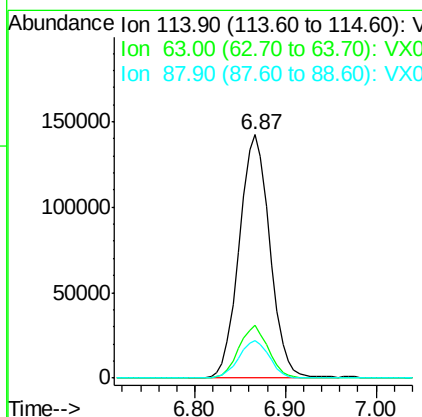

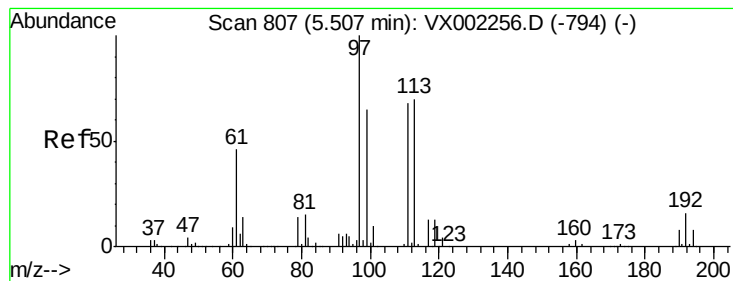

#35

Dibromofluoromethane

Concen: 44.89 ug/l

RT: 5.51 min Scan# 807

Delta R.T. -0.00 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49

Instrument :

MSVOA_X

ClientSampled :

W-25


Tot Ion:113 Resp: 117827

Ion Ratio Lower Upper

113 100

111 100.8 81.4 122.0




192 22.8 19.1 28.7

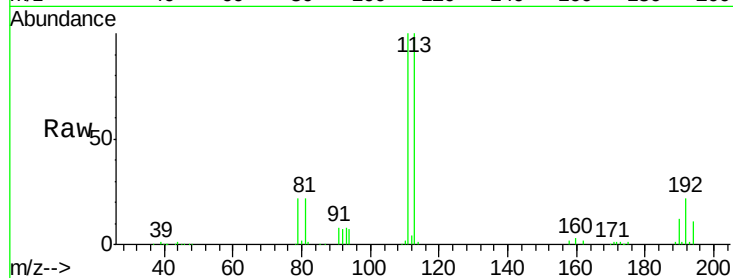

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

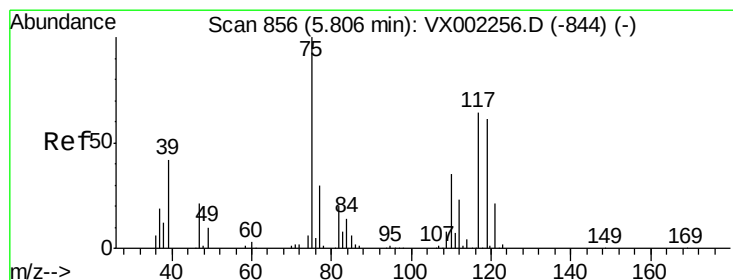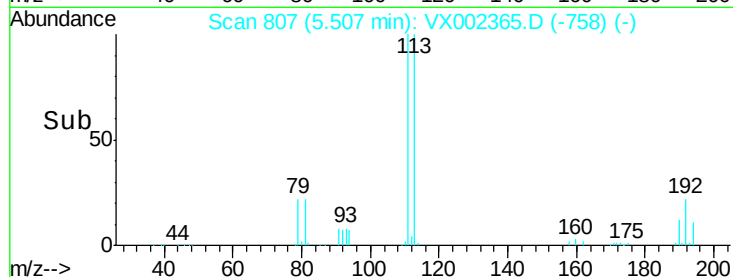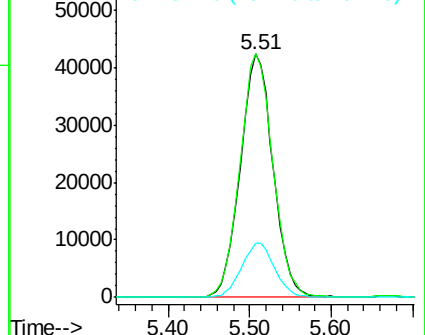

#36

1,1-Dichloropropene

Concen: 4.78 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.13 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49


Tgt Ion: 75 Resp: 16786

Ion Ratio Lower Upper

75 100

110 11.1 18.1 54.4#



77 0.0 24.3 36.5#

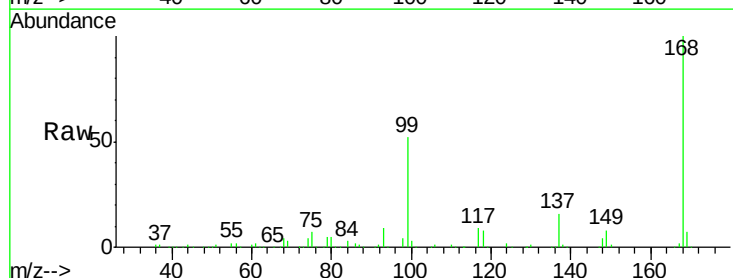


Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

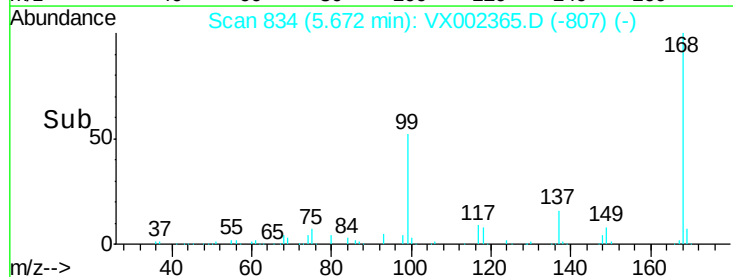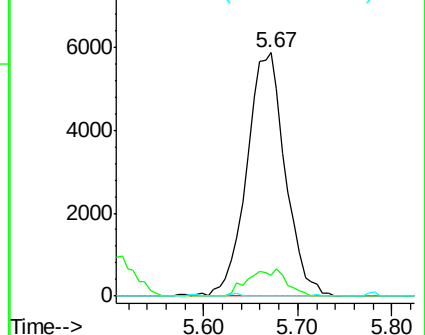



#38

Carbon Tetrachloride

Concen: 5.92 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.12 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49

Instrument :

MSVOA_X

ClientSampleId :

W-25


Tot Ion:117 Resp: 21723

Ion Ratio Lower Upper

117 100

119 5.0 77.4 116.0#




121 0.0 24.4 36.6#

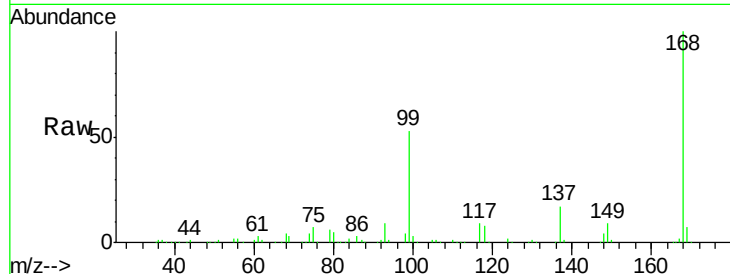

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

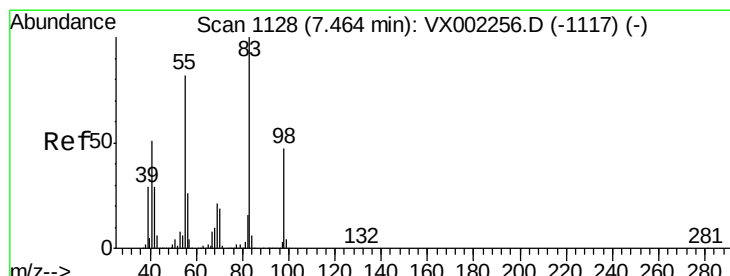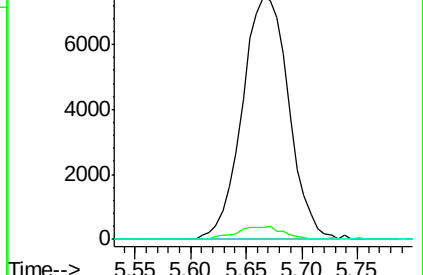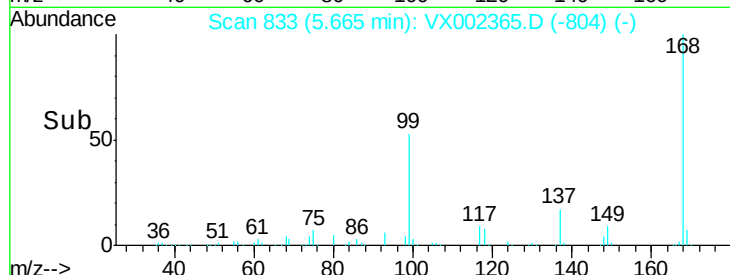

#39

Methylcyclohexane

Concen: 0.27 ug/l

RT: 7.48 min Scan# 1130

Delta R.T. 0.01 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49


Tgt Ion: 83 Resp: 49

Ion Ratio Lower Upper

83 100

55 0.0 65.4 98.0#



98 0.0 37.4 56.0#

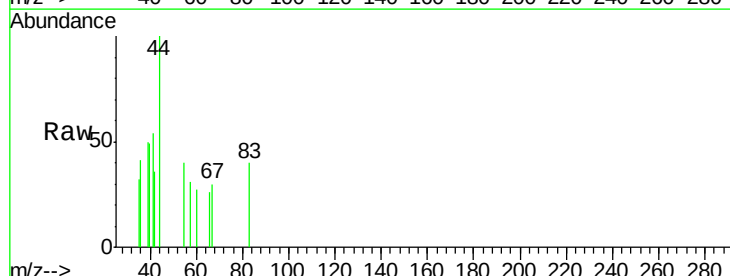


Abundance Ion 83.00 (82.70 to 83.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 98.00 (97.70 to 98.70): VX0

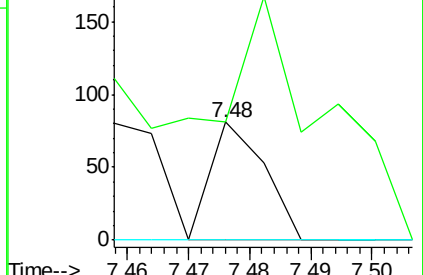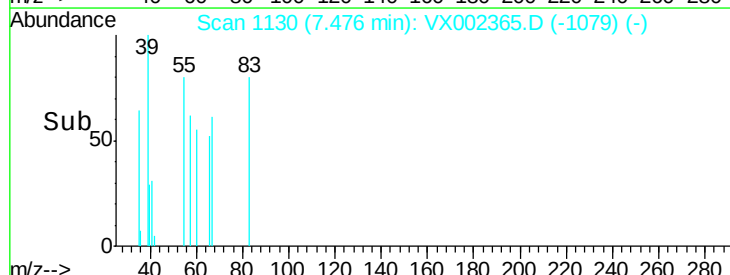

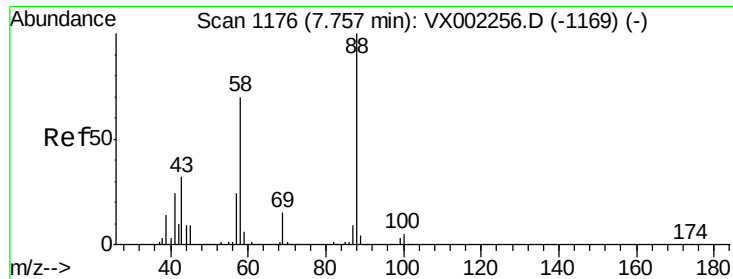

#49

1,4-Dioxane

Concen: 0.30 ug/l

RT: 7.64 min Scan# 1157

Delta R.T. -0.12 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49

Instrument :

MSVOA_X

ClientSampled :

W-25


Tot Ion: 88 Resp: 20

Ion Ratio Lower Upper

88 100

43 1510.0 29.8 44.6#




58 0.0 57.1 85.7#

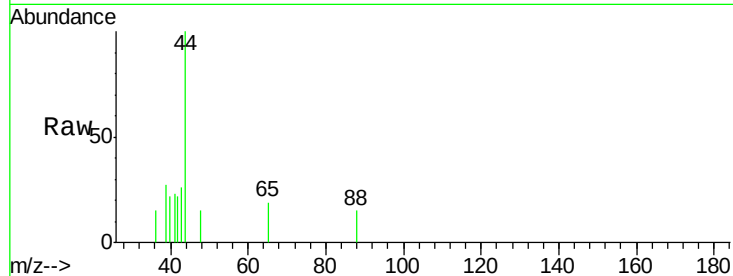

Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

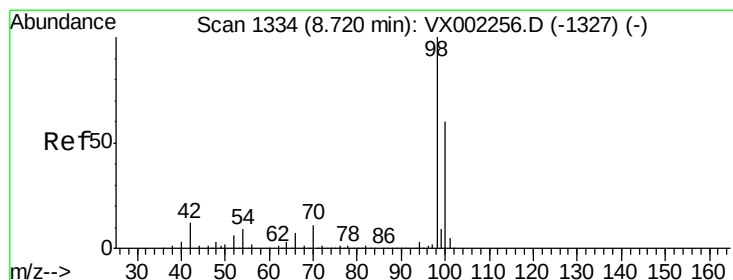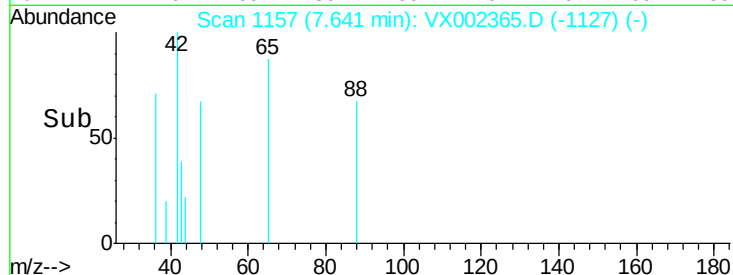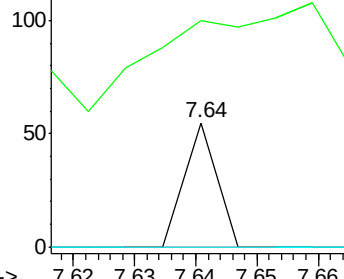

#50

Toluene-d8

Concen: 47.28 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. -0.00 min

Lab File: VX002365.D


Acq: 06 Jun 2018 20:49

Tgt Ion: 98 Resp: 475690

Ion Ratio Lower Upper



98 100


100 63.3 50.9 76.3

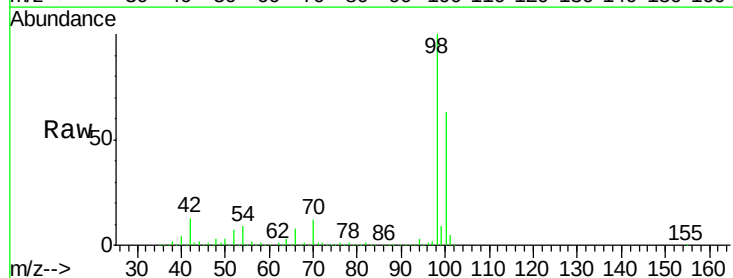

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

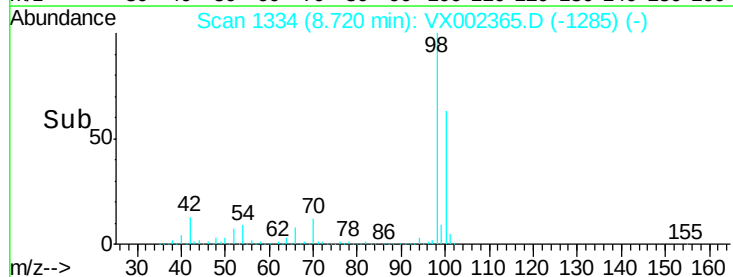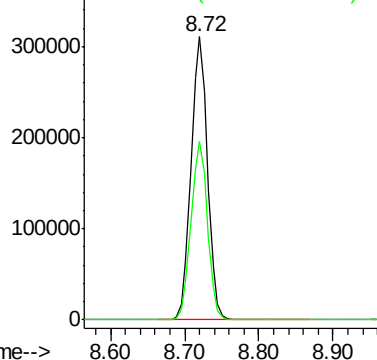



#62

4-Bromofluorobenzene

Concen: 42.74 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.00 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49

Instrument :

MSVOA_X

ClientSampleId :

W-25


Tot Ion: 95 Resp: 165835

Ion Ratio Lower Upper

95 100

174 93.3 0.0 187.4




176 91.4 0.0 181.0

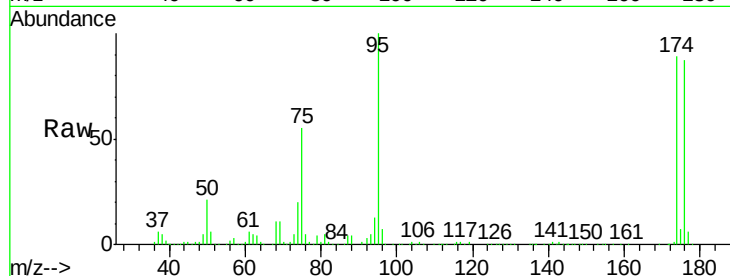

Abundance Ion 94.90 (94.60 to 95.60): VX002256.D (-1724) (-)

Ion 173.80 (173.50 to 174.50): VX002256.D (-1724) (-)

Ion 175.80 (175.50 to 176.50): VX002256.D (-1724) (-)

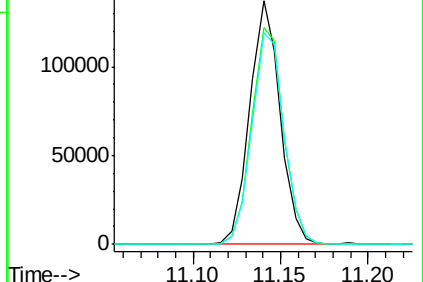

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 10.12 min Scan# 1563

Delta R.T. -0.00 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49


Tgt Ion: 117 Resp: 302240

Ion Ratio Lower Upper

117 100

82 55.2 45.0 67.4



119 32.5 25.8 38.6




Abundance Ion 116.90 (116.60 to 117.60): VX002256.D (-1555) (-)

Ion 82.00 (81.70 to 82.70): VX002256.D (-1555) (-)

Ion 118.90 (118.60 to 119.60): VX002256.D (-1555) (-)



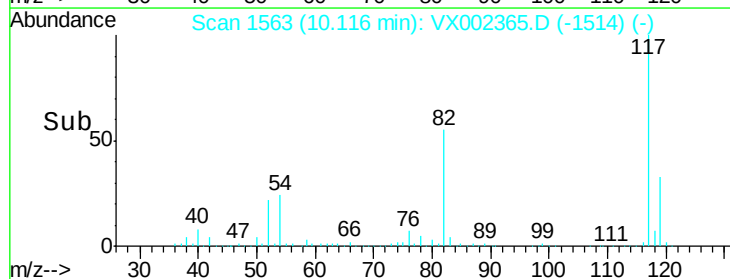
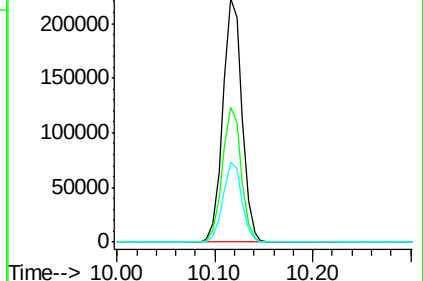


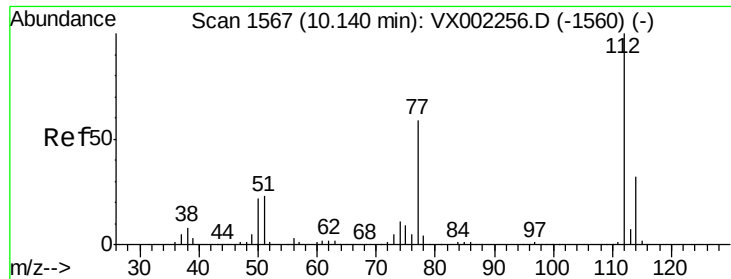

#65
Chlorobenzene
Concen: 0.25 ug/l
RT: 10.14 min Scan# 1567
Delta R.T. -0.00 min
Lab File: VX002365.D
Acq: 06 Jun 2018 20:49




Instrument :
MSVOA_X
ClientSampled :
W-25


Tot Ion:112 Resp: 1902
Ion Ratio Lower Upper
112 100
114 36.2 25.3 37.9

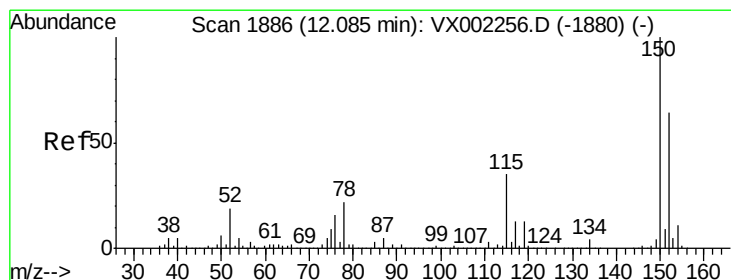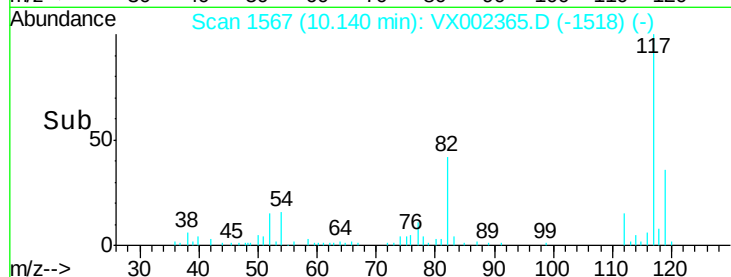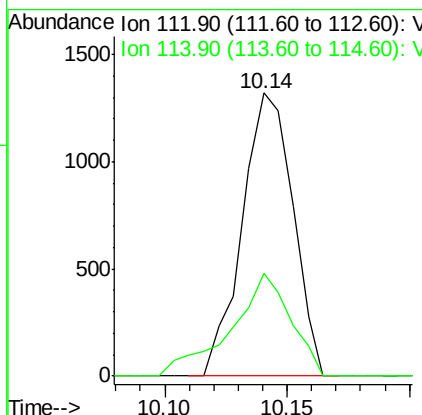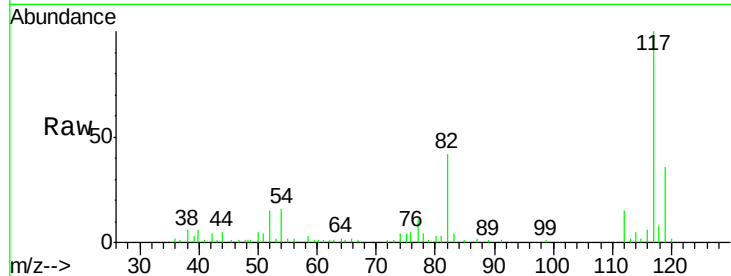

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.09 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX002365.D
Acq: 06 Jun 2018 20:49

Tgt Ion:152 Resp: 170222
Ion Ratio Lower Upper
152 100
115 54.9 40.1 120.2
150 155.0 0.0 347.2


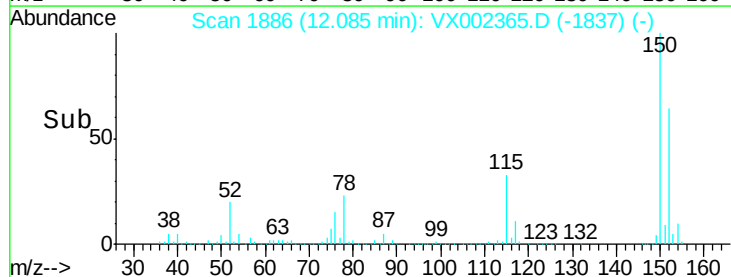
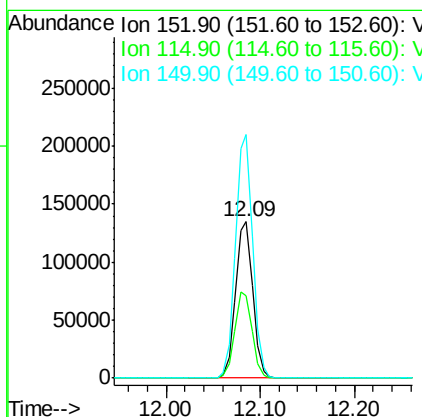
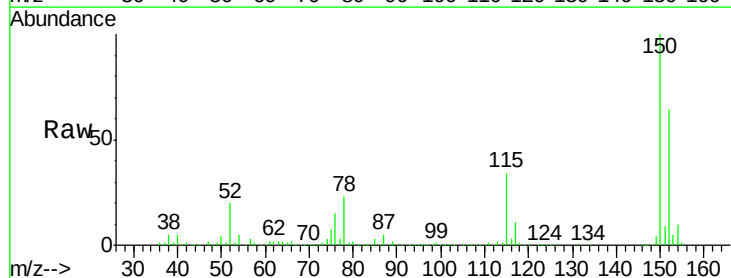




#76
 1,2,3-Trichloropropane
 Concen: 24.13 ug/l
 RT: 11.14 min Scan# 1731
 Delta R.T. -0.16 min
 Lab File: VX002365.D
 Acq: 06 Jun 2018 20:49




Instrument :
 MSVOA_X
 ClientSampled :
 W-25


Tot Ion: 75 Resp: 90124
 Ion Ratio Lower Upper
 75 100
 77 1.4 22.8 68.3#

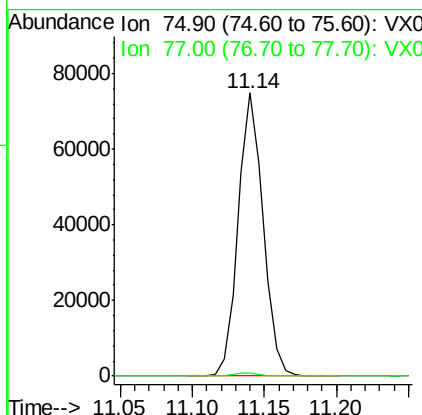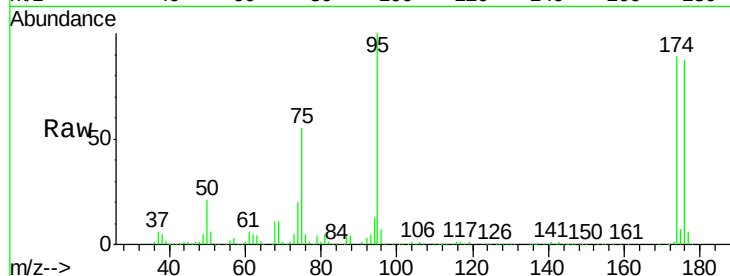

#81
 trans-1,4-Dichloro-2-butene
 Concen: 84.58 ug/l
 RT: 11.14 min Scan# 1731
 Delta R.T. 0.06 min
 Lab File: VX002365.D
 Acq: 06 Jun 2018 20:49

Tgt Ion: 75 Resp: 90124
 Ion Ratio Lower Upper
 75 100
 53 0.1 86.8 130.2#
 89 0.1 38.2 57.2#



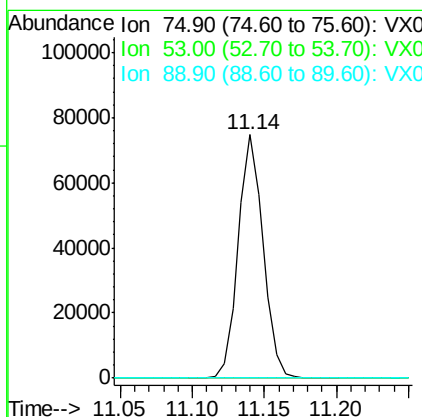



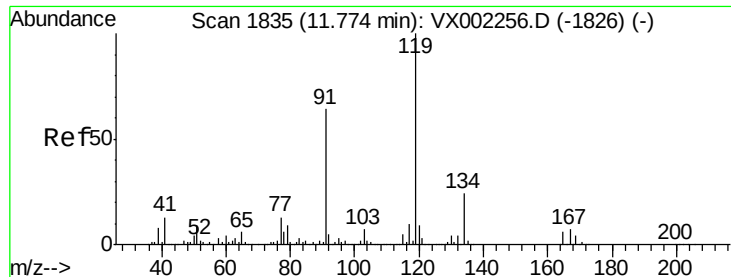

#83
tert-Butylbenzene
Concen: 0.40 ug/l
RT: 11.77 min Scan# 1835
Delta R.T. -0.00 min
Lab File: VX002365.D
Acq: 06 Jun 2018 20:49




Instrument :
MSVOA_X
ClientSampled :
W-25


Tot Ion:119 Resp: 3928
Ion Ratio Lower Upper
119 100
91 73.5 30.3 90.9
134 24.0 11.7 35.1

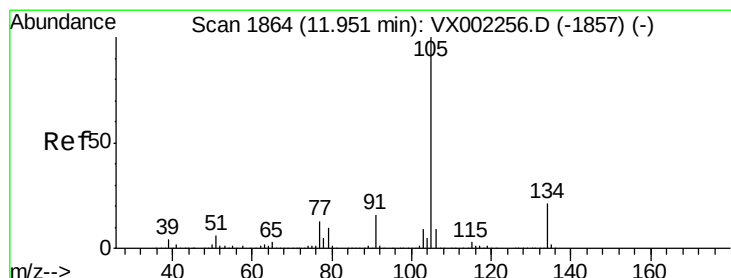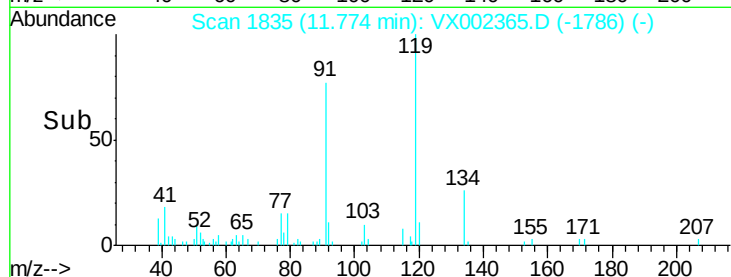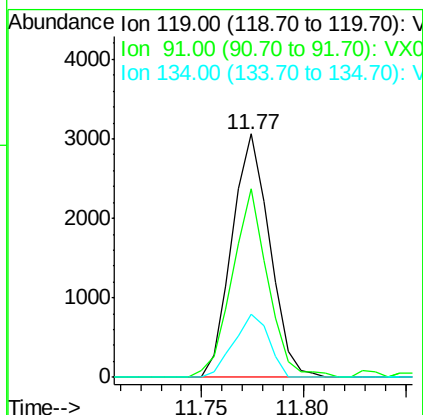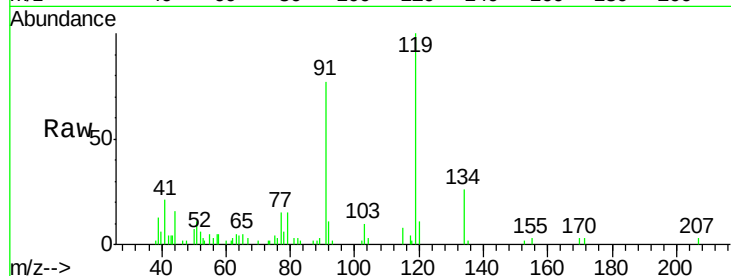

#85
sec-Butylbenzene
Concen: 0.25 ug/l
RT: 11.95 min Scan# 1864
Delta R.T. -0.00 min
Lab File: VX002365.D
Acq: 06 Jun 2018 20:49

Tgt Ion:105 Resp: 2891
Ion Ratio Lower Upper
105 100
134 33.7 10.4 31.1#

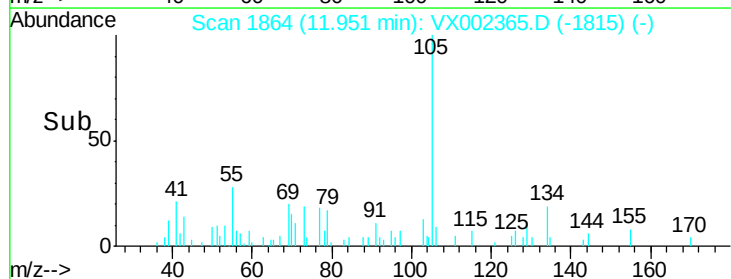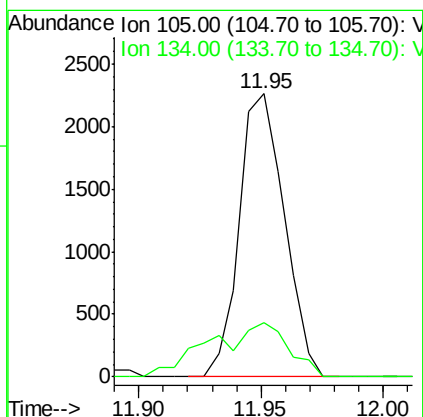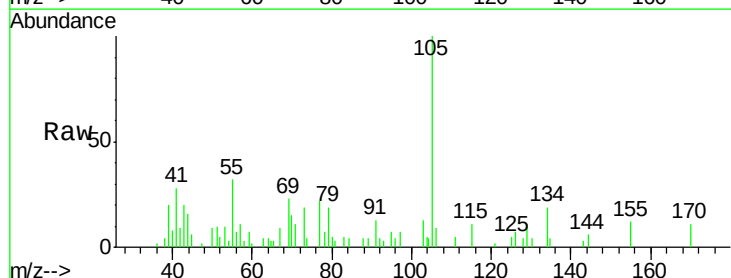



#90

Hexachloroethane

Concen: 0.28 ug/l

RT: 12.66 min Scan# 1981

Delta R.T. 0.06 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49

Instrument :

MSVOA_X

ClientSampled :


W-25

Tot Ion:117 Resp: 464

Ion Ratio Lower Upper




117 100

201 0.0 49.0 147.0#

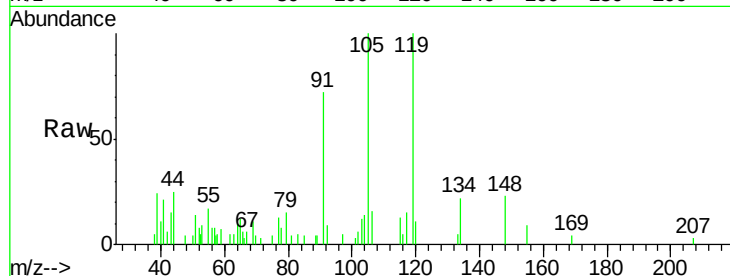

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 200.70 (200.40 to 201.40): V

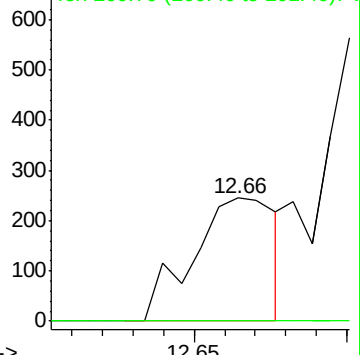

#91

1,2-Dichlorobenzene

Concen: 0.30 ug/l

RT: 12.40 min Scan# 1937

Delta R.T. -0.00 min

Lab File: VX002365.D

Acq: 06 Jun 2018 20:49


Tgt Ion:146 Resp: 1866

Ion Ratio Lower Upper

146 100

111 47.4 19.4 58.1

148 59.4 31.7 95.1



Abundance Ion 145.90 (145.60 to 146.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 147.90 (147.60 to 148.60): V

