


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX060618\
Data File : VX002342.D
Acq On : 06 Jun 2018 09:33
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Title : SW846 8260
Last Update : Tue Jun 05 03:22:35 2018

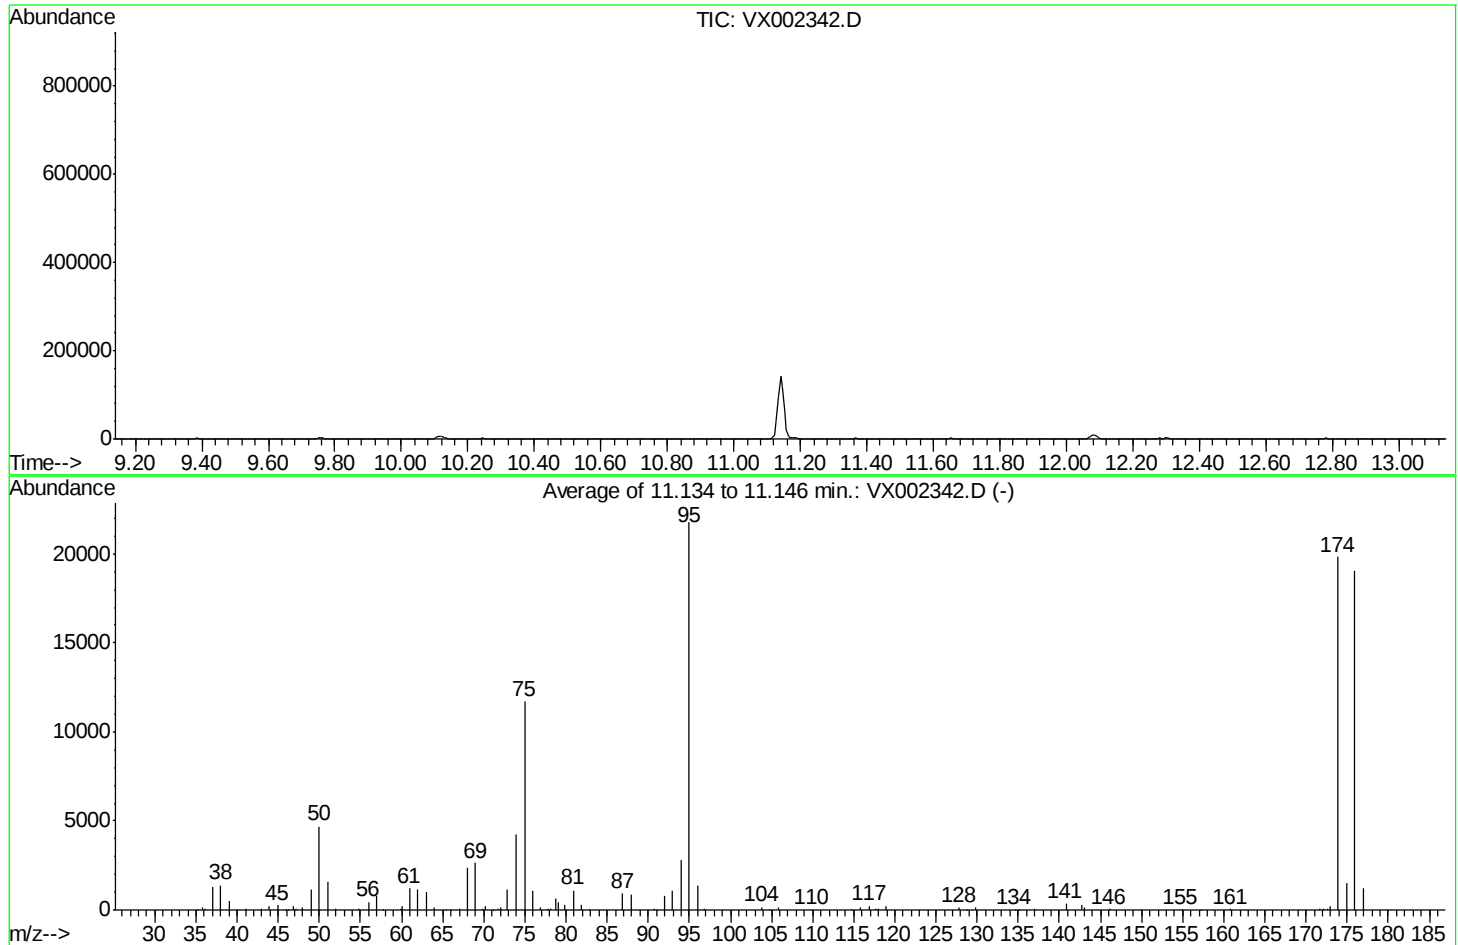

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	4702	PASS
75	95	30	60	53.7	11692	PASS
95	95	100	100	100.0	21770	PASS
96	95	5	9	6.3	1382	PASS
173	174	0.00	2	1.1	224	PASS
174	95	50	100	91.1	19835	PASS
175	174	5	9	7.8	1544	PASS
176	174	95	101	96.1	19067	PASS
177	176	5	9	6.5	1246	PASS