

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX060718\
 Data File : VX002374.D
 Acq On : 07 Jun 2018 13:41
 Operator : JC/MD
 Sample : J3340-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 LF5-FB-2018-1

Quant Time: Jun 07 15:13:39 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 05 03:22:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	244868	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	354004	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	325366	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	184882	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.07	65	187998	53.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.92%	
35) Dibromofluoromethane	5.51	113	142113	51.05	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.10%	
50) Toluene-d8	8.72	98	562346	52.70	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.40%	
62) 4-Bromofluorobenzene	11.14	95	199531	48.49	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.98%	

Target Compounds


					Qvalue	
3) Chloromethane	1.33	50	821	Below Cal	#	44
4) Vinyl Chloride	1.41	62	2978	0.928	ug/l	90
5) Bromomethane	1.65	94	730	Below Cal		98
6) Chloroethane	1.65	64	2276	1.097	ug/l #	43
8) Diethyl Ether	2.19	74	174	Below Cal		60
10) Methyl Iodide	2.53	142	2176	0.587	ug/l	95
11) Tert butyl alcohol	3.07	59	1251	Below Cal	#	48
13) Acrolein	2.28	56	106	Below Cal	#	57
14) Allyl chloride	2.62	41	2567	0.454	ug/l #	64
15) Acrylonitrile	3.15	53	944	Below Cal	#	77
16) Acetone	2.45	43	20691	Below Cal		94
17) Carbon Disulfide	2.57	76	1528	0.222	ug/l #	72
18) Methyl Acetate	2.78	43	1773	Below Cal	#	83
19) Methyl tert-butyl Ether	3.21	73	325	Below Cal	#	54
20) Methylene Chloride	2.86	84	499134	187.898	ug/l	99
22) Diisopropyl ether	3.87	45	77	Below Cal	#	38
25) 2-Butanone	4.71	43	68268	28.434	ug/l	98
28) Bromochloromethane	5.02	49	275	Below Cal	#	22
29) Tetrahydrofuran	5.17	42	2628356	1697.940	ug/l	100
36) 1,1-Dichloropropene	5.67	75	17636	4.739	ug/l #	51
37) Ethyl Acetate	4.71	43	68268	15.253	ug/l #	70
38) Carbon Tetrachloride	5.67	117	23237	5.968	ug/l #	15
39) Methylcyclohexane	7.46	83	79	0.280	ug/l #	67
41) Methacrylonitrile	5.17	41	1512890	590.491	ug/l #	50
52) Toluene	8.79	92	1473	0.203	ug/l	97
67) Ethyl Benzene	10.26	91	4998	0.369	ug/l	99
76) 1,2,3-Trichloropropane	11.14	75	105489	26.003	ug/l #	33
81) trans-1,4-Dichloro-2-buten	11.14	75	105489	91.150	ug/l #	7
84) 1,2,4-Trimethylbenzene	11.81	105	2719	0.239	ug/l #	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX060718\
Data File : VX002374.D
Acq On : 07 Jun 2018 13:41
Operator : JC/MD
Sample : J3340-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LF5-FB-2018-1

Quant Time: Jun 07 15:13:39 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 05 03:22:35 2018
Response via : Initial Calibration

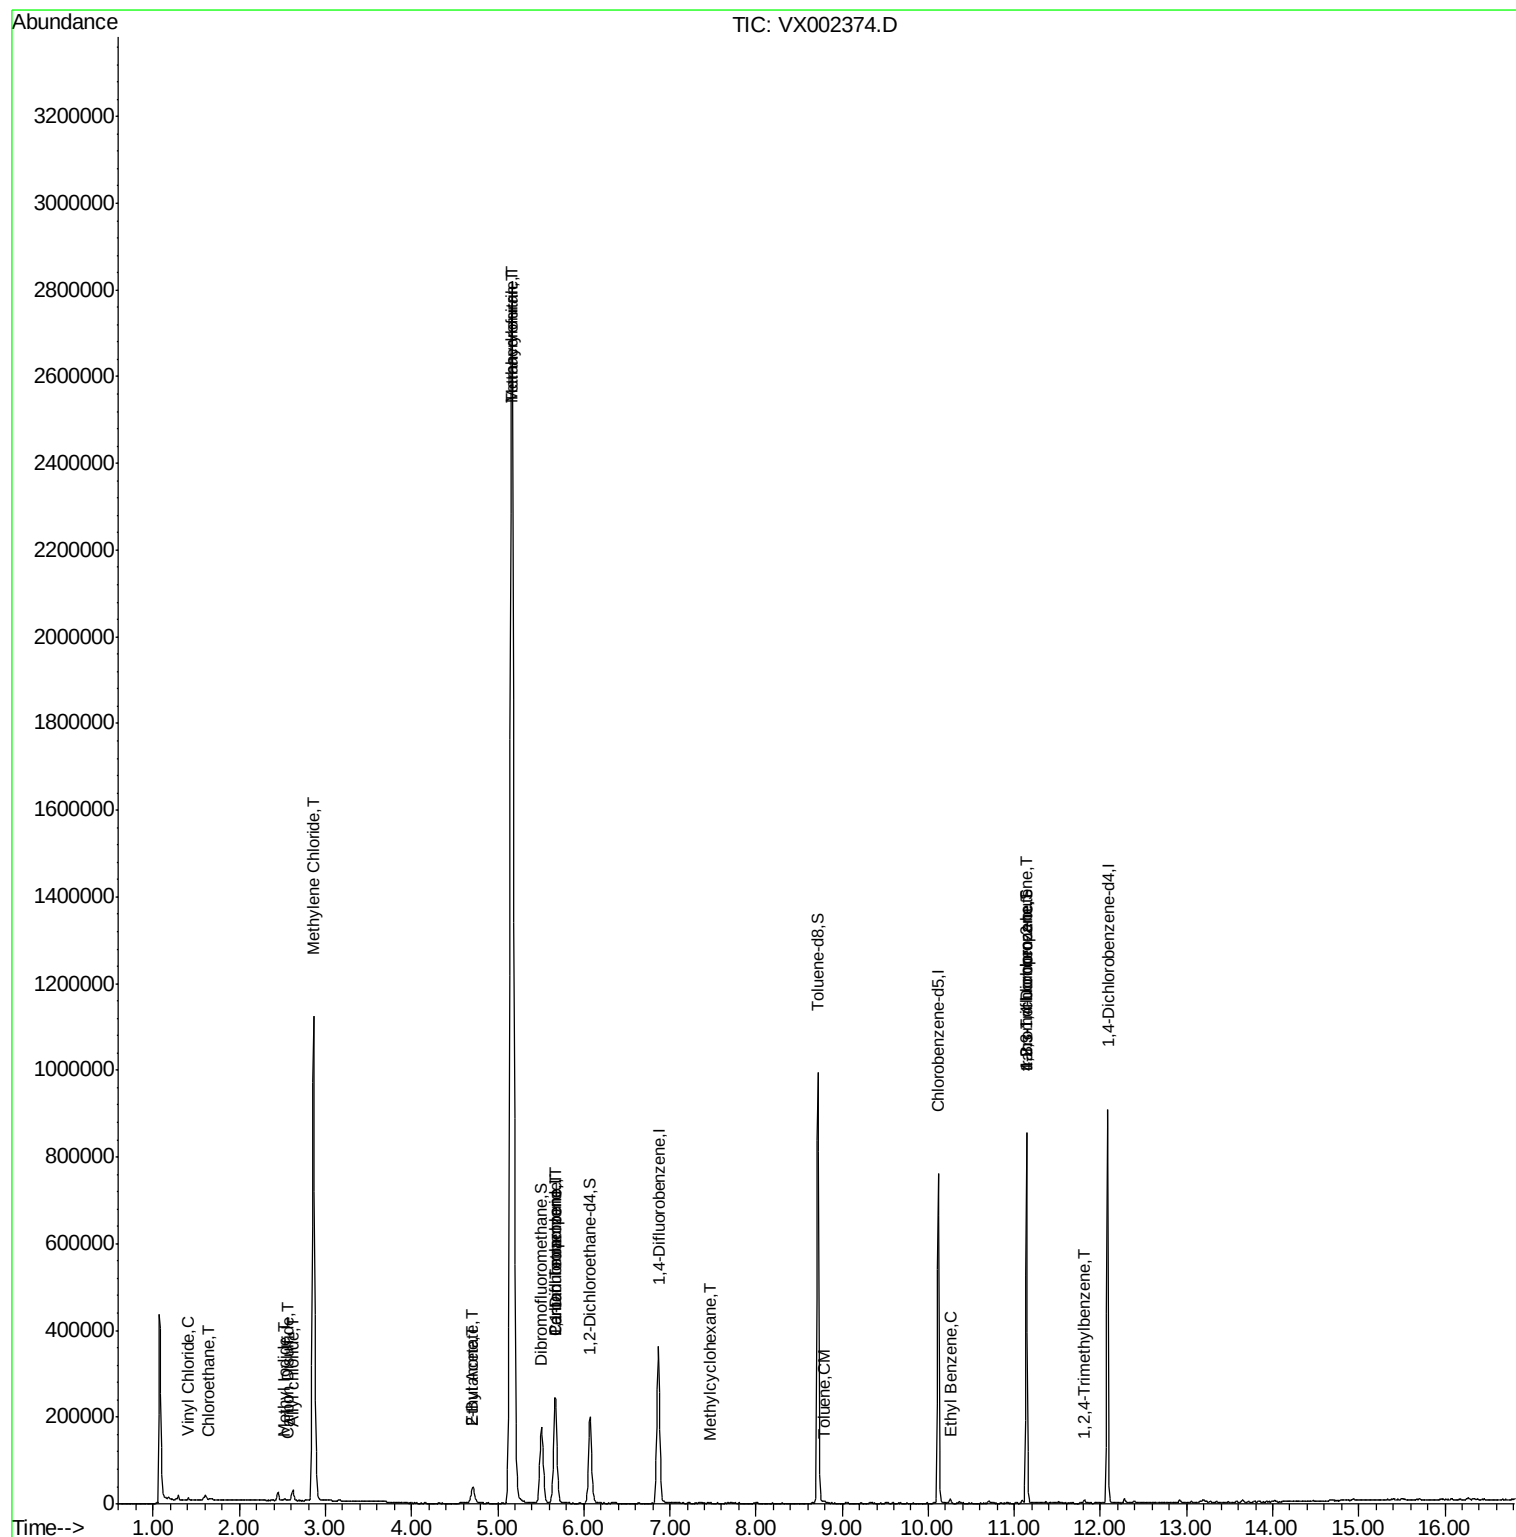



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.00 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41

Instrument :

MSVOA_X

ClientSampleId :


LF5-FB-2018-1

Tot Ion:168 Resp: 244868

Ion Ratio Lower Upper

168 100

99 50.7 39.3 58.9

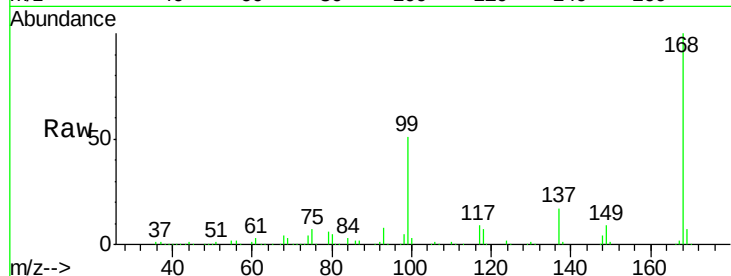

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80



#3

Chloromethane

Concen: Below Cal

RT: 1.33 min Scan# 122

Delta R.T. 0.01 min

Lab File: VX002374.D


Acq: 07 Jun 2018 13:41

Tgt Ion: 50 Resp: 821

Ion Ratio Lower Upper

50 100

52 63.5 25.7 38.5#



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.33

500

400


300


200

100

0

Time--> 1.30 1.35 1.40





#4

Vinyl Chloride

Concen: 0.928 ug/l

RT: 1.41 min Scan# 135

Delta R.T. -0.00 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41

Instrument :

MSVOA_X

ClientSampleId :





LF5-FB-2018-1

Tot Ion: 62 Resp: 2978

Ion Ratio Lower Upper

62 100

64 26.4 25.4 38.2

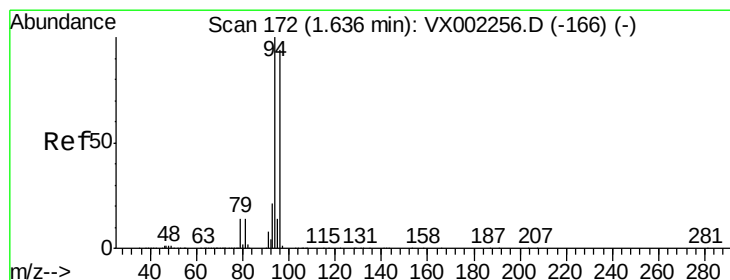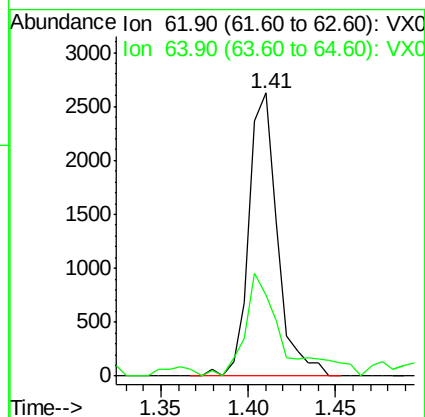

#5

Bromomethane

Concen: Below Cal

RT: 1.65 min Scan# 174

Delta R.T. 0.01 min

Lab File: VX002374.D




Acq: 07 Jun 2018 13:41


Tgt Ion: 94 Resp: 730

Ion Ratio Lower Upper

94 100

96 91.3 74.9 112.3

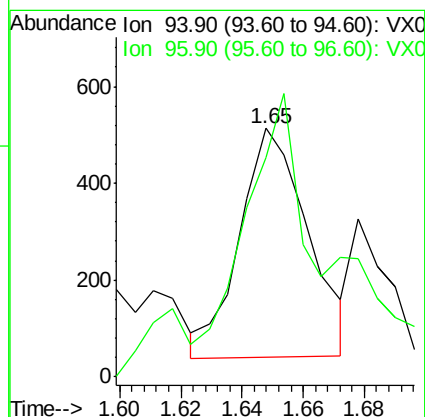



#6

Chloroethane

Concen: 1.097 ug/l

RT: 1.65 min Scan# 175

Delta R.T. -0.07 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41

Instrument :

MSVOA_X

ClientSampleId :





LF5-FB-2018-1

Tot Ion: 64 Resp: 2276

Ion Ratio Lower Upper

64 100

66 0.3 25.5 38.3#

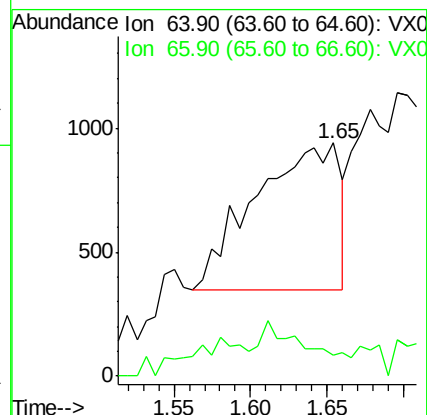

#8

Diethyl Ether

Concen: Below Cal

RT: 2.19 min Scan# 263

Delta R.T. 0.00 min

Lab File: VX002374.D




Acq: 07 Jun 2018 13:41


Tgt Ion: 74 Resp: 174

Ion Ratio Lower Upper

74 100

45 147.7 53.1 159.4



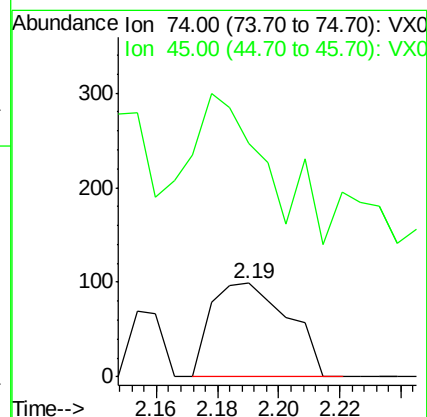





#10
Methvl Iodide
Concen: 0.587 ug/l
RT: 2.53 min Scan# 319
Delta R.T. 0.02 min
Lab File: VX002374.D
Acq: 07 Jun 2018 13:41




Instrument :
MSVOA_X
ClientSampled :
LF5-FB-2018-1


Tot Ion:142 Resp: 2176
Ion Ratio Lower Upper
142 100
127 49.4 36.6 55.0
141 16.1 11.3 16.9

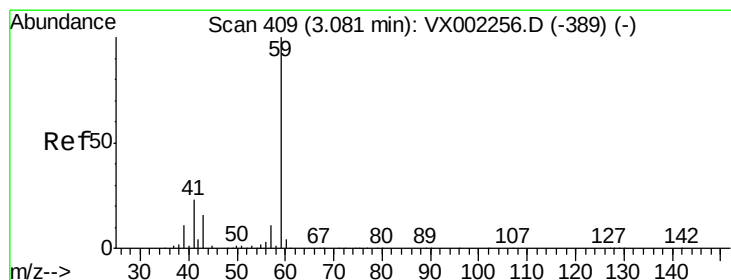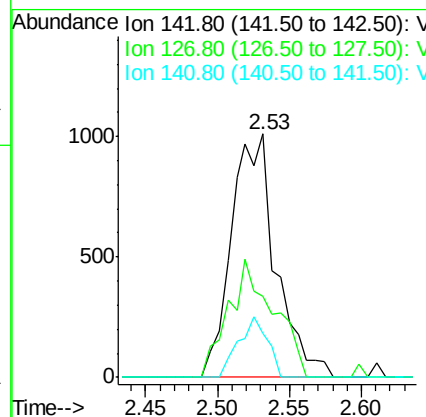

#11
Tert butyl alcohol
Concen: Below Cal
RT: 3.07 min Scan# 408
Delta R.T. -0.01 min
Lab File: VX002374.D
Acq: 07 Jun 2018 13:41

Tgt Ion: 59 Resp: 1251
Ion Ratio Lower Upper
59 100
57 29.6 8.2 12.2#

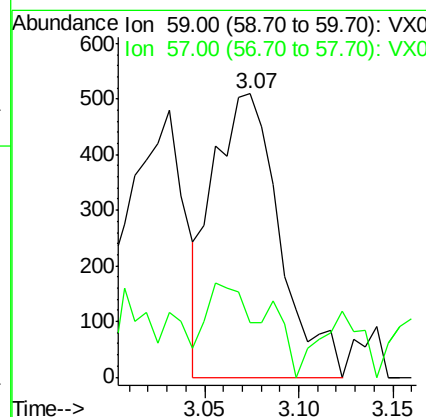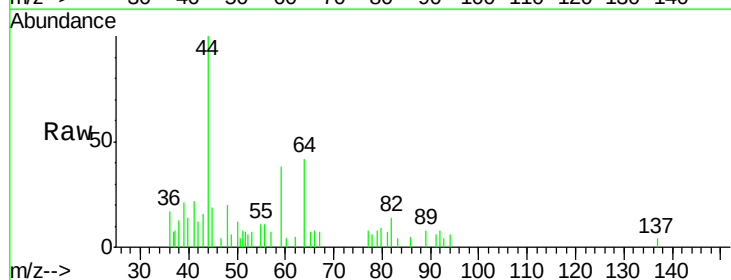

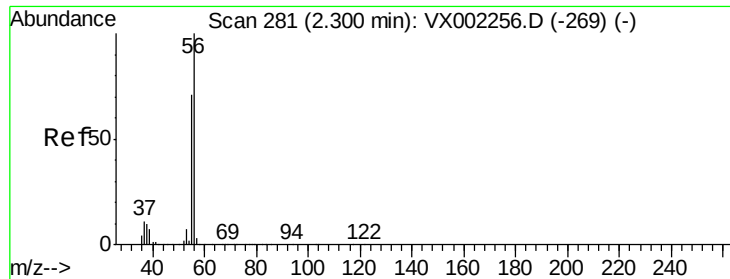

#13

Acrolein

Concen: Below Cal

RT: 2.28 min Scan# 278

Delta R.T. -0.02 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41

Instrument :

MSVOA_X

ClientSampleId :





LF5-FB-2018-1

Tot Ion: 56 Resp: 106

Ion Ratio Lower Upper

56 100

55 35.8 57.0 85.4#

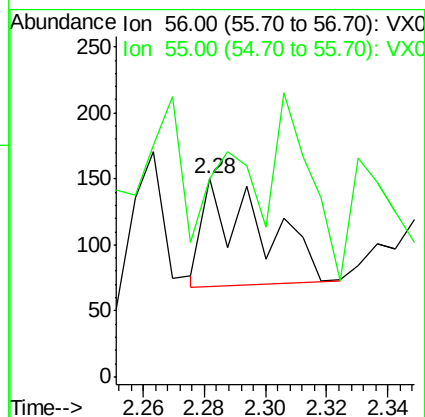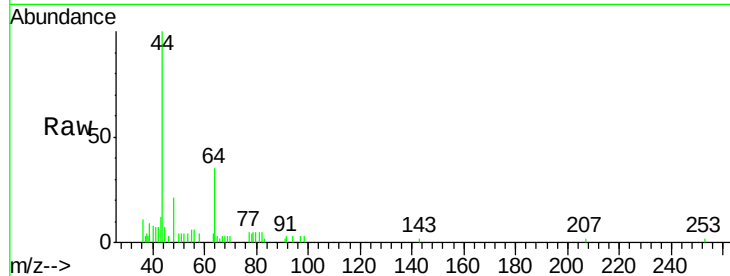

#14

Allyl chloride

Concen: 0.454 ug/l

RT: 2.62 min Scan# 334

Delta R.T. -0.10 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41




Tgt Ion: 41 Resp: 2567


Ion Ratio Lower Upper

41 100

39 94.5 56.8 85.2#

76 0.0 23.8 35.8#

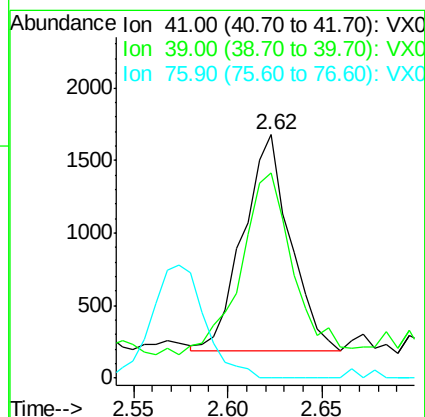



#15

Acrylonitrile

Concen: Below Cal

RT: 3.15 min Scan# 421

Delta R.T. 0.00 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41

Instrument :

MSVOA_X

ClientSampled :

LF5-FB-2018-1





Tot Ion: 53 Resp: 944

Ion Ratio Lower Upper

53 100

52 88.0 66.7 100.1

51 0.0 29.9 44.9#

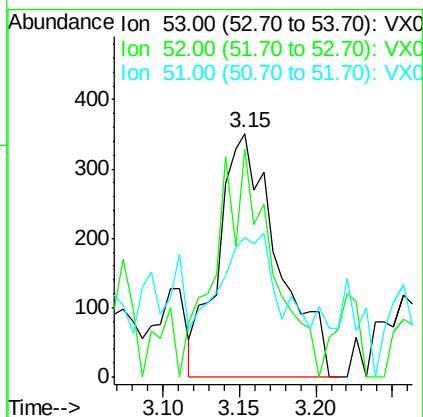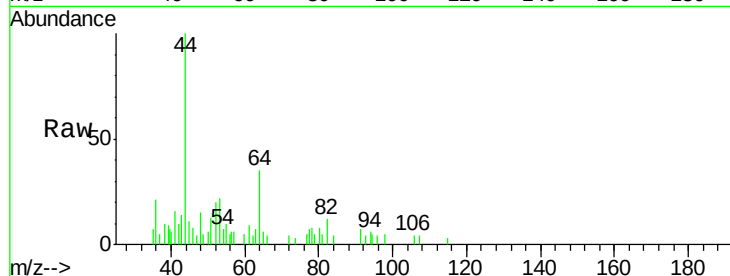

#16

Acetone

Concen: Below Cal

RT: 2.45 min Scan# 306

Delta R.T. 0.00 min

Lab File: VX002374.D




Acq: 07 Jun 2018 13:41


Tgt Ion: 43 Resp: 20691

Ion Ratio Lower Upper

43 100

58 30.9 22.1 33.1

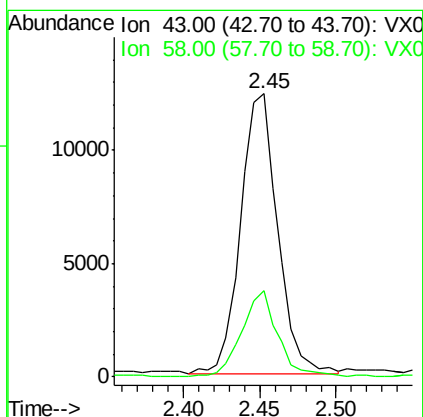



#17

Carbon Disulfide

Concen: 0.222 ug/l

RT: 2.57 min Scan# 326

Delta R.T. 0.01 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41

Instrument :

MSVOA_X

ClientSampleId :


LF5-FB-2018-1

Tot Ion: 76 Resp: 1528

Ion Ratio Lower Upper




76 100

78 18.6 6.9 10.3#

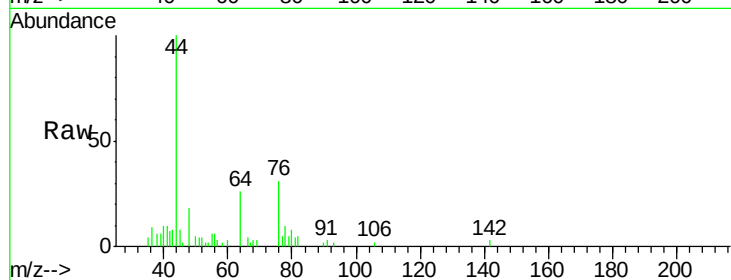

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

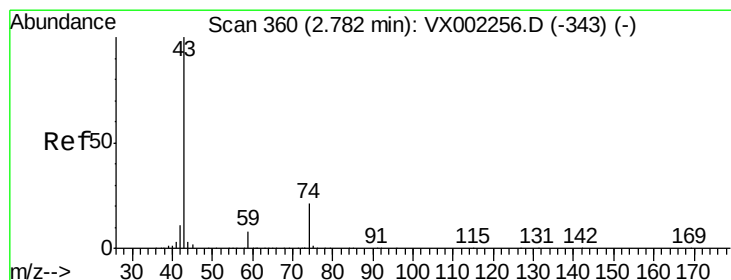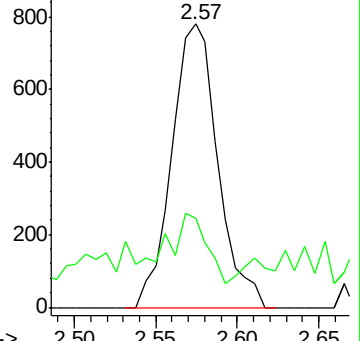

#18

Methyl Acetate

Concen: Below Cal

RT: 2.78 min Scan# 359

Delta R.T. -0.01 min

Lab File: VX002374.D


Acq: 07 Jun 2018 13:41

Tgt Ion: 43 Resp: 1773

Ion Ratio Lower Upper



43 100


74 28.8 16.7 25.1#

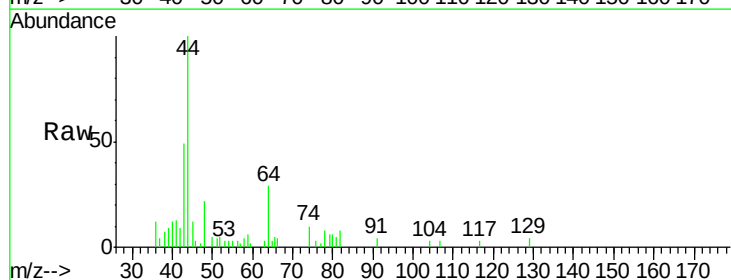

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0




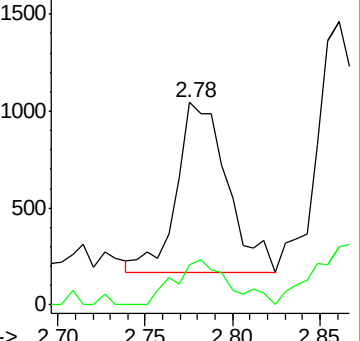


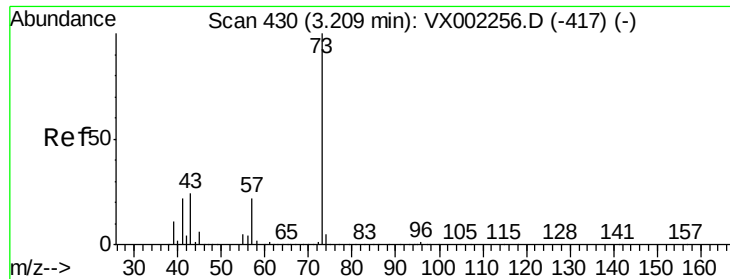

#19
Methyl tert-butyl Ether
Concen: Below Cal
RT: 3.21 min Scan# 430
Delta R.T. 0.00 min
Lab File: VX002374.D
Acq: 07 Jun 2018 13:41




Instrument :
MSVOA_X
ClientSampleId :
LF5-FB-2018-1


Tot Ion: 73 Resp: 325
Ion Ratio Lower Upper
73 100
57 0.0 17.7 26.5#

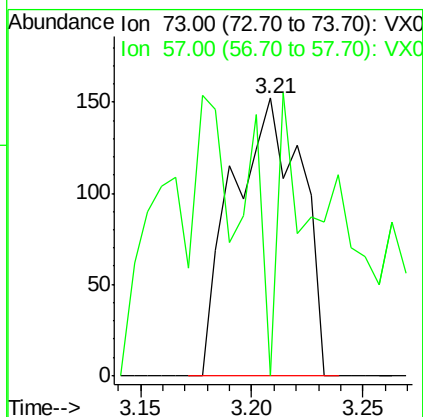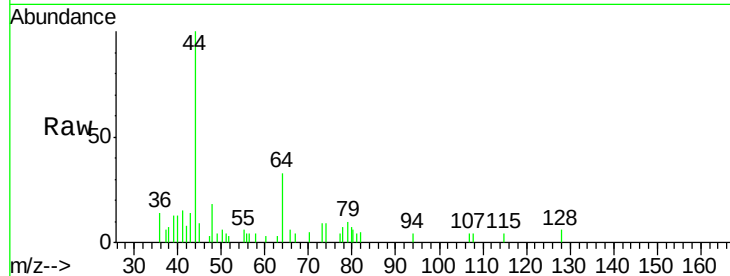

#20
Methylene Chloride
Concen: 187.898 ug/l
RT: 2.86 min Scan# 373
Delta R.T. -0.00 min
Lab File: VX002374.D
Acq: 07 Jun 2018 13:41

Tgt Ion: 84 Resp: 499134
Ion Ratio Lower Upper
84 100
49 135.0 107.8 161.6
51 40.7 32.8 49.2
86 64.6 52.5 78.7

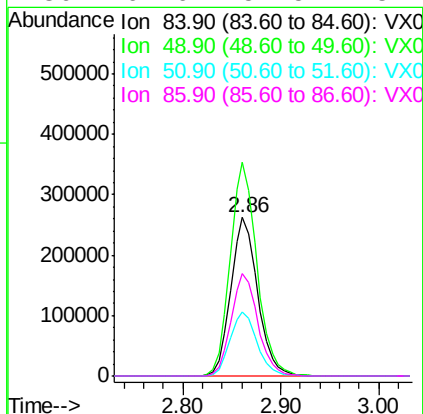







#22

Diisopropyl ether
 Concen: Below Cal
 RT: 3.87 min Scan# 539
 Delta R.T. -0.01 min
 Lab File: VX002374.D
 Acq: 07 Jun 2018 13:41

Instrument :
 MSVOA_X
 ClientSampled :
 LF5-FB-2018-1




Tot Ion:	45	Resp:	77
Ion	Ratio	Lower	Upper
45	100		
43	4.3	46.8	70.2#
87	0.0	20.2	30.4#
59	0.0	8.7	13.1#

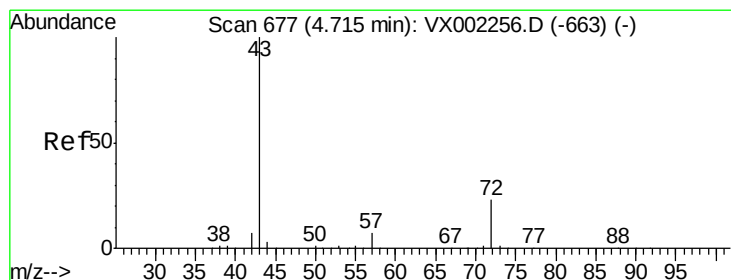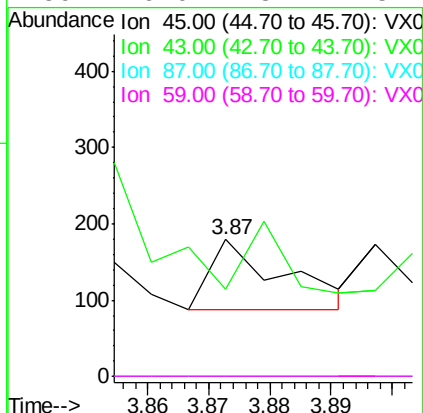


#25

2-Butanone
 Concen: 28.434 ug/l
 RT: 4.71 min Scan# 676
 Delta R.T. -0.01 min
 Lab File: VX002374.D
 Acq: 07 Jun 2018 13:41

Tgt Ion:	43	Resp:	68268
Ion	Ratio	Lower	Upper
43	100		
72	24.3	18.5	27.7

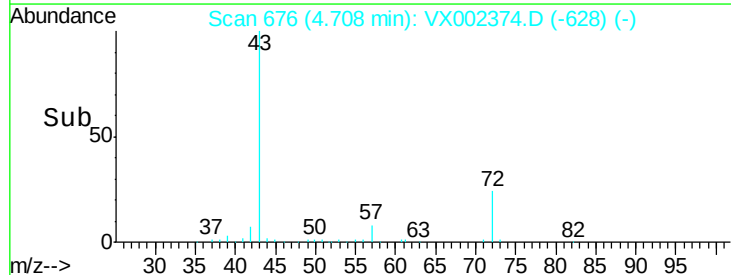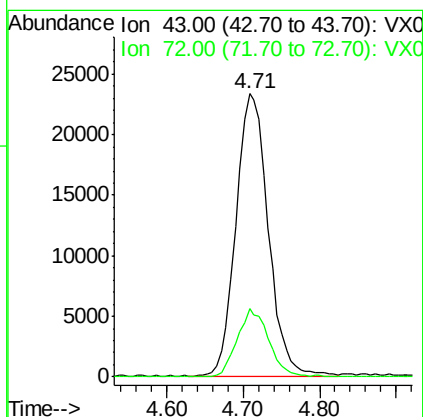

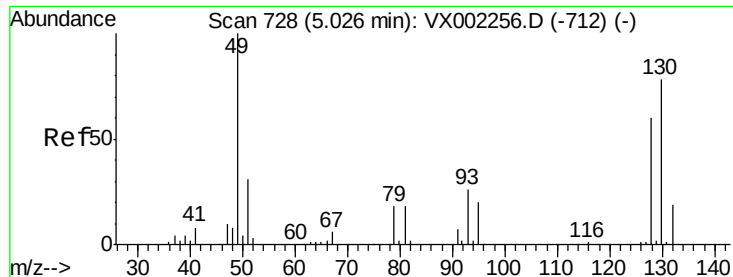

#28

Bromochloromethane

Concen: Below Cal

RT: 5.02 min Scan# 727

Delta R.T. -0.01 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41

Instrument :

MSVOA_X

ClientSampleId :

LF5-FB-2018-1





Tot Ion: 49 Resp: 275

Ion Ratio Lower Upper

49 100

129 0.0 0.0 4.2

130 8.0 61.2 91.8#

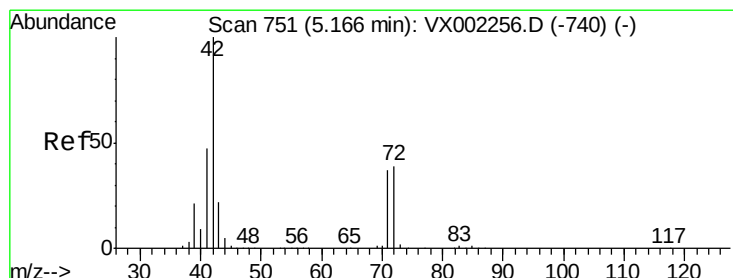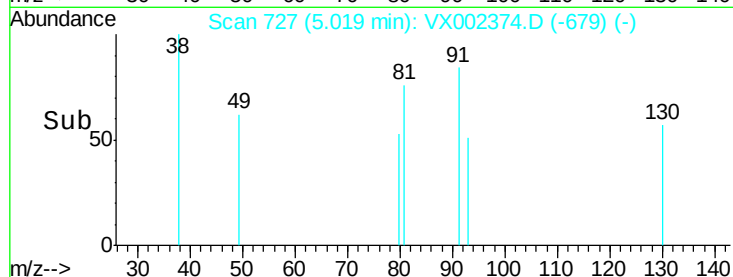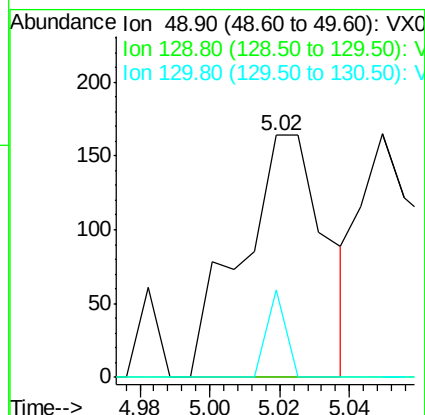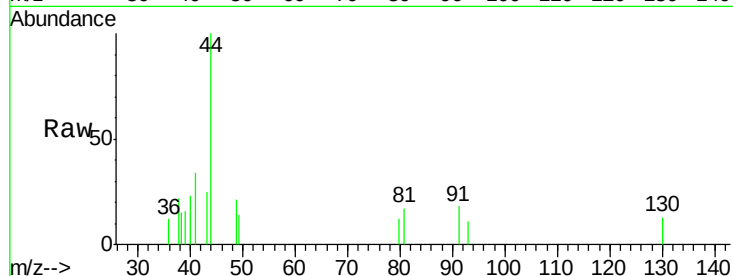

#29

Tetrahydrofuran

Concen: 1697.940 ug/l

RT: 5.17 min Scan# 751

Delta R.T. -0.00 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41




Tgt Ion: 42 Resp: 2628356


Ion Ratio Lower Upper

42 100

72 40.1 32.0 48.0

71 37.8 30.1 45.1


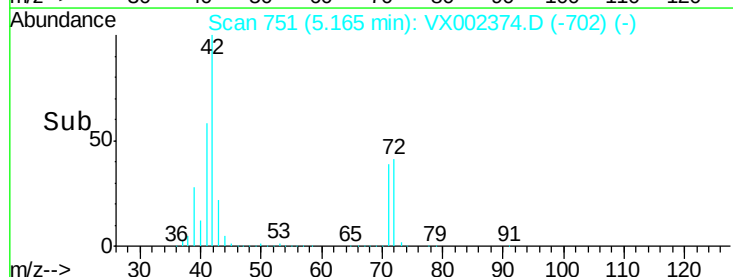
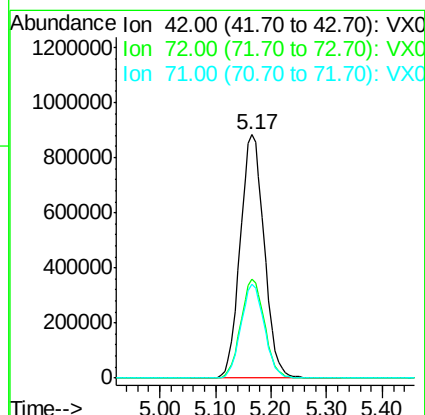
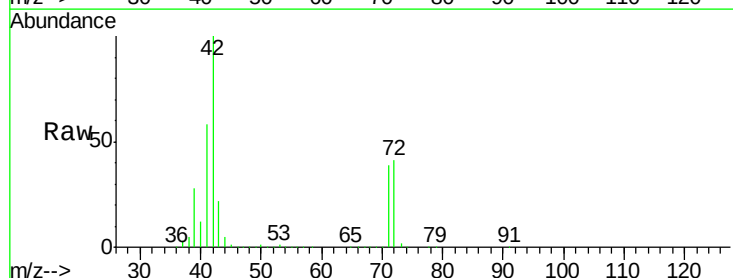




#33
 1,2-Dichloroethane-d4
 Concen: 53.963 ug/l
 RT: 6.07 min Scan# 900
 Delta R.T. -0.00 min
 Lab File: VX002374.D
 Acq: 07 Jun 2018 13:41




Instrument :
 MSVOA_X
 ClientSampleId :
 LF5-FB-2018-1


Tot Ion: 65 Resp: 187998
 Ion Ratio Lower Upper
 65 100
 67 51.5 0.0 102.6

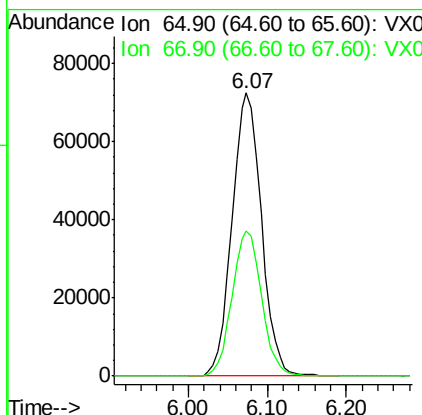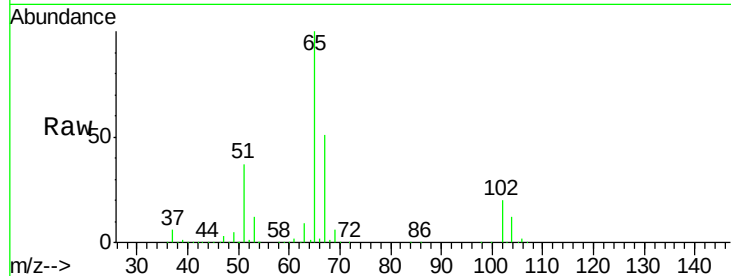

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.87 min Scan# 1030
 Delta R.T. -0.00 min
 Lab File: VX002374.D
 Acq: 07 Jun 2018 13:41

Tgt Ion: 114 Resp: 354004
 Ion Ratio Lower Upper
 114 100
 63 21.2 0.0 41.4
 88 15.5 0.0 30.0

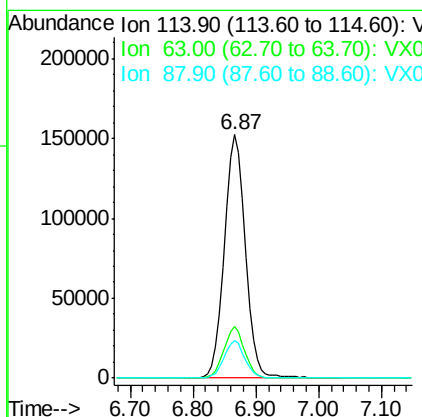

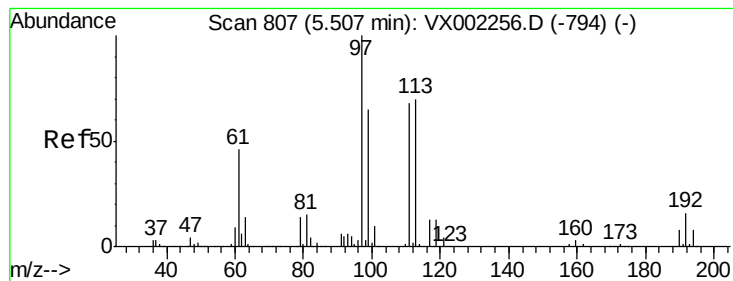

#35

Dibromofluoromethane

Concen: 51.048 ug/l

RT: 5.51 min Scan# 807

Delta R.T. -0.00 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41

Instrument :

MSVOA_X

ClientSampleId :

LF5-FB-2018-1





Tot Ion:113 Resp: 142113

Ion Ratio Lower Upper

113 100

111 102.3 81.4 122.0

192 22.9 19.1 28.7

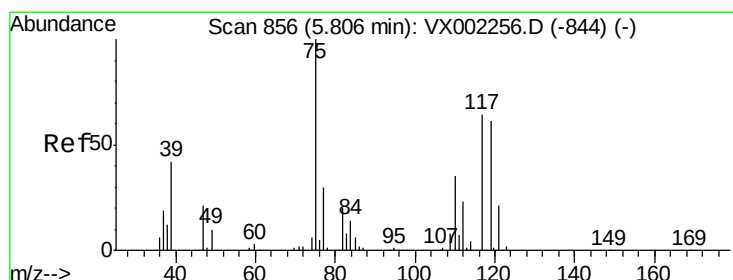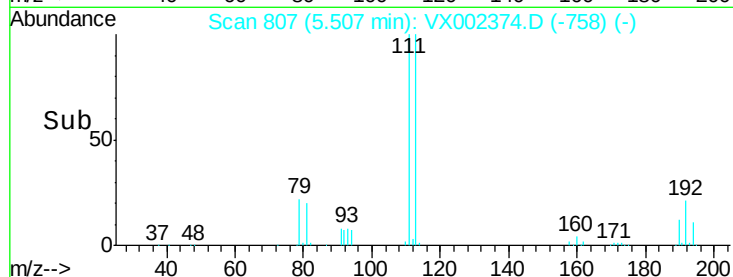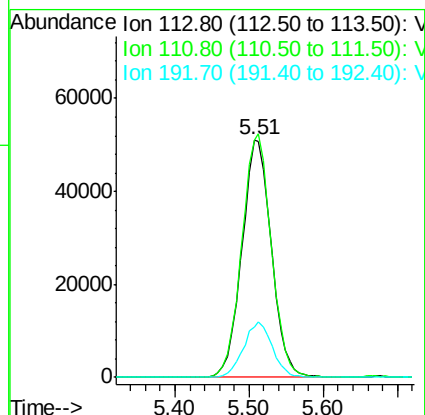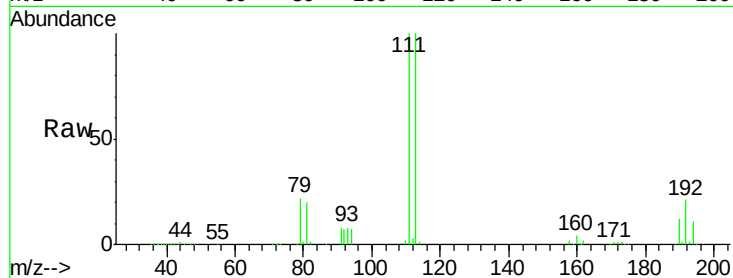

#36

1,1-Dichloropropene

Concen: 4.739 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.14 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41




Tgt Ion: 75 Resp: 17636


Ion Ratio Lower Upper

75 100

110 10.3 18.1 54.4#

77 0.0 24.3 36.5#

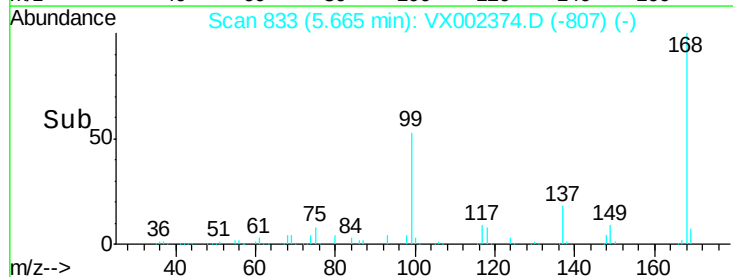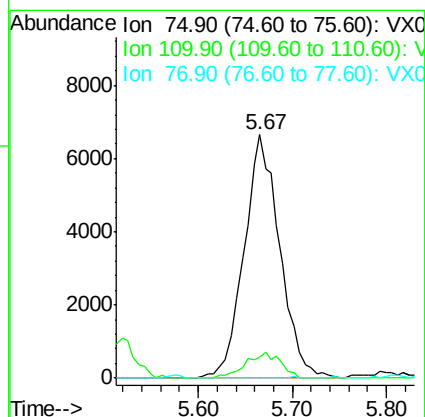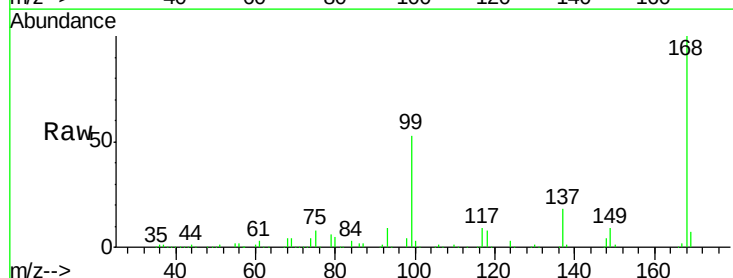



#37

Ethyl Acetate

Concen: 15.253 ug/l

RT: 4.71 min Scan# 676

Delta R.T. -0.16 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41

Instrument :

MSVOA_X

ClientSampleId :

LF5-FB-2018-1





Tot Ion: 43 Resp: 68268

Ion Ratio Lower Upper

43 100

61 0.0 10.4 15.6#

70 0.0 7.6 11.4#

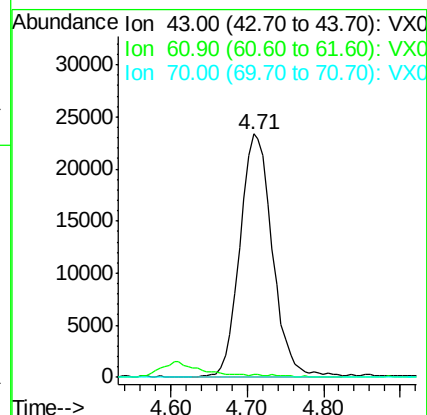

#38

Carbon Tetrachloride

Concen: 5.968 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.12 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41




Tgt Ion: 117 Resp: 23237


Ion Ratio Lower Upper

117 100

119 4.3 77.4 116.0#

121 0.0 24.4 36.6#


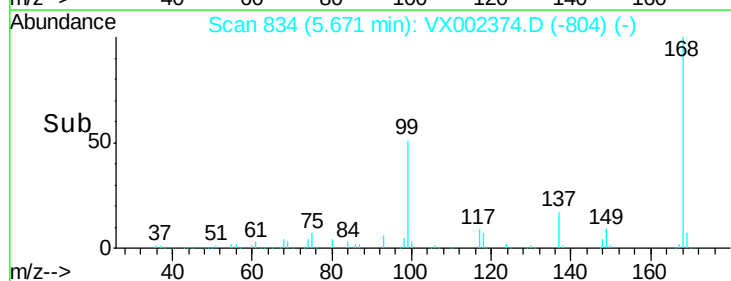
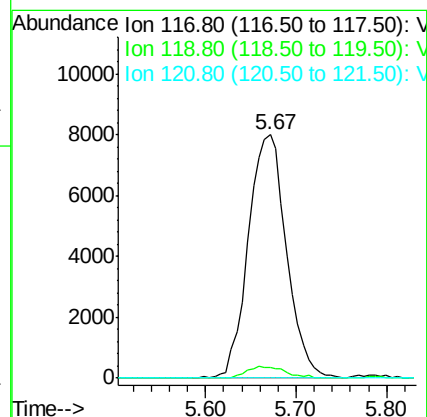



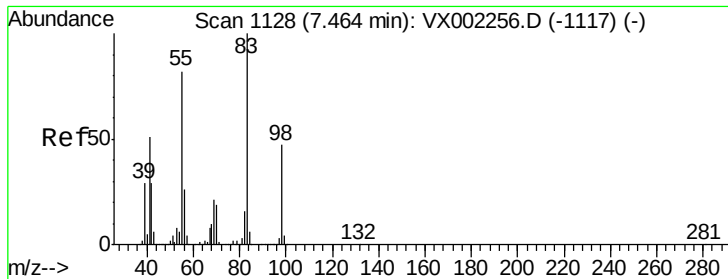

#39
Methylvlcyclohexane
Concen: 0.280 ug/l
RT: 7.46 min Scan# 1128
Delta R.T. -0.00 min
Lab File: VX002374.D
Acq: 07 Jun 2018 13:41




Instrument :
MSVOA_X
ClientSampled :
LF5-FB-2018-1


Tot Ion: 83 Resp: 79
Ion Ratio Lower Upper
83 100
55 75.6 65.4 98.0
98 98.8 37.4 56.0#

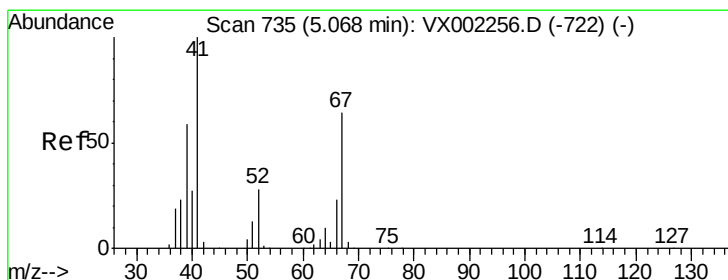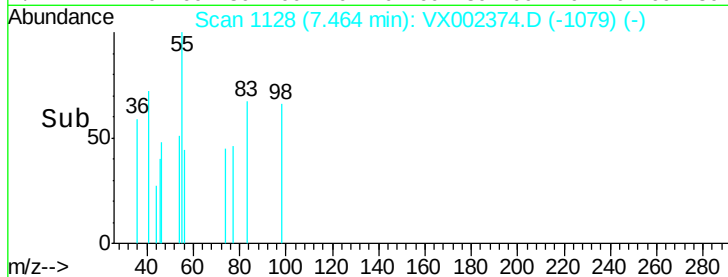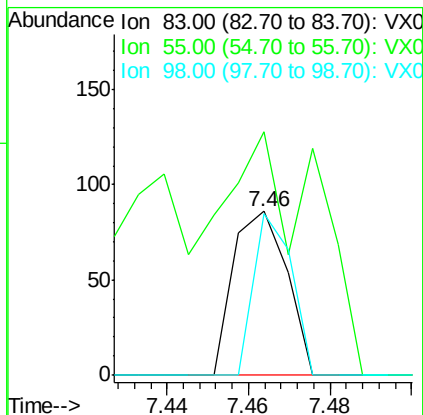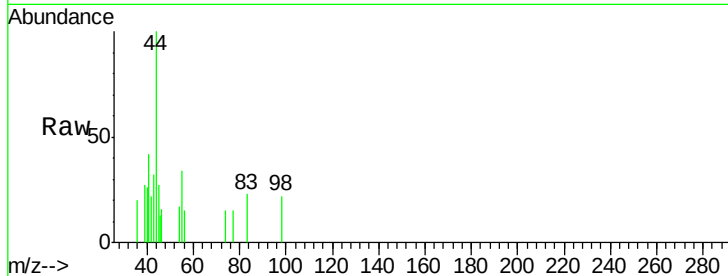

#41
Methacrylonitrile
Concen: 590.491 ug/l
RT: 5.17 min Scan# 751
Delta R.T. 0.10 min
Lab File: VX002374.D
Acq: 07 Jun 2018 13:41

Tgt Ion: 41 Resp: 1512890
Ion Ratio Lower Upper
41 100
39 47.3 45.8 68.6
67 0.0 51.3 76.9#
52 0.1 23.0 34.6#

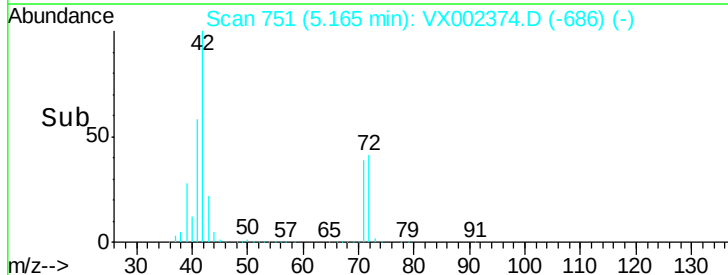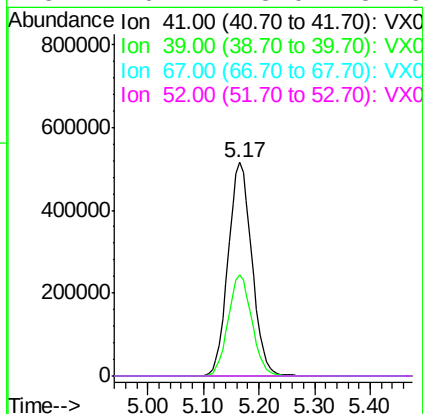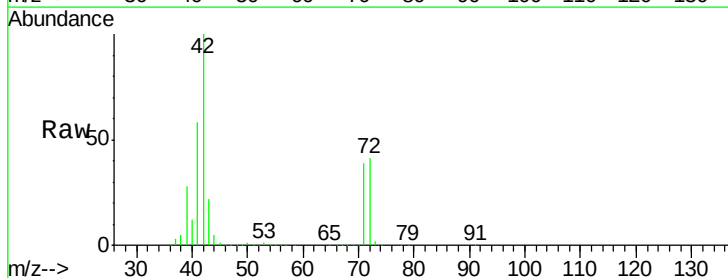



#50

Toluene-d8

Concen: 52.701 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. -0.00 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41

Instrument :

MSVOA_X

ClientSampleId :


LF5-FB-2018-1

Tot Ion: 98 Resp: 562346

Ion Ratio Lower Upper




98 100

100 63.1 50.9 76.3

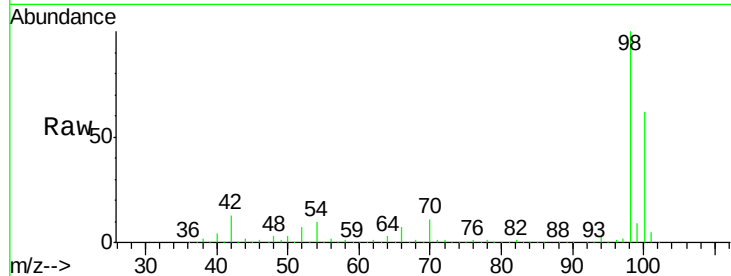

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

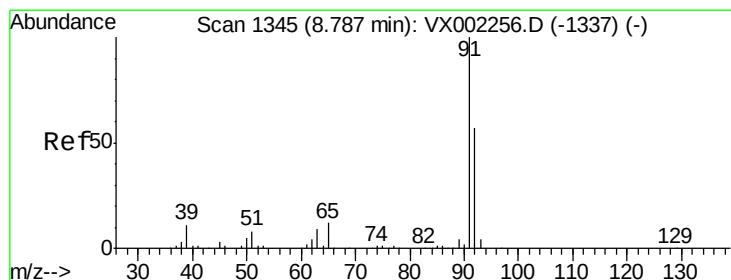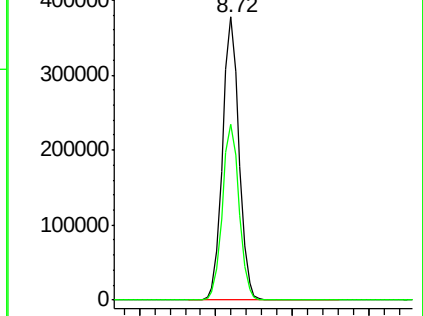

#52

Toluene

Concen: 0.203 ug/l

RT: 8.79 min Scan# 1345

Delta R.T. -0.00 min

Lab File: VX002374.D


Acq: 07 Jun 2018 13:41

Tgt Ion: 92 Resp: 1473

Ion Ratio Lower Upper



92 100


91 179.2 140.4 210.6



Abundance Ion 92.00 (91.70 to 92.70): VX0

Ion 91.00 (90.70 to 91.70): VX0




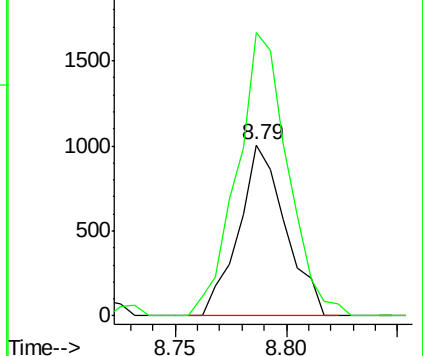




#62
4-Bromofluorobenzene
Concen: 48.492 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. -0.00 min
Lab File: VX002374.D
Acq: 07 Jun 2018 13:41




Instrument :
MSVOA_X
ClientSampleId :
LF5-FB-2018-1


Tot Ion: 95 Resp: 199531
Ion Ratio Lower Upper
95 100
174 92.6 0.0 187.4
176 90.8 0.0 181.0

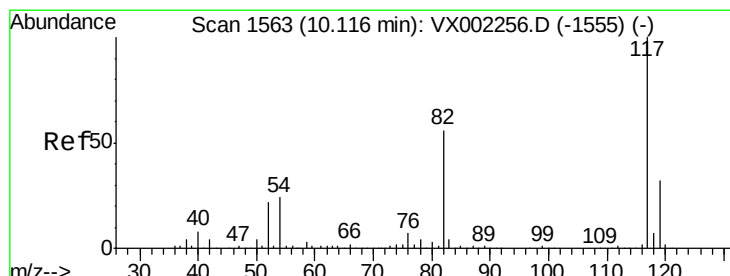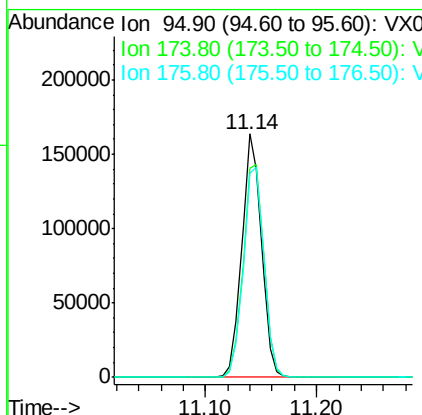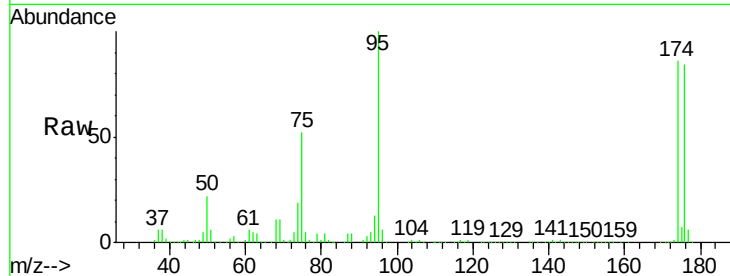

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. -0.00 min
Lab File: VX002374.D
Acq: 07 Jun 2018 13:41

Tgt Ion: 117 Resp: 325366
Ion Ratio Lower Upper
117 100
82 56.0 45.0 67.4
119 32.4 25.8 38.6


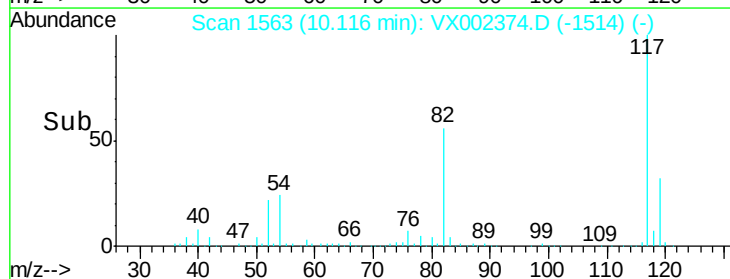
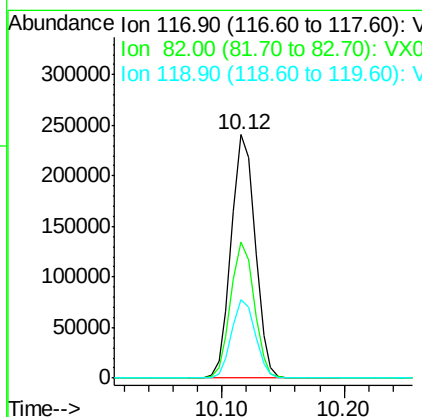
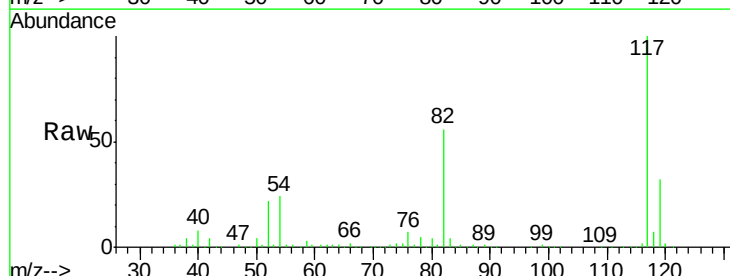




#67
Ethyl Benzene
Concen: 0.369 ug/l
RT: 10.26 min Scan# 1586
Delta R.T. -0.00 min
Lab File: VX002374.D
Acq: 07 Jun 2018 13:41




Instrument :
MSVOA_X
ClientSampleId :
LF5-FB-2018-1


Tot Ion: 91 Resp: 4998
Ion Ratio Lower Upper
91 100
106 32.6 25.5 38.3

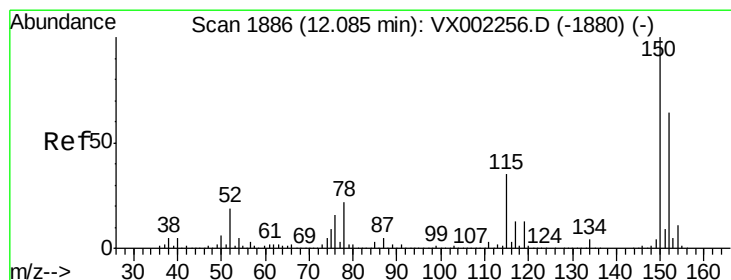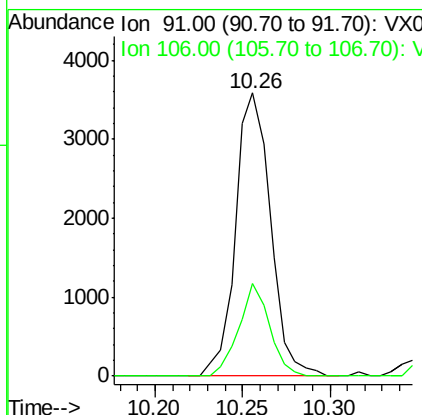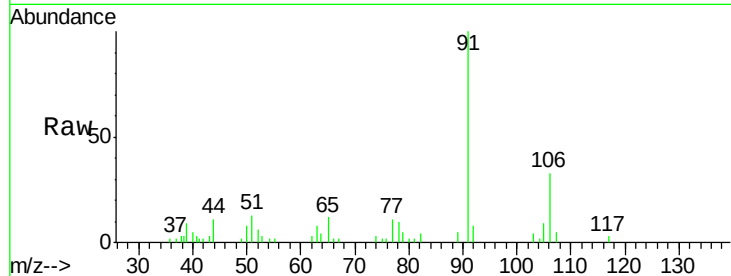

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX002374.D
Acq: 07 Jun 2018 13:41

Tgt Ion: 152 Resp: 184882
Ion Ratio Lower Upper
152 100
115 55.2 40.1 120.2
150 155.8 0.0 347.2

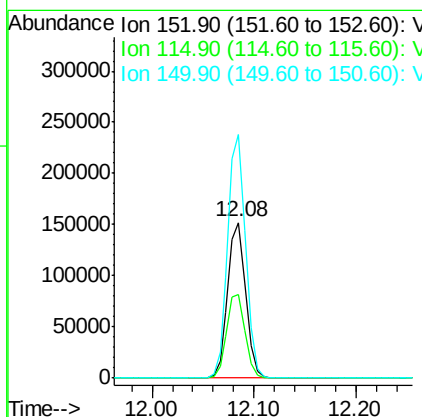



#76

1,2,3-Trichloropropane

Concen: 26.003 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.16 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41

Instrument :

MSVOA_X

ClientSampleId :


LF5-FB-2018-1

Tot Ion: 75 Resp: 105489

Ion Ratio Lower Upper




75 100

77 1.2 22.8 68.3#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

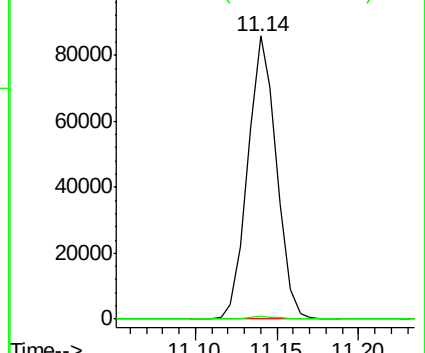

#81

trans-1,4-Dichloro-2-butene

Concen: 91.150 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.06 min

Lab File: VX002374.D

Acq: 07 Jun 2018 13:41


Tgt Ion: 75 Resp: 105489

Ion Ratio Lower Upper

75 100

53 0.2 86.8 130.2#



89 0.0 38.2 57.2#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

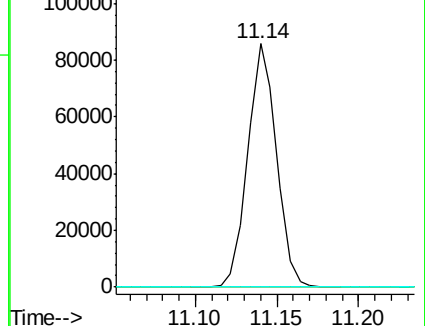



#84
 1,2,4-Trimethylbenzene
 Concen: 0.239 ug/l
 RT: 11.81 min Scan# 1841
 Delta R.T. -0.00 min
 Lab File: VX002374.D
 Acq: 07 Jun 2018 13:41

Instrument :
 MSVOA_X
 ClientSampleId :
 LF5-FB-2018-1

Tot Ion:105 Resp: 2719
 Ion Ratio Lower Upper
 105 100
 120 19.6 22.3 66.8#

