


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060718\
 Data File : VX002367.D
 Acq On : 07 Jun 2018 09:17
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
 Title : SW846 8260
 Last Update : Tue Jun 05 03:22:35 2018

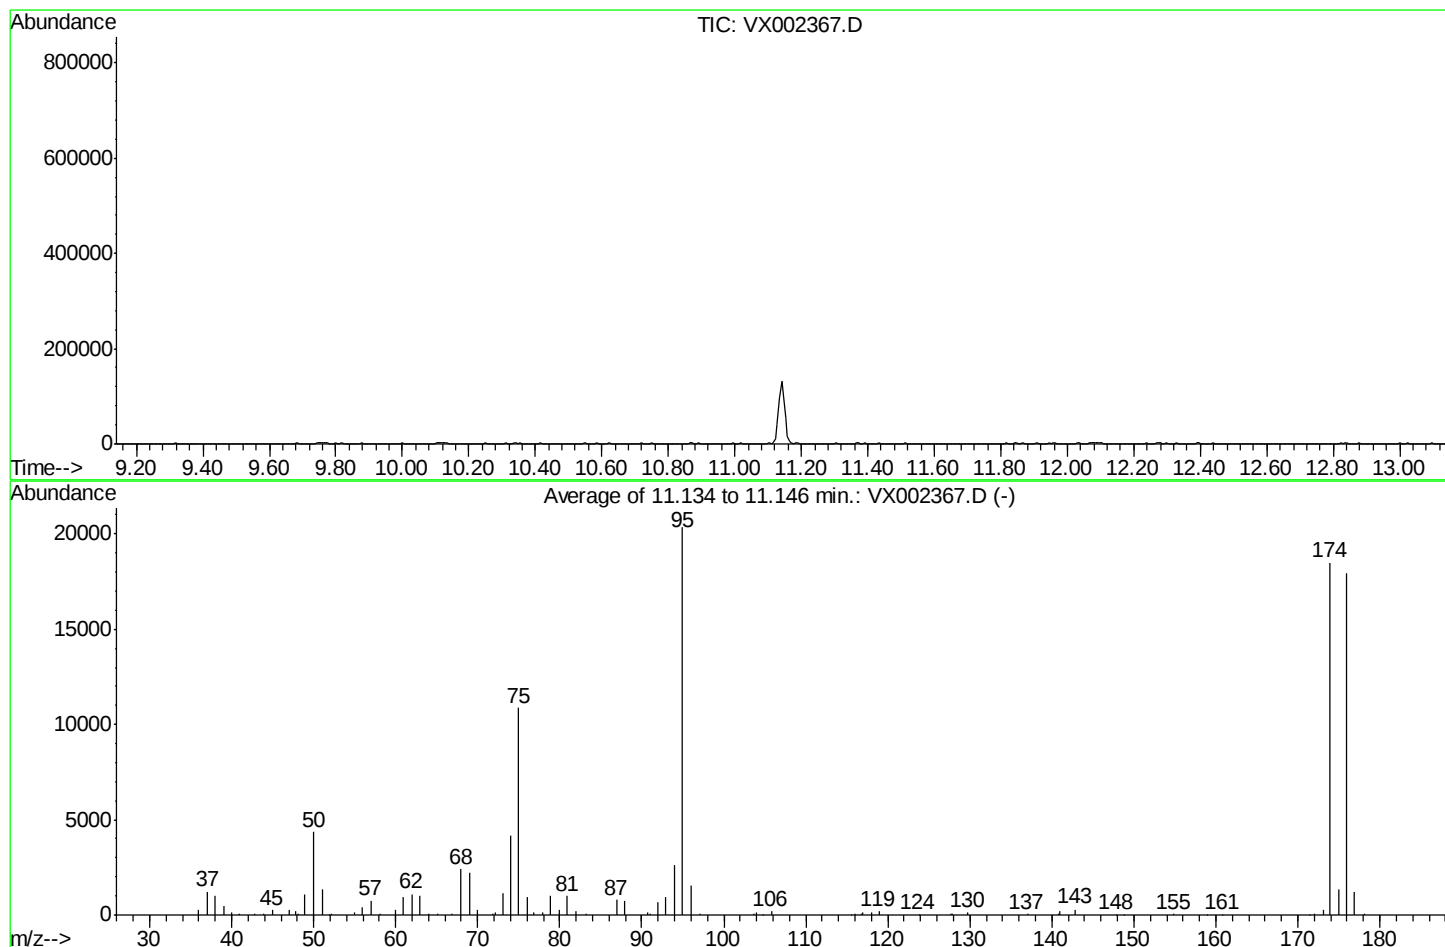

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	4362	PASS
75	95	30	60	53.3	10854	PASS
95	95	100	100	100.0	20346	PASS
96	95	5	9	7.7	1557	PASS
173	174	0.00	2	1.5	275	PASS
174	95	50	100	90.8	18479	PASS
175	174	5	9	7.4	1366	PASS
176	174	95	101	97.1	17940	PASS
177	176	5	9	6.7	1203	PASS