

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX060818\
 Data File : VX002413.D
 Acq On : 08 Jun 2018 20:17
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Jun 09 04:55:51 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X052518W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri May 25 02:17:15 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.03	128	38874	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	6.87	114	225685	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.12	117	199330	30.00	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	6.07	65	97183	31.77	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	105.90%
60) 4-Bromofluorobenzene	11.14	95	90983	26.66	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	88.87%
63) Toluene-d8	8.72	98	255602	28.77	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	95.90%


Target Compounds					Qvalue
11) Methyl Iodide	2.52	142	3373	1.11 ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX060818\
Data File : VX002413.D
Acq On : 08 Jun 2018 20:17
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Jun 09 04:55:51 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\624X052518W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri May 25 02:17:15 2018
Response via : Initial Calibration

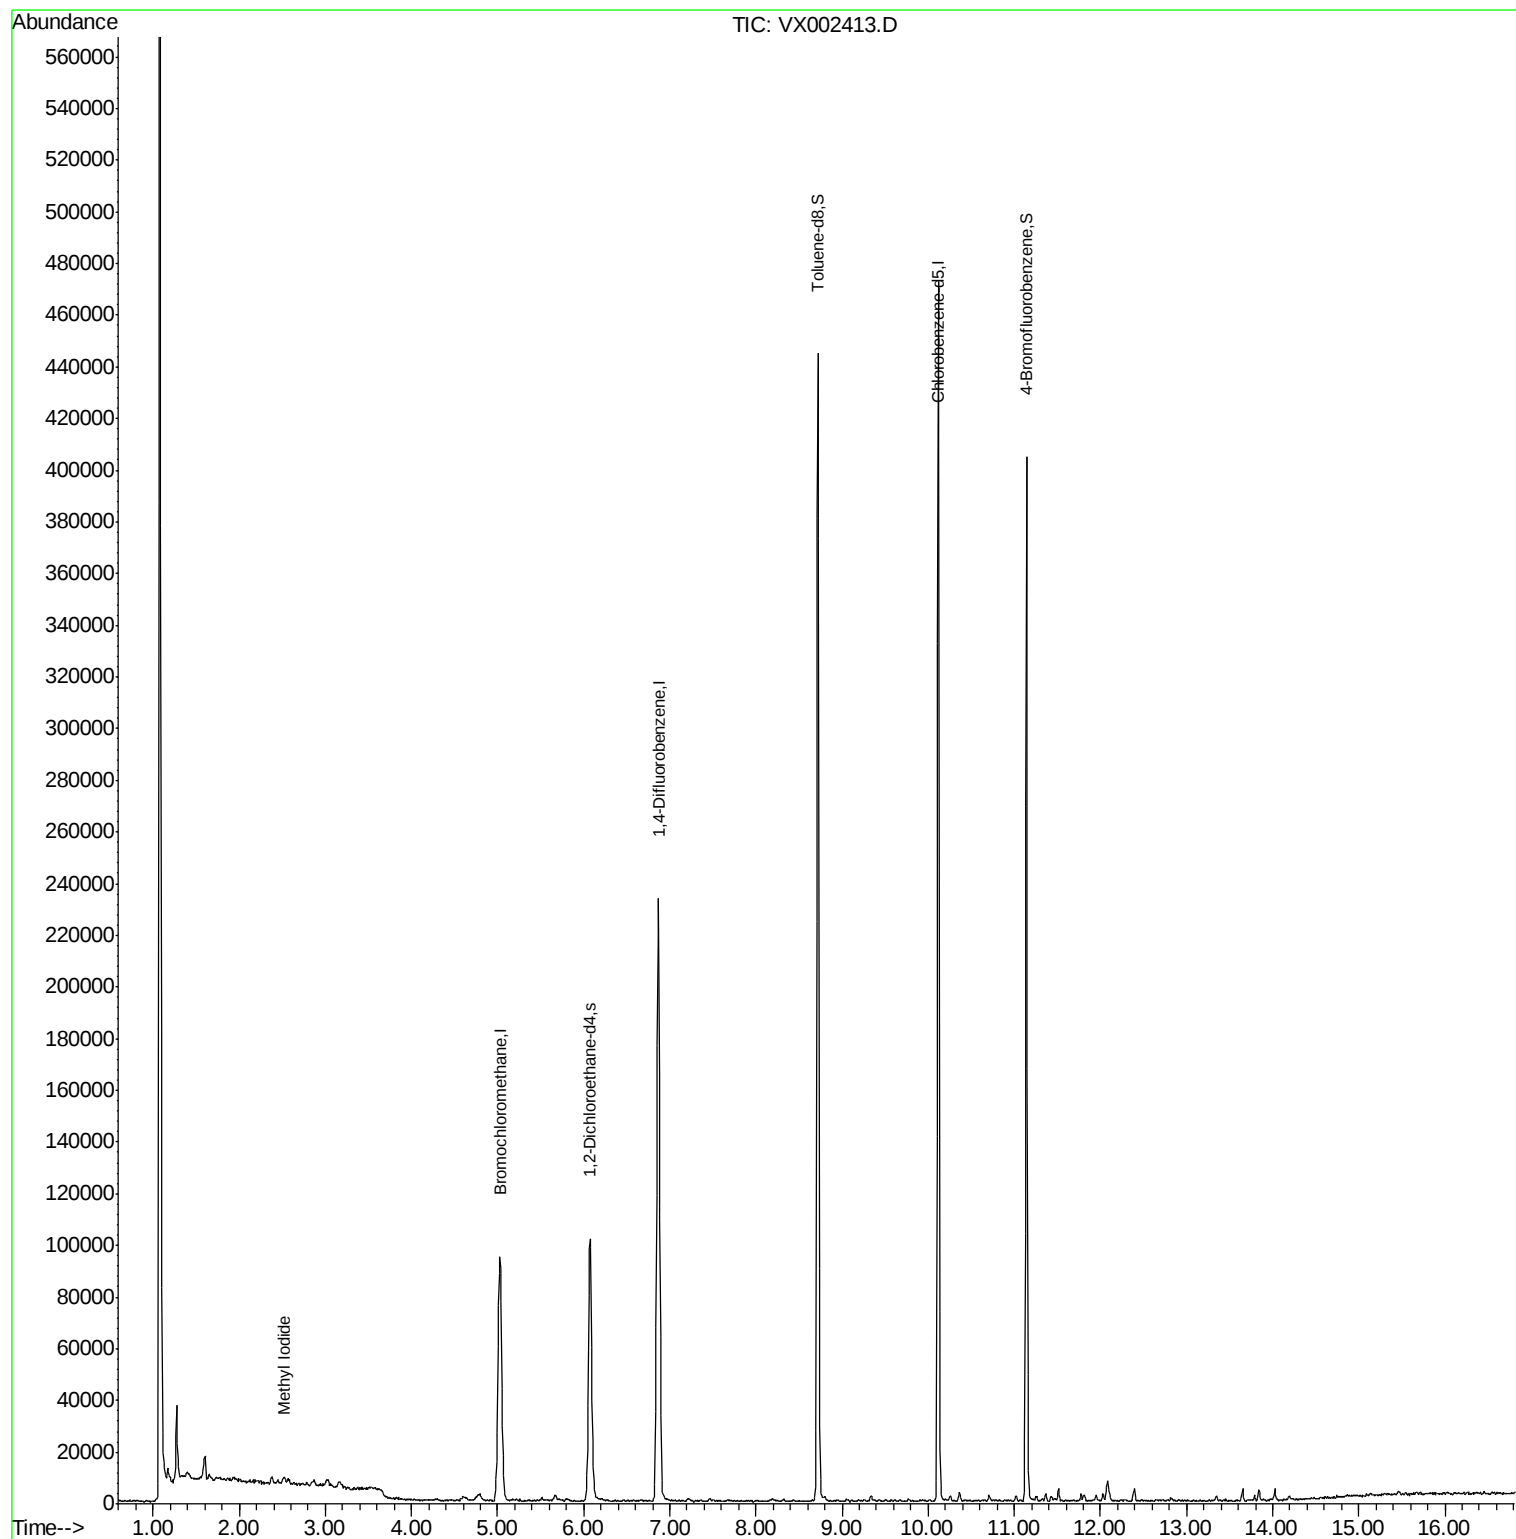

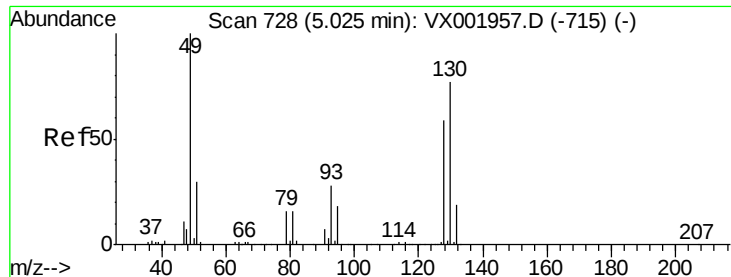

#1

Bromochloromethane

Concen: 30.00 ug/l

RT: 5.03 min Scan# 728

Delta R.T. -0.00 min

Lab File: VX002413.D

Acq: 08 Jun 2018 20:17

Instrument :

MSVOA_X

ClientSampled :

IBLK


Tgt Ion:128 Resp: 38874

Ion Ratio Lower Upper

128 100

49 163.5 0.0 423.0




130 129.5 0.0 324.3

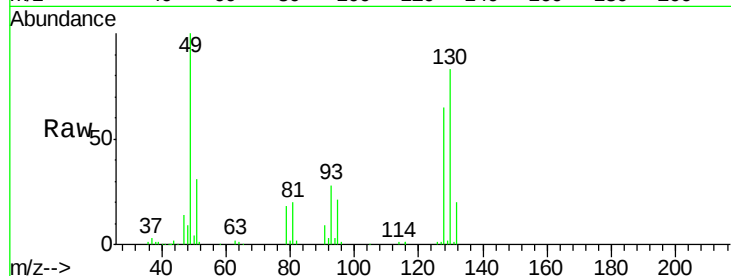

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VX0

Ion 130.00 (129.70 to 130.70): V

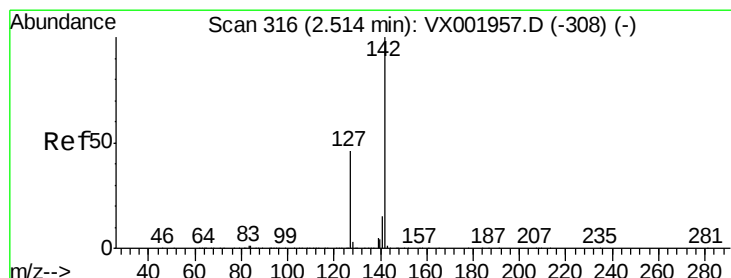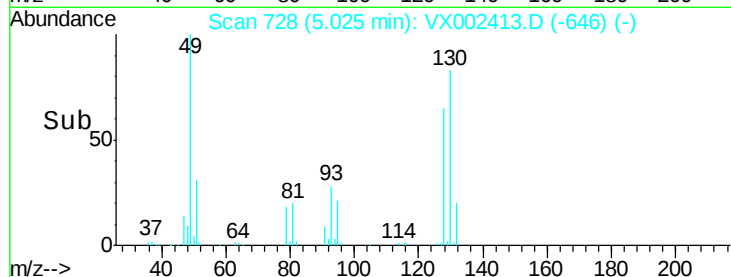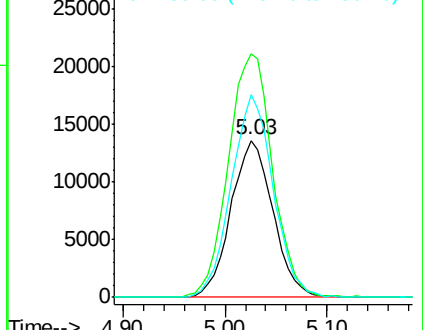

#11

Methyl Iodide

Concen: 1.11 ug/l

RT: 2.52 min Scan# 317

Delta R.T. 0.01 min

Lab File: VX002413.D

Acq: 08 Jun 2018 20:17


Tgt Ion:142 Resp: 3373

Ion Ratio Lower Upper

142 100

127 51.5 23.2 69.6



141 15.5 7.4 22.2

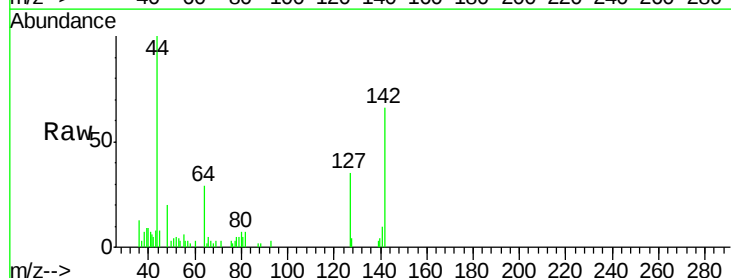


Abundance Ion 142.00 (141.70 to 142.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 141.00 (140.70 to 141.70): V

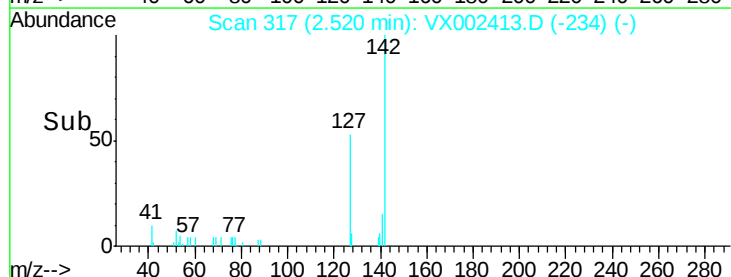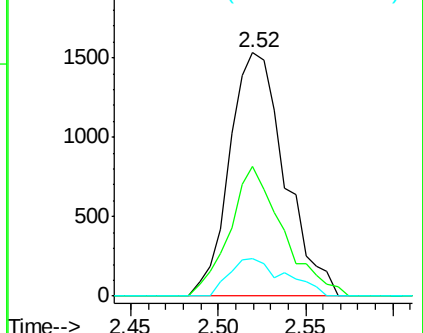

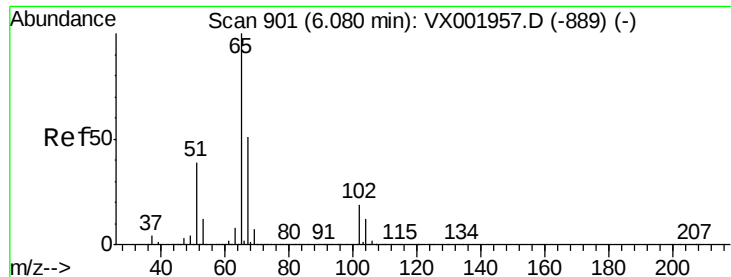

#27

1,2-Dichloroethane-d4

Concen: 31.77 ug/l

RT: 6.07 min Scan# 900

Delta R.T. -0.01 min

Lab File: VX002413.D

Acq: 08 Jun 2018 20:17

Instrument :

MSVOA_X

ClientSampled :





IBLK

Tgt Ion: 65 Resp: 97183

Ion Ratio Lower Upper

65 100

67 51.9 40.9 61.3

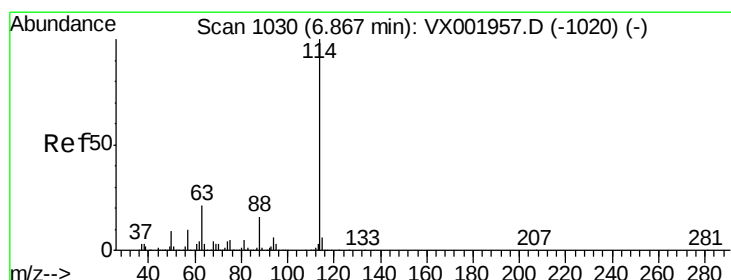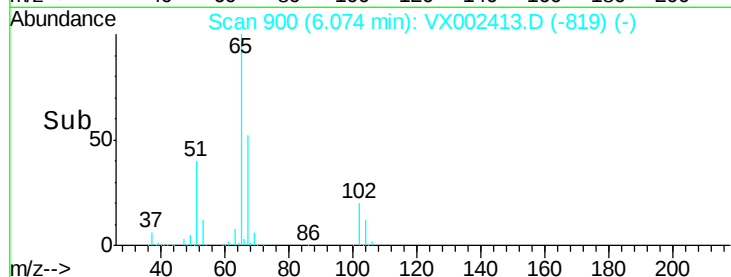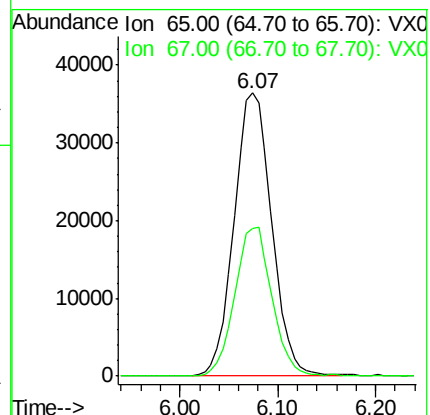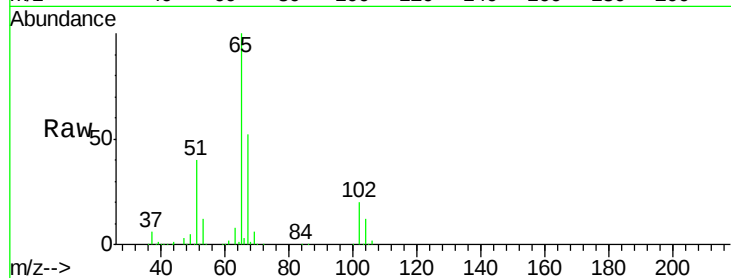

#28

1,4-Difluorobenzene

Concen: 30.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VX002413.D

Acq: 08 Jun 2018 20:17




Tgt Ion: 114 Resp: 225685


Ion Ratio Lower Upper

114 100

63 20.9 17.1 25.7

88 15.4 12.6 19.0


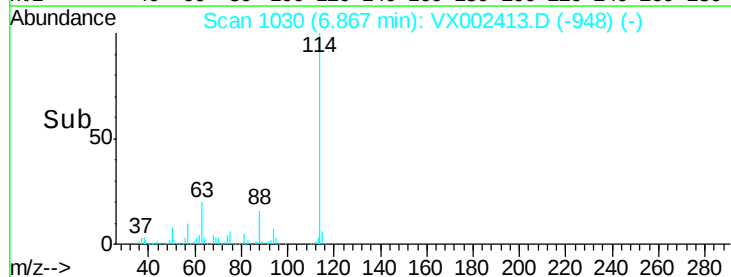
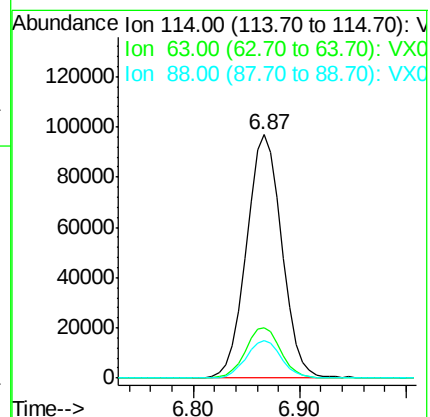
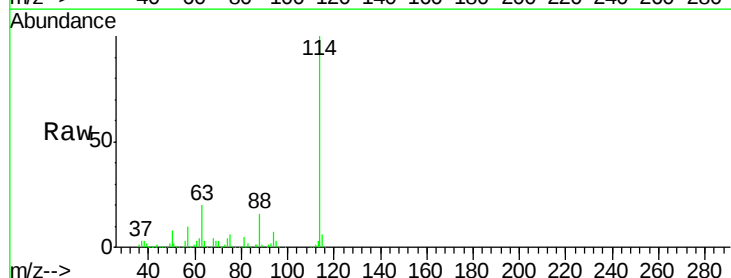


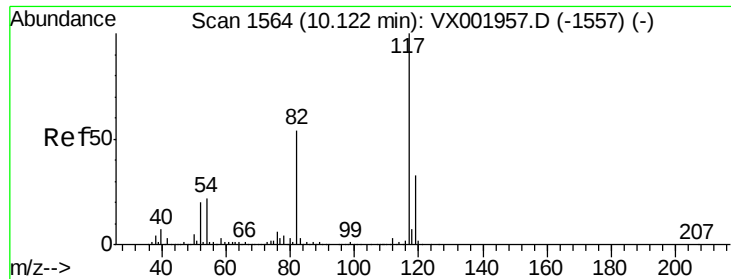

#57
Chlorobenzene-d5
Concen: 30.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. -0.01 min
Lab File: VX002413.D
Acq: 08 Jun 2018 20:17




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion	Ratio	Lower	Upper
117	100		
82	54.4	44.3	66.5
119	32.3	25.7	38.5

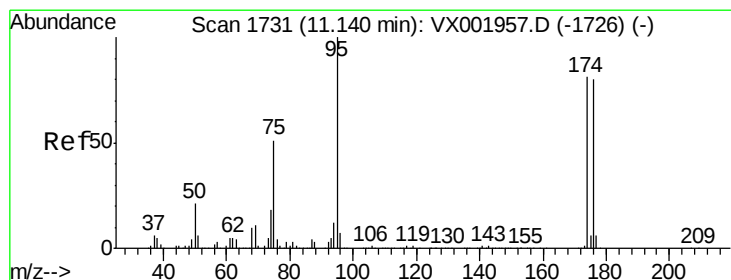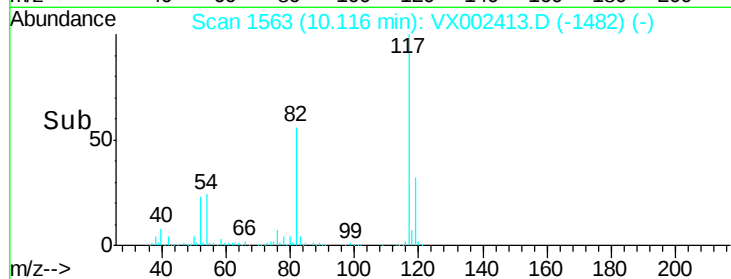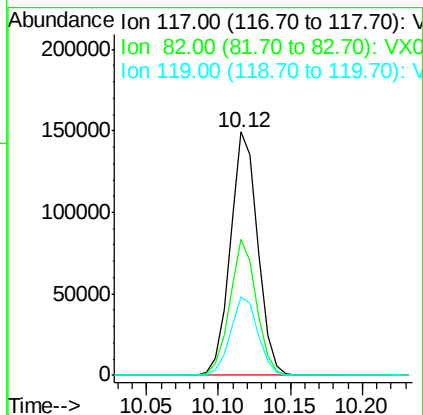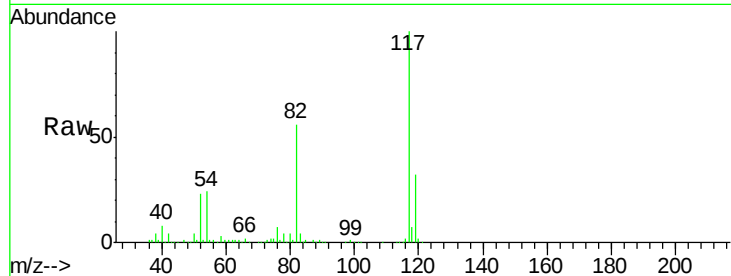

#60
4-Bromofluorobenzene
Concen: 26.66 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. -0.00 min
Lab File: VX002413.D
Acq: 08 Jun 2018 20:17

Tgt Ion	Ratio	Lower	Upper
95	100		
174	94.1	71.8	107.6
176	93.2	70.1	105.1

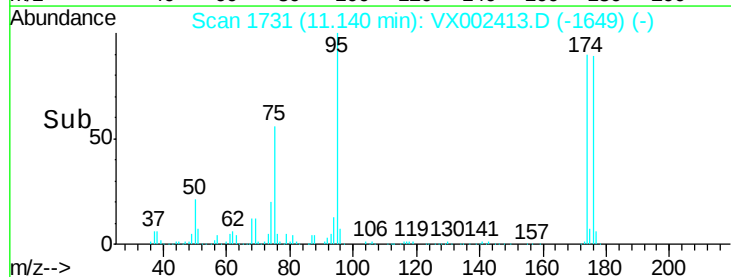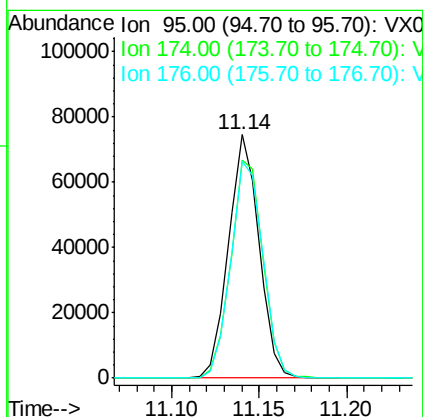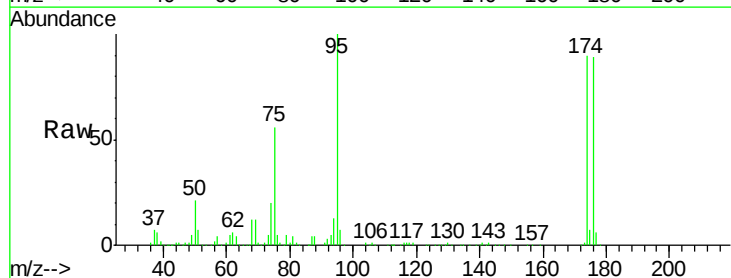

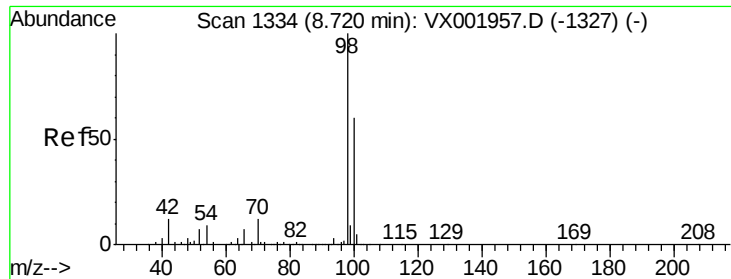

#63

Toluene-d8

Concen: 28.77 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. -0.00 min

Lab File: VX002413.D

Acq: 08 Jun 2018 20:17

Instrument :

MSVOA_X

ClientSampleId :

IBLK

Tgt Ion: 98 Resp: 255602

Ion Ratio Lower Upper

98 100

100 63.7 50.8 76.2

