

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX060918\
 Data File : VX002427.D
 Acq On : 09 Jun 2018 17:56
 Operator : JC/MD
 Sample : J3396-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 W-24

Quant Time: Jun 11 08:12:38 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 05 03:22:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	206153	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	300891	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	266835	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	146888	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	141031	47.68	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.36%	
35) Dibromofluoromethane	5.51	113	109072	46.10	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.20%	
50) Toluene-d8	8.72	98	423519	46.70	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.40%	
62) 4-Bromofluorobenzene	11.14	95	142165	40.65	ug/l	0.00
Spiked Amount	50.000		Recovery	=	81.30%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX060918\
Data File : VX002427.D
Acq On : 09 Jun 2018 17:56
Operator : JC/MD
Sample : J3396-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
W-24

Quant Time: Jun 11 08:12:38 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 05 03:22:35 2018
Response via : Initial Calibration

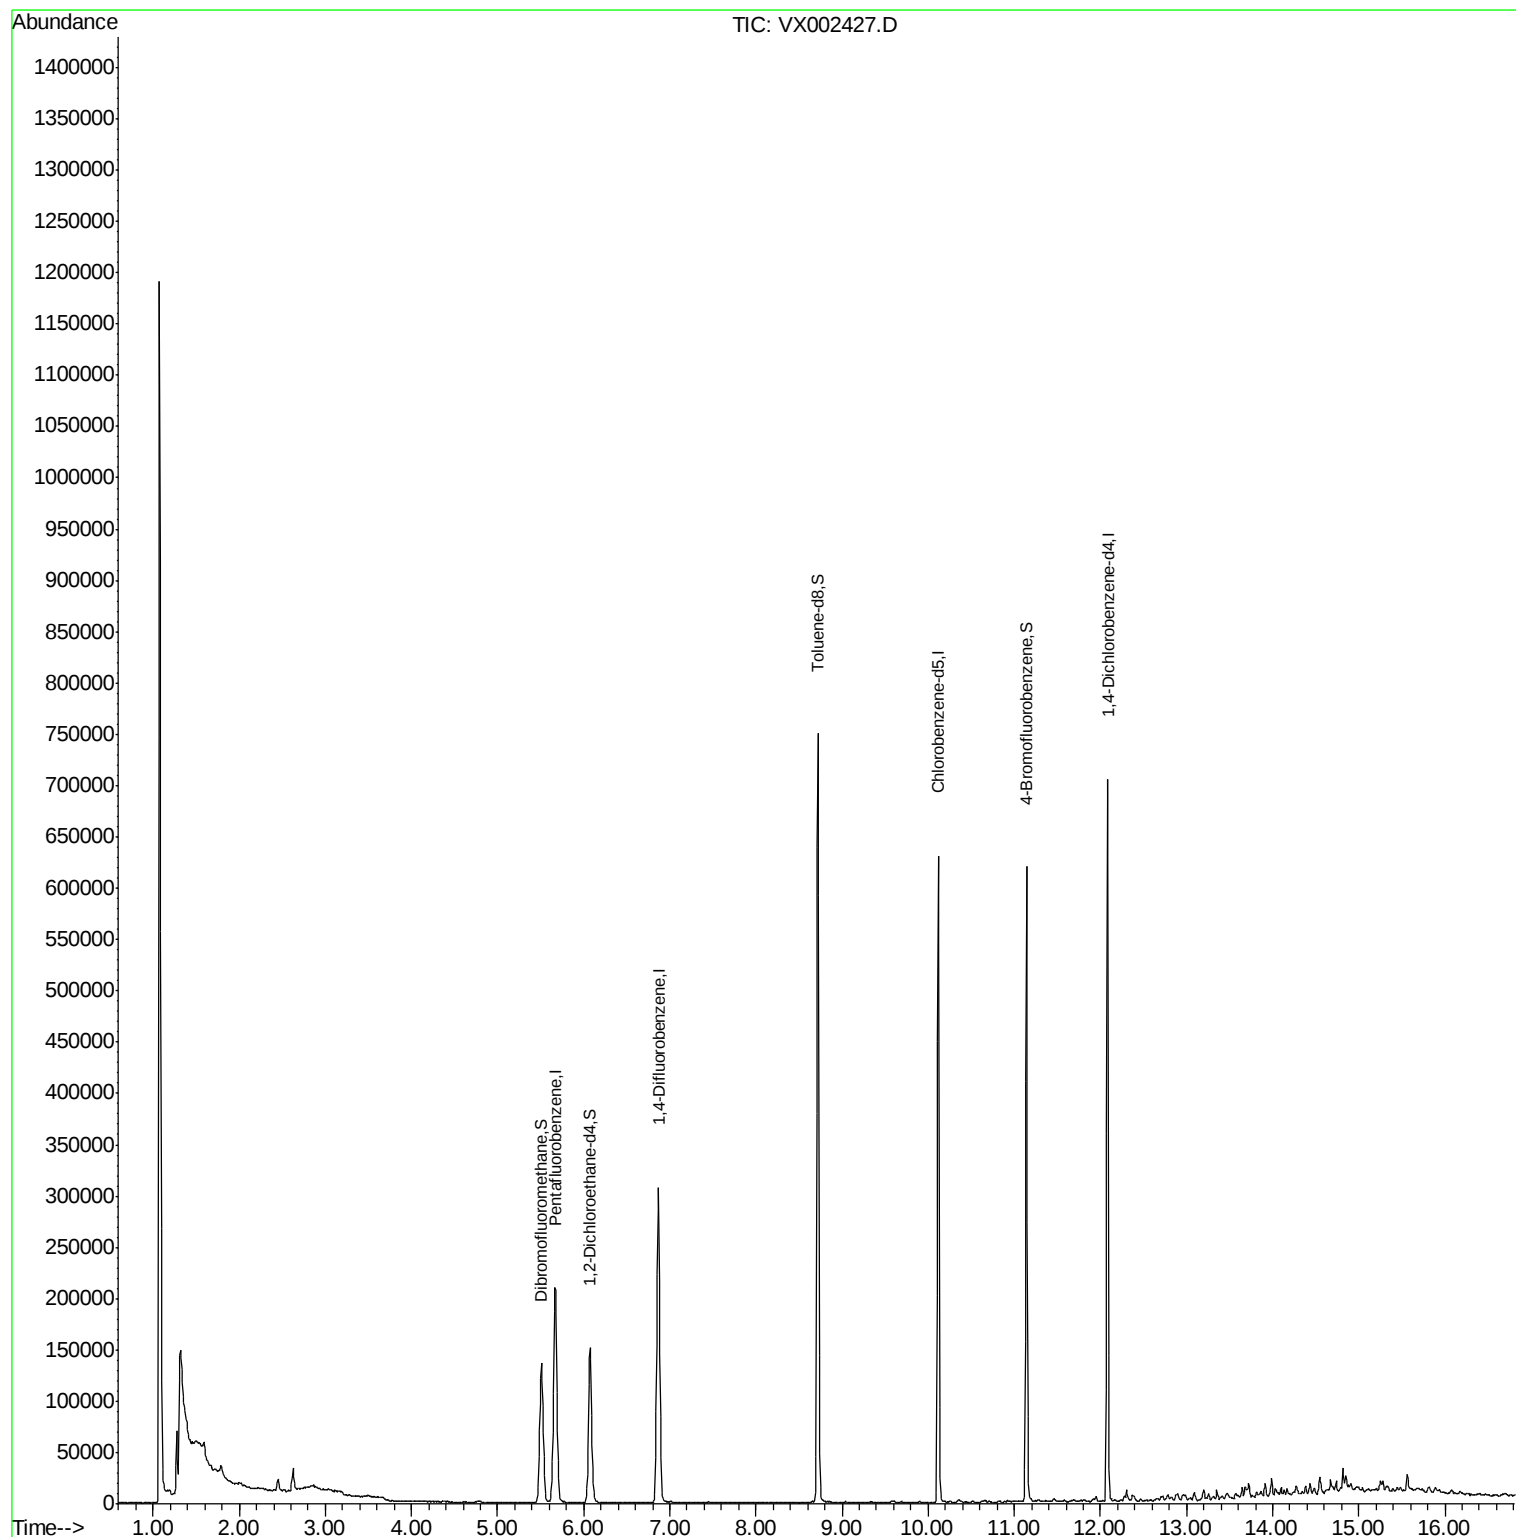



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.00 min

Lab File: VX002427.D

Acq: 09 Jun 2018 17:56

Instrument :

MSVOA_X

ClientSampleId :


W-24

Tot Ion:168 Resp: 206153

Ion Ratio Lower Upper

168 100

99 49.7 39.3 58.9

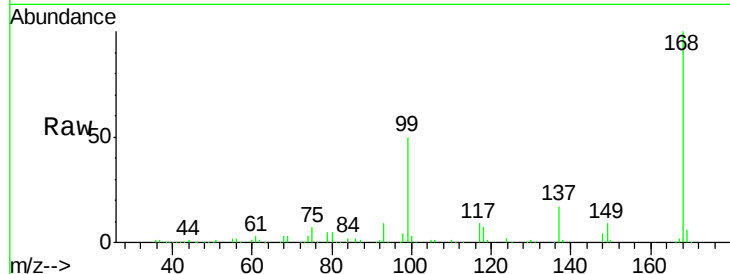

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

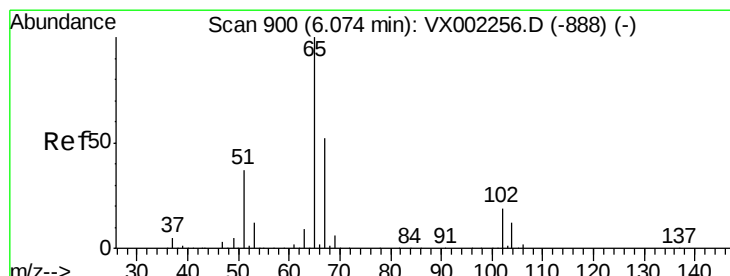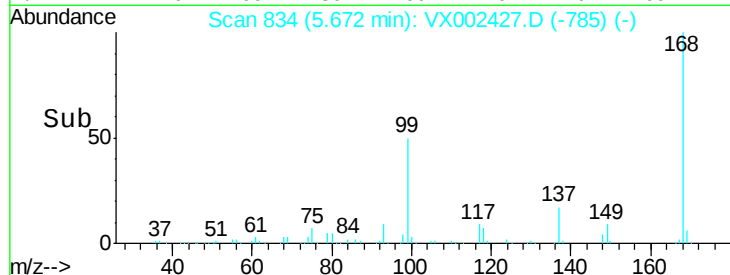

#33

1,2-Dichloroethane-d4

Concen: 47.68 ug/l

RT: 6.07 min Scan# 900

Delta R.T. -0.00 min

Lab File: VX002427.D


Acq: 09 Jun 2018 17:56

Tgt Ion: 65 Resp: 141031

Ion Ratio Lower Upper

65 100

67 51.3 0.0 102.6

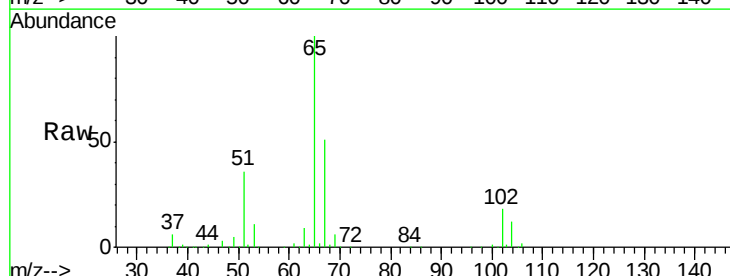

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

60000

50000

40000


30000

20000

10000

0

Time--> 5.90 6.00 6.10 6.20 6.30

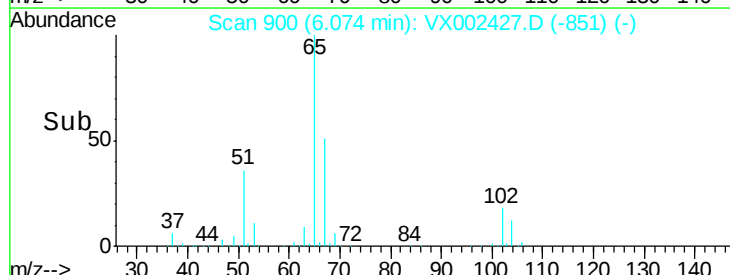



#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VX002427.D

Acq: 09 Jun 2018 17:56

Instrument :

MSVOA_X

ClientSampleId :

W-24


Tot Ion:114 Resp: 300891

Ion Ratio Lower Upper

114 100

63 20.2 0.0 41.4




88 14.3 0.0 30.0

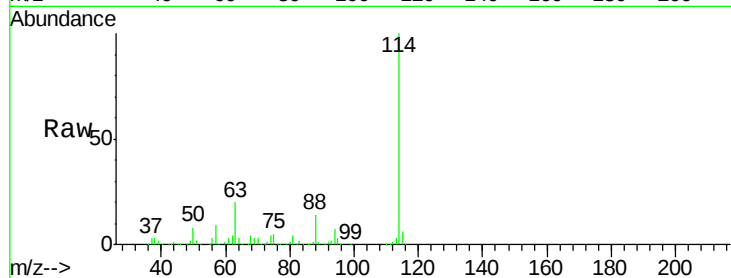

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

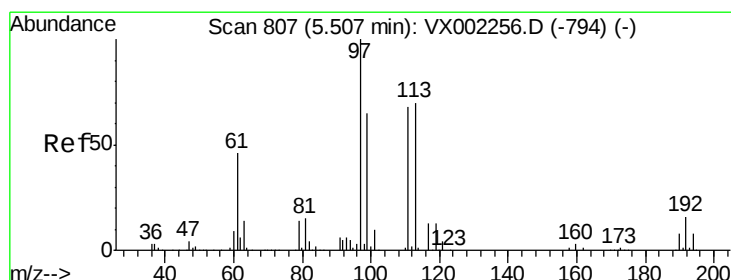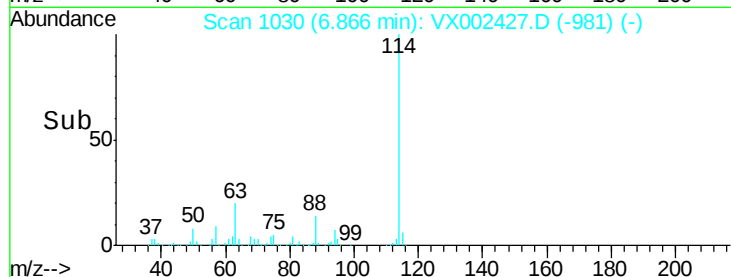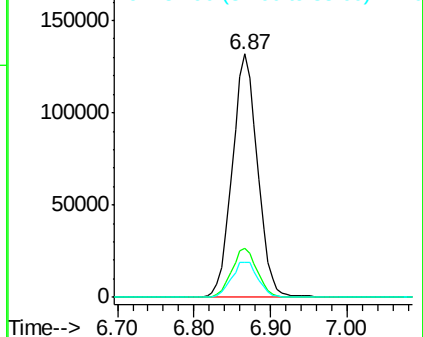

#35

Dibromofluoromethane

Concen: 46.10 ug/l

RT: 5.51 min Scan# 807

Delta R.T. -0.00 min

Lab File: VX002427.D

Acq: 09 Jun 2018 17:56


Tgt Ion:113 Resp: 109072

Ion Ratio Lower Upper

113 100

111 101.9 81.4 122.0



192 22.7 19.1 28.7

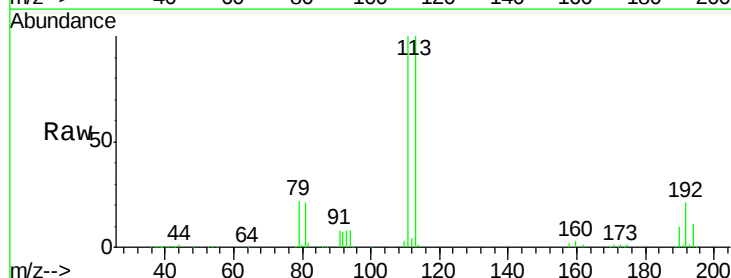


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

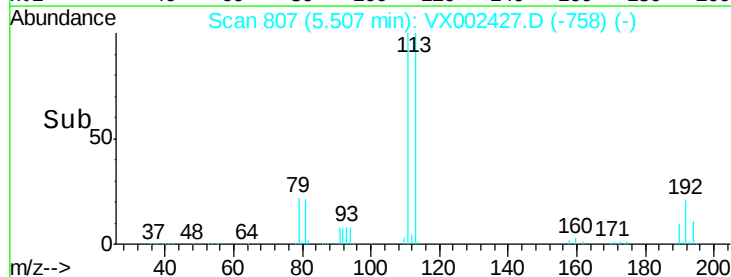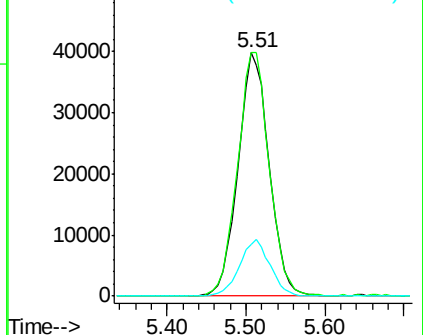

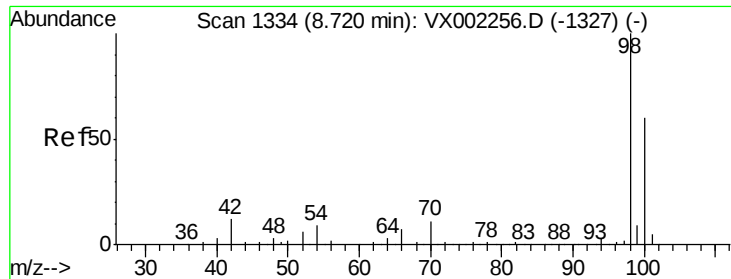

#50

Toluene-d8

Concen: 46.70 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. -0.00 min

Lab File: VX002427.D

Acq: 09 Jun 2018 17:56

Instrument :

MSVOA_X

ClientSampleId :


W-24

Tot Ion: 98 Resp: 423519

Ion Ratio Lower Upper

98 100

100 63.4 50.9 76.3

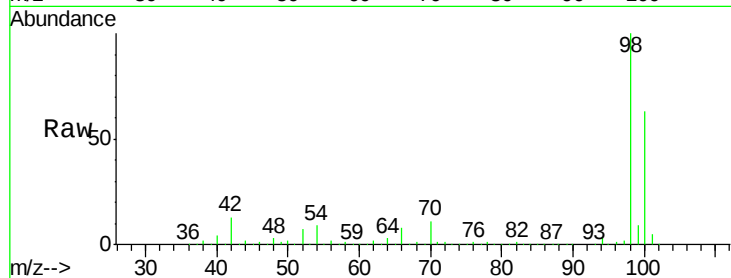

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

8.72

300000

250000

200000

150000



100000

50000

0

Time-->

8.60 8.70 8.80

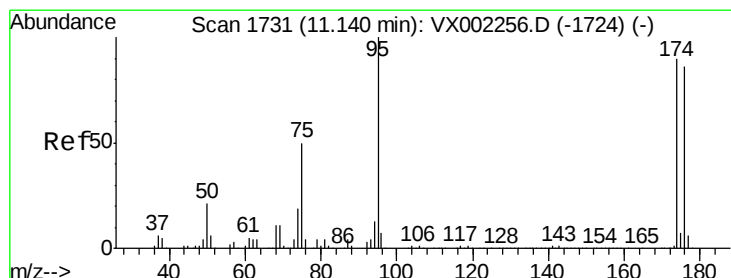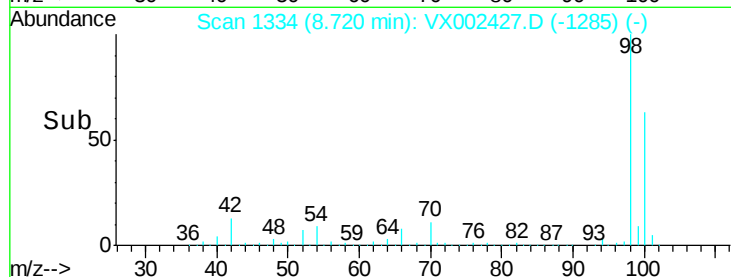

#62

4-Bromofluorobenzene

Concen: 40.65 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.00 min

Lab File: VX002427.D

Acq: 09 Jun 2018 17:56


Tgt Ion: 95 Resp: 142165

Ion Ratio Lower Upper

95 100

174 95.0 0.0 187.4

176 92.9 0.0 181.0

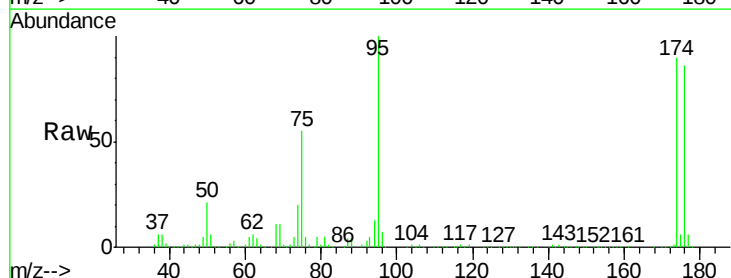

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

11.14

150000


100000

50000

0

Time-->

11.10 11.15 11.20




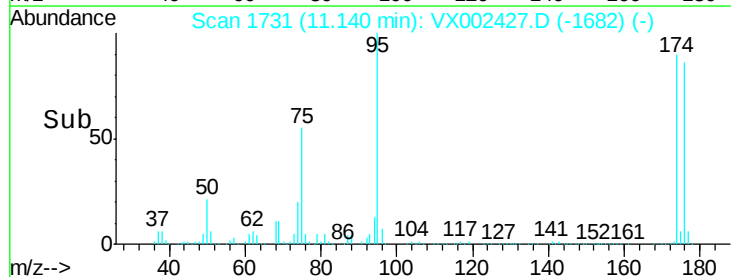




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. -0.00 min
Lab File: VX002427.D
Acq: 09 Jun 2018 17:56

Instrument :
MSVOA_X
ClientSampled :
W-24

Tot Ion:117 Resp: 266835
Ion Ratio Lower Upper
117 100
82 55.9 45.0 67.4
119 32.1 25.8 38.6

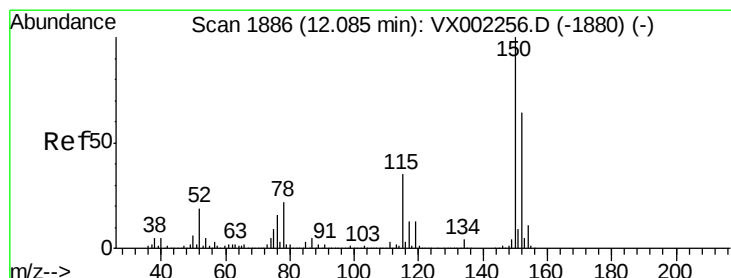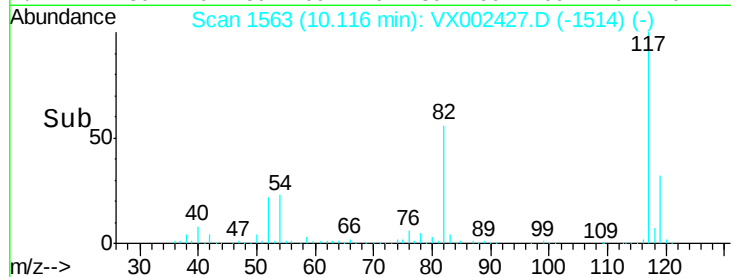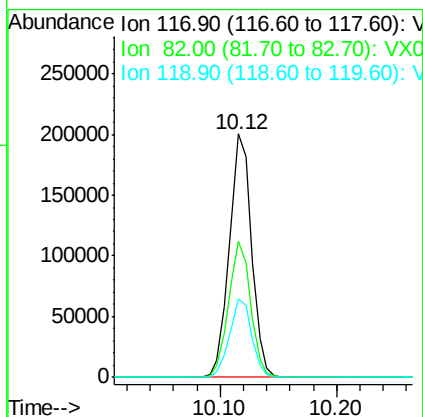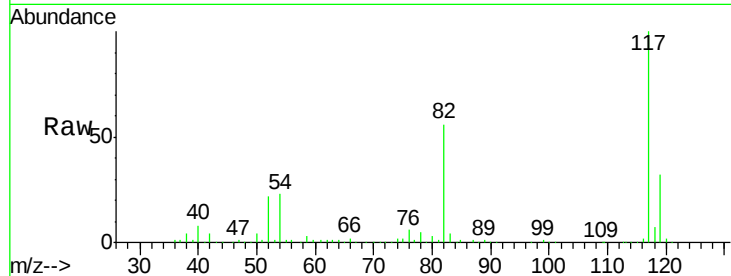

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.08 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX002427.D
Acq: 09 Jun 2018 17:56

Tgt Ion:152 Resp: 146888
Ion Ratio Lower Upper
152 100
115 54.5 40.1 120.2
150 157.0 0.0 347.2

