

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX060918\
 Data File : VX002427.D
 Acq On : 09 Jun 2018 17:56
 Operator : JC/MD
 Sample : J3396-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 W-24

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	94	rBV	1189029	1510363	100.00%	18.480%
2	1.270	109	112	115	rBV	61259	74969	4.96%	0.917%
3	1.319	115	120	140	rVV	126128	603004	39.92%	7.378%
4	2.453	301	306	310	rBV	10781	17754	1.18%	0.217%
5	2.623	329	334	342	rBV	22076	41432	2.74%	0.507%
6	5.507	794	807	822	rBV2	136234	385306	25.51%	4.714%
7	5.665	822	833	845	rVV	208526	582595	38.57%	7.128%
8	6.074	889	900	913	rBV	151212	393483	26.05%	4.814%
9	6.866	1019	1030	1046	rBV	307425	713603	47.25%	8.731%
10	8.720	1326	1334	1350	rBV	749396	1145469	75.84%	14.015%
11	10.116	1557	1563	1571	rBV	630263	839772	55.60%	10.275%
12	11.140	1726	1731	1737	rBV	618299	782050	51.78%	9.569%
13	12.085	1880	1886	1896	rBV	704597	913164	60.46%	11.173%
14	13.682	2145	2148	2150	rVV3	10656	15789	1.05%	0.193%
15	13.725	2152	2155	2159	rVB	13473	17879	1.18%	0.219%
16	13.914	2182	2186	2191	rBV4	12482	17722	1.17%	0.217%
17	13.987	2192	2198	2202	rBV3	17226	24567	1.63%	0.301%
18	14.548	2285	2290	2298	rBV5	17612	34494	2.28%	0.422%
19	14.676	2307	2311	2317	rBV8	11007	16380	1.08%	0.200%
20	14.816	2331	2334	2337	rBV	20582	22375	1.48%	0.274%
21	15.566	2453	2457	2460	rBV2	15475	20799	1.38%	0.254%


Sum of corrected areas: 8172969

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX060918\
Data File : VX002427.D
Acq On : 09 Jun 2018 17:56
Operator : JC/MD
Sample : J3396-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
W-24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

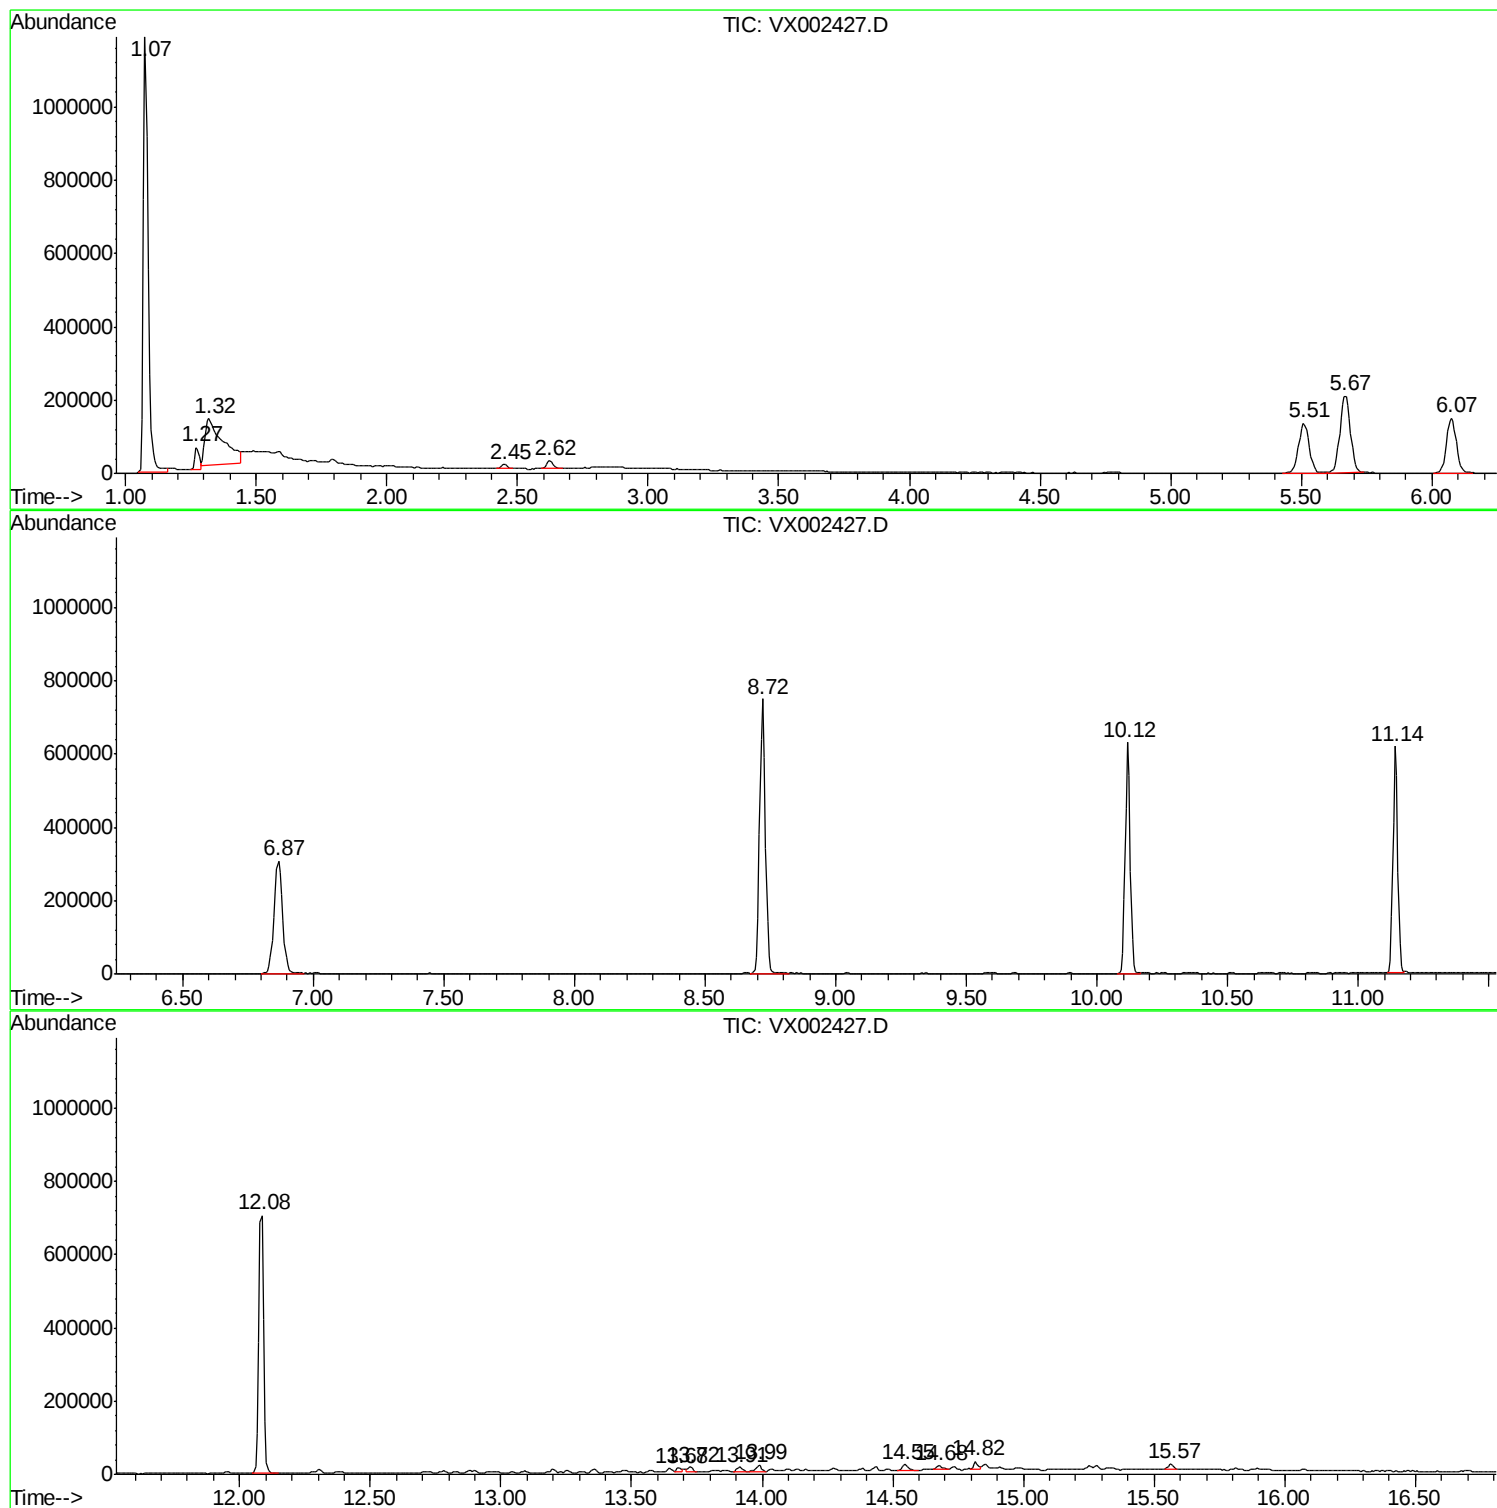

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX060918\
Data File : VX002427.D
Acq On : 09 Jun 2018 17:56
Operator : JC/MD
Sample : J3396-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
W-24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.27	6.43 ug/l	74969	Pentafluorobenzene	5.67

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	83
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
4			Ethyl Chloride	64	C2H5Cl	000075-00-3	3
5			Ethene, 1,2-difluoro-	64	C2H2F2	001691-13-0	3

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX060918\
Data File : VX002427.D
Acq On : 09 Jun 2018 17:56
Operator : JC/MD
Sample : J3396-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
W-24

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.27	6.4	ug/l	74969	1	5.67	582595	50.0