


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061118\
Data File : VX002435.D
Acq On : 11 Jun 2018 09:31
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Title : SW846 8260
Last Update : Tue Jun 05 03:22:35 2018

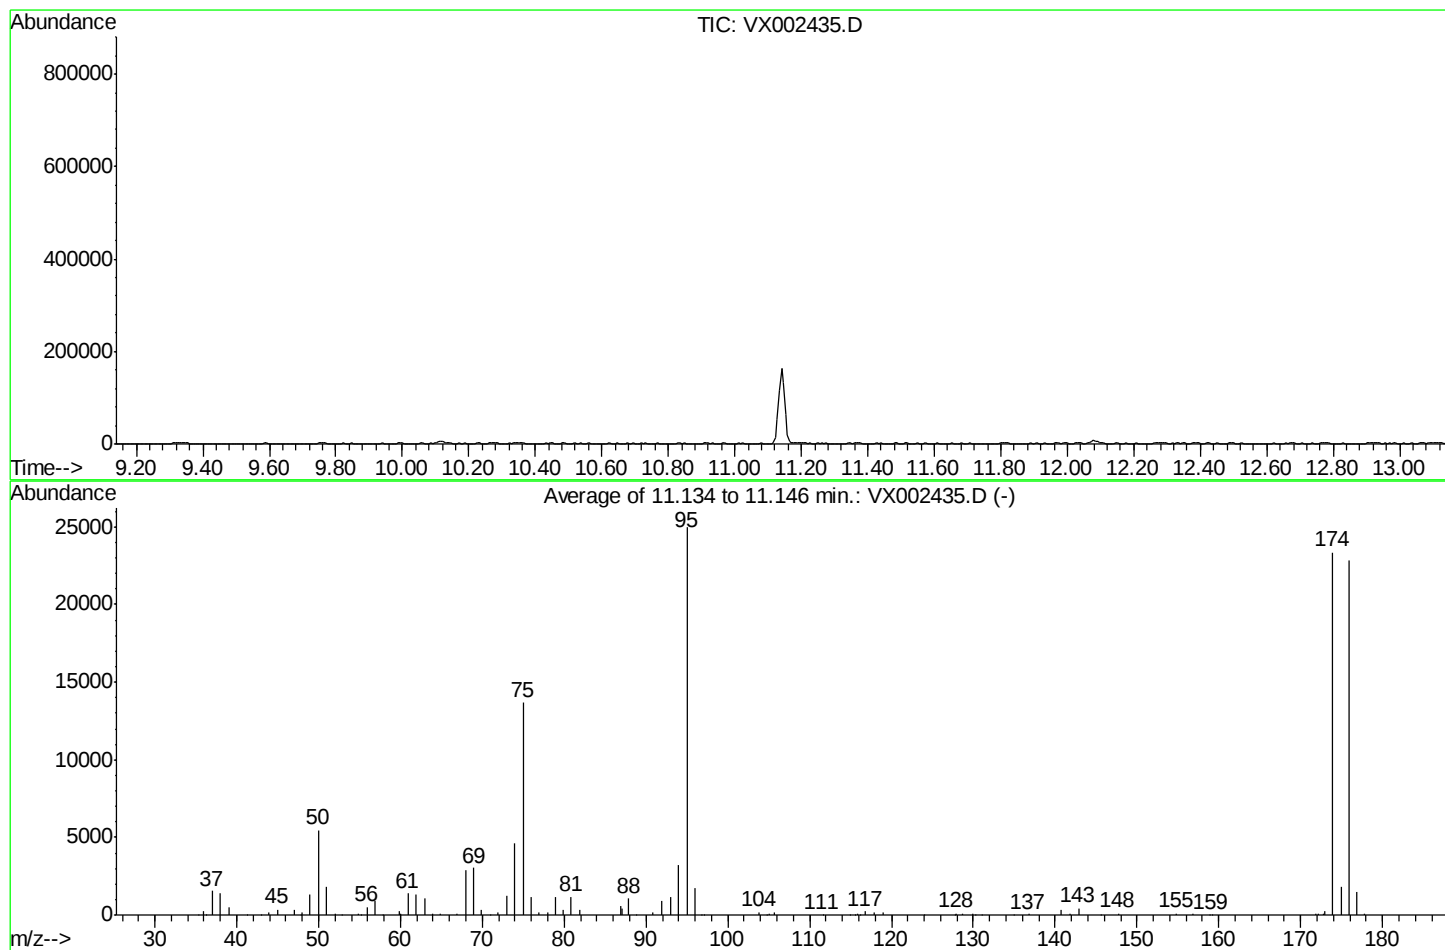

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	5480	PASS
75	95	30	60	54.8	13677	PASS
95	95	100	100	100.0	24973	PASS
96	95	5	9	6.8	1709	PASS
173	174	0.00	2	1.1	246	PASS
174	95	50	100	93.4	23336	PASS
175	174	5	9	7.8	1824	PASS
176	174	95	101	98.0	22866	PASS
177	176	5	9	6.6	1500	PASS