


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX061218\
Data File : VX002457.D
Acq On : 12 Jun 2018 09:35
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Title : SW846 8260
Last Update : Tue Jun 05 03:22:35 2018

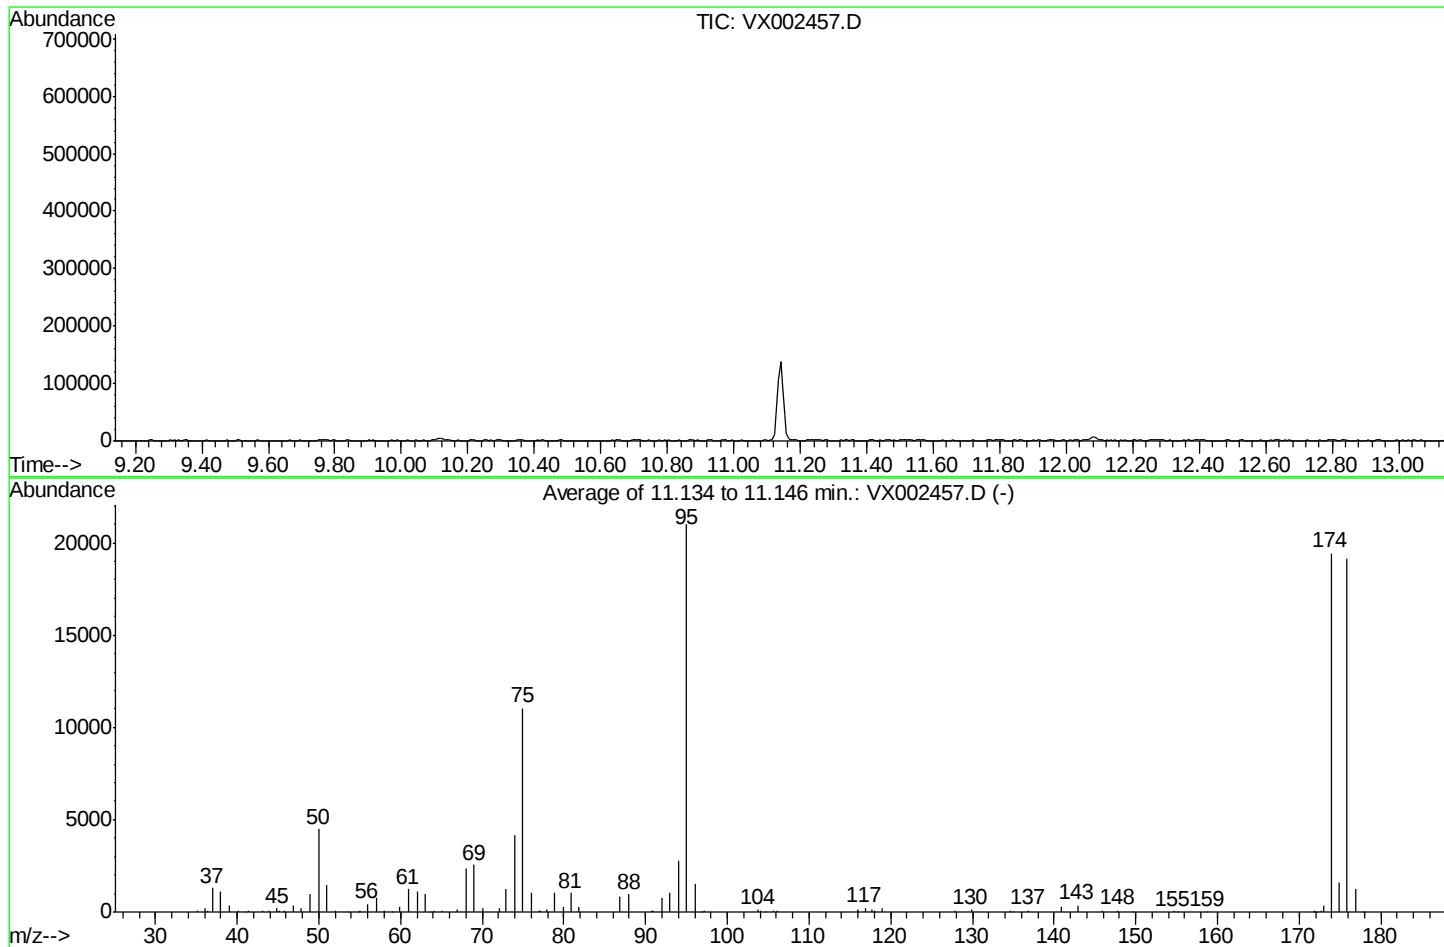

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	4492	PASS
75	95	30	60	52.7	11057	PASS
95	95	100	100	100.0	20997	PASS
96	95	5	9	7.2	1515	PASS
173	174	0.00	2	1.7	324	PASS
174	95	50	100	92.6	19440	PASS
175	174	5	9	8.1	1570	PASS
176	174	95	101	98.5	19139	PASS
177	176	5	9	6.4	1222	PASS