

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061318\
 Data File : VX002520.D
 Acq On : 13 Jun 2018 20:28
 Operator : JC/MD
 Sample : J3404-06 10X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SS050MW513-180607MSD

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	94	rBV	961467	1219691	100.00%	16.296%
2	1.489	144	148	156	rVB	57808	65752	5.39%	0.879%
3	1.611	160	168	170	rVB2	8848	16372	1.34%	0.219%
4	2.355	284	290	298	rBV	17082	29883	2.45%	0.399%
5	2.446	300	305	312	rBV	14615	25413	2.08%	0.340%
6	4.361	609	619	630	rBV3	17189	48331	3.96%	0.646%
7	4.605	651	659	666	rBV3	5135	15726	1.29%	0.210%
8	4.714	666	677	683	rBV2	15233	46011	3.77%	0.615%
9	5.507	794	807	820	rBV	134353	383980	31.48%	5.130%
10	5.665	822	833	849	rVB	203060	575838	47.21%	7.694%
11	6.074	889	900	916	rBV	152015	400623	32.85%	5.353%
12	6.866	1018	1030	1042	rBV	297097	700359	57.42%	9.358%
13	7.561	1137	1144	1153	rBV	18071	35045	2.87%	0.468%
14	7.671	1157	1162	1167	rBV3	8290	15800	1.30%	0.211%
15	7.738	1167	1173	1180	rVB	17455	33424	2.74%	0.447%
16	8.720	1327	1334	1343	rBV	743470	1155130	94.71%	15.434%
17	10.116	1557	1563	1577	rBV	645766	872945	71.57%	11.664%
18	11.140	1726	1731	1739	rBV	659943	824400	67.59%	11.015%
19	11.817	1839	1842	1851	rVB	9700	13843	1.13%	0.185%
20	11.908	1851	1857	1862	rBV3	8941	15996	1.31%	0.214%
21	12.085	1880	1886	1895	rBV	763738	989822	81.15%	13.225%


Sum of corrected areas: 7484384

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061318\
Data File : VX002520.D
Acq On : 13 Jun 2018 20:28
Operator : JC/MD
Sample : J3404-06 10X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SS050MW513-180607MSD

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

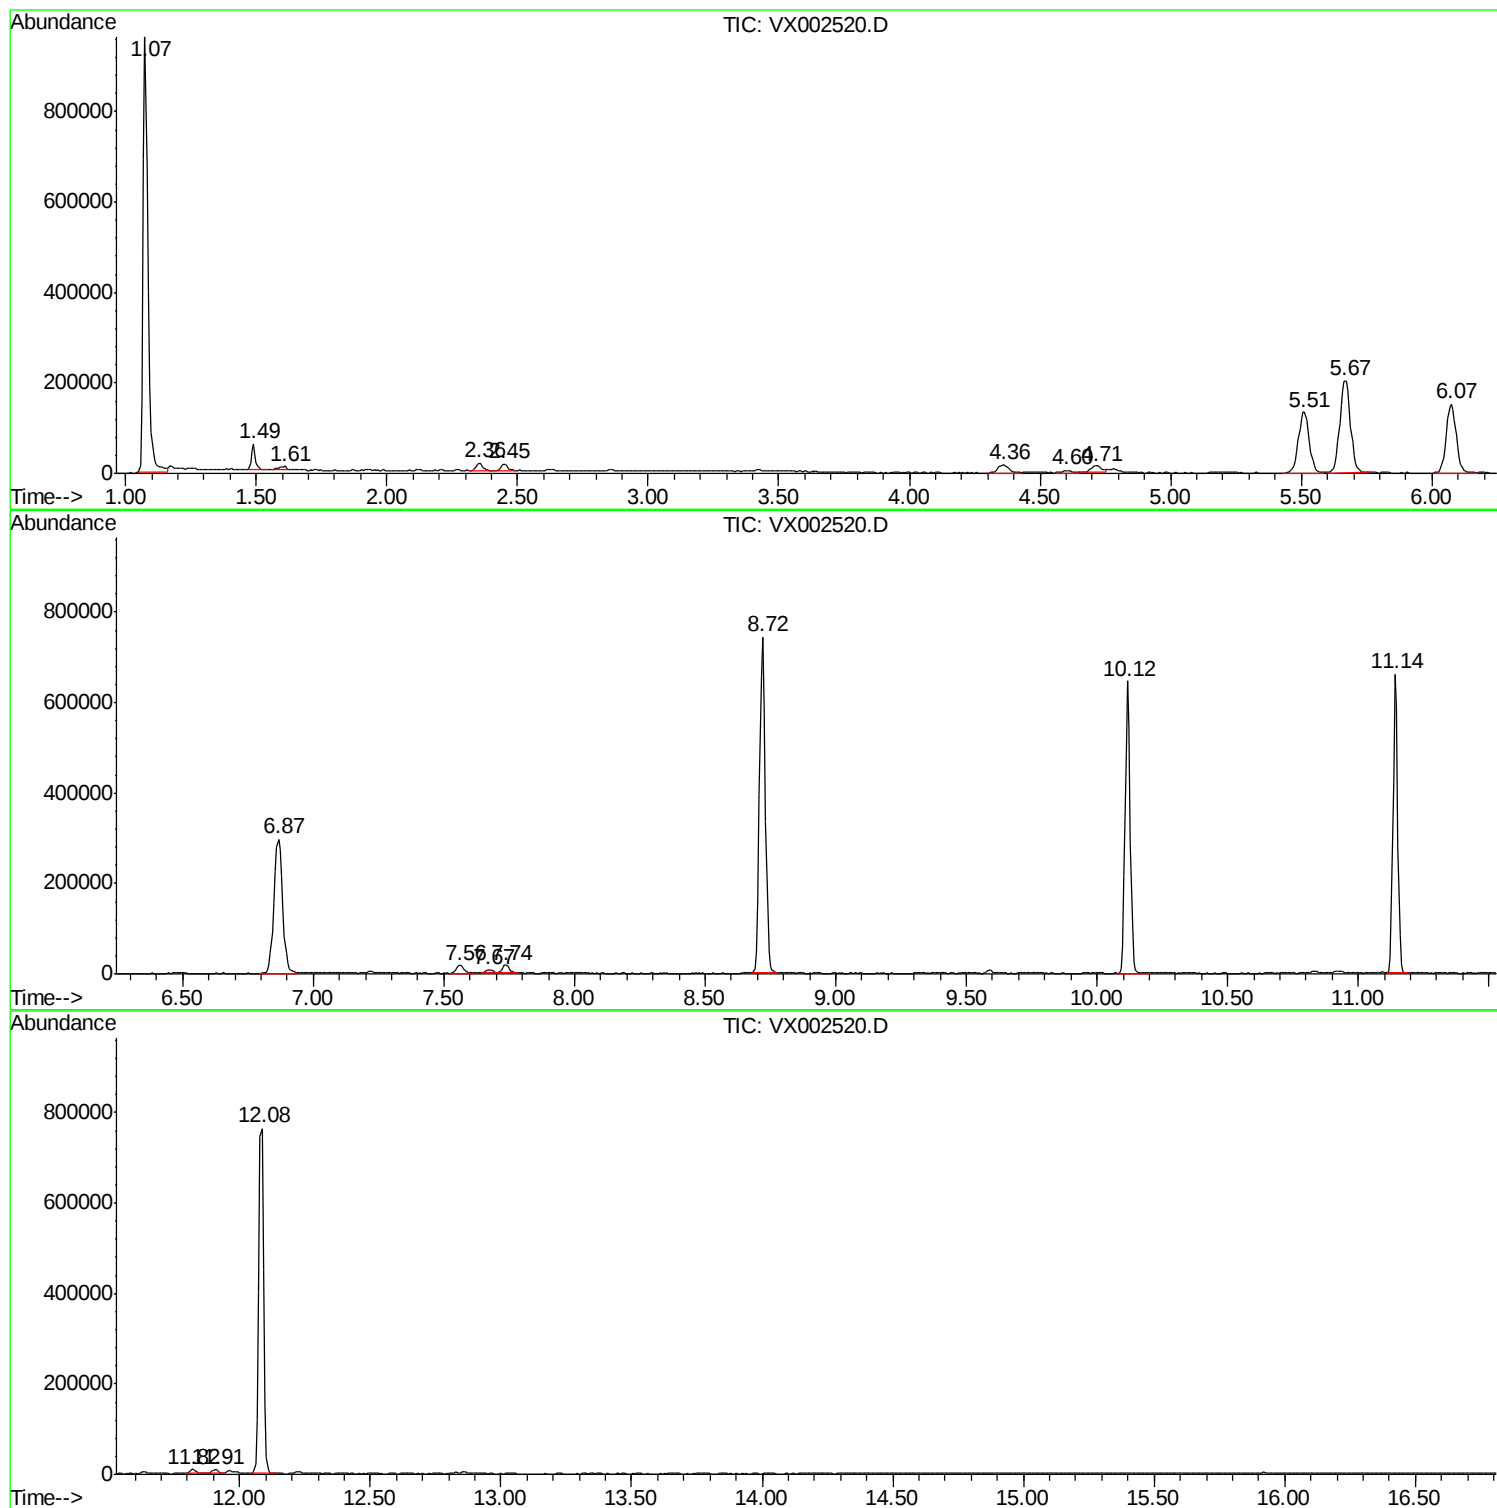

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX061318\
Data File : VX002520.D
Acq On : 13 Jun 2018 20:28
Operator : JC/MD
Sample : J3404-06 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SS050MW513-180607MSD

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.49 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.49	5.71 ug/l	65752	Pentafluorobenzene	5.67

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Acetaldehyde	44	C2H4O	000075-07-0	9
2			Propane	44	C3H8	000074-98-6	5
3			Ethylene oxide	44	C2H4O	000075-21-8	5
4			Propane, 1-chloro-2-methyl-	92	C4H9Cl	000513-36-0	5
5			Acetic acid, [(aminocarbonyl)ami...	132	C3H4N2O4	000585-05-7	4

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_X\DATA\VX061318\
Data File : VX002520.D
Acq On : 13 Jun 2018 20:28
Operator : JC/MD
Sample : J3404-06 10X
Misc : 5.0mL/MSV0A_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSV0A_X
ClientSampleId :
SS050MW513-180607MSD

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_X\METHOD\82X060418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.49	1.49	5.7	ug/l	65752	1	5.67	575838	50.0