


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX061318\
Data File : VX002523.D
Acq On : 13 Jun 2018 21:48
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Title : SW846 8260
Last Update : Tue Jun 05 03:22:35 2018

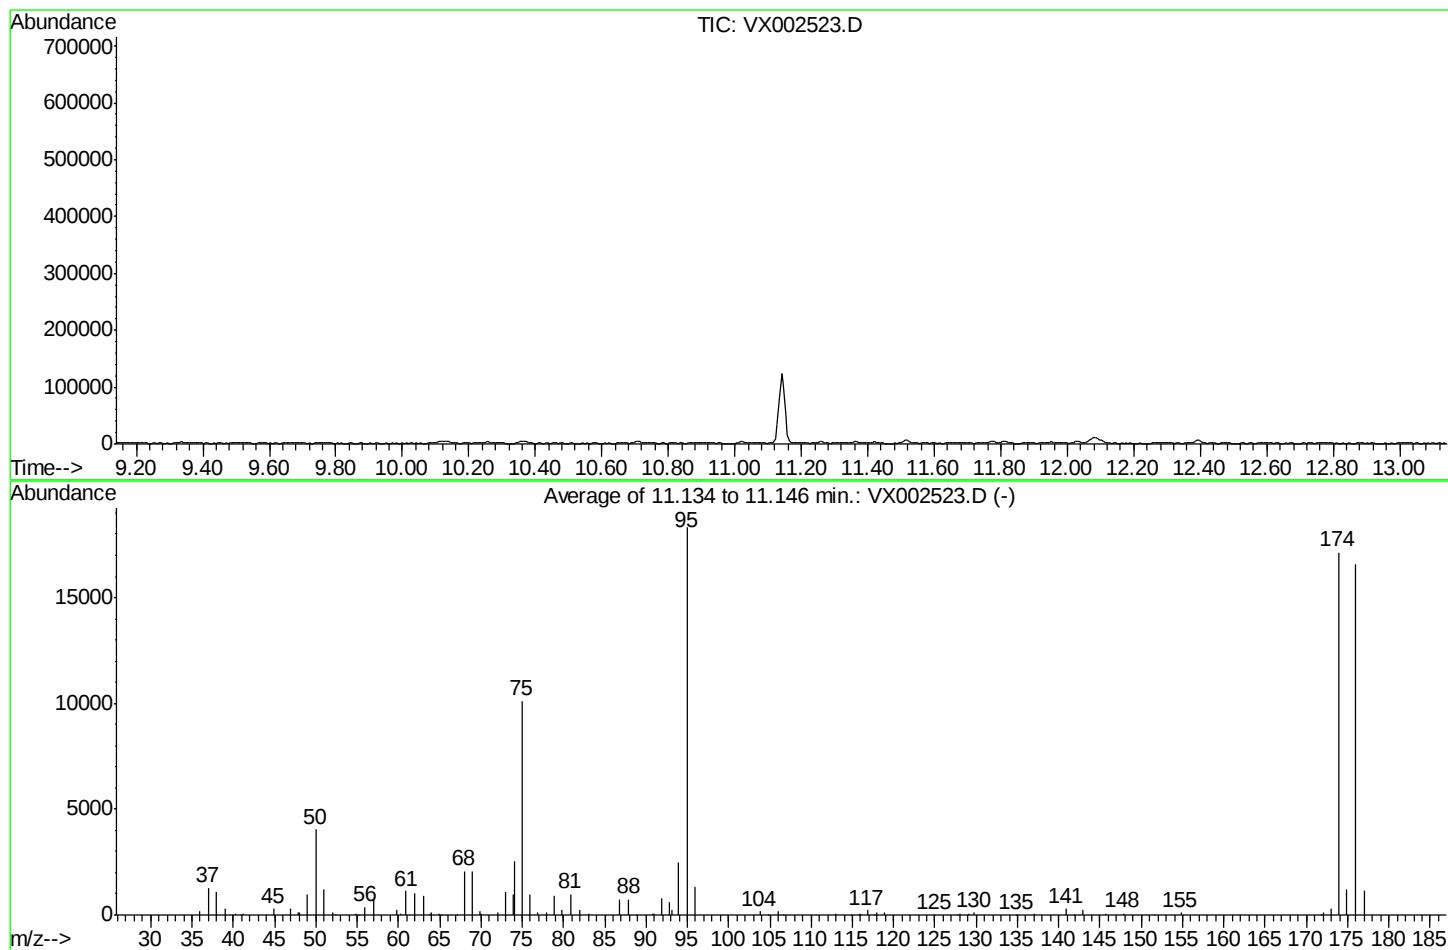

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	4041	PASS
75	95	30	60	55.3	10132	PASS
95	95	100	100	100.0	18320	PASS
96	95	5	9	7.3	1330	PASS
173	174	0.00	2	1.9	323	PASS
174	95	50	100	93.5	17126	PASS
175	174	5	9	7.2	1229	PASS
176	174	95	101	96.7	16561	PASS
177	176	5	9	7.0	1159	PASS