

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061418\
 Data File : VX002583.D
 Acq On : 15 Jun 2018 06:02
 Operator : JC/MD
 Sample : J3480-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jun 15 07:04:33 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 05 03:22:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	223532	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	324689	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	300004	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	171130	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	155874	48.67	ug/l	0.00
Spiked Amount			Recovery	=	97.34%	
35) Dibromofluoromethane	5.51	113	114613	44.89	ug/l	0.00
Spiked Amount			Recovery	=	89.78%	
50) Toluene-d8	8.72	98	466643	47.68	ug/l	0.00
Spiked Amount			Recovery	=	95.36%	
62) 4-Bromofluorobenzene	11.14	95	164344	43.55	ug/l	0.00
Spiked Amount			Recovery	=	87.10%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.32	50	458	Below Cal		99
5) Bromomethane	1.67	94	758	Below Cal	#	63
8) Diethyl Ether	2.20	74	261	Below Cal	#	30
11) Tert butyl alcohol	3.07	59	1221	Below Cal	#	39
13) Acrolein	2.28	56	206	Below Cal	#	71
15) Acrylonitrile	3.17	53	202	Below Cal	#	17
16) Acetone	2.45	43	21559	Below Cal		97
18) Methyl Acetate	2.78	43	22817	4.68	ug/l	98
19) Methyl tert-butyl Ether	3.09	73	21	Below Cal	#	1
20) Methylene Chloride	2.86	84	9752	1.16	ug/l	97
22) Diisopropyl ether	3.92	45	211	Below Cal	#	44
25) 2-Butanone	4.72	43	5119	2.34	ug/l	96
28) Bromochloromethane	5.02	49	62	Below Cal	#	13
29) Tetrahydrofuran	5.18	42	2099	1.49	ug/l	90
30) Chloroform	5.22	83	2336	0.47	ug/l	91
36) 1,1-Dichloropropene	5.67	75	15206	4.45	ug/l	# 52
38) Carbon Tetrachloride	5.67	117	20840	5.84	ug/l	# 16
39) Methylcyclohexane	7.47	83	118	0.29	ug/l	# 47
44) Trichloroethene	7.22	130	705	0.24	ug/l	97
47) Bromodichloromethane	7.90	83	847	0.24	ug/l	# 74
51) 4-Methyl-2-Pentanone	8.65	43	2382	0.55	ug/l	98
65) Chlorobenzene	10.14	112	3222	0.43	ug/l	95
68) m/p-Xylenes	10.36	106	1463	0.30	ug/l	92
76) 1,2,3-Trichloropropane	11.14	75	88490	23.57	ug/l	# 33
80) 1,3,5-Trimethylbenzene	11.51	105	2354	0.23	ug/l	96
81) trans-1,4-Dichloro-2-buten	11.14	75	88490	82.61	ug/l	# 6
84) 1,2,4-Trimethylbenzene	11.81	105	8504	0.81	ug/l	99
86) p-Isopropyltoluene	12.07	119	2267	0.21	ug/l	# 67
95) Naphthalene	13.84	128	133486	10.72	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061418\
Data File : VX002583.D
Acq On : 15 Jun 2018 06:02
Operator : JC/MD
Sample : J3480-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jun 15 07:04:33 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 05 03:22:35 2018
Response via : Initial Calibration

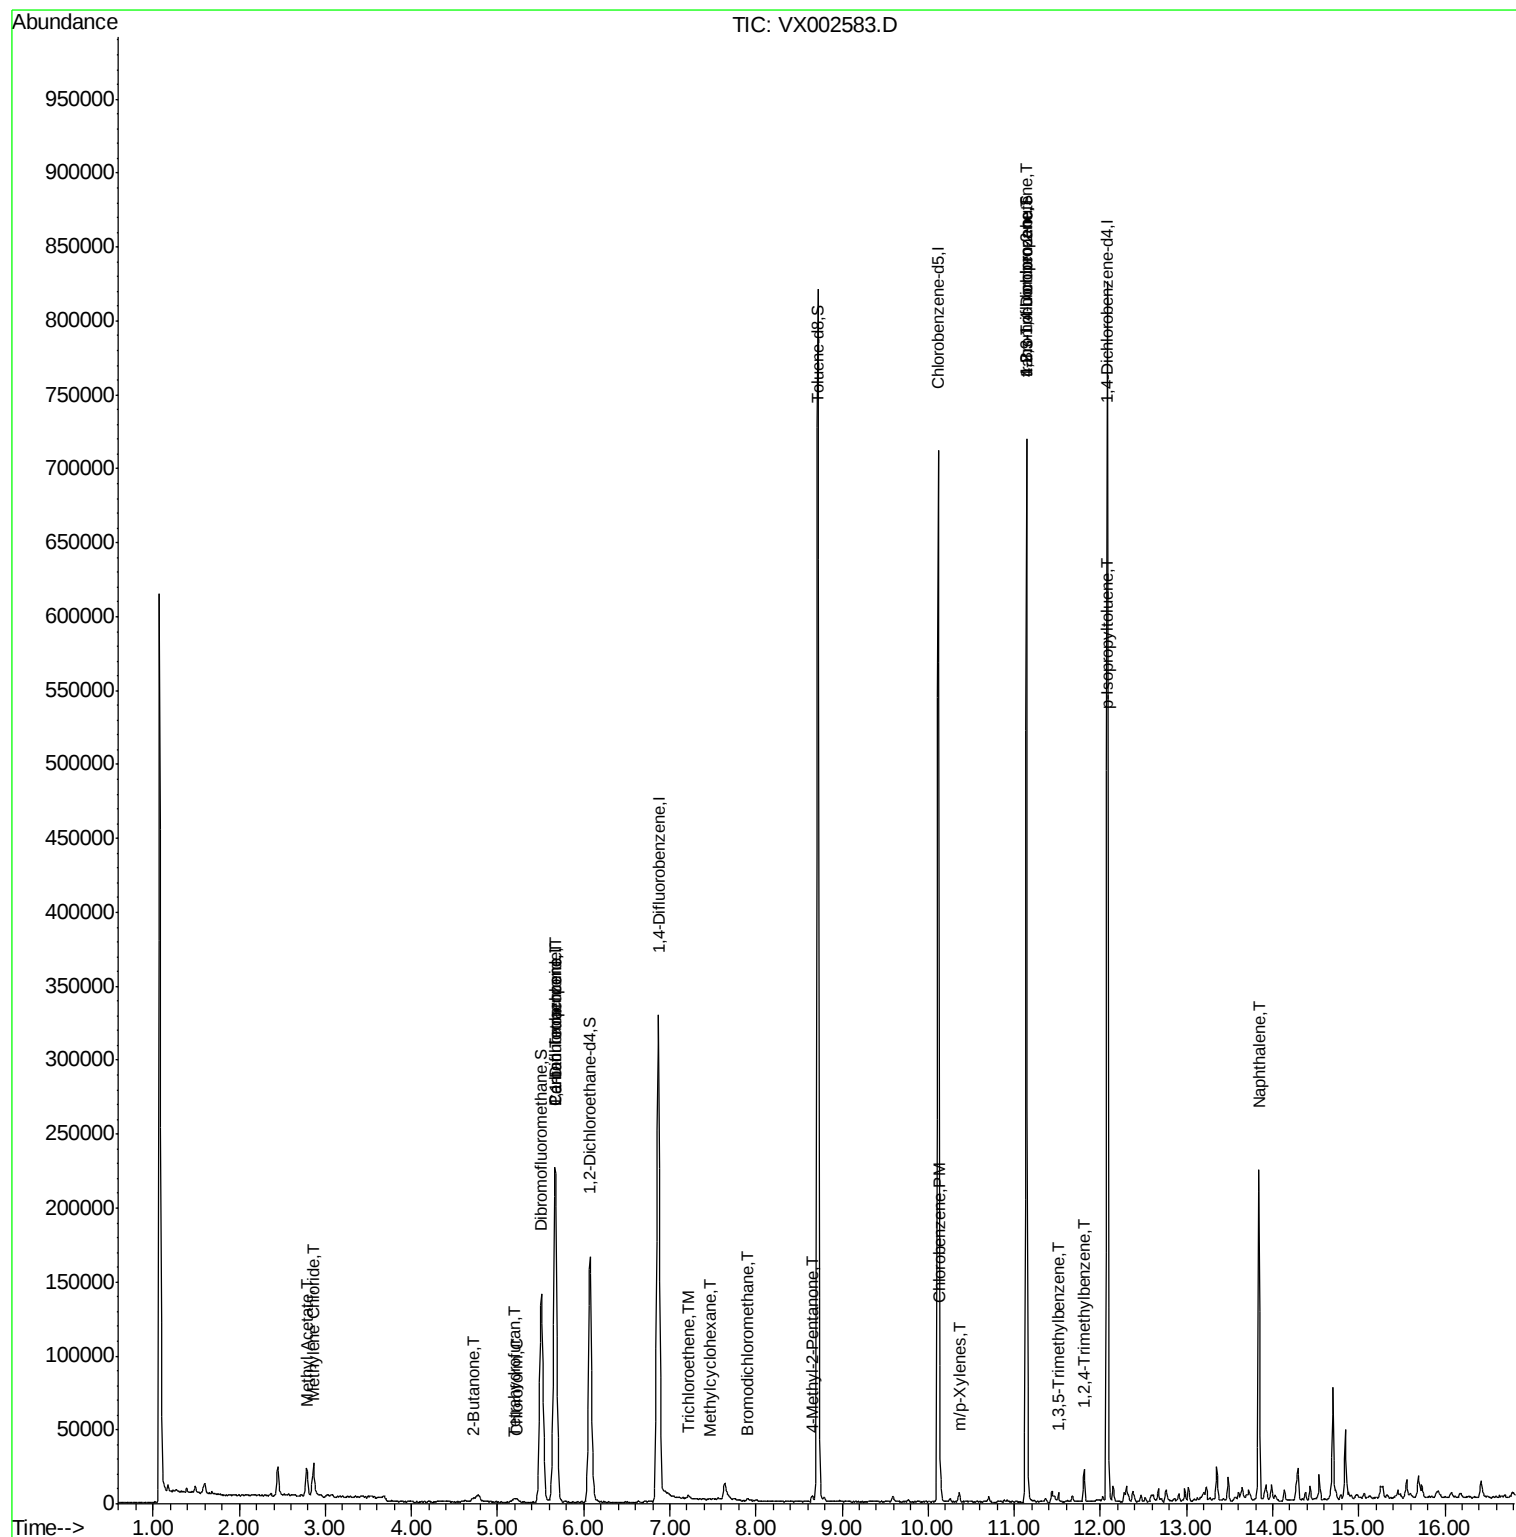



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.01 min

Lab File: VX002583.D

Acq: 15 Jun 2018 06:02

Instrument :

MSVOA_X


ClientSampled :

Tot Ion:168 Resp: 223532

Ion Ratio Lower Upper




168 100

99 53.7 39.3 58.9

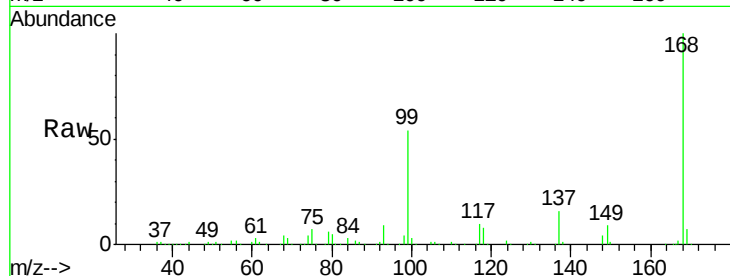

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

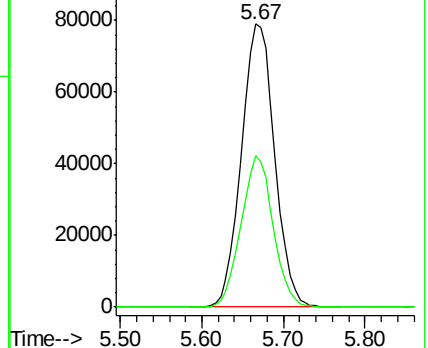

#3

Chloromethane

Concen: Below Cal

RT: 1.32 min Scan# 121

Delta R.T. 0.00 min

Lab File: VX002583.D


Acq: 15 Jun 2018 06:02

Tgt Ion: 50 Resp: 458

Ion Ratio Lower Upper



50 100

52 31.6 25.7 38.5



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

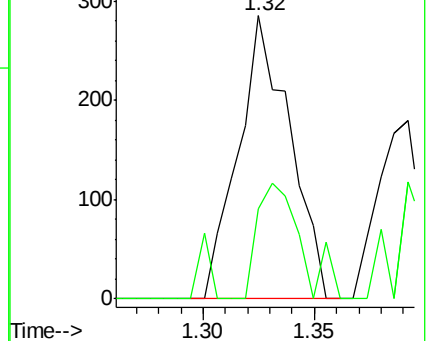



#5

Bromomethane

Concen: Below Cal

RT: 1.67 min Scan# 177

Delta R.T. 0.03 min

Lab File: VX002583.D

Acq: 15 Jun 2018 06:02

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 94 Resp: 758

Ion Ratio Lower Upper

94 100

96 57.8 74.9 112.3#

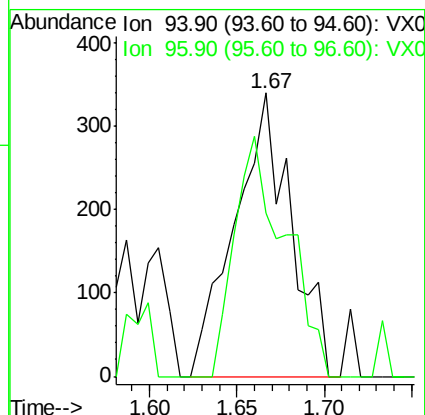

#8

Diethyl Ether

Concen: Below Cal

RT: 2.20 min Scan# 264

Delta R.T. 0.01 min

Lab File: VX002583.D




Acq: 15 Jun 2018 06:02


Tgt Ion: 74 Resp: 261

Ion Ratio Lower Upper

74 100

45 178.9 53.1 159.4#



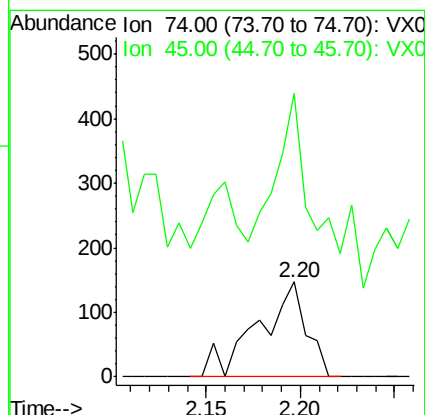



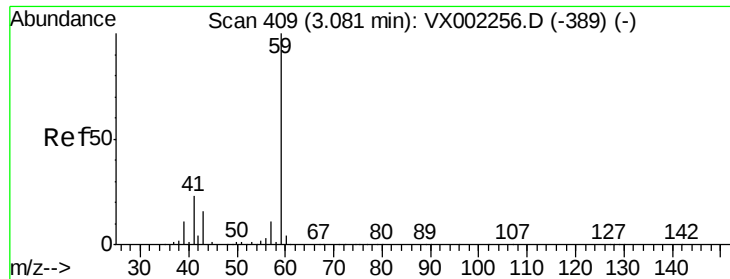

#11
Tert butyl alcohol
Concen: Below Cal
RT: 3.07 min Scan# 407
Delta R.T. -0.01 min
Lab File: VX002583.D
Acq: 15 Jun 2018 06:02




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 59 Resp: 1221
Ion Ratio Lower Upper
59 100
57 33.1 8.2 12.2#

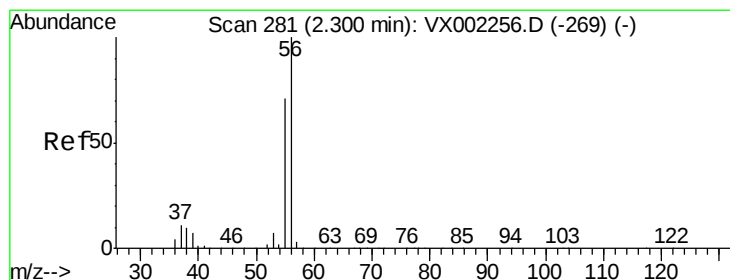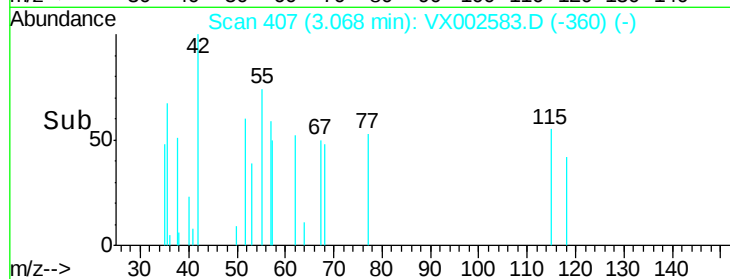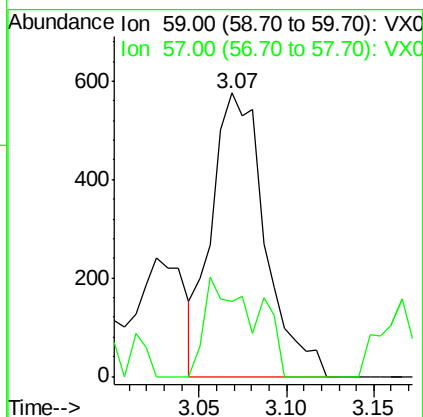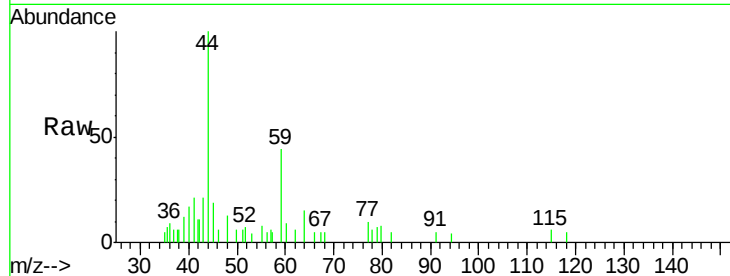

#13
Acrolein
Concen: Below Cal
RT: 2.28 min Scan# 278
Delta R.T. -0.02 min
Lab File: VX002583.D
Acq: 15 Jun 2018 06:02

Tgt Ion: 56 Resp: 206
Ion Ratio Lower Upper
56 100
55 47.1 57.0 85.4#

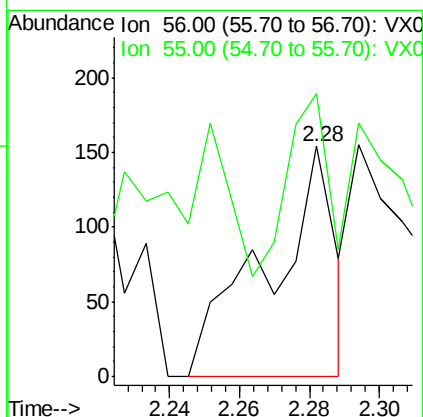



#15

Acrylonitrile

Concen: Below Cal

RT: 3.17 min Scan# 423

Delta R.T. 0.01 min

Lab File: VX002583.D

Acq: 15 Jun 2018 06:02

Instrument :

MSVOA_X

ClientSampled :


Tot Ion: 53 Resp: 202

Ion Ratio Lower Upper

53 100

52 0.0 66.7 100.1#


51 0.0 29.9 44.9#





Abundance Ion 53.00 (52.70 to 53.70): VX0

Ion 52.00 (51.70 to 52.70): VX0

Ion 51.00 (50.70 to 51.70): VX0

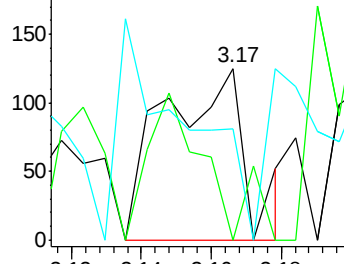

Time-->



#16

Acetone

Concen: Below Cal

RT: 2.45 min Scan# 305

Delta R.T. -0.01 min

Lab File: VX002583.D


Acq: 15 Jun 2018 06:02

Tgt Ion: 43 Resp: 21559

Ion Ratio Lower Upper


43 100

58 25.8 22.1 33.1





Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

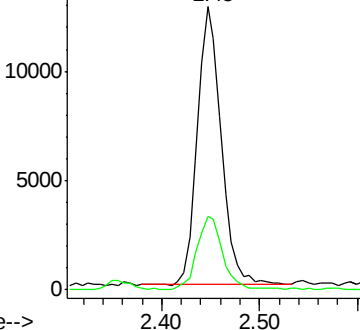

Time-->









#18
Methyl Acetate
Concen: 4.68 ug/l
RT: 2.78 min Scan# 360
Delta R.T. -0.00 min
Lab File: VX002583.D
Acq: 15 Jun 2018 06:02




Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 43 Resp: 22817
Ion Ratio Lower Upper
43 100
74 21.7 16.7 25.1

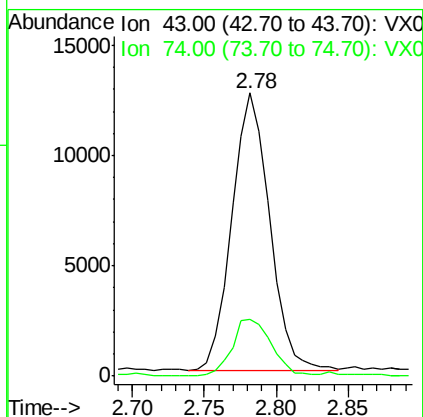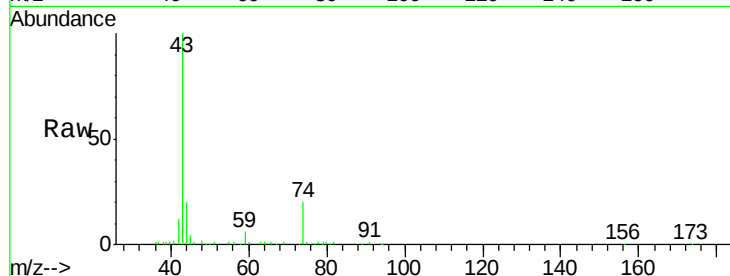

#19
Methyl tert-butyl Ether
Concen: Below Cal
RT: 3.09 min Scan# 410
Delta R.T. -0.12 min
Lab File: VX002583.D
Acq: 15 Jun 2018 06:02

Tgt Ion: 73 Resp: 21
Ion Ratio Lower Upper
73 100
57 165.5 17.7 26.5#



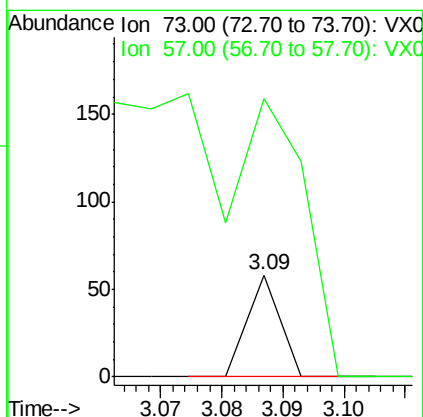



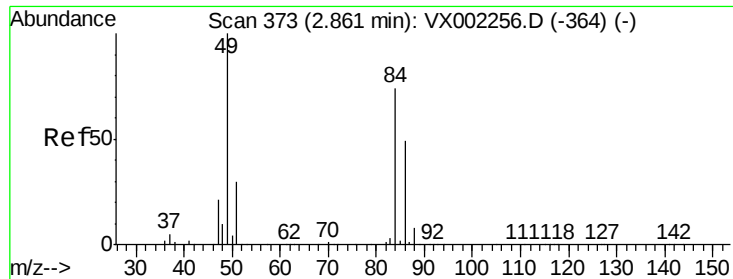

#20
Methvlene Chloride
Concen: 1.16 ua/l
RT: 2.86 min Scan# 373
Delta R.T. 0.00 min
Lab File: VX002583.D
Acq: 15 Jun 2018 06:02




Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 84 Resp: 9752
Ion Ratio Lower Upper
84 100
49 138.4 107.8 161.6
51 40.6 32.8 49.2
86 62.4 52.5 78.7

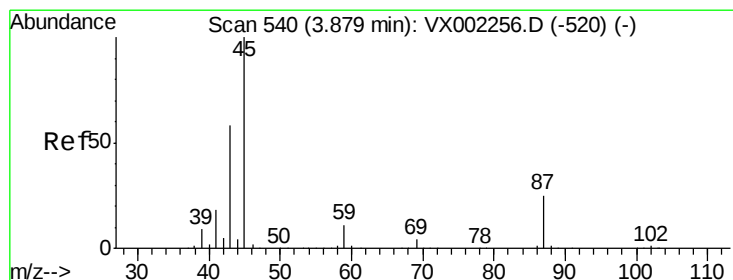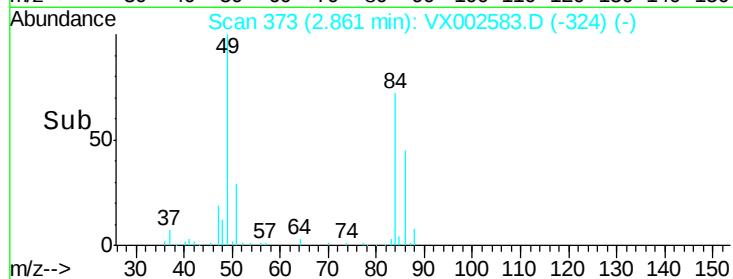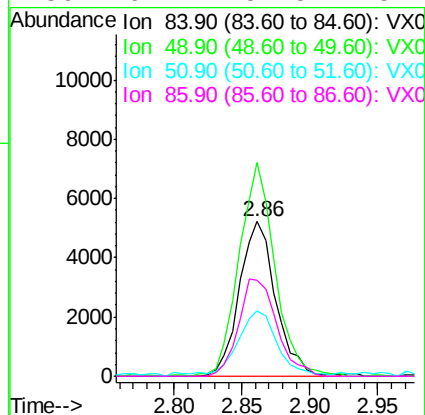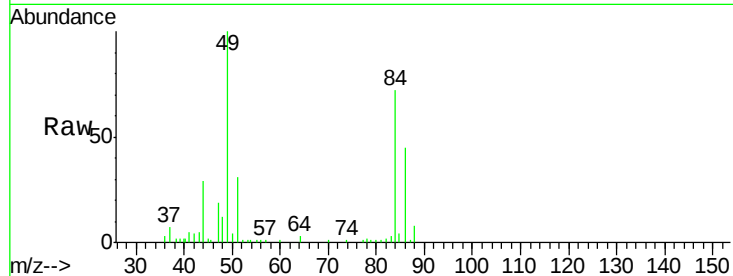

#22
Diisopropyl ether
Concen: Below Cal
RT: 3.92 min Scan# 546
Delta R.T. 0.04 min
Lab File: VX002583.D
Acq: 15 Jun 2018 06:02

Tgt Ion: 45 Resp: 211
Ion Ratio Lower Upper
45 100
43 11.2 46.8 70.2#
87 0.0 20.2 30.4#
59 0.0 8.7 13.1#

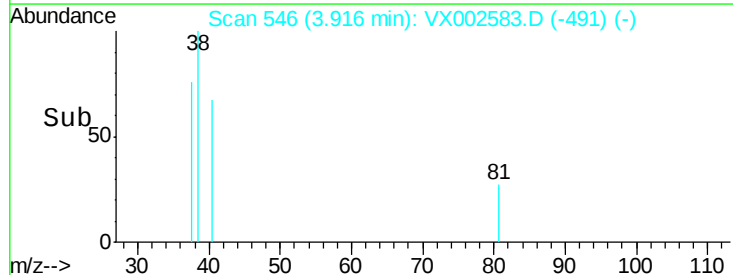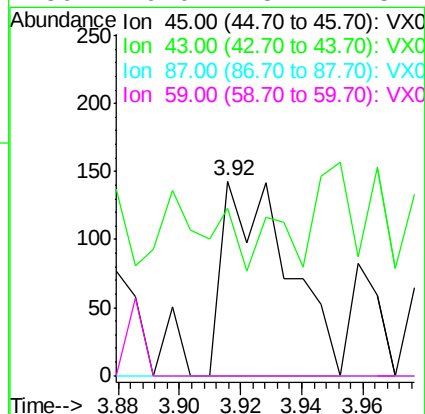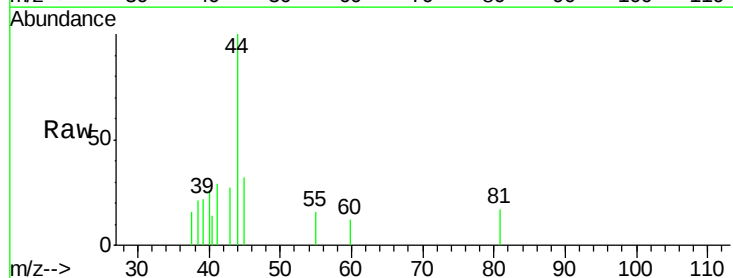

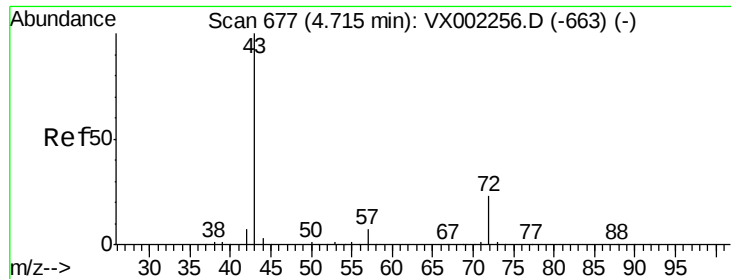

#25

2-Butanone

Concen: 2.34 ug/l

RT: 4.72 min Scan# 678

Delta R.T. 0.01 min

Lab File: VX002583.D

Acq: 15 Jun 2018 06:02

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 43 Resp: 5119

Ion Ratio Lower Upper

43 100

72 24.9 18.5 27.7

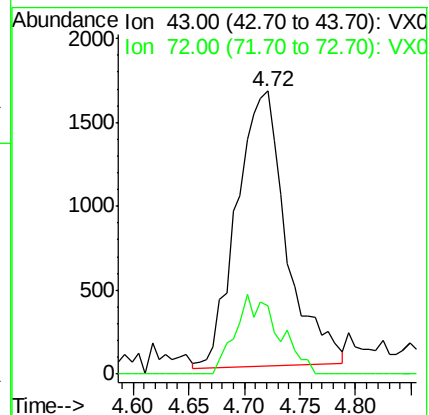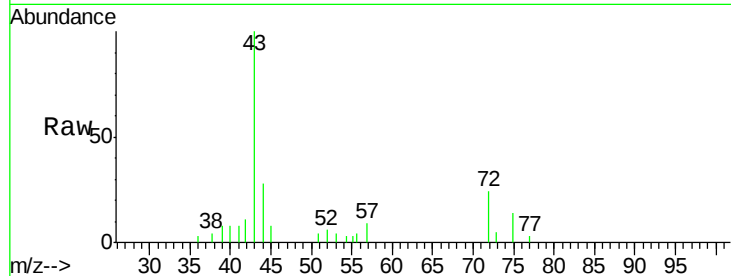

#28

Bromochloromethane

Concen: Below Cal

RT: 5.02 min Scan# 727

Delta R.T. -0.01 min

Lab File: VX002583.D

Acq: 15 Jun 2018 06:02




Tgt Ion: 49 Resp: 62


Ion Ratio Lower Upper

49 100

129 0.0 0.0 4.2

130 0.0 61.2 91.8#


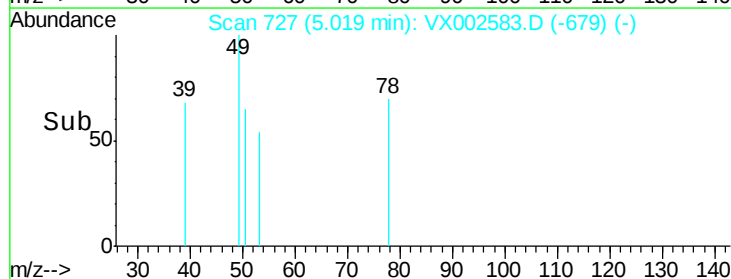
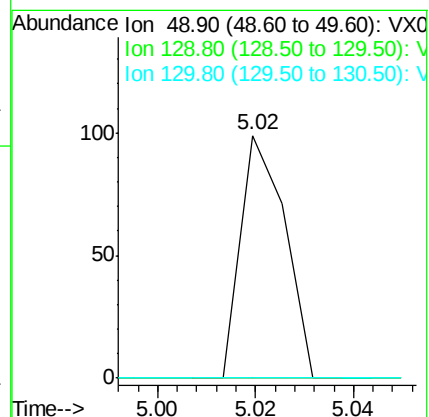





#29
Tetrahydrofuran
Concen: 1.49 ug/l
RT: 5.18 min Scan# 754
Delta R.T. 0.02 min
Lab File: VX002583.D
Acq: 15 Jun 2018 06:02




Instrument :
MSVOA_X
ClientSampleId :

Tot Ion: 42 Resp: 2099
Ion Ratio Lower Upper
42 100
72 34.5 32.0 48.0
71 31.3 30.1 45.1

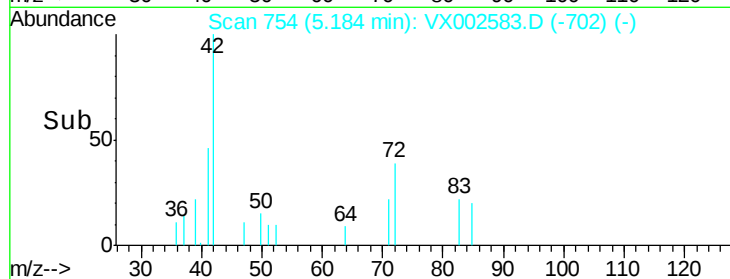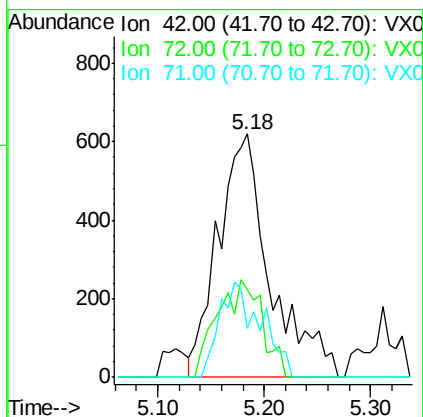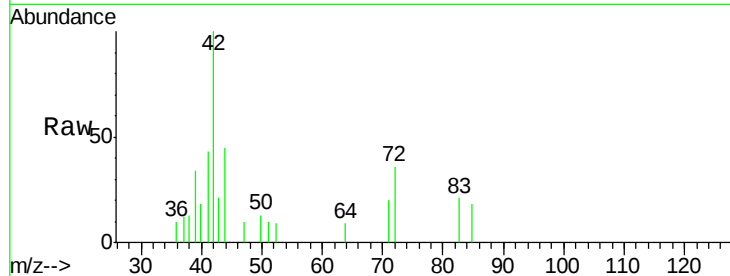

#30
Chloroform
Concen: 0.47 ug/l
RT: 5.22 min Scan# 760
Delta R.T. -0.00 min
Lab File: VX002583.D
Acq: 15 Jun 2018 06:02

Tgt Ion: 83 Resp: 2336
Ion Ratio Lower Upper
83 100
85 55.8 50.4 75.6


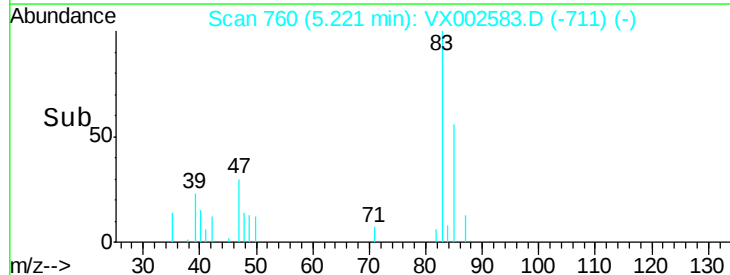
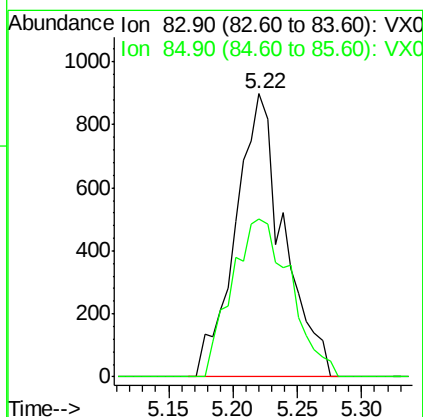





#33
 1,2-Dichloroethane-d4
 Concen: 48.67 ug/l
 RT: 6.07 min Scan# 900
 Delta R.T. 0.00 min
 Lab File: VX002583.D
 Acq: 15 Jun 2018 06:02




Instrument :
 MSVOA_X
 ClientSampleId :


Tot Ion: 65 Resp: 155874
 Ion Ratio Lower Upper
 65 100
 67 51.8 0.0 102.6

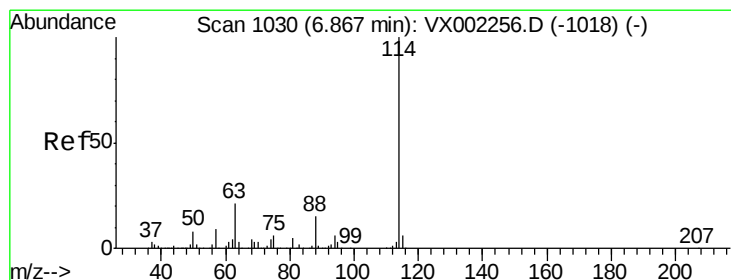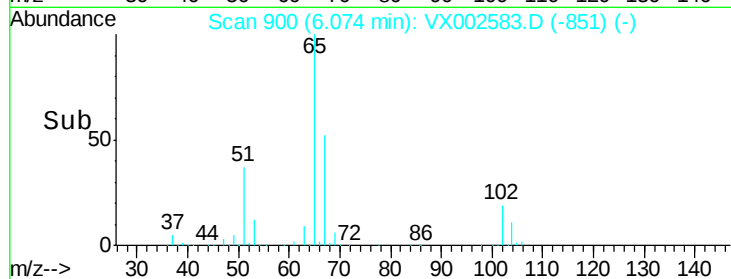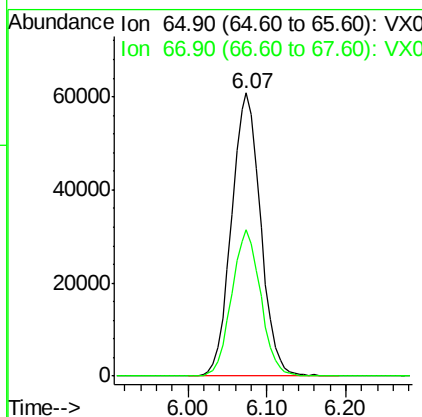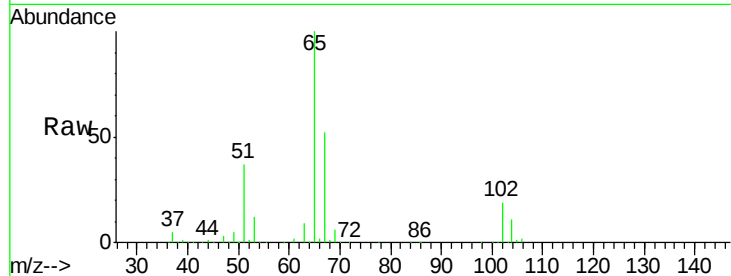

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.87 min Scan# 1030
 Delta R.T. -0.00 min
 Lab File: VX002583.D
 Acq: 15 Jun 2018 06:02

Tgt Ion: 114 Resp: 324689
 Ion Ratio Lower Upper
 114 100
 63 20.0 0.0 41.4
 88 14.3 0.0 30.0


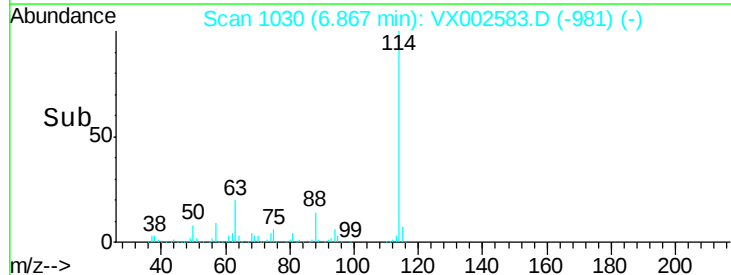
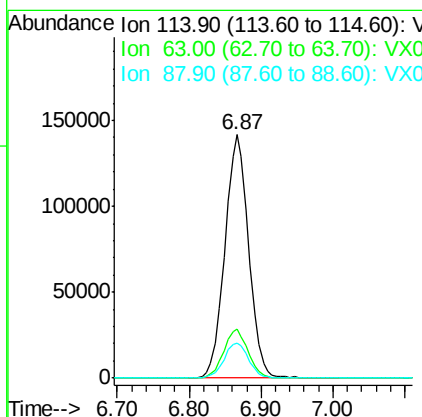



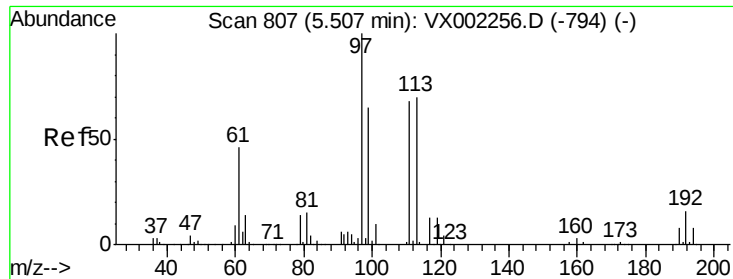

#35
 Dibromofluoromethane
 Concen: 44.89 ug/l
 RT: 5.51 min Scan# 807
 Delta R.T. -0.00 min
 Lab File: VX002583.D
 Acq: 15 Jun 2018 06:02




Instrument :
 MSVOA_X
 ClientSampled :


Tot Ion:113 Resp: 114613
 Ion Ratio Lower Upper
 113 100
 111 103.4 81.4 122.0
 192 23.1 19.1 28.7

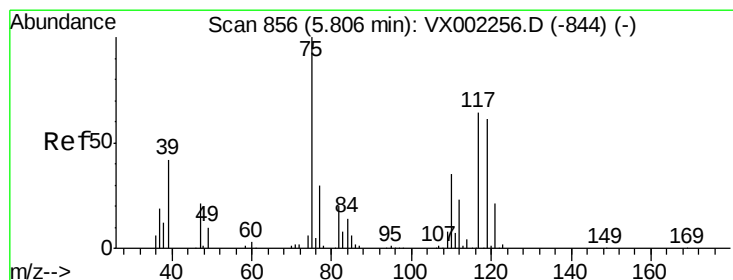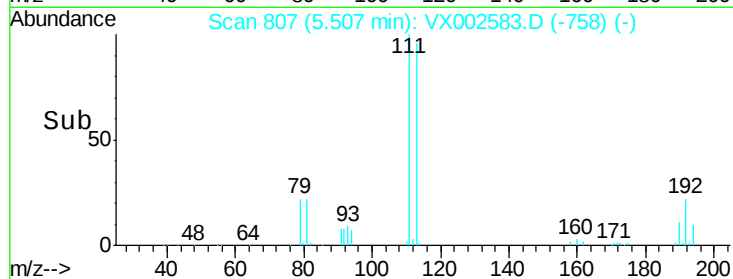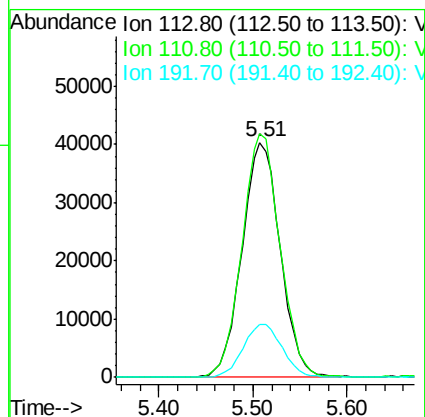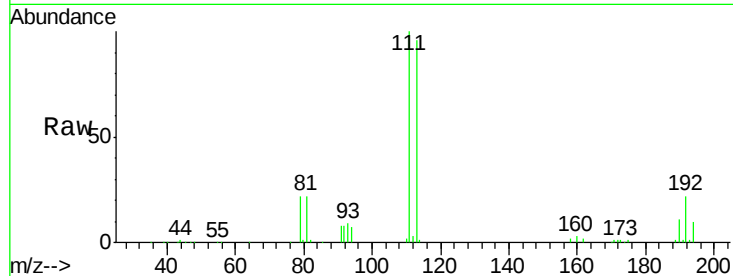

#36
 1,1-Dichloropropene
 Concen: 4.45 ug/l
 RT: 5.67 min Scan# 833
 Delta R.T. -0.14 min
 Lab File: VX002583.D
 Acq: 15 Jun 2018 06:02

Tgt Ion: 75 Resp: 15206
 Ion Ratio Lower Upper
 75 100
 110 11.5 18.1 54.4#
 77 0.3 24.3 36.5#

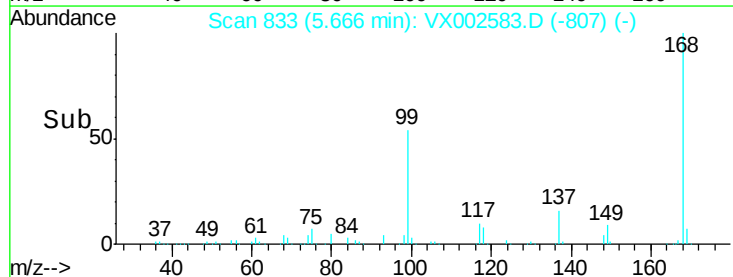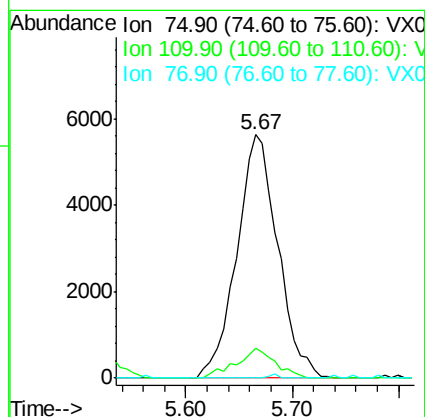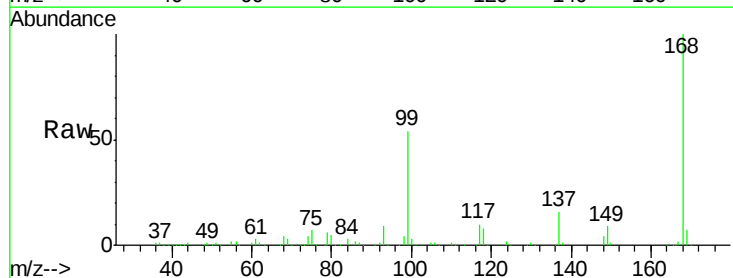

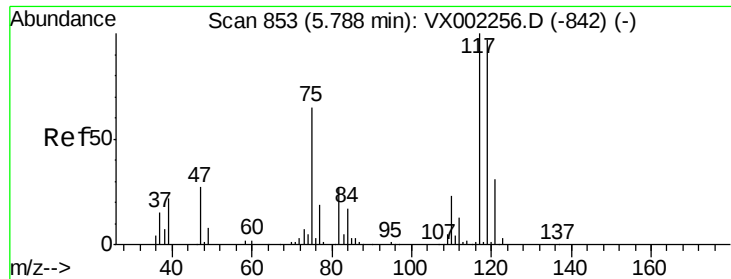

#38

Carbon Tetrachloride

Concen: 5.84 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.12 min

Lab File: VX002583.D

Acq: 15 Jun 2018 06:02

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:117 Resp: 20840

Ion Ratio Lower Upper

117 100

119 5.0 77.4 116.0#




121 0.0 24.4 36.6#

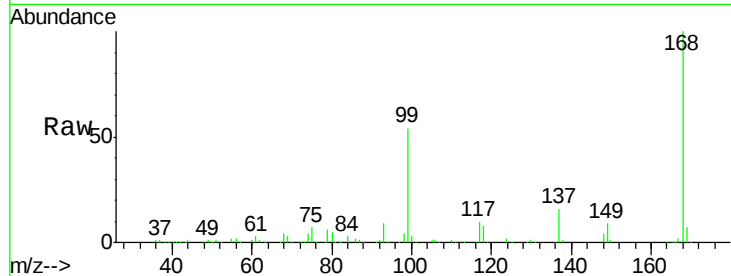

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

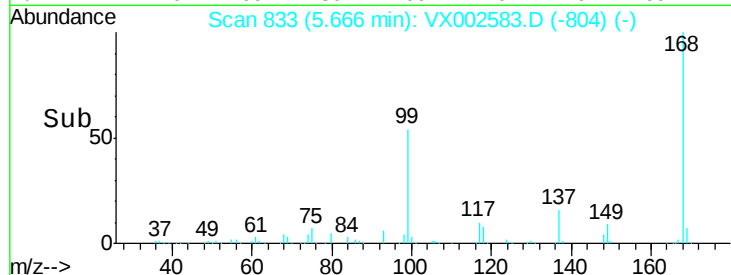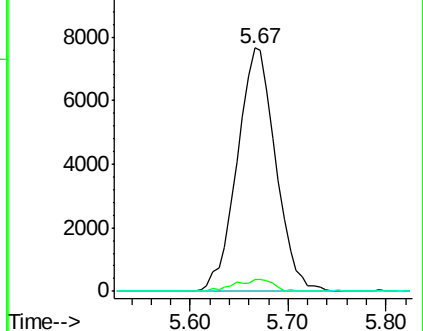

#39

Methylcyclohexane

Concen: 0.29 ug/l

RT: 7.47 min Scan# 1129

Delta R.T. 0.01 min

Lab File: VX002583.D

Acq: 15 Jun 2018 06:02


Tgt Ion: 83 Resp: 118

Ion Ratio Lower Upper

83 100

55 119.8 65.4 98.0#



98 0.0 37.4 56.0#

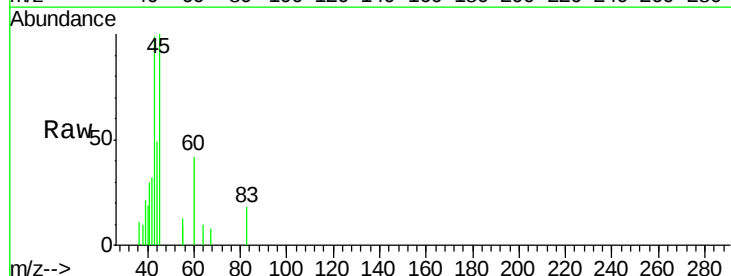


Abundance Ion 83.00 (82.70 to 83.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 98.00 (97.70 to 98.70): VX0

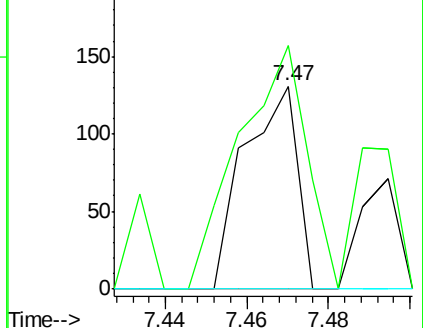

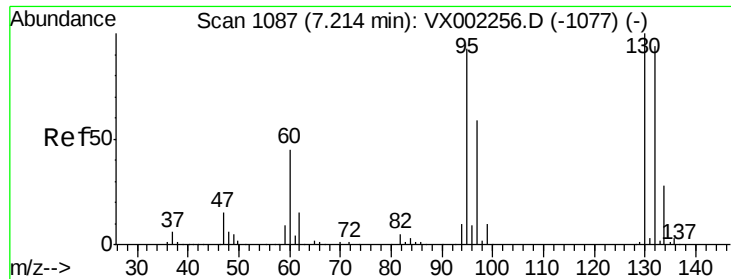

#44

Trichloroethene

Concen: 0.24 ug/l

RT: 7.22 min Scan# 1088

Delta R.T. 0.01 min

Lab File: VX002583.D

Acq: 15 Jun 2018 06:02

Instrument :

MSVOA_X


ClientSampled :

Tot Ion:130 Resp: 705

Ion Ratio Lower Upper




130 100

95 95.2 0.0 185.4

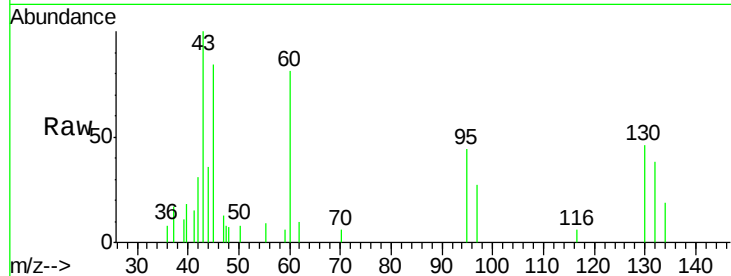

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

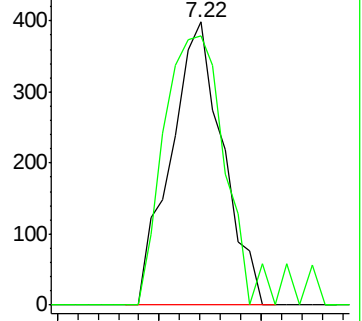

#47

Bromodichloromethane

Concen: 0.24 ug/l

RT: 7.90 min Scan# 1200

Delta R.T. -0.00 min

Lab File: VX002583.D

Acq: 15 Jun 2018 06:02


Tgt Ion: 83 Resp: 847

Ion Ratio Lower Upper

83 100

85 42.9 50.3 75.5#



127 0.0 7.0 10.4#




Abundance Ion 82.90 (82.60 to 83.60): VX0

Ion 84.90 (84.60 to 85.60): VX0

Ion 126.80 (126.50 to 127.50): V




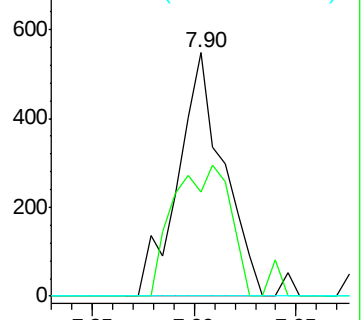


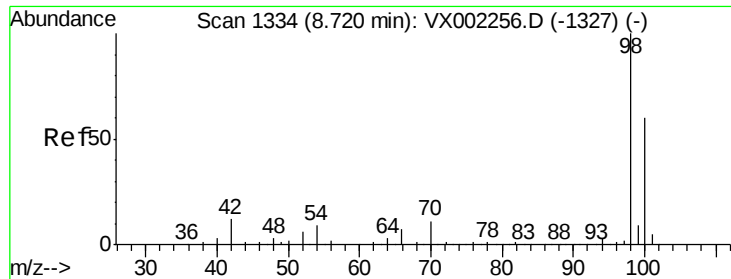

#50
Toluene-d8
Concen: 47.68 ug/l
RT: 8.72 min Scan# 1334
Delta R.T. -0.00 min
Lab File: VX002583.D
Acq: 15 Jun 2018 06:02




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 98 Resp: 466643
Ion Ratio Lower Upper
98 100
100 62.5 50.9 76.3

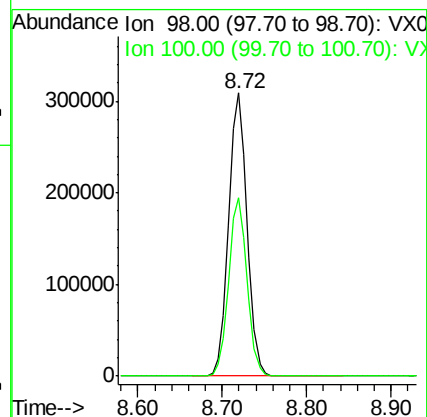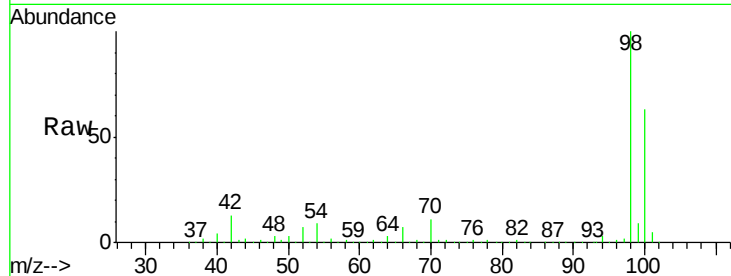

#51
4-Methyl-2-Pentanone
Concen: 0.55 ug/l
RT: 8.65 min Scan# 1323
Delta R.T. -0.00 min
Lab File: VX002583.D
Acq: 15 Jun 2018 06:02

Tgt Ion: 43 Resp: 2382
Ion Ratio Lower Upper
43 100
58 34.3 28.6 42.8



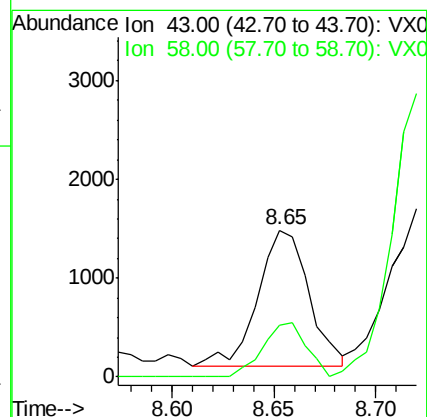





#62
4-Bromofluorobenzene
Concen: 43.55 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. -0.00 min
Lab File: VX002583.D
Acq: 15 Jun 2018 06:02




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 95 Resp: 164344
Ion Ratio Lower Upper
95 100
174 93.8 0.0 187.4
176 91.3 0.0 181.0

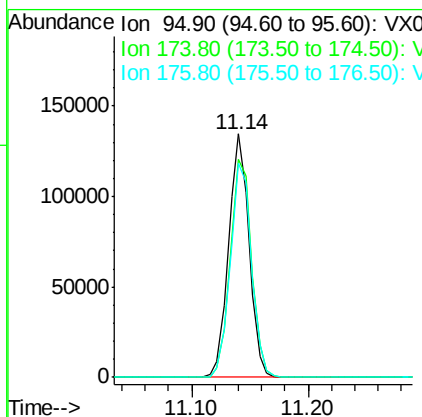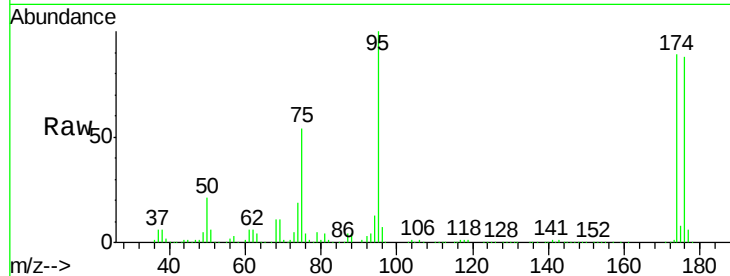

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. -0.00 min
Lab File: VX002583.D
Acq: 15 Jun 2018 06:02

Tgt Ion: 117 Resp: 300004
Ion Ratio Lower Upper
117 100
82 54.8 45.0 67.4
119 32.3 25.8 38.6

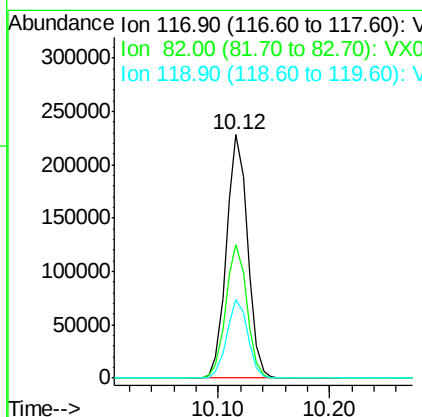



#65

Chlorobenzene

Concen: 0.43 ug/l

RT: 10.14 min Scan# 1567

Delta R.T. -0.00 min

Lab File: VX002583.D

Acq: 15 Jun 2018 06:02

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion:112 Resp: 3222

Ion Ratio Lower Upper




112 100

114 34.5 25.3 37.9



Abundance Ion 111.90 (111.60 to 112.60): V

Ion 113.90 (113.60 to 114.60): V

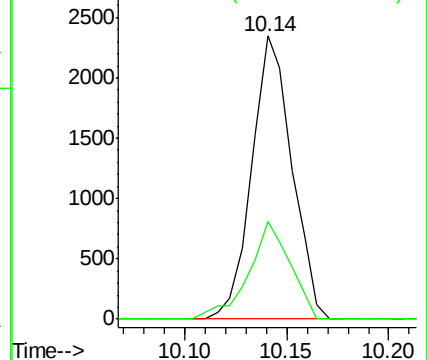

#68

m/p-Xylenes

Concen: 0.30 ug/l

RT: 10.36 min Scan# 1603

Delta R.T. -0.01 min

Lab File: VX002583.D


Acq: 15 Jun 2018 06:02

Tgt Ion:106 Resp: 1463

Ion Ratio Lower Upper



106 100


91 192.5 163.4 245.2



Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VX0

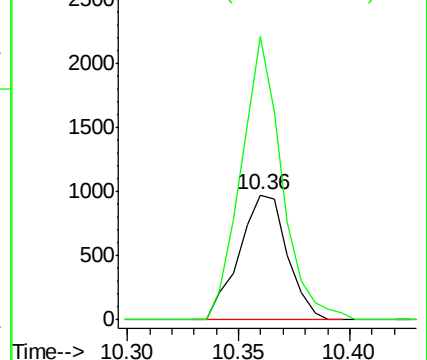

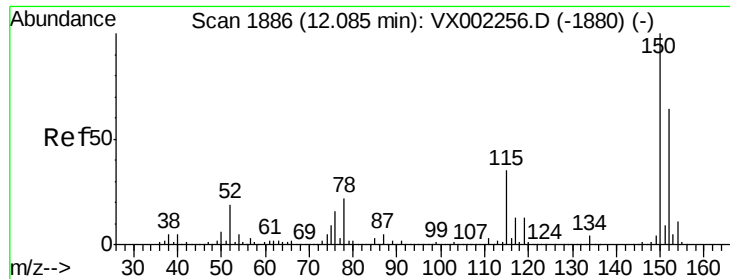

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.09 min Scan# 1886

Delta R.T. -0.00 min

Lab File: VX002583.D

Acq: 15 Jun 2018 06:02

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:152 Resp: 171130

Ion Ratio Lower Upper

152 100

115 54.8 40.1 120.2




150 154.4 0.0 347.2

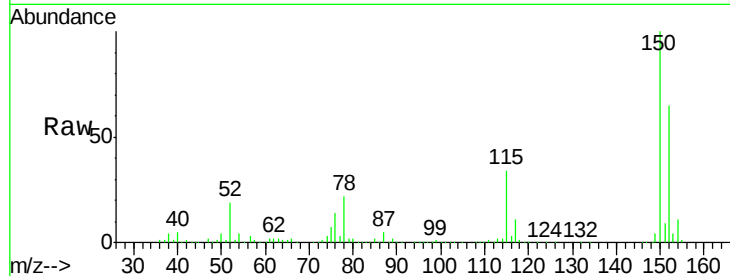

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

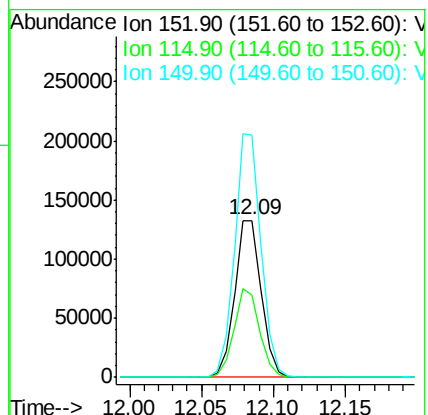

#76

1,2,3-Trichloropropane

Concen: 23.57 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.16 min

Lab File: VX002583.D


Acq: 15 Jun 2018 06:02

Tgt Ion: 75 Resp: 88490

Ion Ratio Lower Upper



75 100


77 1.1 22.8 68.3#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0



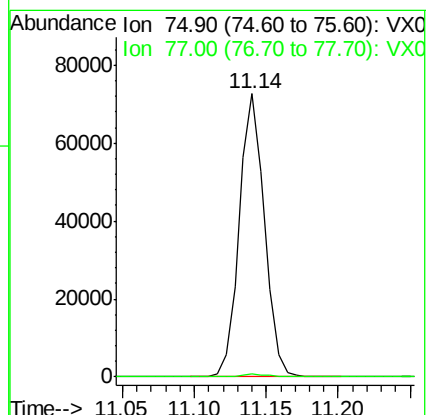



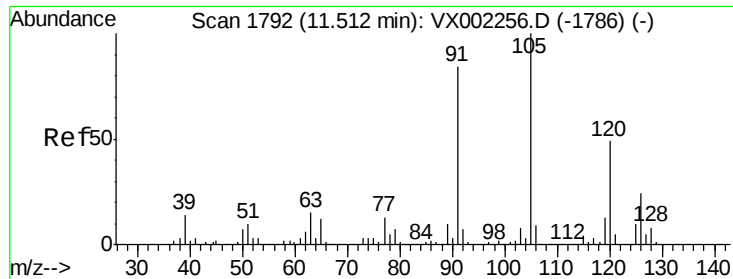

#80
 1,3,5-Trimethylbenzene
 Concen: 0.23 ug/l
 RT: 11.51 min Scan# 1791
 Delta R.T. -0.01 min
 Lab File: VX002583.D
 Acq: 15 Jun 2018 06:02




Instrument :
 MSVOA_X
 ClientSampled :


Tot Ion:105 Resp: 2354
 Ion Ratio Lower Upper
 105 100
 120 51.8 24.4 73.4

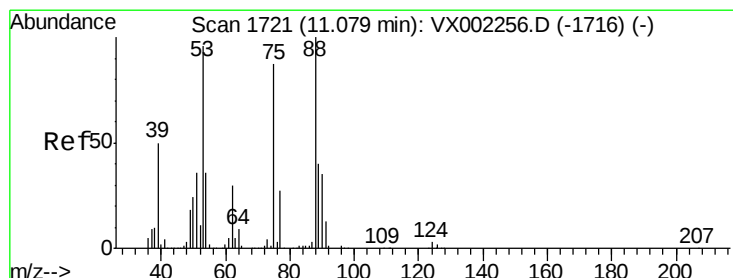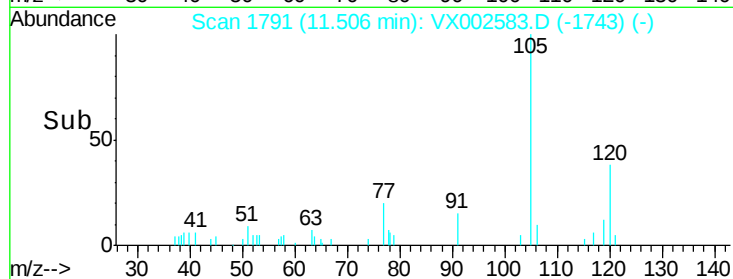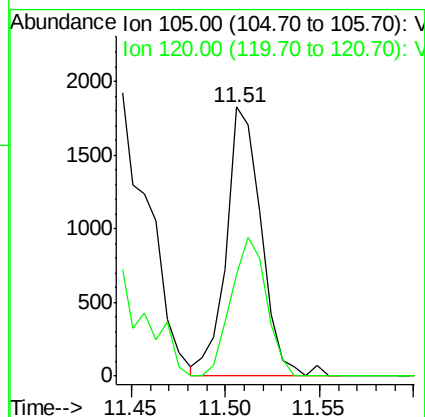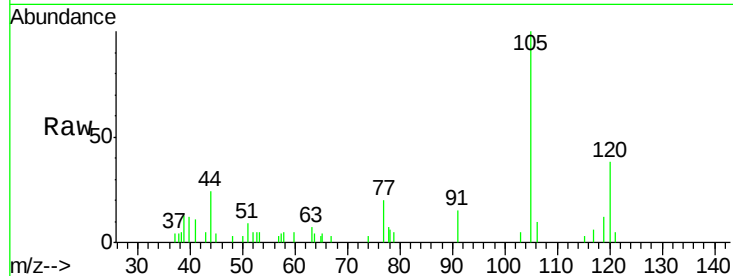

#81
 trans-1,4-Dichloro-2-butene
 Concen: 82.61 ug/l
 RT: 11.14 min Scan# 1731
 Delta R.T. 0.06 min
 Lab File: VX002583.D
 Acq: 15 Jun 2018 06:02

Tgt Ion: 75 Resp: 88490
 Ion Ratio Lower Upper
 75 100
 53 0.1 86.8 130.2#
 89 0.0 38.2 57.2#


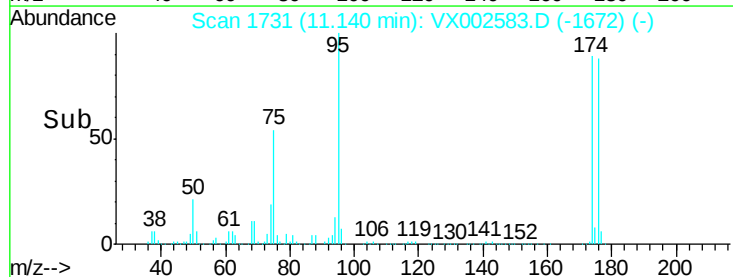
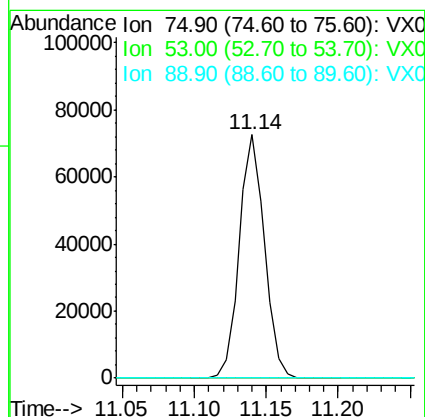
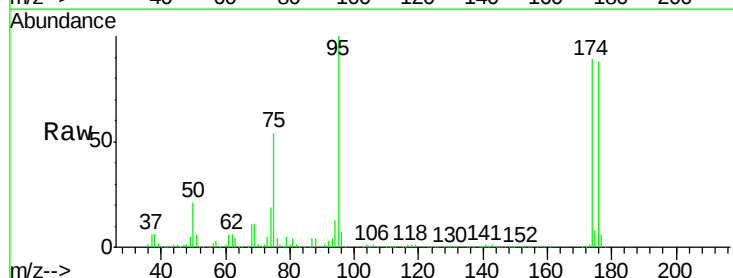


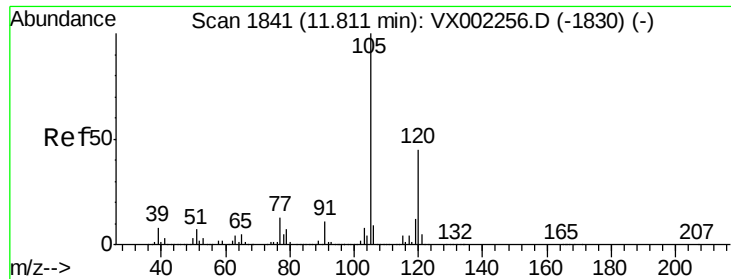

#84
 1,2,4-Trimethylbenzene
 Concen: 0.81 ug/l
 RT: 11.81 min Scan# 1841
 Delta R.T. -0.00 min
 Lab File: VX002583.D
 Acq: 15 Jun 2018 06:02




Instrument :
 MSVOA_X
 ClientSampleId :


Tot Ion:105 Resp: 8504
 Ion Ratio Lower Upper
 105 100
 120 44.9 22.3 66.8

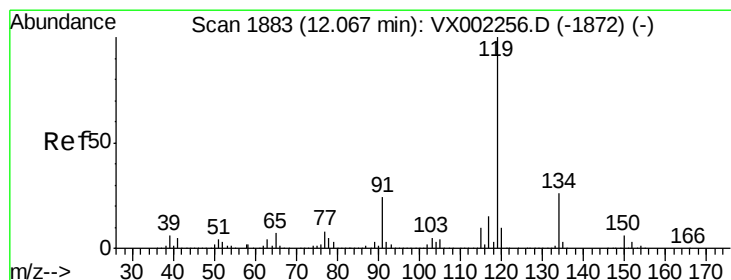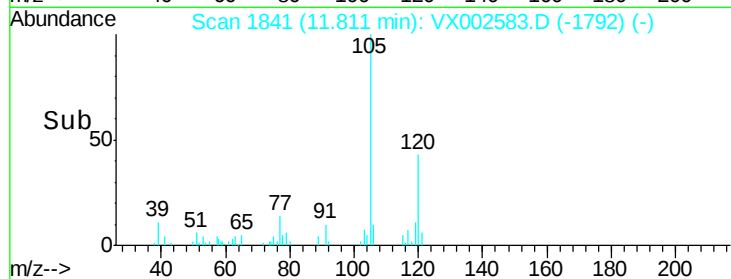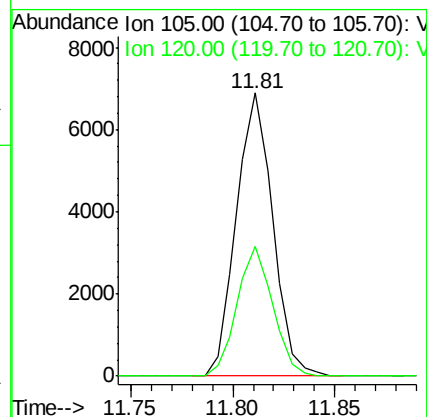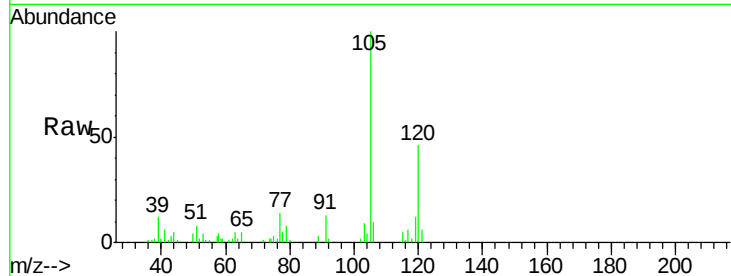

#86
 p-Isopropyltoluene
 Concen: 0.21 ug/l
 RT: 12.07 min Scan# 1883
 Delta R.T. -0.00 min
 Lab File: VX002583.D
 Acq: 15 Jun 2018 06:02

Tgt Ion:119 Resp: 2267
 Ion Ratio Lower Upper
 119 100
 134 38.7 13.4 40.1
 91 45.7 11.9 35.7#

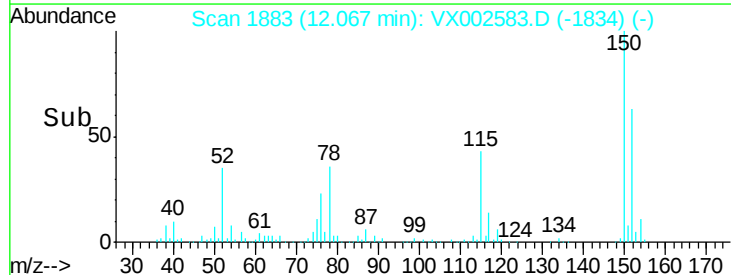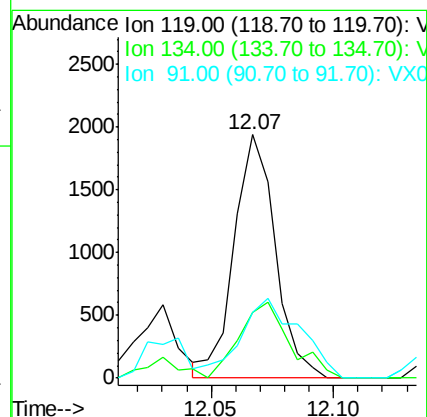



#95

Naphthalene

Concen: 10.72 ug/l

RT: 13.84 min Scan# 2174

Delta R.T. -0.00 min


Lab File: VX002583.D

Acq: 15 Jun 2018 06:02

Instrument :

MSVOA_X

ClientSampleId :



Tot Ion:128 Resp: 133486

Ion Ratio Lower Upper

128 100

127 13.5 10.4 15.6

129 11.0 8.6 13.0

