


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX061418\
Data File : VX002546.D
Acq On : 14 Jun 2018 09:30
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X060418W.M
Title : SW846 8260
Last Update : Tue Jun 05 03:22:35 2018

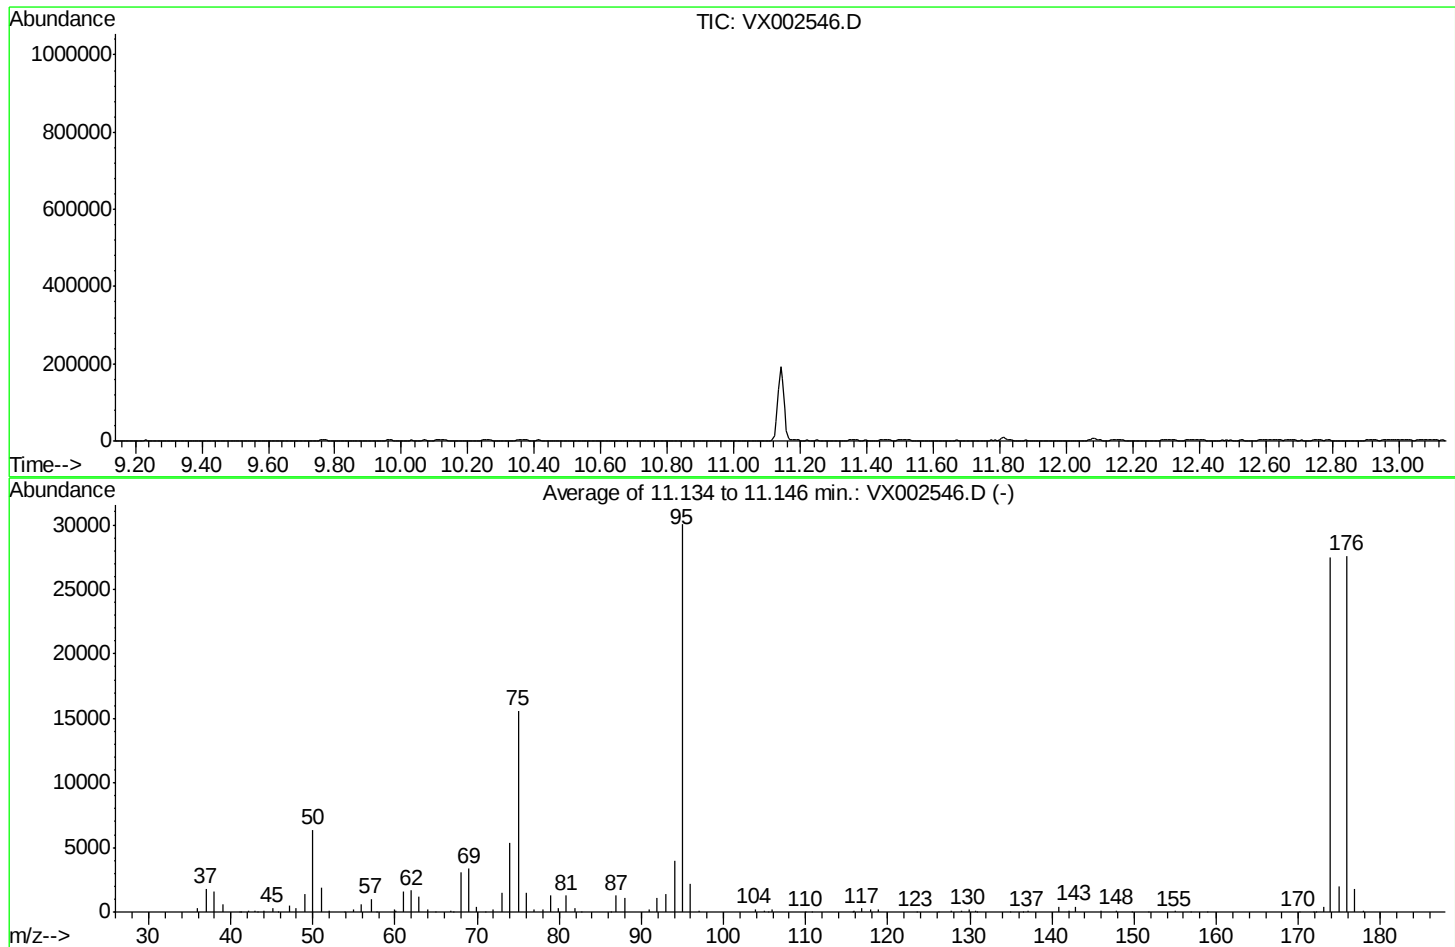

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	6369	PASS
75	95	30	60	51.9	15602	PASS
95	95	100	100	100.0	30037	PASS
96	95	5	9	7.3	2185	PASS
173	174	0.00	2	1.5	399	PASS
174	95	50	100	91.5	27498	PASS
175	174	5	9	7.2	1980	PASS
176	174	95	101	100.3	27584	PASS
177	176	5	9	6.4	1769	PASS