



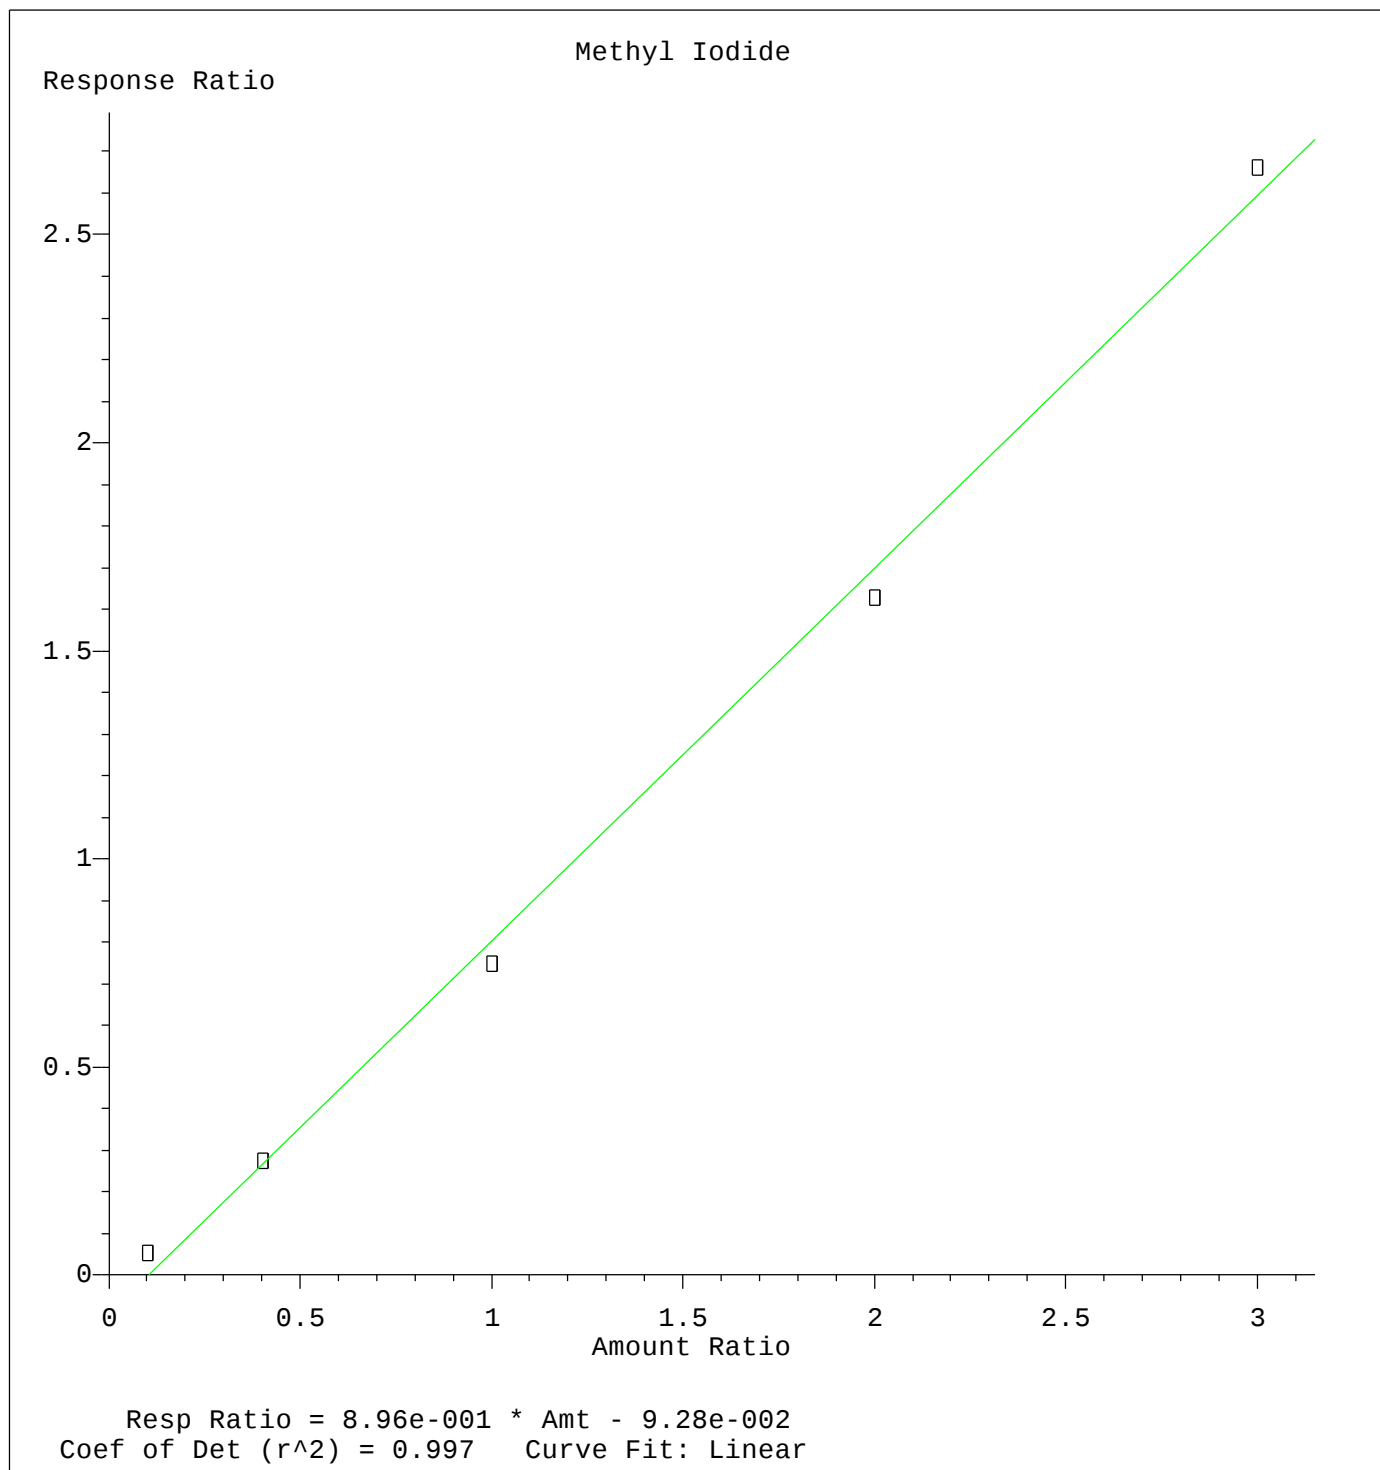


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Calibration Table Last Updated: Sat Jun 16 01:37:33 2018

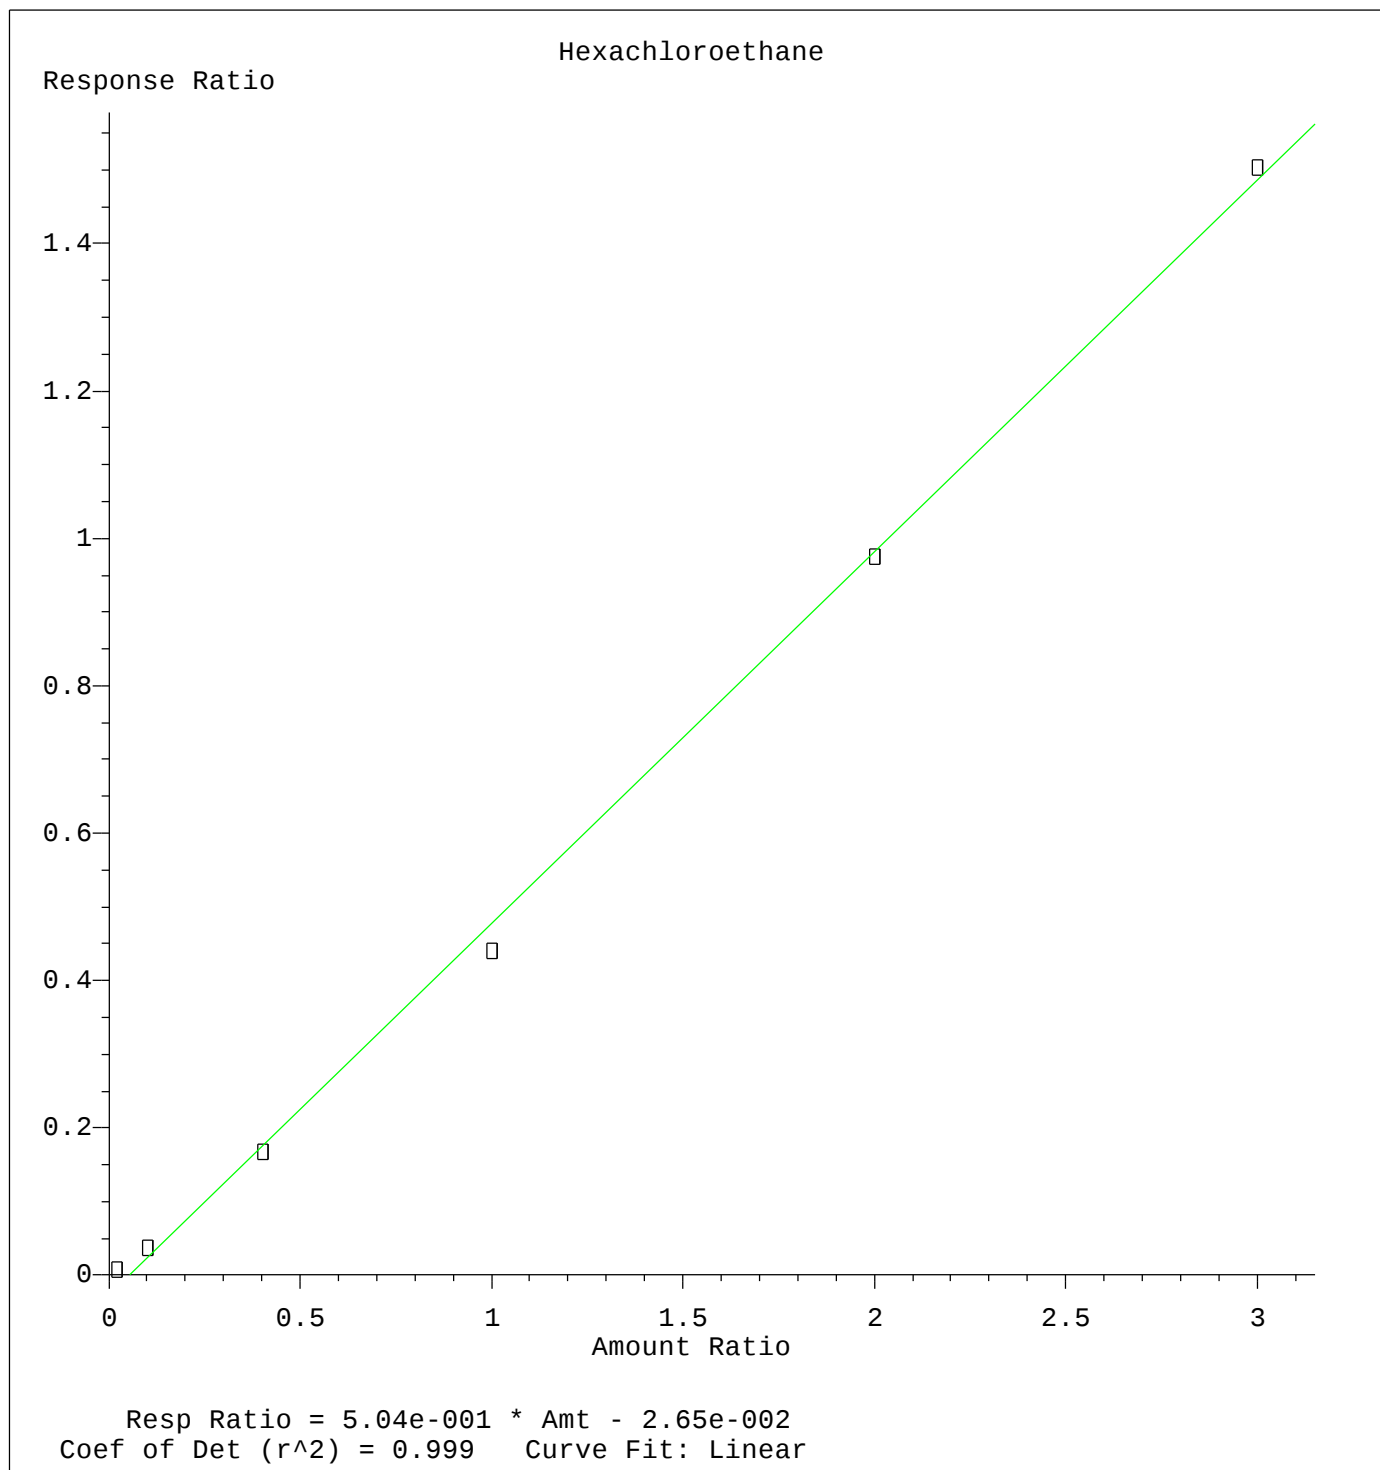

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Calibration Table Last Updated: Sat Jun 16 01:37:33 2018


trans-1,4-Dichloro-2-butene

Response Ratio

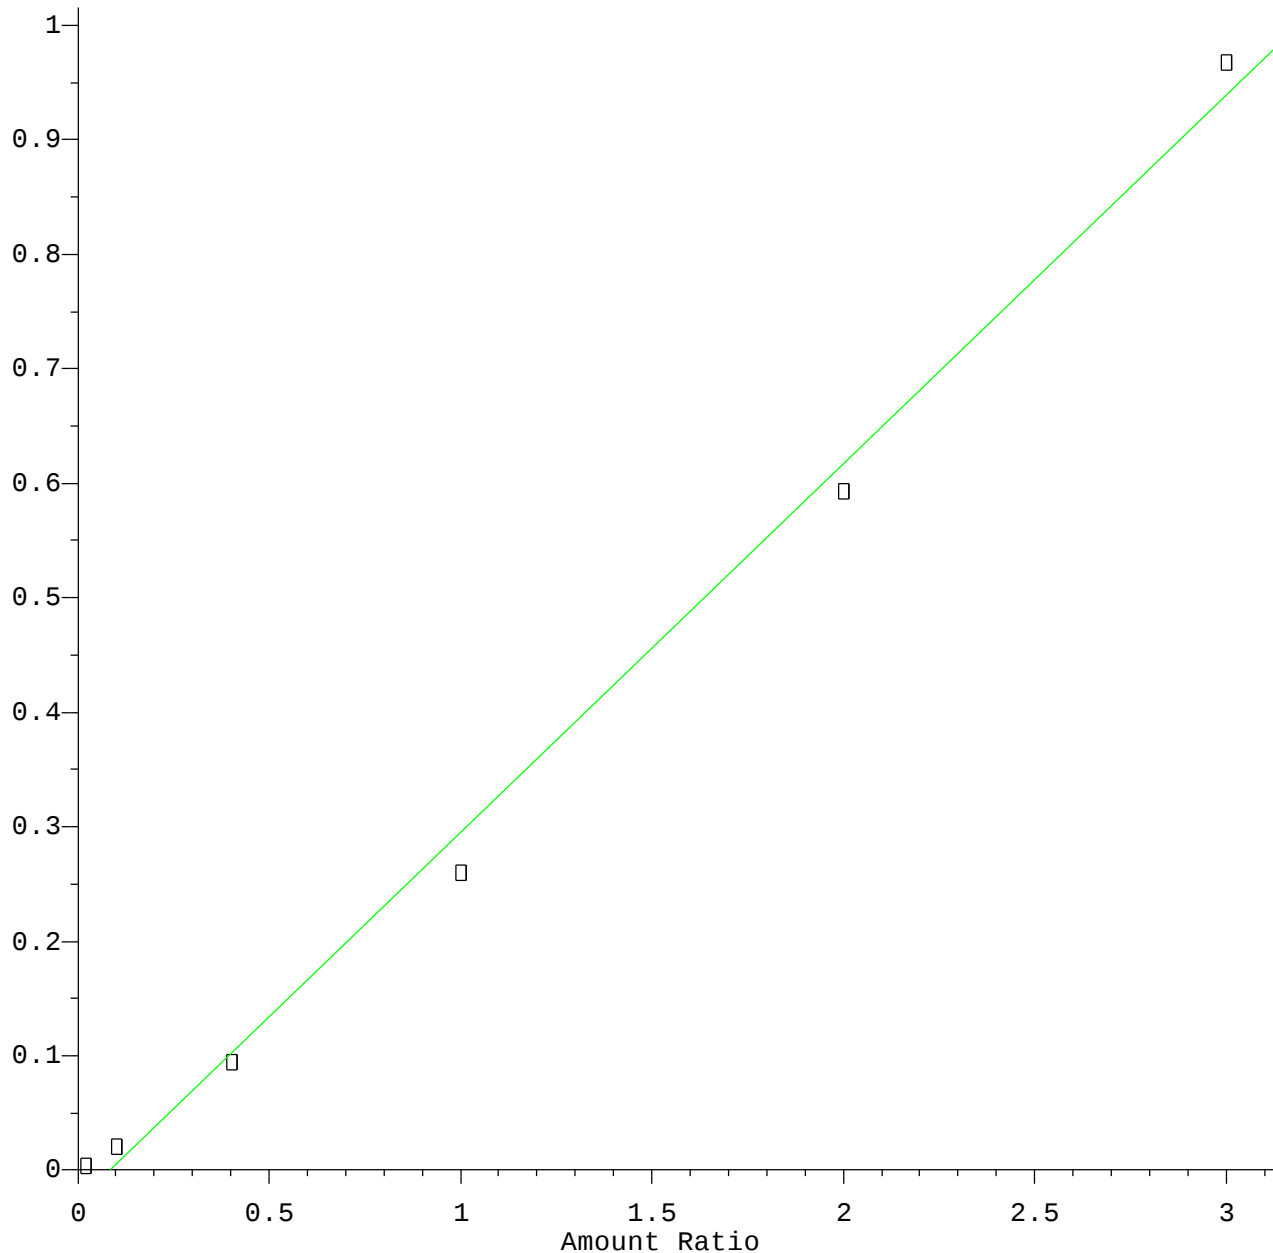

Resp Ratio = $3.22 \times 10^{-1} \times \text{Amt} - 2.69 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Calibration Table Last Updated: Sat Jun 16 01:37:33 2018

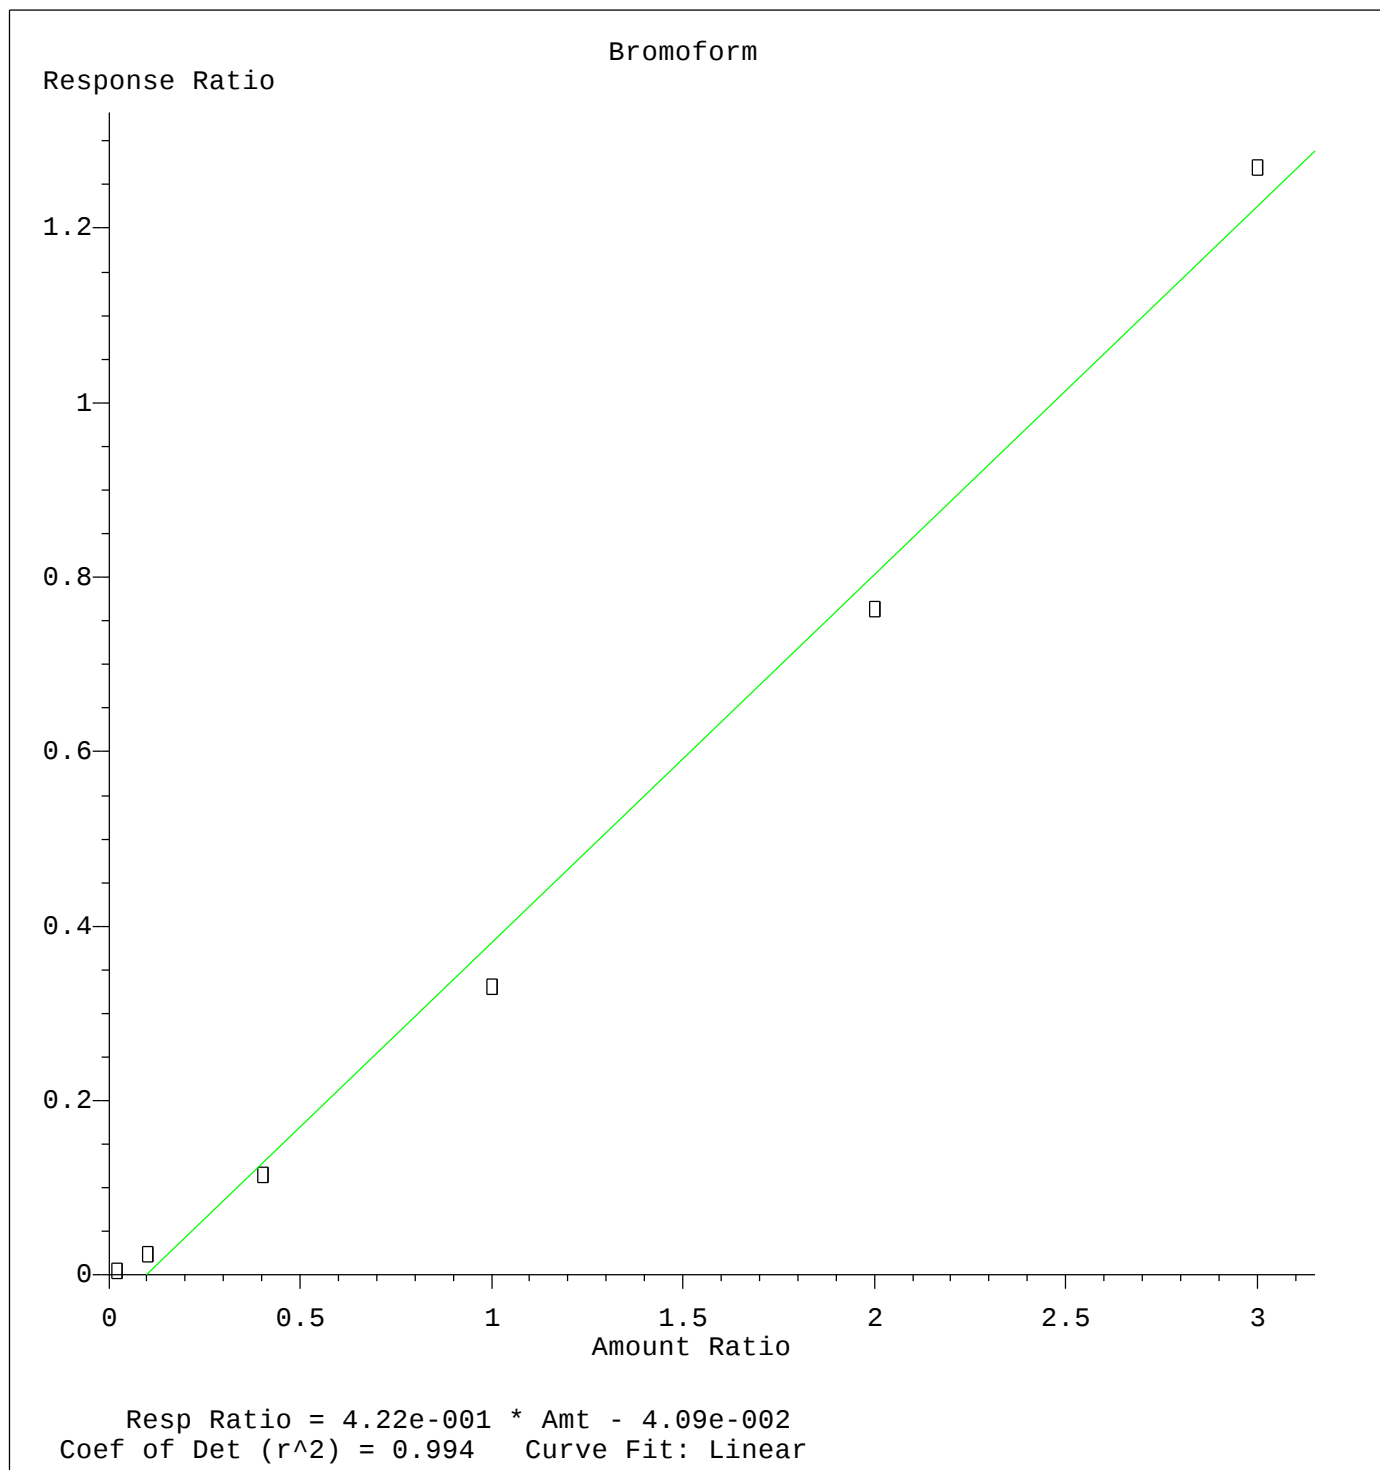

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Calibration Table Last Updated: Sat Jun 16 01:37:33 2018

Dibromochloromethane

Response Ratio

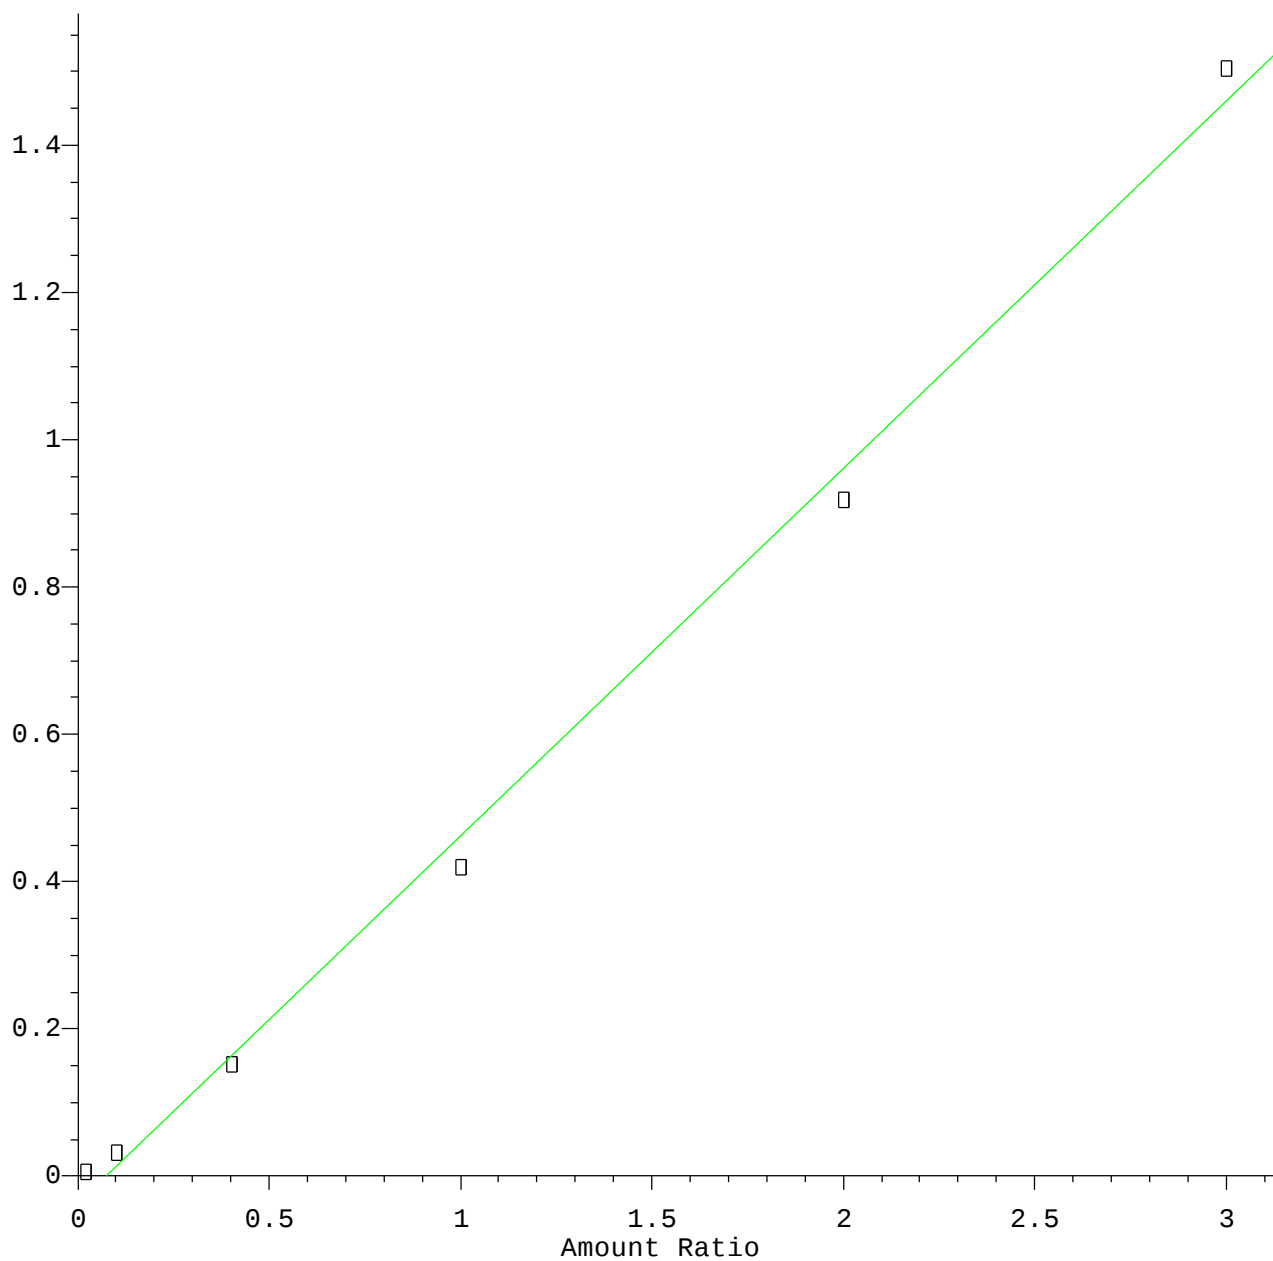


Resp Ratio = $4.99 \times 10^{-1} \times \text{Amt} - 3.75 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Calibration Table Last Updated: Sat Jun 16 01:37:33 2018

cis-1,3-Dichloropropene

Response Ratio

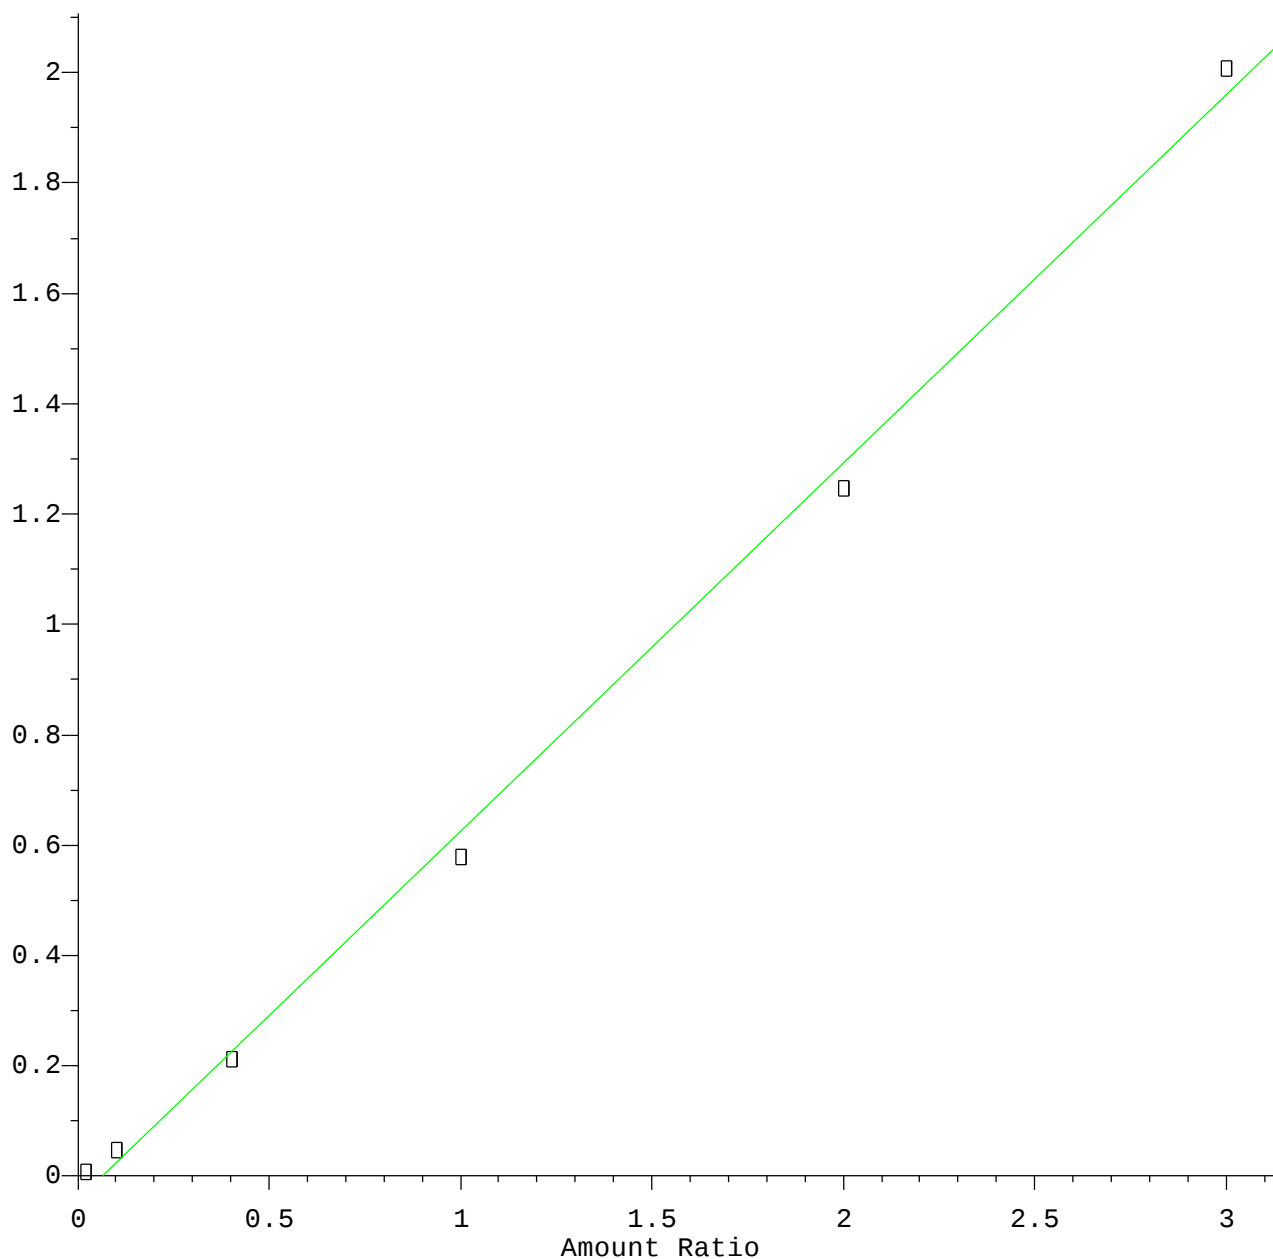


Resp Ratio = $6.67 \times 10^{-1} \times \text{Amt} - 4.29 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Calibration Table Last Updated: Sat Jun 16 01:37:33 2018

t-1,3-Dichloropropene

Response Ratio

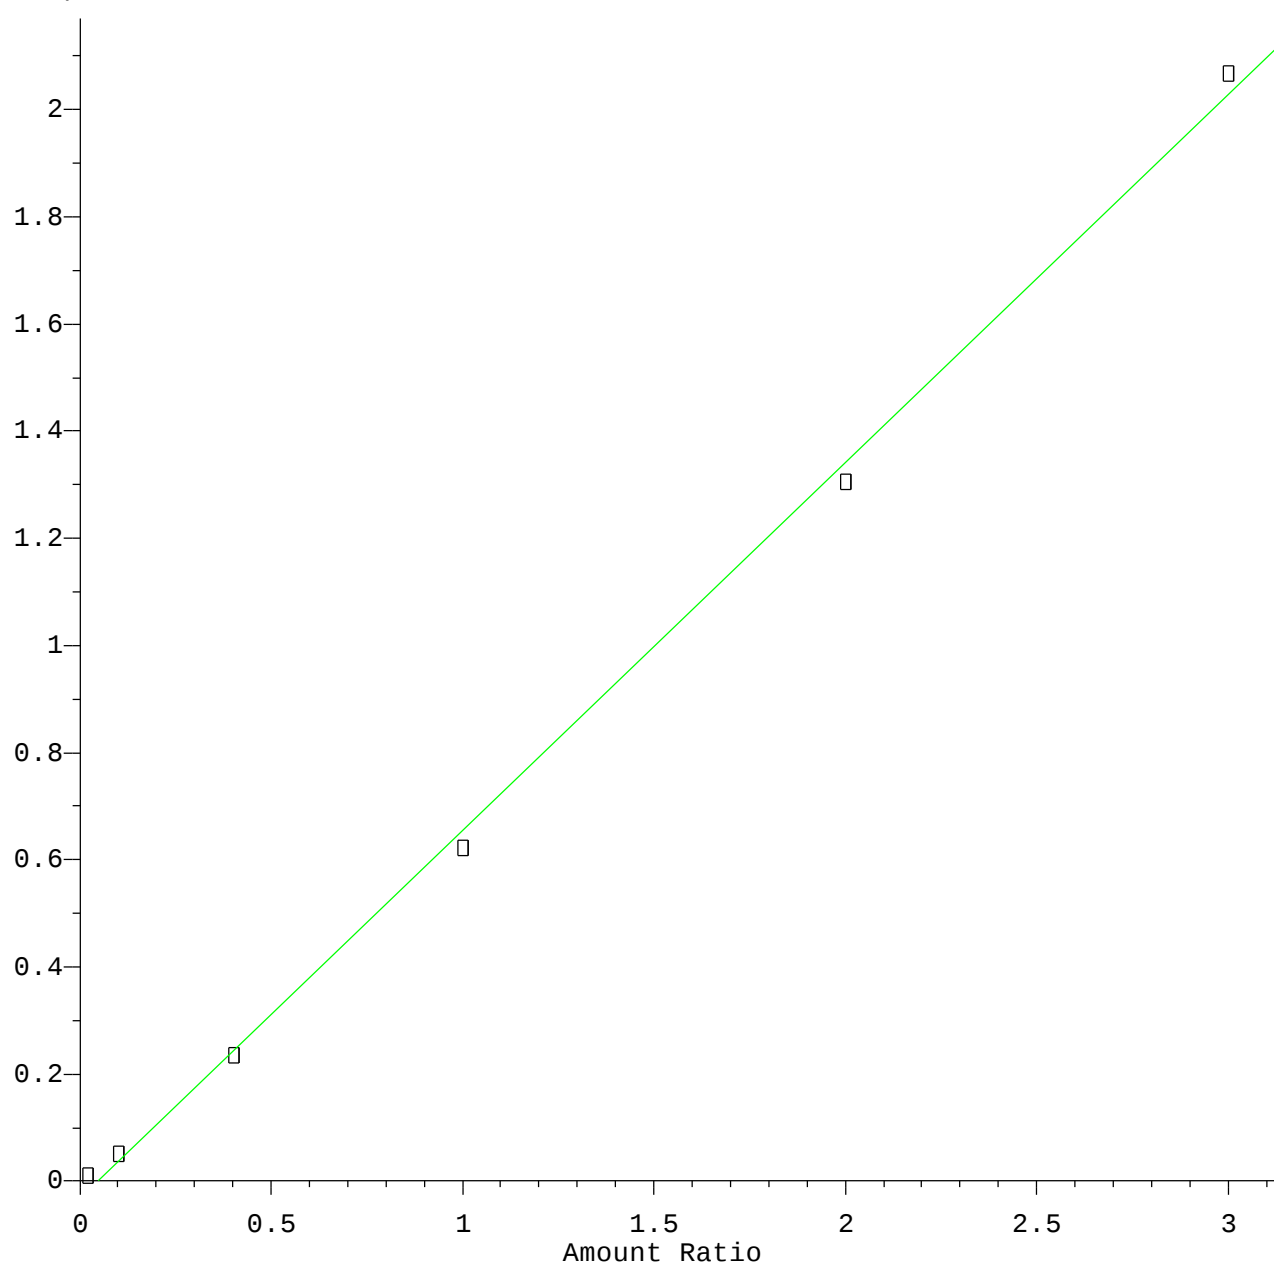


Resp Ratio = $6.87 \times 10^{-1} \times \text{Amt} - 3.29 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Calibration Table Last Updated: Sat Jun 16 01:37:33 2018

Acrolein

Response Ratio

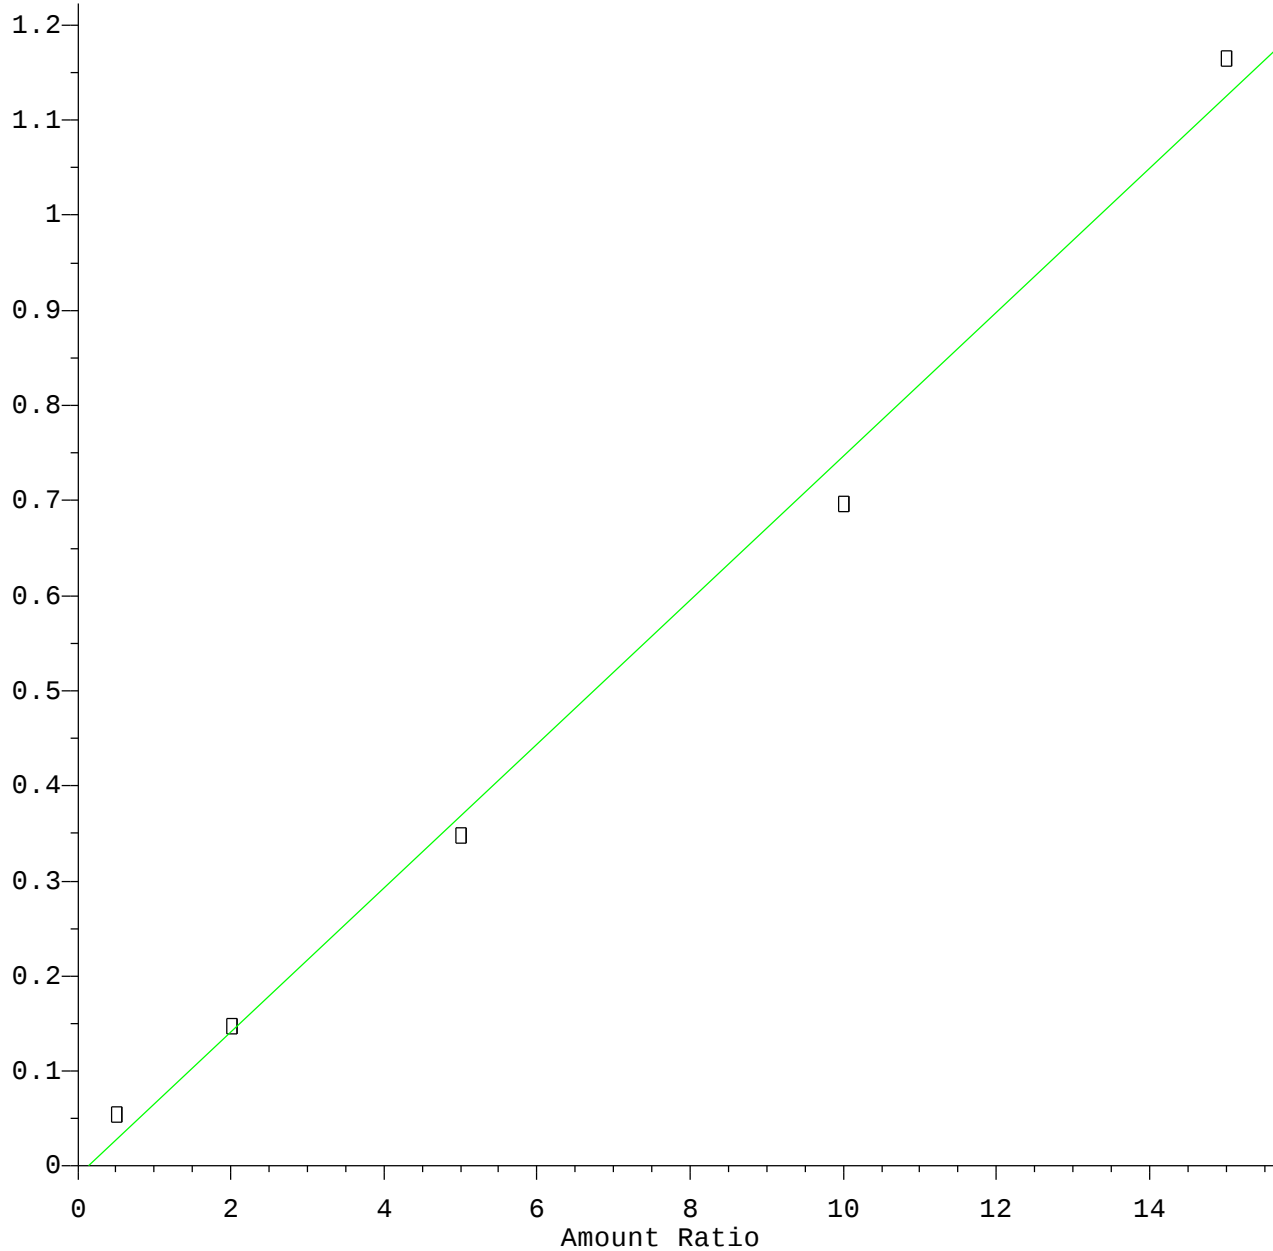

Resp Ratio = $7.57 \times 10^{-2} \times \text{Amt} - 1.04 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Calibration Table Last Updated: Sat Jun 16 01:37:33 2018