

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061518\  
 Data File : VX002627.D  
 Acq On : 16 Jun 2018 05:53  
 Operator : JC/MD  
 Sample : VX0615WBL02  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 38 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0615WBL02

Quant Time: Jun 16 07:25:14 2018  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X061518W.M  
 Quant Title : SW846 8260  
 QLast Update : Sat Jun 16 01:37:33 2018  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) Pentafluorobenzene      | 5.67  | 168  | 215297   | 50.00 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 6.87  | 114  | 307624   | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 10.12 | 117  | 286377   | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 12.09 | 152  | 156483   | 50.00 | ug/l  | 0.00     |

| System Monitoring Compounds |        |     |          |       |         |      |
|-----------------------------|--------|-----|----------|-------|---------|------|
| 33) 1,2-Dichloroethane-d4   | 6.07   | 65  | 156877   | 47.95 | ug/l    | 0.00 |
| Spiked Amount               | 50.000 |     | Recovery | =     | 95.90%  |      |
| 35) Dibromofluoromethane    | 5.51   | 113 | 119940   | 48.85 | ug/l    | 0.00 |
| Spiked Amount               | 50.000 |     | Recovery | =     | 97.70%  |      |
| 50) Toluene-d8              | 8.72   | 98  | 470935   | 50.52 | ug/l    | 0.00 |
| Spiked Amount               | 50.000 |     | Recovery | =     | 101.04% |      |
| 62) 4-Bromofluorobenzene    | 11.14  | 95  | 162276   | 45.94 | ug/l    | 0.00 |
| Spiked Amount               | 50.000 |     | Recovery | =     | 91.88%  |      |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061518\  
Data File : VX002627.D  
Acq On : 16 Jun 2018 05:53  
Operator : JC/MD  
Sample : VX0615WBL02  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 38 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0615WBL02

Quant Time: Jun 16 07:25:14 2018  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X061518W.M  
Quant Title : SW846 8260  
QLast Update : Sat Jun 16 01:37:33 2018  
Response via : Initial Calibration

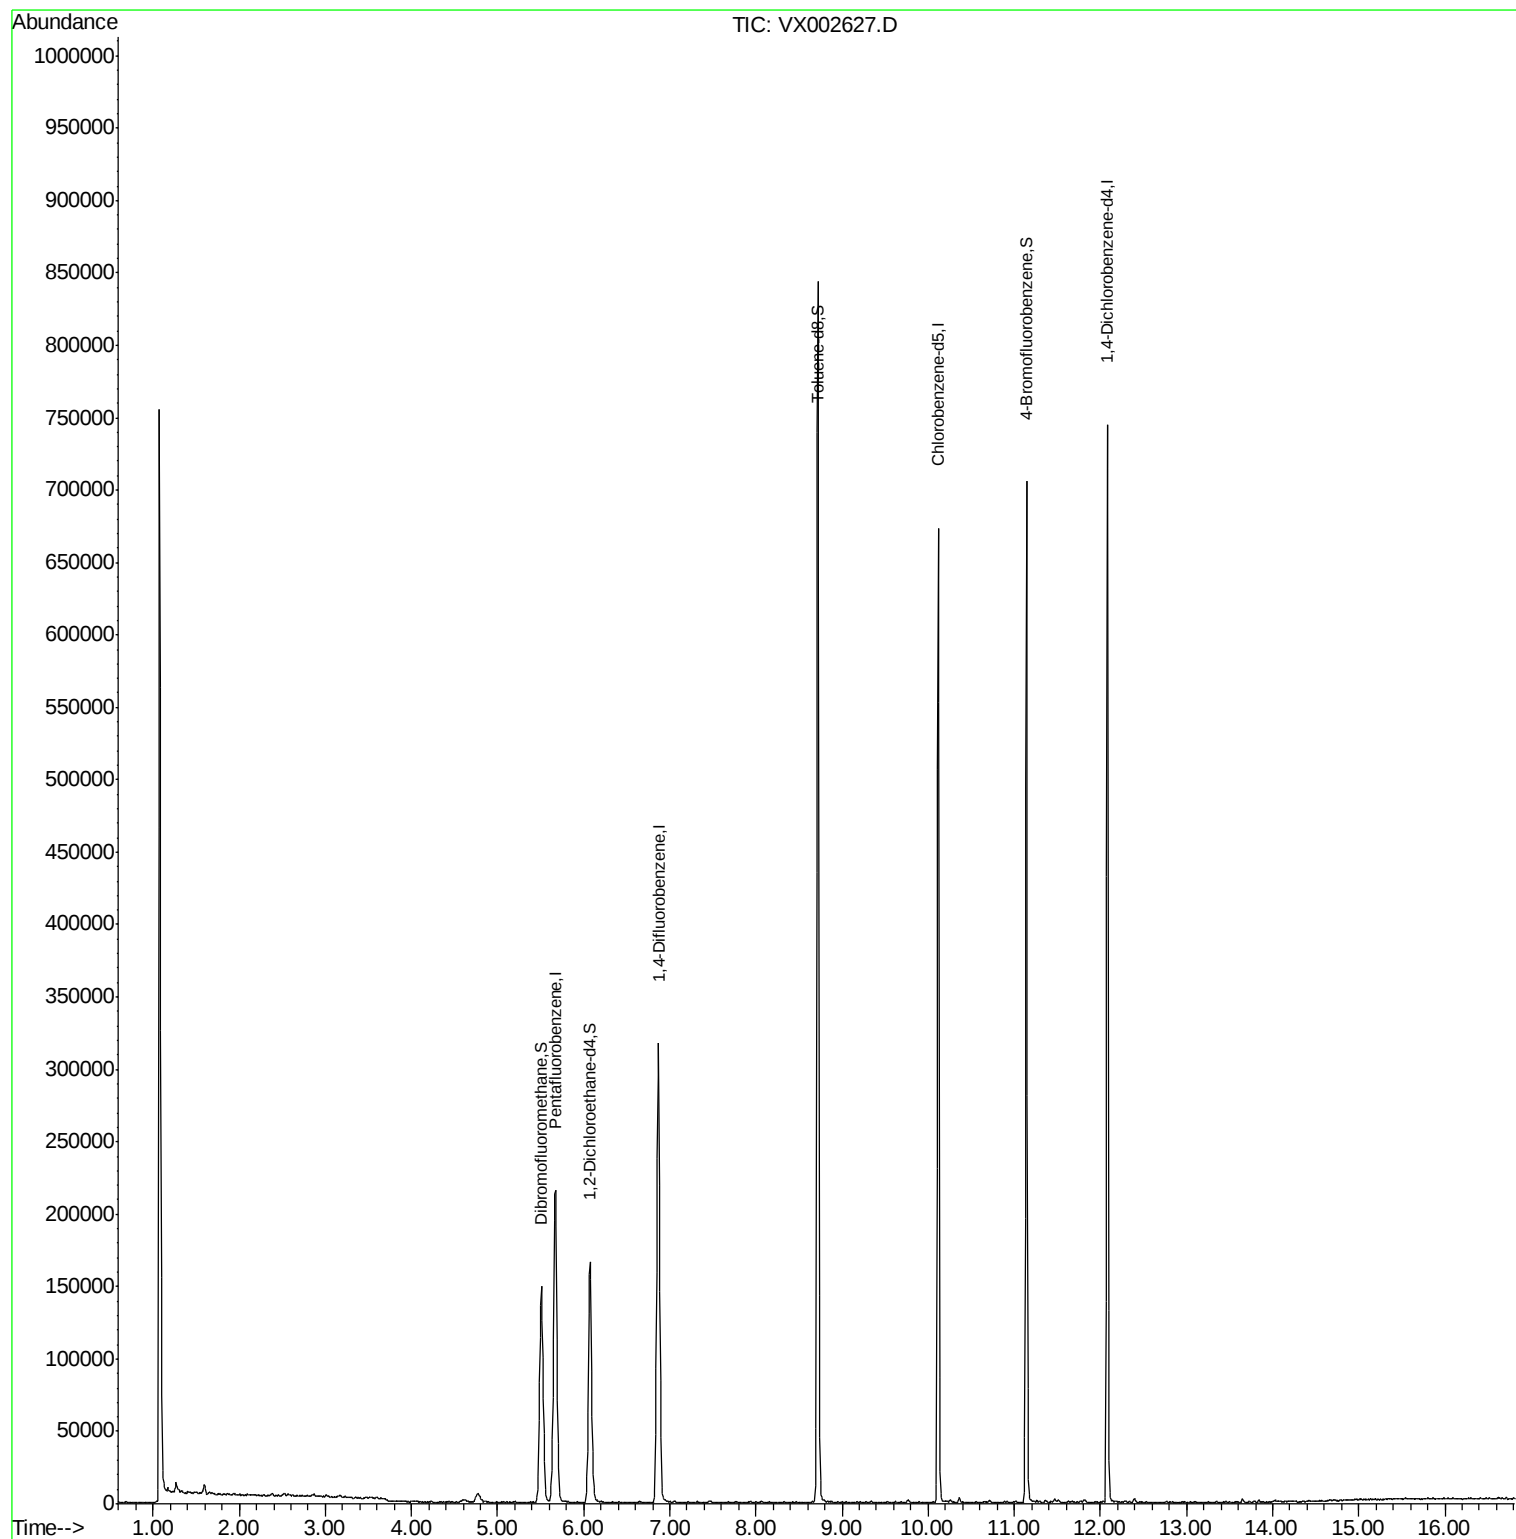

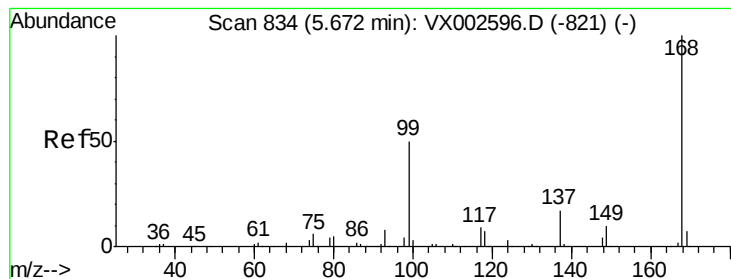

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. 0.00 min

Lab File: VX002627.D

Acq: 16 Jun 2018 05:53

Instrument :

MSVOA\_X

ClientSampleId :


VX0615WBL02

Tot Ion:168 Resp: 215297

Ion Ratio Lower Upper




168 100

99 49.7 39.3 58.9

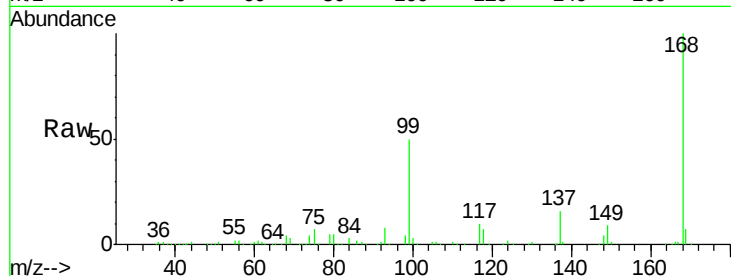

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

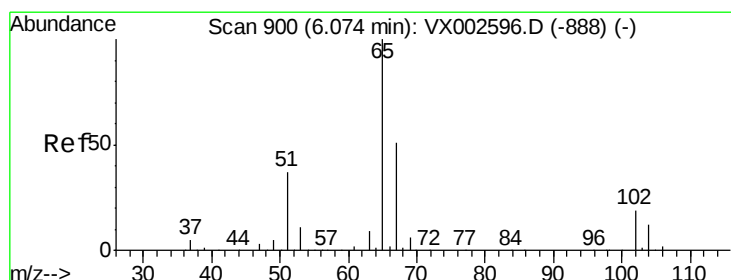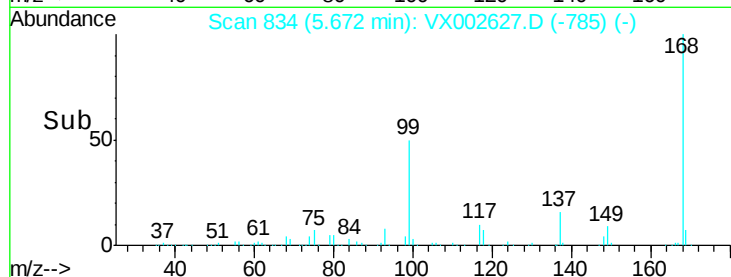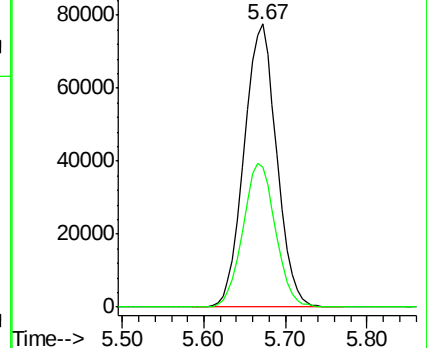

#33

1,2-Dichloroethane-d4

Concen: 47.95 ug/l

RT: 6.07 min Scan# 900

Delta R.T. 0.00 min

Lab File: VX002627.D


Acq: 16 Jun 2018 05:53

Tgt Ion: 65 Resp: 156877

Ion Ratio Lower Upper



65 100


67 51.2 0.0 102.6

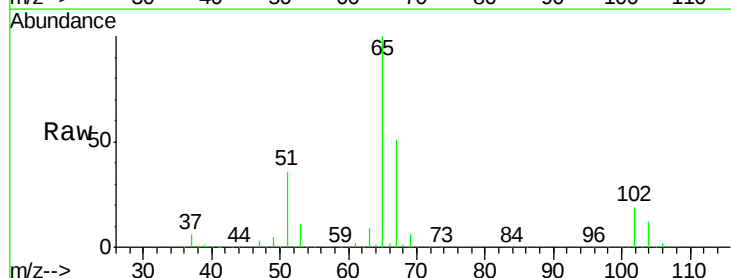

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

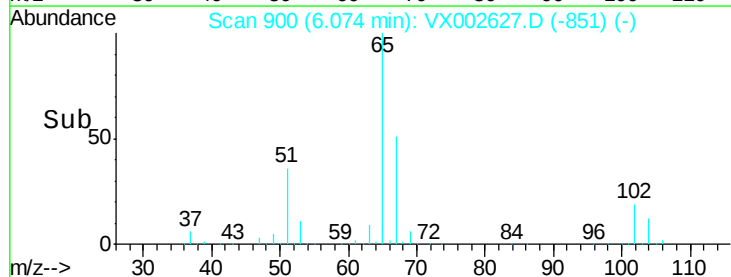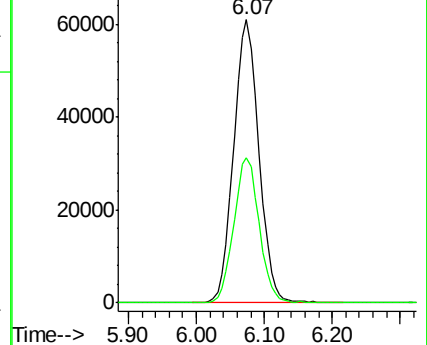

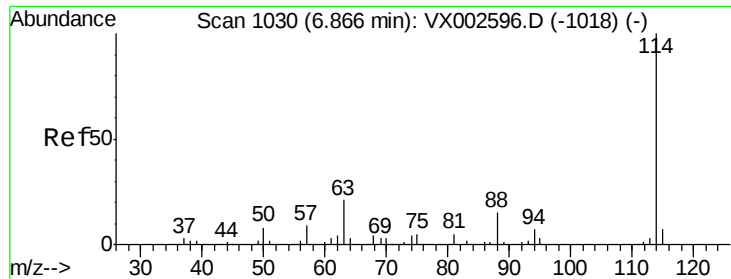

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. 0.00 min

Lab File: VX002627.D

Acq: 16 Jun 2018 05:53

Instrument :

MSVOA\_X

ClientSampleId :

VX0615WBL02


Tot Ion:114 Resp: 307624

Ion Ratio Lower Upper

114 100

63 20.1 0.0 41.4




88 15.0 0.0 30.0

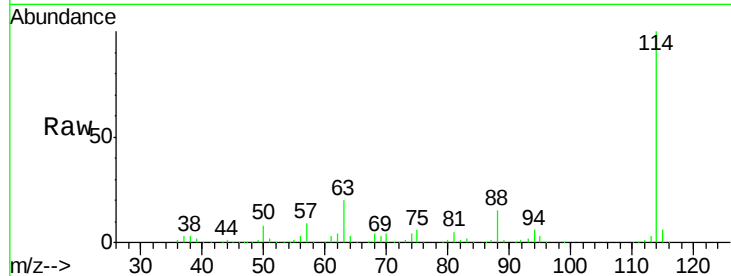

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

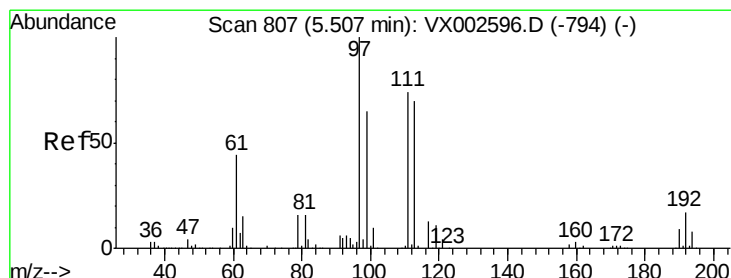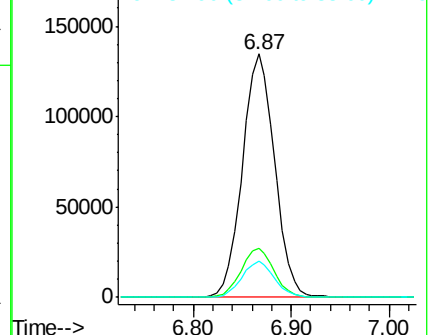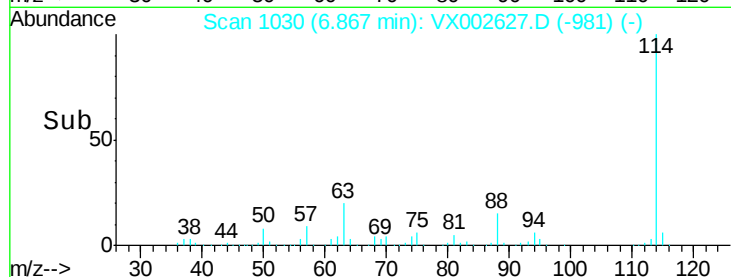

#35

Dibromofluoromethane

Concen: 48.85 ug/l

RT: 5.51 min Scan# 807

Delta R.T. 0.00 min

Lab File: VX002627.D

Acq: 16 Jun 2018 05:53


Tgt Ion:113 Resp: 119940

Ion Ratio Lower Upper

113 100

111 102.6 81.4 122.0



192 23.3 19.1 28.7

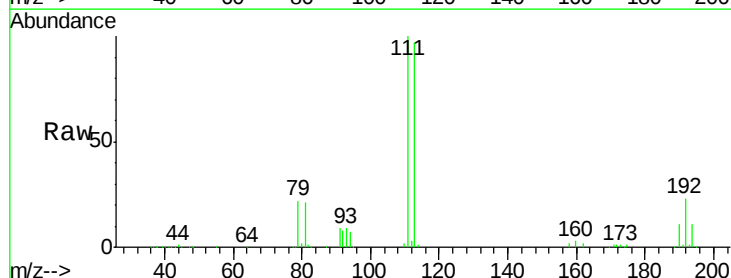


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

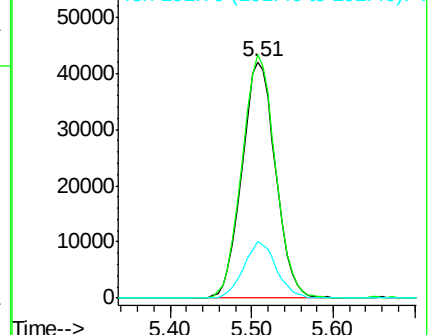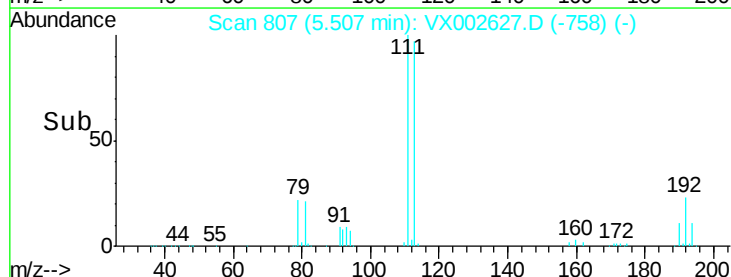

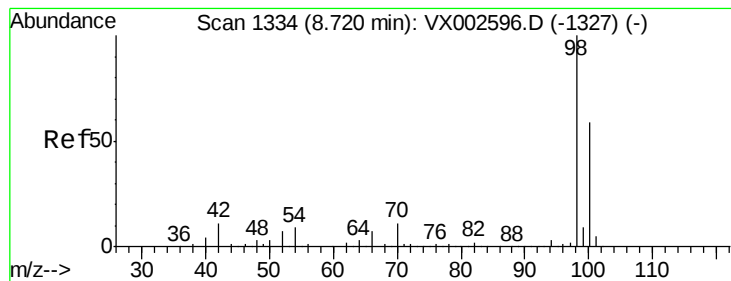

#50

Toluene-d8

Concen: 50.52 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX002627.D

Acq: 16 Jun 2018 05:53

Instrument :

MSVOA\_X

ClientSampleId :


VX0615WBL02

Tot Ion: 98 Resp: 470935

Ion Ratio Lower Upper




98 100

100 63.8 50.9 76.3

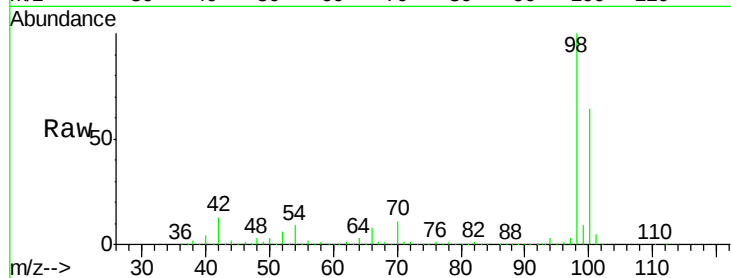

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

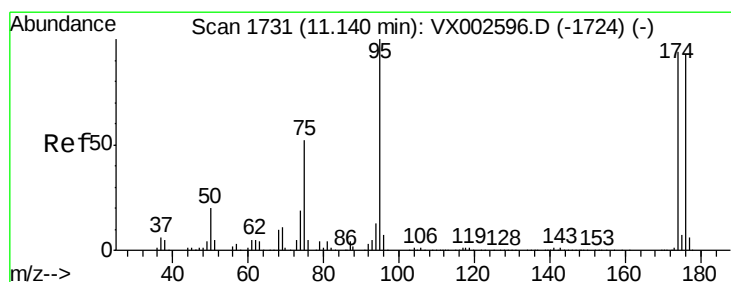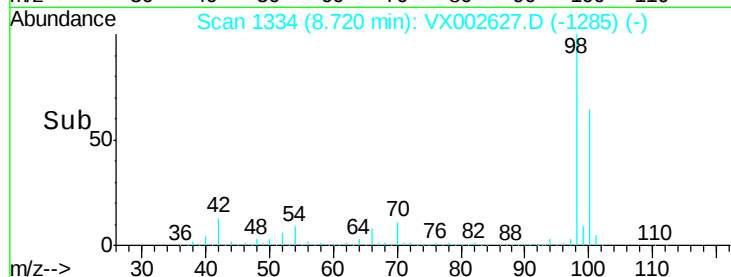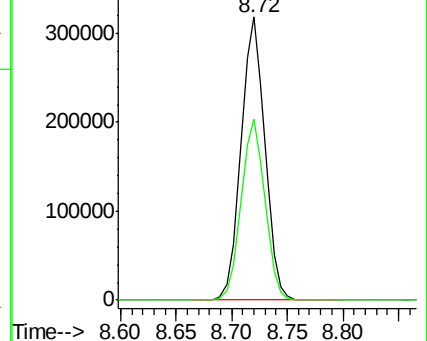

#62

4-Bromofluorobenzene

Concen: 45.94 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.00 min

Lab File: VX002627.D

Acq: 16 Jun 2018 05:53


Tgt Ion: 95 Resp: 162276

Ion Ratio Lower Upper

95 100

174 94.6 0.0 187.4



176 92.6 0.0 181.0

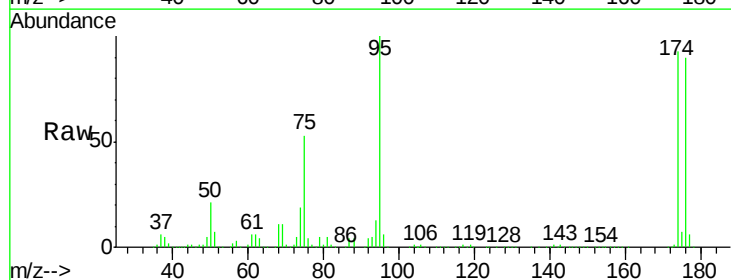


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V



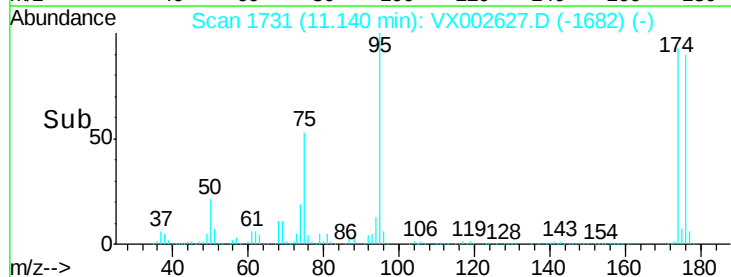
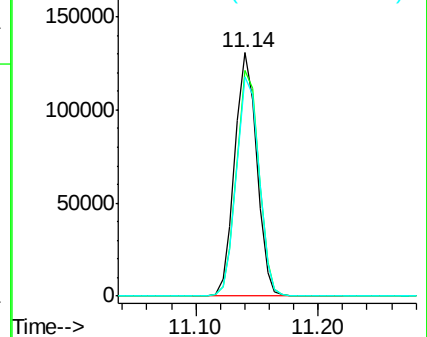


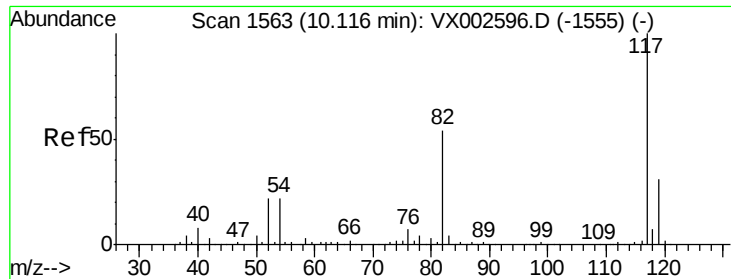

#63  
Chlorobenzene-d5  
Concen: 50.00 ug/l  
RT: 10.12 min Scan# 1563  
Delta R.T. 0.00 min  
Lab File: VX002627.D  
Acq: 16 Jun 2018 05:53

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0615WBL02

Tot Ion:117 Resp: 286377  
Ion Ratio Lower Upper  
117 100  
82 54.5 45.0 67.4  
119 31.8 25.8 38.6

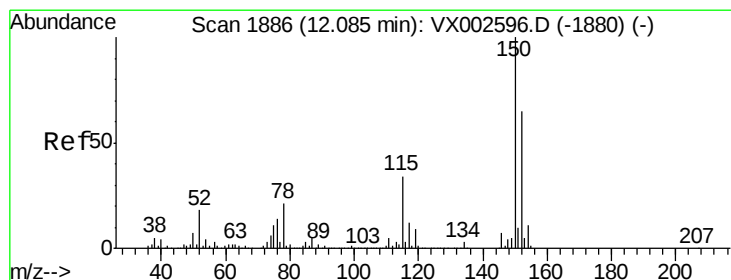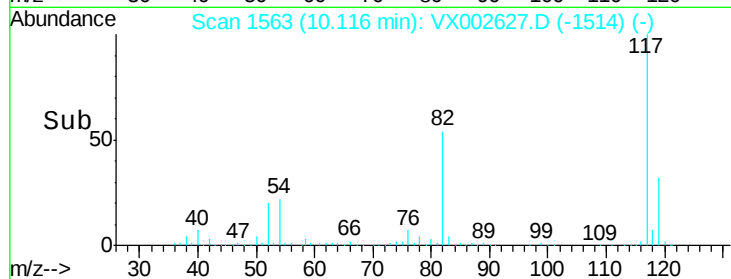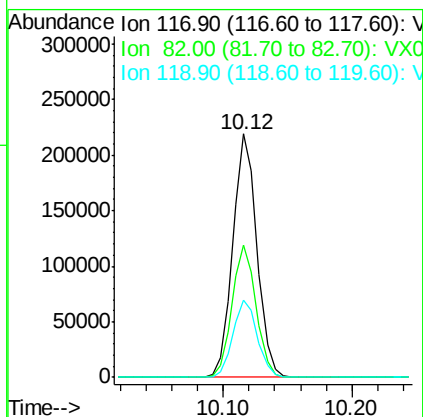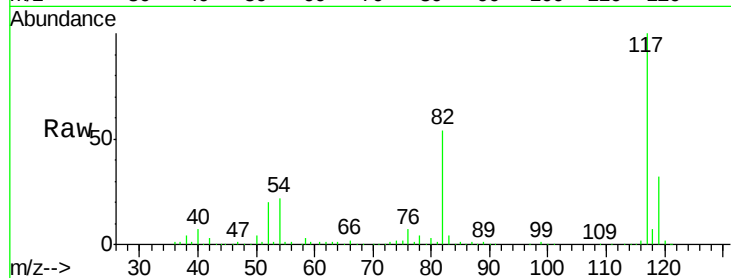

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.00 ug/l  
RT: 12.09 min Scan# 1886  
Delta R.T. 0.00 min  
Lab File: VX002627.D  
Acq: 16 Jun 2018 05:53

Tgt Ion:152 Resp: 156483  
Ion Ratio Lower Upper  
152 100  
115 54.4 40.1 120.2  
150 156.8 0.0 347.2

