

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061518\
 Data File : VX002640.D
 Acq On : 16 Jun 2018 11:36
 Operator : JC/MD
 Sample : J3477-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S36-0135

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	91	rBV	1083133	1306109	100.00%	15.732%
2	1.270	108	112	116	rBV	13665	23589	1.81%	0.284%
3	1.325	116	121	132	rBV	130218	514821	39.42%	6.201%
4	1.404	132	134	145	rVB	89320	147540	11.30%	1.777%
5	2.623	329	334	340	rBV	11171	21165	1.62%	0.255%
6	3.172	418	424	433	rVB3	13618	32219	2.47%	0.388%
7	4.605	646	659	672	rBV	63645	177879	13.62%	2.143%
8	5.507	796	807	822	rBV	141463	402015	30.78%	4.842%
9	5.665	822	833	847	rVB	215154	606831	46.46%	7.309%
10	6.074	889	900	913	rBV	153928	402889	30.85%	4.853%
11	6.867	1020	1030	1043	rBV	311837	728778	55.80%	8.778%
12	8.720	1324	1334	1343	rBV	784029	1183179	90.59%	14.251%
13	10.116	1556	1563	1574	rBV	682734	896263	68.62%	10.796%
14	11.140	1725	1731	1741	rBV	668249	832437	63.73%	10.027%
15	12.085	1880	1886	1895	rBV	743058	980172	75.05%	11.806%
16	12.396	1931	1937	1944	rVB	35565	46267	3.54%	0.557%


Sum of corrected areas: 8302153

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061518\
Data File : VX002640.D
Acq On : 16 Jun 2018 11:36
Operator : JC/MD
Sample : J3477-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S36-0135

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

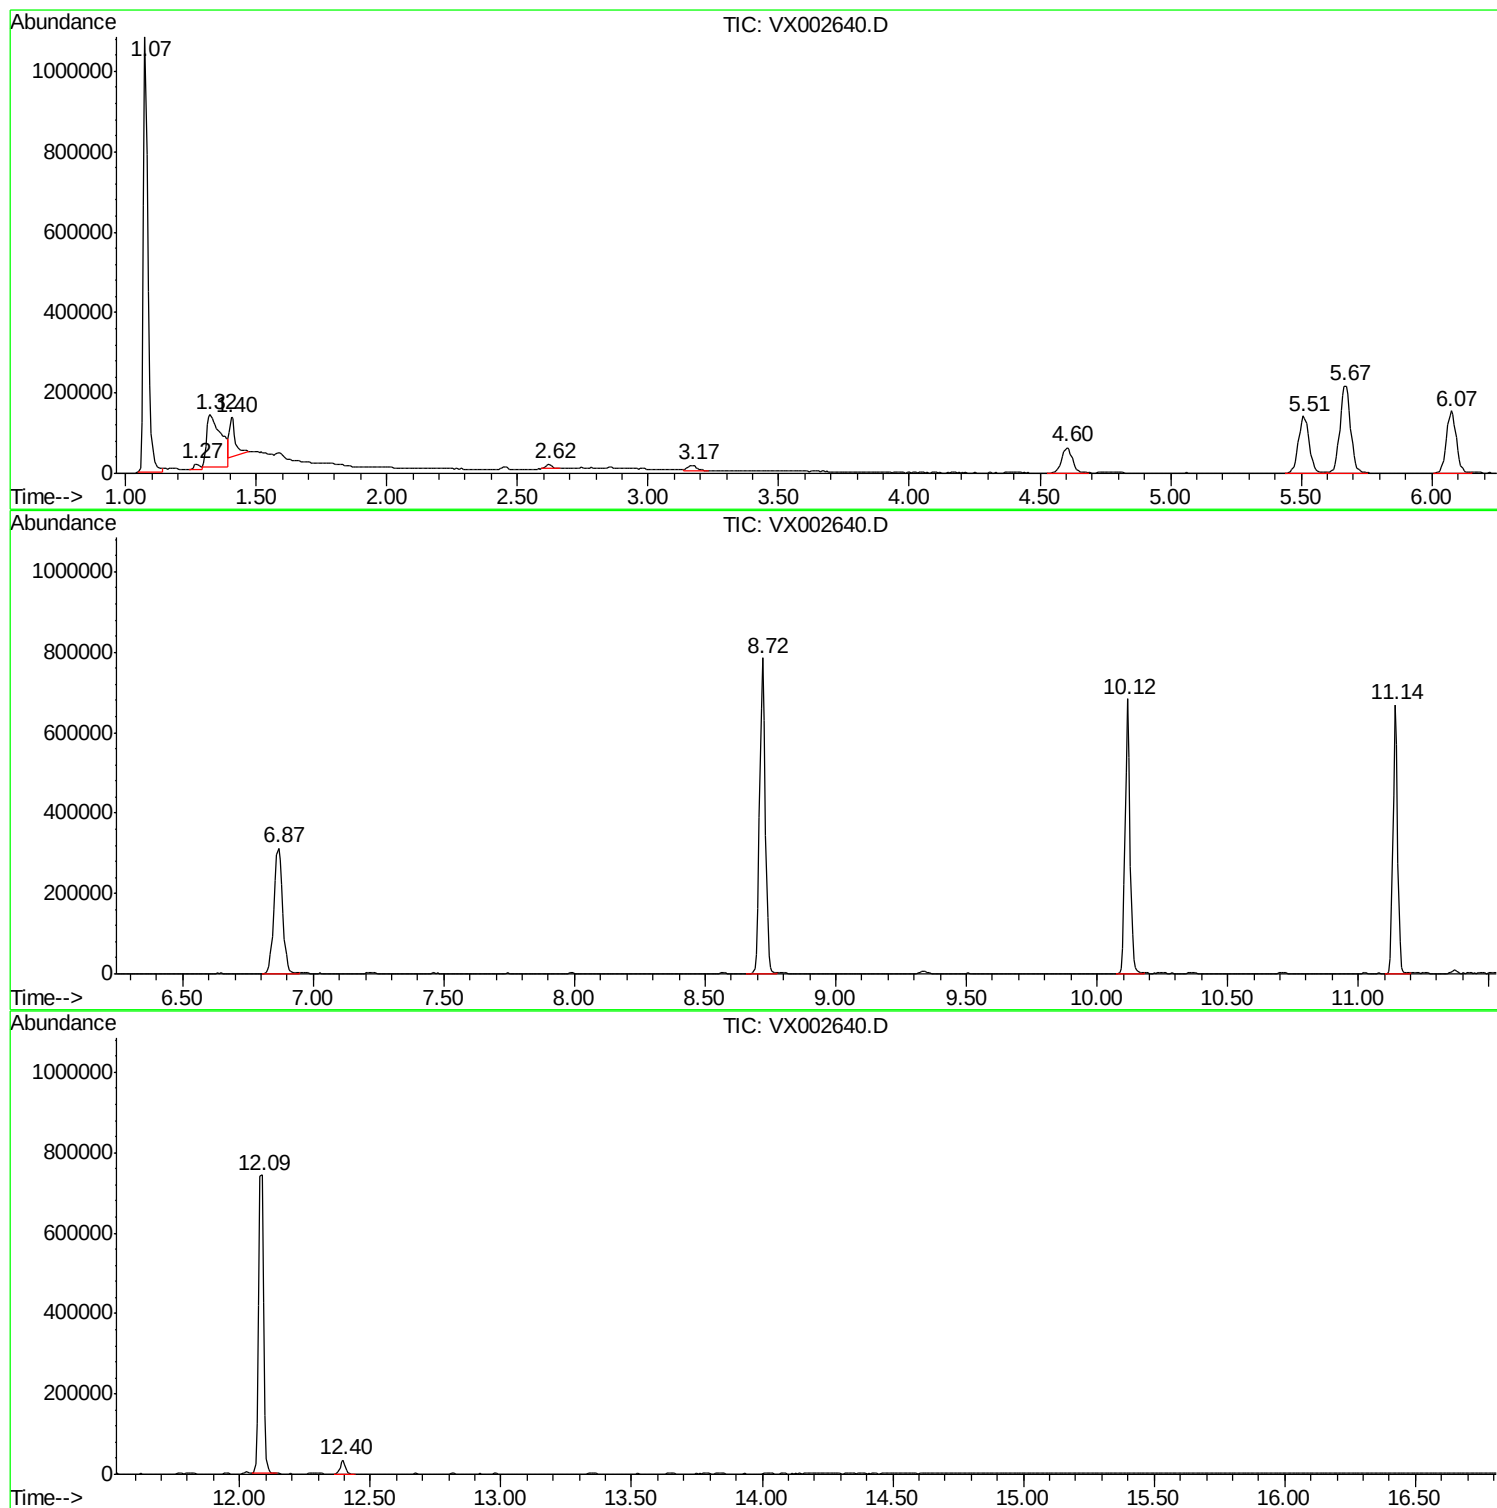

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061518\
Data File : VX002640.D
Acq On : 16 Jun 2018 11:36
Operator : JC/MD
Sample : J3477-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S36-0135










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Sulfur dioxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.32	42.42 ug/l	514821	Pentafluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Sulfur dioxide	64	O2S	007446-09-5	83
2		Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3		L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4		Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5		Ethyl Chloride	64	C2H5Cl	000075-00-3	3

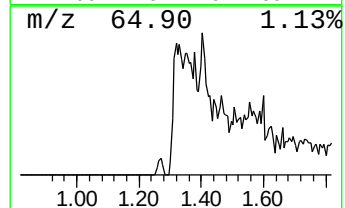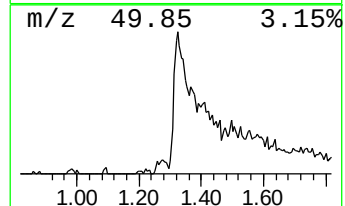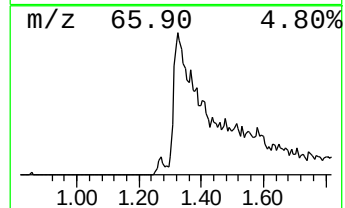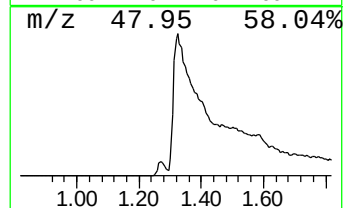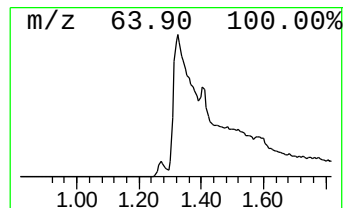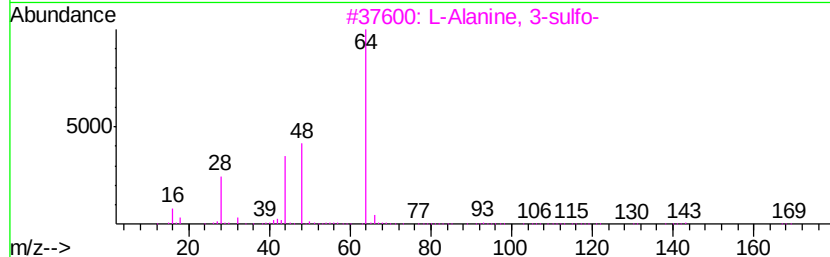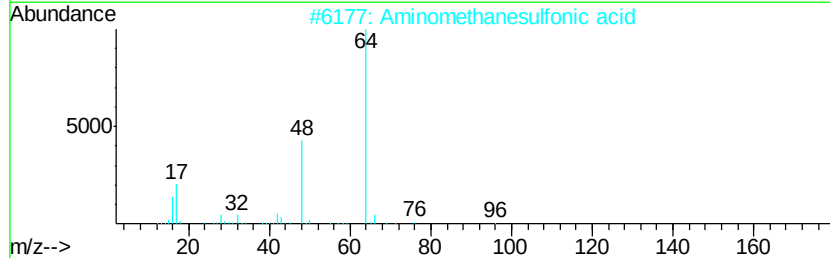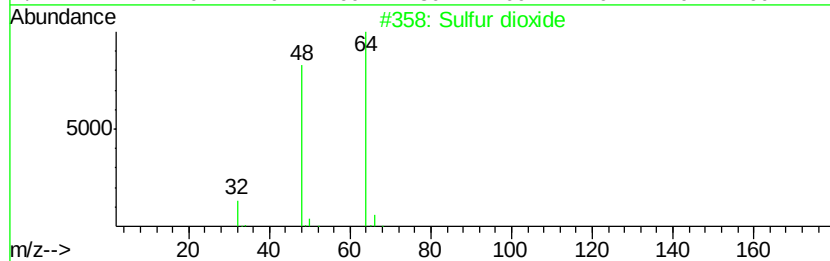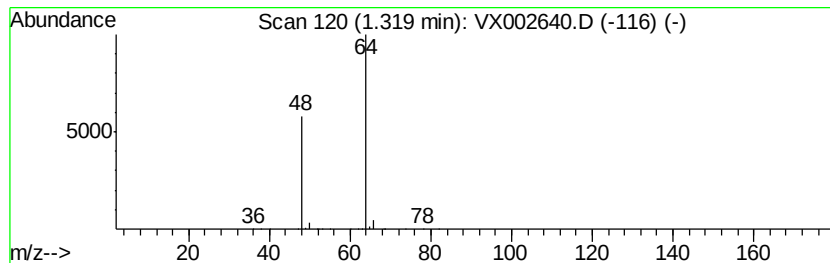

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061518\
Data File : VX002640.D
Acq On : 16 Jun 2018 11:36
Operator : JC/MD
Sample : J3477-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S36-0135










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Ethene, chloro- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.40	12.16 ug/l	147540	Pentafluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Ethene, chloro-	62	C2H3Cl	000075-01-4	90
2		Phosphine, ethyl-	62	C2H7P	000593-68-0	5
3		Peroxide, dimethyl	62	C2H6O2	000690-02-8	5
4		Ethanethiol	62	C2H6S	000075-08-1	4
5		Ethyne, difluoro-	62	C2F2	000689-99-6	3

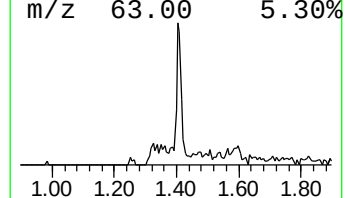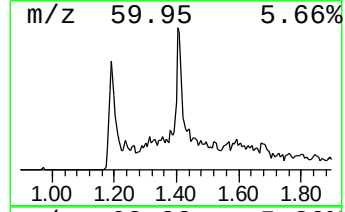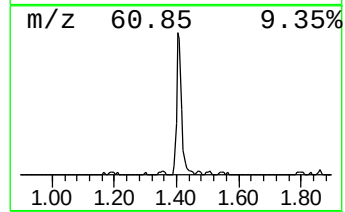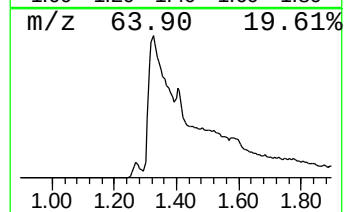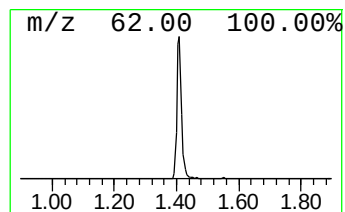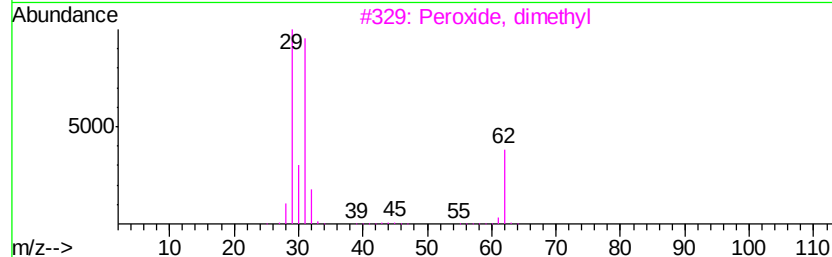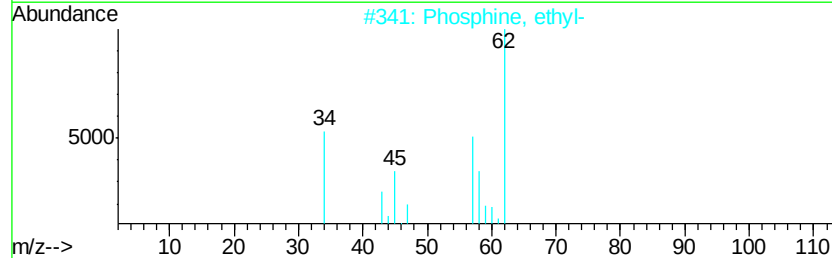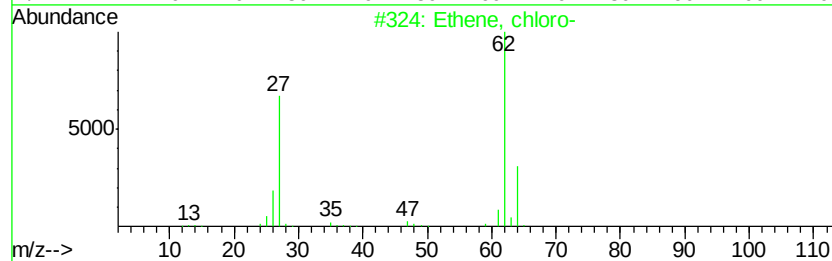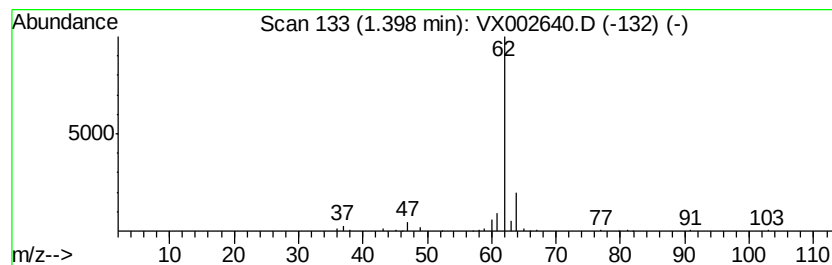

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX061518\
Data File : VX002640.D
Acq On : 16 Jun 2018 11:36
Operator : JC/MD
Sample : J3477-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S36-0135

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Sulfur dioxide	1.32	42.4	ug/l	514821	1	5.67	606831	50.0
Ethene, chloro-	1.40	12.2	ug/l	147540	1	5.67	606831	50.0