


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX061518\
Data File : VX002592.D
Acq On : 15 Jun 2018 10:49
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Title : SW846 8260
Last Update : Sat Jun 16 01:37:33 2018

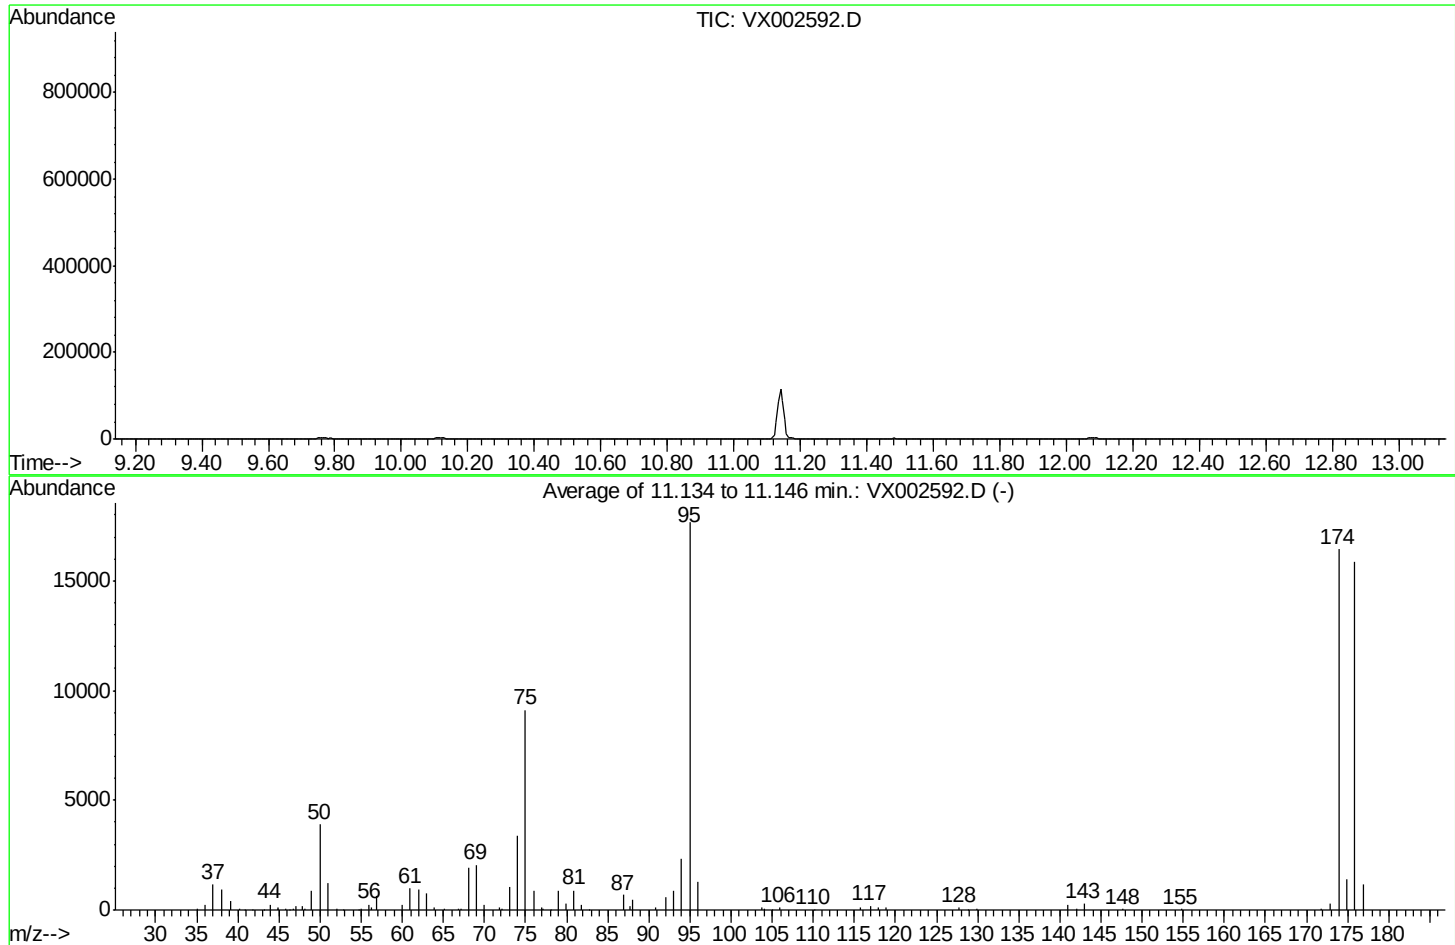

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	3907	PASS
75	95	30	60	51.7	9129	PASS
95	95	100	100	100.0	17667	PASS
96	95	5	9	7.1	1261	PASS
173	174	0.00	2	1.8	294	PASS
174	95	50	100	93.0	16427	PASS
175	174	5	9	8.4	1386	PASS
176	174	95	101	96.7	15881	PASS
177	176	5	9	7.3	1158	PASS