


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061518\
Data File : VX002600.D
Acq On : 15 Jun 2018 15:50
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Title : SW846 8260
Last Update : Sat Jun 16 01:37:33 2018

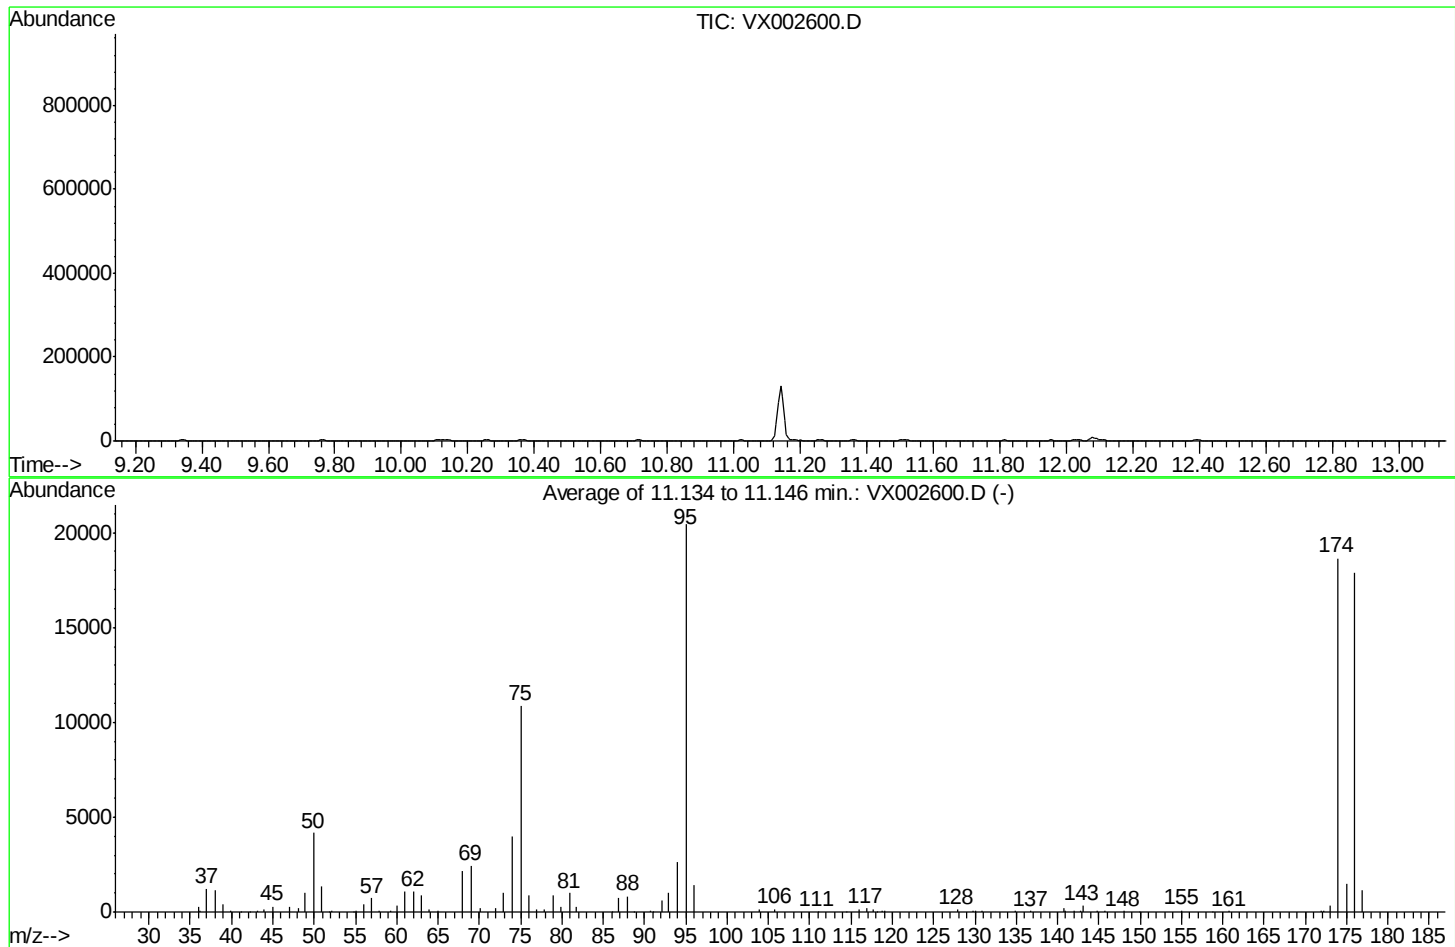

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	4163	PASS
75	95	30	60	53.2	10878	PASS
95	95	100	100	100.0	20437	PASS
96	95	5	9	6.9	1402	PASS
173	174	0.00	2	1.8	340	PASS
174	95	50	100	91.1	18628	PASS
175	174	5	9	8.1	1511	PASS
176	174	95	101	96.1	17907	PASS
177	176	5	9	6.3	1131	PASS