


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061518\
Data File : VX002625.D
Acq On : 16 Jun 2018 04:33
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Title : SW846 8260
Last Update : Sat Jun 16 01:37:33 2018

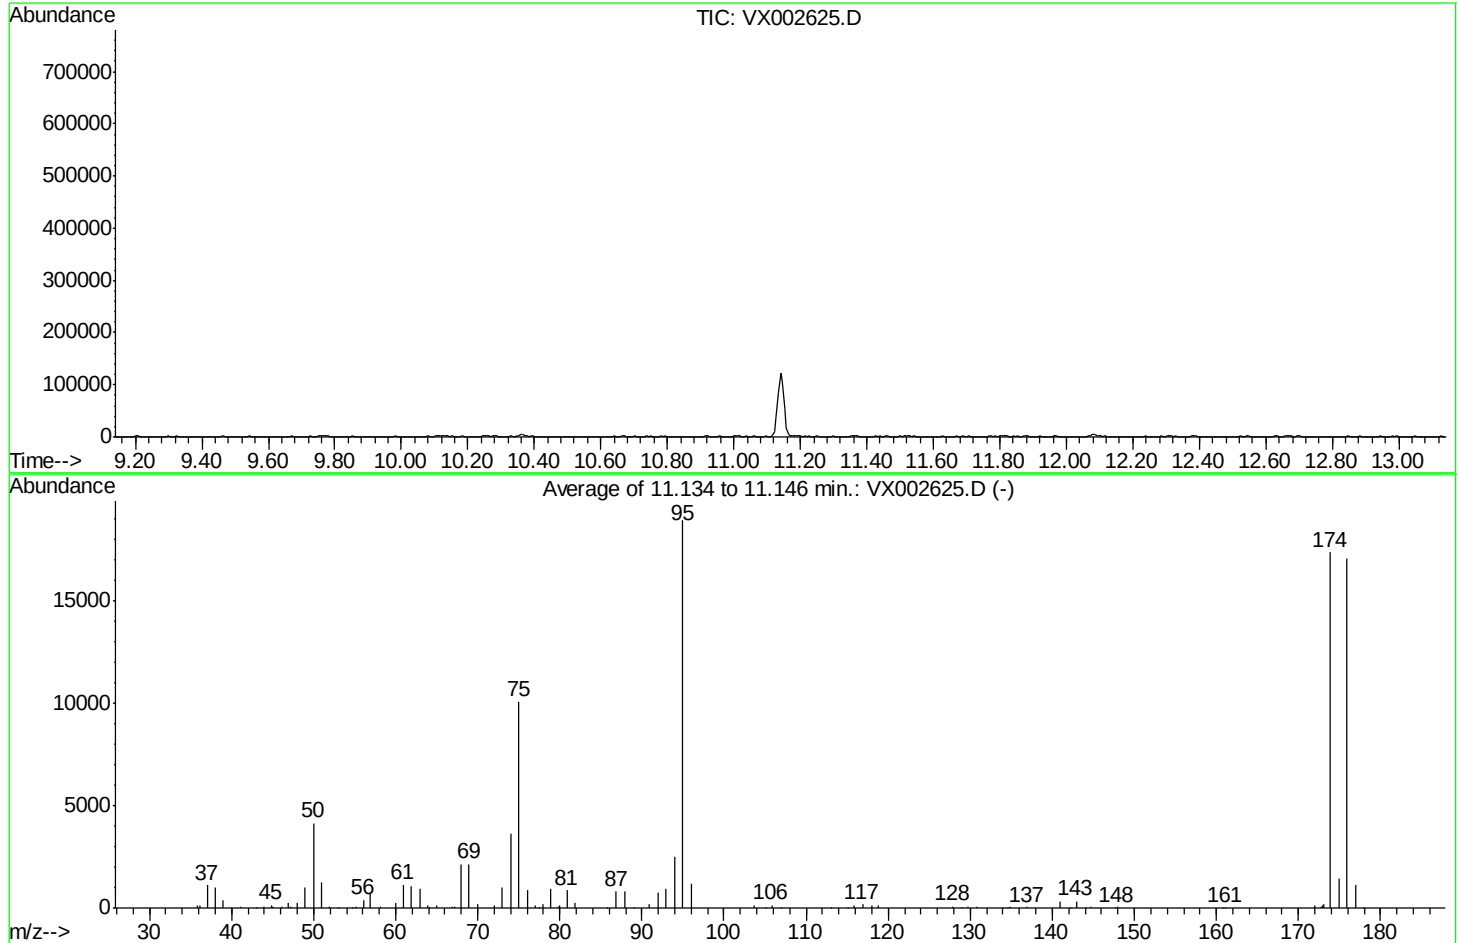

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	4146	PASS
75	95	30	60	53.3	10079	PASS
95	95	100	100	100.0	18924	PASS
96	95	5	9	6.2	1176	PASS
173	174	0.00	2	0.9	159	PASS
174	95	50	100	91.7	17344	PASS
175	174	5	9	8.1	1411	PASS
176	174	95	101	98.4	17062	PASS
177	176	5	9	6.6	1131	PASS