

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061618\
 Data File : VX002667.D
 Acq On : 17 Jun 2018 00:17
 Operator : JC/MD
 Sample : J3485-05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 T11-MW-16-10.5-061318

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	94	rBV	2297016	2590043	100.00%	29.819%
2	1.276	108	113	120	rBV	48200	70471	2.72%	0.811%
3	2.453	300	306	311	rBV	19080	32135	1.24%	0.370%
4	2.623	329	334	340	rVB	15527	29393	1.13%	0.338%
5	5.507	797	807	821	rBV2	140689	397841	15.36%	4.580%
6	5.672	821	834	850	rVB	209128	597270	23.06%	6.876%
7	6.074	887	900	918	rBV	153744	406852	15.71%	4.684%
8	6.867	1019	1030	1044	rBV	308093	722251	27.89%	8.315%
9	8.720	1326	1334	1343	rBV	744777	1165729	45.01%	13.421%
10	10.116	1557	1563	1574	rBV	666697	879640	33.96%	10.127%
11	11.140	1723	1731	1743	rBV	667616	828812	32.00%	9.542%
12	12.079	1880	1885	1893	rBV	743413	965429	37.27%	11.115%


Sum of corrected areas: 8685866

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061618\
Data File : VX002667.D
Acq On : 17 Jun 2018 00:17
Operator : JC/MD
Sample : J3485-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
T11-MW-16-10.5-061318

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

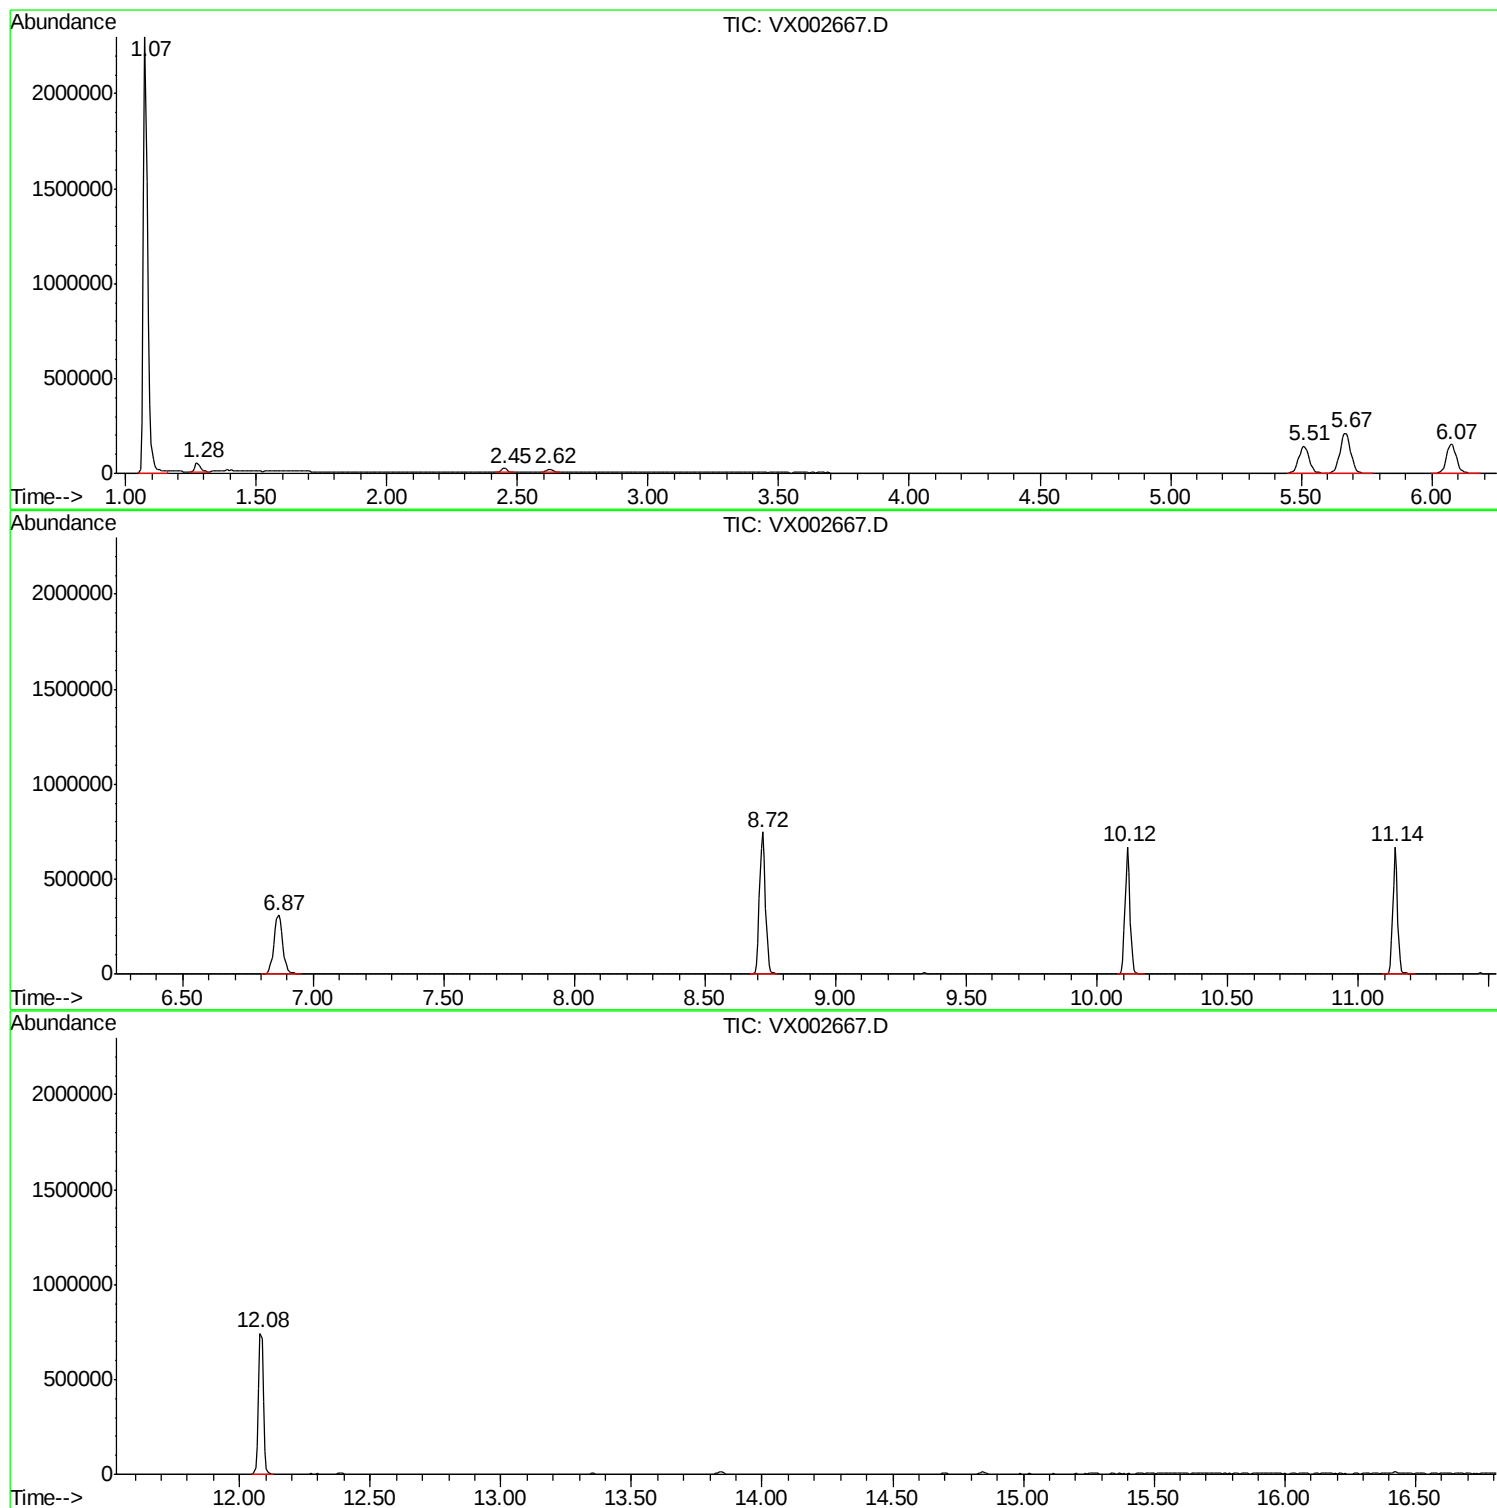

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061618\
Data File : VX002667.D
Acq On : 17 Jun 2018 00:17
Operator : JC/MD
Sample : J3485-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
T11-MW-16-10.5-061318










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Sulfur dioxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.28	5.90 ug/l	70471	Pentafluorobenzene	5.67

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Sulfur dioxide	64	O2S	007446-09-5	83
2		Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3		L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4		Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5		Ethyl Chloride	64	C2H5Cl	000075-00-3	3

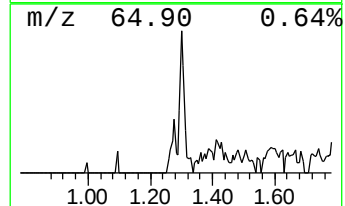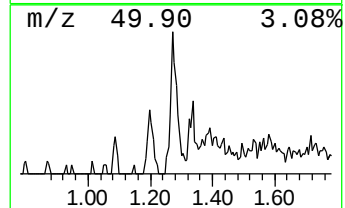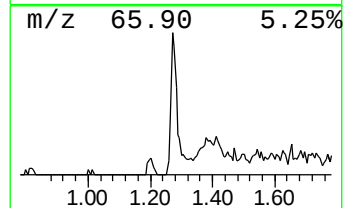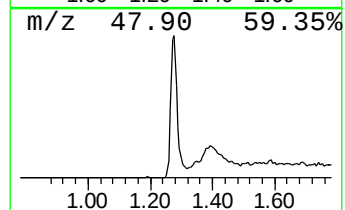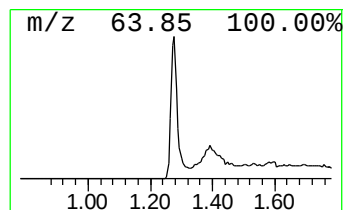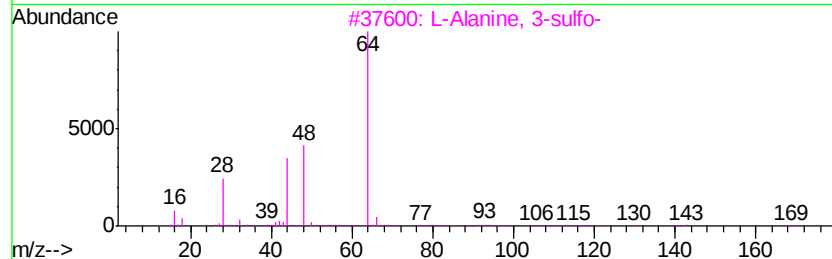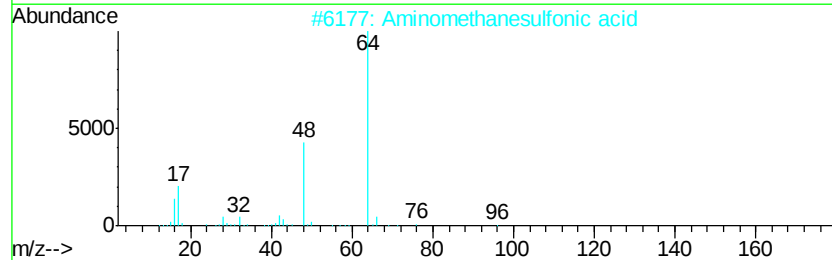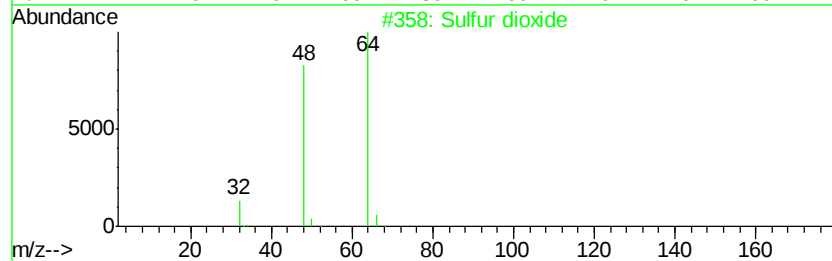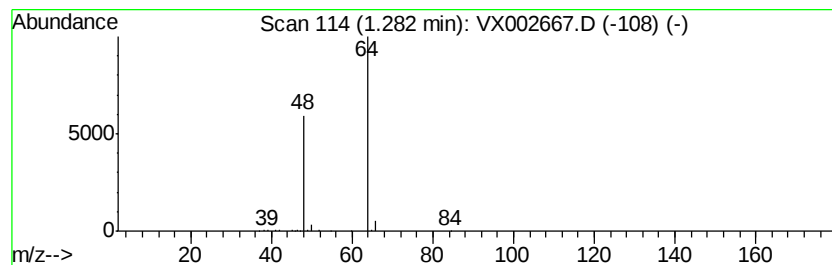

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX061618\
Data File : VX002667.D
Acq On : 17 Jun 2018 00:17
Operator : JC/MD
Sample : J3485-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
T11-MW-16-10.5-061318

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.28	5.9	ug/l	70471	1	5.67	597270	50.0