


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX061618\
 Data File : VX002651.D
 Acq On : 16 Jun 2018 17:13
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
 Title : SW846 8260
 Last Update : Sat Jun 16 01:37:33 2018

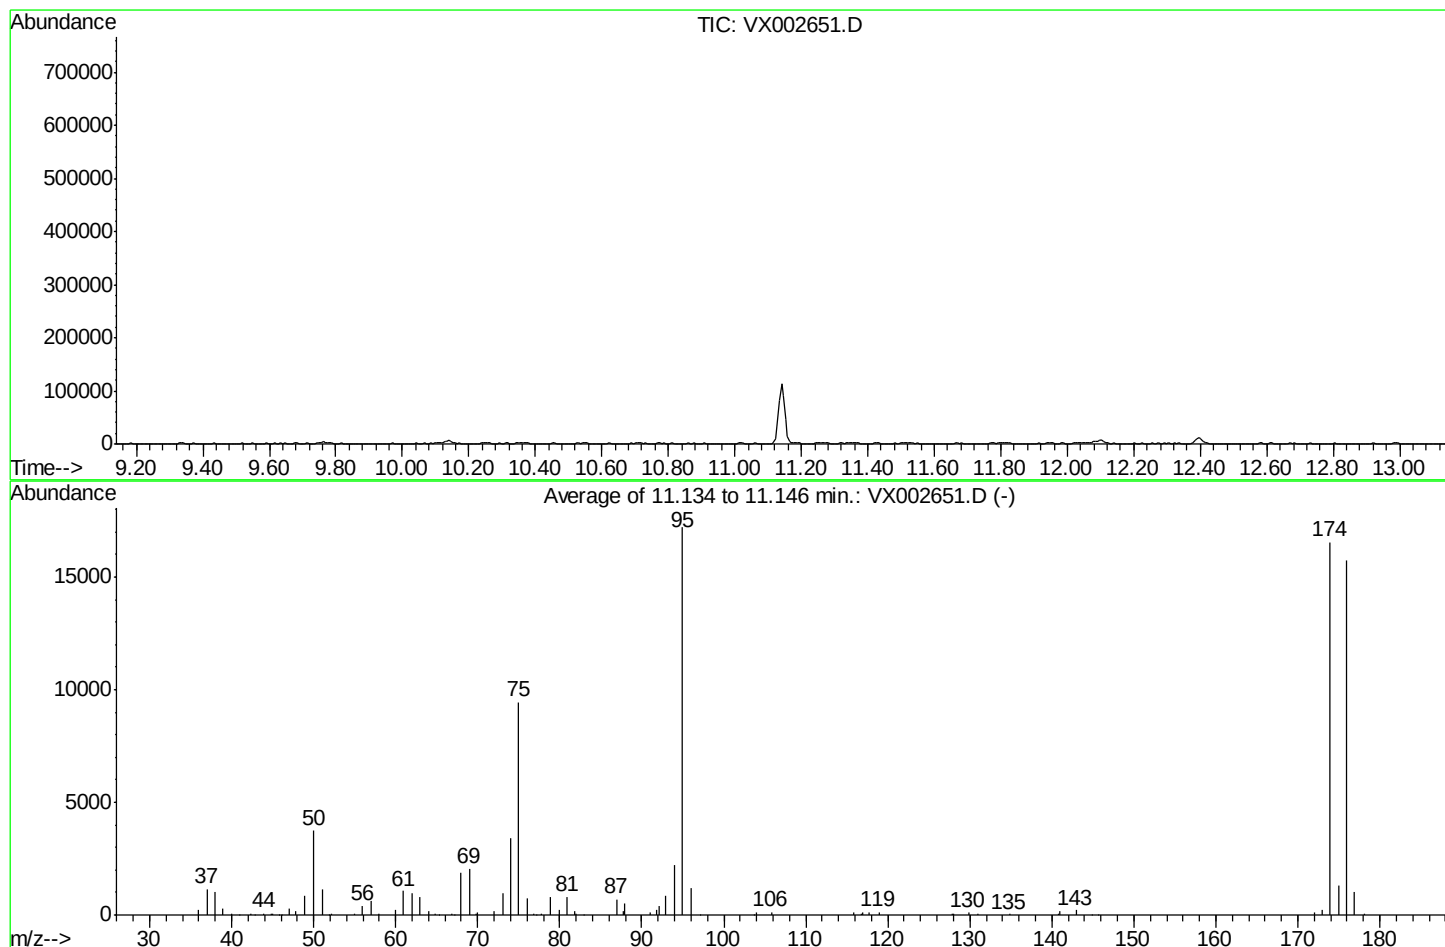

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	3739	PASS
75	95	30	60	54.8	9437	PASS
95	95	100	100	100.0	17211	PASS
96	95	5	9	7.1	1223	PASS
173	174	0.00	2	1.5	252	PASS
174	95	50	100	96.2	16561	PASS
175	174	5	9	7.8	1297	PASS
176	174	95	101	95.2	15764	PASS
177	176	5	9	6.4	1008	PASS