


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX061818\
 Data File : VX002676.D
 Acq On : 18 Jun 2018 11:52
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X061818W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Mon Jun 18 15:18:02 2018

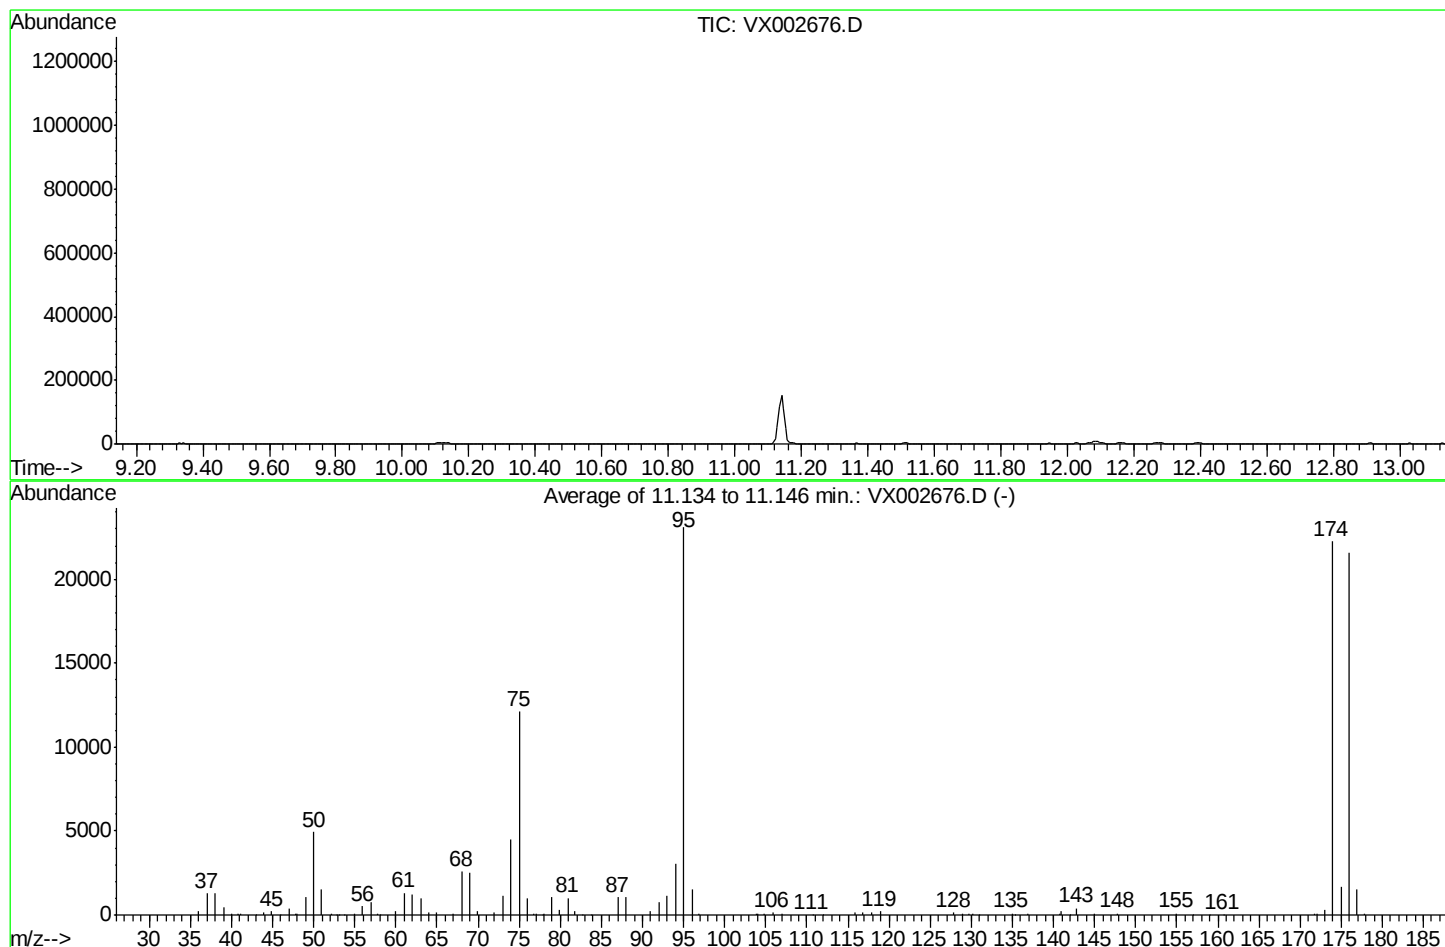

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	4949	PASS
75	95	30	60	52.4	12105	PASS
95	95	100	100	100.0	23093	PASS
96	95	5	9	6.6	1534	PASS
173	174	0.00	2	1.3	300	PASS
174	95	50	100	96.4	22264	PASS
175	174	5	9	7.7	1712	PASS
176	174	95	101	96.9	21578	PASS
177	176	5	9	7.0	1511	PASS