


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX061818\
 Data File : VX002690.D
 Acq On : 18 Jun 2018 20:07
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
 Title : SW846 8260
 Last Update : Sat Jun 16 01:37:33 2018

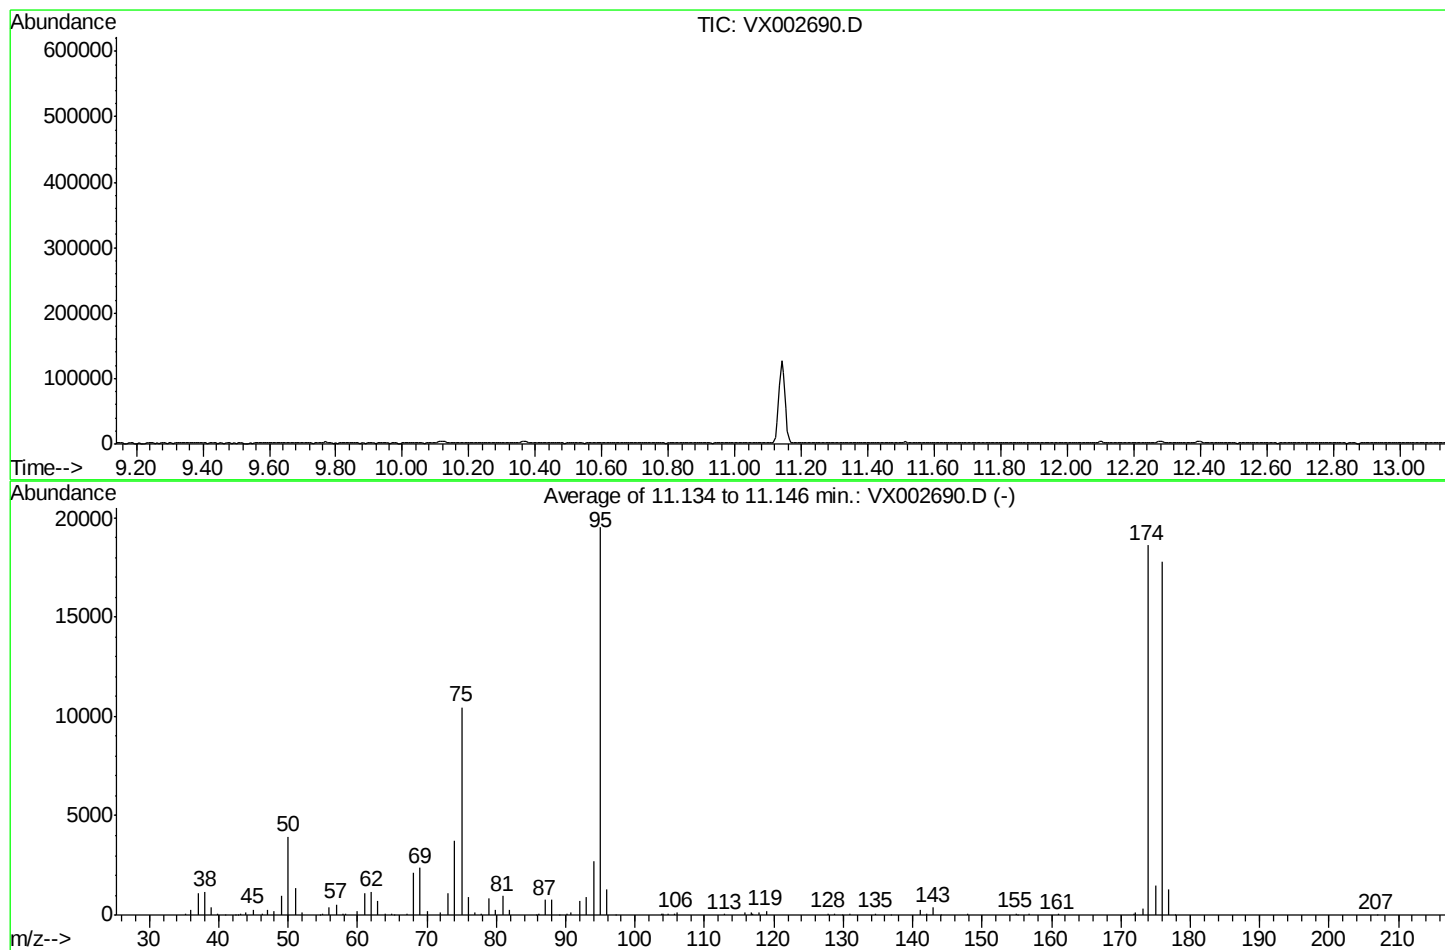

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	3963	PASS
75	95	30	60	53.5	10447	PASS
95	95	100	100	100.0	19530	PASS
96	95	5	9	6.5	1273	PASS
173	174	0.00	2	1.6	293	PASS
174	95	50	100	95.3	18616	PASS
175	174	5	9	8.0	1493	PASS
176	174	95	101	95.8	17826	PASS
177	176	5	9	7.4	1314	PASS