

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX061918\
Data File : VX002728.D
Acq On : 19 Jun 2018 22:04
Operator : JC/MD
Sample : J3502-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20180367-SITE-WATER

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	92	rBV	574456	766389	65.01%	11.051%
2	1.270	108	112	121	rBV	64498	97159	8.24%	1.401%
3	1.605	160	167	171	rBV3	7627	14777	1.25%	0.213%
4	2.446	301	305	313	rBV	6325	12147	1.03%	0.175%
5	5.507	795	807	818	rBV	142014	407502	34.57%	5.876%
6	5.665	822	833	849	rVB	217061	607828	51.56%	8.765%
7	6.074	889	900	914	rBV	157698	414953	35.20%	5.984%
8	6.866	1018	1030	1043	rBV	314407	731401	62.05%	10.547%
9	8.720	1327	1334	1343	rBV	786005	1178810	100.00%	16.999%
10	10.116	1557	1563	1573	rBV	676897	889592	75.47%	12.828%
11	11.140	1725	1731	1740	rBV	668844	837439	71.04%	12.076%
12	12.085	1880	1886	1894	rVB	757851	976779	82.86%	14.085%


Sum of corrected areas: 6934776

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061918\
Data File : VX002728.D
Acq On : 19 Jun 2018 22:04
Operator : JC/MD
Sample : J3502-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20180367-SITE-WATER

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

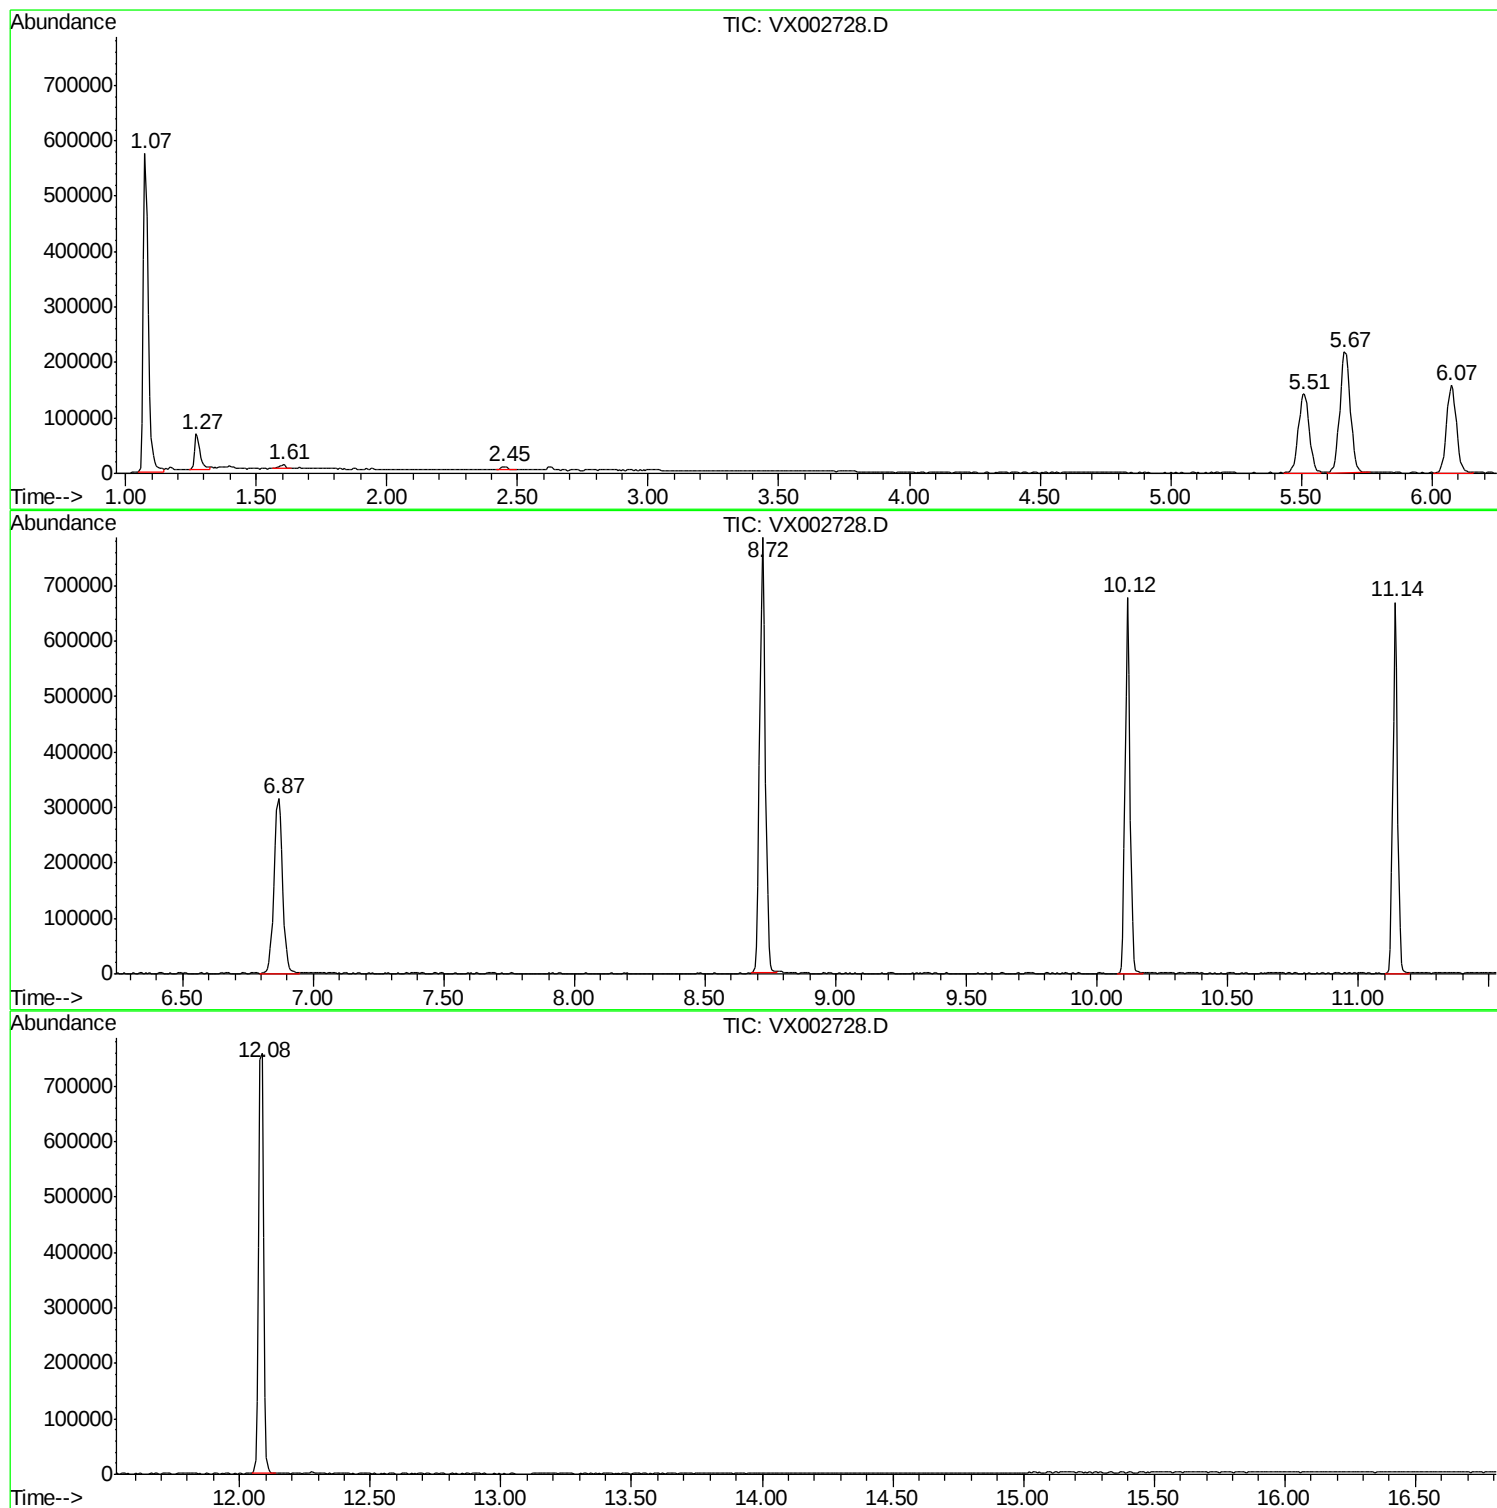

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX061918\
Data File : VX002728.D
Acq On : 19 Jun 2018 22:04
Operator : JC/MD
Sample : J3502-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20180367-SITE-WATER










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Sulfur dioxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.27	7.99 ug/l	97159	Pentafluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Sulfur dioxide	64	O2S	007446-09-5	83
2		Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3		L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4		Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5		Ethyl Chloride	64	C2H5Cl	000075-00-3	3

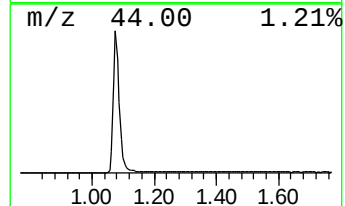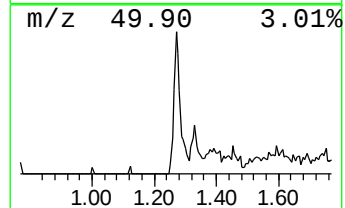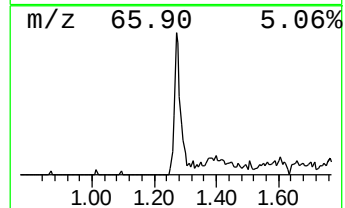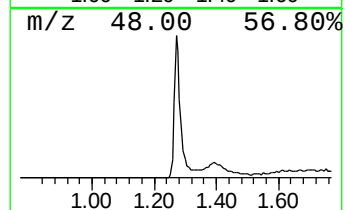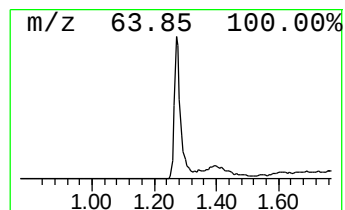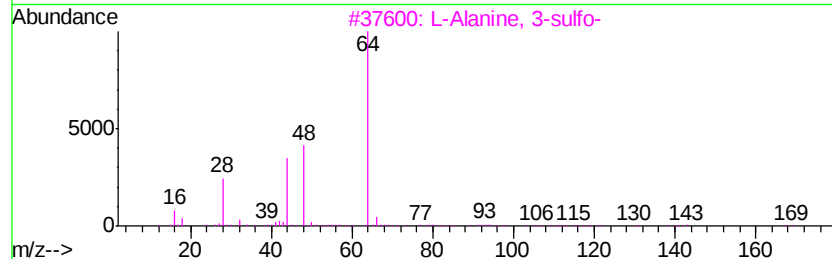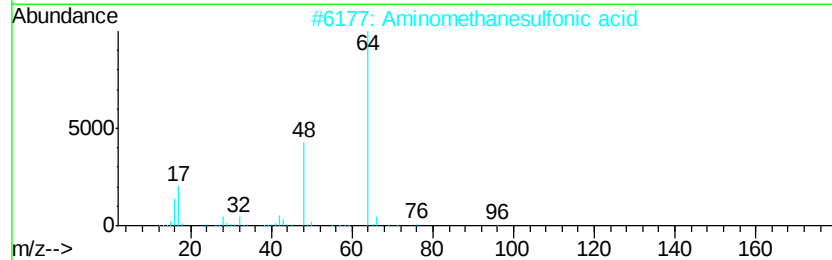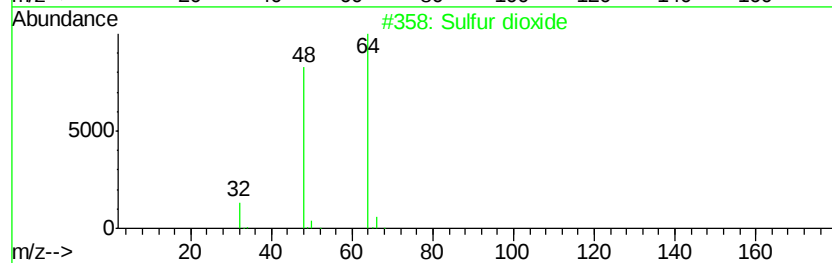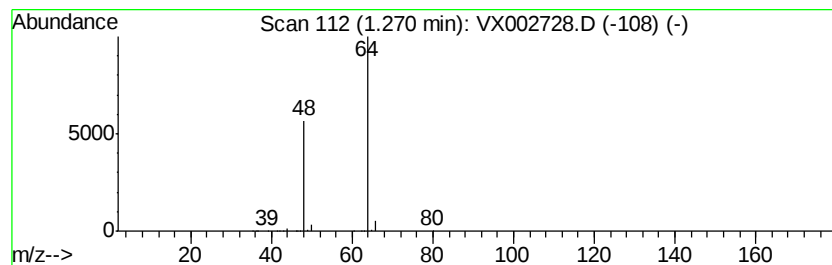

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX061918\
Data File : VX002728.D
Acq On : 19 Jun 2018 22:04
Operator : JC/MD
Sample : J3502-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20180367-SITE-WATER

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.27	8.0	ug/l	97159	1	5.67	607828	50.0