

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062018\
Data File : VX002746.D
Acq On : 20 Jun 2018 17:13
Operator : JC/MD
Sample : J3596-08
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MANHATTANVILLE-TRIP-BLANK-2-

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	91	rBV	515263	703779	58.47%	9.486%
2	1.270	108	112	117	rBV	198944	241972	20.10%	3.262%
3	1.331	117	122	143	rVB	53535	242659	20.16%	3.271%
4	2.624	330	334	341	rVB	6835	12263	1.02%	0.165%
5	5.507	795	807	820	rBV3	149005	421589	35.02%	5.683%
6	5.666	823	833	849	rVB	225854	629503	52.30%	8.485%
7	6.074	888	900	919	rBV	160925	415202	34.49%	5.597%
8	6.867	1019	1030	1049	rBV	321041	755859	62.79%	10.188%
9	8.720	1327	1334	1352	rBV	782792	1203698	100.00%	16.225%
10	10.116	1557	1563	1574	rBV	673269	904328	75.13%	12.190%
11	11.140	1725	1731	1740	rBV	694741	864887	71.85%	11.658%
12	12.079	1879	1885	1893	rBV	806523	1023052	84.99%	13.790%


Sum of corrected areas: 7418791

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062018\
Data File : VX002746.D
Acq On : 20 Jun 2018 17:13
Operator : JC/MD
Sample : J3596-08
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MANHATTANVILLE-TRIP-BLANK-2-

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

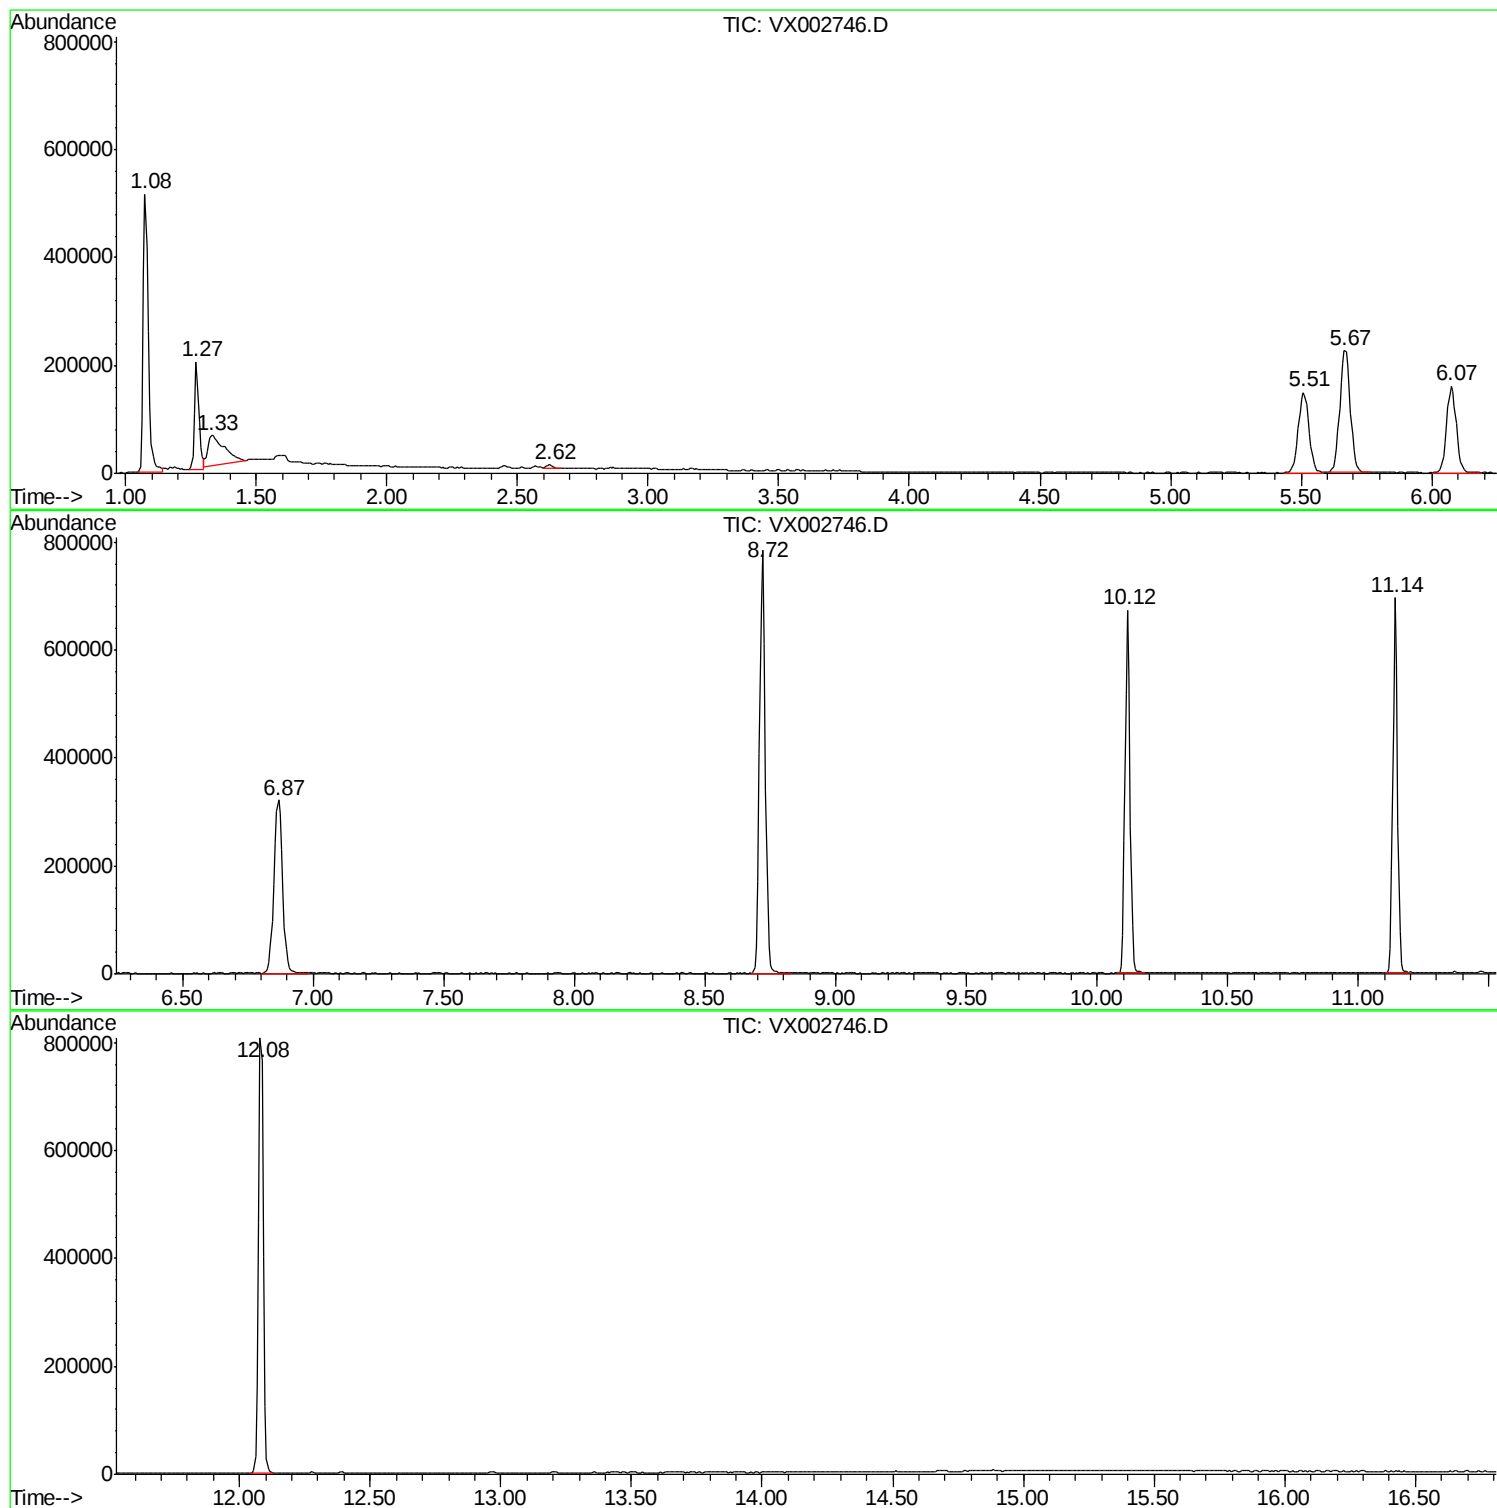

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062018\
Data File : VX002746.D
Acq On : 20 Jun 2018 17:13
Operator : JC/MD
Sample : J3596-08
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1










Instrument :
MSVOA_X
ClientSampleId :
MANHATTANVILLE-TRIP-BLANK-2-

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Sulfur dioxide Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.27	19.22 ug/l	241972	Pentafluorobenzene	5.67
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1		Sulfur dioxide	64 O2S	007446-09-5 83
2		Aminomethanesulfonic acid	111 CH5NO3S	013881-91-9 74
3		L-Alanine, 3-sulfo-	169 C3H7NO5S	000498-40-8 9
4		Ethene, 1,1-difluoro-	64 C2H2F2	000075-38-7 4
5		Ethyl Chloride	64 C2H5Cl	000075-00-3 3

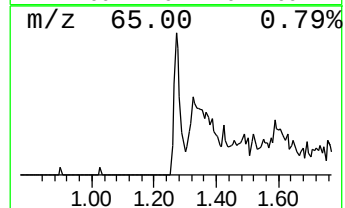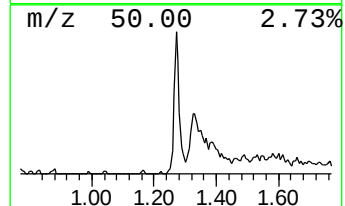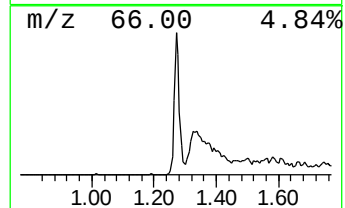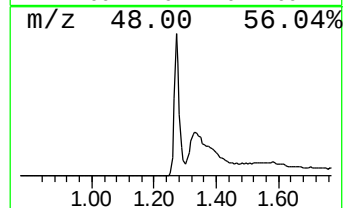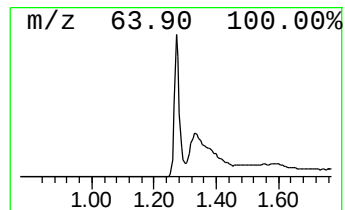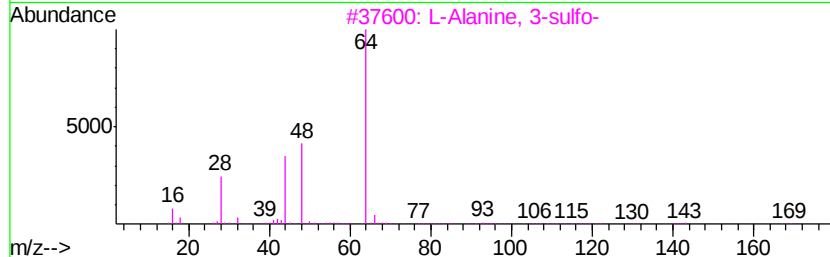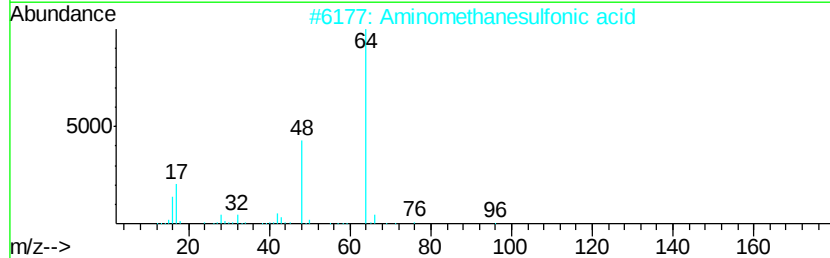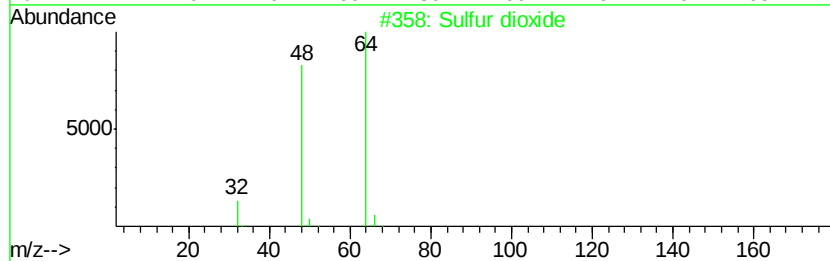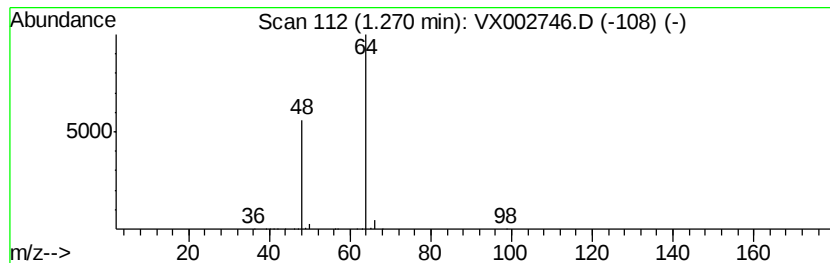

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX062018\
Data File : VX002746.D
Acq On : 20 Jun 2018 17:13
Operator : JC/MD
Sample : J3596-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MANHATTANVILLE-TRIP-BLANK-2-

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.27	19.2	ug/l	241972	1	5.67	629503	50.0