


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX062018\
Data File : VX002732.D
Acq On : 20 Jun 2018 09:33
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Title : SW846 8260
Last Update : Sat Jun 16 01:37:33 2018

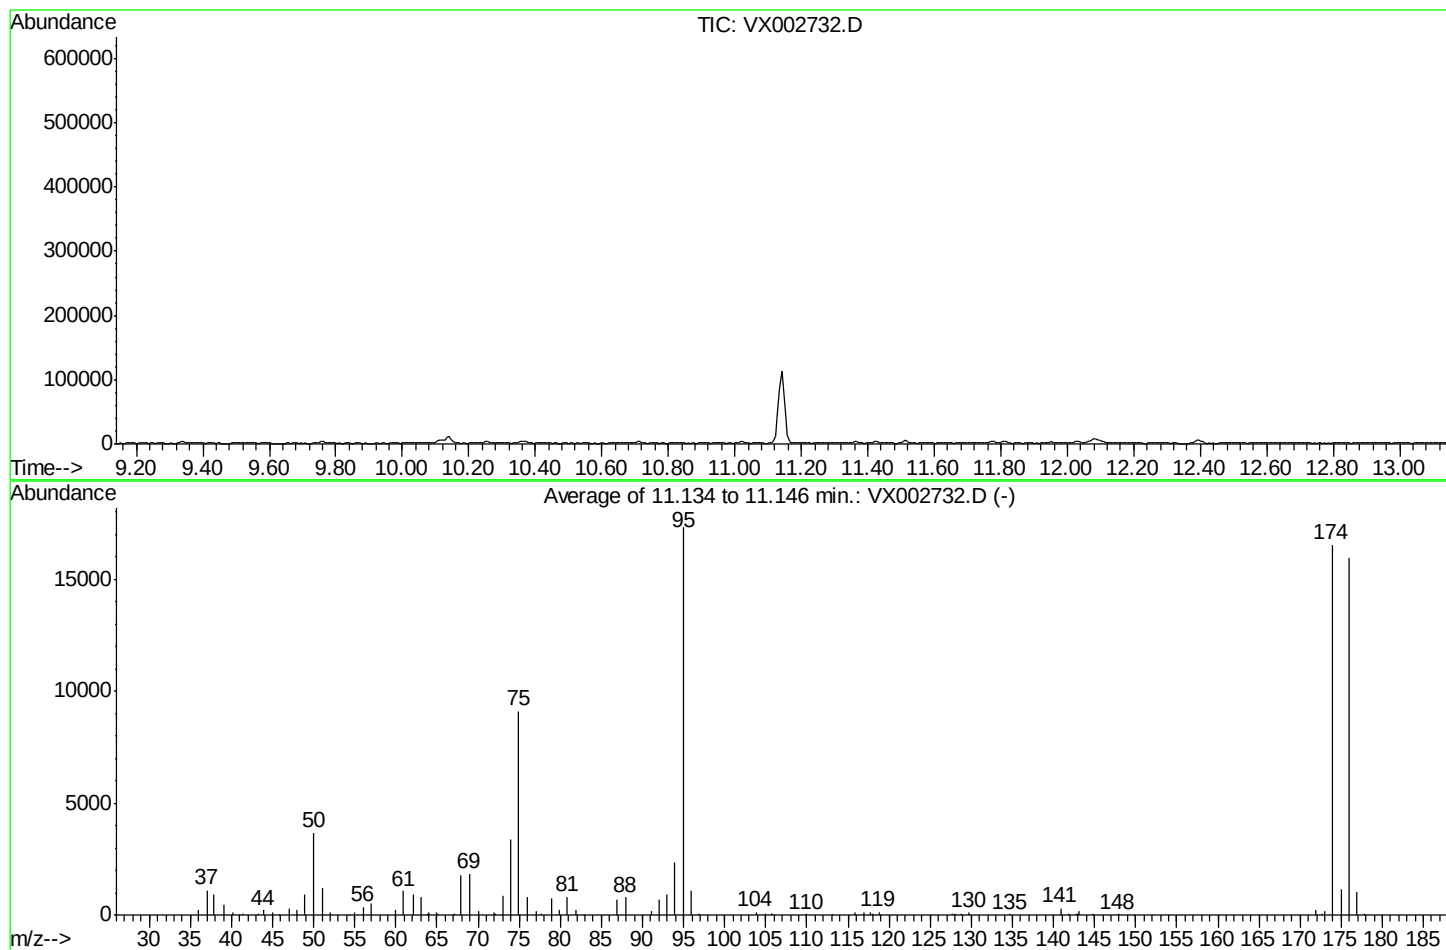

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	3682	PASS
75	95	30	60	52.5	9097	PASS
95	95	100	100	100.0	17325	PASS
96	95	5	9	6.2	1072	PASS
173	174	0.00	2	1.0	158	PASS
174	95	50	100	95.4	16533	PASS
175	174	5	9	7.0	1164	PASS
176	174	95	101	96.5	15957	PASS
177	176	5	9	6.4	1017	PASS