

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX062118\
 Data File : VX002826.D
 Acq On : 22 Jun 2018 08:51
 Operator : JC/MD
 Sample : J3603-24
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 26KV-TP-11

Quant Time: Jun 22 09:41:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 16 01:37:33 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	243252	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	346279	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	327819	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	183809	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	170898	46.23	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.46%	
35) Dibromofluoromethane	5.51	113	132054	47.78	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.56%	
50) Toluene-d8	8.72	98	496319	47.30	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.60%	
62) 4-Bromofluorobenzene	11.14	95	176339	44.35	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.70%	
Target Compounds						
16) Acetone	2.45	43	19431	11.91	ug/l	99
18) Methyl Acetate	2.78	43	19679	4.53	ug/l	96
20) Methylene Chloride	2.86	84	57895	17.31	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX062118\
Data File : VX002826.D
Acq On : 22 Jun 2018 08:51
Operator : JC/MD
Sample : J3603-24
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
26KV-TP-11

Quant Time: Jun 22 09:41:11 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061518W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 16 01:37:33 2018
Response via : Initial Calibration




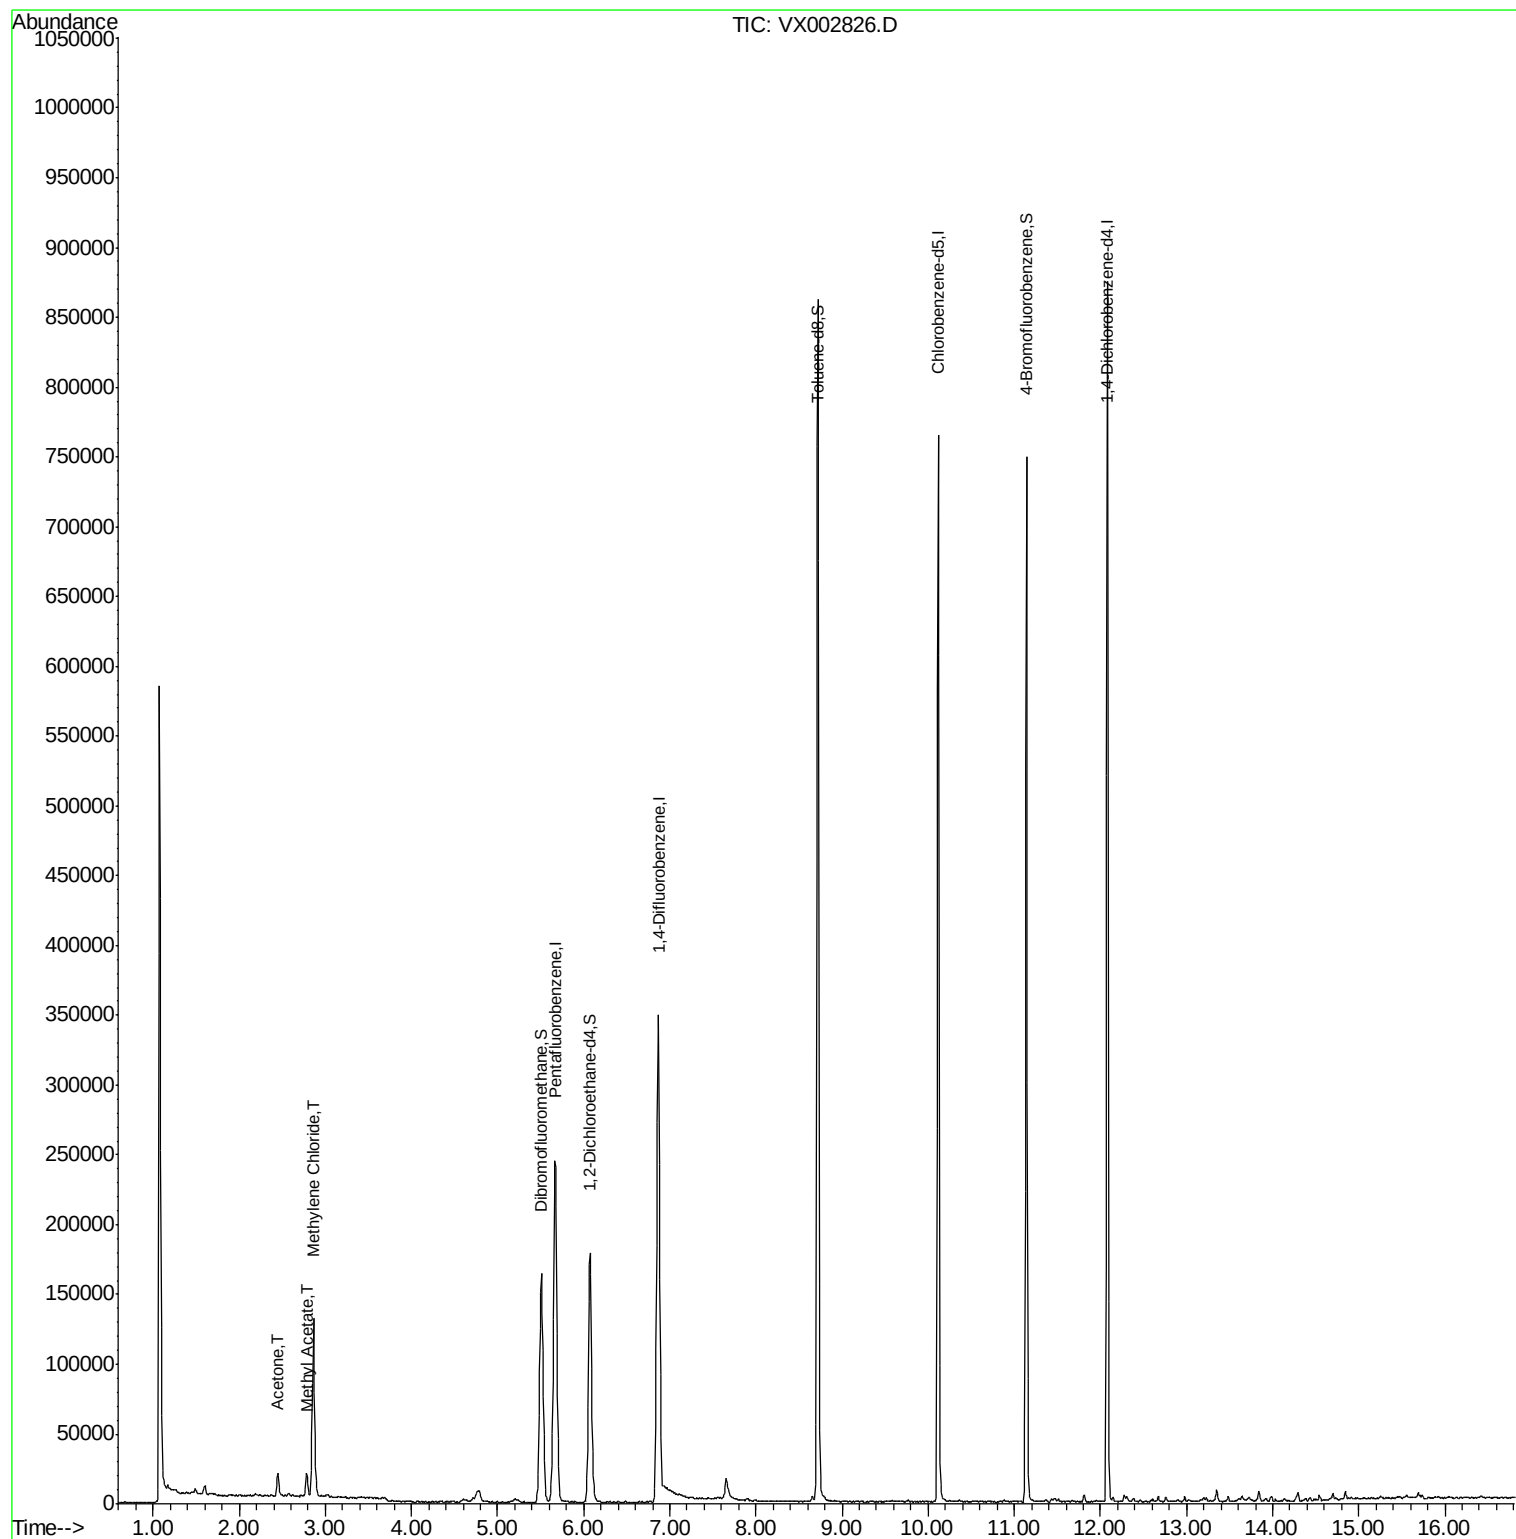


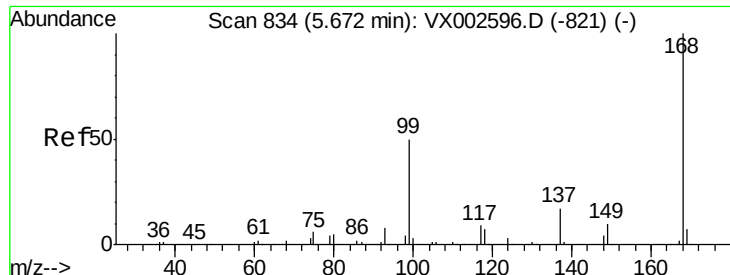

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.67 min Scan# 833
Delta R.T. -0.01 min
Lab File: VX002826.D
Acq: 22 Jun 2018 08:51




Instrument :
MSVOA_X
ClientSampleId :
26KV-TP-11


Tot Ion:168 Resp: 243252
Ion Ratio Lower Upper
168 100
99 51.3 39.3 58.9

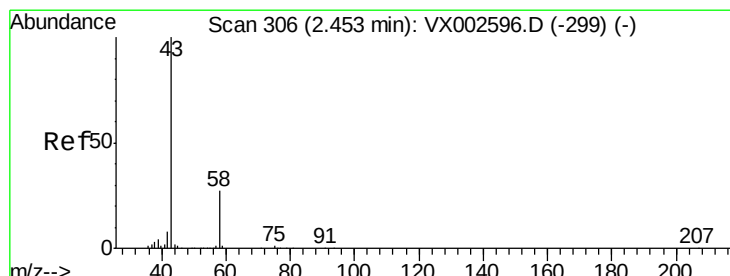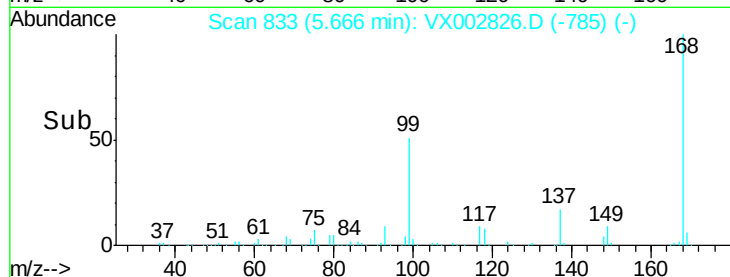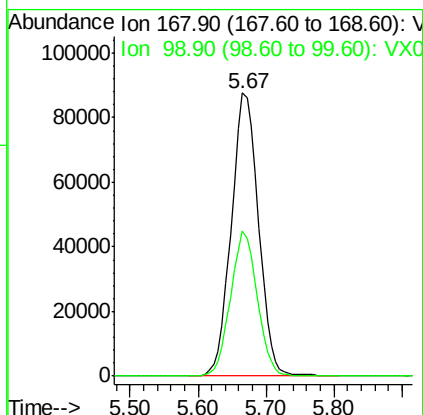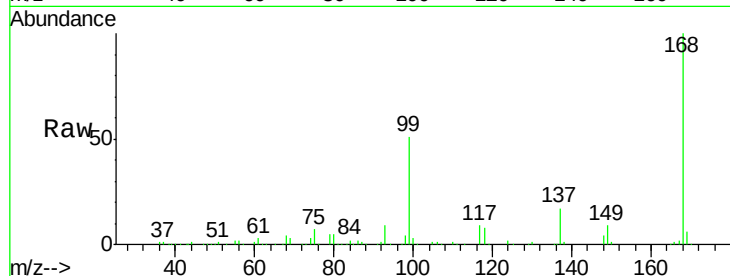

#16
Acetone
Concen: 11.91 ug/l
RT: 2.45 min Scan# 305
Delta R.T. -0.01 min
Lab File: VX002826.D
Acq: 22 Jun 2018 08:51

Tgt Ion: 43 Resp: 19431
Ion Ratio Lower Upper
43 100
58 28.1 22.1 33.1


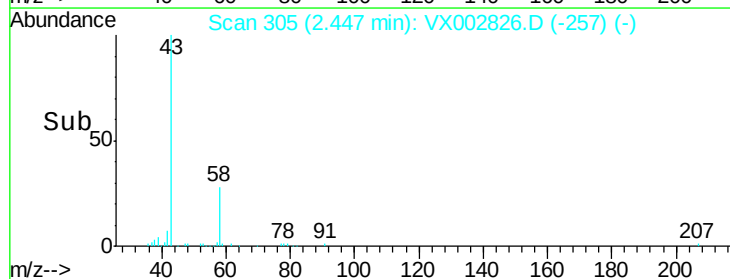
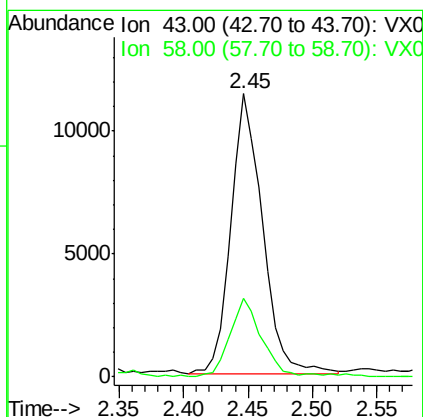
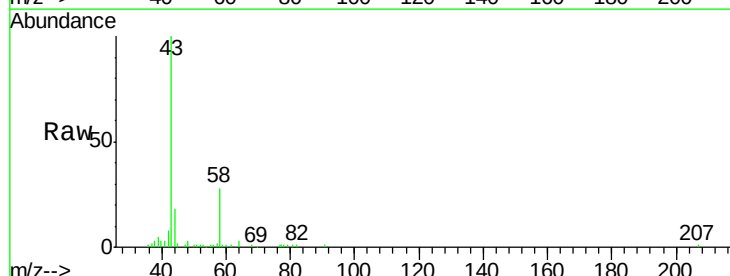


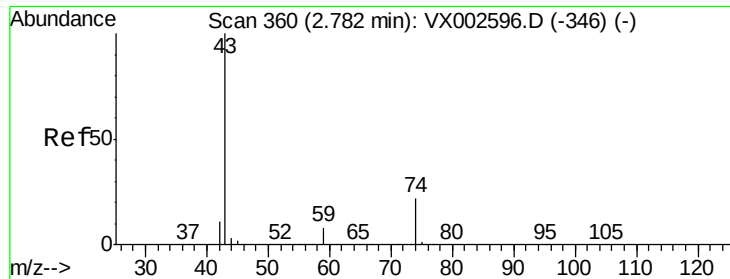

#18
Methvl Acetate
Concen: 4.53 ug/l
RT: 2.78 min Scan# 360
Delta R.T. 0.00 min
Lab File: VX002826.D
Acq: 22 Jun 2018 08:51




Instrument :
MSVOA_X
ClientSampleId :
26KV-TP-11


Tot Ion: 43 Resp: 19679
Ion Ratio Lower Upper
43 100
74 22.6 16.7 25.1

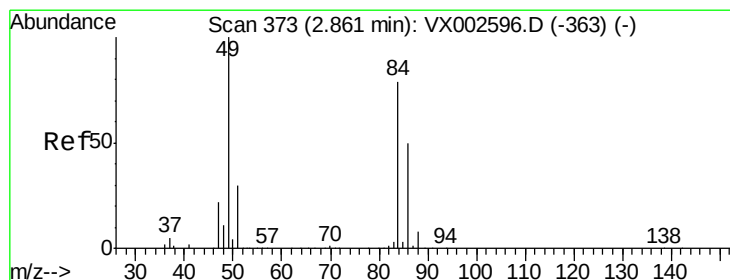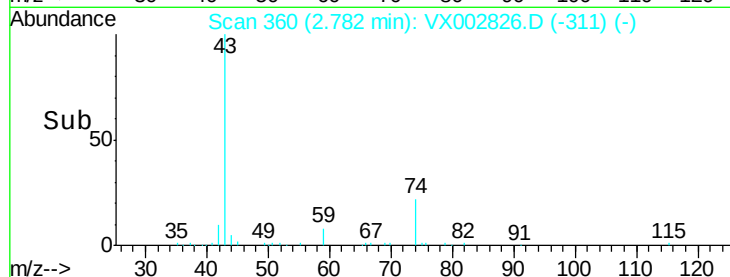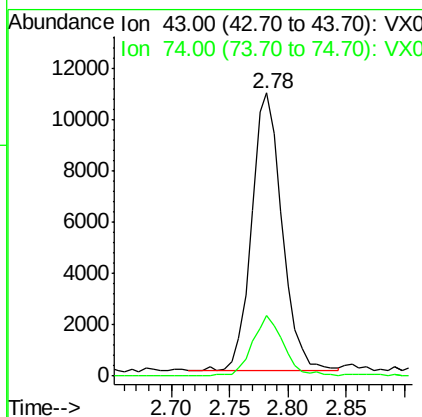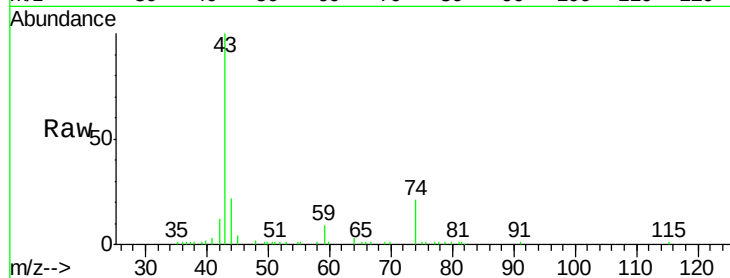

#20
Methylene Chloride
Concen: 17.31 ug/l
RT: 2.86 min Scan# 373
Delta R.T. 0.00 min
Lab File: VX002826.D
Acq: 22 Jun 2018 08:51

Tgt Ion: 84 Resp: 57895
Ion Ratio Lower Upper
84 100
49 130.2 107.8 161.6
51 38.6 32.8 49.2
86 67.0 52.5 78.7


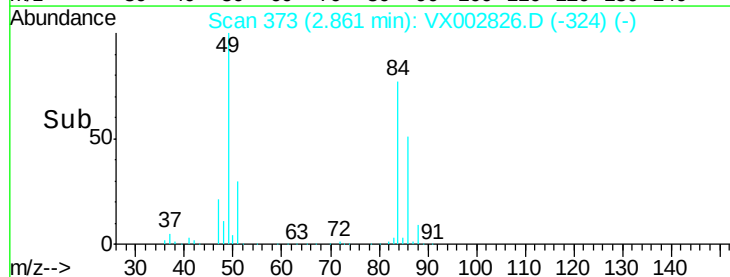
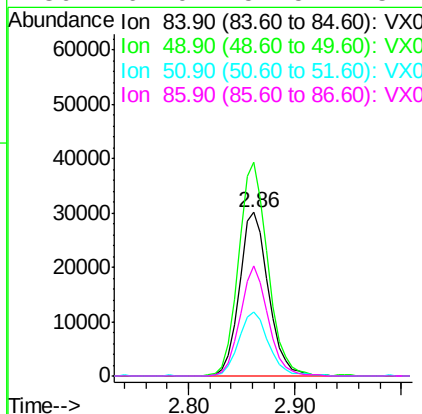
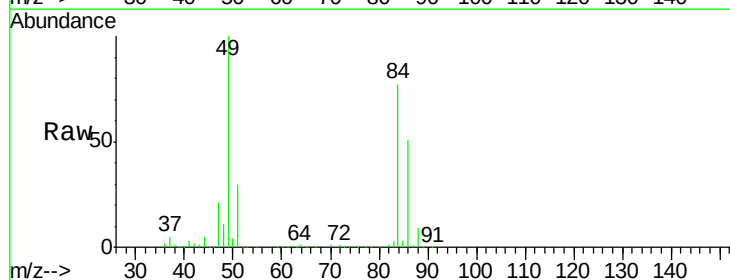


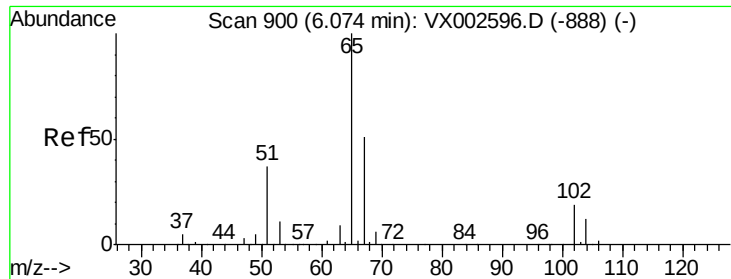

#33
 1,2-Dichloroethane-d4
 Concen: 46.23 ug/l
 RT: 6.07 min Scan# 900
 Delta R.T. 0.00 min
 Lab File: VX002826.D
 Acq: 22 Jun 2018 08:51




Instrument :
 MSVOA_X
 ClientSampleId :
 26KV-TP-11


Tot Ion: 65 Resp: 170898
 Ion Ratio Lower Upper
 65 100
 67 50.7 0.0 102.6

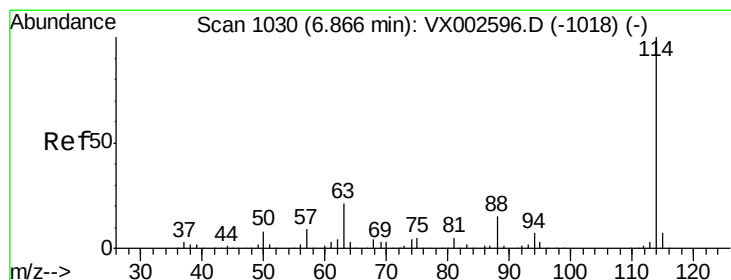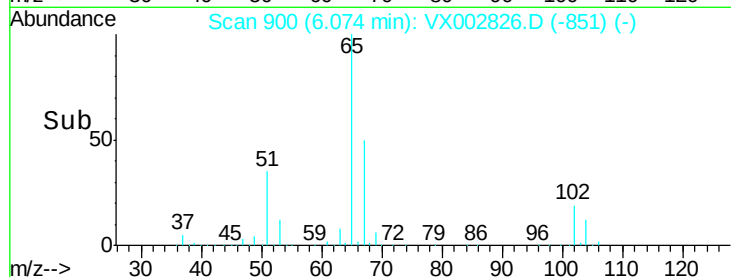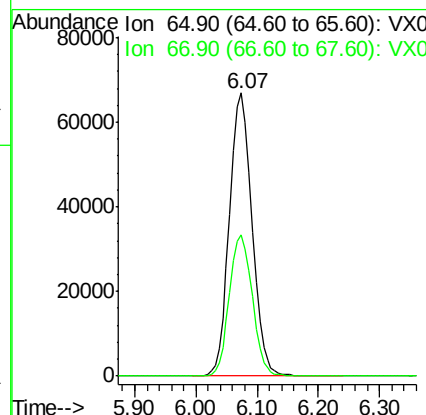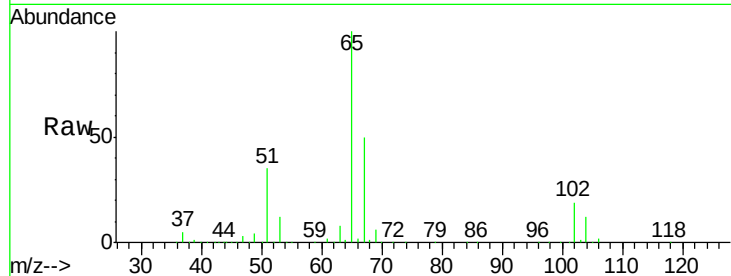

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.87 min Scan# 1030
 Delta R.T. 0.00 min
 Lab File: VX002826.D
 Acq: 22 Jun 2018 08:51

Tgt Ion: 114 Resp: 346279
 Ion Ratio Lower Upper
 114 100
 63 21.5 0.0 41.4
 88 15.7 0.0 30.0

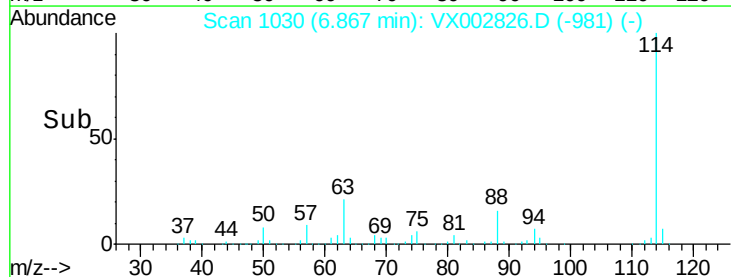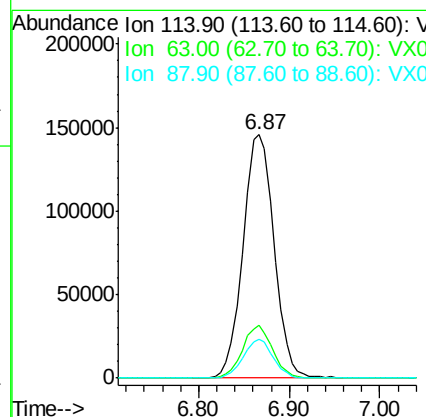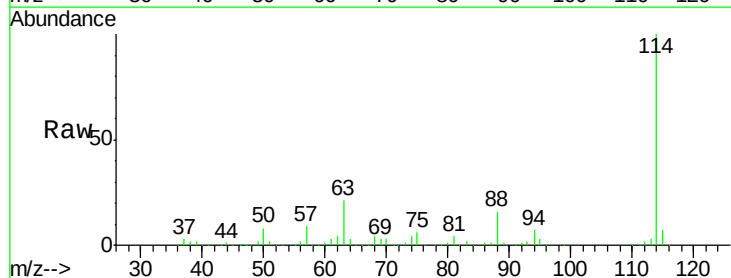

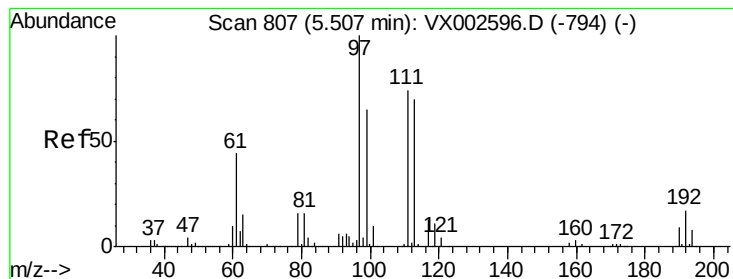

#35

Dibromofluoromethane

Concen: 47.78 ug/l

RT: 5.51 min Scan# 807

Delta R.T. 0.00 min

Lab File: VX002826.D

Acq: 22 Jun 2018 08:51

Instrument :

MSVOA_X

ClientSampled :

26KV-TP-11


Tot Ion:113 Resp: 132054

Ion Ratio Lower Upper

113 100

111 102.2 81.4 122.0




192 24.2 19.1 28.7

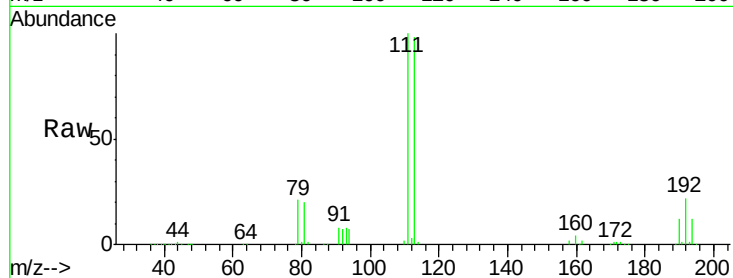

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

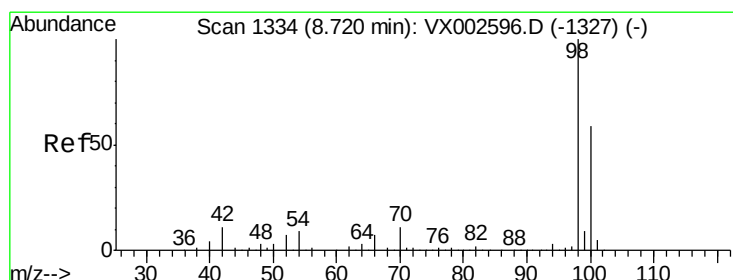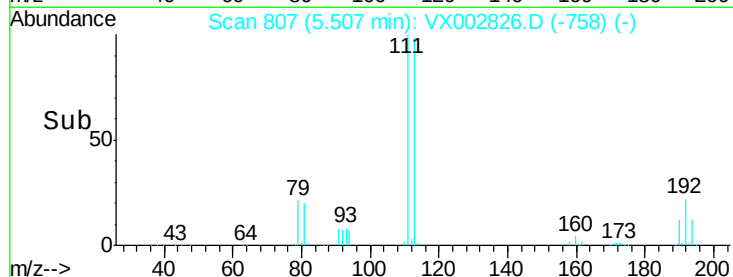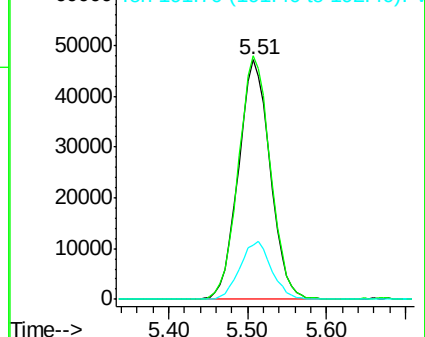

#50

Toluene-d8

Concen: 47.30 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX002826.D


Acq: 22 Jun 2018 08:51

Tgt Ion: 98 Resp: 496319

Ion Ratio Lower Upper



98 100


100 63.9 50.9 76.3

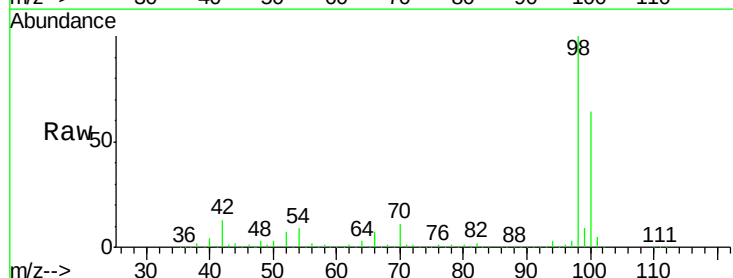

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

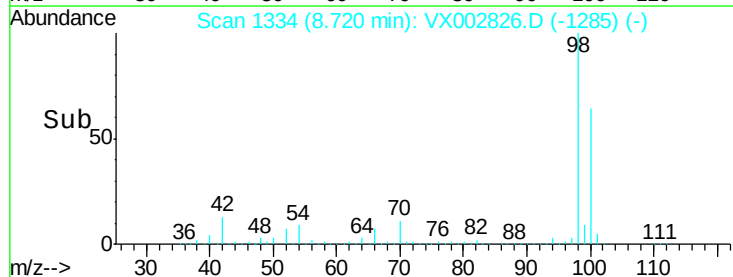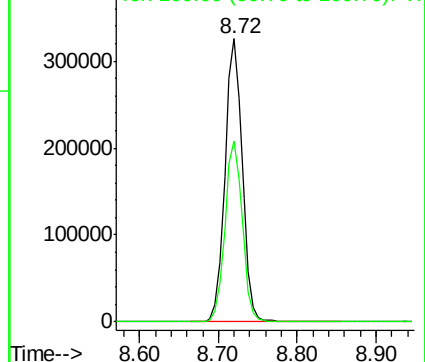

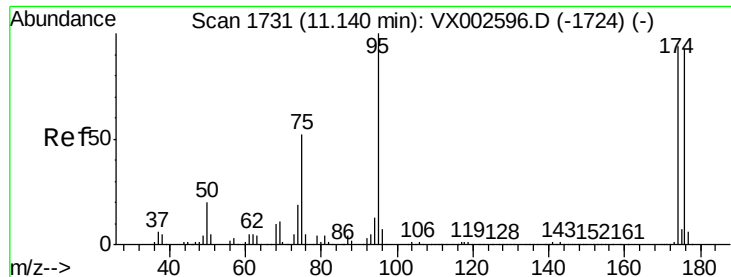

#62

4-Bromofluorobenzene

Concen: 44.35 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.00 min

Lab File: VX002826.D

Acq: 22 Jun 2018 08:51

Instrument :

MSVOA_X

ClientSampled :

26KV-TP-11


Tot Ion: 95 Resp: 176339

Ion Ratio Lower Upper

95 100

174 95.7 0.0 187.4




176 93.2 0.0 181.0

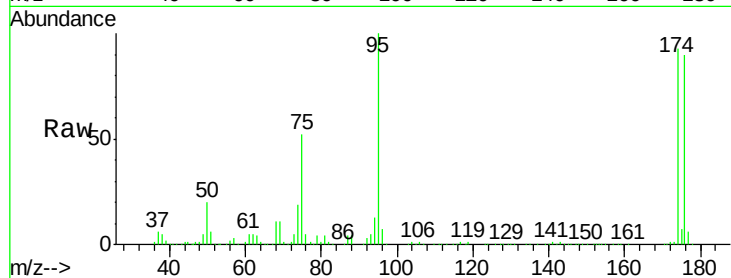

Abundance Ion 94.90 (94.60 to 95.60): VX002826.D (-1682) (-)

Ion 173.80 (173.50 to 174.50): VX002826.D (-1682) (-)

Ion 175.80 (175.50 to 176.50): VX002826.D (-1682) (-)

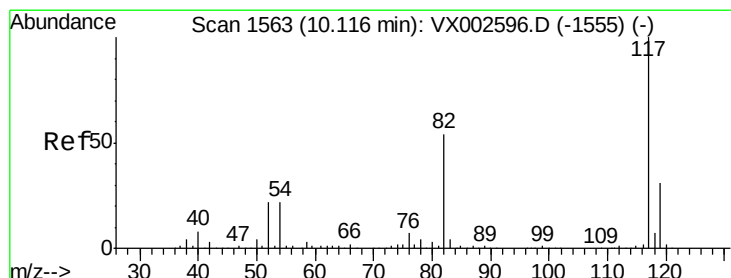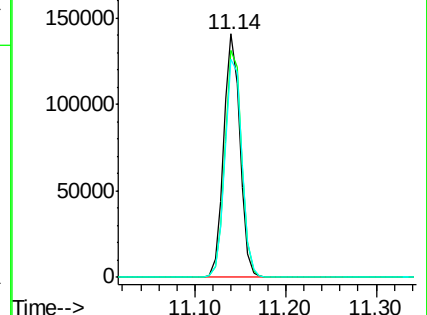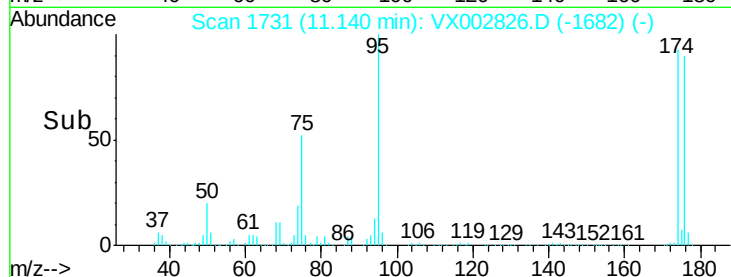

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 10.12 min Scan# 1563

Delta R.T. 0.00 min

Lab File: VX002826.D

Acq: 22 Jun 2018 08:51


Tgt Ion: 117 Resp: 327819

Ion Ratio Lower Upper

117 100

82 52.8 45.0 67.4



119 31.9 25.8 38.6

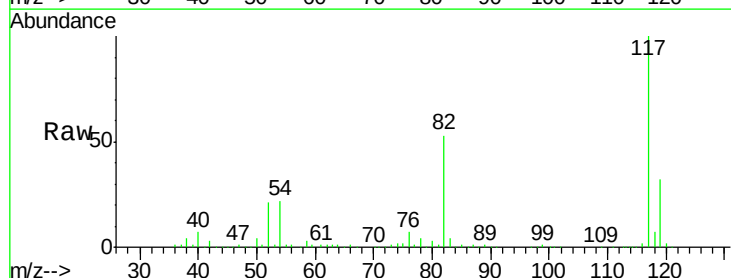


Abundance Ion 116.90 (116.60 to 117.60): VX002826.D (-1514) (-)

Ion 82.00 (81.70 to 82.70): VX002826.D (-1514) (-)

Ion 118.90 (118.60 to 119.60): VX002826.D (-1514) (-)

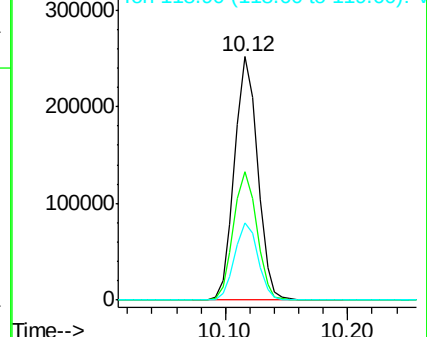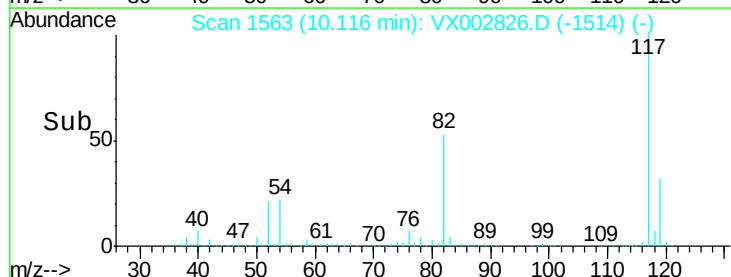

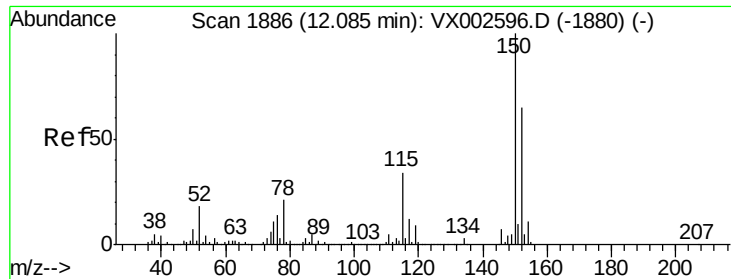

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.09 min Scan# 1886

Delta R.T. 0.00 min

Lab File: VX002826.D

Acq: 22 Jun 2018 08:51

Instrument :

MSVOA_X

ClientSampleId :

26KV-TP-11


Tot Ion:152 Resp: 183809

Ion Ratio Lower Upper

152 100

115 55.2 40.1 120.2

150 158.8 0.0 347.2

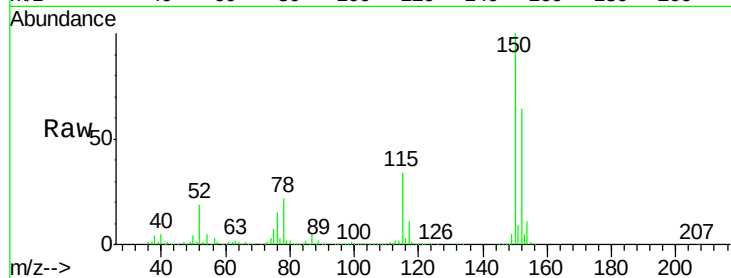

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

