

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062824\
 Data File : VX042082.D
 Acq On : 28 Jun 2024 13:16
 Operator : JC/MD
 Sample : VX0628MBL01
 Misc : 5.00g/10.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0628MBL01

Quant Time: Jun 29 04:18:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 21 23:51:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	170110	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.757	114	258928	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	254786	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	127000	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	78626	40.083	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	80.160%
35) Dibromofluoromethane	5.379	113	79708	43.385	ug/l	-0.01
Spiked Amount	50.000	Range	75 - 124	Recovery	=	86.760%
50) Toluene-d8	8.647	98	298417	46.235	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	92.480%
62) 4-Bromofluorobenzene	11.079	95	115055	48.359	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	96.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062824\
Data File : VX042082.D
Acq On : 28 Jun 2024 13:16
Operator : JC/MD
Sample : VX0628MBL01
Misc : 5.00g/10.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0628MBL01

Quant Time: Jun 29 04:18:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 21 23:51:58 2024
Response via : Initial Calibration




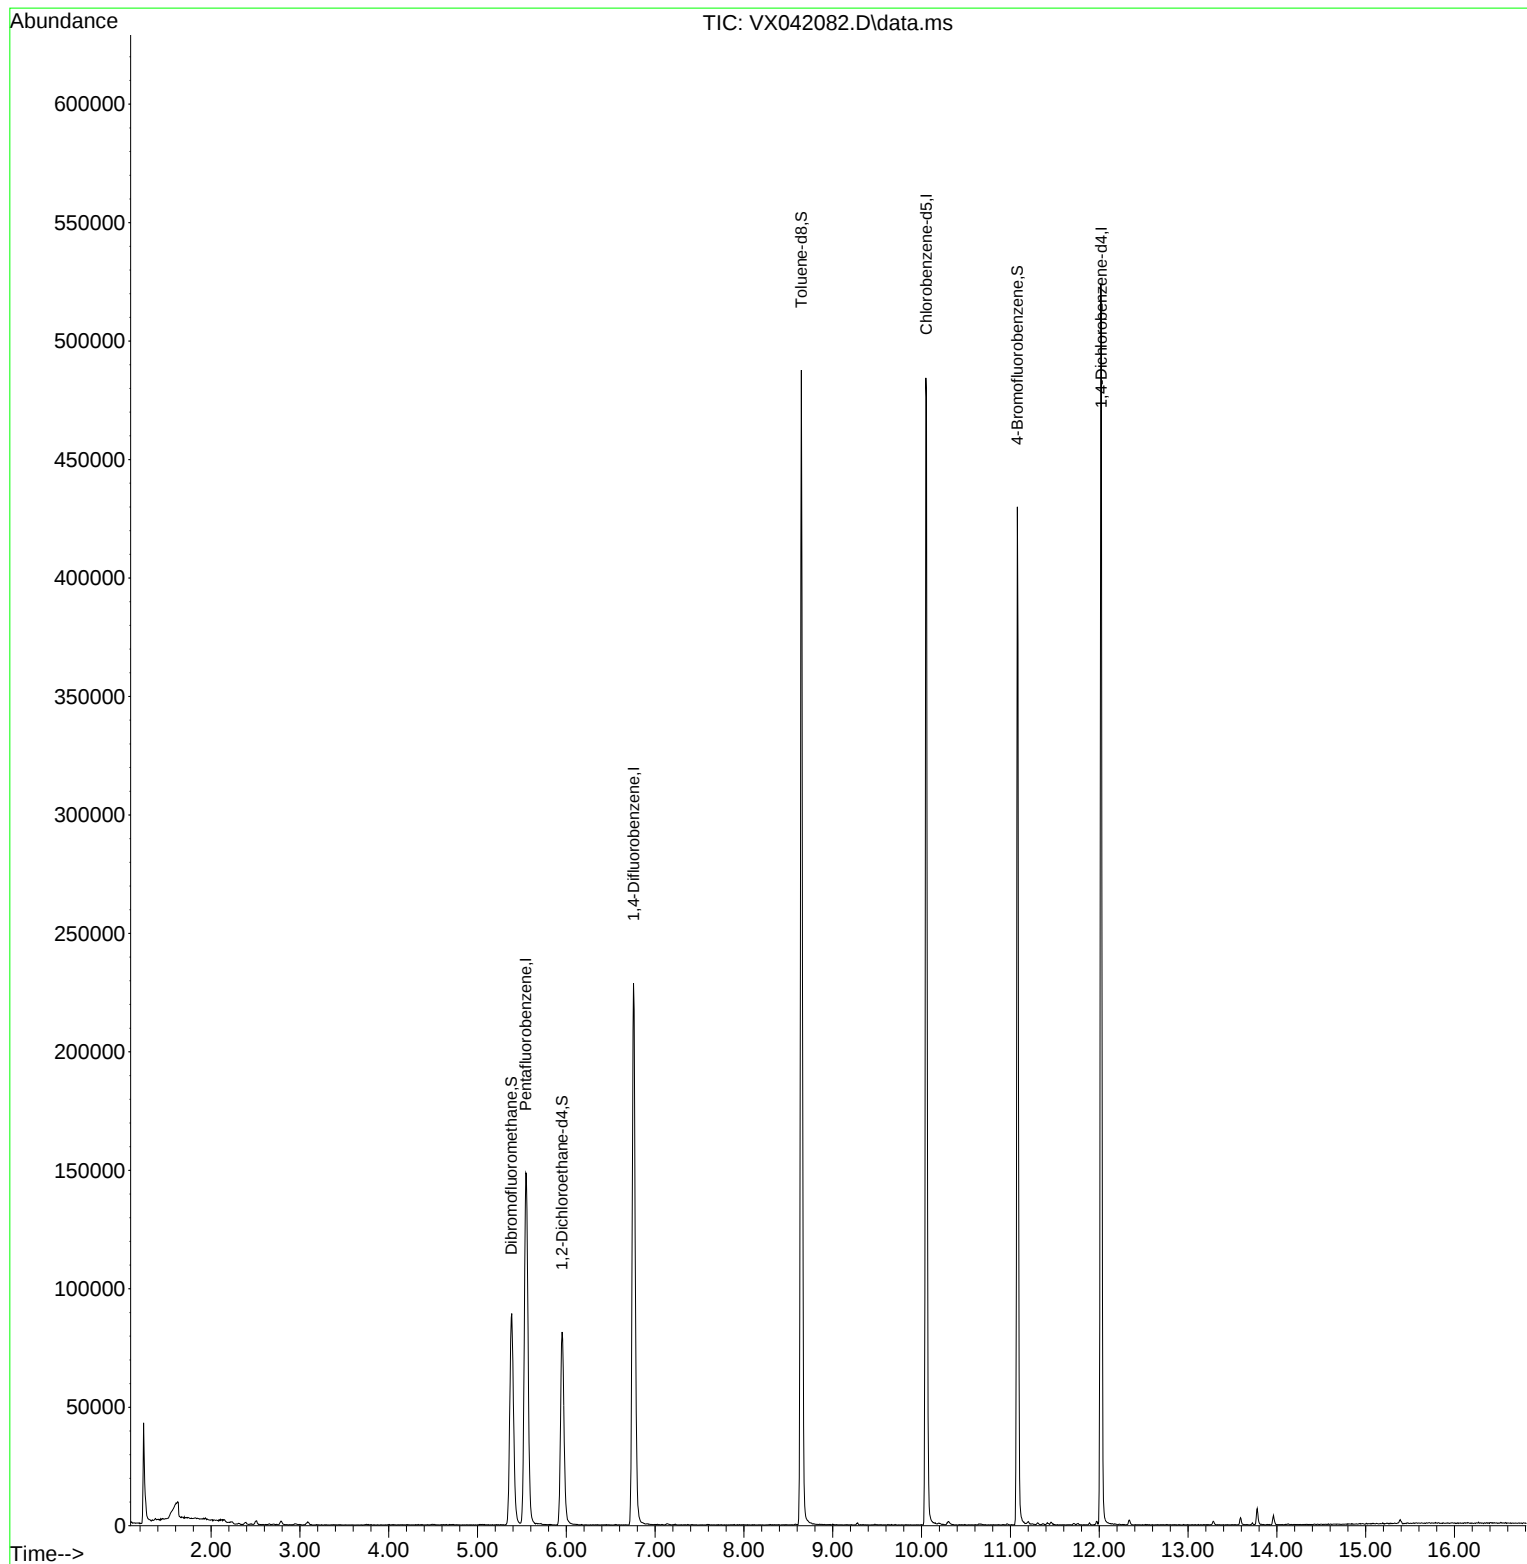


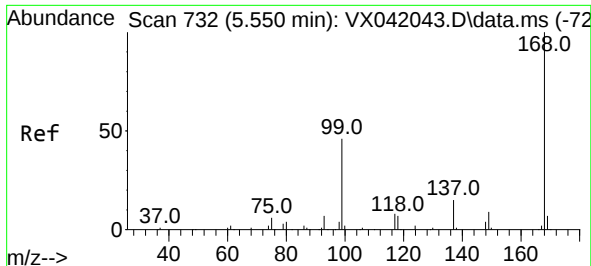

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX042082.D
Acq: 28 Jun 2024 13:16




Instrument :
MSVOA_X
ClientSampleId :
VX0628MBL01


Tgt Ion:168 Resp: 170110
Ion Ratio Lower Upper
168 100
99 47.1 56.6 85.0#

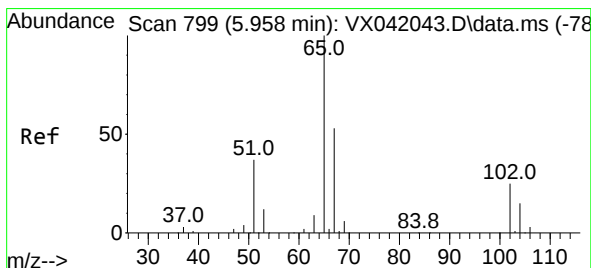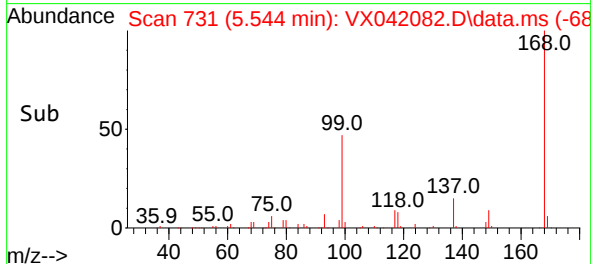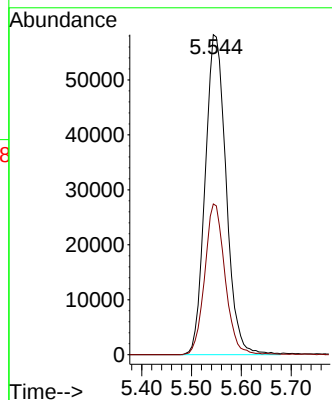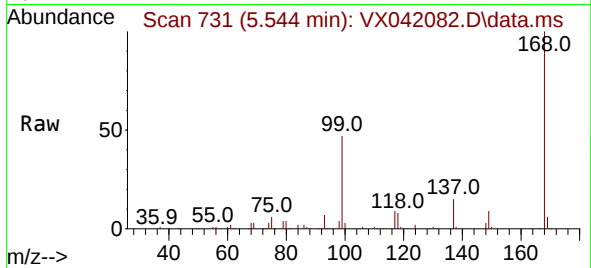

#33
1,2-Dichloroethane-d4
Concen: 40.083 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX042082.D
Acq: 28 Jun 2024 13:16

Tgt Ion: 65 Resp: 78626
Ion Ratio Lower Upper
65 100
67 54.2 0.0 100.2


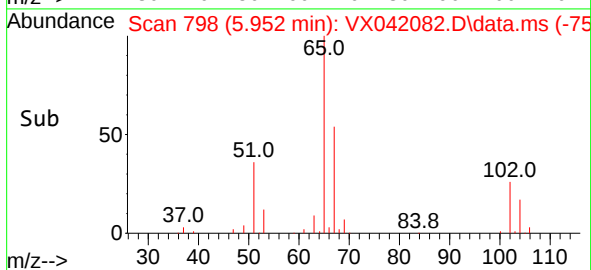
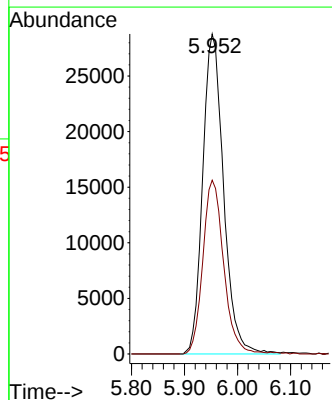
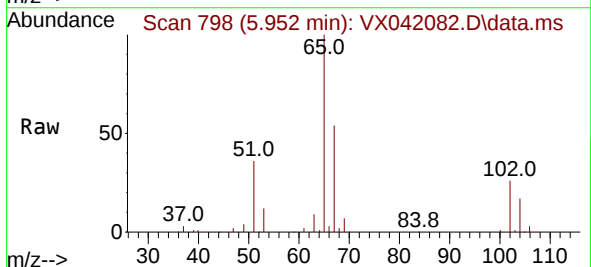


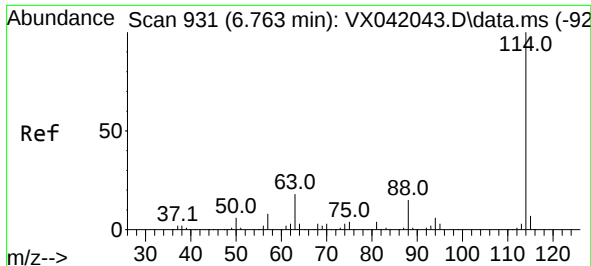

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX042082.D
Acq: 28 Jun 2024 13:16




Instrument :
MSVOA_X
ClientSampleId :
VX0628MBL01


Tgt Ion:114 Resp: 258928
Ion Ratio Lower Upper
114 100
63 18.1 0.0 45.0
88 14.9 0.0 36.6

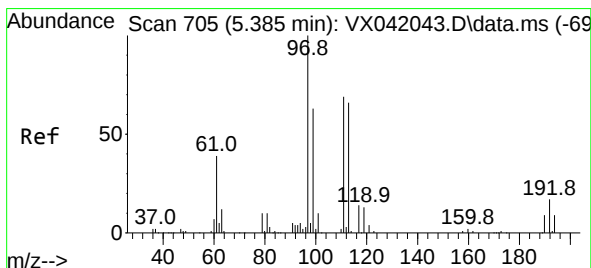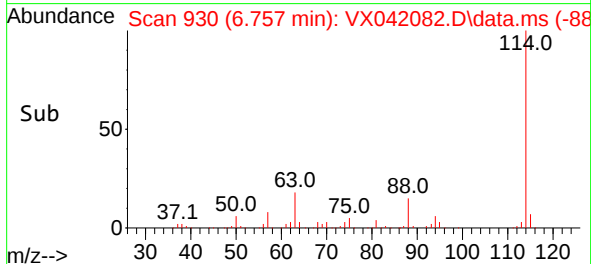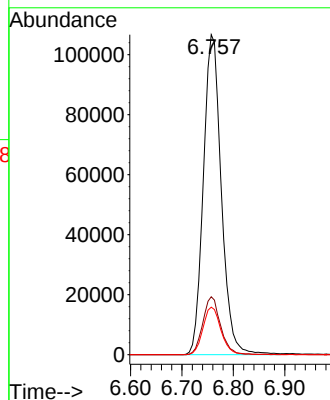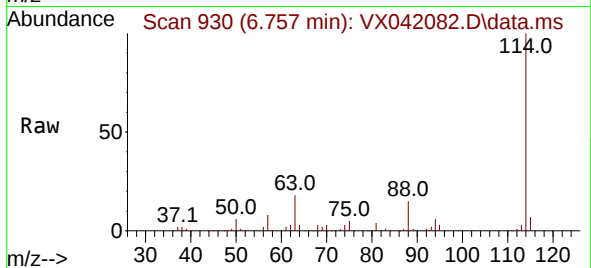

#35
Dibromofluoromethane
Concen: 43.385 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.012 min
Lab File: VX042082.D
Acq: 28 Jun 2024 13:16

Tgt Ion:113 Resp: 79708
Ion Ratio Lower Upper
113 100
111 102.9 82.9 124.3
192 26.5 13.3 19.9#


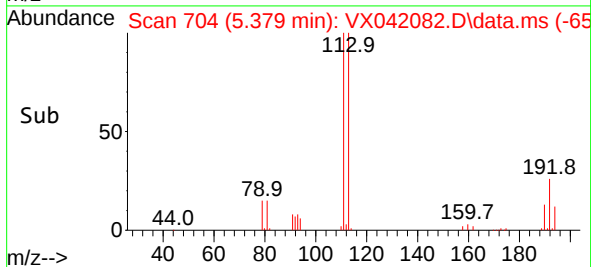
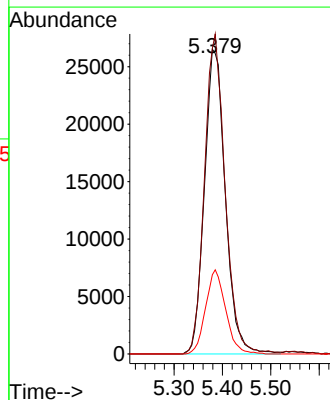
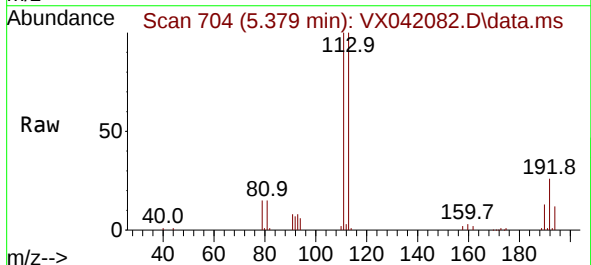


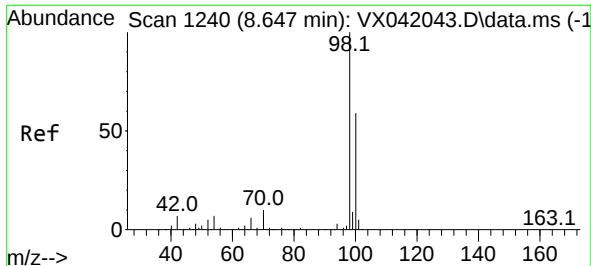

#50
Toluene-d8
Concen: 46.235 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX042082.D
Acq: 28 Jun 2024 13:16




Instrument :
MSVOA_X
ClientSampleId :
VX0628MBL01


Tgt Ion: 98 Resp: 298417
Ion Ratio Lower Upper
98 100
100 67.1 53.1 79.7

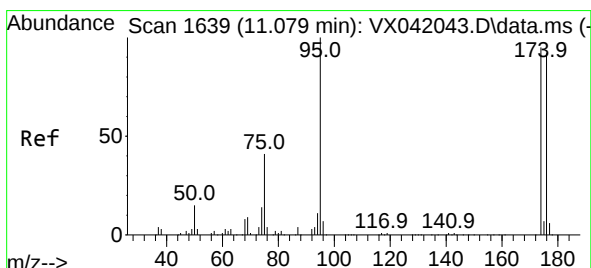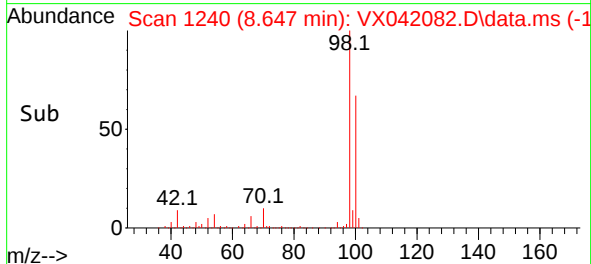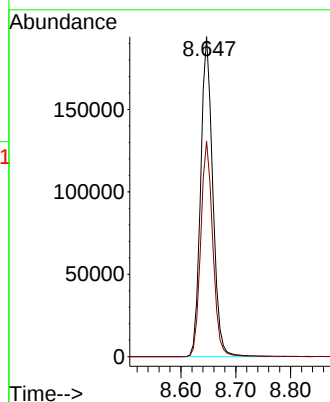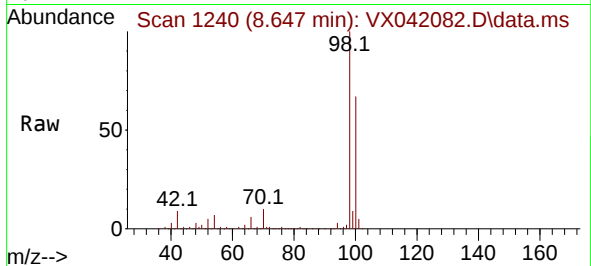

#62
4-Bromofluorobenzene
Concen: 48.359 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX042082.D
Acq: 28 Jun 2024 13:16

Tgt Ion: 95 Resp: 115055
Ion Ratio Lower Upper
95 100
174 98.7 0.0 135.6
176 95.7 0.0 131.0


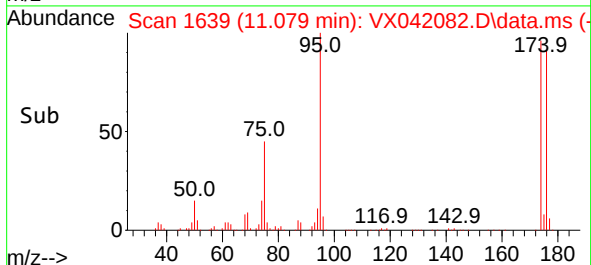
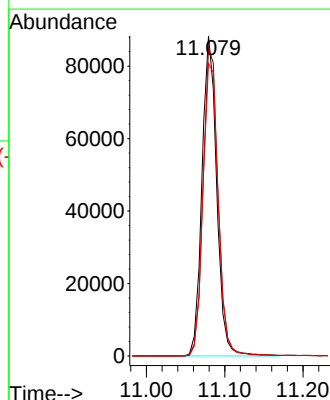
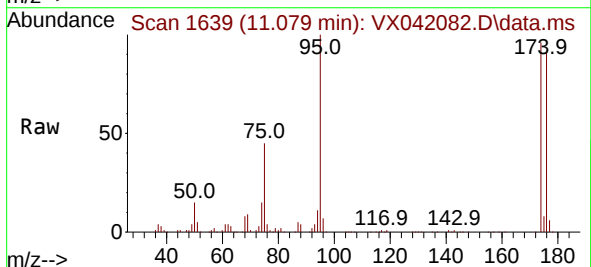


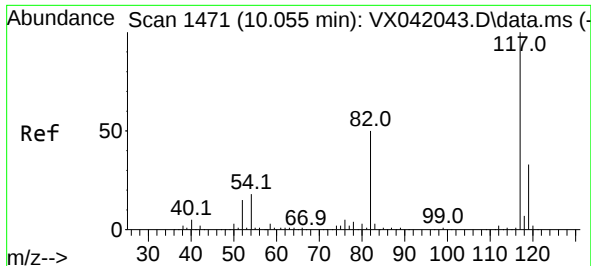

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX042082.D
Acq: 28 Jun 2024 13:16

Instrument :
MSVOA_X
ClientSampleId :
VX0628MBL01

Tgt Ion:117 Resp: 254786
Ion Ratio Lower Upper
117 100
82 49.0 46.2 69.4
119 33.2 25.5 38.3

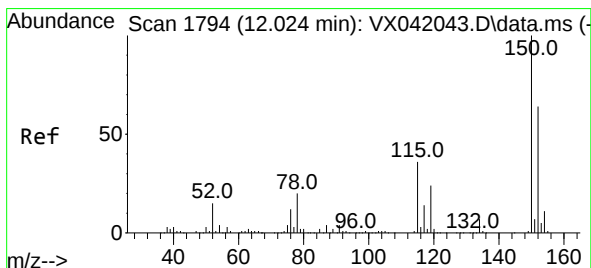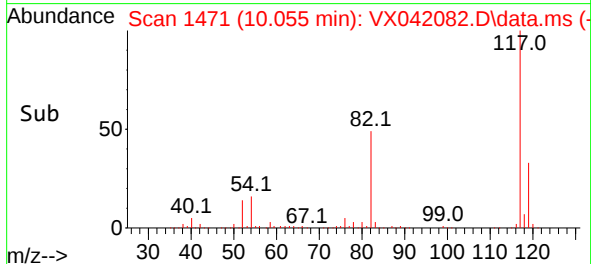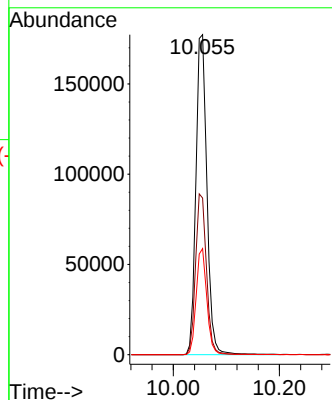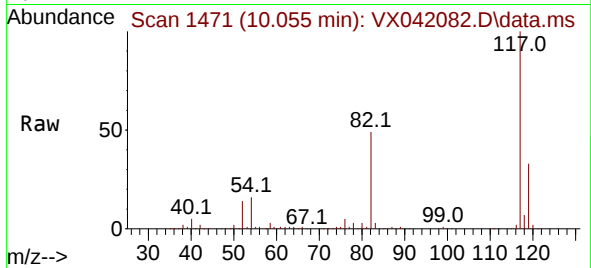

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX042082.D
Acq: 28 Jun 2024 13:16

Tgt Ion:152 Resp: 127000
Ion Ratio Lower Upper
152 100
115 53.0 43.3 129.9
150 157.0 0.0 345.0

