
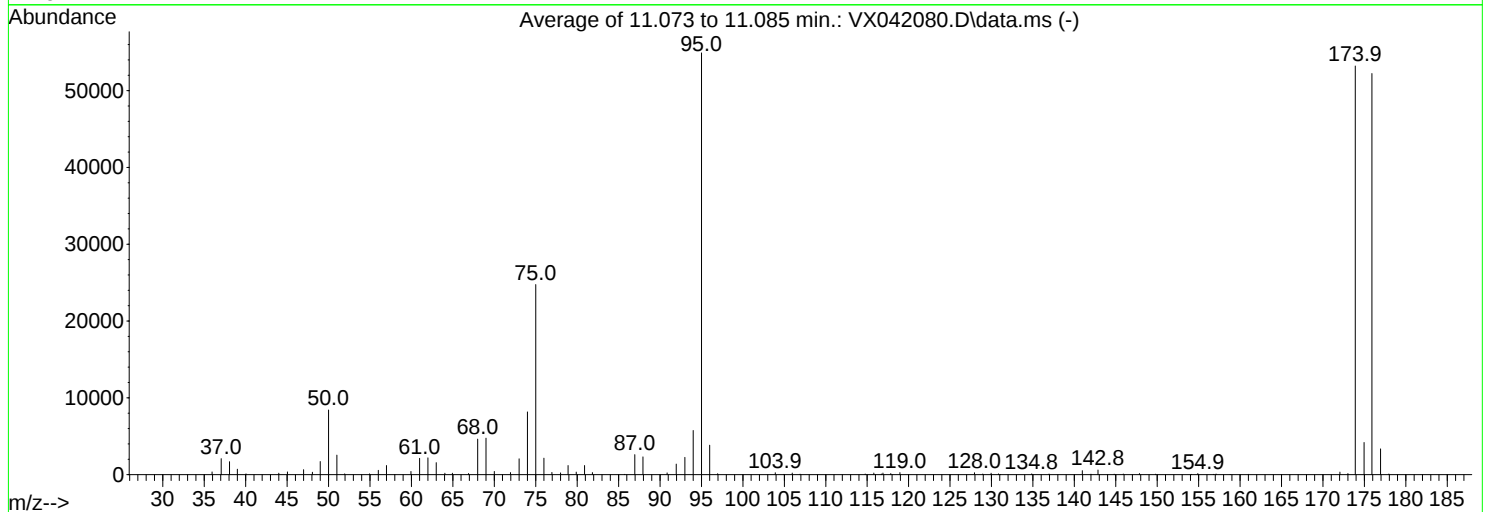


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062824\
Data File : VX042080.D
Acq On : 28 Jun 2024 10:08
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Title : SW846 8260
Last Update : Fri Jun 21 23:51:58 2024

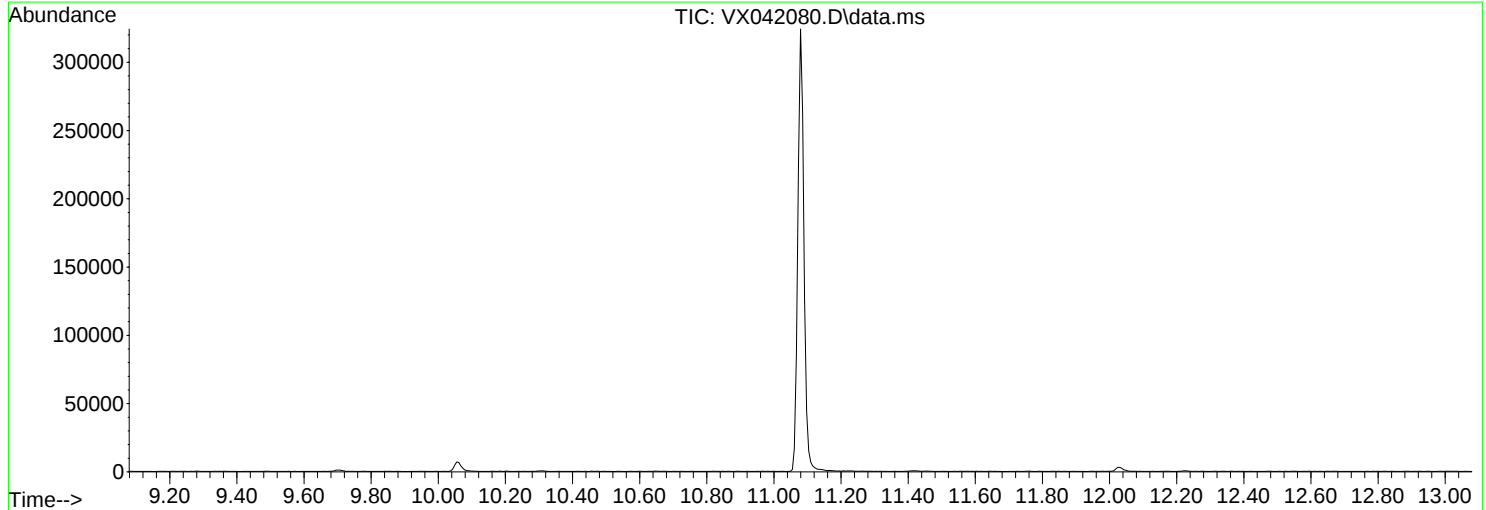

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	8420	PASS
75	95	30	60	45.1	24752	PASS
95	95	100	100	100.0	54912	PASS
96	95	5	9	7.0	3826	PASS
173	174	0.00	2	0.3	148	PASS
174	95	50	100	96.9	53200	PASS
175	174	5	9	7.9	4179	PASS
176	174	95	101	98.2	52227	PASS
177	176	5	9	6.4	3357	PASS